

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS053019\  
 Data File : PS004842.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 30 May 2019 20:01  
 Operator : SM\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 31 02:21:04 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS052019.M  
 Quant Title : 8080.M  
 QLast Update : Tue May 21 04:53:35 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound | RT#1  | RT#2  | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|----------|-------|-------|----------|---------|---------|---------|
| -----                       |          |       |       |          |         |         |         |
| System Monitoring Compounds |          |       |       |          |         |         |         |
| 4) S                        | 2,4-DCAA | 5.574 | 5.284 | 566.7E6  | 388.4E6 | 404.307 | 402.514 |
| Target Compounds            |          |       |       |          |         |         |         |
| 9) T                        | 2,4-D    | 6.663 | 0.000 | 48226693 | 0       | 35.256  | N.D. #  |
| 15) T                       | Picloram | 9.114 | 0.000 | 124.1E6  | 0       | 11.909  | N.D. #  |
| -----                       |          |       |       |          |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS053019\  
Data File : PS004842.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 30 May 2019 20:01  
Operator : SM\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 31 02:21:04 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS052019.M  
Quant Title : 8080.M  
QLast Update : Tue May 21 04:53:35 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

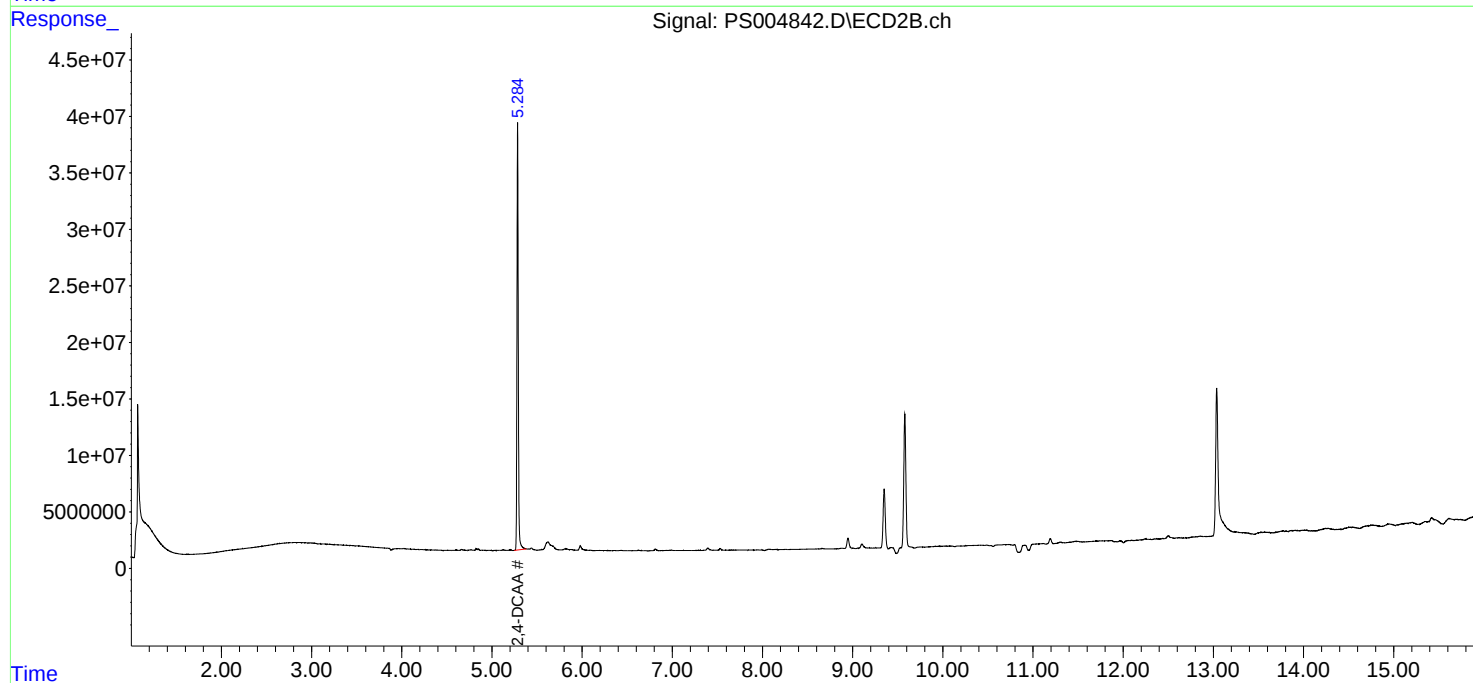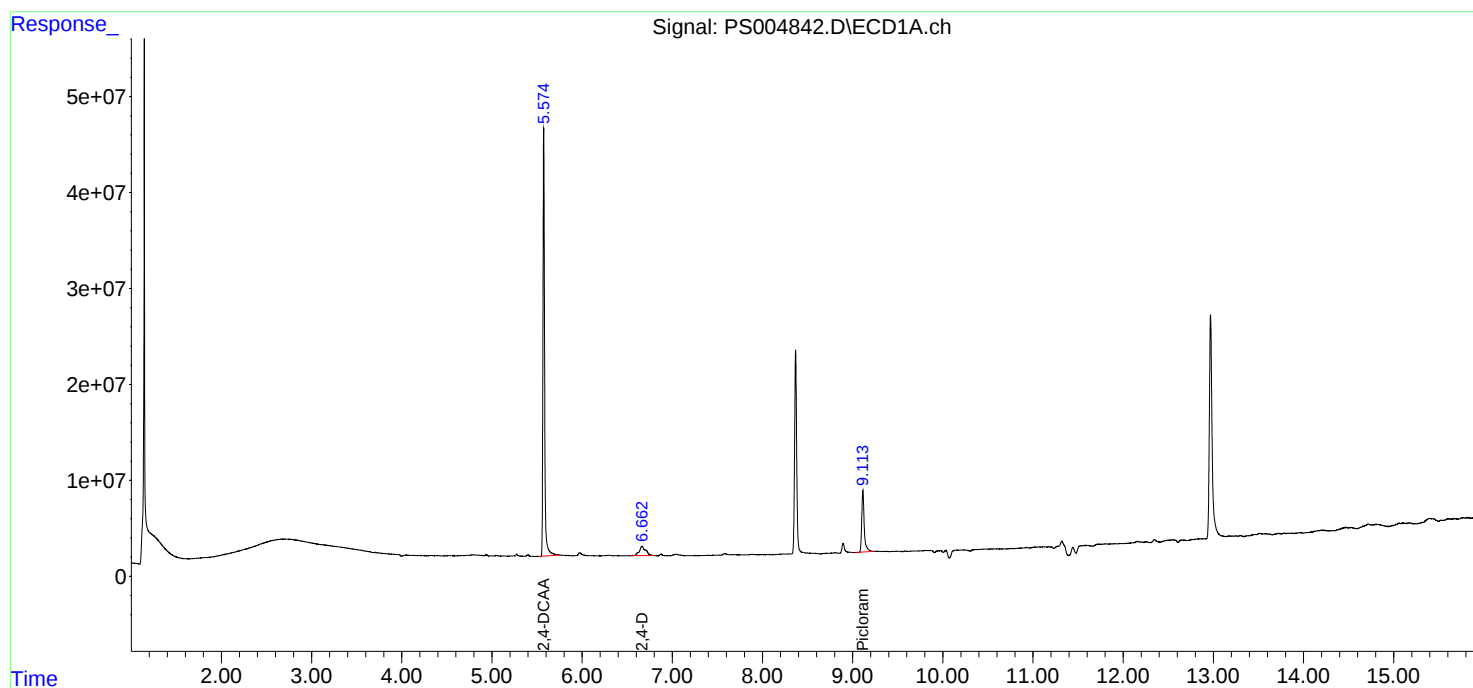


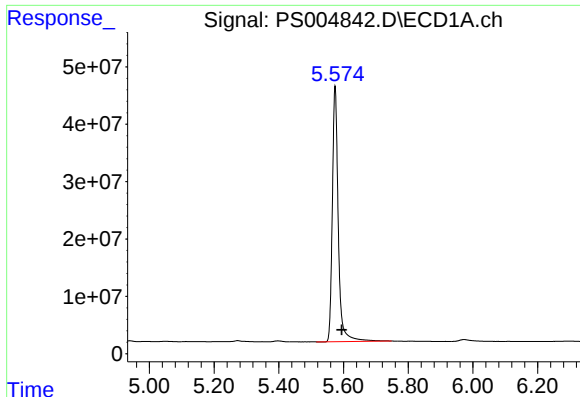

#4 2,4-DCAA


R.T.: 5.574 min  
Delta R.T.: -0.021 min  
Response: 566739449  
Conc: 404.31 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

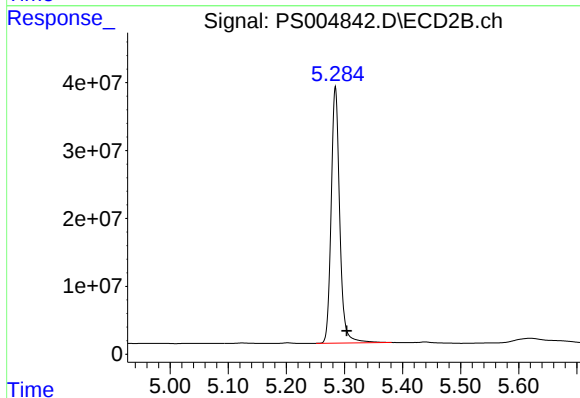


#4 2,4-DCAA

R.T.: 5.284 min  
Delta R.T.: -0.019 min  
Response: 388360284  
Conc: 402.51 ng/ml

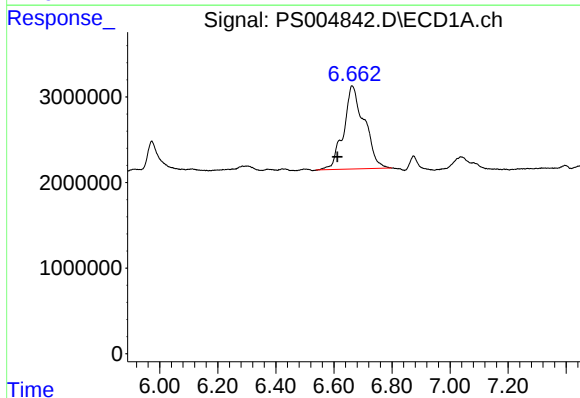


#9 2,4-D

R.T.: 6.663 min  
Delta R.T.: 0.051 min  
Response: 48226693  
Conc: 35.26 ng/ml

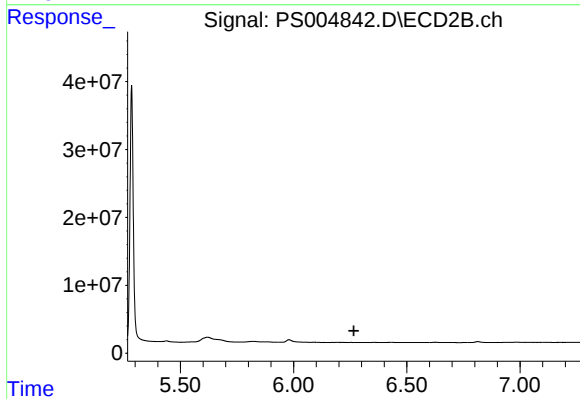

#9 2,4-D


R.T.: 0.000 min  
Exp R.T.: 6.266 min  
Response: 0  
Conc: N.D.

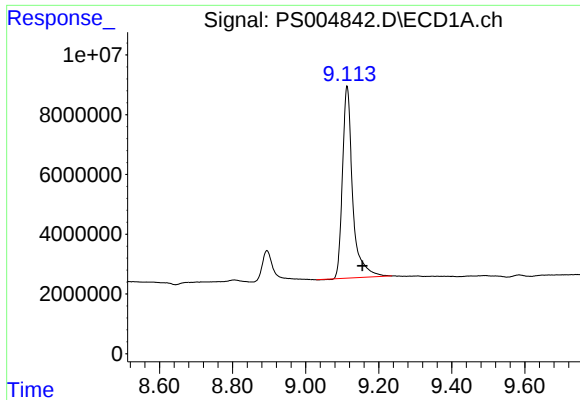

#15 Picloram

R.T.: 9.114 min  
Delta R.T.: -0.042 min  
Response: 124094406  
Conc: 11.91 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

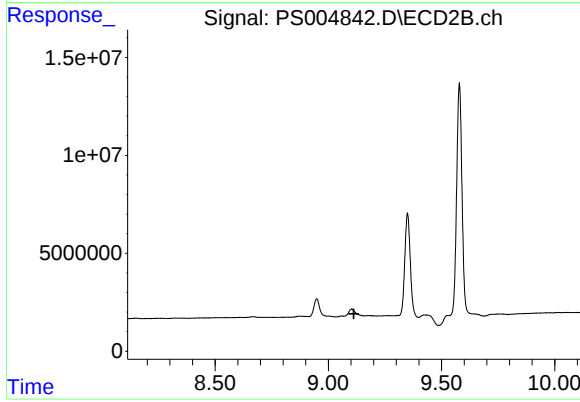

#15 Picloram

R.T.: 0.000 min  
Exp R.T. : 9.113 min  
Response: 0  
Conc: N.D.