

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053019\
 Data File : PS004844.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2019 20:45
 Operator : SM\AJ
 Sample : PB120184BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 02:21:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.611	5.322	786.6E6	527.9E6	561.142	547.138
Target Compounds							
2) T	3,5-DICHL...	0.000	4.641	0	270.7E6	N.D.	219.677
3) T	4-Nitroph...	5.415	0.000	34049085	0	54.609	N.D. #
5) T	DICAMBA	5.713	5.429	10639184	11019713	2.004	2.983 #
6) T	MCP	5.966	0.000	10905751	0	2.620	N.D. #
7) T	MCPA	6.106	5.715	16697673	20056102	2.883	4.902 #
10) T	Pentachlo...	0.000	6.591	0	19625684	N.D.	1.598
11) T	2,4,5-TP ...	0.000	6.979	0	36239820	N.D.	7.043
12) T	2,4,5-T	7.636	7.428	108.8E6	36677670	14.615	8.230 #
13) T	2,4-DB	8.261	7.883	76056974	21377990	78.737	32.707 #
14) T	DINOSEB	0.000	8.188	0	67319538	N.D.	17.512
15) T	Picloram	9.179	9.136	164.4E6	117.9E6	15.776	15.807
16) T	DCPA	0.000	9.136	0	117.9E6	N.D.	18.205



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053019\
Data File : PS004844.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2019 20:45
Operator : SM\AJ
Sample : PB120184BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 02:21:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

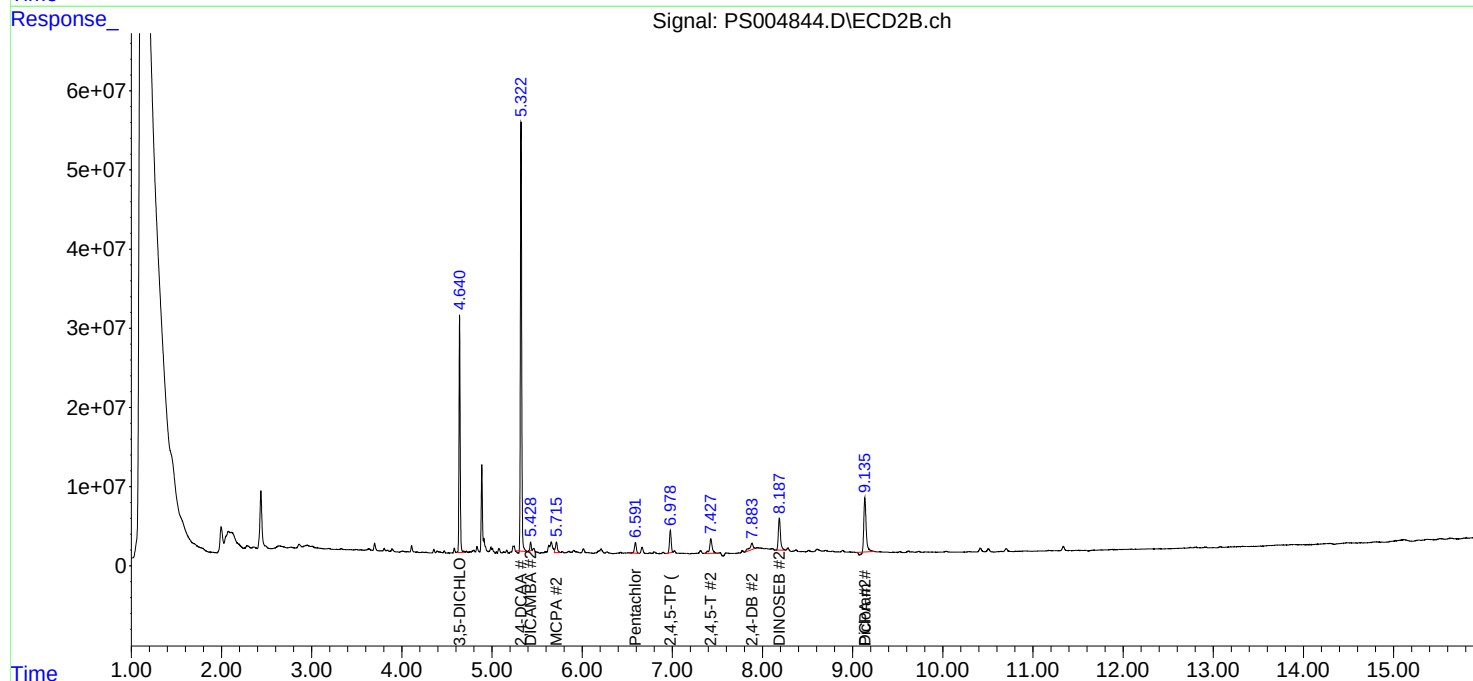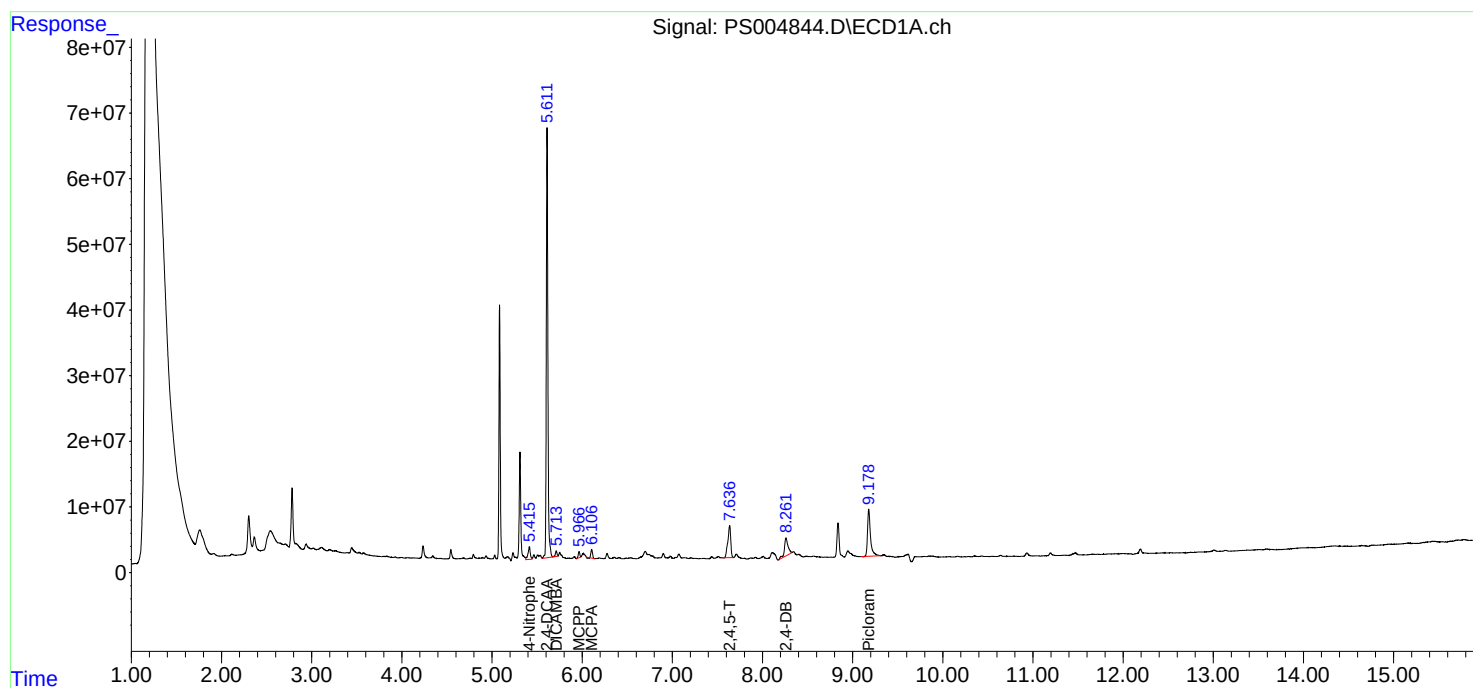


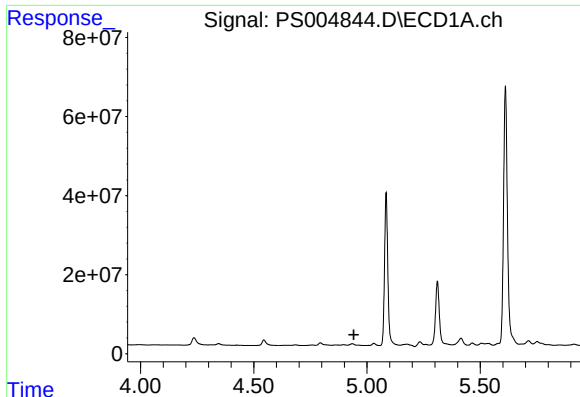

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

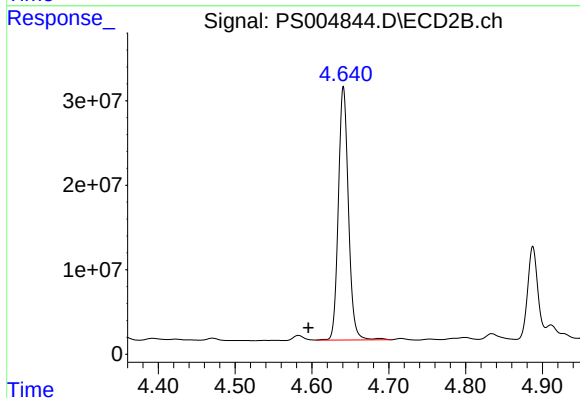


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.641 min
Delta R.T.: 0.045 min
Response: 270670623
Conc: 219.68 ng/ml

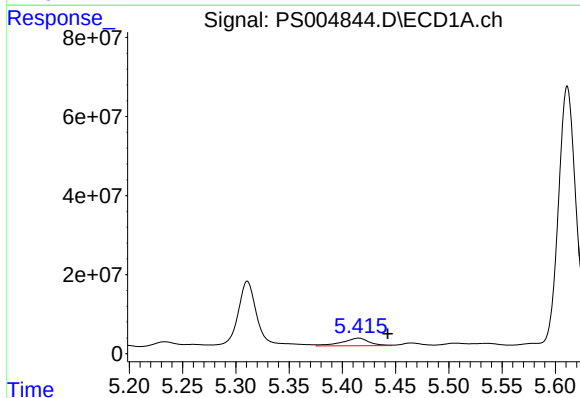


#3 4-Nitrophenol

R.T.: 5.415 min
Delta R.T.: -0.028 min
Response: 34049085
Conc: 54.61 ng/ml

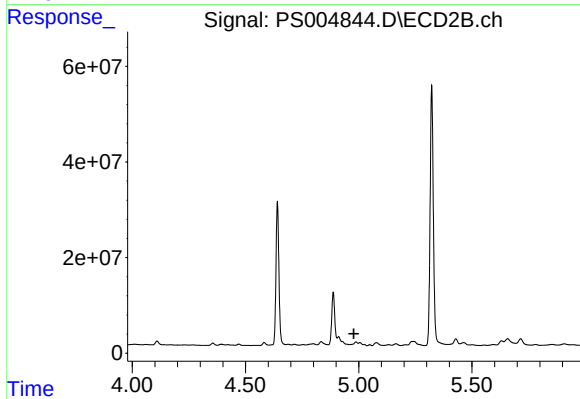

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

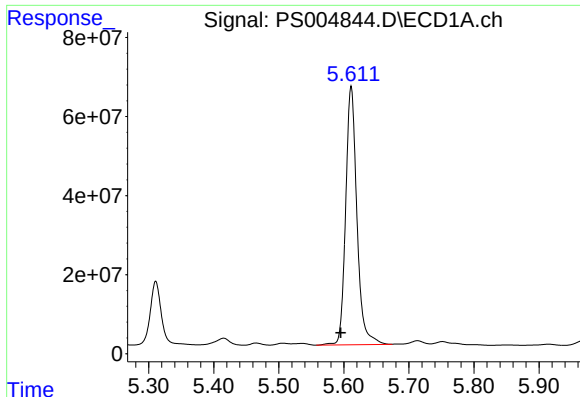

#4 2,4-DCAA


R.T.: 5.611 min
Delta R.T.: 0.016 min
Response: 786584518
Conc: 561.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

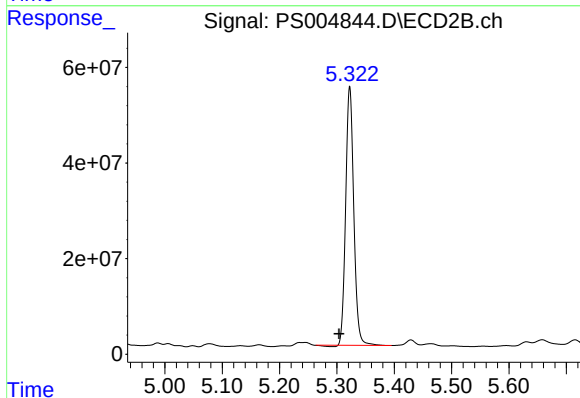


#4 2,4-DCAA

R.T.: 5.322 min
Delta R.T.: 0.019 min
Response: 527898457
Conc: 547.14 ng/ml

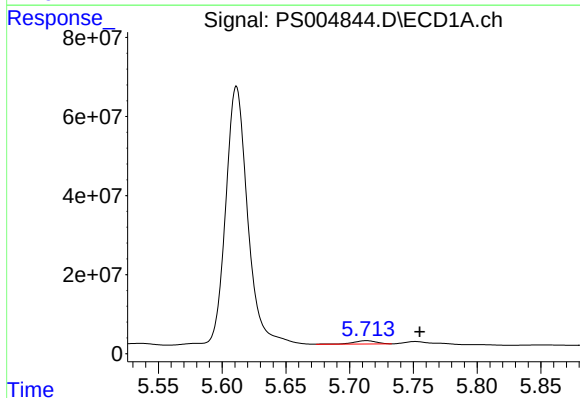


#5 DICAMBA

R.T.: 5.713 min
Delta R.T.: -0.042 min
Response: 10639184
Conc: 2.00 ng/ml

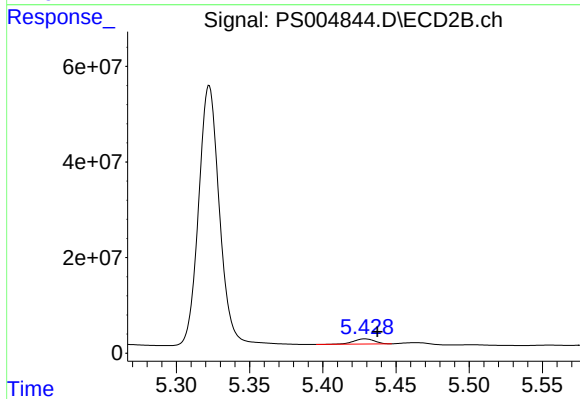

#5 DICAMBA


R.T.: 5.429 min
Delta R.T.: -0.008 min
Response: 11019713
Conc: 2.98 ng/ml

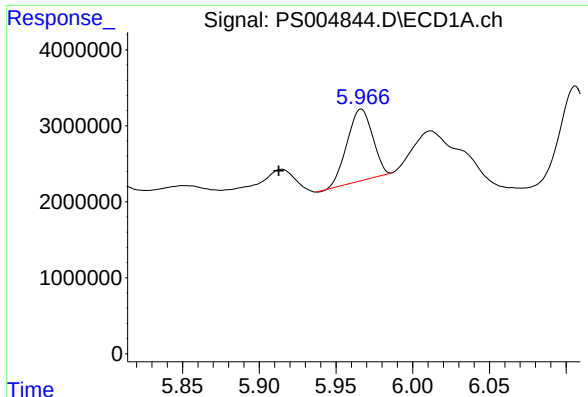

#6 MCPP


R.T.: 5.966 min
Delta R.T.: 0.054 min
Response: 10905751
Conc: 2.62 ug/ml

Instrument :
ECD_S
ClientSampleId :

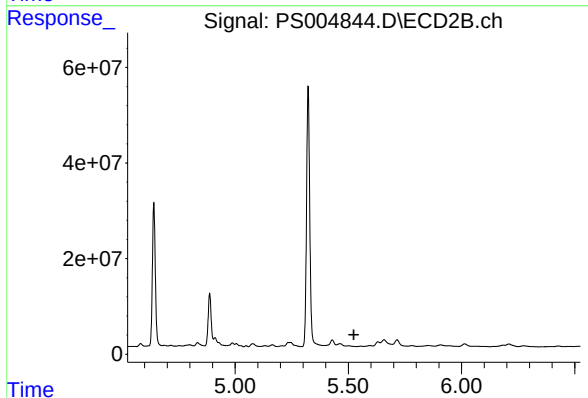


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

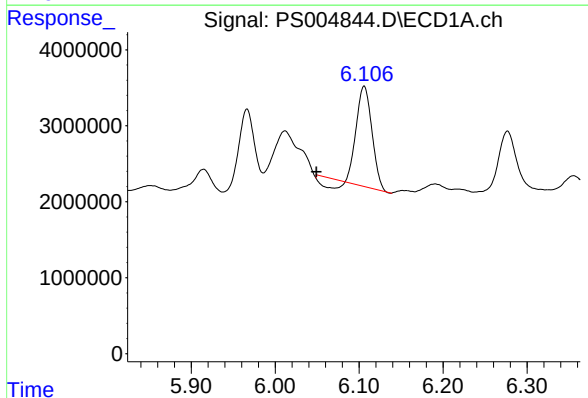


#7 MCPA

R.T.: 6.106 min
Delta R.T.: 0.057 min
Response: 16697673
Conc: 2.88 ug/ml

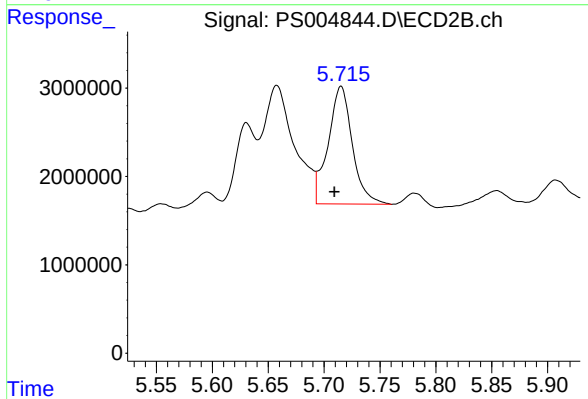

#7 MCPA


R.T.: 5.715 min
Delta R.T.: 0.006 min
Response: 20056102
Conc: 4.90 ug/ml

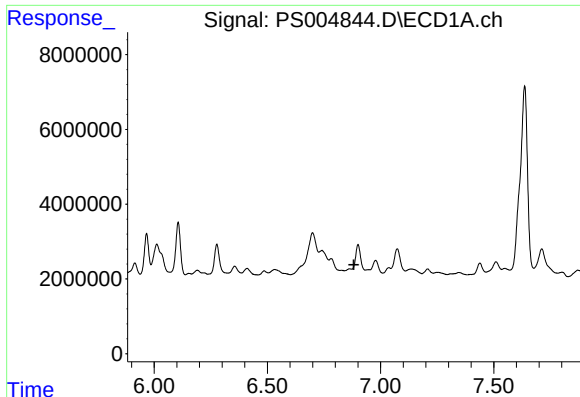

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

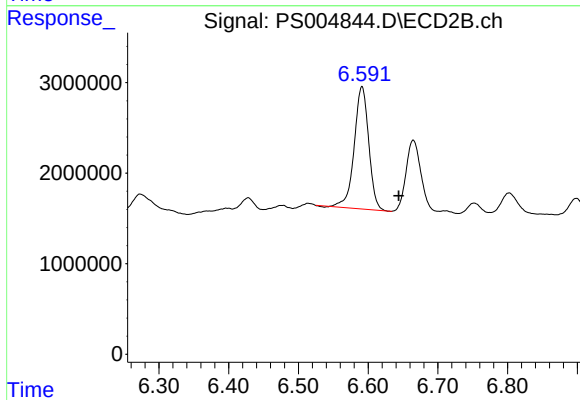


#10 Pentachlorophenol

R.T.: 6.591 min
Delta R.T.: -0.053 min
Response: 19625684
Conc: 1.60 ng/ml

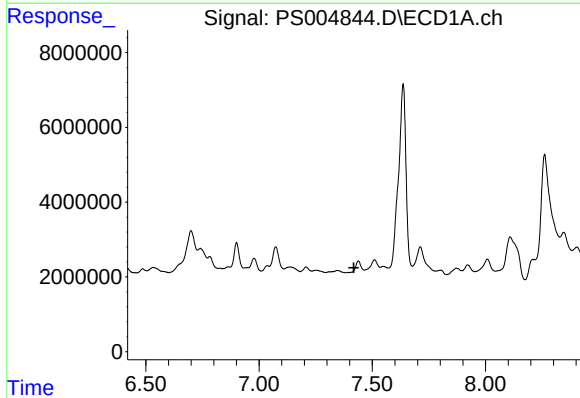


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

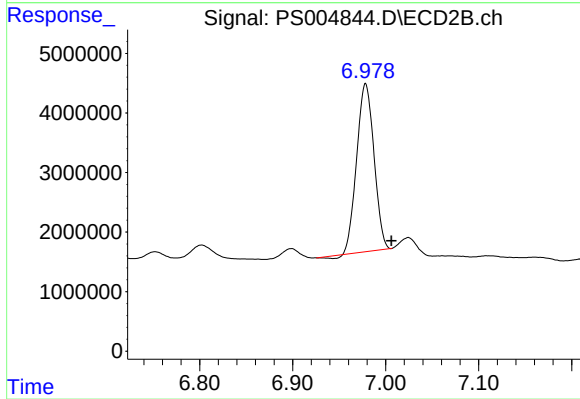

#11 2,4,5-TP (SILVEX)


R.T.: 6.979 min
Delta R.T.: -0.028 min
Response: 36239820
Conc: 7.04 ng/ml

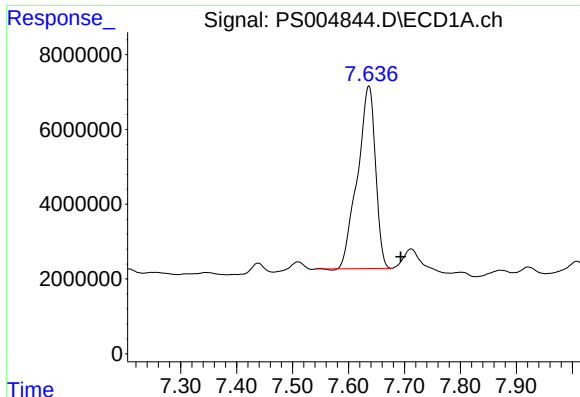

#12 2,4,5-T


R.T.: 7.636 min
Delta R.T.: -0.057 min
Response: 108846532
Conc: 14.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

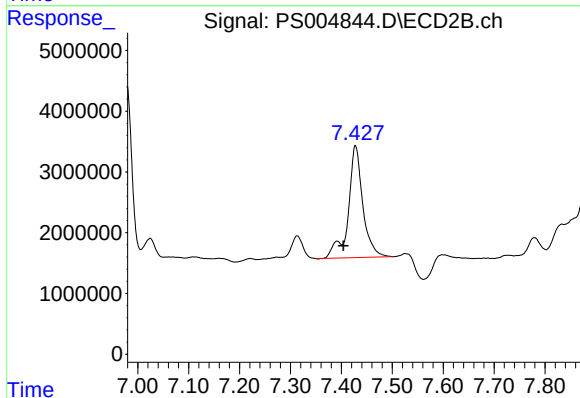


#12 2,4,5-T

R.T.: 7.428 min
Delta R.T.: 0.024 min
Response: 36677670
Conc: 8.23 ng/ml

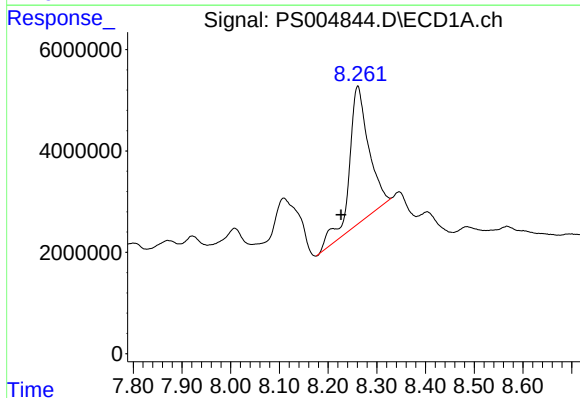


#13 2,4-DB

R.T.: 8.261 min
Delta R.T.: 0.034 min
Response: 76056974
Conc: 78.74 ng/ml

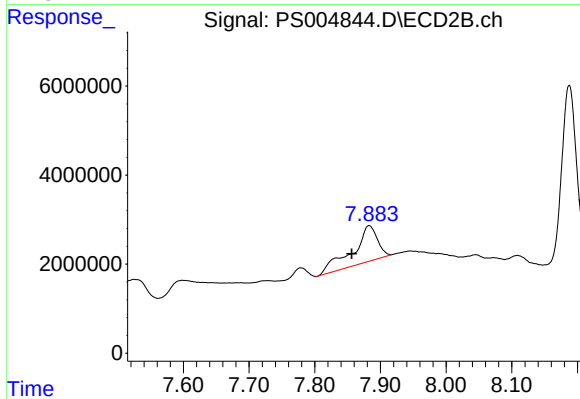

#13 2,4-DB


R.T.: 7.883 min
Delta R.T.: 0.026 min
Response: 21377990
Conc: 32.71 ng/ml

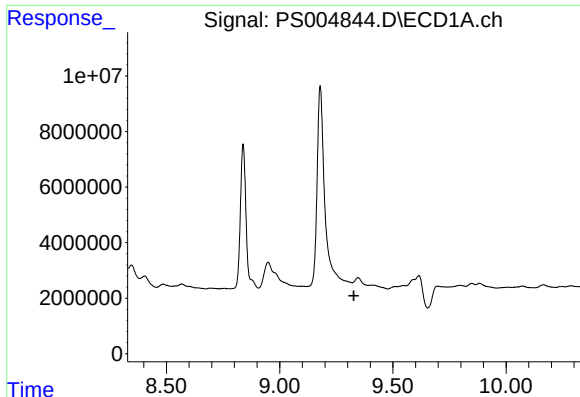

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

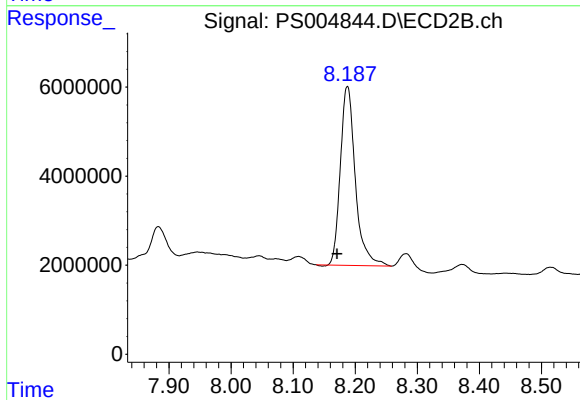


#14 DINOSEB

R.T.: 8.188 min
Delta R.T.: 0.016 min
Response: 67319538
Conc: 17.51 ng/ml

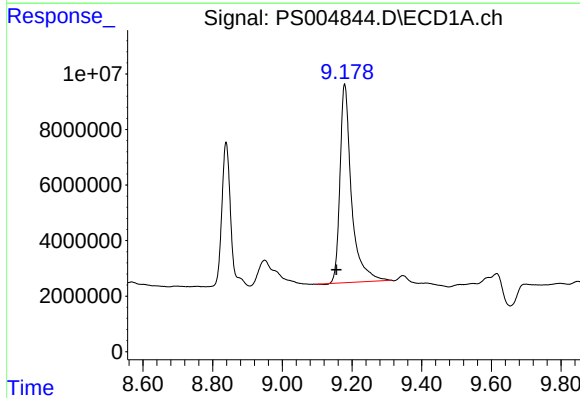


#15 Picloram

R.T.: 9.179 min
Delta R.T.: 0.024 min
Response: 164383903
Conc: 15.78 ng/ml

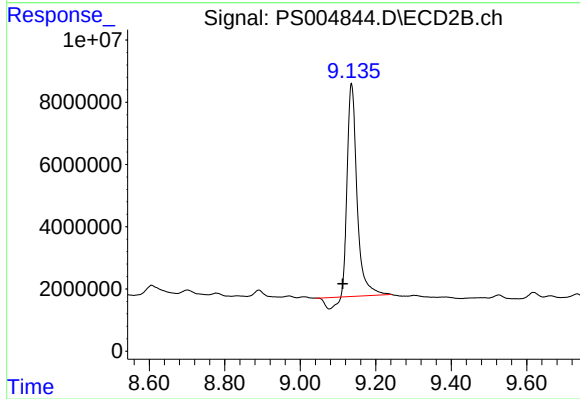

#15 Picloram


R.T.: 9.136 min
Delta R.T.: 0.023 min
Response: 117930370
Conc: 15.81 ng/ml

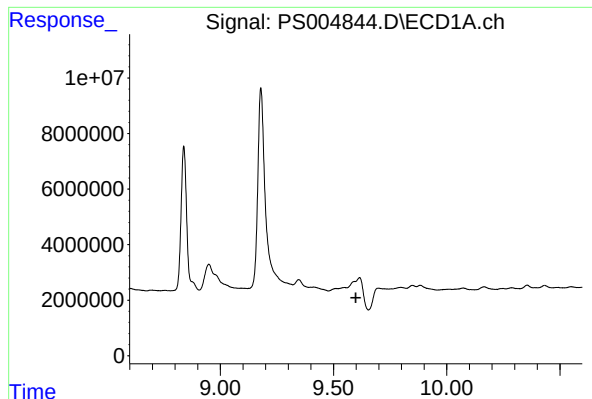

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

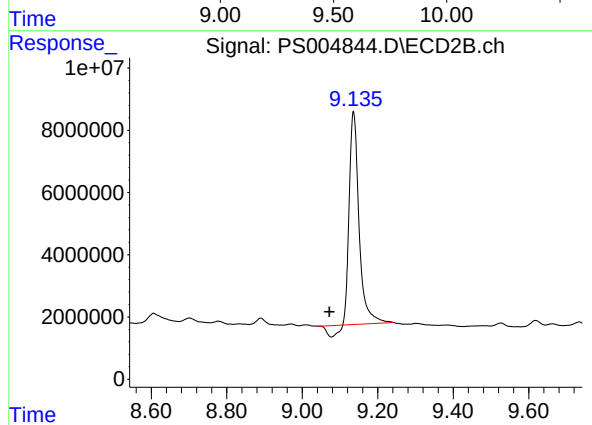

#16 DCPA

R.T.: 9.136 min
Delta R.T.: 0.064 min
Response: 117930370
Conc: 18.20 ng/ml