

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053019\
 Data File : PS004847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2019 21:51
 Operator : SM\AJ
 Sample : K3041-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 02:22:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.572	5.283	780.6E6	510.1E6	556.886	528.659
Target Compounds							
2) T	3,5-DICHL...	0.000	4.602	0	301.5E6	N.D.	244.735
3) T	4-Nitroph...	0.000	4.948	0	11215277	N.D.	23.665
5) T	DICAMBA	5.712	5.389	13750036	20000213	2.590	5.414 #
6) T	MCP	5.927	5.591	4055597	11927688	<MDL	4.353 #
7) T	MCPA	5.993	5.740	-6957124	273.6E6	N.D.	66.860
8) T	DICHLORPROP	0.000	5.972	0	20007051	N.D.	21.220
9) T	2,4-D	6.660	0.000	26030744	0	19.030	N.D. #
11) T	2,4,5-TP ...	0.000	6.938	0	223.6E6	N.D.	43.463



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053019\
Data File : PS004847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2019 21:51
Operator : SM\AJ
Sample : K3041-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 02:22:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

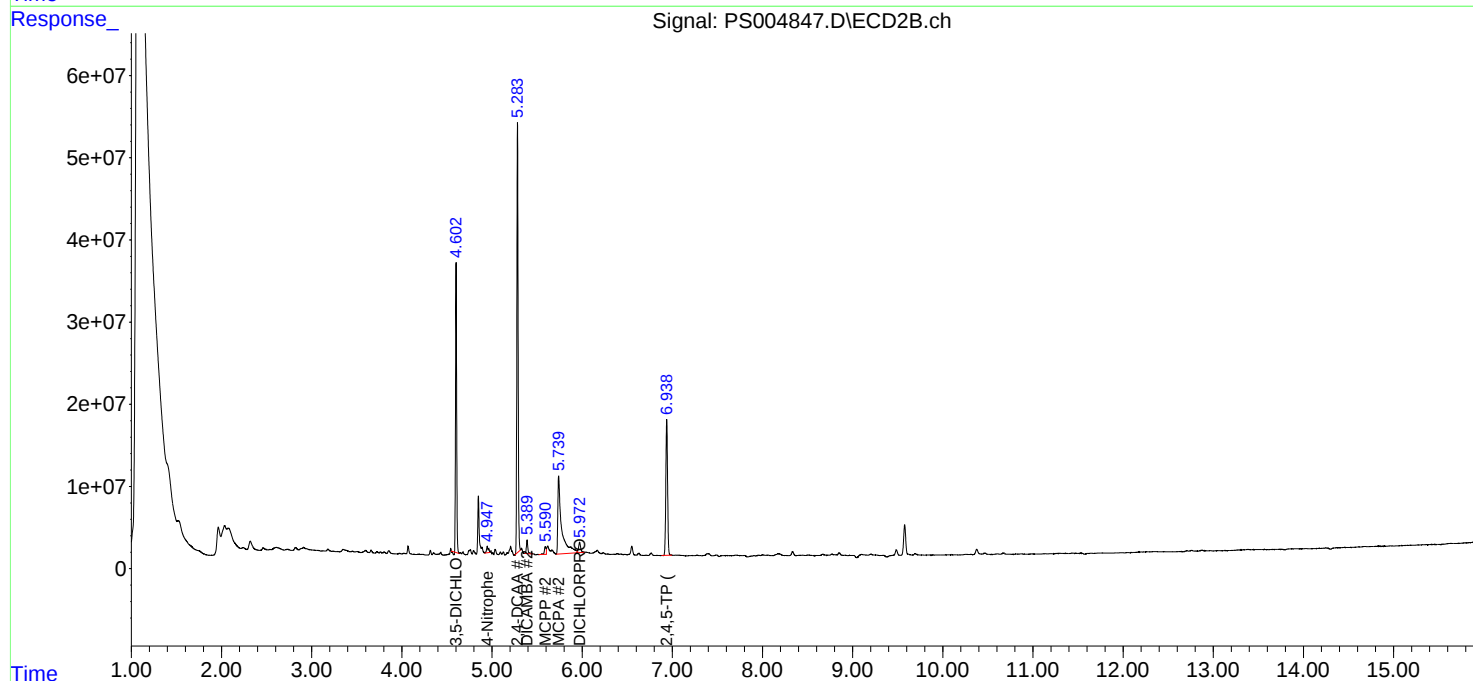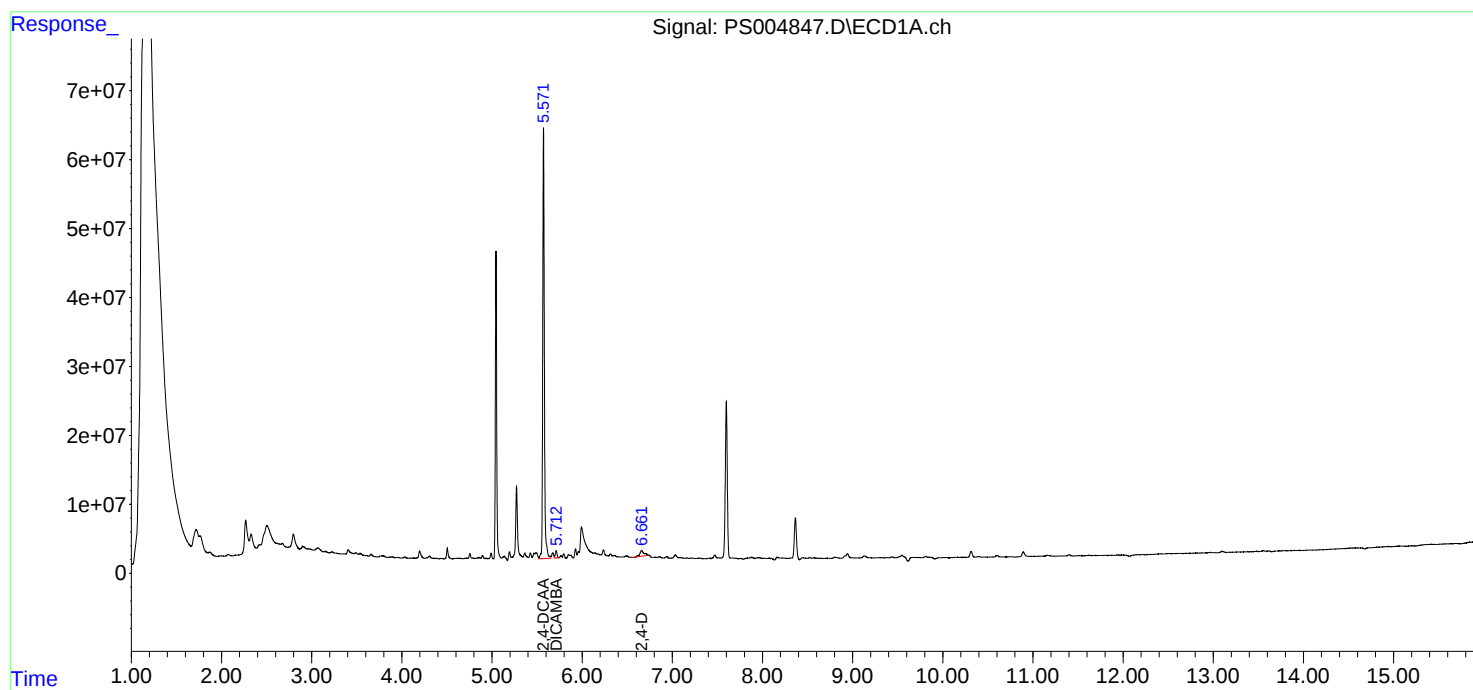


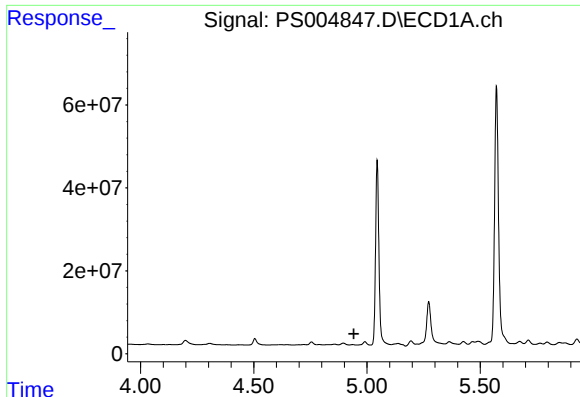

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

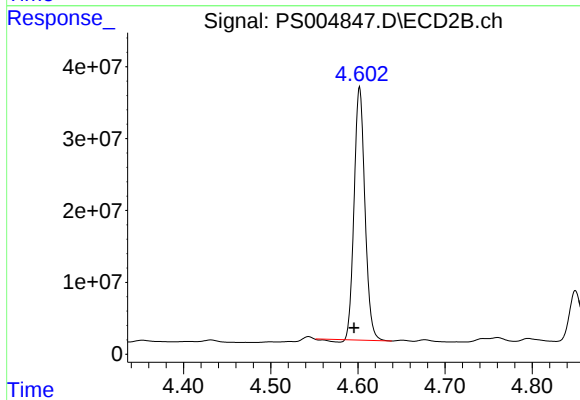


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.602 min
Delta R.T.: 0.007 min
Response: 301544702
Conc: 244.73 ng/ml

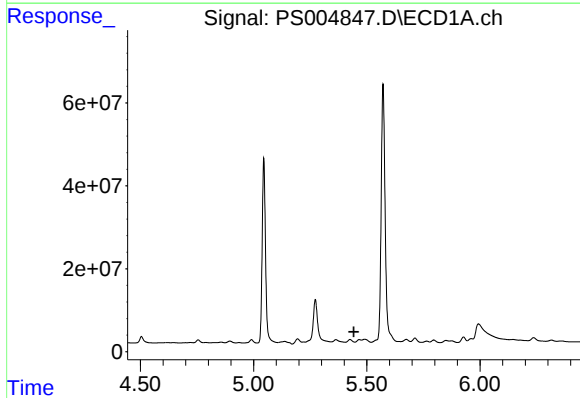


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 5.443 min
Response: 0
Conc: N.D.

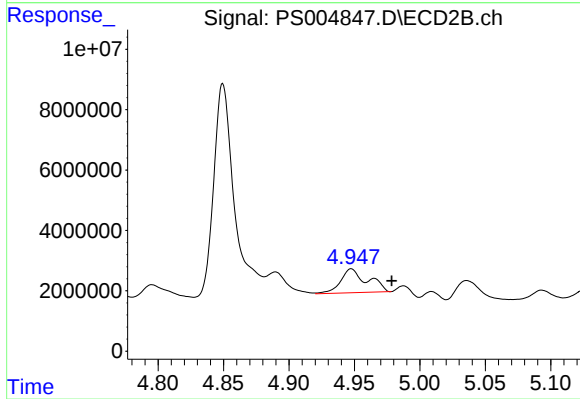

#3 4-Nitrophenol


R.T.: 4.948 min
Delta R.T.: -0.031 min
Response: 11215277
Conc: 23.66 ng/ml

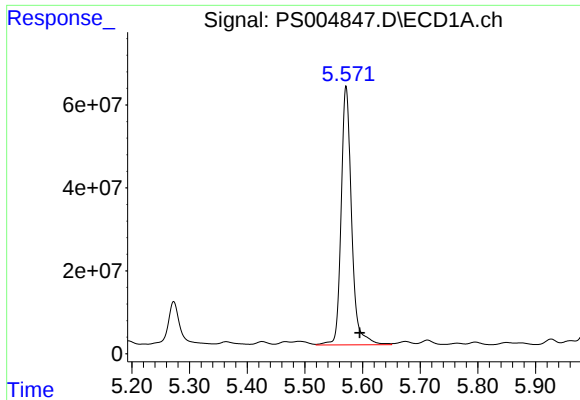

#4 2,4-DCAA


R.T.: 5.572 min
Delta R.T.: -0.023 min
Response: 780618360
Conc: 556.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

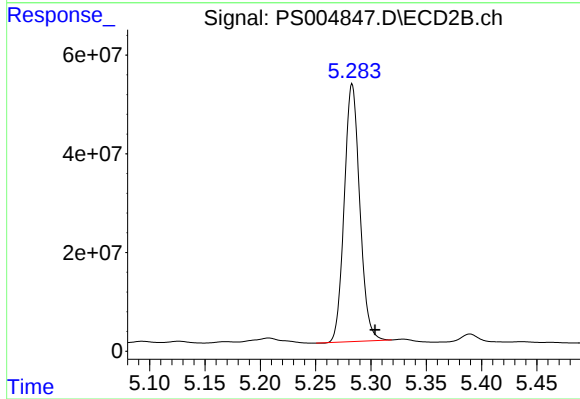


#4 2,4-DCAA

R.T.: 5.283 min
Delta R.T.: -0.021 min
Response: 510068797
Conc: 528.66 ng/ml

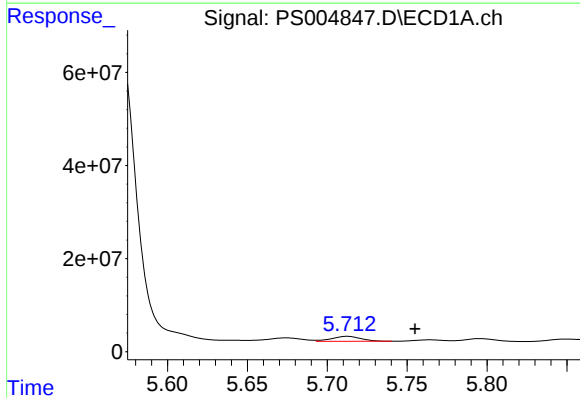


#5 DICAMBA

R.T.: 5.712 min
Delta R.T.: -0.043 min
Response: 13750036
Conc: 2.59 ng/ml

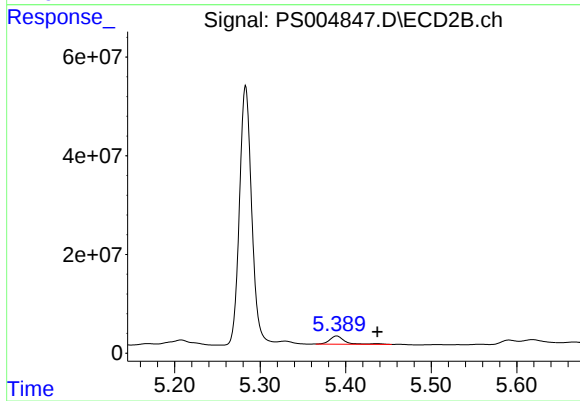

#5 DICAMBA


R.T.: 5.389 min
Delta R.T.: -0.048 min
Response: 20000213
Conc: 5.41 ng/ml

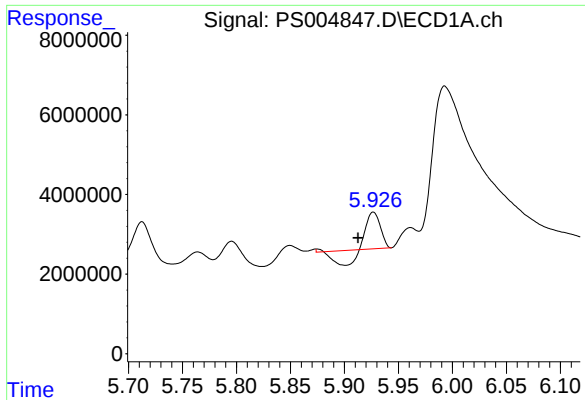

#6 MCPP


R.T.: 5.927 min
Delta R.T.: 0.014 min
Response: 4055597
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

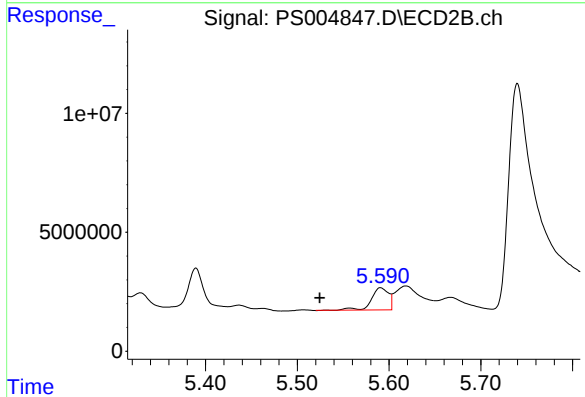


#6 MCPP

R.T.: 5.591 min
Delta R.T.: 0.067 min
Response: 11927688
Conc: 4.35 ug/ml

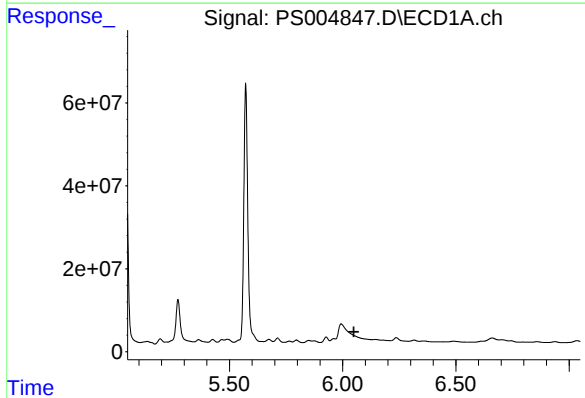


#7 MCPA

R.T.: 5.993 min
Delta R.T.: -0.056 min
Response: -6957124
Conc: N.D.

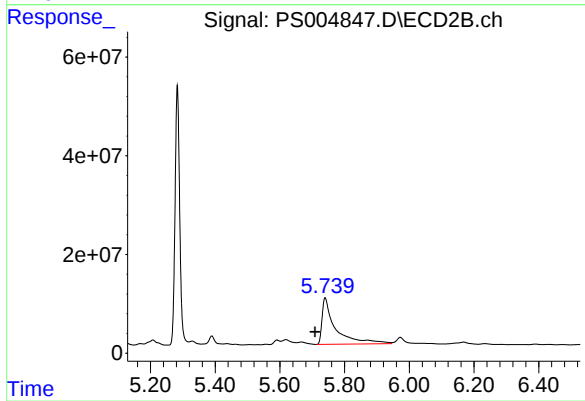

#7 MCPA


R.T.: 5.740 min
Delta R.T.: 0.031 min
Response: 273567878
Conc: 66.86 ug/ml

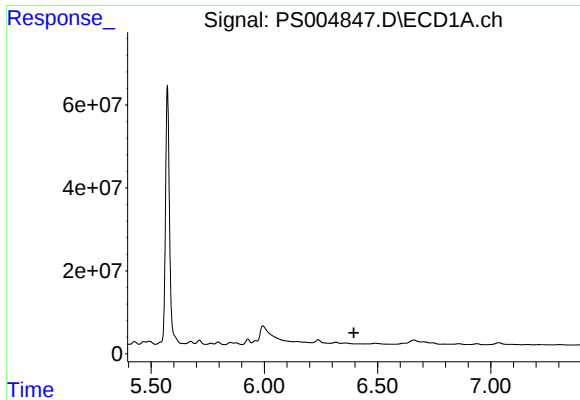

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

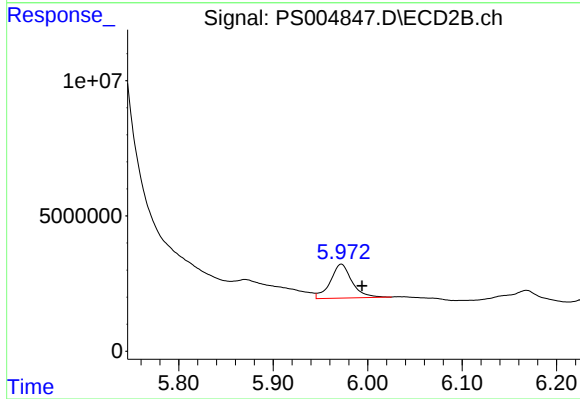


#8 DICHLORPROP

R.T.: 5.972 min
Delta R.T.: -0.022 min
Response: 20007051
Conc: 21.22 ng/ml

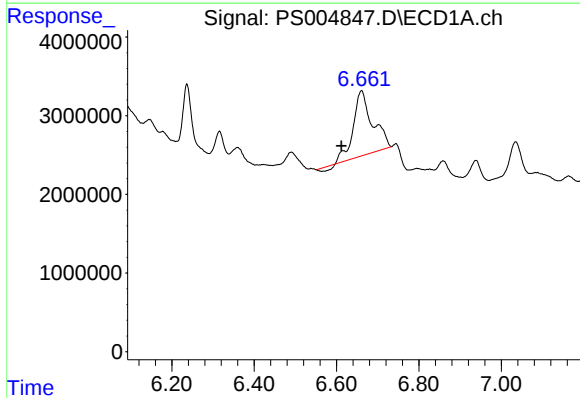


#9 2,4-D

R.T.: 6.660 min
Delta R.T.: 0.049 min
Response: 26030744
Conc: 19.03 ng/ml

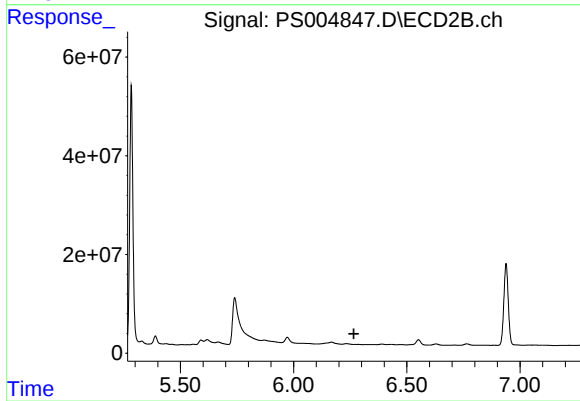

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

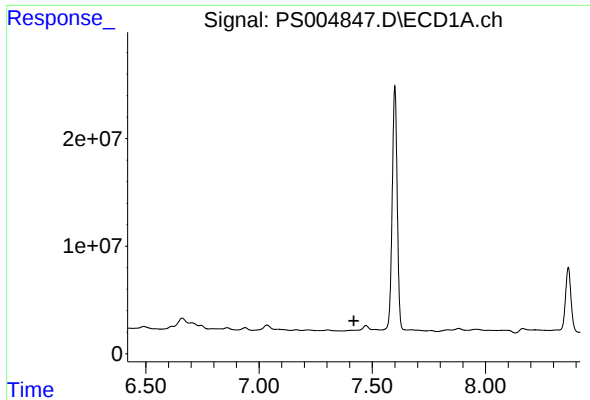

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

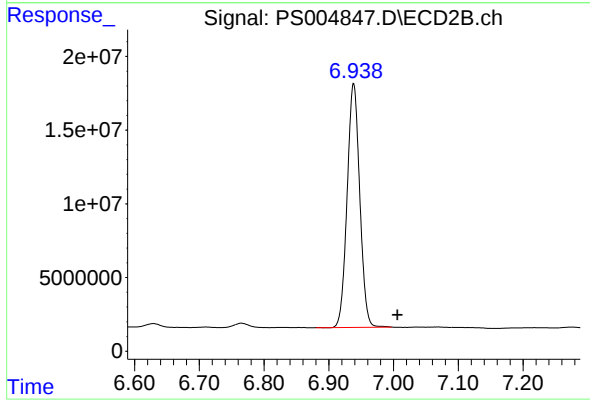

#11 2,4,5-TP (SILVEX)

R.T.: 6.938 min
Delta R.T.: -0.068 min
Response: 223633462
Conc: 43.46 ng/ml