

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053019\
 Data File : PS004850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2019 22:57
 Operator : SM\AJ
 Sample : K3041-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 02:24:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.576	5.287	767.9E6	496.4E6	547.807	514.508
Target Compounds							
2) T	3,5-DICHL...	4.994	4.606	20819306	322.1E6	12.072	261.419 #
3) T	4-Nitroph...	5.430	4.952	17884528	11040664	28.684	23.297
5) T	DICAMBA	5.716	5.394	21657144	15279554	4.079	4.136
6) T	MCP	5.931	0.000	8304538	0	1.995	N.D. #
7) T	MCPA	5.992	5.743	-5065658	369.1E6	N.D.	90.219
8) T	DICHLORPROP	0.000	5.976	0	21075437	N.D.	22.353
9) T	2,4-D	6.664	0.000	25158499	0	18.392	N.D. #
11) T	2,4,5-TP ...	0.000	6.944	0	247.5E6	N.D.	48.093



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053019\
Data File : PS004850.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2019 22:57
Operator : SM\AJ
Sample : K3041-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 02:24:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

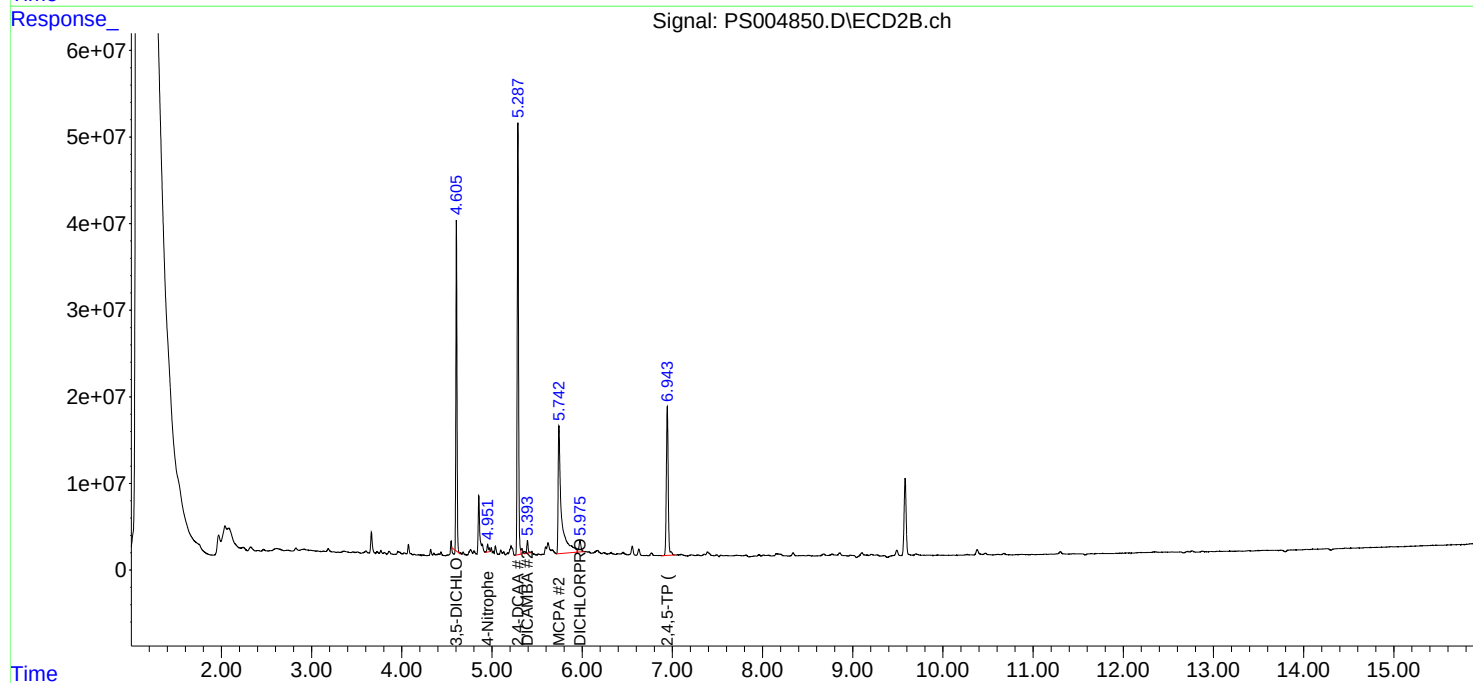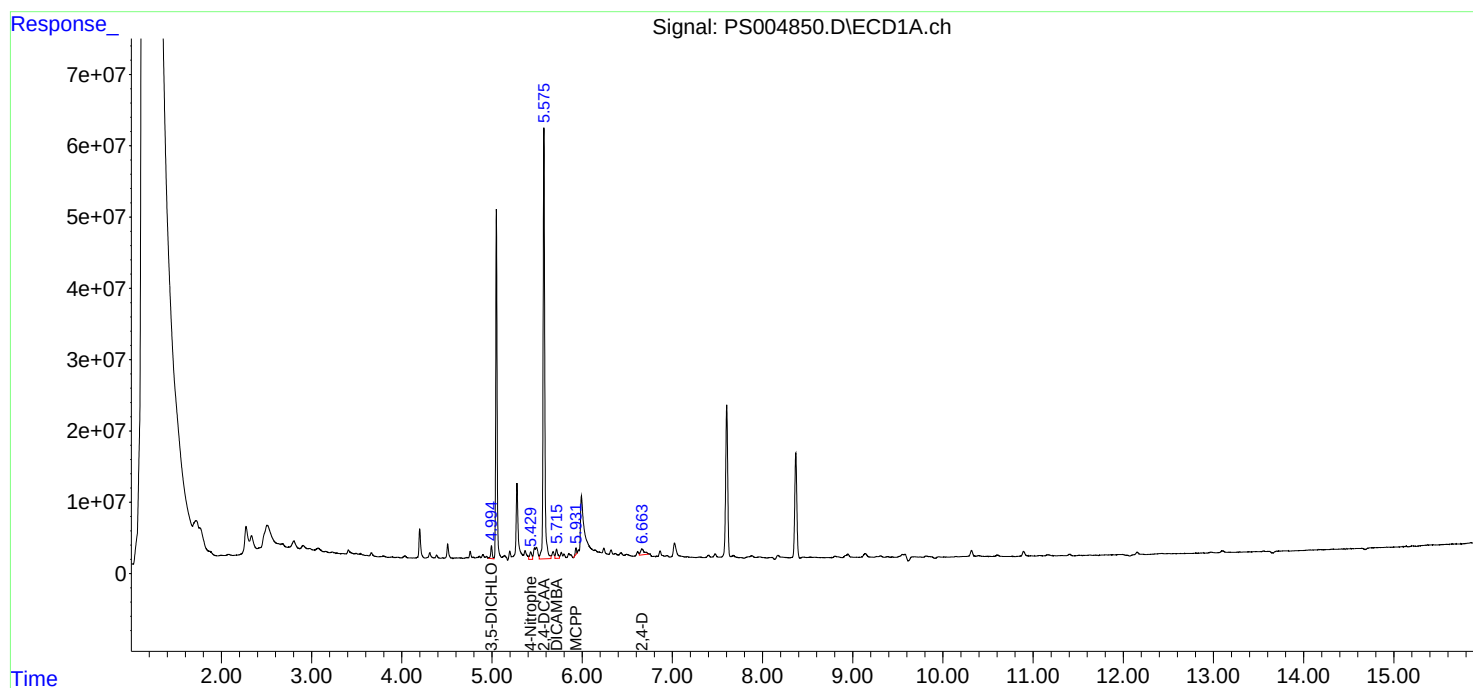


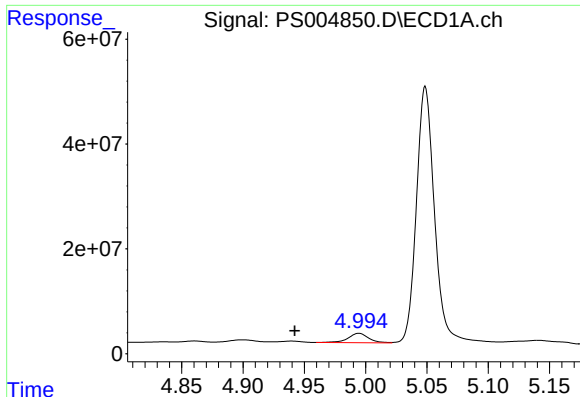

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.994 min
Delta R.T.: 0.052 min
Response: 20819306
Conc: 12.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

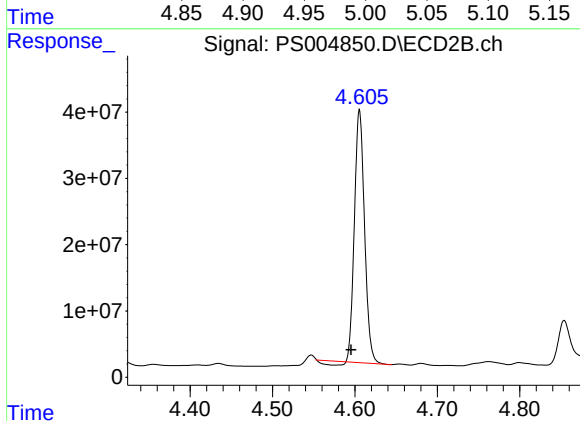


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.606 min
Delta R.T.: 0.010 min
Response: 322101378
Conc: 261.42 ng/ml

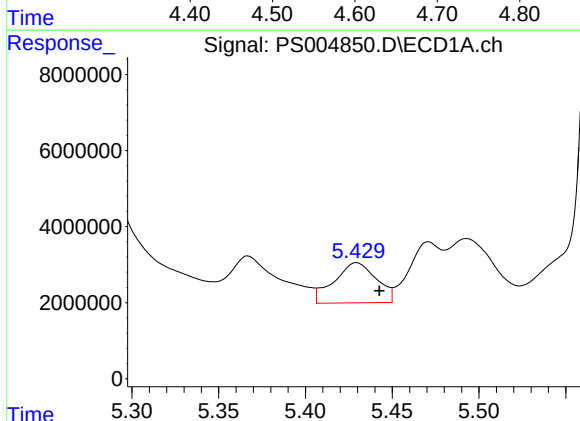


#3 4-Nitrophenol

R.T.: 5.430 min
Delta R.T.: -0.013 min
Response: 17884528
Conc: 28.68 ng/ml

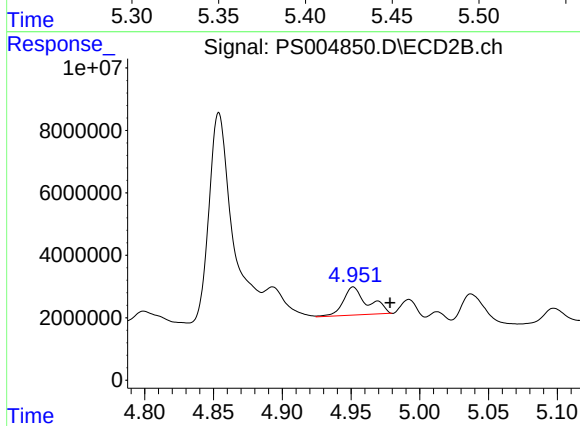

#3 4-Nitrophenol


R.T.: 4.952 min
Delta R.T.: -0.027 min
Response: 11040664
Conc: 23.30 ng/ml

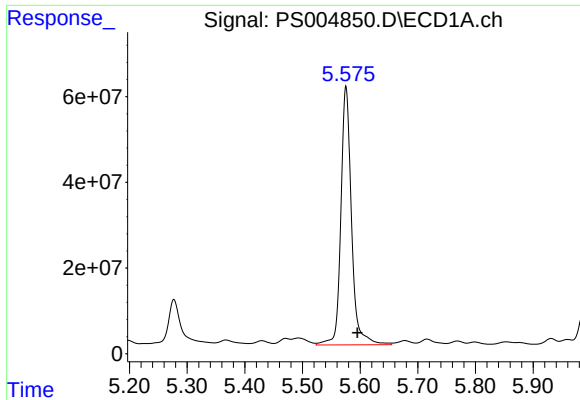

#4 2,4-DCAA


R.T.: 5.576 min
Delta R.T.: -0.019 min
Response: 767892139
Conc: 547.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

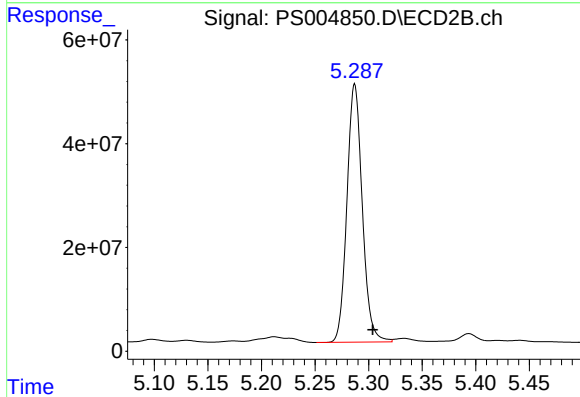


#4 2,4-DCAA

R.T.: 5.287 min
Delta R.T.: -0.017 min
Response: 496416233
Conc: 514.51 ng/ml

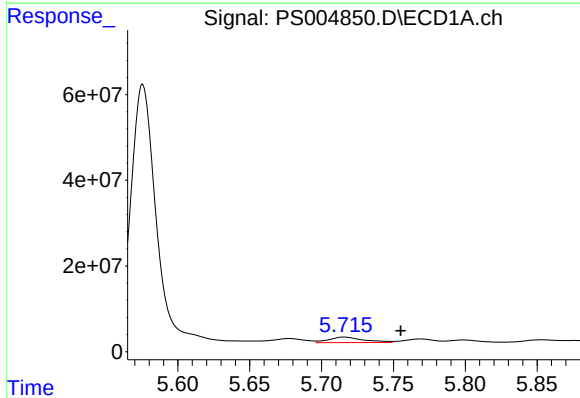


#5 DICAMBA

R.T.: 5.716 min
Delta R.T.: -0.039 min
Response: 21657144
Conc: 4.08 ng/ml

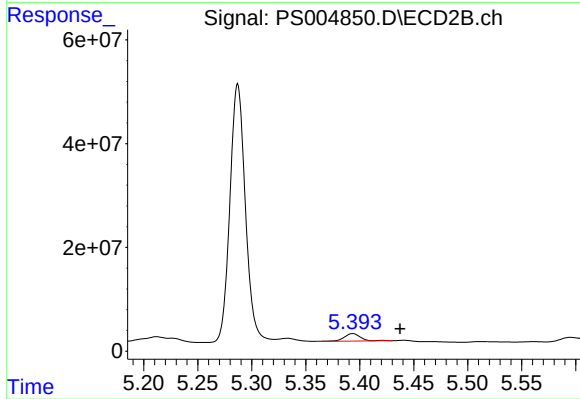

#5 DICAMBA


R.T.: 5.394 min
Delta R.T.: -0.044 min
Response: 15279554
Conc: 4.14 ng/ml

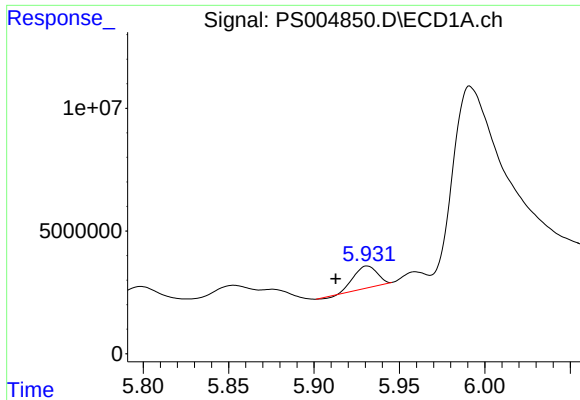

#6 MCPP


R.T.: 5.931 min
Delta R.T.: 0.019 min
Response: 8304538
Conc: 1.99 ug/ml

Instrument :
ECD_S
ClientSampleId :

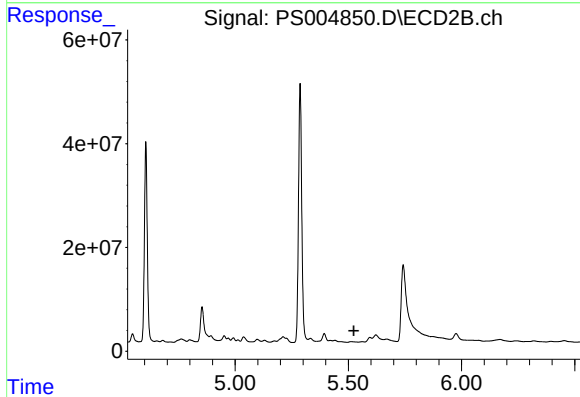


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

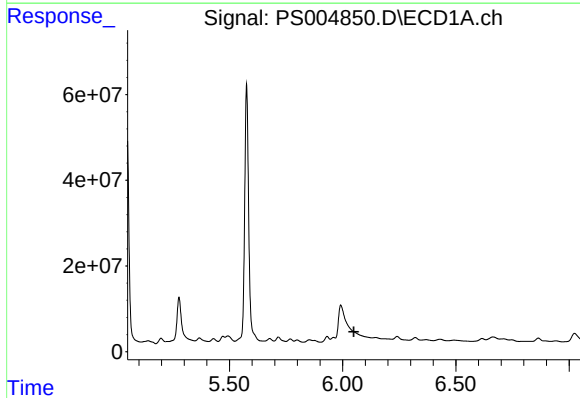


#7 MCPA

R.T.: 5.992 min
Delta R.T.: -0.057 min
Response: -5065658
Conc: N.D.

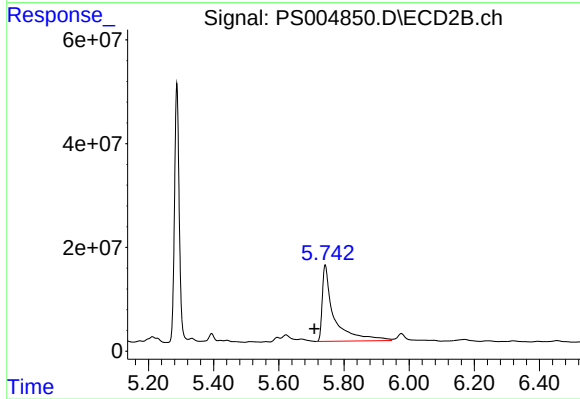

#7 MCPA


R.T.: 5.743 min
Delta R.T.: 0.033 min
Response: 369145713
Conc: 90.22 ug/ml

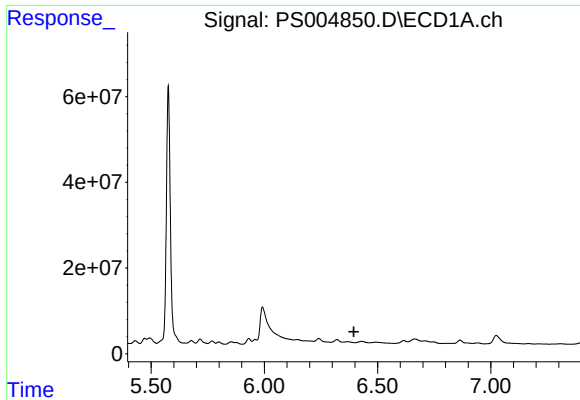

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

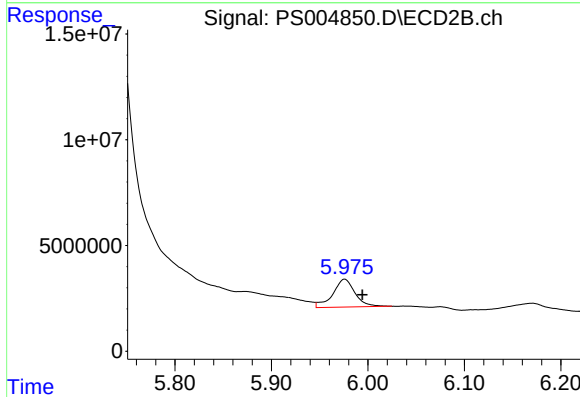


#8 DICHLORPROP

R.T.: 5.976 min
Delta R.T.: -0.018 min
Response: 21075437
Conc: 22.35 ng/ml

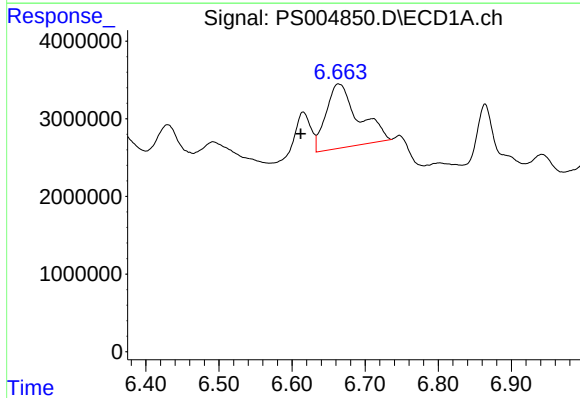


#9 2,4-D

R.T.: 6.664 min
Delta R.T.: 0.052 min
Response: 25158499
Conc: 18.39 ng/ml

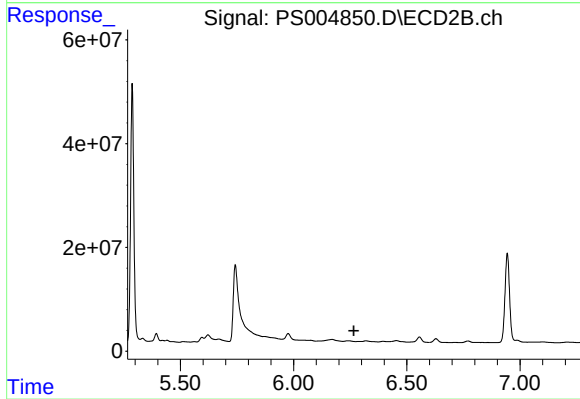

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

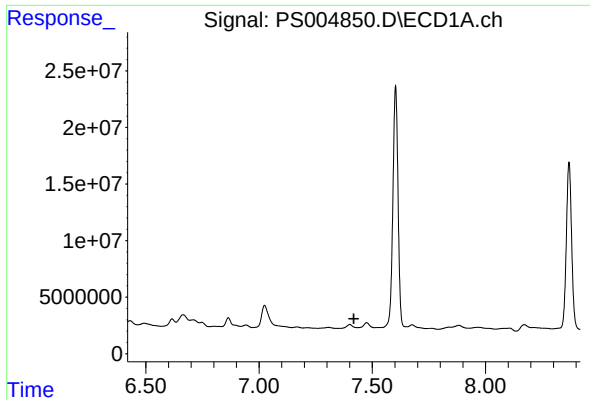

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

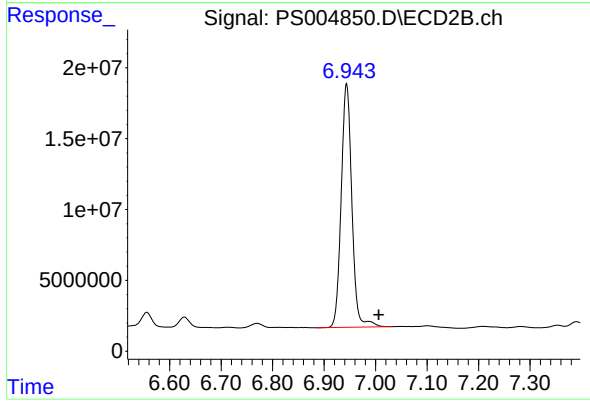

#11 2,4,5-TP (SILVEX)

R.T.: 6.944 min
Delta R.T.: -0.062 min
Response: 247452010
Conc: 48.09 ng/ml