

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053019\
 Data File : PS004851.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2019 23:19
 Operator : SM\AJ
 Sample : K3074-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 02:24:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.591	5.301	749.9E6	490.0E6	534.965	507.870
Target Compounds							
2) T	3,5-DICHL...	5.009	4.620	21803610	343.5E6	12.643	278.760 #
3) T	4-Nitroph...	5.444	4.966	16598571	13293606	26.621	28.050
5) T	DICAMBA	5.731	5.408	16581727	17062062	3.123	4.619 #
6) T	MCP	5.946	0.000	10414915	0	2.502	N.D. #
7) T	MCPA	0.000	5.758	0	428.8E6	N.D.	104.793
8) T	DICHLORPROP	0.000	5.990	0	24979016	N.D.	26.494
9) T	2,4-D	6.679	0.000	12580081	0	9.197	N.D. #
11) T	2,4,5-TP ...	0.000	6.957	0	240.2E6	N.D.	46.690



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053019\
Data File : PS004851.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2019 23:19
Operator : SM\AJ
Sample : K3074-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 02:24:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

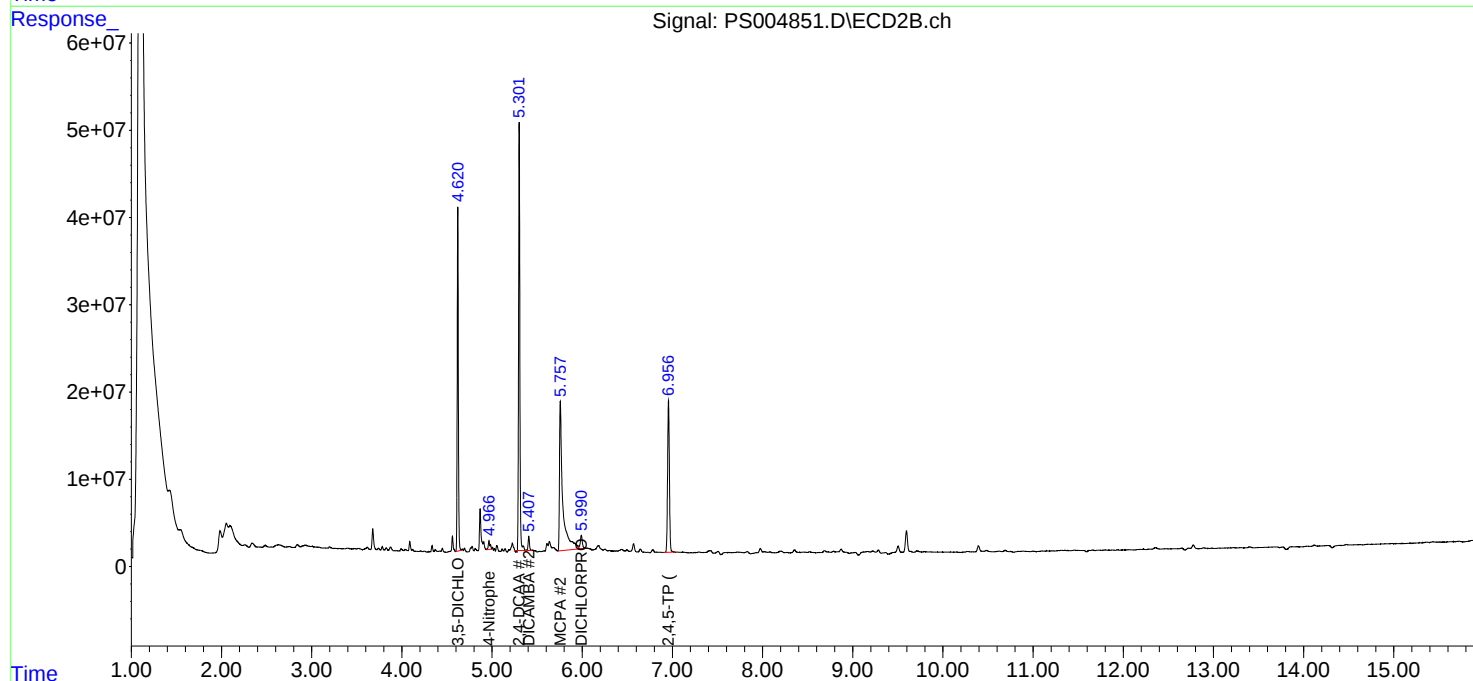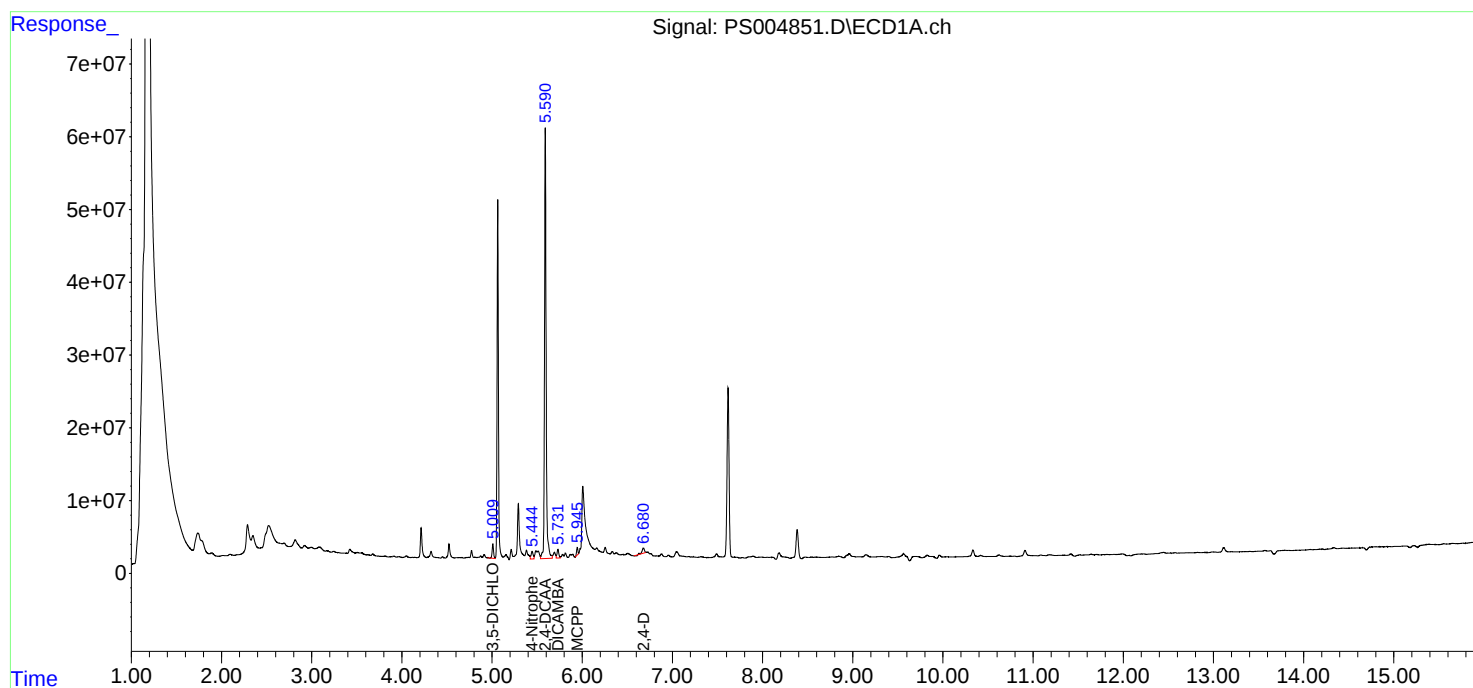


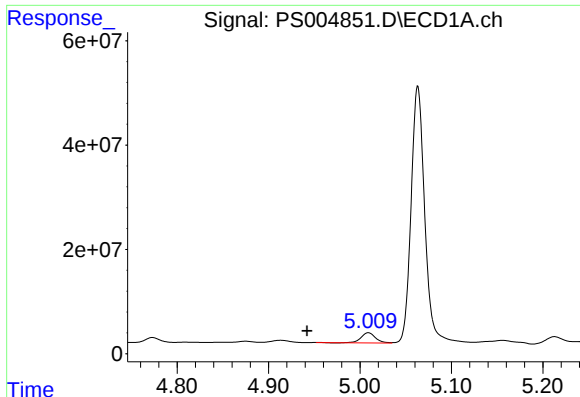

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.009 min
Delta R.T.: 0.067 min
Response: 21803610
Conc: 12.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

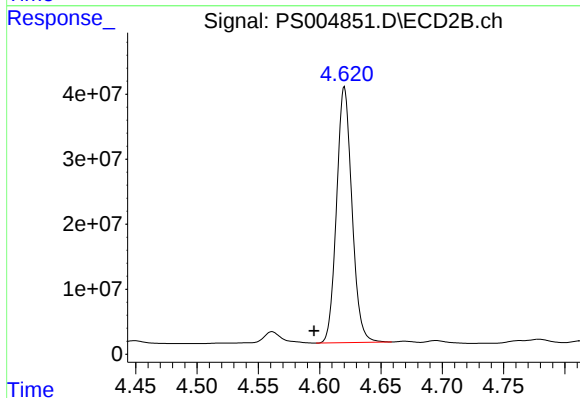


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.620 min
Delta R.T.: 0.025 min
Response: 343468574
Conc: 278.76 ng/ml

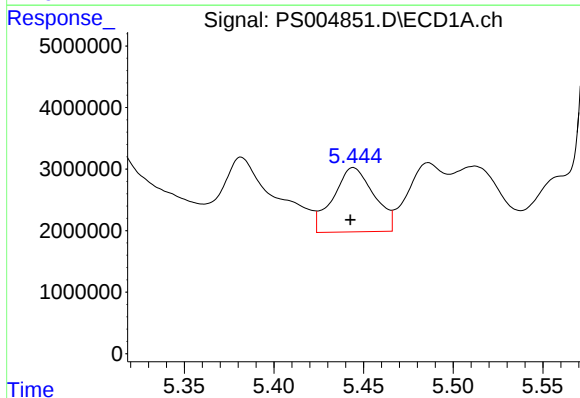


#3 4-Nitrophenol

R.T.: 5.444 min
Delta R.T.: 0.002 min
Response: 16598571
Conc: 26.62 ng/ml

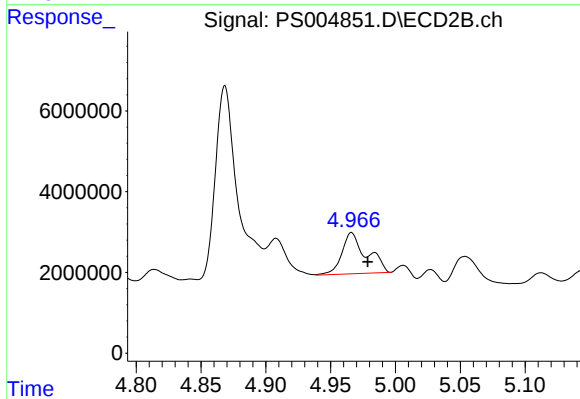

#3 4-Nitrophenol


R.T.: 4.966 min
Delta R.T.: -0.012 min
Response: 13293606
Conc: 28.05 ng/ml

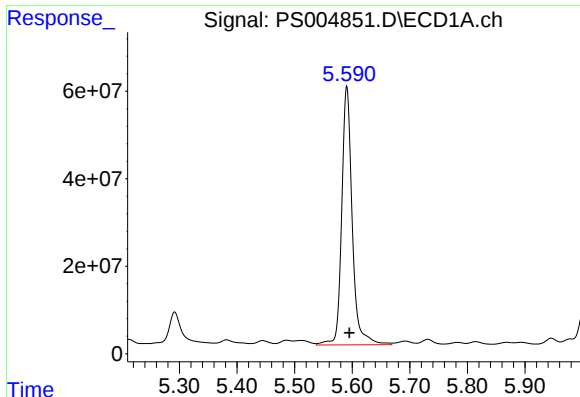

#4 2,4-DCAA


R.T.: 5.591 min
Delta R.T.: -0.004 min
Response: 749889788
Conc: 534.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

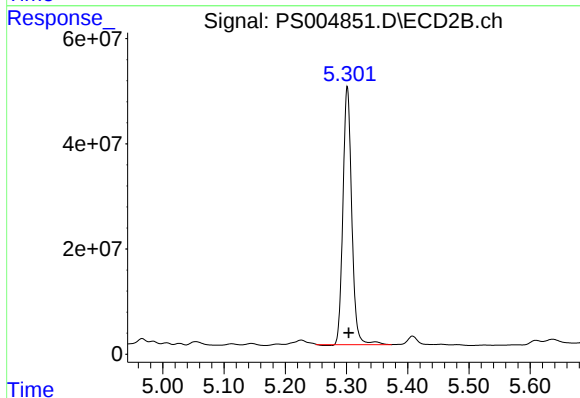


#4 2,4-DCAA

R.T.: 5.301 min
Delta R.T.: -0.002 min
Response: 490011330
Conc: 507.87 ng/ml

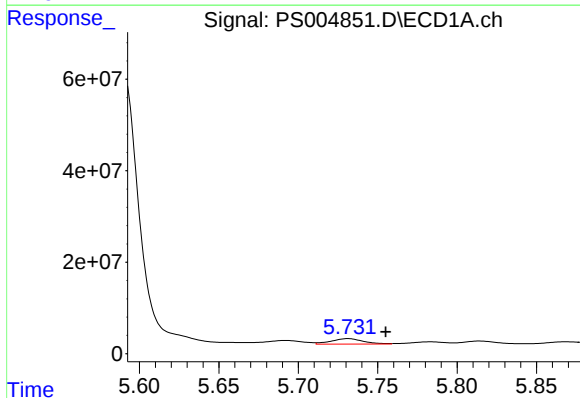


#5 DICAMBA

R.T.: 5.731 min
Delta R.T.: -0.024 min
Response: 16581727
Conc: 3.12 ng/ml

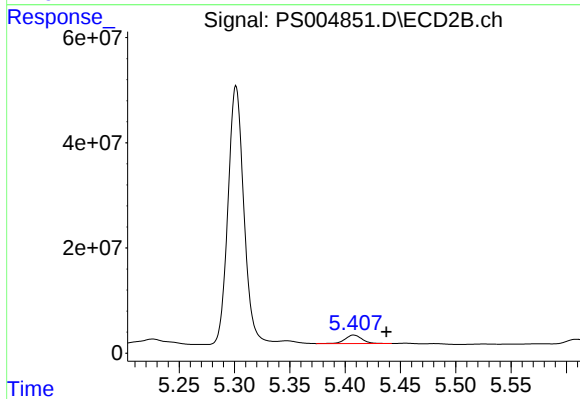

#5 DICAMBA


R.T.: 5.408 min
Delta R.T.: -0.029 min
Response: 17062062
Conc: 4.62 ng/ml

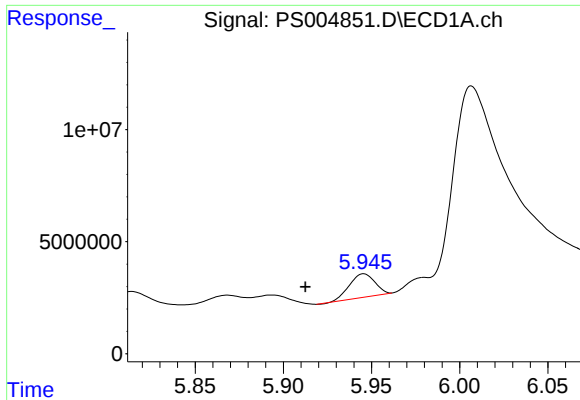

#6 MCPP


R.T.: 5.946 min
Delta R.T.: 0.033 min
Response: 10414915
Conc: 2.50 ug/ml

Instrument :
ECD_S
ClientSampleId :

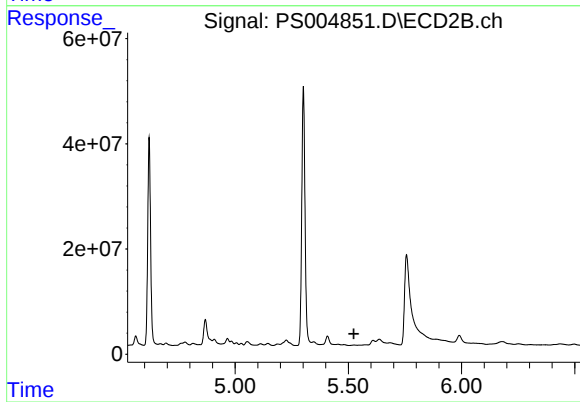


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

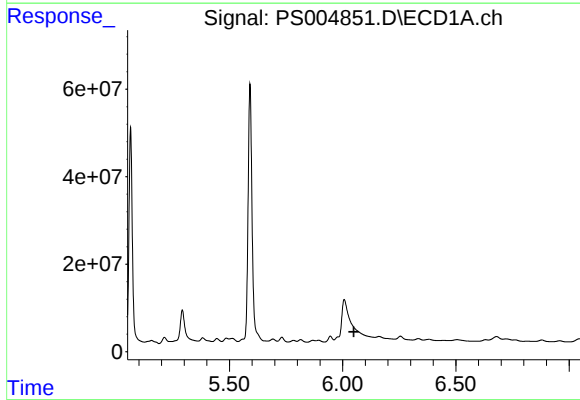


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

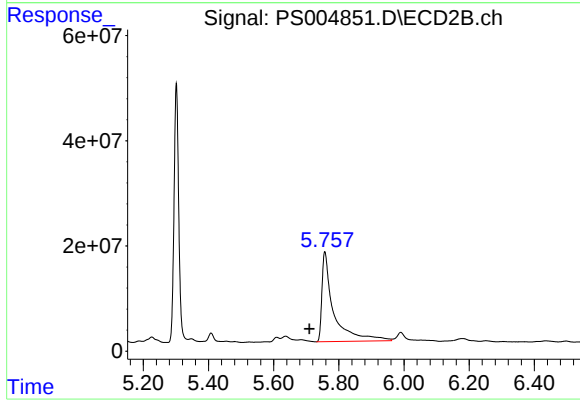

#7 MCPA


R.T.: 5.758 min
Delta R.T.: 0.048 min
Response: 428776087
Conc: 104.79 ug/ml

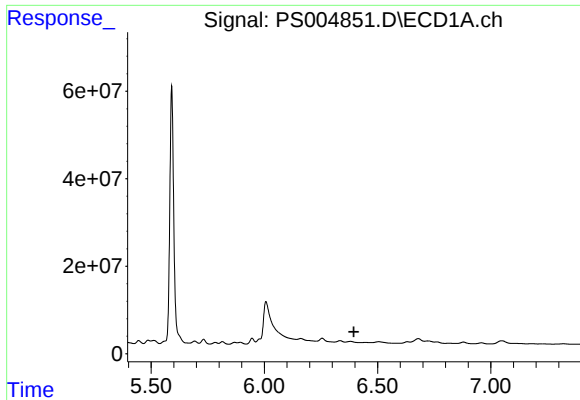

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

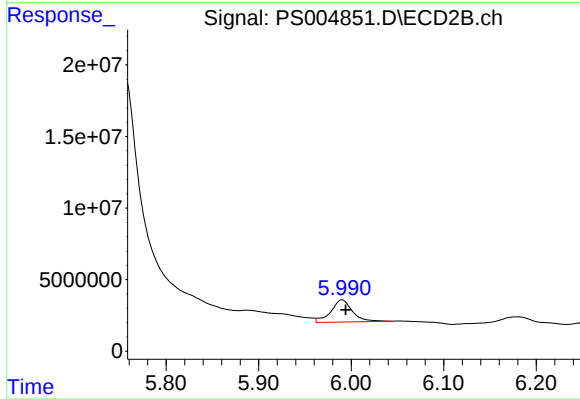


#8 DICHLORPROP

R.T.: 5.990 min
Delta R.T.: -0.004 min
Response: 24979016
Conc: 26.49 ng/ml

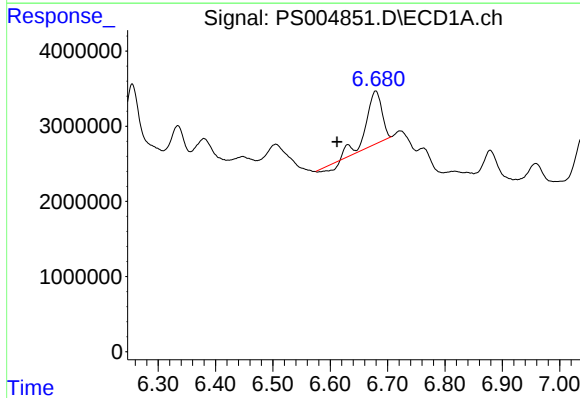


#9 2,4-D

R.T.: 6.679 min
Delta R.T.: 0.067 min
Response: 12580081
Conc: 9.20 ng/ml

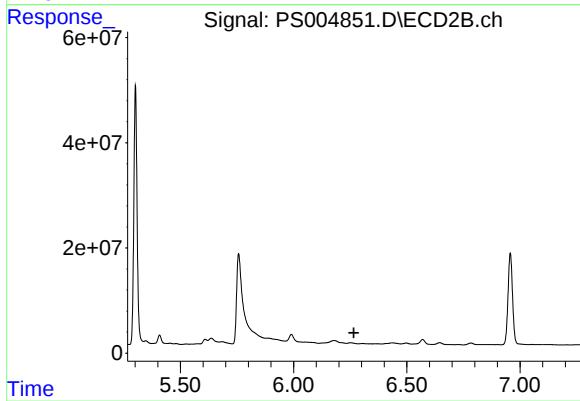

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

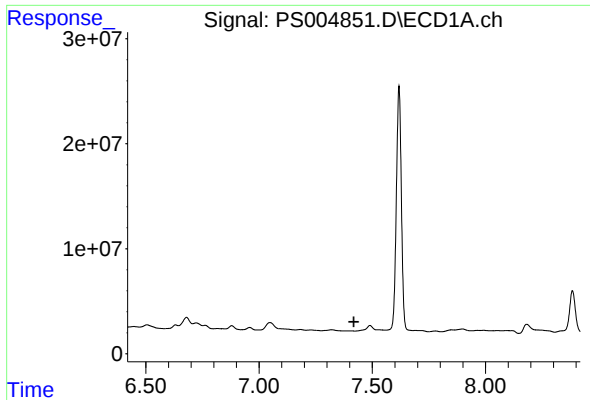

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

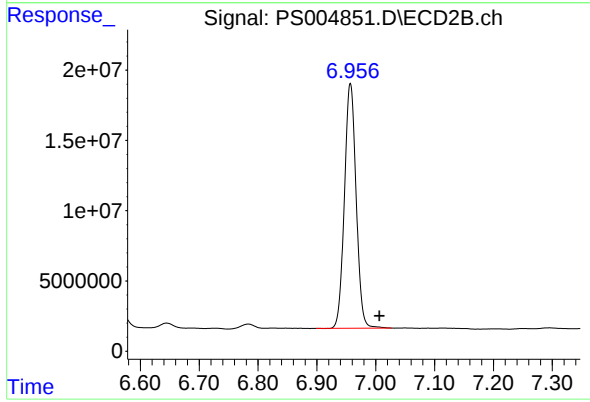

#11 2,4,5-TP (SILVEX)

R.T.: 6.957 min
Delta R.T.: -0.049 min
Response: 240236089
Conc: 46.69 ng/ml