

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053019\
 Data File : PS004852.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2019 23:41
 Operator : SM\AJ
 Sample : K3074-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 02:24:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.571	5.283	679.0E6	436.0E6	484.394	451.872
Target Compounds							
2) T	3,5-DICHL...	4.990	4.601	35809397	585.7E6	20.764	475.342 #
3) T	4-Nitroph...	5.425	4.947	26047654	37709206	41.776	79.569 #
5) T	DICAMBA	5.712	5.389	26809512	35185260	5.049	9.524 #
6) T	MCP	5.926	5.590	21806080	4892755	5.238	1.786 #
7) T	MCPA	5.992	5.741	2454109	289.2E6	<MDL	70.685 #
8) T	DICHLORPROP	0.000	5.971	0	20977029	N.D.	22.249
9) T	2,4-D	6.659	0.000	10213748	0	7.467	N.D. #
11) T	2,4,5-TP ...	0.000	6.938	0	419.3E6	N.D.	81.484



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053019\
Data File : PS004852.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2019 23:41
Operator : SM\AJ
Sample : K3074-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 02:24:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

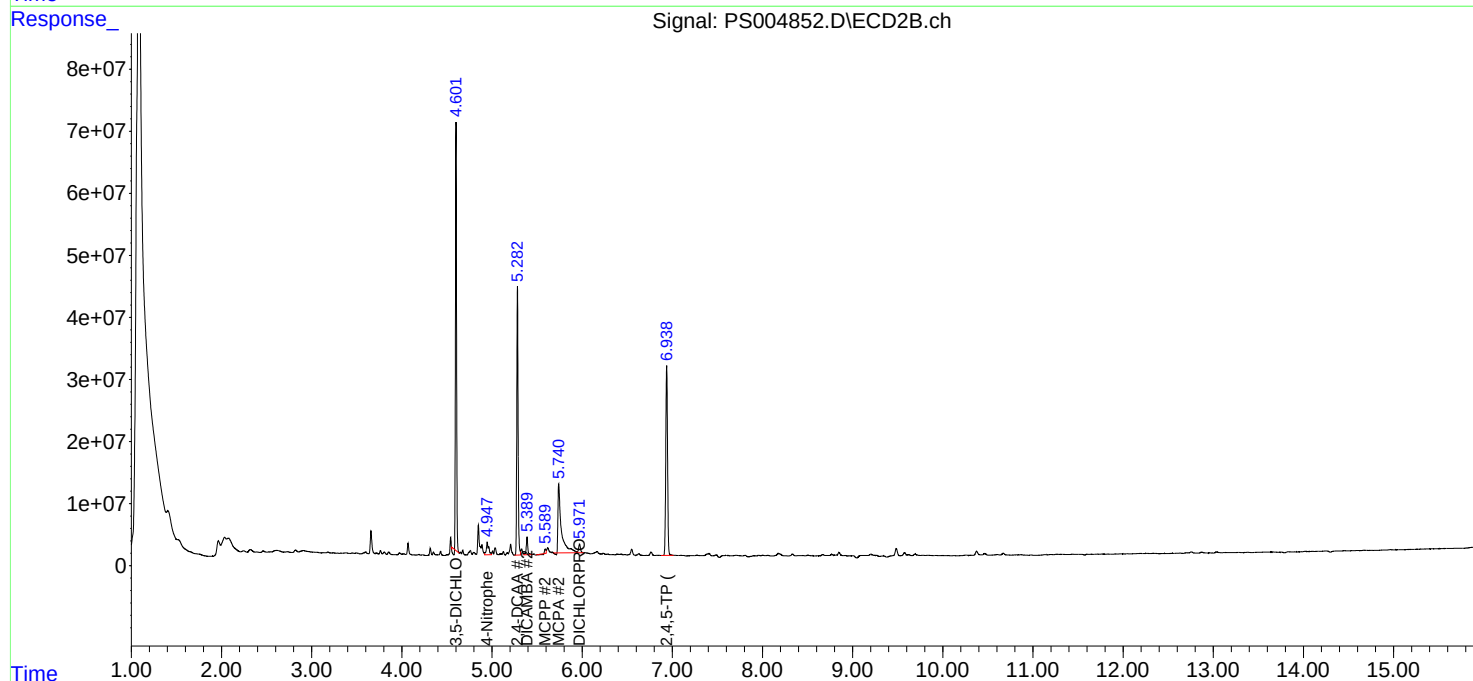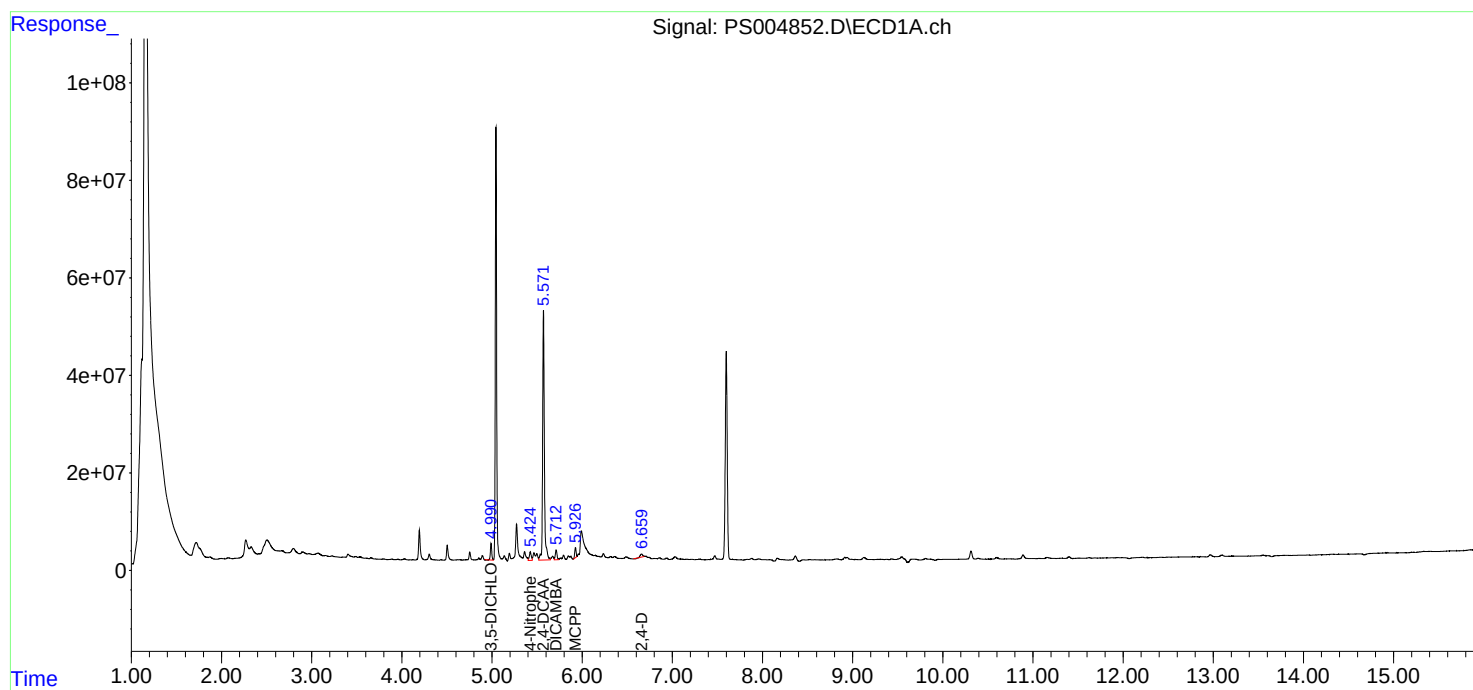


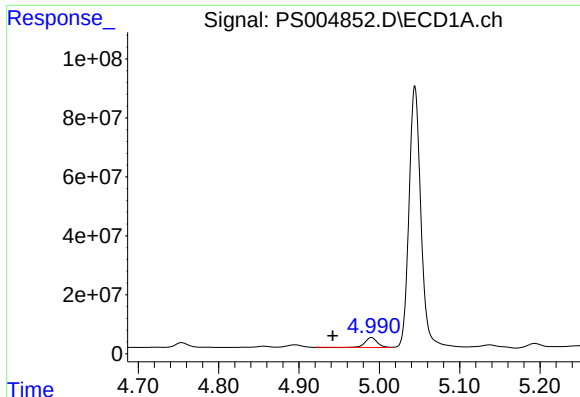

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.990 min
Delta R.T.: 0.048 min
Response: 35809397
Conc: 20.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

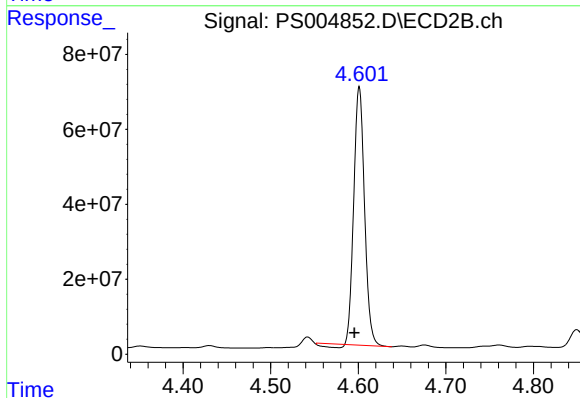


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.601 min
Delta R.T.: 0.006 min
Response: 585681888
Conc: 475.34 ng/ml

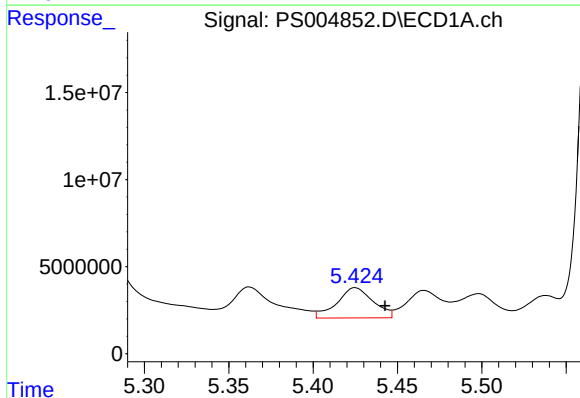


#3 4-Nitrophenol

R.T.: 5.425 min
Delta R.T.: -0.018 min
Response: 26047654
Conc: 41.78 ng/ml

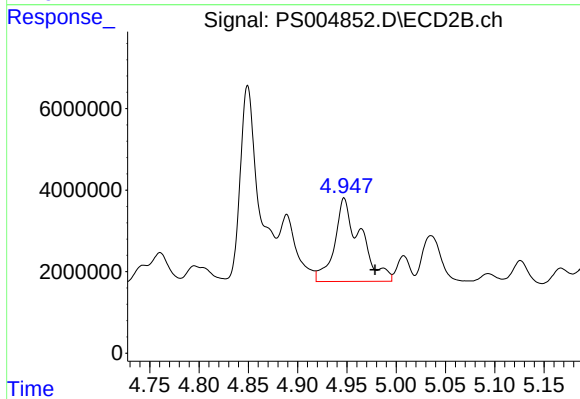

#3 4-Nitrophenol


R.T.: 4.947 min
Delta R.T.: -0.031 min
Response: 37709206
Conc: 79.57 ng/ml

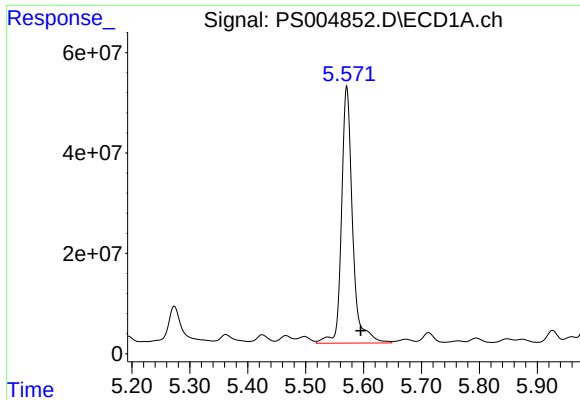

#4 2,4-DCAA


R.T.: 5.571 min
Delta R.T.: -0.024 min
Response: 679002773
Conc: 484.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

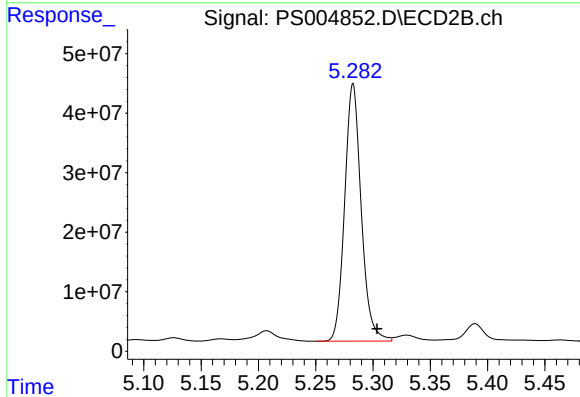


#4 2,4-DCAA

R.T.: 5.283 min
Delta R.T.: -0.021 min
Response: 435982449
Conc: 451.87 ng/ml

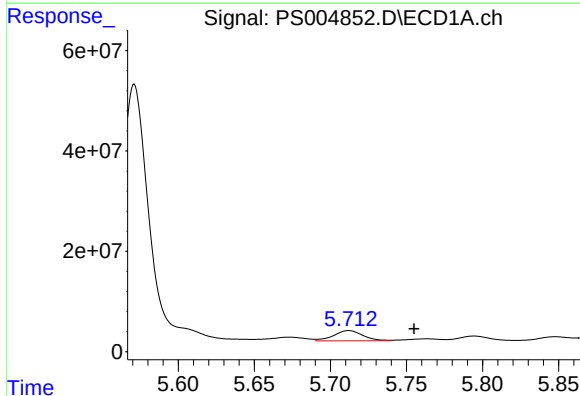


#5 DICAMBA

R.T.: 5.712 min
Delta R.T.: -0.043 min
Response: 26809512
Conc: 5.05 ng/ml

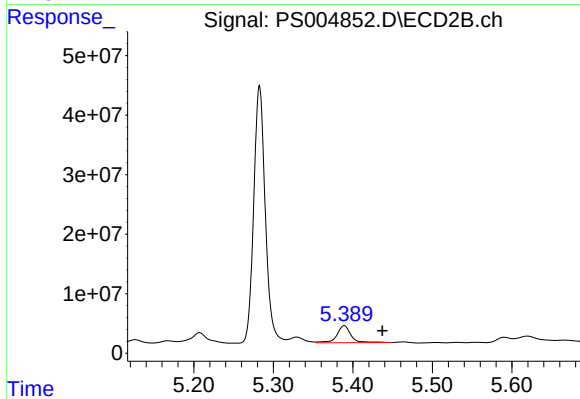

#5 DICAMBA


R.T.: 5.389 min
Delta R.T.: -0.048 min
Response: 35185260
Conc: 9.52 ng/ml

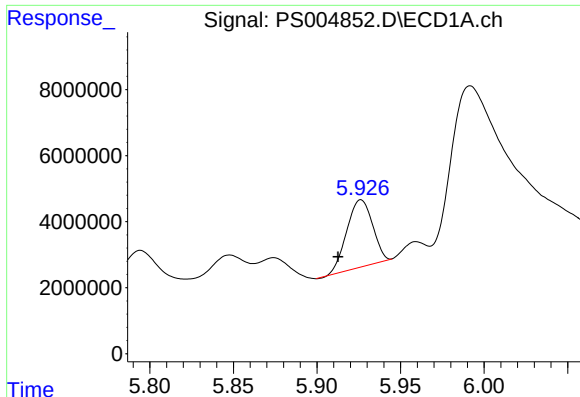

#6 MCPP


R.T.: 5.926 min
Delta R.T.: 0.014 min
Response: 21806080
Conc: 5.24 ug/ml

Instrument :
ECD_S
ClientSampleId :

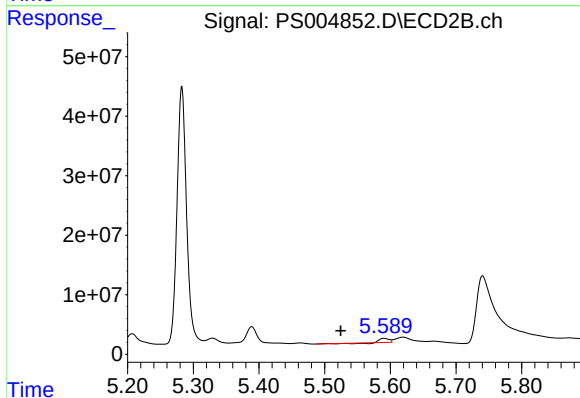


#6 MCPP

R.T.: 5.590 min
Delta R.T.: 0.066 min
Response: 4892755
Conc: 1.79 ug/ml

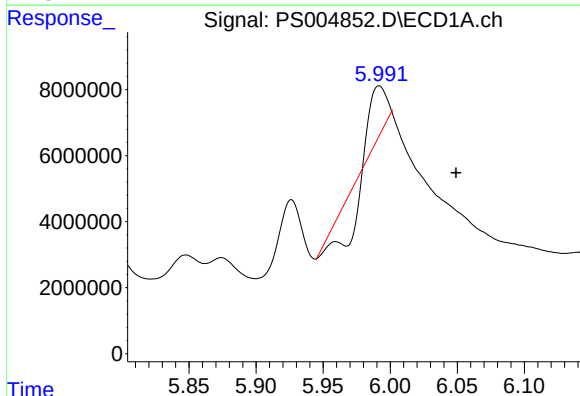


#7 MCPA

R.T.: 5.992 min
Delta R.T.: -0.057 min
Response: 2454109
Conc: N.D.

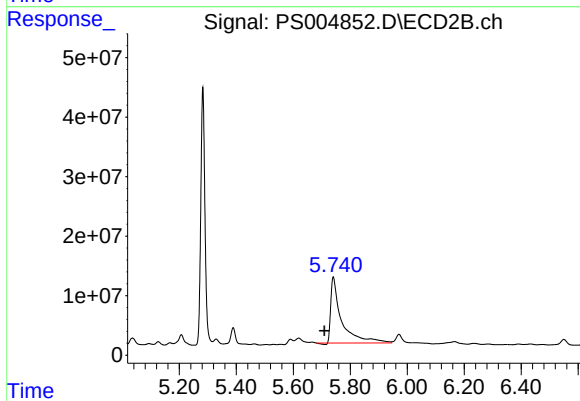

#7 MCPA


R.T.: 5.741 min
Delta R.T.: 0.032 min
Response: 289219812
Conc: 70.69 ug/ml

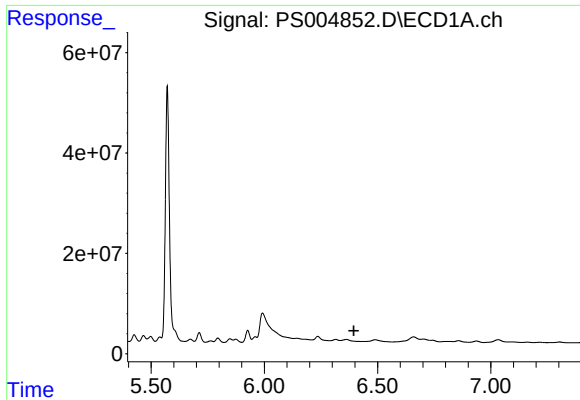

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

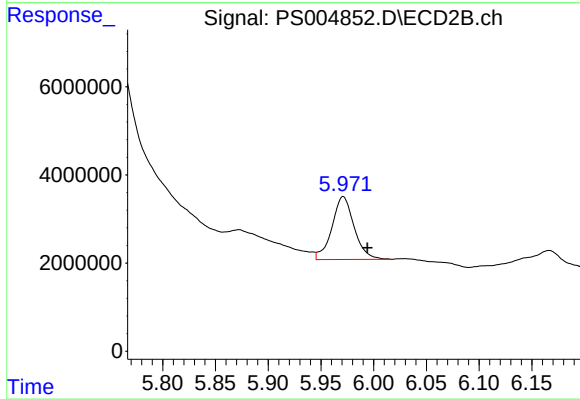


#8 DICHLORPROP

R.T.: 5.971 min
Delta R.T.: -0.023 min
Response: 20977029
Conc: 22.25 ng/ml

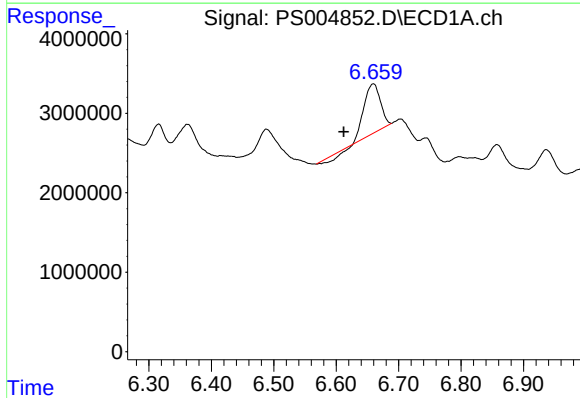


#9 2,4-D

R.T.: 6.659 min
Delta R.T.: 0.047 min
Response: 10213748
Conc: 7.47 ng/ml

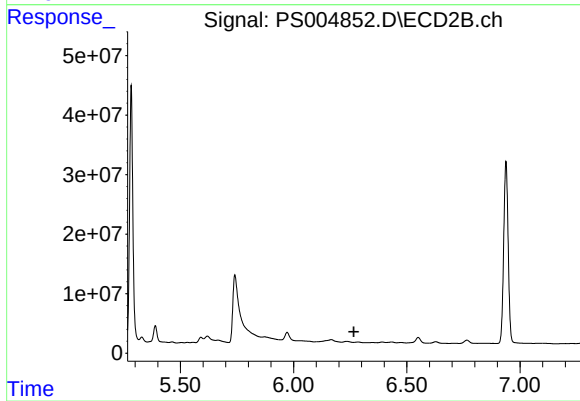

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

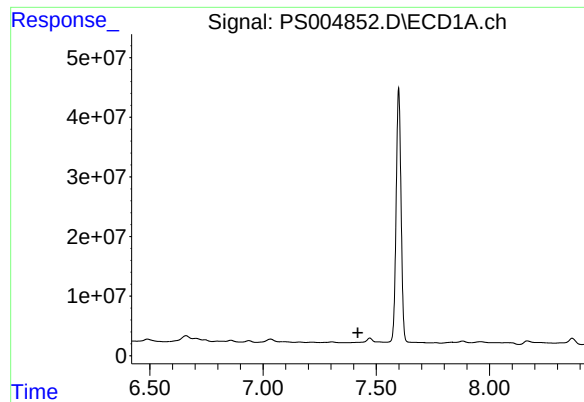

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

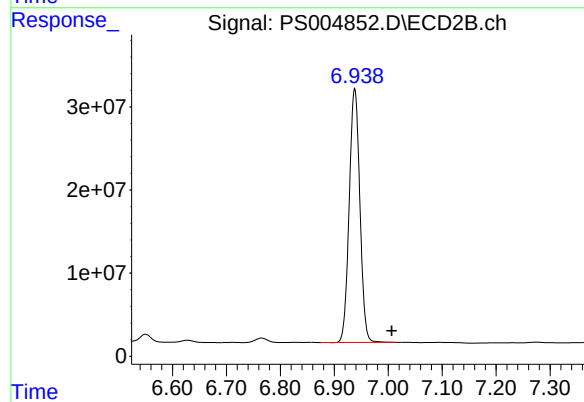

#11 2,4,5-TP (SILVEX)

R.T.: 6.938 min
Delta R.T.: -0.068 min
Response: 419260287
Conc: 81.48 ng/ml