

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053119\
 Data File : PS004859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2019 10:09
 Operator : SM\AJ
 Sample : K2648-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TR-04-052919

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 00:57:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.591	5.283	591.8E6	412.8E6	422.176	427.812
Target Compounds							
1) T	Dalapon	2.092	0.000	22248333	0	13.421	N.D. #
2) T	3,5-DICHL...	5.009	4.602	23117927	261.7E6	13.405	212.397 #
3) T	4-Nitroph...	5.382	4.947	32650712	22808819	52.366	48.128
5) T	DICAMBA	5.814	5.389	14658297	20654256	2.761	5.591 #
6) T	MCPD	5.946	0.000	8894391	0	2.137	N.D. #
7) T	MCPA	0.000	5.740	0	332.3E6	N.D.	81.223
8) T	DICHLORPROP	0.000	5.972	0	22245526	N.D.	23.594
9) T	2,4-D	6.677	0.000	20718878	0	15.146	N.D. #
11) T	2,4,5-TP ...	0.000	6.938	0	154.4E6	N.D.	30.013



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053119\
Data File : PS004859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2019 10:09
Operator : SM\AJ
Sample : K2648-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TR-04-052919

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 00:57:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

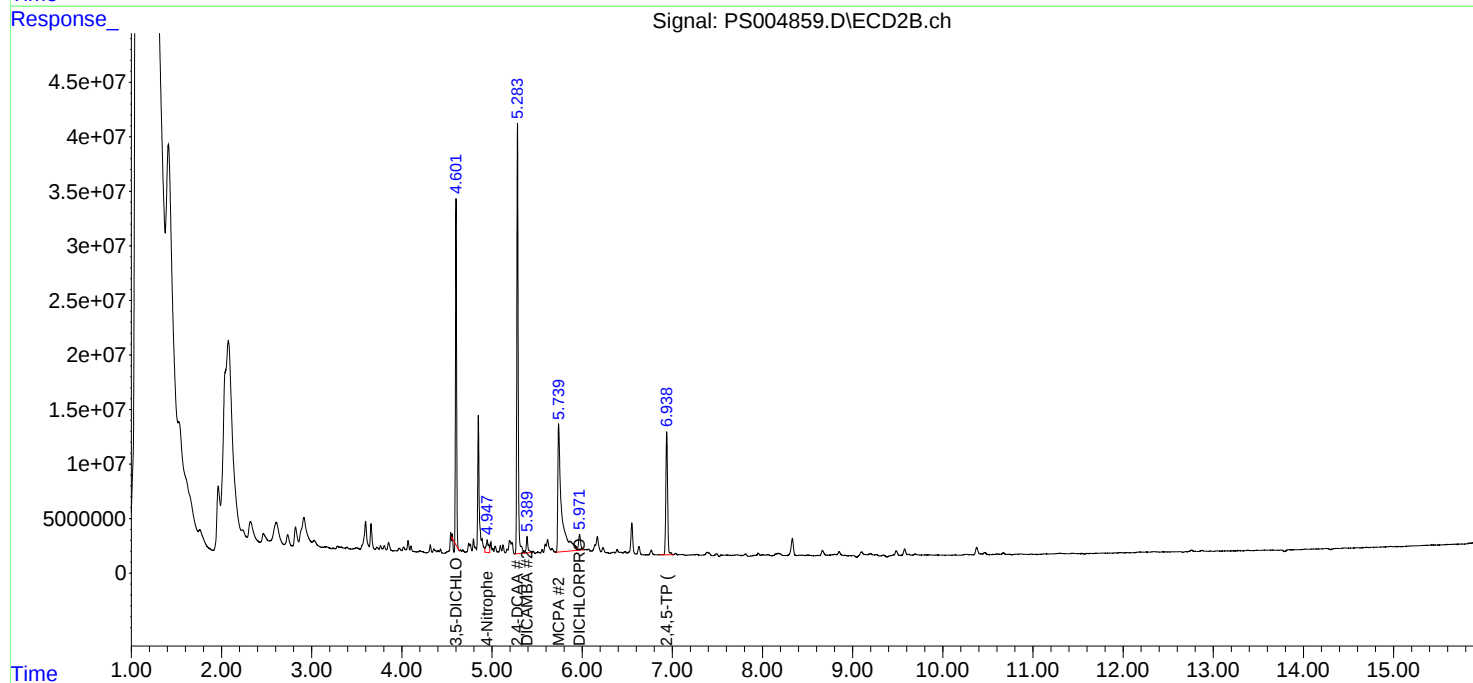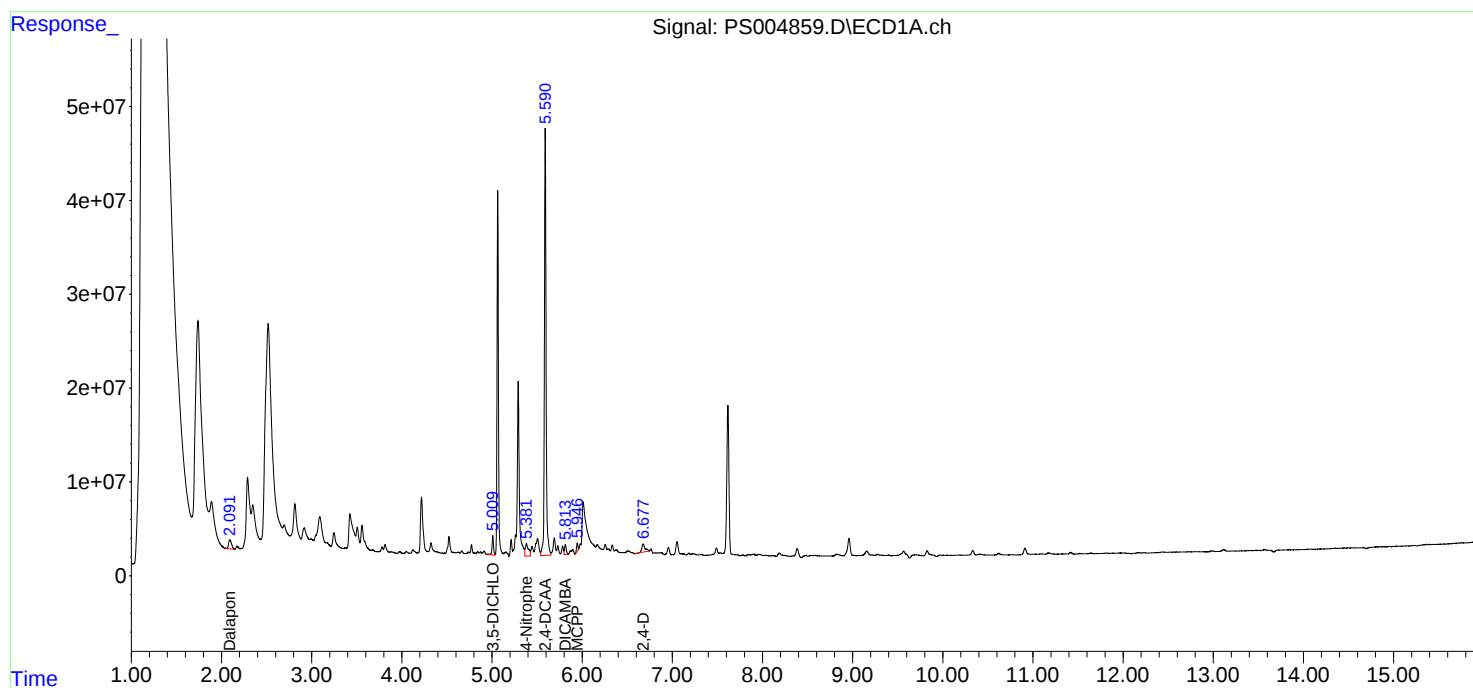


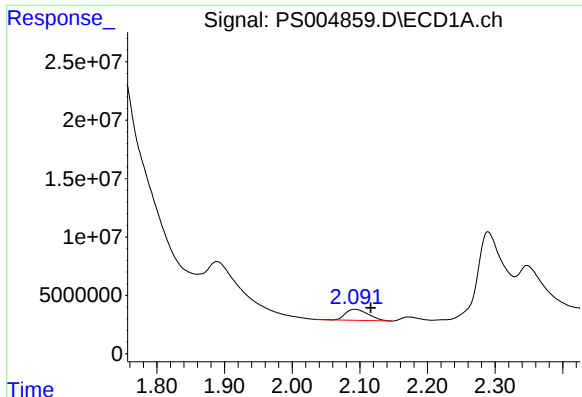

#1 Dalapon


R.T.: 2.092 min
Delta R.T.: -0.024 min
Response: 22248333
Conc: 13.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-052919

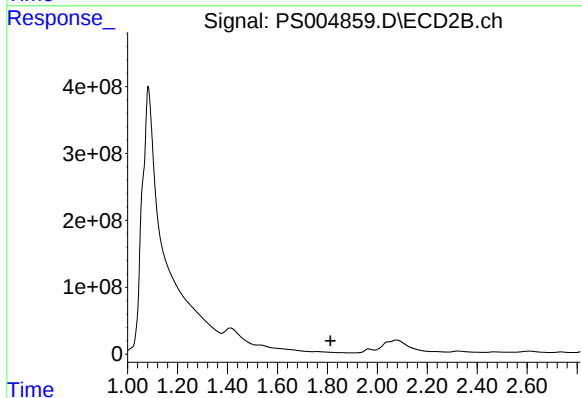


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

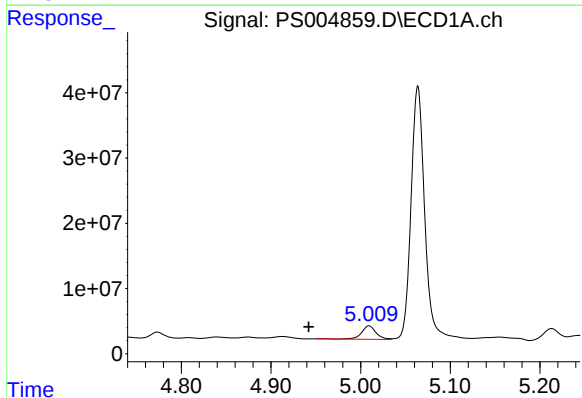


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.009 min
Delta R.T.: 0.067 min
Response: 23117927
Conc: 13.41 ng/ml

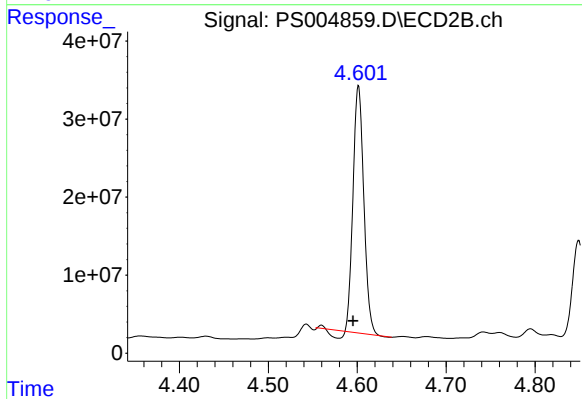

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.602 min
Delta R.T.: 0.006 min
Response: 261699887
Conc: 212.40 ng/ml

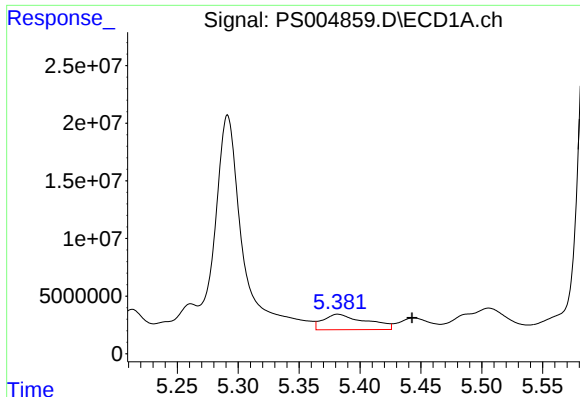

#3 4-Nitrophenol


R.T.: 5.382 min
Delta R.T.: -0.061 min
Response: 32650712
Conc: 52.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-052919

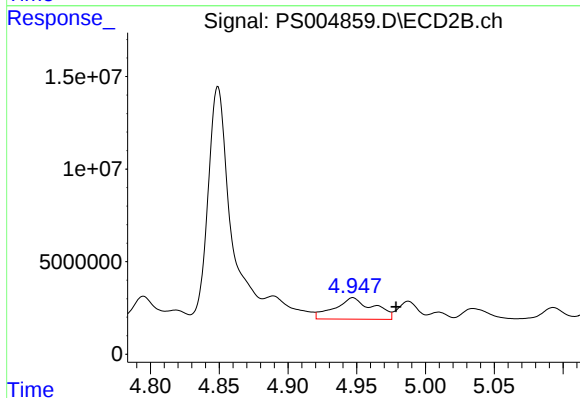


#3 4-Nitrophenol

R.T.: 4.947 min
Delta R.T.: -0.031 min
Response: 22808819
Conc: 48.13 ng/ml

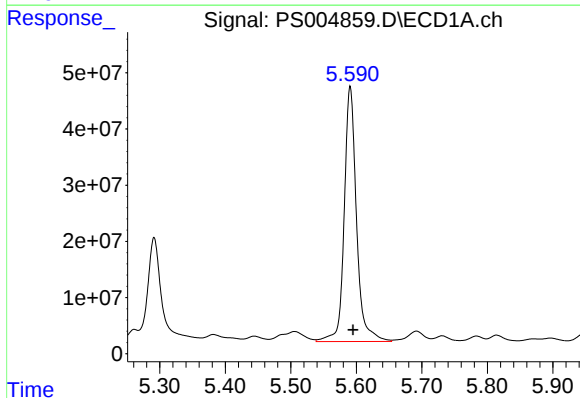


#4 2,4-DCAA

R.T.: 5.591 min
Delta R.T.: -0.004 min
Response: 591787636
Conc: 422.18 ng/ml

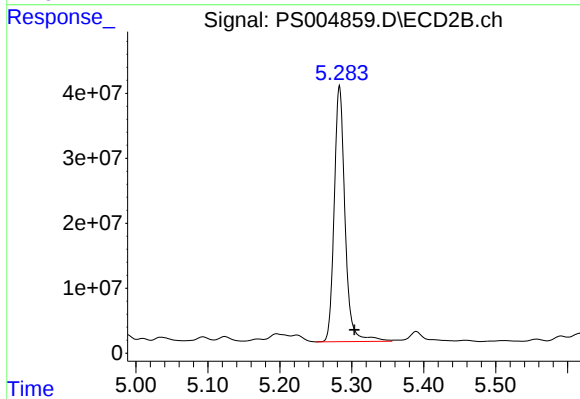

#4 2,4-DCAA


R.T.: 5.283 min
Delta R.T.: -0.021 min
Response: 412768365
Conc: 427.81 ng/ml

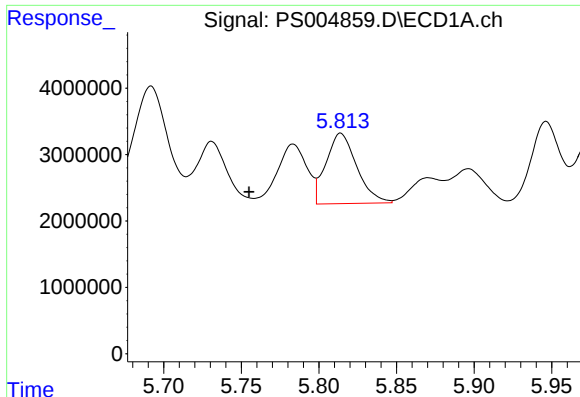

#5 DICAMBA


R.T.: 5.814 min
Delta R.T.: 0.059 min
Response: 14658297
Conc: 2.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-052919

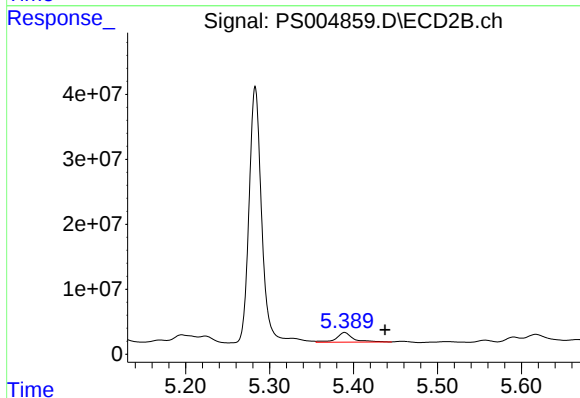


#5 DICAMBA

R.T.: 5.389 min
Delta R.T.: -0.048 min
Response: 20654256
Conc: 5.59 ng/ml

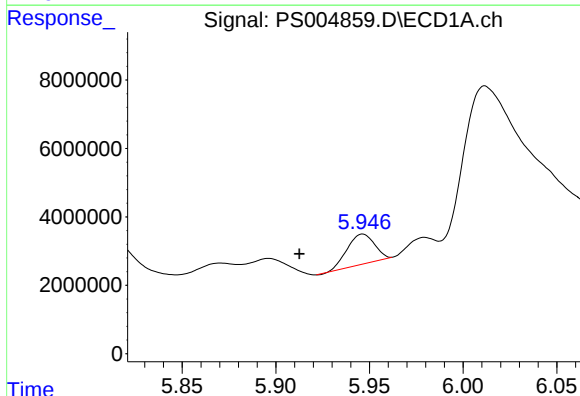


#6 MCP

R.T.: 5.946 min
Delta R.T.: 0.034 min
Response: 8894391
Conc: 2.14 ug/ml

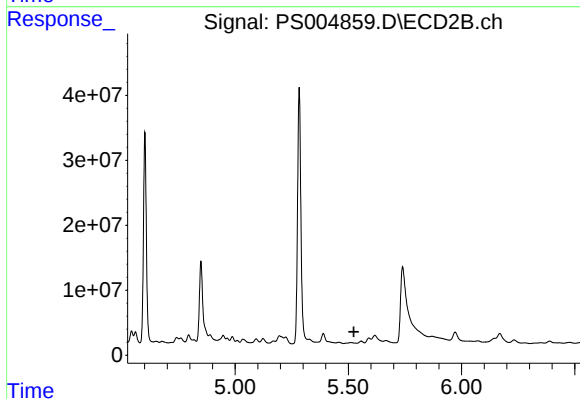

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

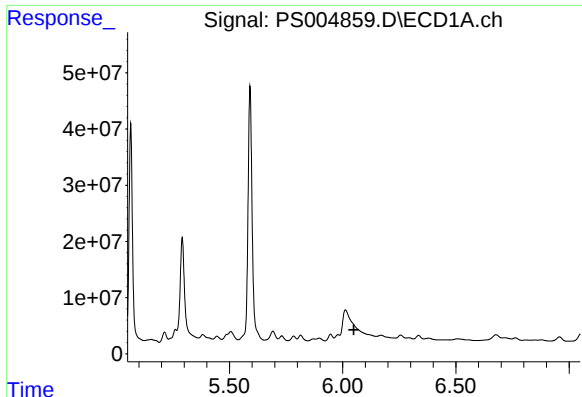

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-04-052919

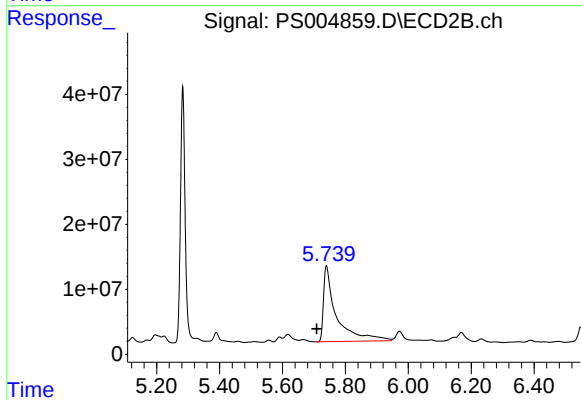


#7 MCPA

R.T.: 5.740 min
Delta R.T.: 0.031 min
Response: 332335807
Conc: 81.22 ug/ml

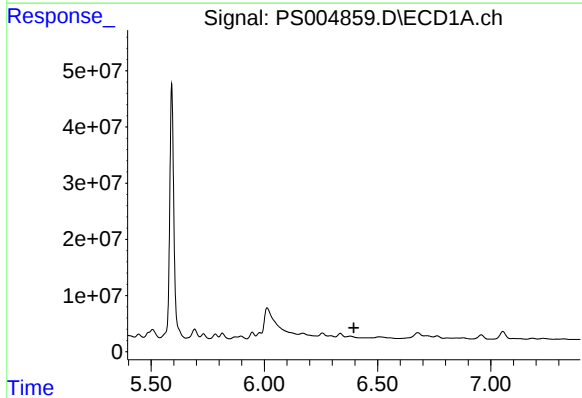


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

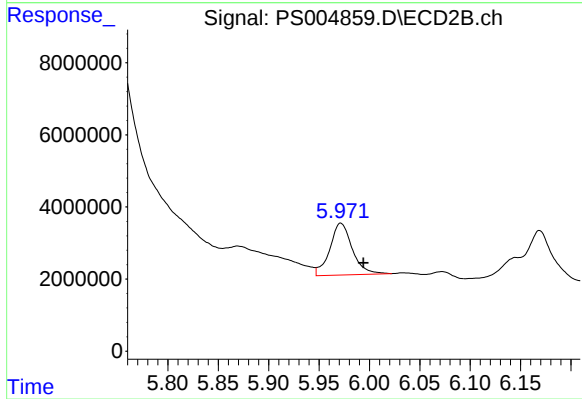

#8 DICHLORPROP


R.T.: 5.972 min
Delta R.T.: -0.022 min
Response: 22245526
Conc: 23.59 ng/ml

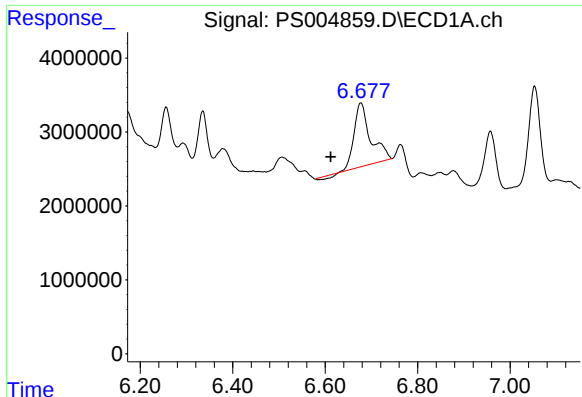

#9 2,4-D


R.T.: 6.677 min
Delta R.T.: 0.065 min
Response: 20718878
Conc: 15.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-052919

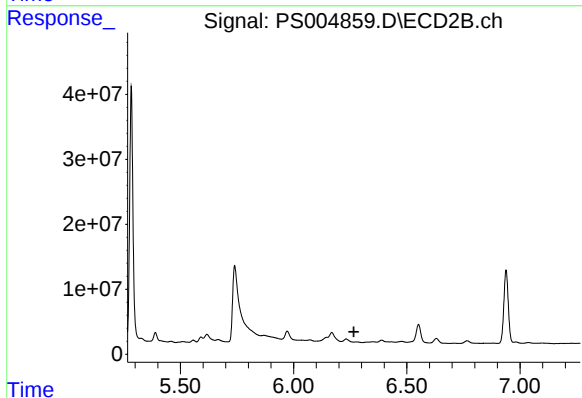


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

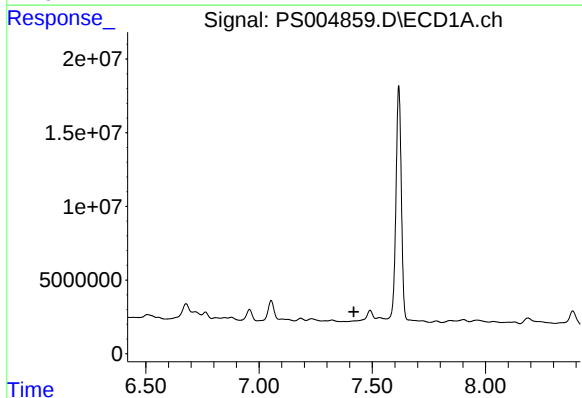

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

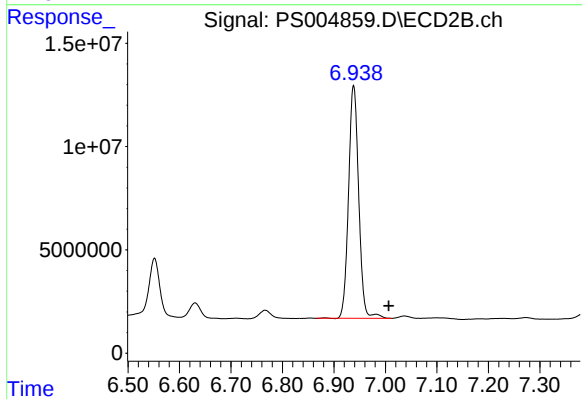

#11 2,4,5-TP (SILVEX)

R.T.: 6.938 min
Delta R.T.: -0.068 min
Response: 154427458
Conc: 30.01 ng/ml