

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053119\
 Data File : PS004862.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2019 11:15
 Operator : SM\AJ
 Sample : K3080-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MASONRY-COMPOSITE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 00:58:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.593	5.293	535.8E6	350.1E6	382.215	362.887
Target Compounds							
2) T	3,5-DICHL...	0.000	4.611	0	315.3E6	N.D.	255.880
3) T	4-Nitroph...	5.394	0.000	33778171	0	54.175	N.D. #
5) T	DICAMBA	5.695	5.399	31895514	23293343	6.007	6.305
6) T	MCP	5.949	0.000	11303338	0	2.715	N.D. #
7) T	MCPA	6.087	5.686	23511614	38096427	4.059	9.311 #
8) T	DICHLORPROP	0.000	5.988	0	42882591	N.D.	45.483
9) T	2,4-D	6.679	0.000	20434464	0	14.938	N.D. #
11) T	2,4,5-TP ...	0.000	6.948	0	143.3E6	N.D.	27.860
13) T	2,4-DB	8.245	7.845	51909667	19773685	53.739	30.253 #
14) T	DINOSEB	0.000	8.158	0	96220389	N.D.	25.030
15) T	Picloram	0.000	9.156	0	22034702	N.D.	2.954



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053119\
Data File : PS004862.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2019 11:15
Operator : SM\AJ
Sample : K3080-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MASONRY-COMPOSITE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 00:58:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

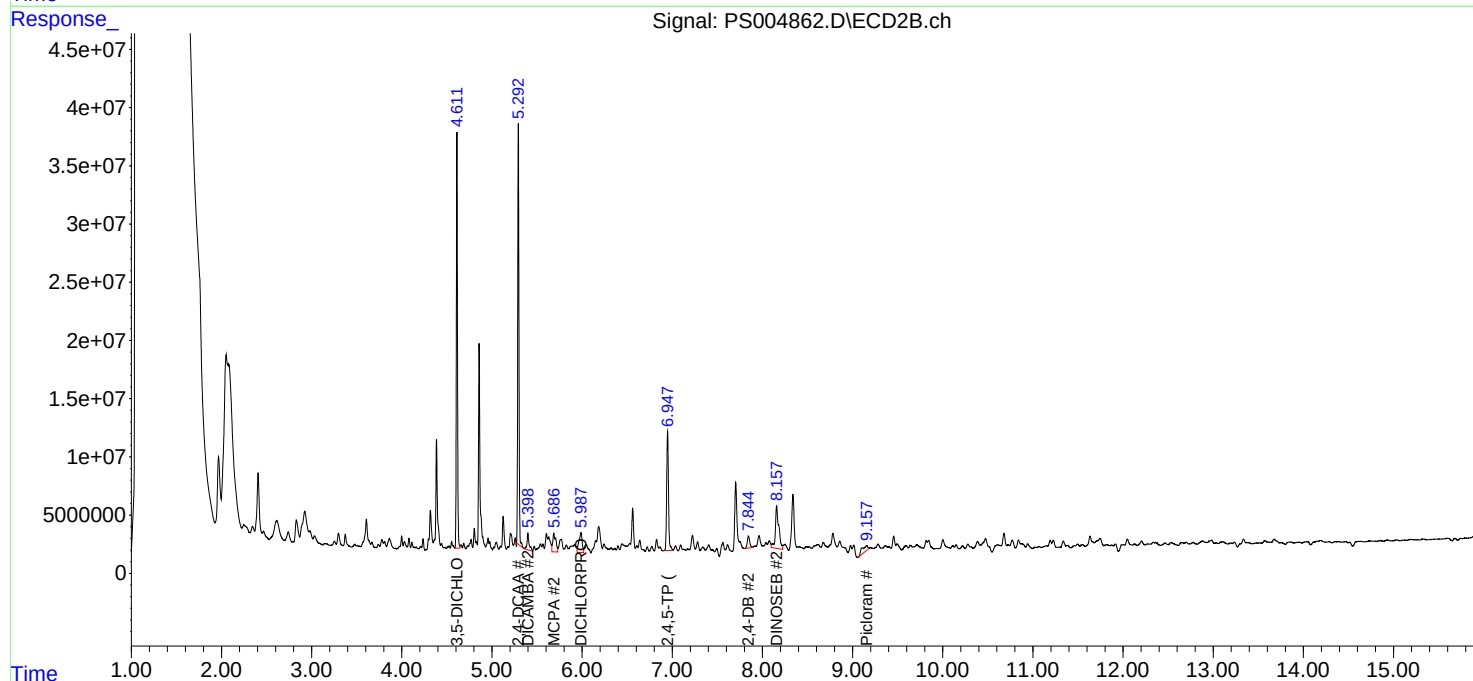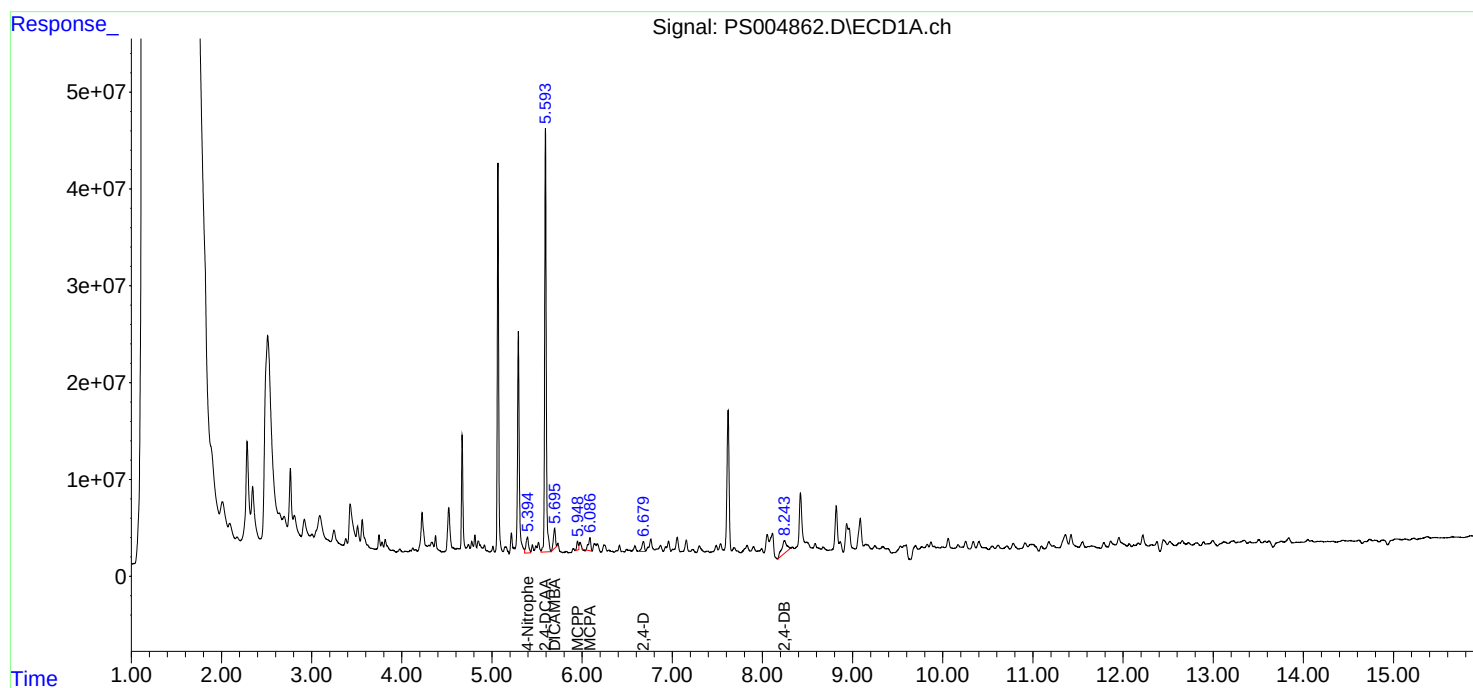


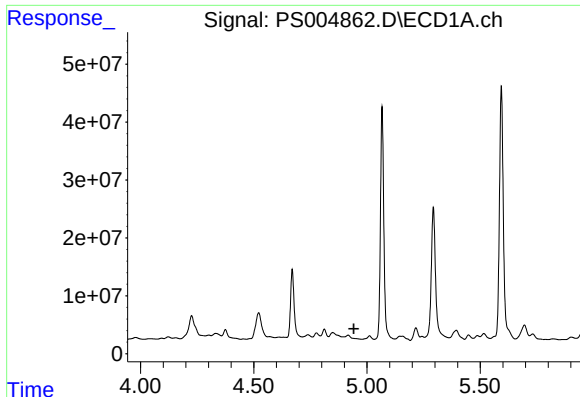

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
MASONRY-COMPOSITE

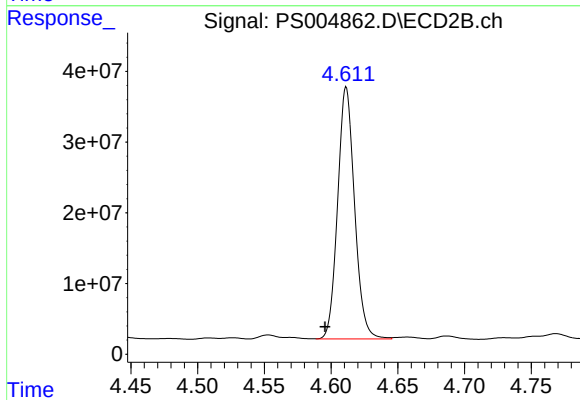


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.611 min
Delta R.T.: 0.016 min
Response: 315277462
Conc: 255.88 ng/ml

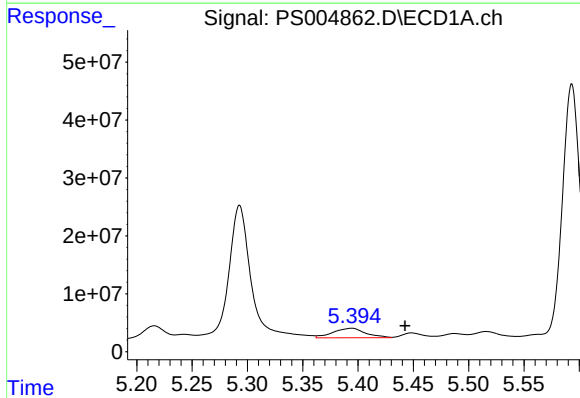


#3 4-Nitrophenol

R.T.: 5.394 min
Delta R.T.: -0.049 min
Response: 33778171
Conc: 54.17 ng/ml

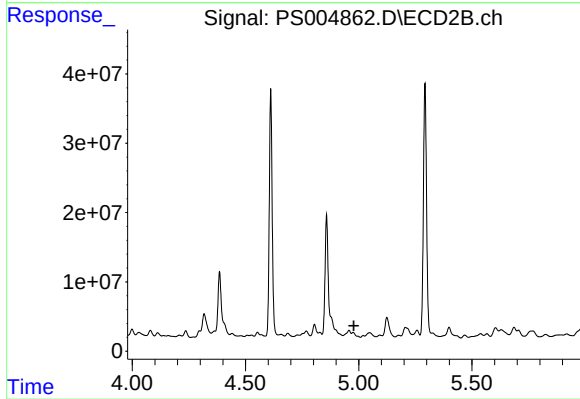

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

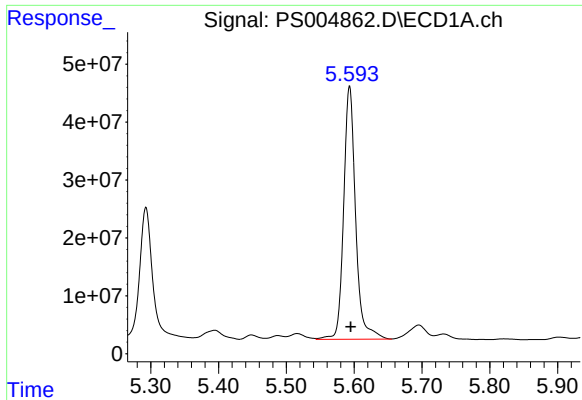

#4 2,4-DCAA


R.T.: 5.593 min
Delta R.T.: -0.002 min
Response: 535772792
Conc: 382.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
MASONRY-COMPOSITE

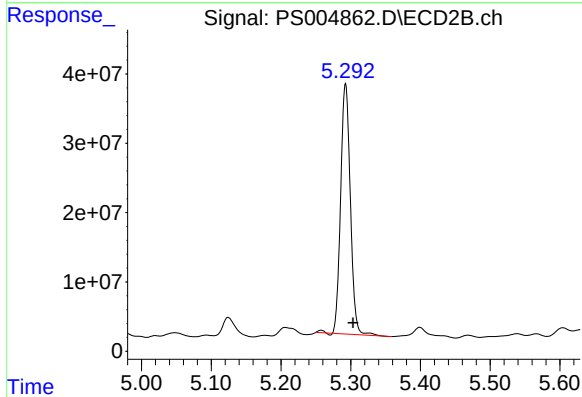


#4 2,4-DCAA

R.T.: 5.293 min
Delta R.T.: -0.011 min
Response: 350126532
Conc: 362.89 ng/ml

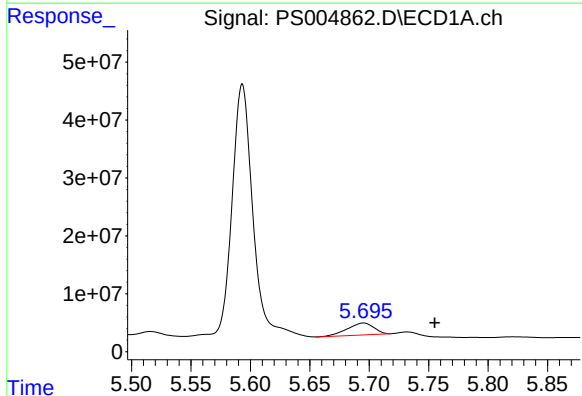


#5 DICAMBA

R.T.: 5.695 min
Delta R.T.: -0.060 min
Response: 31895514
Conc: 6.01 ng/ml

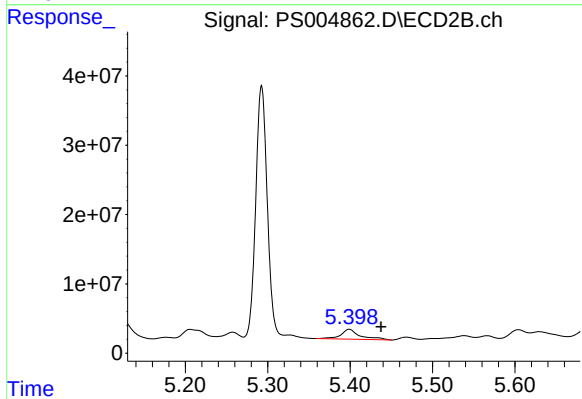

#5 DICAMBA


R.T.: 5.399 min
Delta R.T.: -0.038 min
Response: 23293343
Conc: 6.31 ng/ml

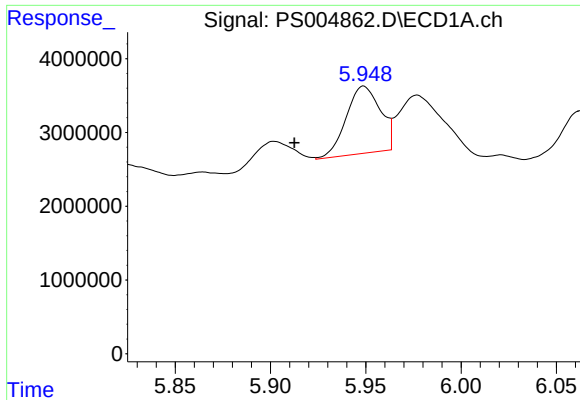

#6 MCPP


R.T.: 5.949 min
Delta R.T.: 0.036 min
Response: 11303338
Conc: 2.72 ug/ml

Instrument :
ECD_S
ClientSampleId :
MASONRY-COMPOSITE

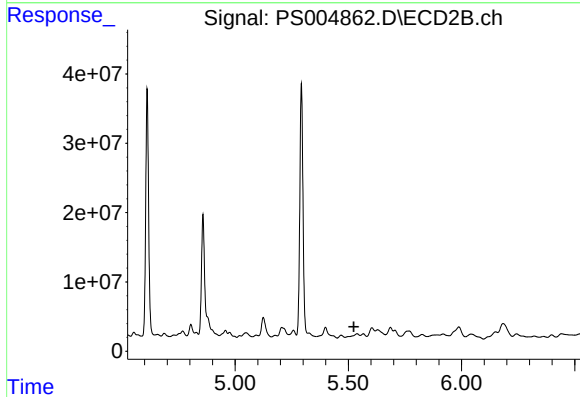


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

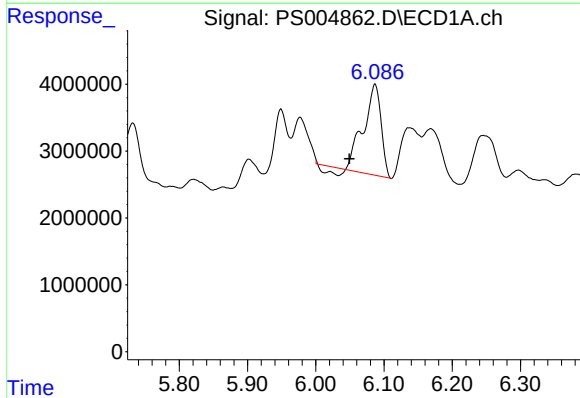


#7 MCPA

R.T.: 6.087 min
Delta R.T.: 0.038 min
Response: 23511614
Conc: 4.06 ug/ml

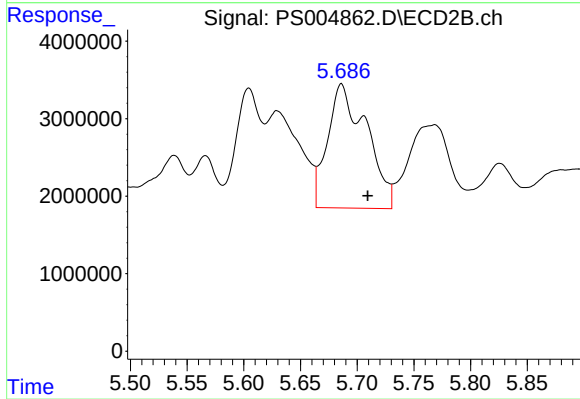

#7 MCPA


R.T.: 5.686 min
Delta R.T.: -0.023 min
Response: 38096427
Conc: 9.31 ug/ml

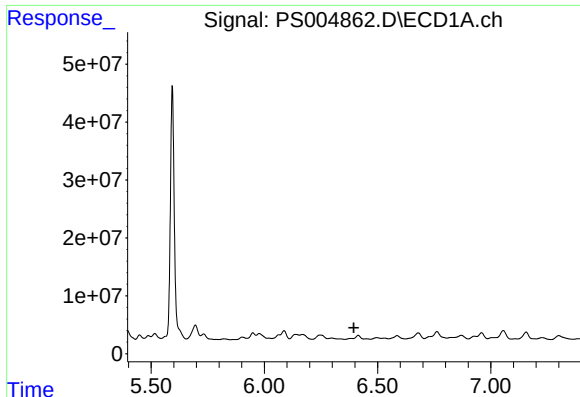

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
MASONRY-COMPOSITE

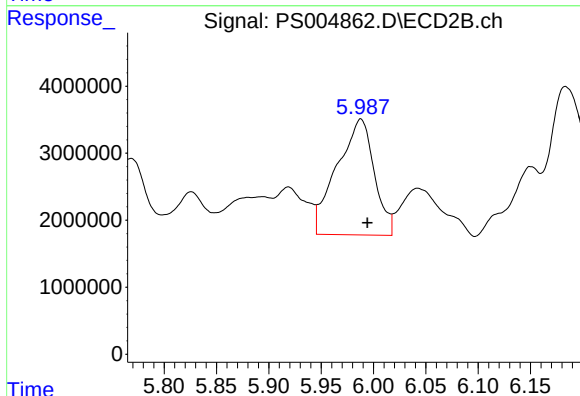


#8 DICHLORPROP

R.T.: 5.988 min
Delta R.T.: -0.006 min
Response: 42882591
Conc: 45.48 ng/ml

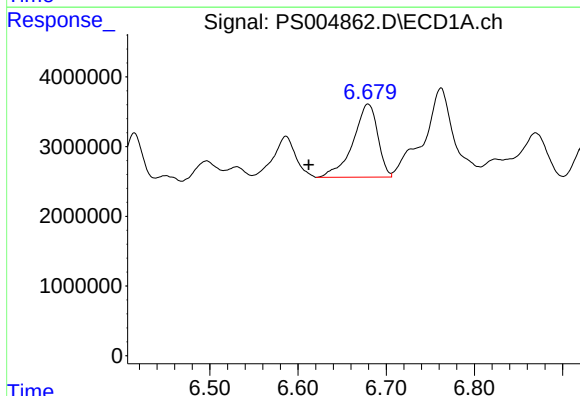


#9 2,4-D

R.T.: 6.679 min
Delta R.T.: 0.067 min
Response: 20434464
Conc: 14.94 ng/ml

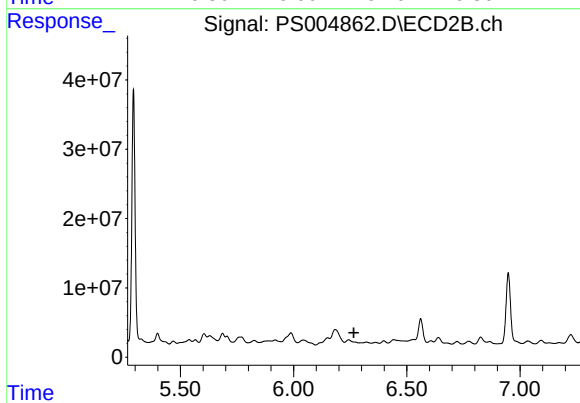

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

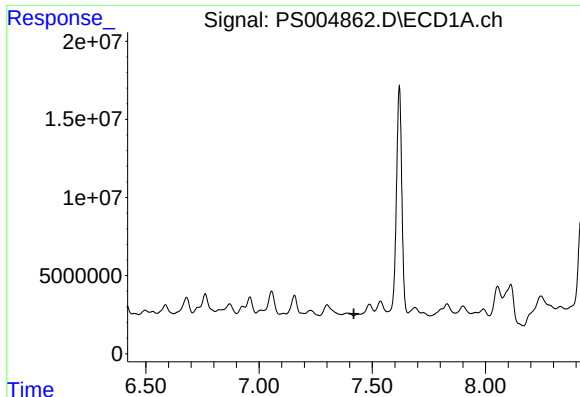

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
MASONRY-COMPOSITE

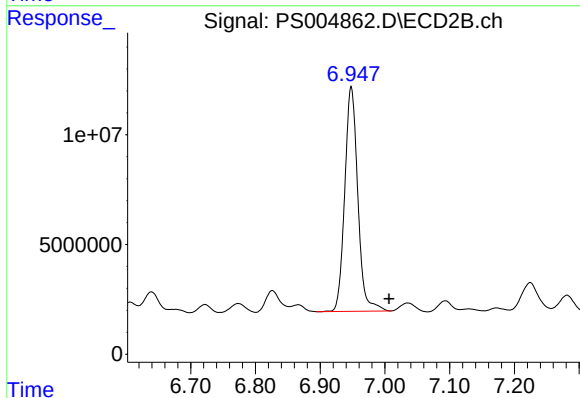


#11 2,4,5-TP (SILVEX)

R.T.: 6.948 min
Delta R.T.: -0.058 min
Response: 143346372
Conc: 27.86 ng/ml

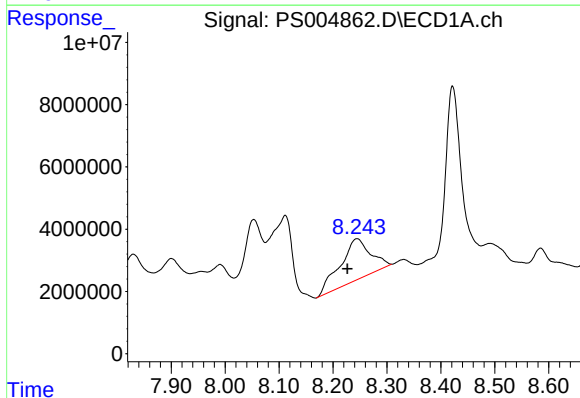


#13 2,4-DB

R.T.: 8.245 min
Delta R.T.: 0.018 min
Response: 51909667
Conc: 53.74 ng/ml

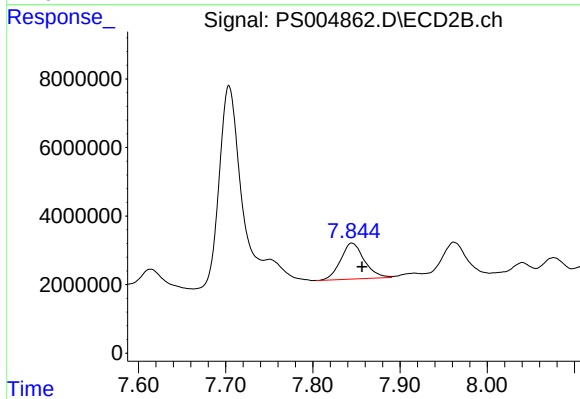

#13 2,4-DB


R.T.: 7.845 min
Delta R.T.: -0.011 min
Response: 19773685
Conc: 30.25 ng/ml

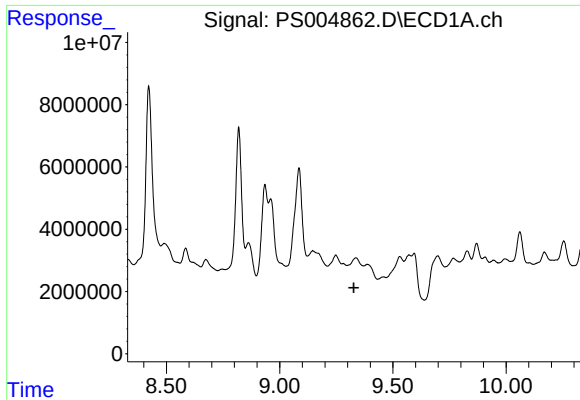

#14 DINoseb


R.T.: 0.000 min
Exp R.T.: 9.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
MASONRY-COMPOSITE

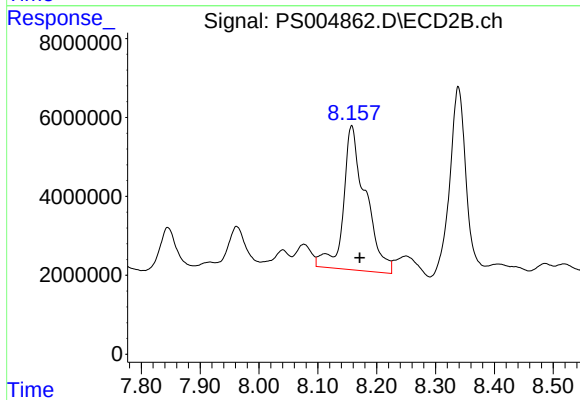


#14 DINoseb

R.T.: 8.158 min
Delta R.T.: -0.013 min
Response: 96220389
Conc: 25.03 ng/ml

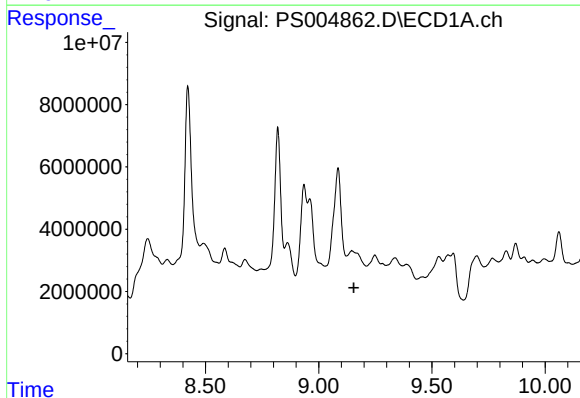

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.155 min
Response: 0
Conc: N.D.

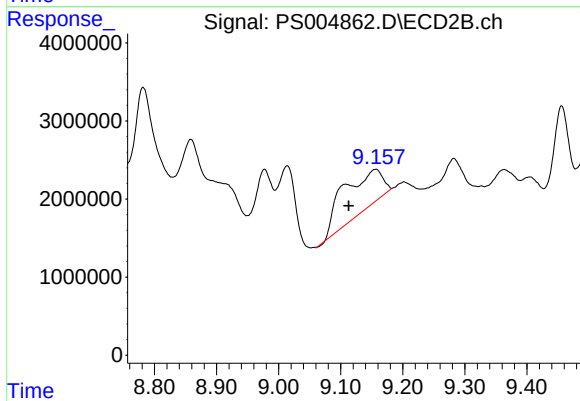

#15 Picloram

R.T.: 9.156 min
Delta R.T.: 0.043 min
Response: 22034702
Conc: 2.95 ng/ml