

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053119\
 Data File : PS004863.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2019 11:37
 Operator : SM\AJ
 Sample : K3084-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TEST-PIT-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 00:59:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.575	5.288	361.0E6	244.3E6	257.560	253.214
Target Compounds							
2) T	3,5-DICHL...	0.000	4.606	0	303.8E6	N.D.	246.586
3) T	4-Nitroph...	5.378	0.000	41404746	0	66.406	N.D. #
5) T	DICAMBA	5.714	5.394	17507719	23520544	3.297	6.367 #
6) T	MCP	5.930	0.000	13719396	0	3.296	N.D. #
7) T	MCPA	6.069	5.680	18522737	21334983	3.198	5.214 #
8) T	DICHLORPROP	0.000	5.978	0	13857507	N.D.	14.698
9) T	2,4-D	6.664	0.000	41748021	0	30.520	N.D. #
10) T	Pentachlo...	6.942	0.000	13174519	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	6.944	0	142.7E6	N.D.	27.740
13) T	2,4-DB	8.228	0.000	59986310	0	62.100	N.D. #
14) T	DINOSEB	0.000	8.152	0	70205740	N.D.	18.263



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053119\
Data File : PS004863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2019 11:37
Operator : SM\AJ
Sample : K3084-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 00:59:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

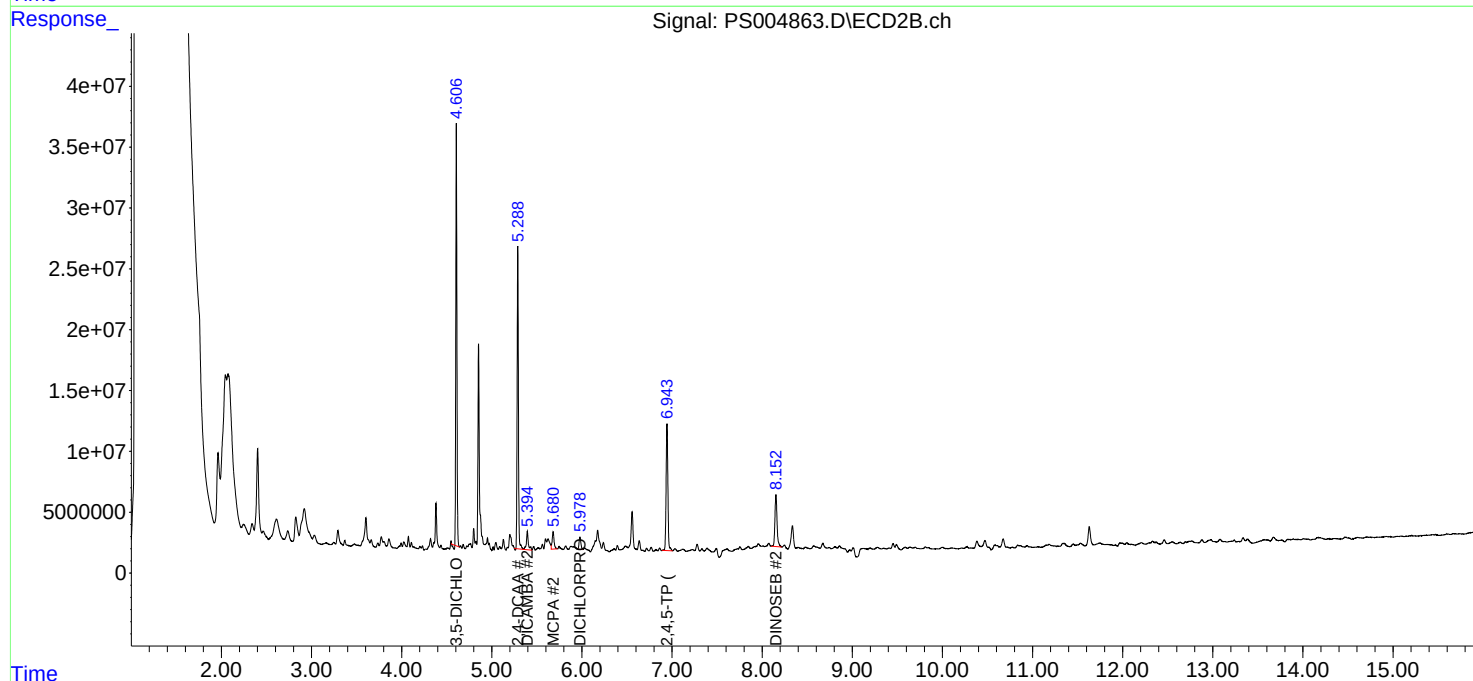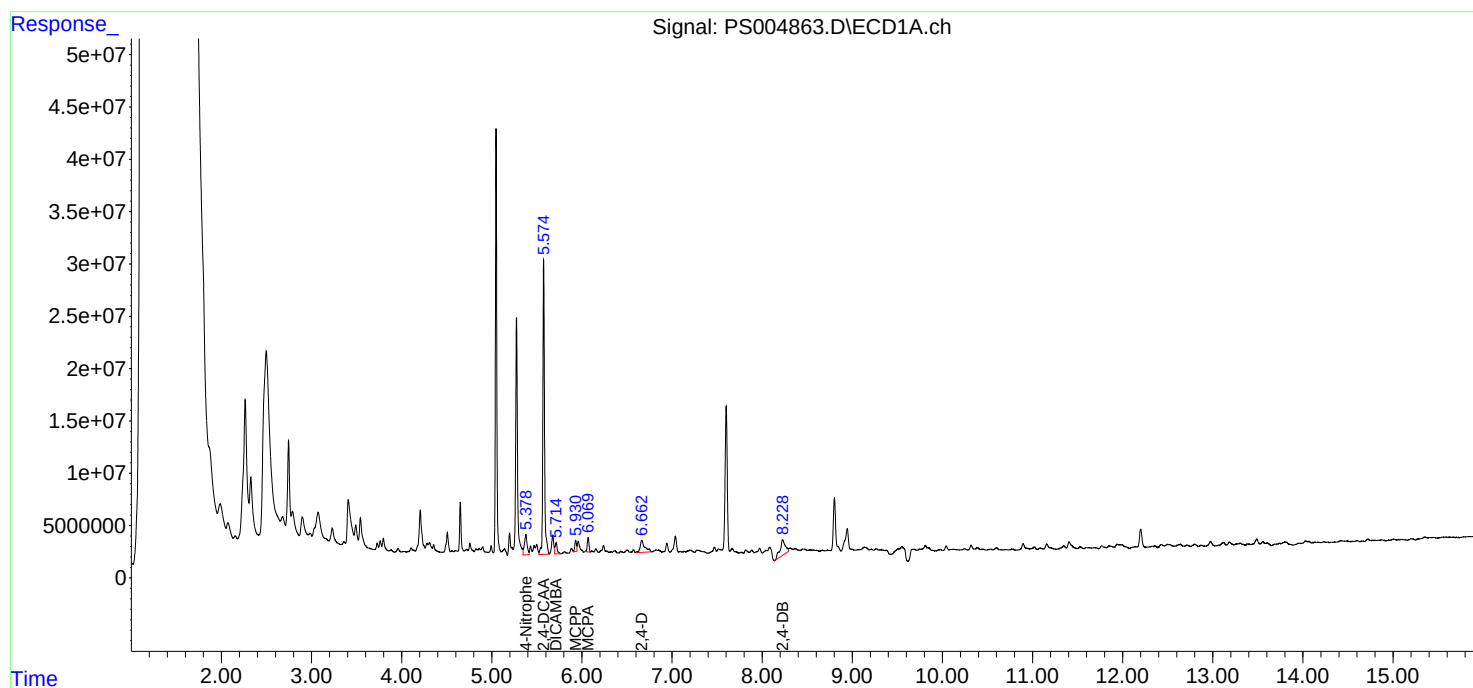


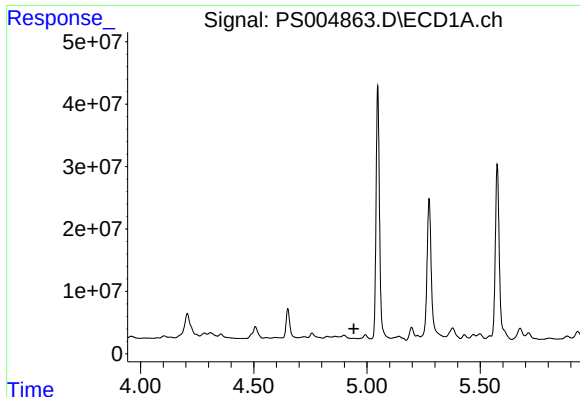

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-6

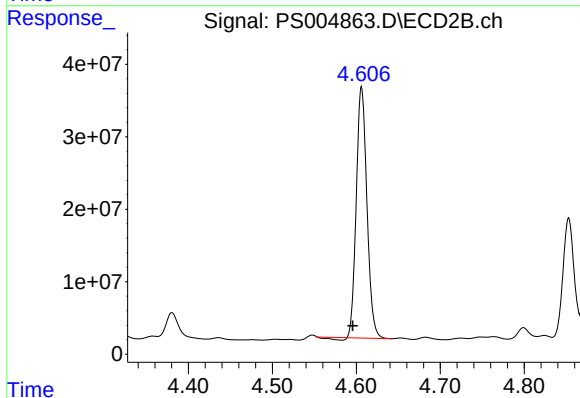


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.606 min
Delta R.T.: 0.011 min
Response: 303825127
Conc: 246.59 ng/ml

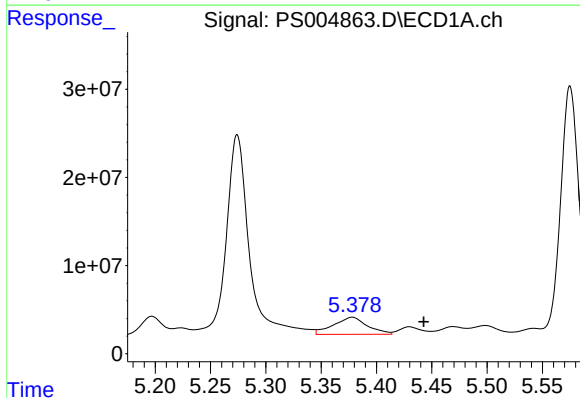


#3 4-Nitrophenol

R.T.: 5.378 min
Delta R.T.: -0.065 min
Response: 41404746
Conc: 66.41 ng/ml

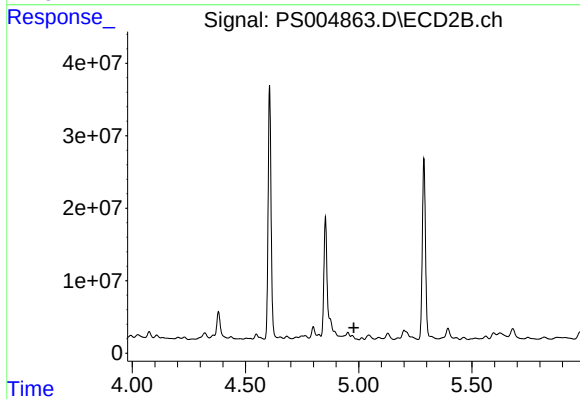

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

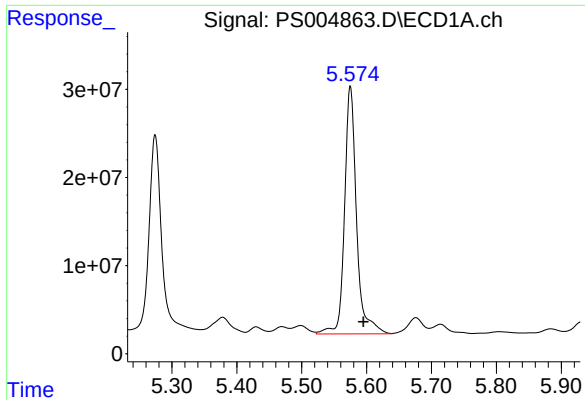

#4 2,4-DCAA


R.T.: 5.575 min
Delta R.T.: -0.020 min
Response: 361036556
Conc: 257.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-6

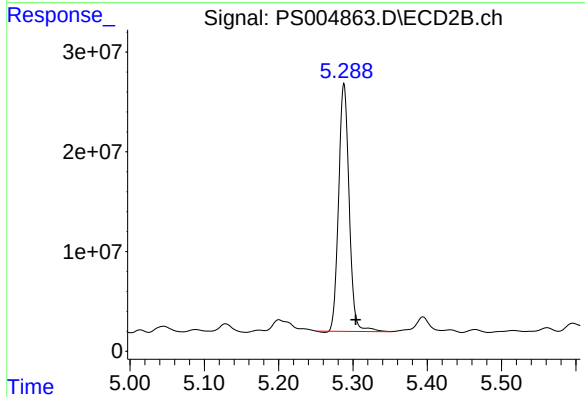


#4 2,4-DCAA

R.T.: 5.288 min
Delta R.T.: -0.016 min
Response: 244309609
Conc: 253.21 ng/ml

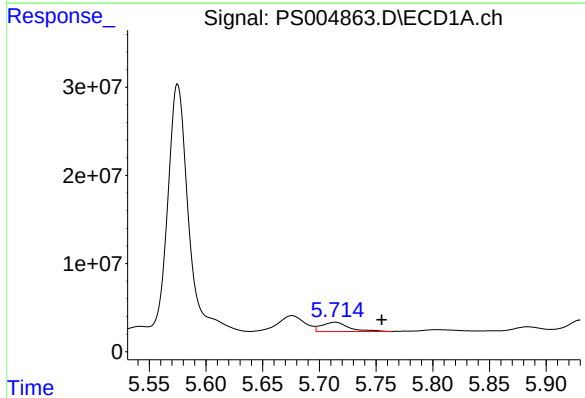


#5 DICAMBA

R.T.: 5.714 min
Delta R.T.: -0.041 min
Response: 17507719
Conc: 3.30 ng/ml

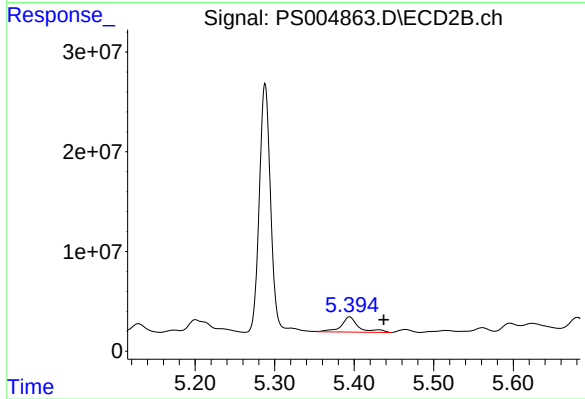

#5 DICAMBA


R.T.: 5.394 min
Delta R.T.: -0.043 min
Response: 23520544
Conc: 6.37 ng/ml

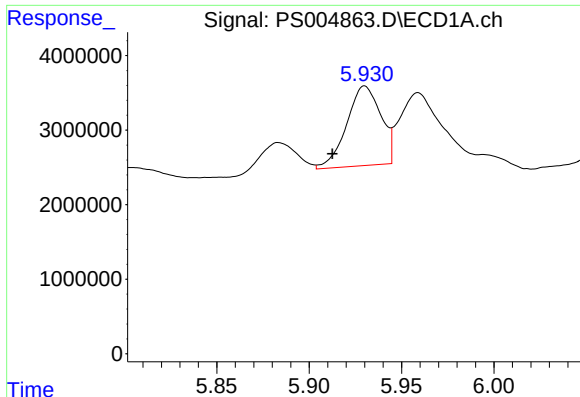

#6 MCPP


R.T.: 5.930 min
Delta R.T.: 0.018 min
Response: 13719396
Conc: 3.30 ug/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-6

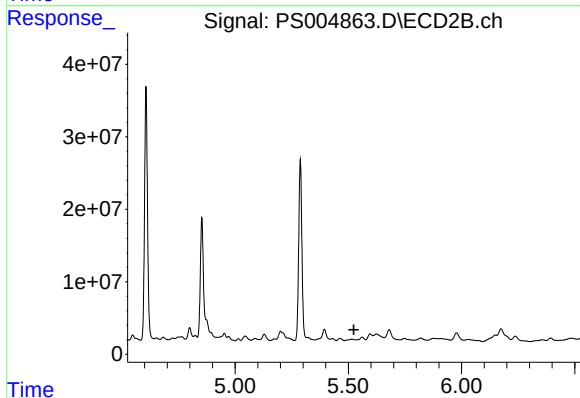


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

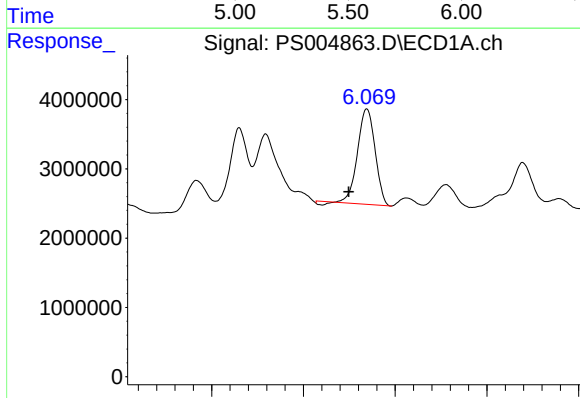


#7 MCPA

R.T.: 6.069 min
Delta R.T.: 0.020 min
Response: 18522737
Conc: 3.20 ug/ml

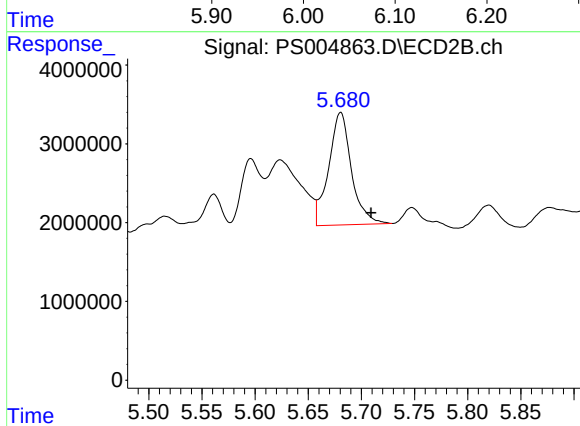

#7 MCPA


R.T.: 5.680 min
Delta R.T.: -0.029 min
Response: 21334983
Conc: 5.21 ug/ml

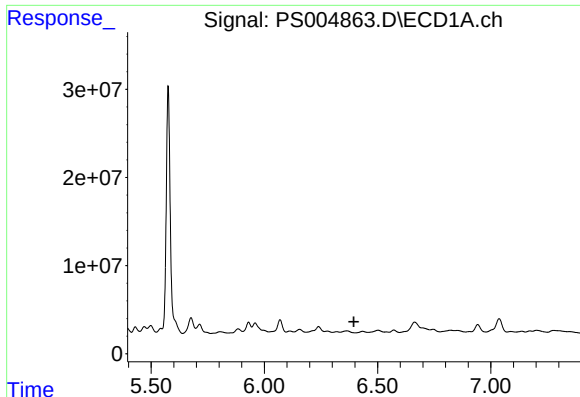

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-6

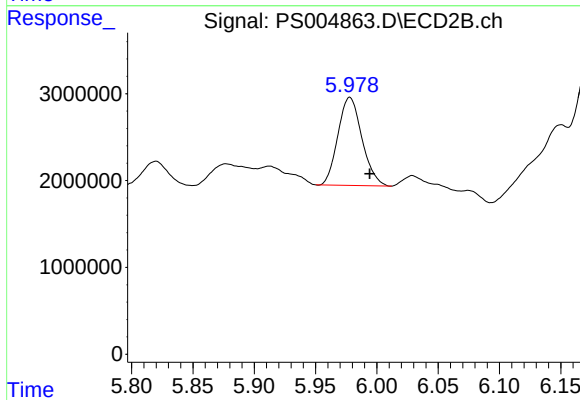


#8 DICHLORPROP

R.T.: 5.978 min
Delta R.T.: -0.016 min
Response: 13857507
Conc: 14.70 ng/ml

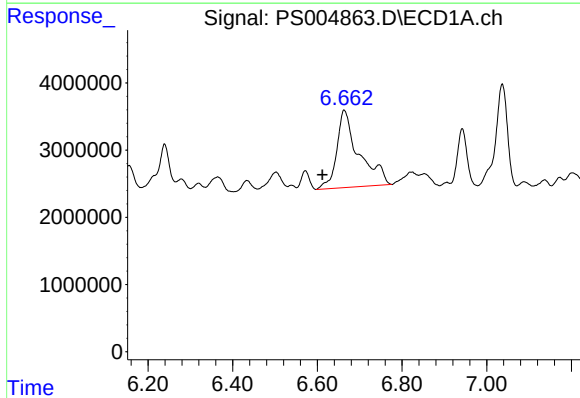


#9 2,4-D

R.T.: 6.664 min
Delta R.T.: 0.052 min
Response: 41748021
Conc: 30.52 ng/ml

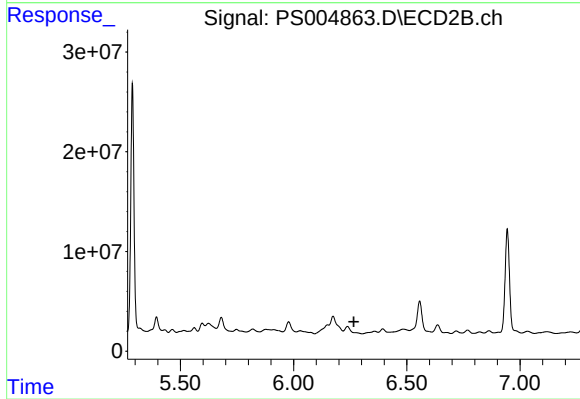

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

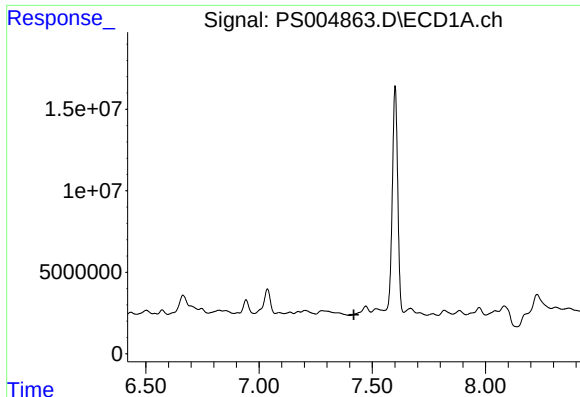

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-6

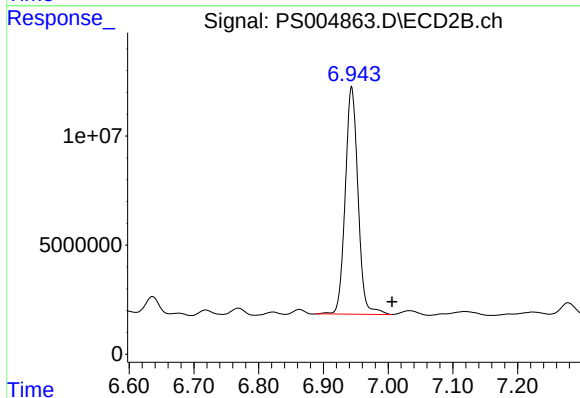


#11 2,4,5-TP (SILVEX)

R.T.: 6.944 min
Delta R.T.: -0.063 min
Response: 142731812
Conc: 27.74 ng/ml

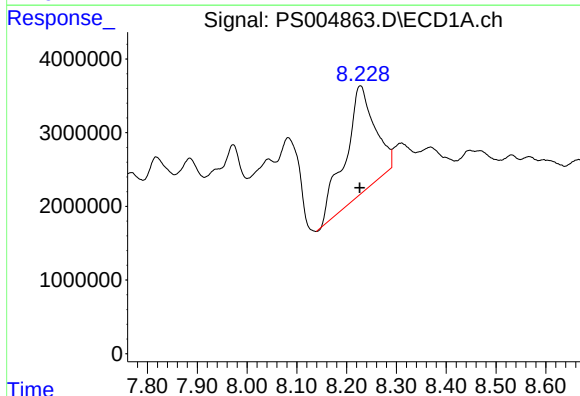


#13 2,4-DB

R.T.: 8.228 min
Delta R.T.: 0.001 min
Response: 59986310
Conc: 62.10 ng/ml

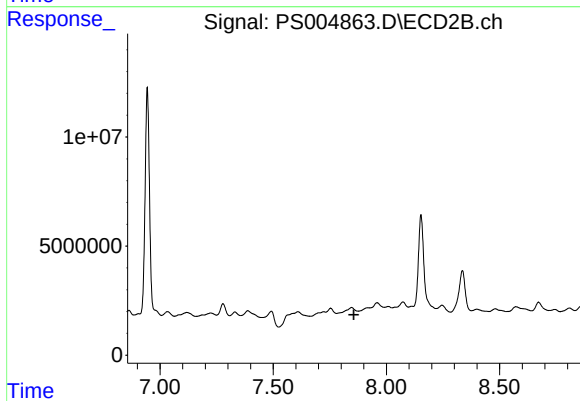

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 7.856 min
Response: 0
Conc: N.D.

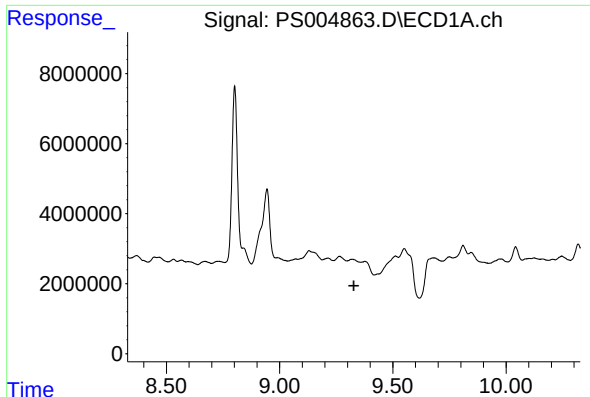

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-6

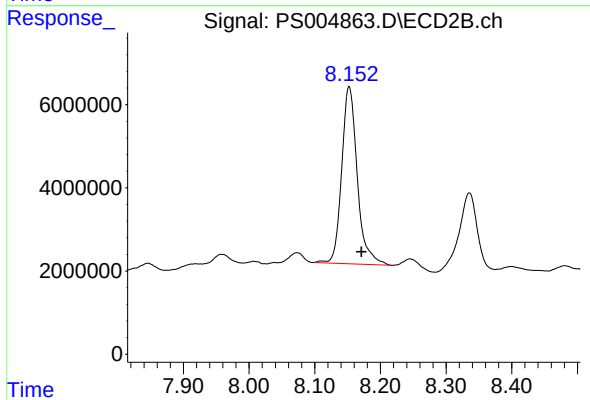

#14 DINOSEB

R.T.: 8.152 min
Delta R.T.: -0.019 min
Response: 70205740
Conc: 18.26 ng/ml