

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053119\
 Data File : PS004864.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2019 11:59
 Operator : SM\AJ
 Sample : K3084-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TEST-PIT-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 00:59:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.595	5.306	458.5E6	318.2E6	327.057	329.751
Target Compounds							
2) T	3,5-DICHL...	0.000	4.624	0	374.8E6	N.D.	304.162
3) T	4-Nitroph...	5.398	0.000	41108341	0	65.931	N.D. #
5) T	DICAMBA	5.735	5.412	18663327	21321808	3.515	5.772 #
6) T	MCP	5.950	0.000	10316839	0	2.478	N.D. #
7) T	MCPA	6.090	5.698	15900673	21272893	2.745	5.199 #
10) T	Pentachlo...	0.000	6.574	0	42369080	N.D.	3.449
11) T	2,4,5-TP ...	0.000	6.961	0	167.8E6	N.D.	32.621
13) T	2,4-DB	8.248	0.000	58225024	0	60.277	N.D. #
14) T	DINOSEB	0.000	8.170	0	69943918	N.D.	18.195



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053119\
Data File : PS004864.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2019 11:59
Operator : SM\AJ
Sample : K3084-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 00:59:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

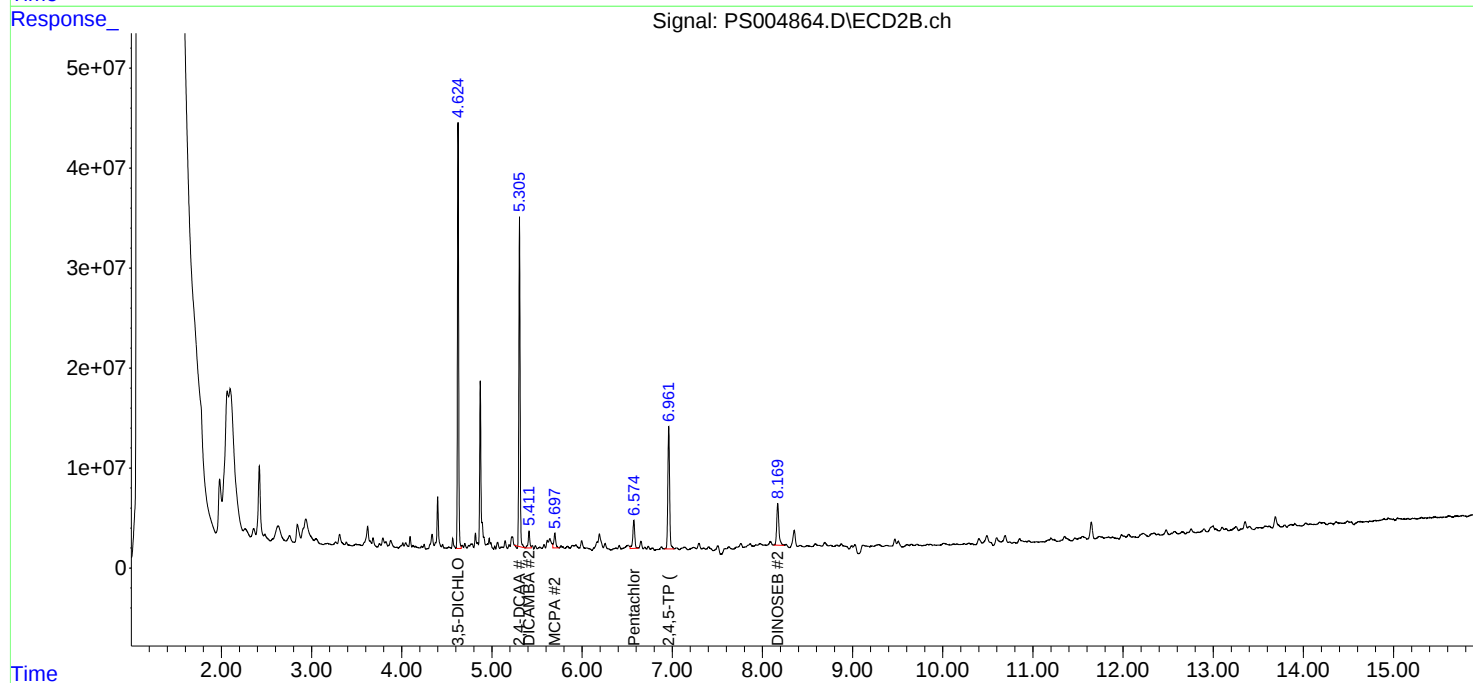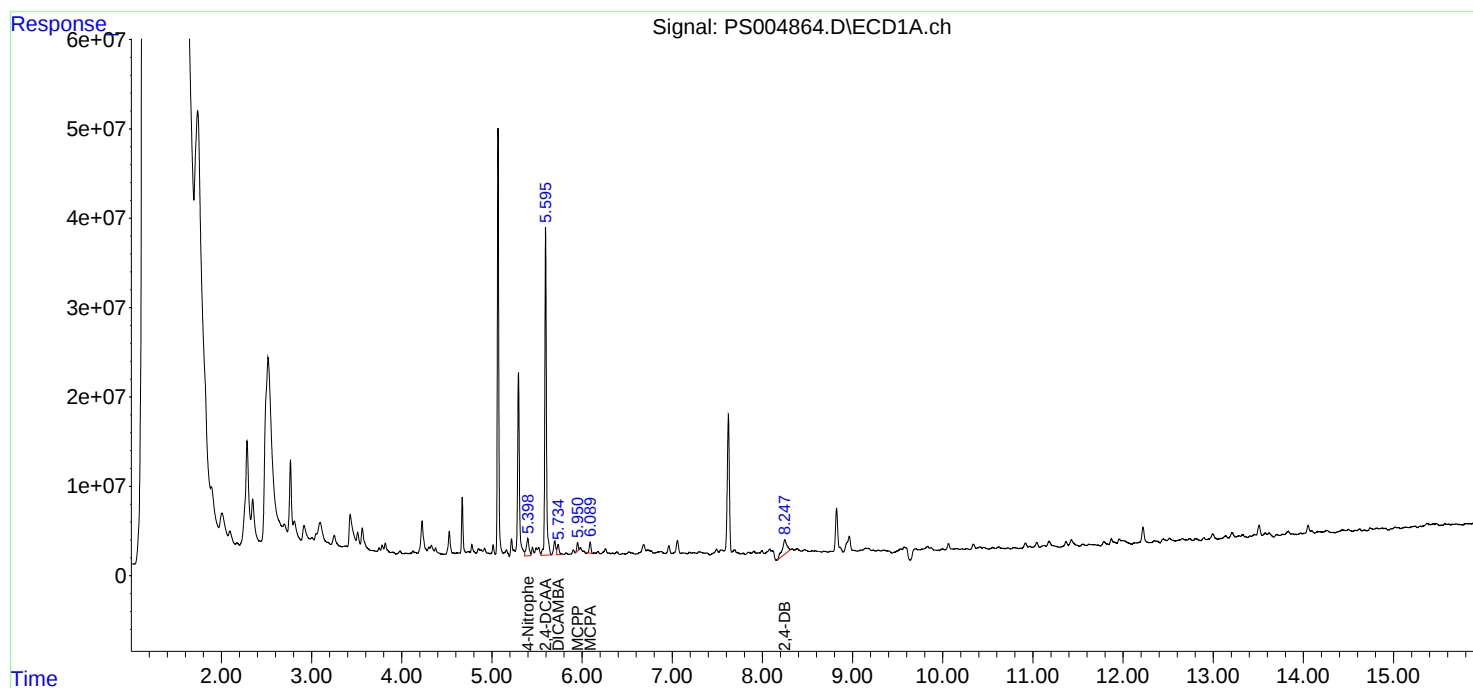


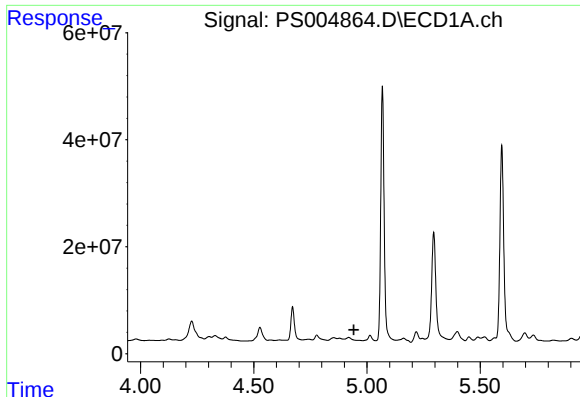

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-7

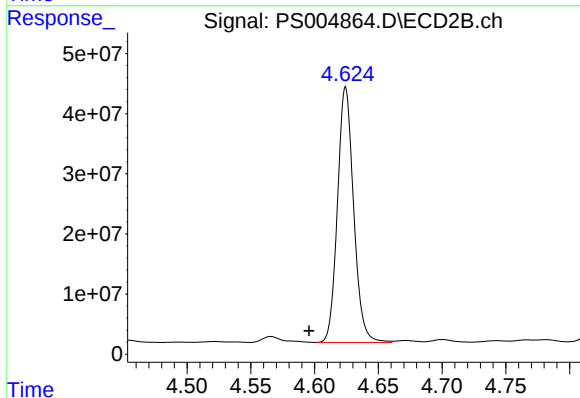


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.624 min
Delta R.T.: 0.029 min
Response: 374766472
Conc: 304.16 ng/ml

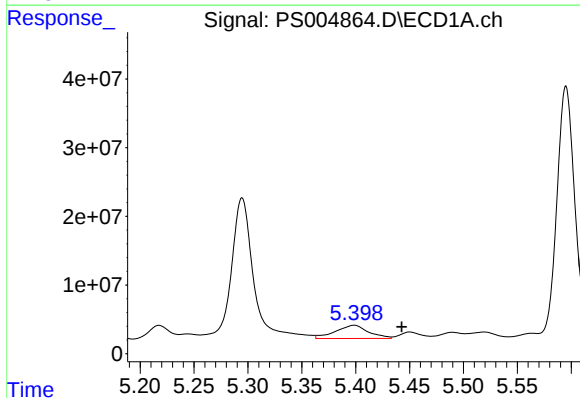


#3 4-Nitrophenol

R.T.: 5.398 min
Delta R.T.: -0.044 min
Response: 41108341
Conc: 65.93 ng/ml

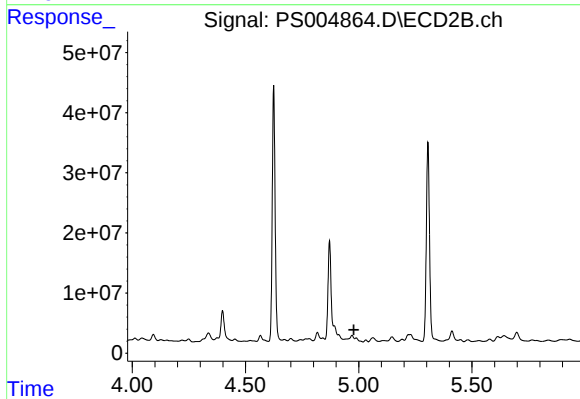

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

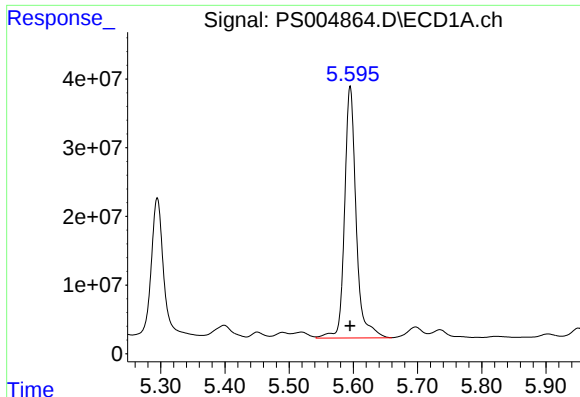

#4 2,4-DCAA


R.T.: 5.595 min
Delta R.T.: 0.000 min
Response: 458454499
Conc: 327.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-7

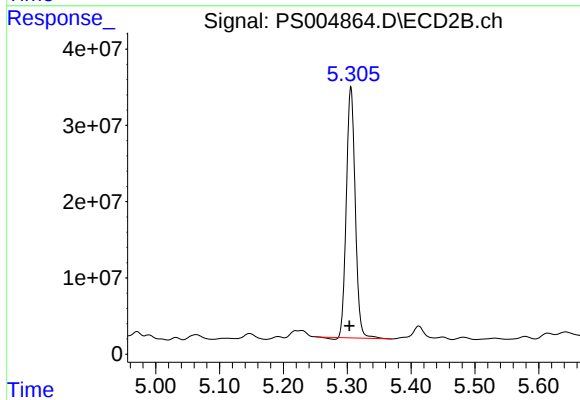


#4 2,4-DCAA

R.T.: 5.306 min
Delta R.T.: 0.002 min
Response: 318155207
Conc: 329.75 ng/ml

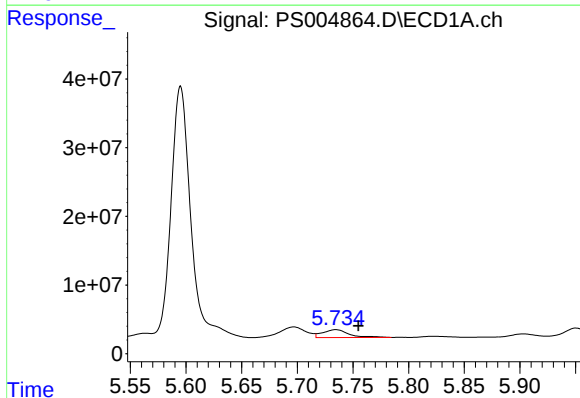


#5 DICAMBA

R.T.: 5.735 min
Delta R.T.: -0.020 min
Response: 18663327
Conc: 3.51 ng/ml

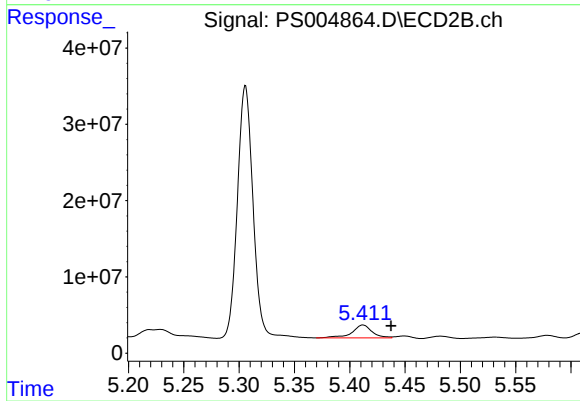

#5 DICAMBA


R.T.: 5.412 min
Delta R.T.: -0.025 min
Response: 21321808
Conc: 5.77 ng/ml

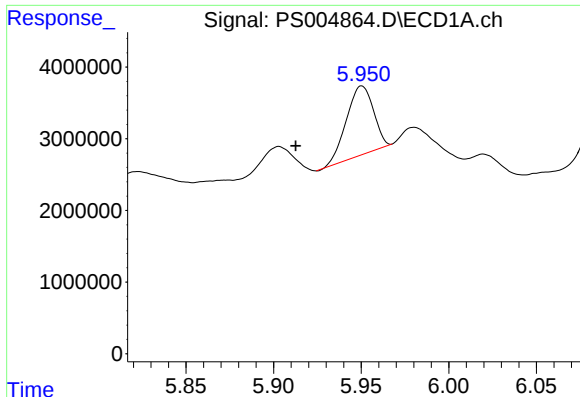

#6 MCPP


R.T.: 5.950 min
Delta R.T.: 0.038 min
Response: 10316839
Conc: 2.48 ug/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-7

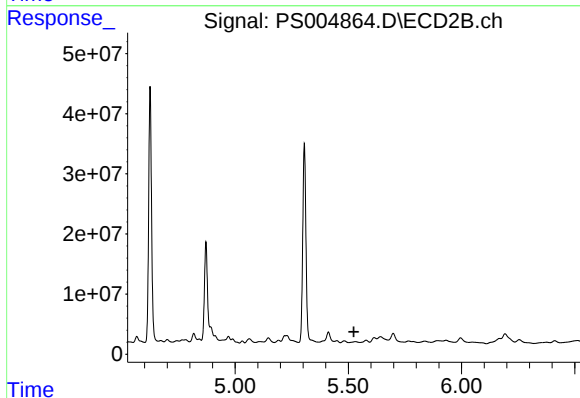


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

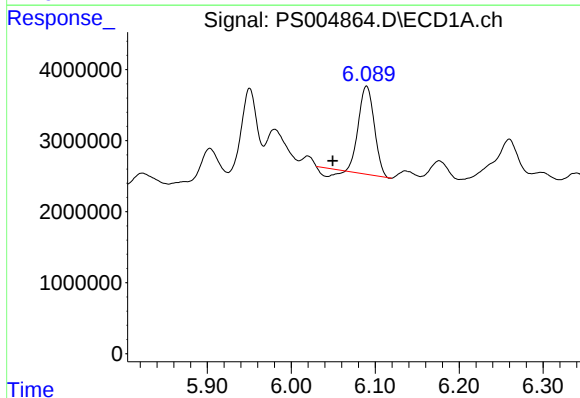


#7 MCPA

R.T.: 6.090 min
Delta R.T.: 0.040 min
Response: 15900673
Conc: 2.75 ug/ml

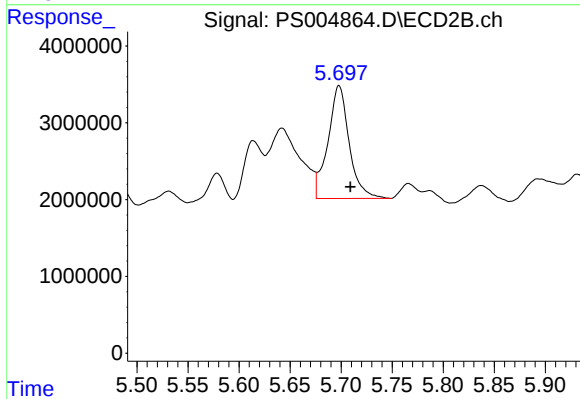

#7 MCPA


R.T.: 5.698 min
Delta R.T.: -0.011 min
Response: 21272893
Conc: 5.20 ug/ml

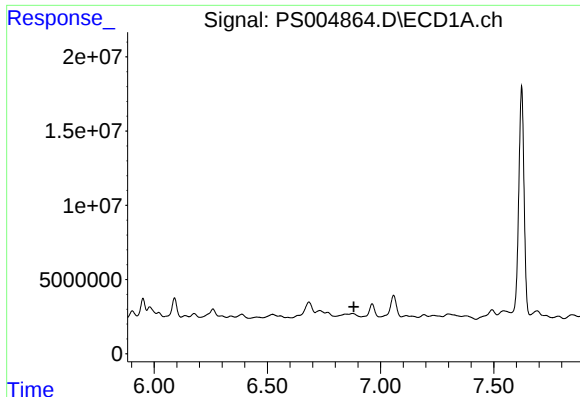

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-7

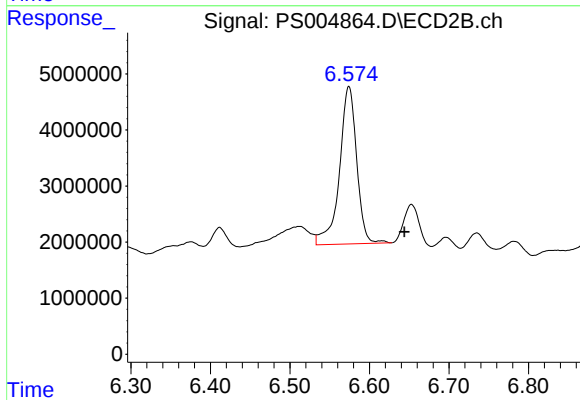


#10 Pentachlorophenol

R.T.: 6.574 min
Delta R.T.: -0.070 min
Response: 42369080
Conc: 3.45 ng/ml

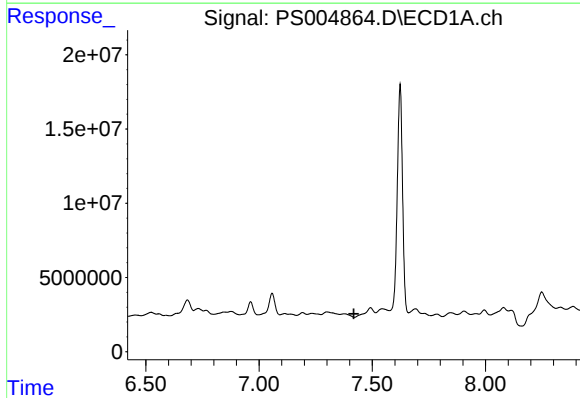


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

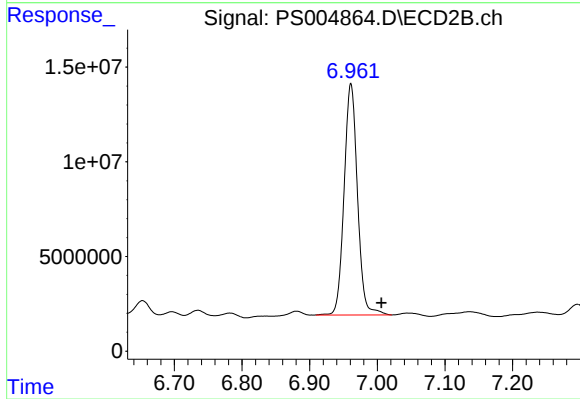

#11 2,4,5-TP (SILVEX)


R.T.: 6.961 min
Delta R.T.: -0.045 min
Response: 167847197
Conc: 32.62 ng/ml

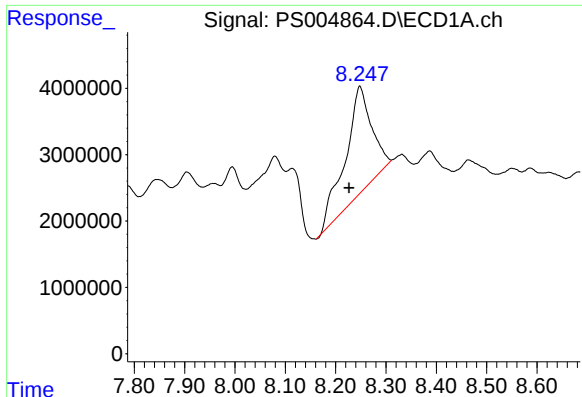

#13 2,4-DB


R.T.: 8.248 min
Delta R.T.: 0.022 min
Response: 58225024
Conc: 60.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-7

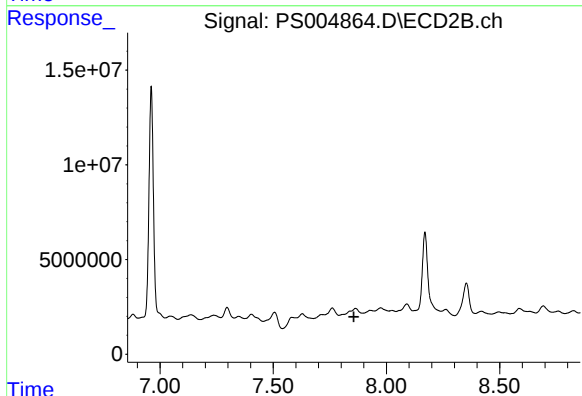


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.856 min
Response: 0
Conc: N.D.

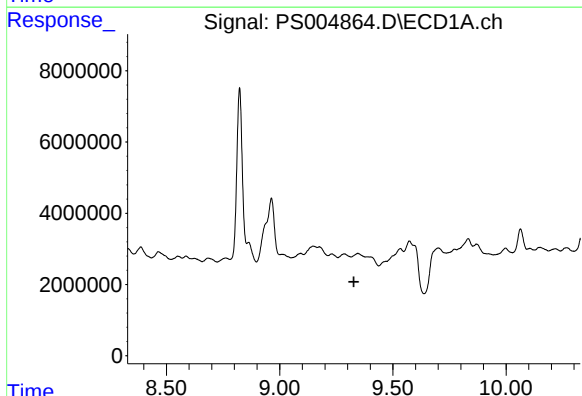

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.328 min
Response: 0
Conc: N.D.

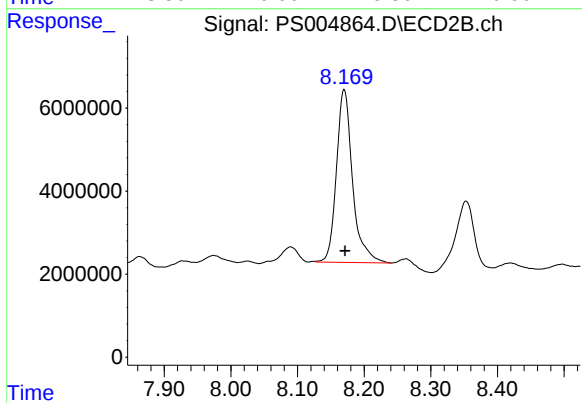

#14 DINOSEB

R.T.: 8.170 min
Delta R.T.: -0.001 min
Response: 69943918
Conc: 18.19 ng/ml