

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053119\
 Data File : PS004866.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2019 12:43
 Operator : SM\AJ
 Sample : K3084-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TEST-PIT-9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 01:00:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.579	5.290	410.6E6	287.2E6	292.909	297.691
Target Compounds							
2) T	3,5-DICHL...	4.997	4.608	10271781	334.6E6	5.956	271.576 #
3) T	4-Nitroph...	5.382	0.000	39890538	0	63.978	N.D. #
5) T	DICAMBA	5.718	5.396	16513328	19395015	3.110	5.250 #
6) T	MCP	5.934	0.000	10890534	0	2.616	N.D. #
7) T	MCPA	6.073	5.682	16640647	22750841	2.873	5.560 #
9) T	2,4-D	6.671	0.000	45379154	0	33.174	N.D. #
11) T	2,4,5-TP ...	0.000	6.946	0	149.6E6	N.D.	29.081
13) T	2,4-DB	8.231	0.000	67592858	0	69.975	N.D. #
14) T	DINOSEB	0.000	8.154	0	64640581	N.D.	16.815



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053119\
Data File : PS004866.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2019 12:43
Operator : SM\AJ
Sample : K3084-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 01:00:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

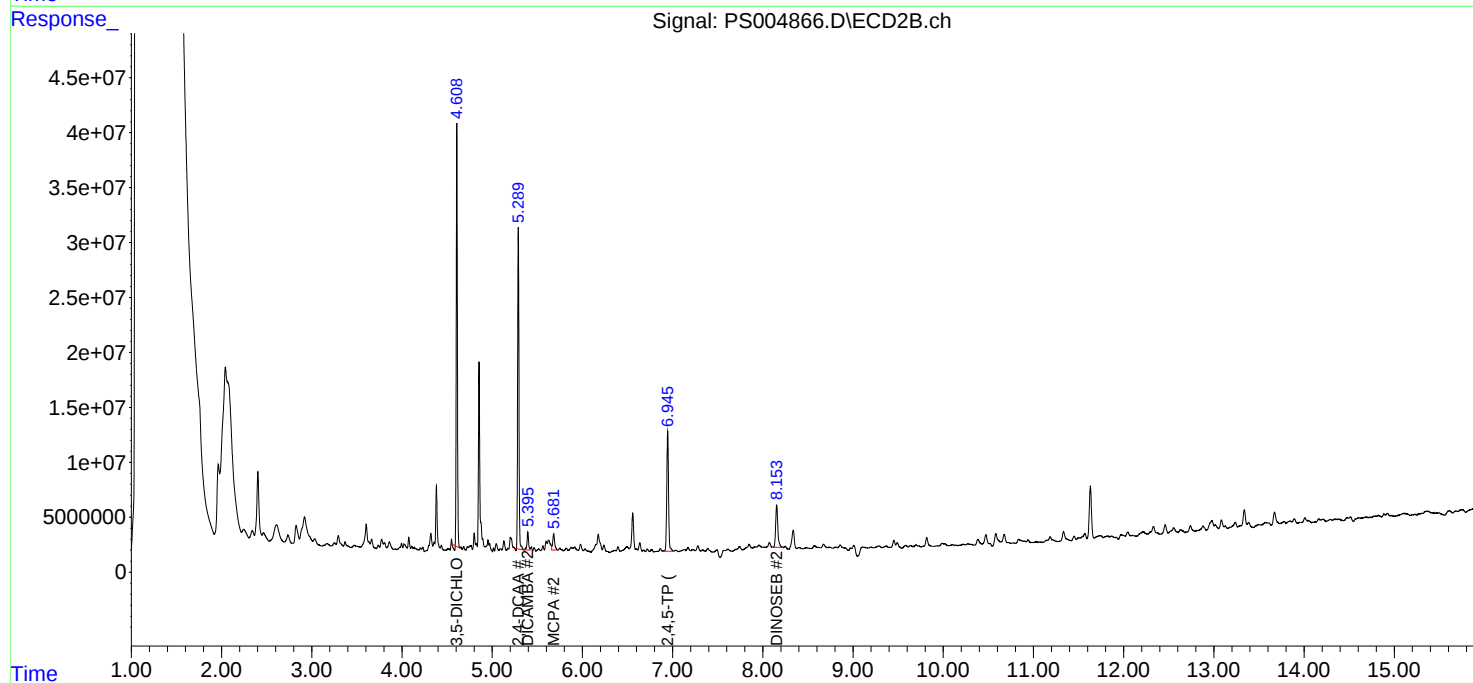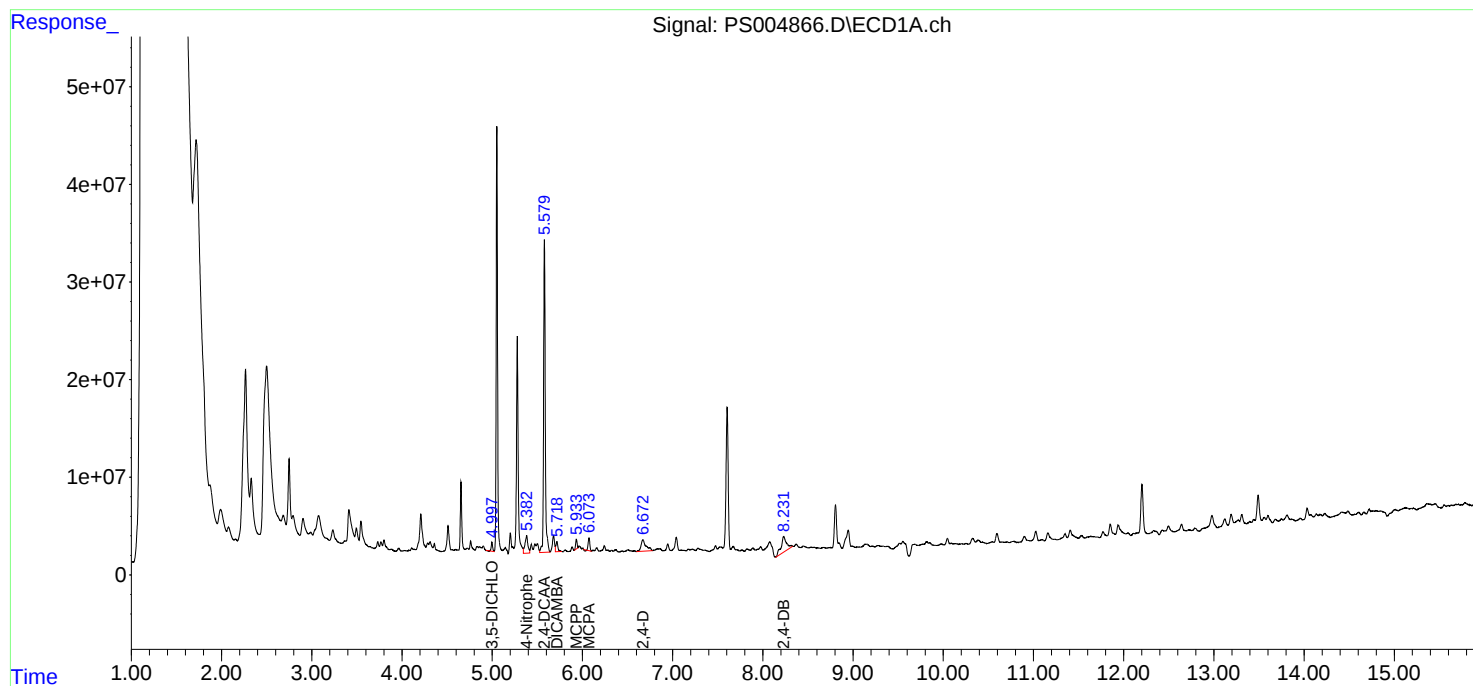


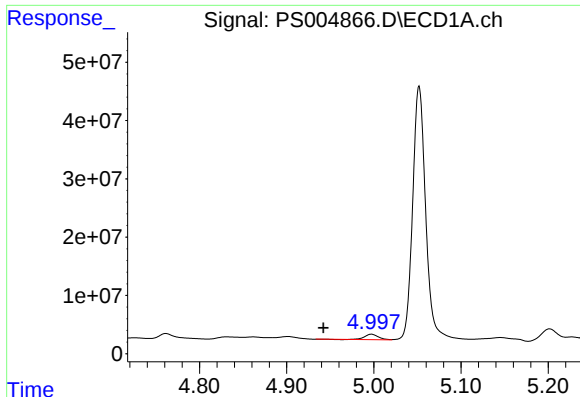

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.997 min
Delta R.T.: 0.055 min
Response: 10271781
Conc: 5.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-9

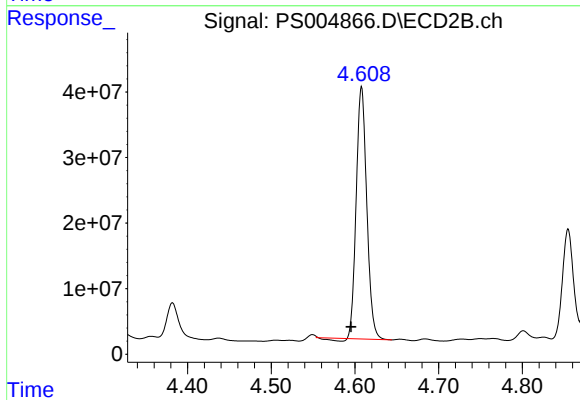


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.608 min
Delta R.T.: 0.012 min
Response: 334616343
Conc: 271.58 ng/ml

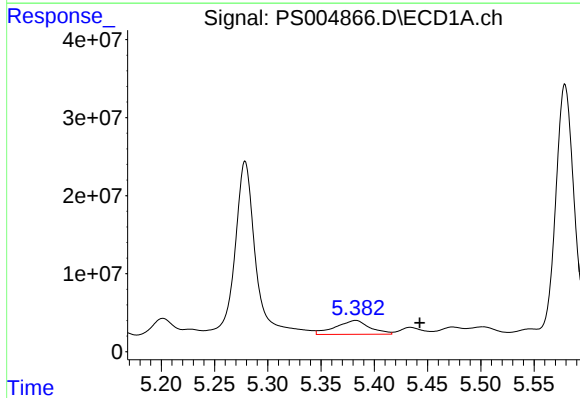


#3 4-Nitrophenol

R.T.: 5.382 min
Delta R.T.: -0.060 min
Response: 39890538
Conc: 63.98 ng/ml

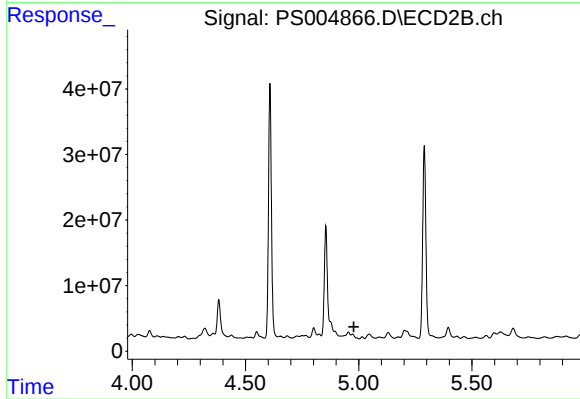

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

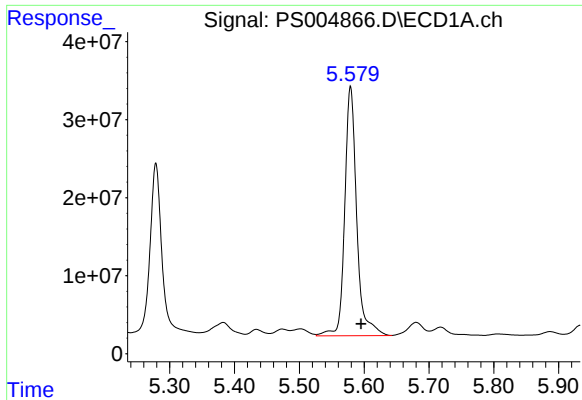

#4 2,4-DCAA


R.T.: 5.579 min
Delta R.T.: -0.016 min
Response: 410586721
Conc: 292.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-9

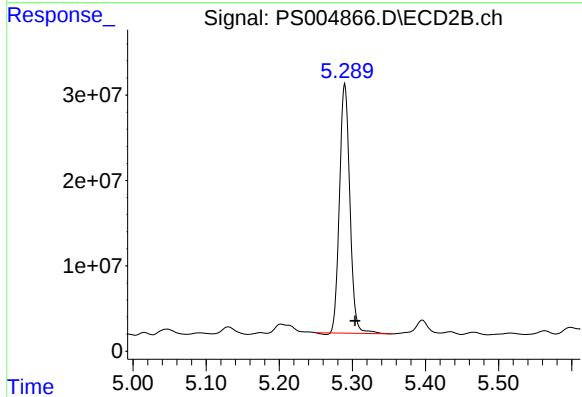


#4 2,4-DCAA

R.T.: 5.290 min
Delta R.T.: -0.014 min
Response: 287222713
Conc: 297.69 ng/ml

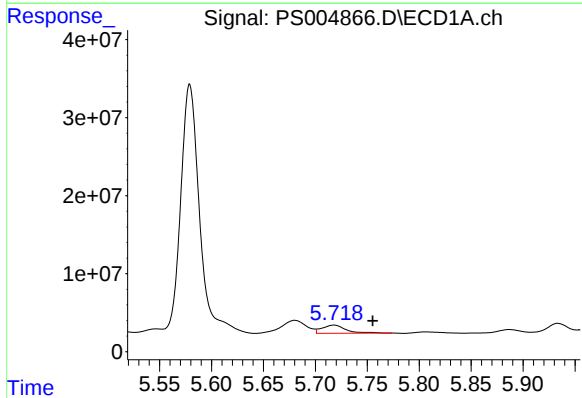


#5 DICAMBA

R.T.: 5.718 min
Delta R.T.: -0.037 min
Response: 16513328
Conc: 3.11 ng/ml

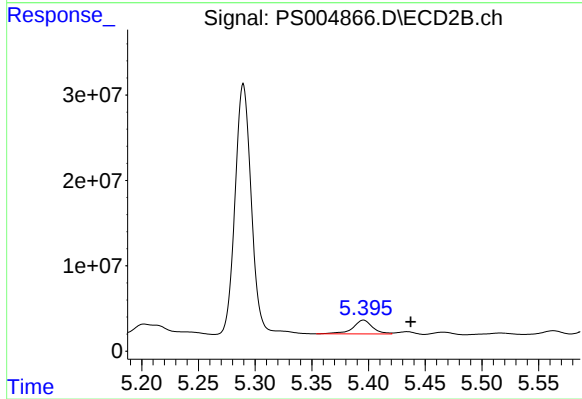

#5 DICAMBA


R.T.: 5.396 min
Delta R.T.: -0.042 min
Response: 19395015
Conc: 5.25 ng/ml

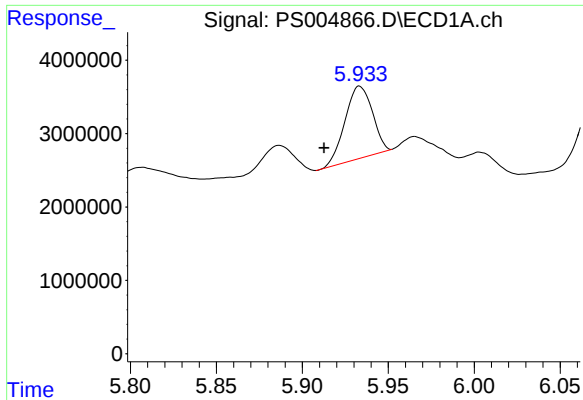

#6 MCPP


R.T.: 5.934 min
Delta R.T.: 0.021 min
Response: 10890534
Conc: 2.62 ug/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-9

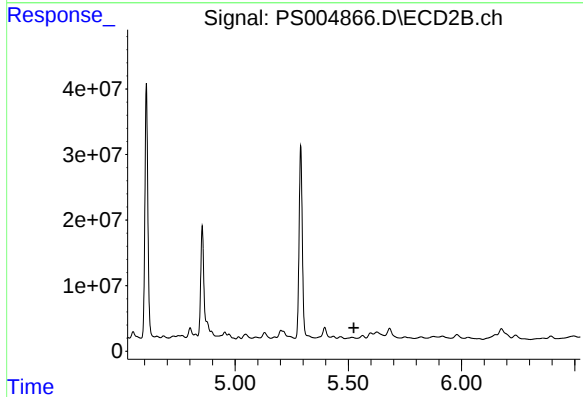


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

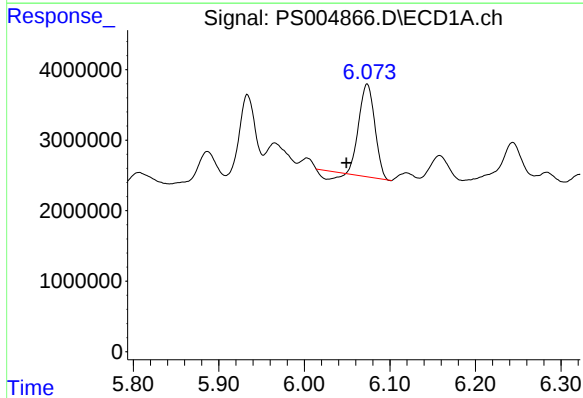


#7 MCPA

R.T.: 6.073 min
Delta R.T.: 0.024 min
Response: 16640647
Conc: 2.87 ug/ml

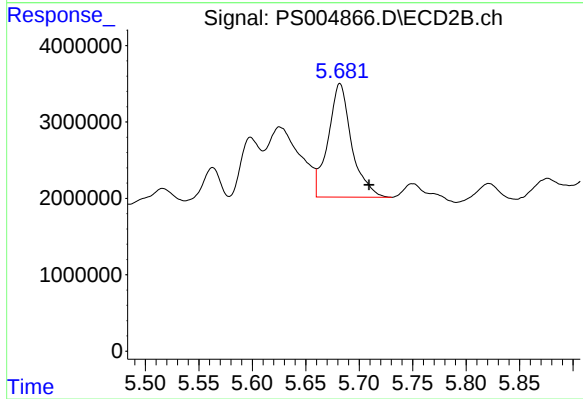

#7 MCPA


R.T.: 5.682 min
Delta R.T.: -0.027 min
Response: 22750841
Conc: 5.56 ug/ml

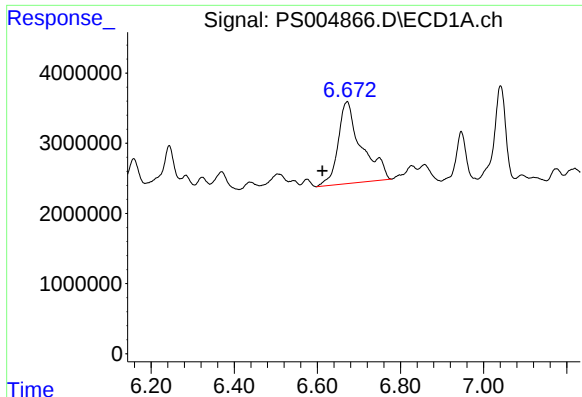

#9 2,4-D


R.T.: 6.671 min
Delta R.T.: 0.059 min
Response: 45379154
Conc: 33.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-9

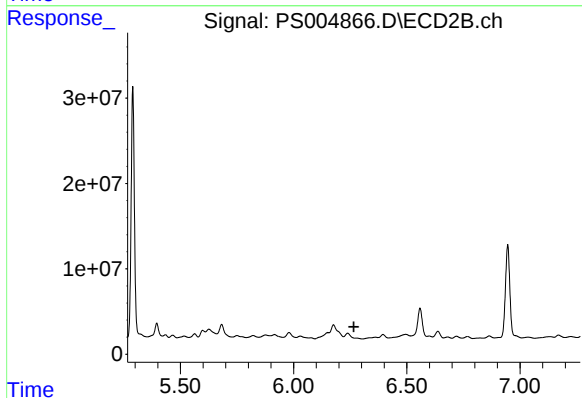


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

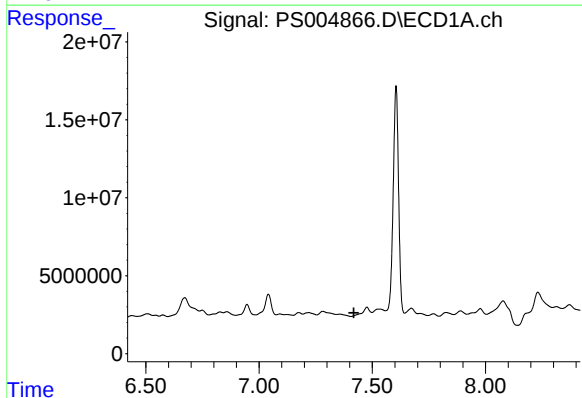


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

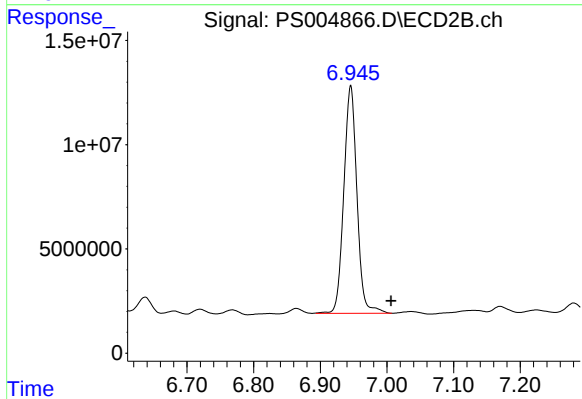

#11 2,4,5-TP (SILVEX)


R.T.: 6.946 min
Delta R.T.: -0.061 min
Response: 149633167
Conc: 29.08 ng/ml

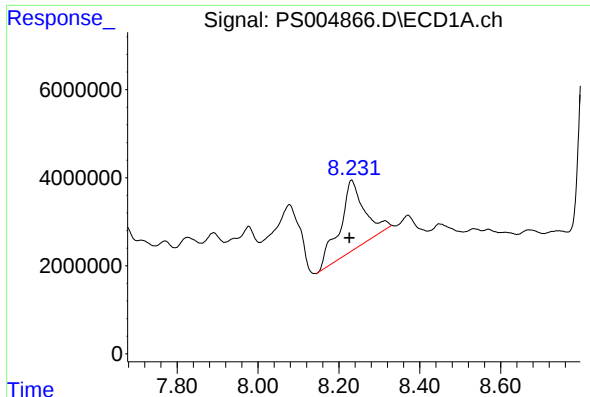

#13 2,4-DB


R.T.: 8.231 min
Delta R.T.: 0.005 min
Response: 67592858
Conc: 69.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-9

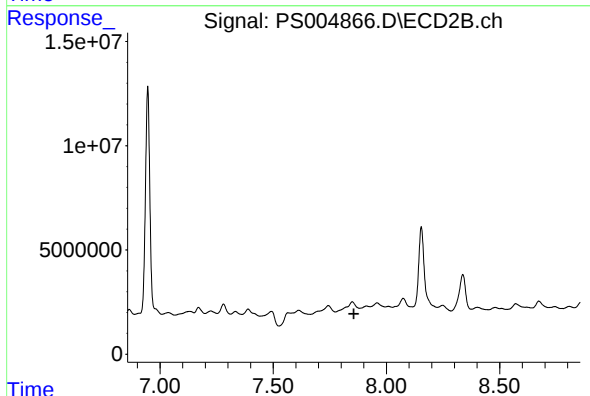


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.856 min
Response: 0
Conc: N.D.

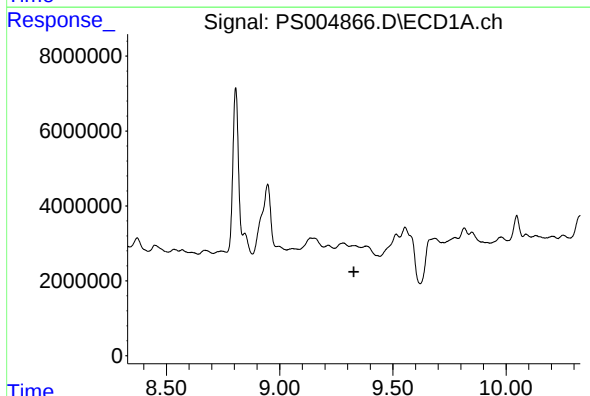

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.328 min
Response: 0
Conc: N.D.

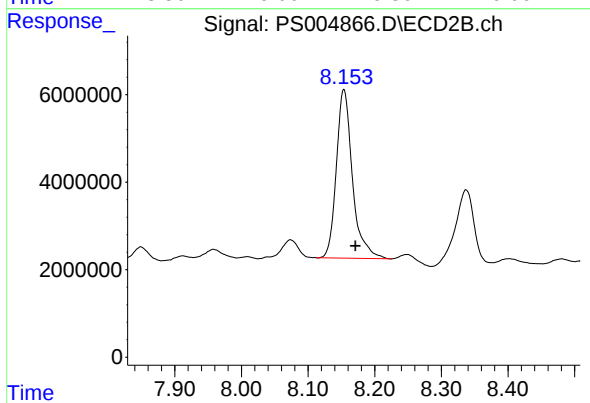

#14 DINOSEB

R.T.: 8.154 min
Delta R.T.: -0.017 min
Response: 64640581
Conc: 16.82 ng/ml