

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053119\
 Data File : PS004867.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2019 13:05
 Operator : SM\AJ
 Sample : K3084-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TEST-PIT-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 01:00:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.594	5.305	368.1E6	240.6E6	262.605	249.349
Target Compounds							
2) T	3,5-DICHL...	0.000	4.624	0	331.3E6	N.D.	268.865
3) T	4-Nitroph...	5.397	0.000	38258955	0	61.361	N.D. #
5) T	DICAMBA	5.733	5.412	17555495	20955486	3.306	5.672 #
6) T	MCP	5.949	0.000	10595430	0	2.545	N.D. #
7) T	MCPA	6.088	5.698	20211539	22969187	3.489	5.614 #
9) T	2,4-D	6.591	0.000	10714734	0	7.833	N.D. #
10) T	Pentachlo...	0.000	6.574	0	55047606	N.D.	4.481
11) T	2,4,5-TP ...	0.000	6.961	0	143.8E6	N.D.	27.947
13) T	2,4-DB	8.247	7.865	4567652	12314768	4.729	18.841 #
14) T	DINOSEB	0.000	8.170	0	67412396	N.D.	17.536



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053119\
Data File : PS004867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2019 13:05
Operator : SM\AJ
Sample : K3084-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 01:00:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

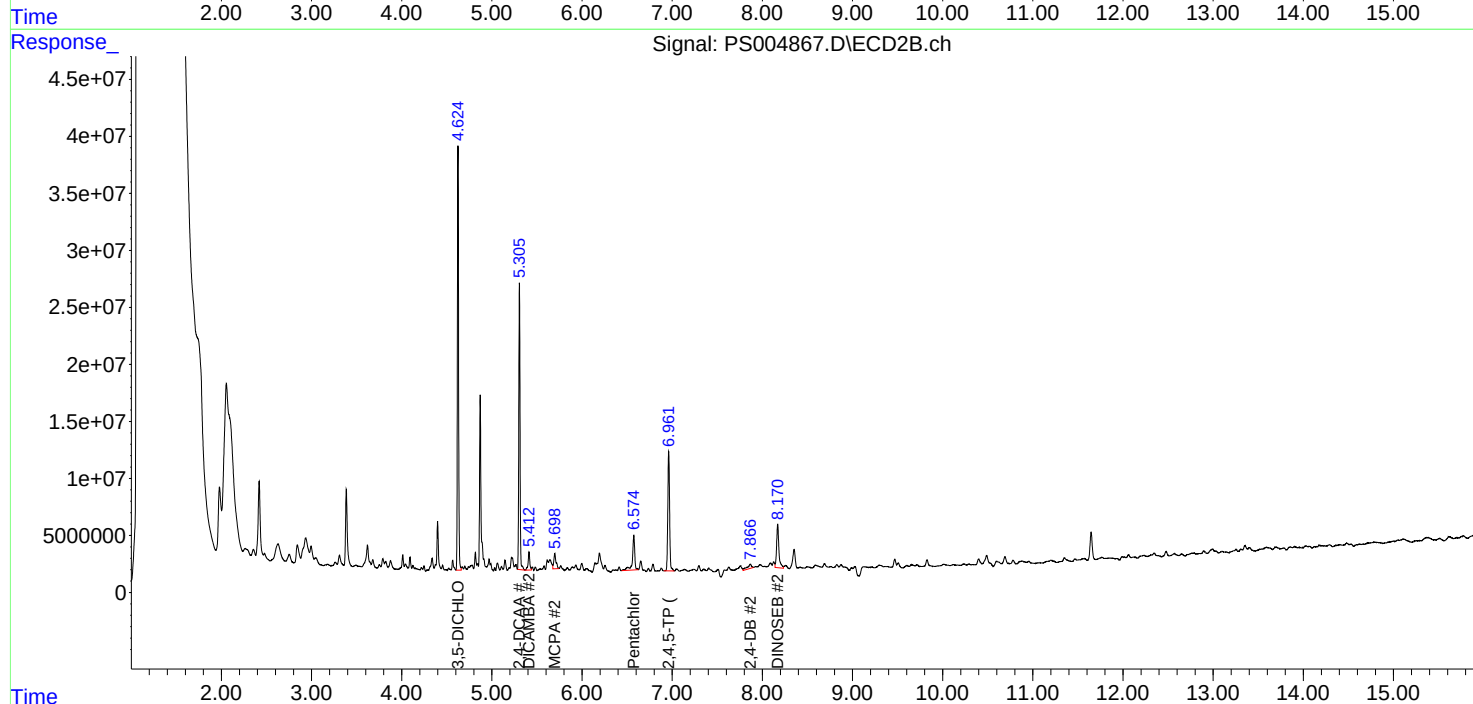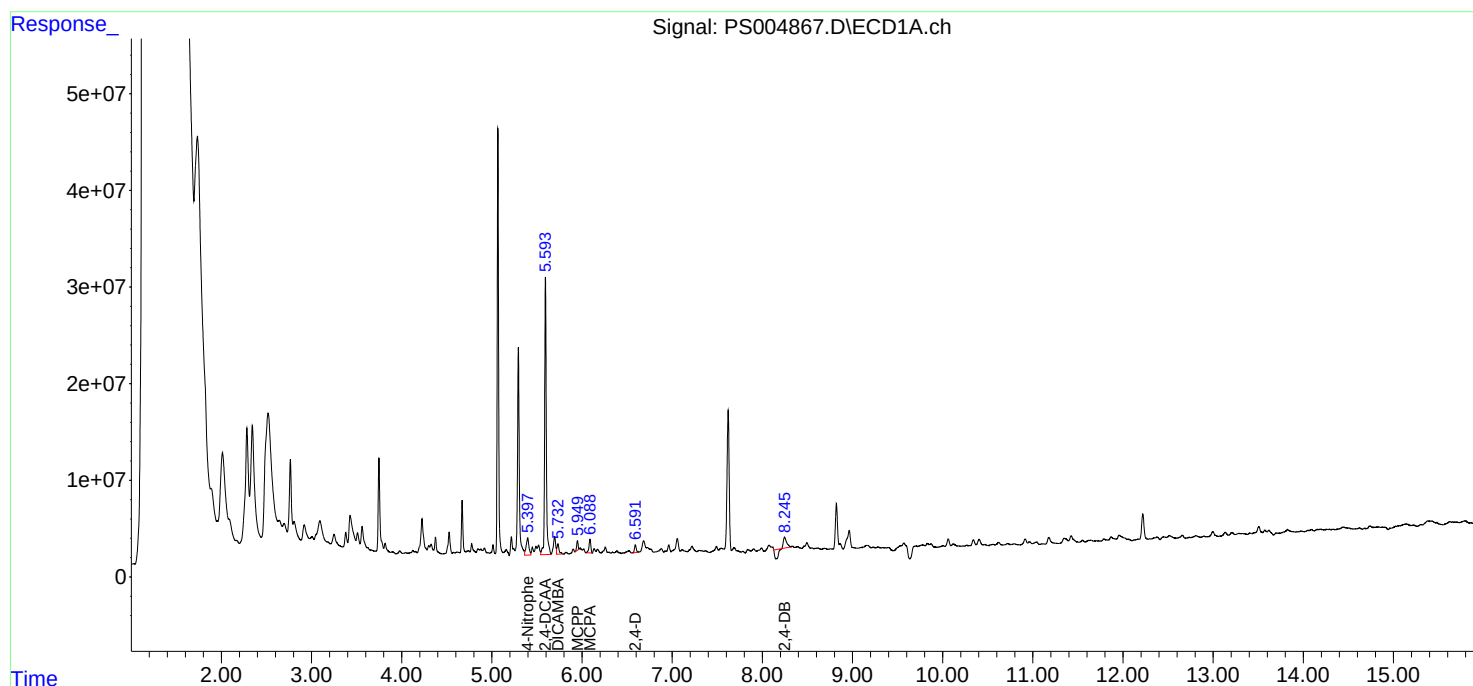


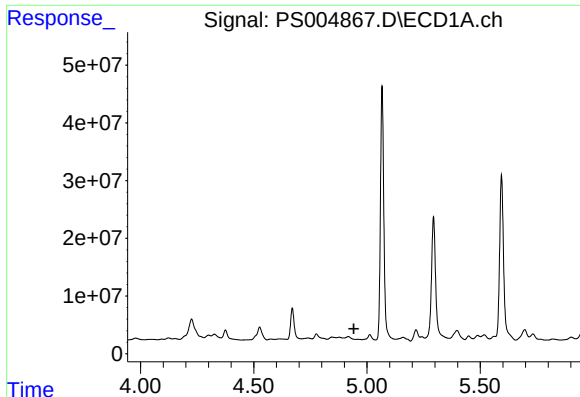

#2 3,5-DICHLOROBenzoIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-10

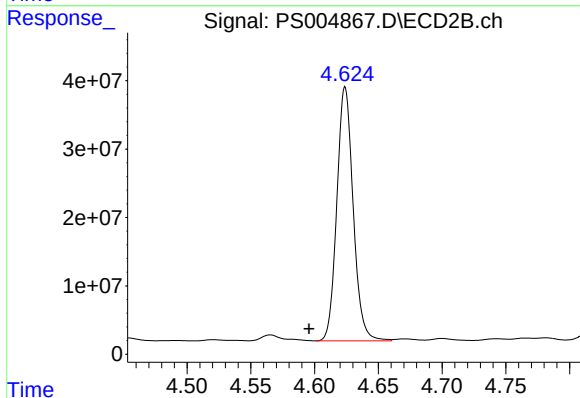


#2 3,5-DICHLOROBenzoIC ACID

R.T.: 4.624 min
Delta R.T.: 0.029 min
Response: 331275600
Conc: 268.86 ng/ml

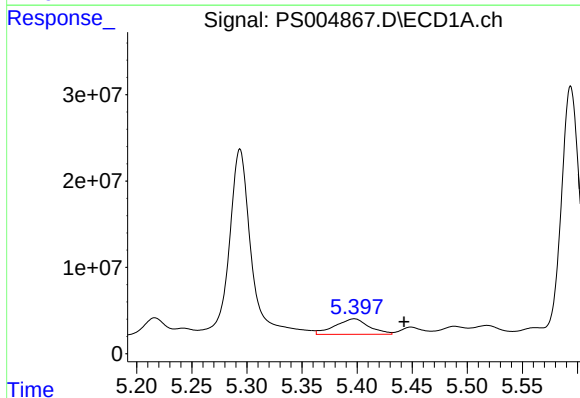


#3 4-Nitrophenol

R.T.: 5.397 min
Delta R.T.: -0.045 min
Response: 38258955
Conc: 61.36 ng/ml

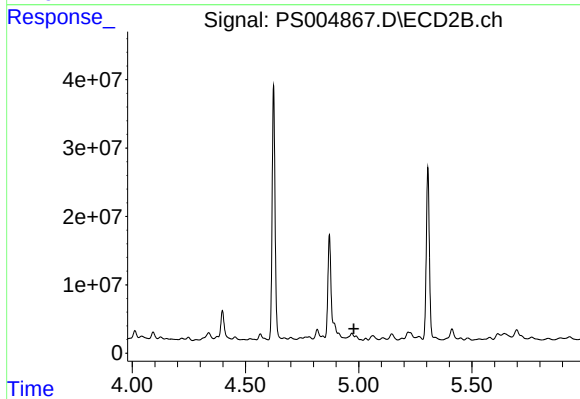

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

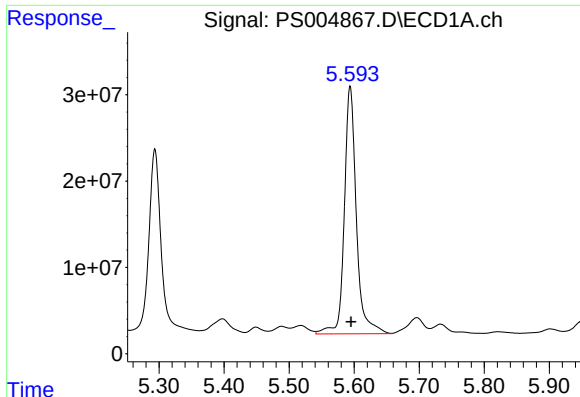

#4 2,4-DCAA


R.T.: 5.594 min
Delta R.T.: -0.001 min
Response: 368107853
Conc: 262.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-10

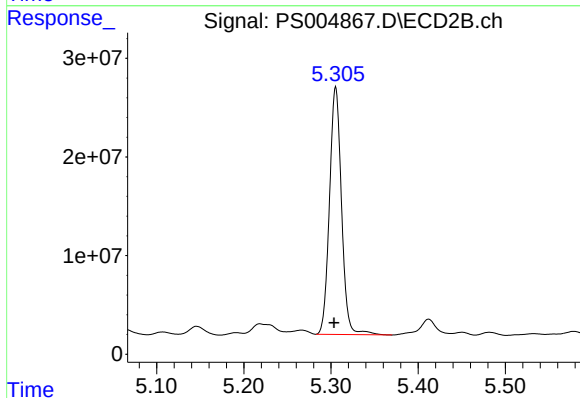


#4 2,4-DCAA

R.T.: 5.305 min
Delta R.T.: 0.002 min
Response: 240580700
Conc: 249.35 ng/ml

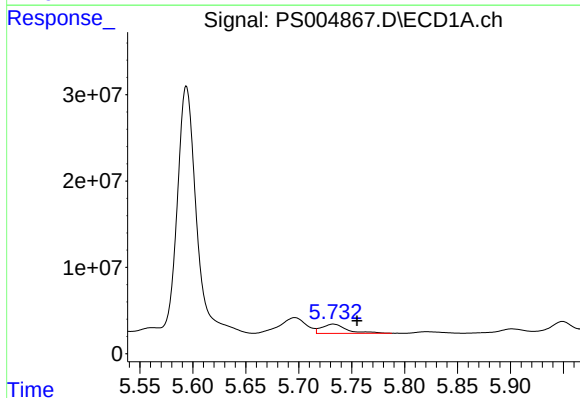


#5 DICAMBA

R.T.: 5.733 min
Delta R.T.: -0.022 min
Response: 17555495
Conc: 3.31 ng/ml

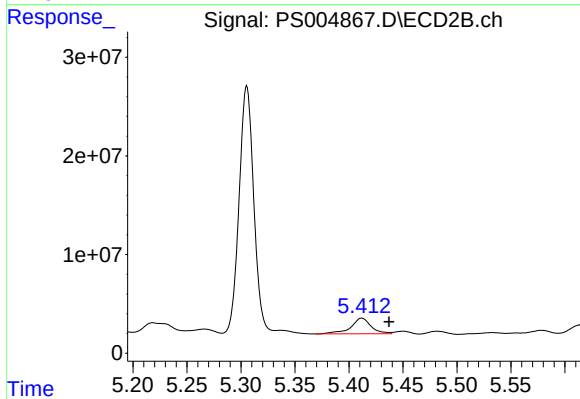

#5 DICAMBA


R.T.: 5.412 min
Delta R.T.: -0.025 min
Response: 20955486
Conc: 5.67 ng/ml

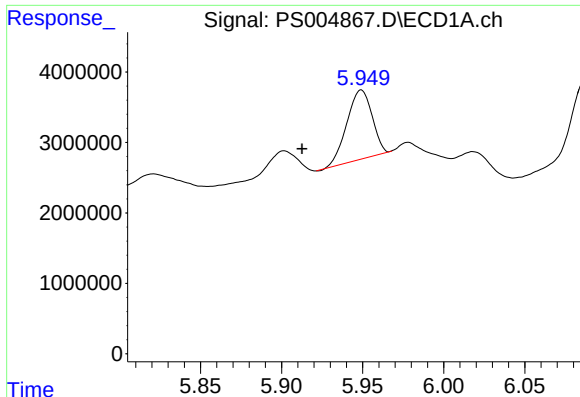

#6 MCPP


R.T.: 5.949 min
Delta R.T.: 0.036 min
Response: 10595430
Conc: 2.55 ug/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-10

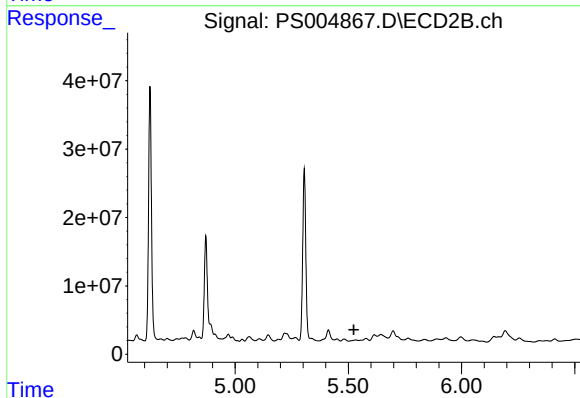


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

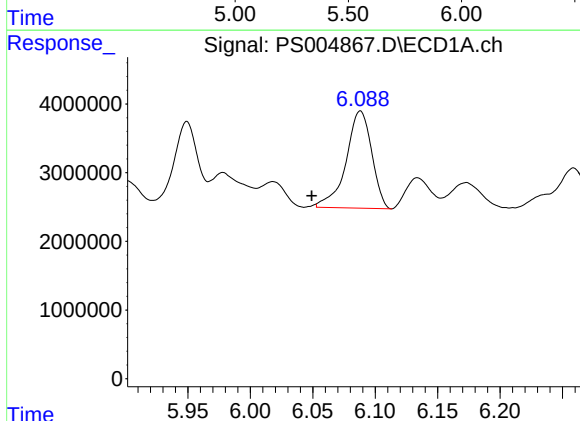


#7 MCPA

R.T.: 6.088 min
Delta R.T.: 0.039 min
Response: 20211539
Conc: 3.49 ug/ml

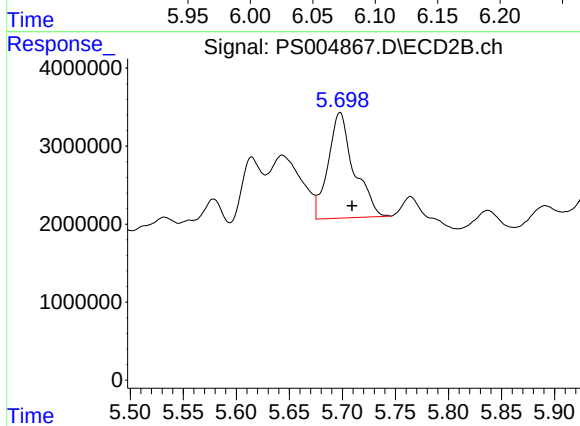

#7 MCPA


R.T.: 5.698 min
Delta R.T.: -0.011 min
Response: 22969187
Conc: 5.61 ug/ml

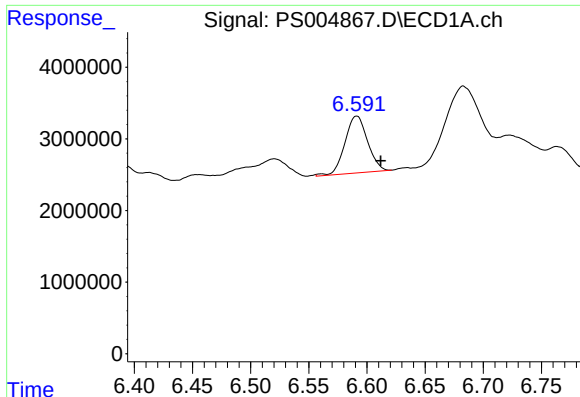

#9 2,4-D


R.T.: 6.591 min
Delta R.T.: -0.021 min
Response: 10714734
Conc: 7.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-10

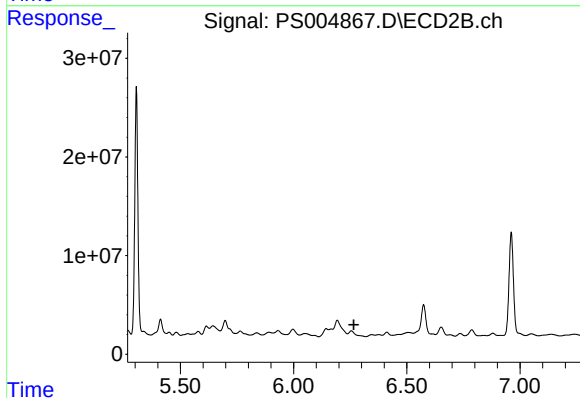


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

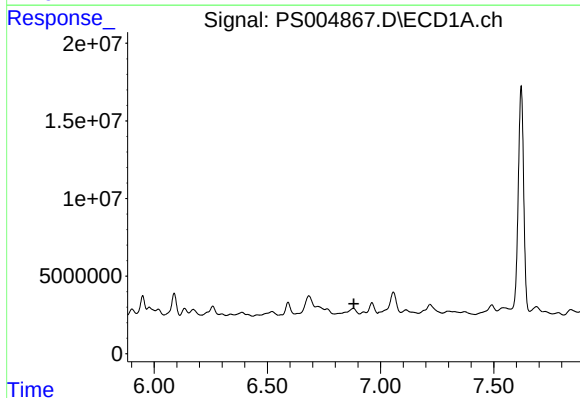


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.882 min
Response: 0
Conc: N.D.

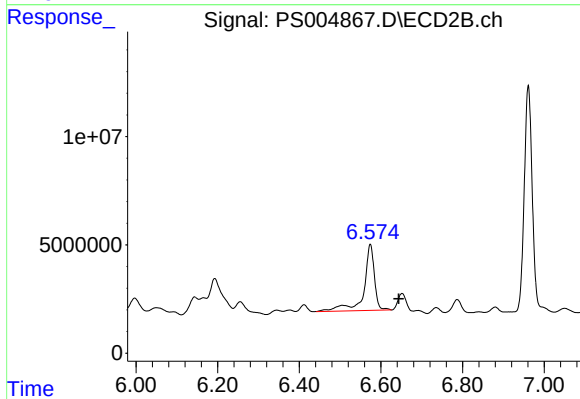

#10 Pentachlorophenol


R.T.: 6.574 min
Delta R.T.: -0.070 min
Response: 55047606
Conc: 4.48 ng/ml

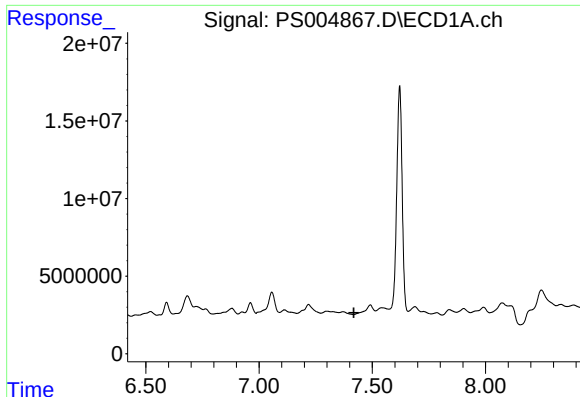

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-10

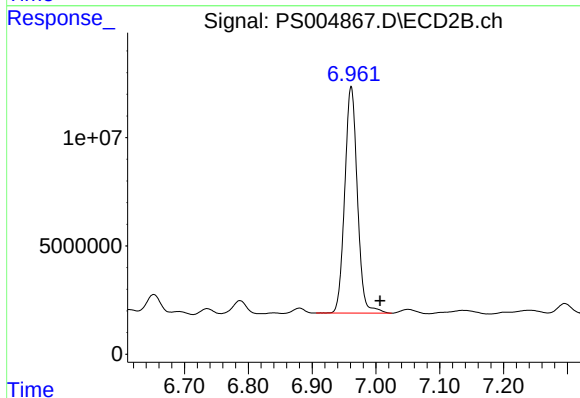


#11 2,4,5-TP (SILVEX)

R.T.: 6.961 min
Delta R.T.: -0.045 min
Response: 143794408
Conc: 27.95 ng/ml

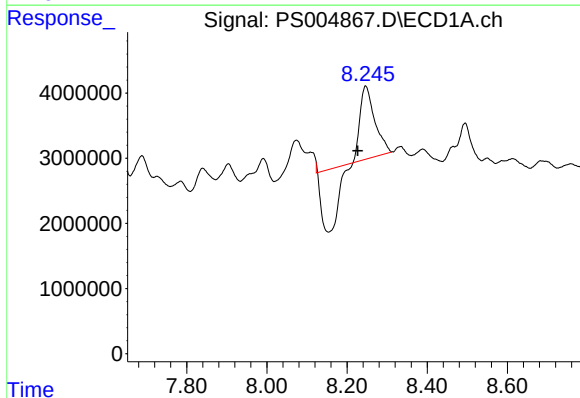


#13 2,4-DB

R.T.: 8.247 min
Delta R.T.: 0.020 min
Response: 4567652
Conc: 4.73 ng/ml

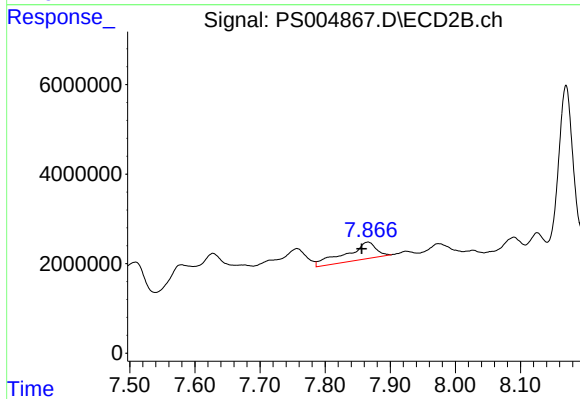

#13 2,4-DB


R.T.: 7.865 min
Delta R.T.: 0.009 min
Response: 12314768
Conc: 18.84 ng/ml

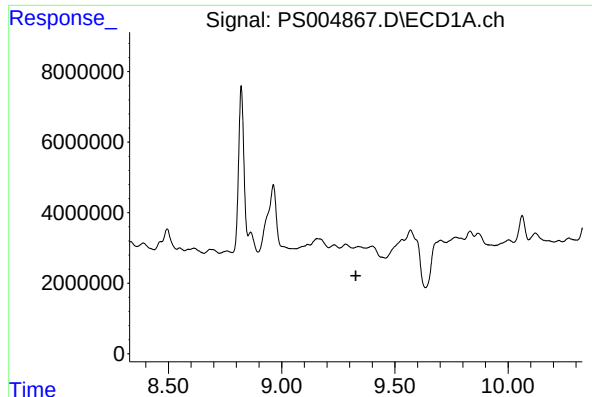

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-10

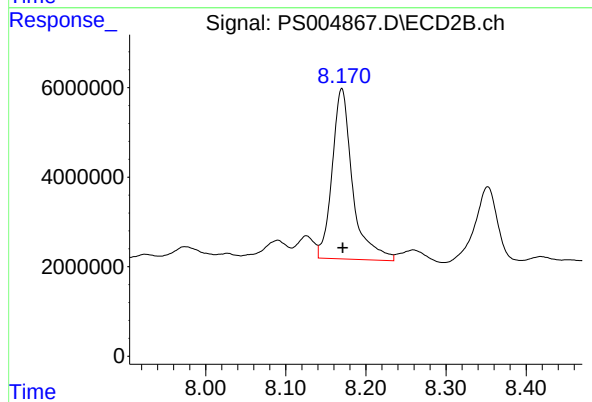

#14 DINOSEB

R.T.: 8.170 min
Delta R.T.: -0.001 min
Response: 67412396
Conc: 17.54 ng/ml