

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
 Data File : PS004870.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2019 07:49
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 05:23:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds								
2) T	3,5-DICHL...	4.961	0.000	22667642	0	13.144	N.D.	#
5) T	DICAMBA	0.000	5.458	0	19067684	N.D.	5.161	
6) T	MCP	0.000	5.458	0	19067684	N.D.	6.959	
9) T	2,4-D	6.636	0.000	49633206	0	36.284	N.D.	#
12) T	2,4,5-T	0.000	7.408	0	14521930	N.D.	3.258	
15) T	Picloram	9.161	9.116	107.7E6	72554410	10.337	9.725	
16) T	DCPA	0.000	9.116	0	72554410	N.D.	11.200	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
Data File : PS004870.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2019 07:49
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 05:23:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

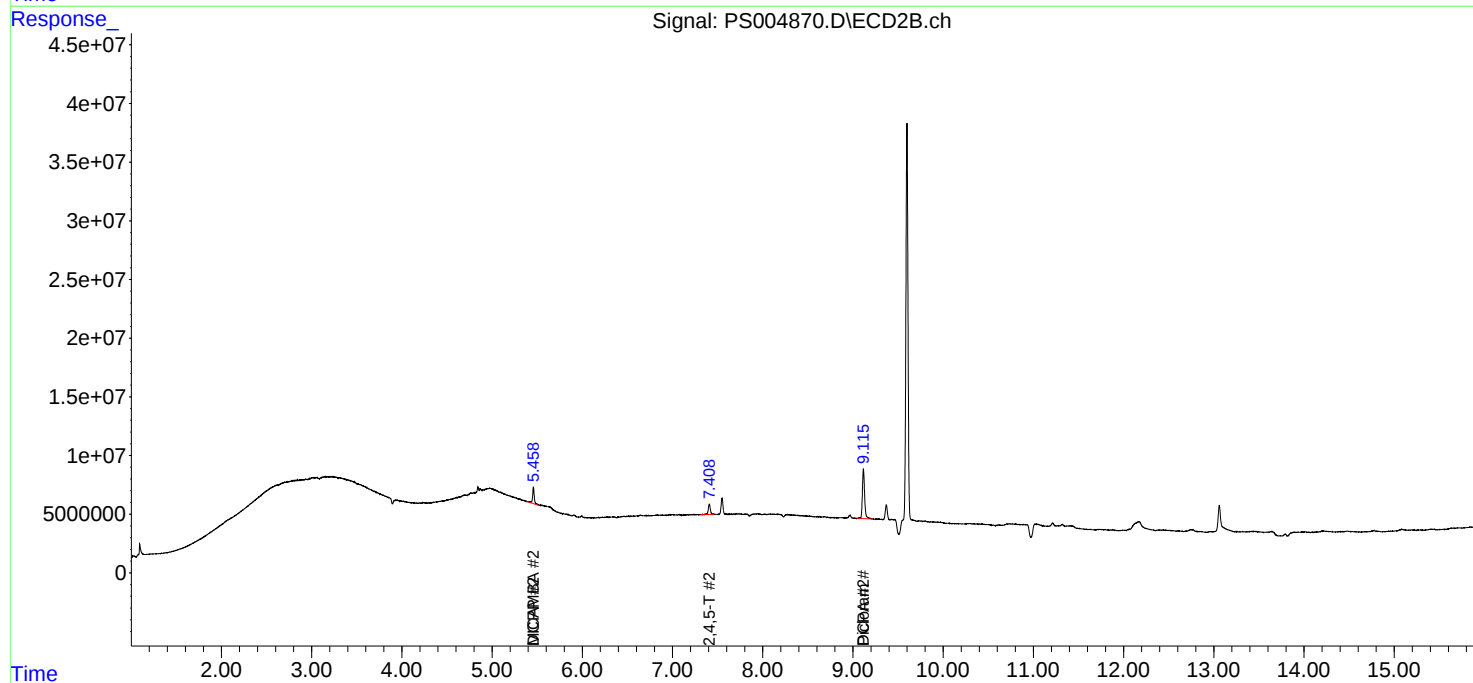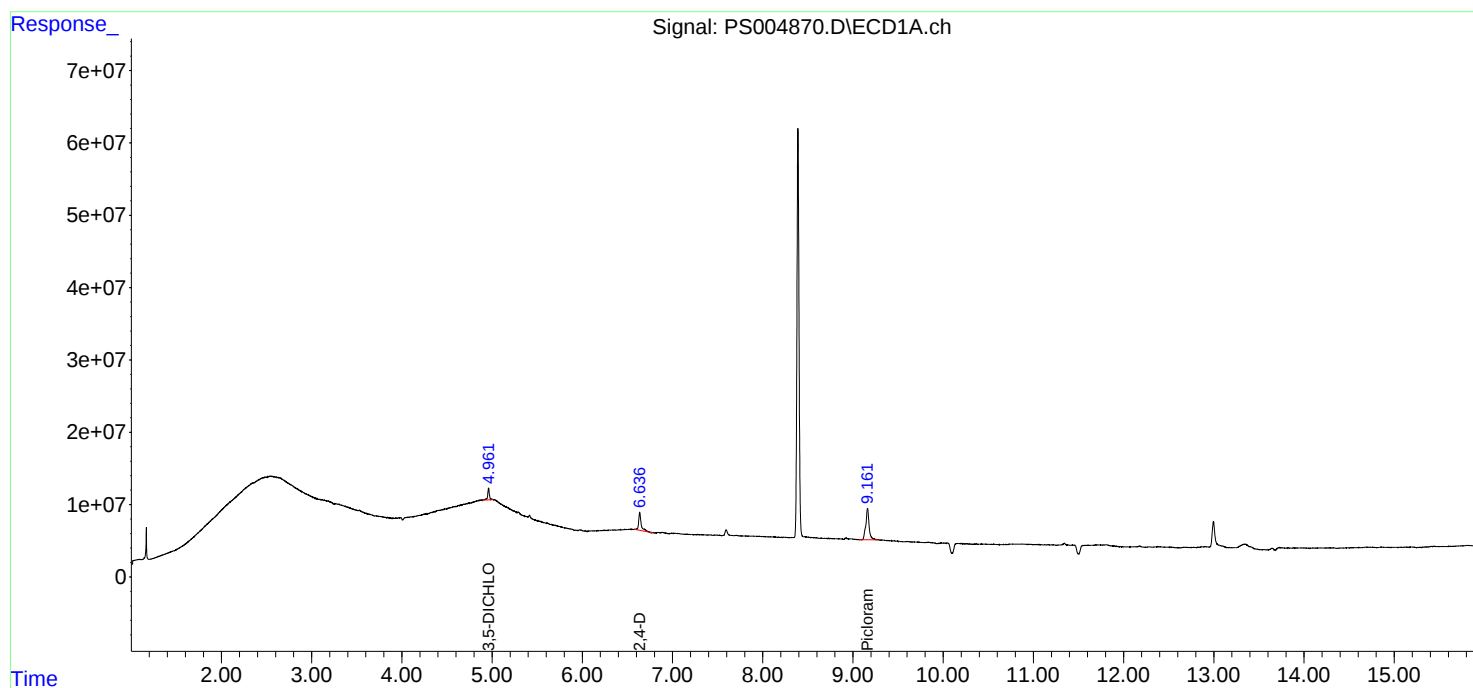


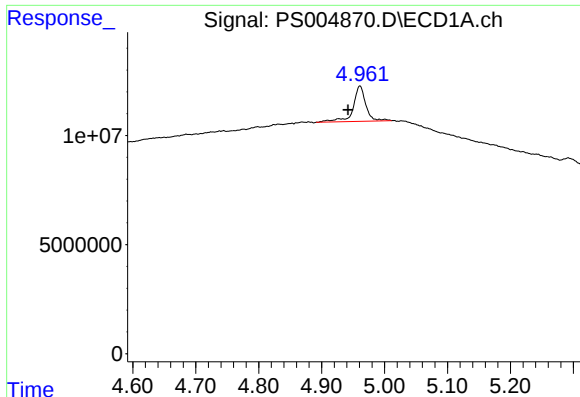

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.961 min
Delta R.T.: 0.019 min
Response: 22667642
Conc: 13.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

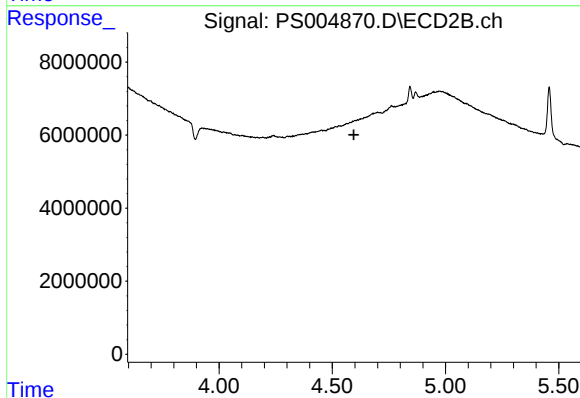


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

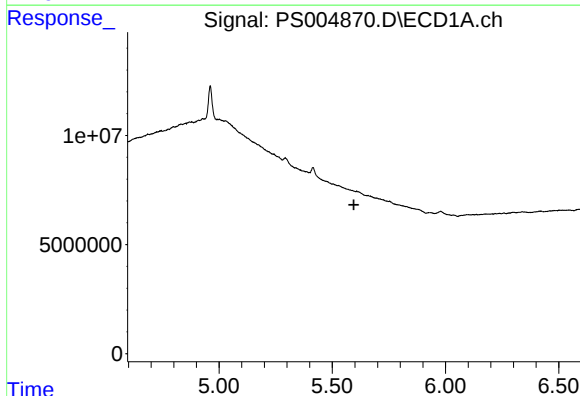


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.595 min
Response: 0
Conc: N.D.

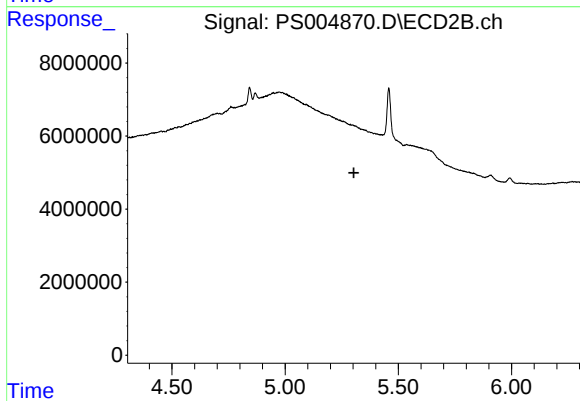

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.304 min
Response: 0
Conc: N.D.

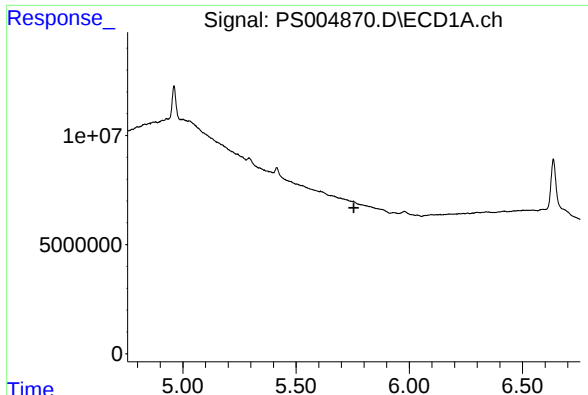

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

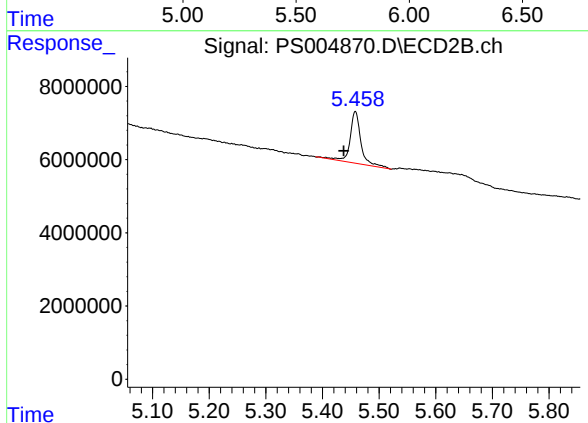


#5 DICAMBA

R.T.: 5.458 min
Delta R.T.: 0.021 min
Response: 19067684
Conc: 5.16 ng/ml

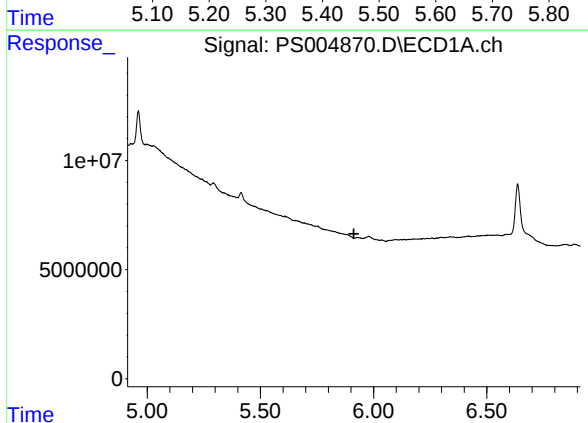


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.913 min
Response: 0
Conc: N.D.

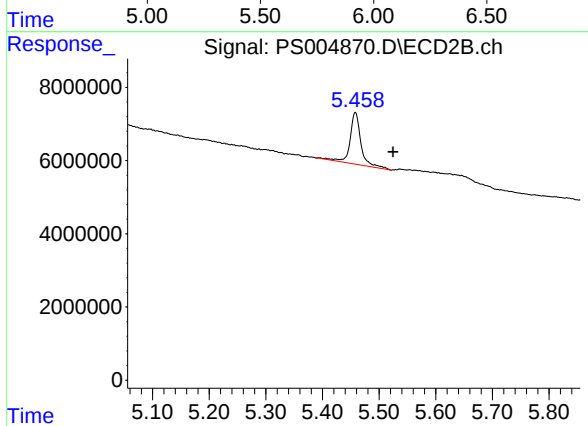

#6 MCPP


R.T.: 5.458 min
Delta R.T.: -0.066 min
Response: 19067684
Conc: 6.96 ug/ml

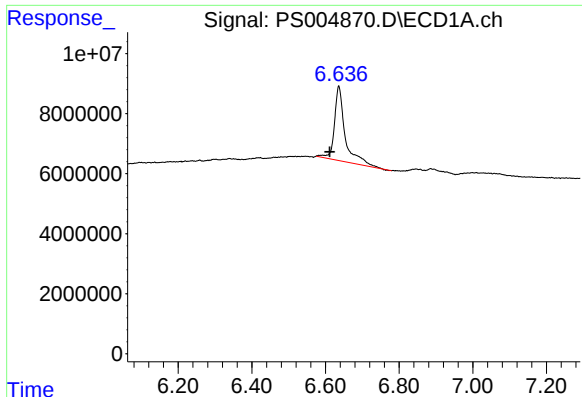

#9 2,4-D


R.T.: 6.636 min
Delta R.T.: 0.024 min
Response: 49633206
Conc: 36.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

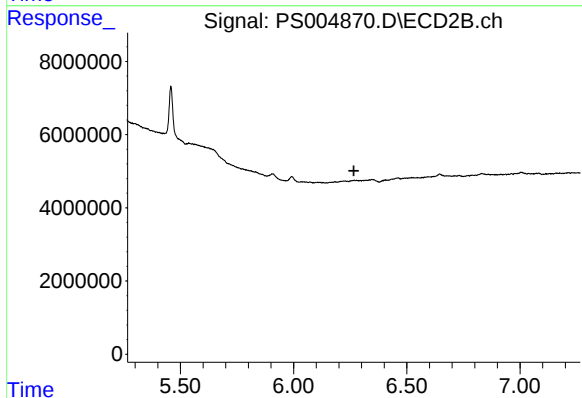


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

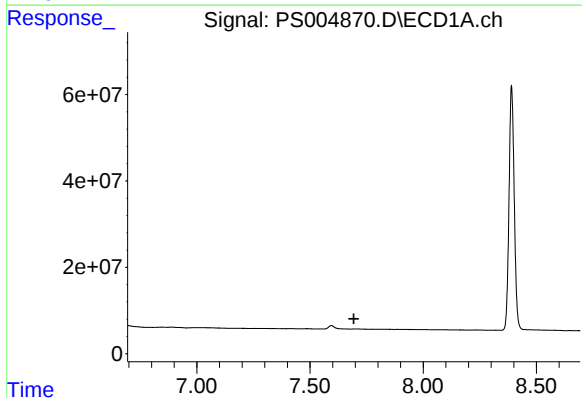


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.693 min
Response: 0
Conc: N.D.

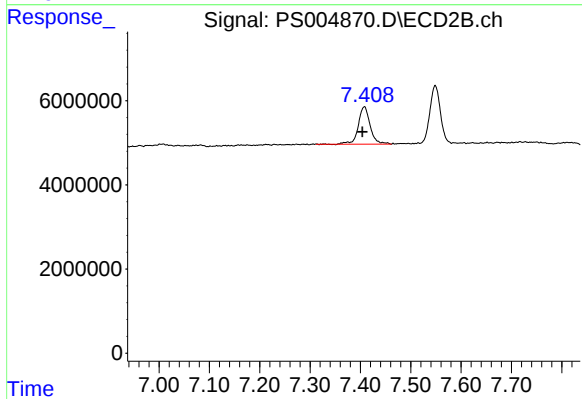

#12 2,4,5-T


R.T.: 7.408 min
Delta R.T.: 0.004 min
Response: 14521930
Conc: 3.26 ng/ml

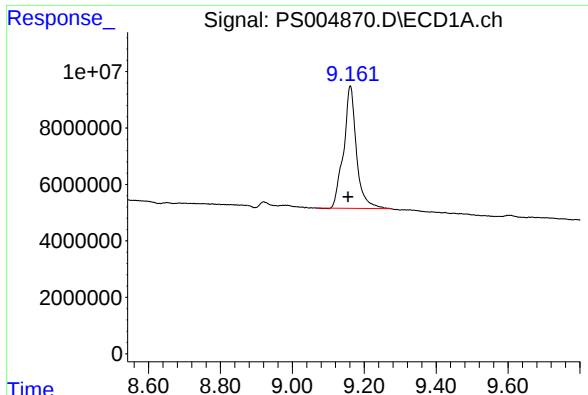

#15 Picloram


R.T.: 9.161 min
Delta R.T.: 0.006 min
Response: 107715912
Conc: 10.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

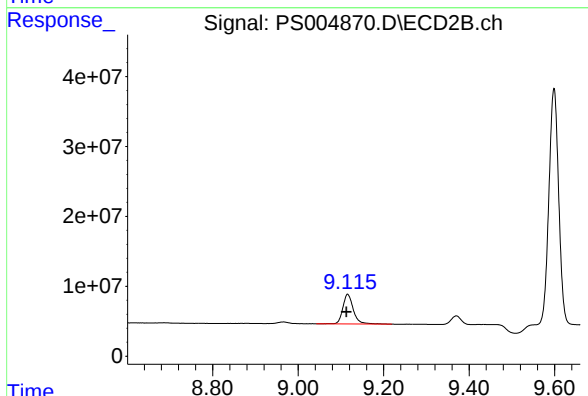


#15 Picloram

R.T.: 9.116 min
Delta R.T.: 0.003 min
Response: 72554410
Conc: 9.73 ng/ml

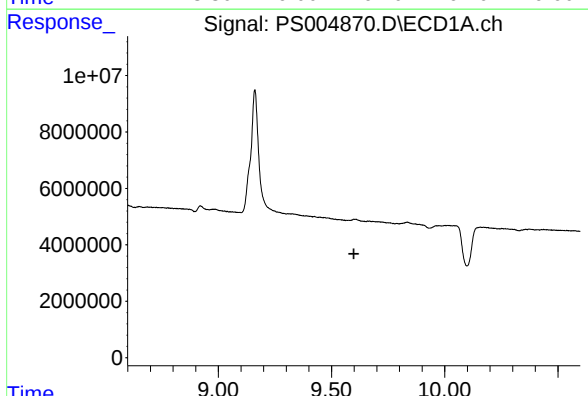

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.599 min
Response: 0
Conc: N.D.

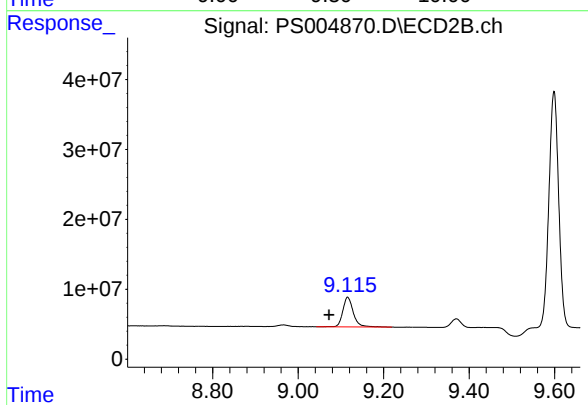

#16 DCPA

R.T.: 9.116 min
Delta R.T.: 0.044 min
Response: 72554410
Conc: 11.20 ng/ml