

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
 Data File : PS004871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2019 08:11
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 05:24:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.588	5.299	619.7E6	475.2E6	442.121	492.568
Target Compounds							
2) T	3,5-DICHL...	4.955	0.000	17333694	0	10.051	N.D. #
5) T	DICAMBA	0.000	5.455	0	19465897	N.D.	5.269
6) T	MCP	0.000	5.455	0	19465897	N.D.	7.104
9) T	2,4-D	6.631	0.000	30226345	0	22.097	N.D. #
15) T	Picloram	9.126	9.115	432.7E6	40408841	41.527	5.416 #
16) T	DCPA	0.000	9.115	0	40408841	N.D.	6.238



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
Data File : PS004871.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2019 08:11
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 05:24:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

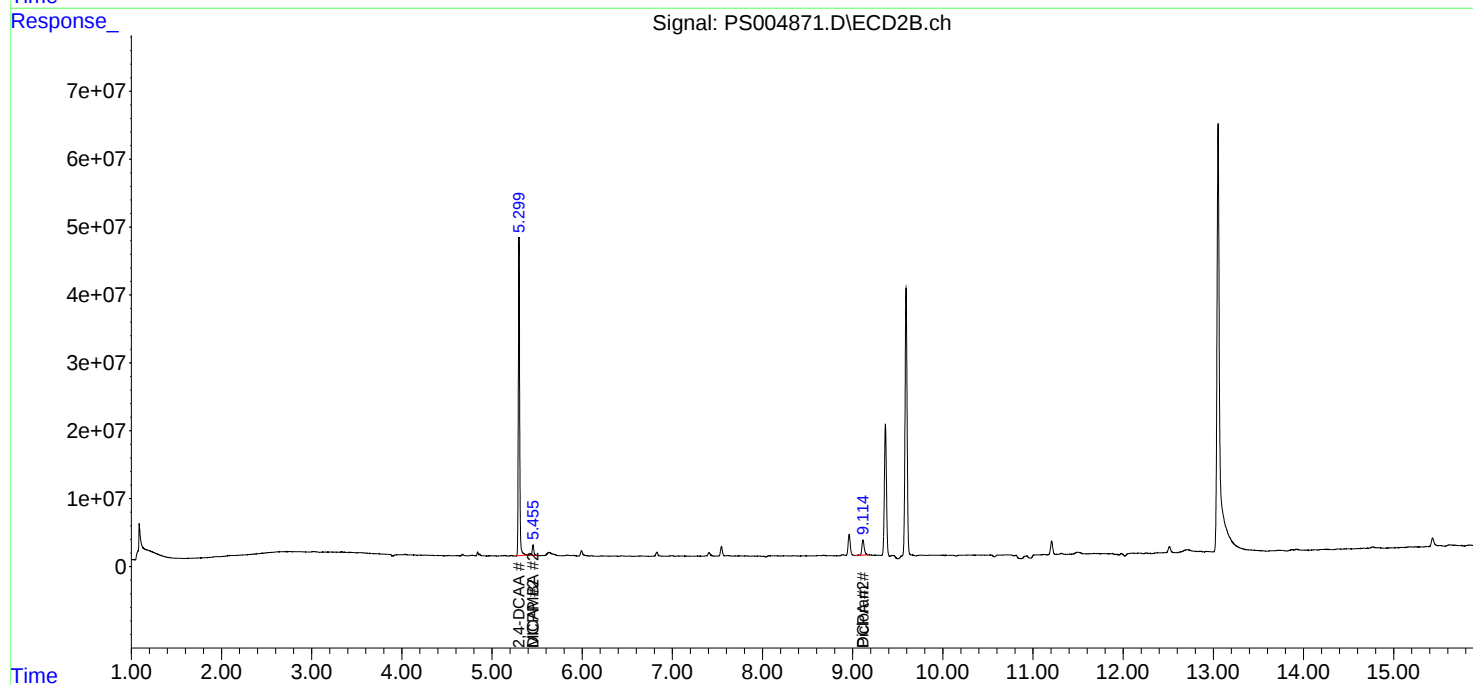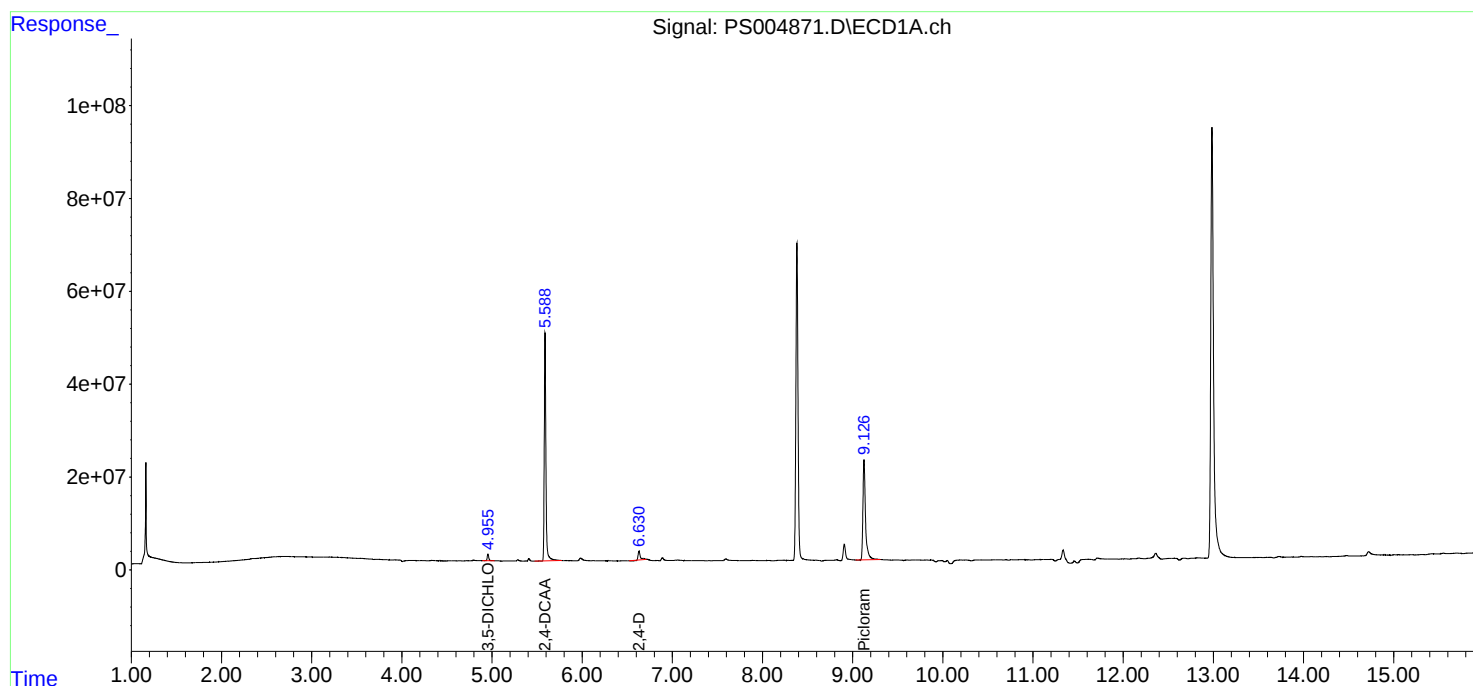


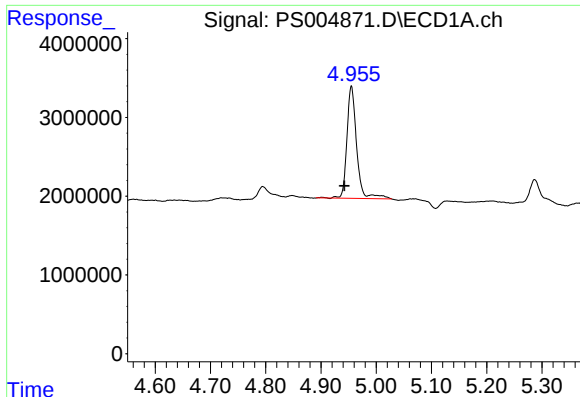

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.955 min
Delta R.T.: 0.013 min
Response: 17333694
Conc: 10.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

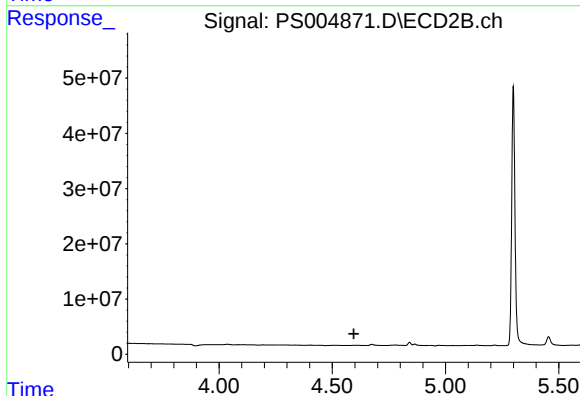


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

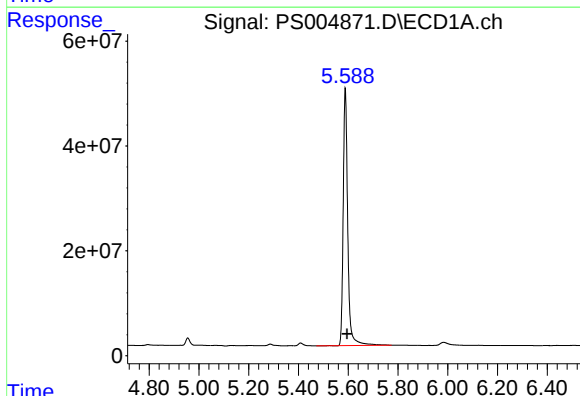


#4 2,4-DCAA

R.T.: 5.588 min
Delta R.T.: -0.007 min
Response: 619746447
Conc: 442.12 ng/ml

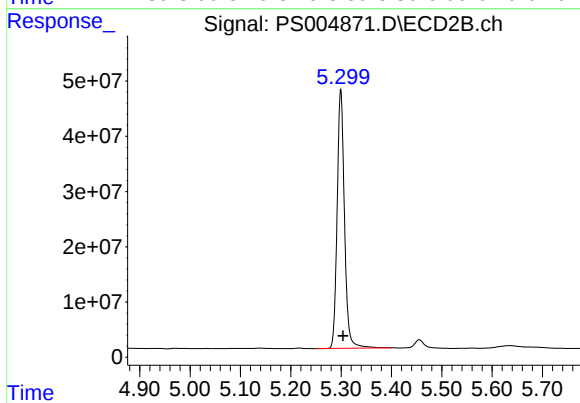

#4 2,4-DCAA


R.T.: 5.299 min
Delta R.T.: -0.004 min
Response: 475247221
Conc: 492.57 ng/ml

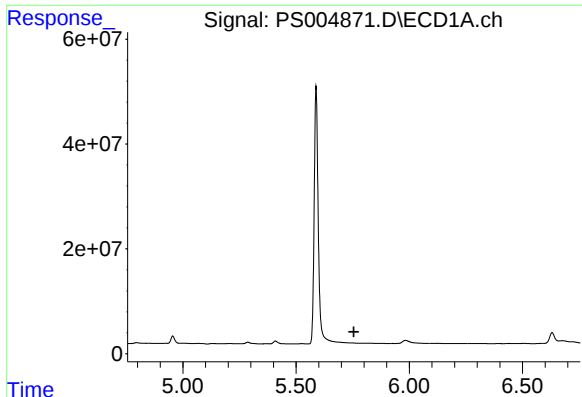

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

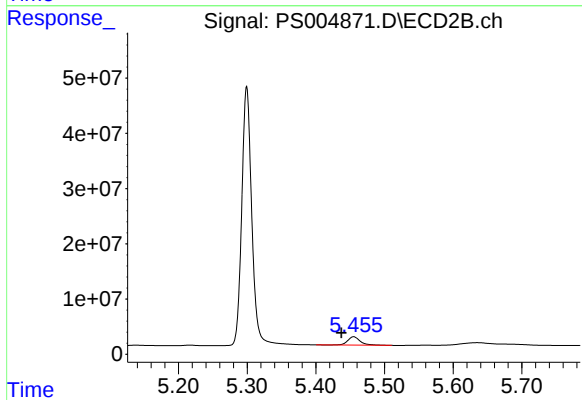


#5 DICAMBA

R.T.: 5.455 min
Delta R.T.: 0.018 min
Response: 19465897
Conc: 5.27 ng/ml

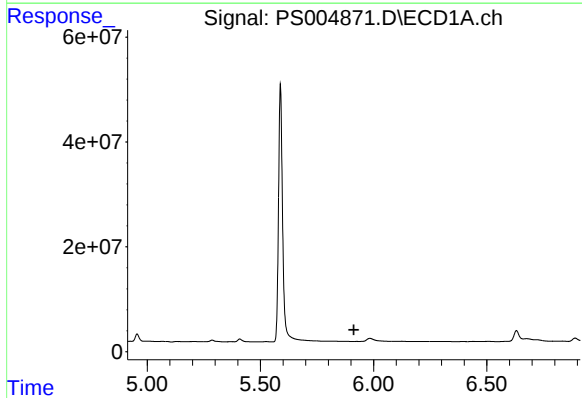


#6 MCP

R.T.: 0.000 min
Exp R.T.: 5.913 min
Response: 0
Conc: N.D.

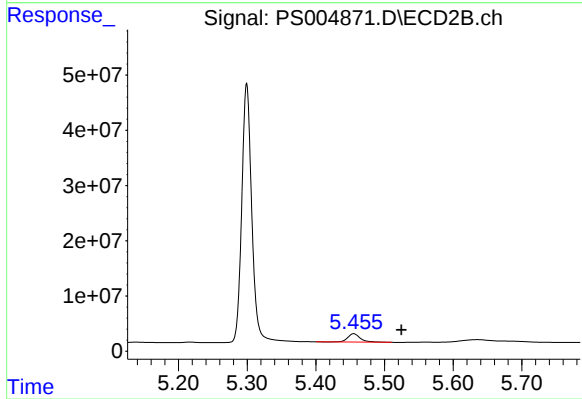

#6 MCP


R.T.: 5.455 min
Delta R.T.: -0.069 min
Response: 19465897
Conc: 7.10 ug/ml

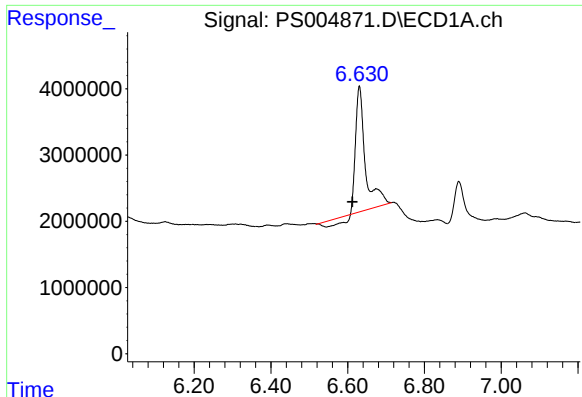

#9 2,4-D


R.T.: 6.631 min
Delta R.T.: 0.019 min
Response: 30226345
Conc: 22.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

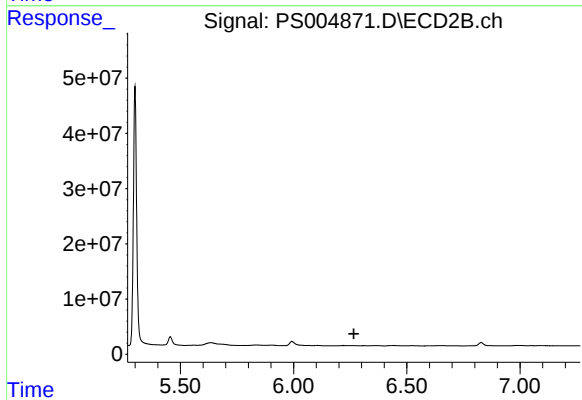


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

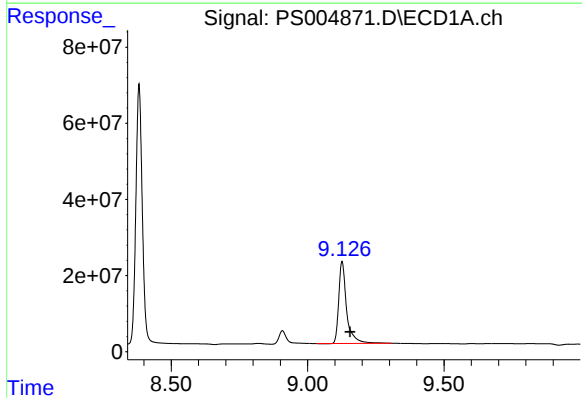


#15 Picloram

R.T.: 9.126 min
Delta R.T.: -0.029 min
Response: 432709518
Conc: 41.53 ng/ml

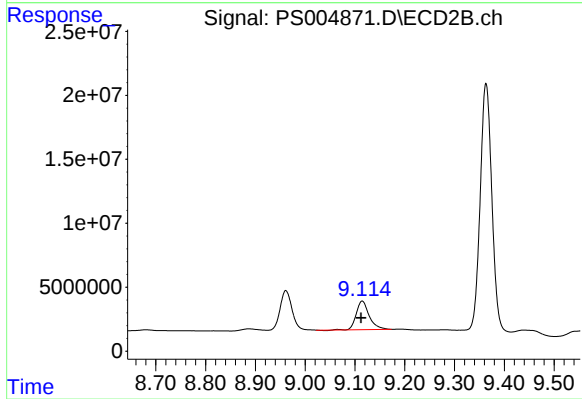

#15 Picloram


R.T.: 9.115 min
Delta R.T.: 0.002 min
Response: 40408841
Conc: 5.42 ng/ml

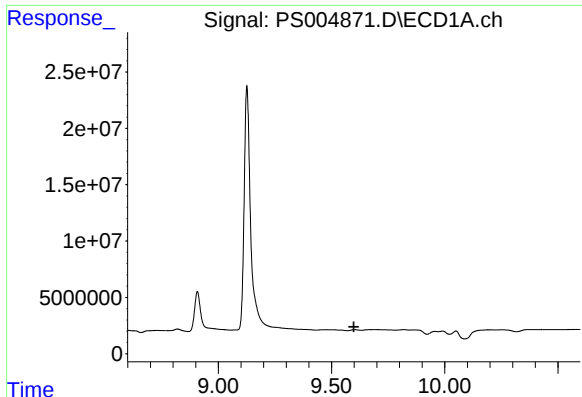

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

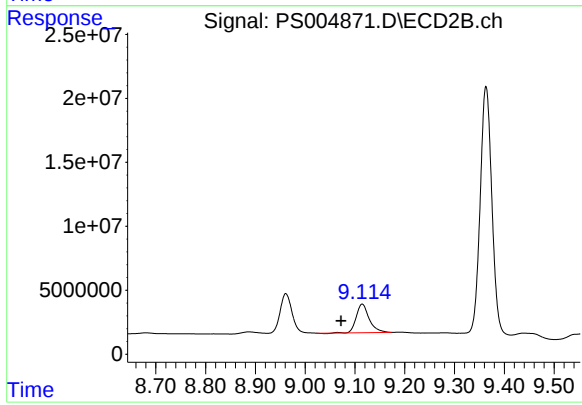

#16 DCPA

R.T.: 9.115 min
Delta R.T.: 0.043 min
Response: 40408841
Conc: 6.24 ng/ml