

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
 Data File : PS004873.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2019 09:38
 Operator : SM\AJ
 Sample : PB120234BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 05:24:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.576	5.287	795.1E6	596.0E6	567.202	617.762
Target Compounds							
1) T	Dalapon	2.079	1.767	48780827	16797812	29.427	13.017 #
2) T	3,5-DICHL...	0.000	4.606	0	193.9E6	N.D.	157.402
3) T	4-Nitroph...	5.381	0.000	32101084	0	51.485	N.D. #
7) T	MCPA	6.071	5.680	19321119	18880248	3.336	4.614 #
9) T	2,4-D	6.662	0.000	25134835	0	18.375	N.D. #
10) T	Pentachlo...	6.944	6.635	20597487	17154740	1.173	1.396
11) T	2,4,5-TP ...	0.000	6.943	0	31413915	N.D.	6.105
12) T	2,4,5-T	0.000	7.393	0	18473438	N.D.	4.145
13) T	2,4-DB	8.230	0.000	12116863	0	12.544	N.D. #
14) T	DINOSEB	0.000	8.152	0	33321343	N.D.	8.668
15) T	Picloram	9.146	9.102	102.7E6	94687537	9.855	12.692 #
16) T	DCPA	0.000	9.102	0	94687537	N.D.	14.617



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
Data File : PS004873.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2019 09:38
Operator : SM\AJ
Sample : PB120234BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 05:24:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

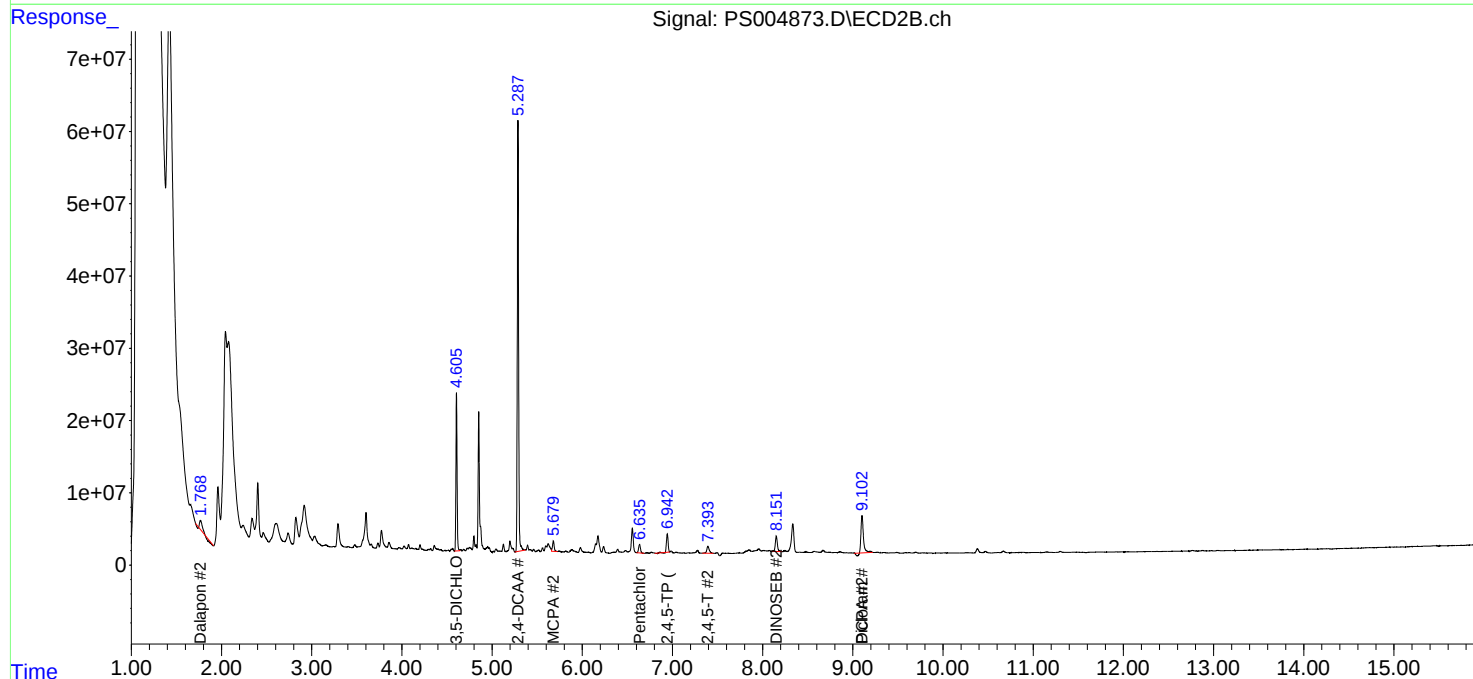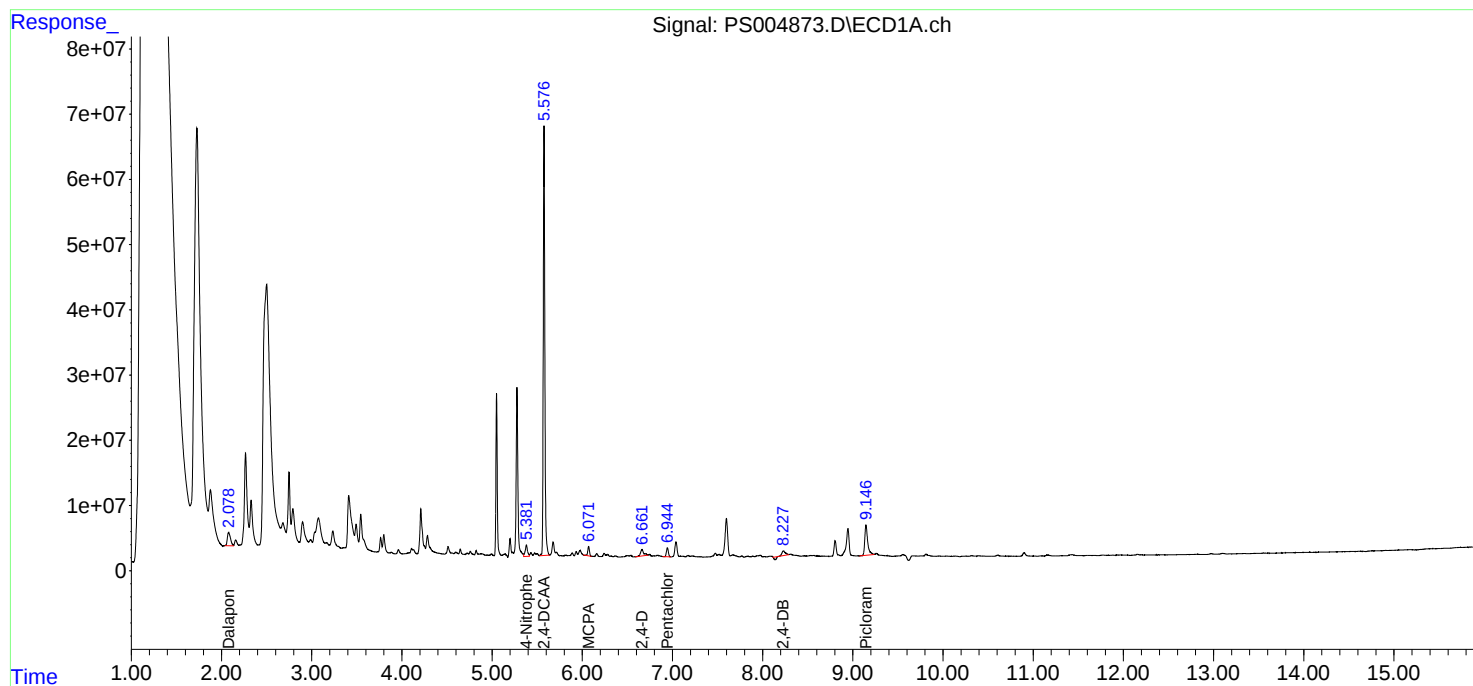


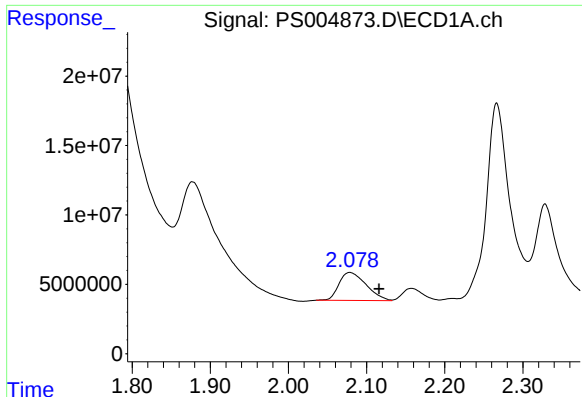

#1 Dalapon


R.T.: 2.079 min
Delta R.T.: -0.037 min
Response: 48780827
Conc: 29.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

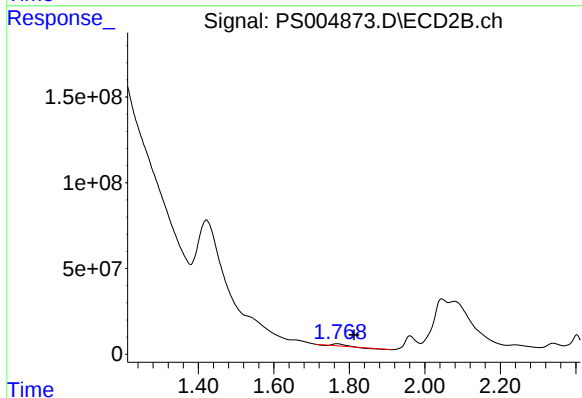


#1 Dalapon

R.T.: 1.767 min
Delta R.T.: -0.046 min
Response: 16797812
Conc: 13.02 ng/ml

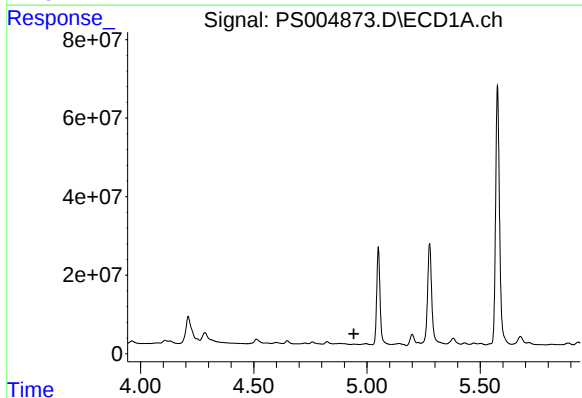


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

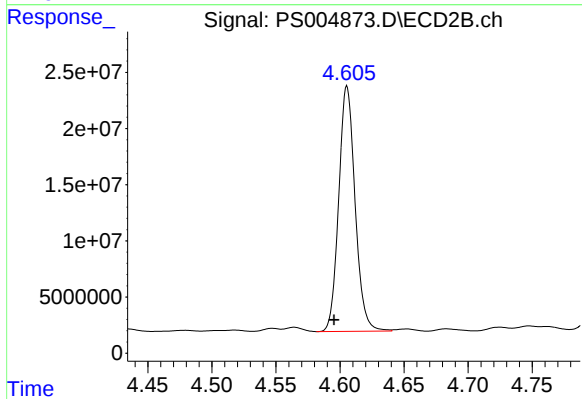

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.606 min
Delta R.T.: 0.010 min
Response: 193939161
Conc: 157.40 ng/ml

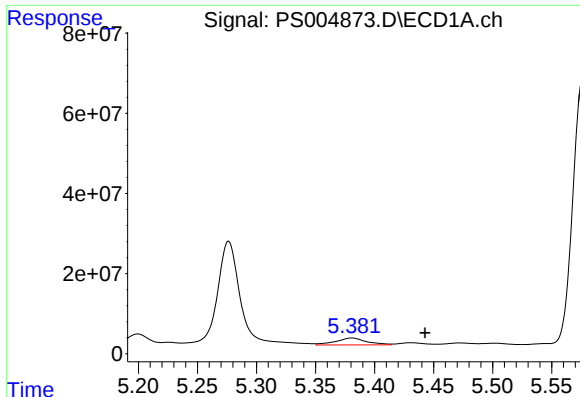

#3 4-Nitrophenol


R.T.: 5.381 min
Delta R.T.: -0.062 min
Response: 32101084
Conc: 51.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

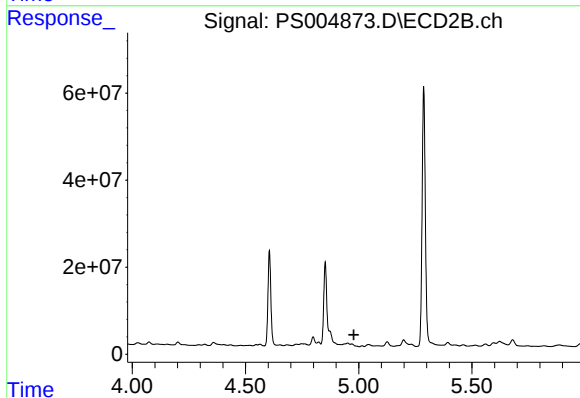


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

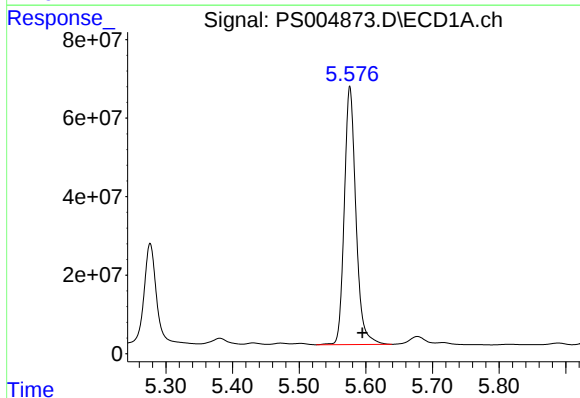


#4 2,4-DCAA

R.T.: 5.576 min
Delta R.T.: -0.019 min
Response: 795078960
Conc: 567.20 ng/ml

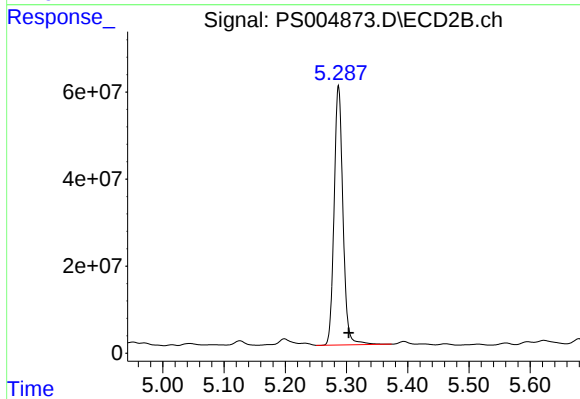

#4 2,4-DCAA


R.T.: 5.287 min
Delta R.T.: -0.017 min
Response: 596038519
Conc: 617.76 ng/ml

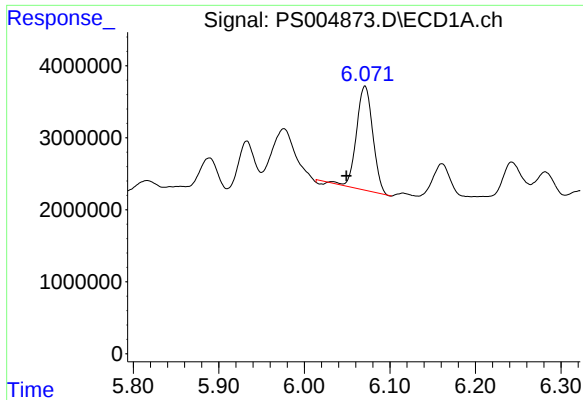

#7 MCPA


R.T.: 6.071 min
Delta R.T.: 0.022 min
Response: 19321119
Conc: 3.34 ug/ml

Instrument :
ECD_S
ClientSampleId :

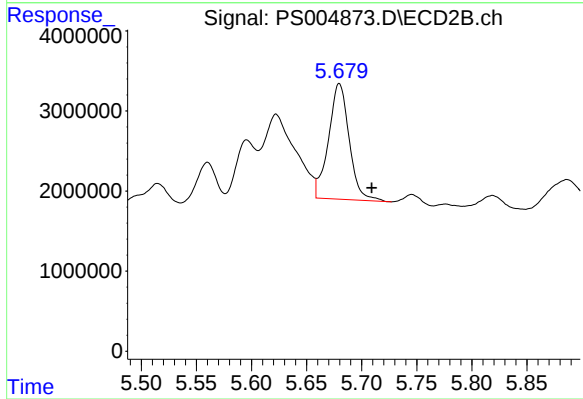


#7 MCPA

R.T.: 5.680 min
Delta R.T.: -0.029 min
Response: 18880248
Conc: 4.61 ug/ml

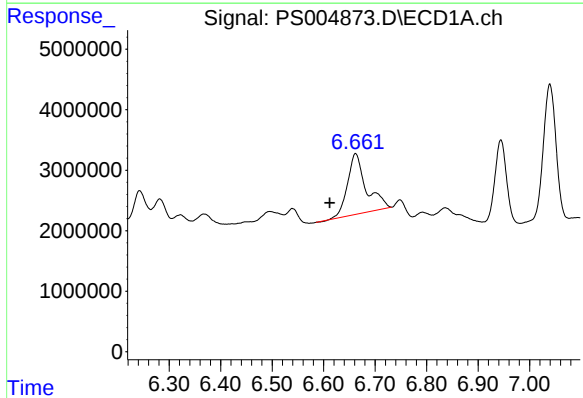


#9 2,4-D

R.T.: 6.662 min
Delta R.T.: 0.050 min
Response: 25134835
Conc: 18.37 ng/ml

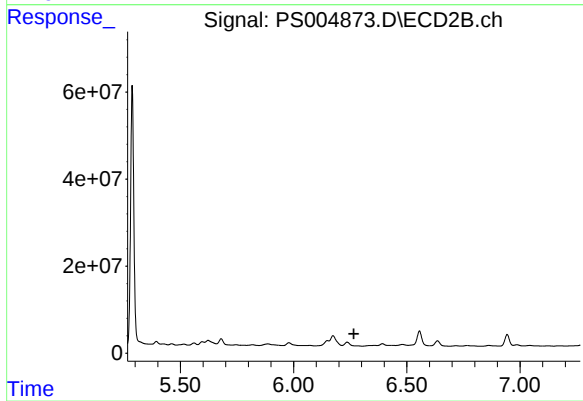

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

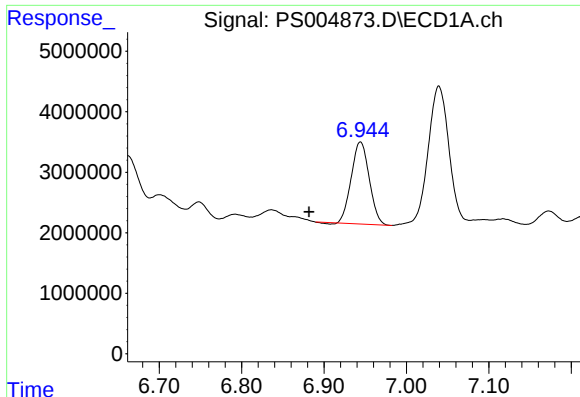

#10 Pentachlorophenol


R.T.: 6.944 min
Delta R.T.: 0.062 min
Response: 20597487
Conc: 1.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

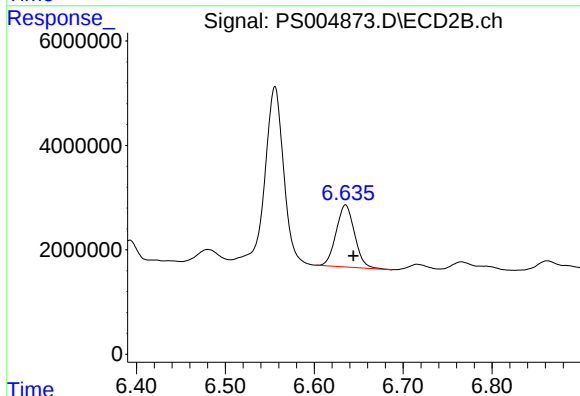


#10 Pentachlorophenol

R.T.: 6.635 min
Delta R.T.: -0.009 min
Response: 17154740
Conc: 1.40 ng/ml

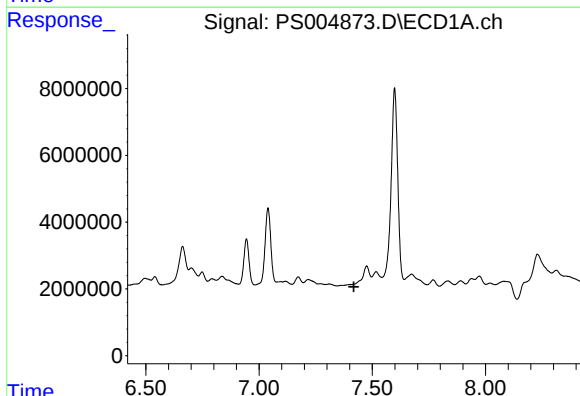


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

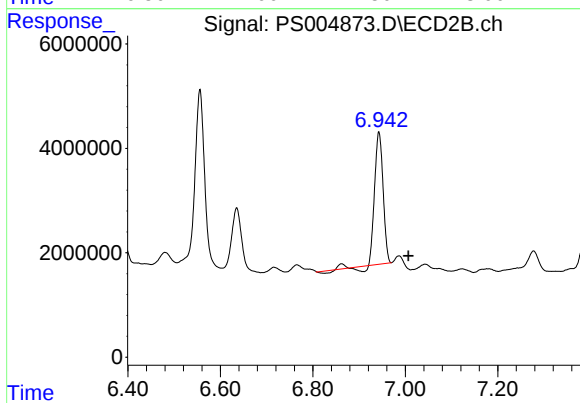

#11 2,4,5-TP (SILVEX)


R.T.: 6.943 min
Delta R.T.: -0.063 min
Response: 31413915
Conc: 6.11 ng/ml

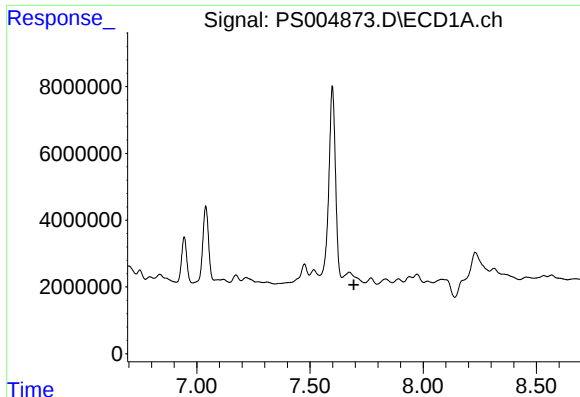

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

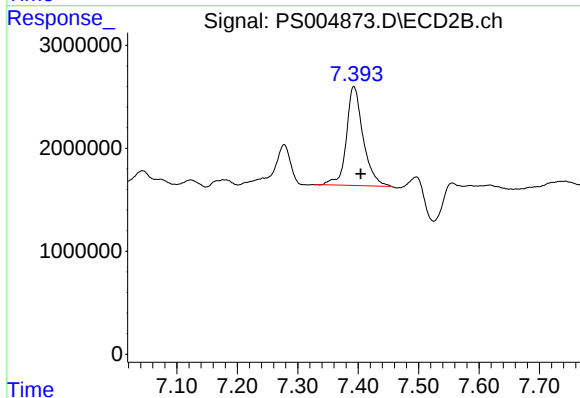


#12 2,4,5-T

R.T.: 7.393 min
Delta R.T.: -0.011 min
Response: 18473438
Conc: 4.15 ng/ml

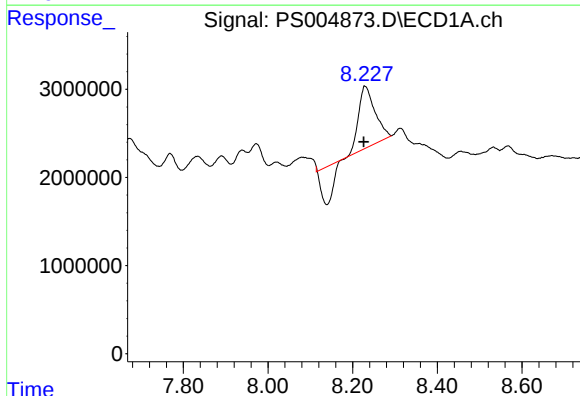


#13 2,4-DB

R.T.: 8.230 min
Delta R.T.: 0.003 min
Response: 12116863
Conc: 12.54 ng/ml

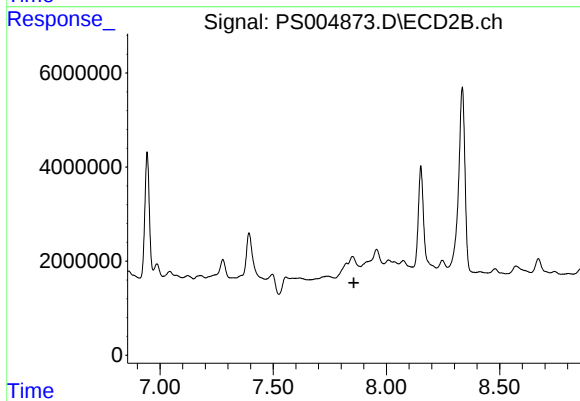

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 7.856 min
Response: 0
Conc: N.D.

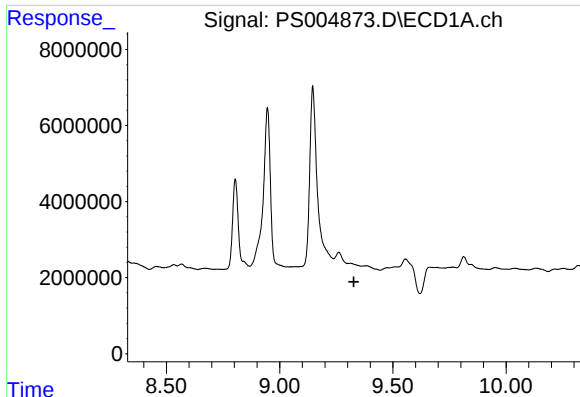

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

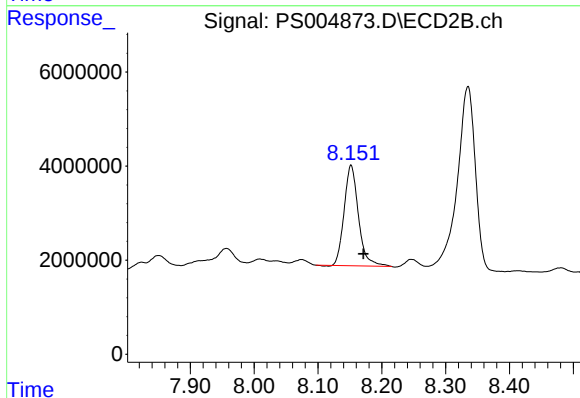


#14 DINOSEB

R.T.: 8.152 min
Delta R.T.: -0.019 min
Response: 33321343
Conc: 8.67 ng/ml

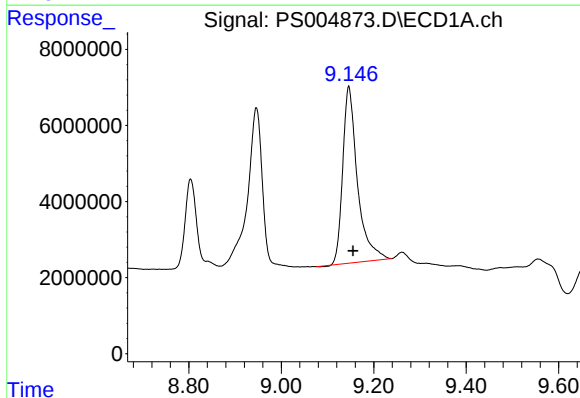


#15 Picloram

R.T.: 9.146 min
Delta R.T.: -0.009 min
Response: 102686464
Conc: 9.85 ng/ml

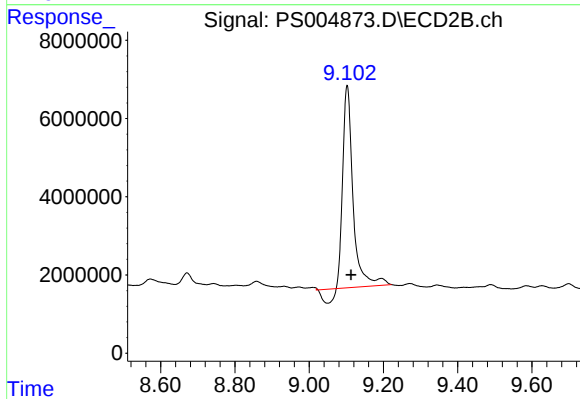

#15 Picloram


R.T.: 9.102 min
Delta R.T.: -0.010 min
Response: 94687537
Conc: 12.69 ng/ml

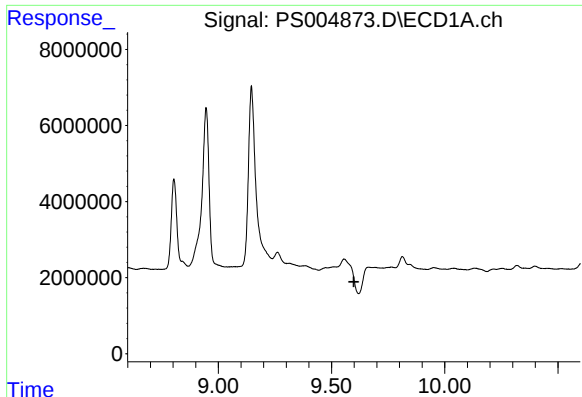

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

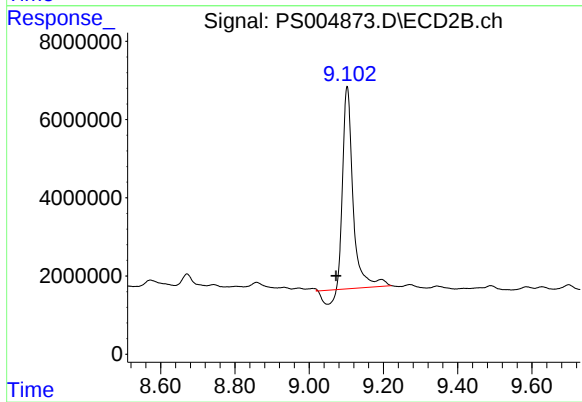

#16 DCPA

R.T.: 9.102 min
Delta R.T.: 0.030 min
Response: 94687537
Conc: 14.62 ng/ml