

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
 Data File : PS004876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2019 10:44
 Operator : SM\AJ
 Sample : K2639-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 05:26:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.574	5.285	526.2E6	392.0E6	375.369	406.296
Target Compounds							
1) T	Dalapon	2.075	0.000	40680267	0	24.540	N.D. #
2) T	3,5-DICHL...	0.000	4.603	0	252.0E6	N.D.	204.557
5) T	DICAMBA	0.000	5.390	0	17692488	N.D.	4.789
6) T	MCP	5.929	0.000	6105561	0	1.467	N.D. #
7) T	MCPA	0.000	5.741	0	370.9E6	N.D.	90.637
8) T	DICHLORPROP	0.000	5.974	0	18863772	N.D.	20.008
9) T	2,4-D	6.659	0.000	26746456	0	19.553	N.D. #
10) T	Pentachlo...	6.940	0.000	13650591	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	6.940	0	160.6E6	N.D.	31.220



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
Data File : PS004876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2019 10:44
Operator : SM\AJ
Sample : K2639-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 05:26:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

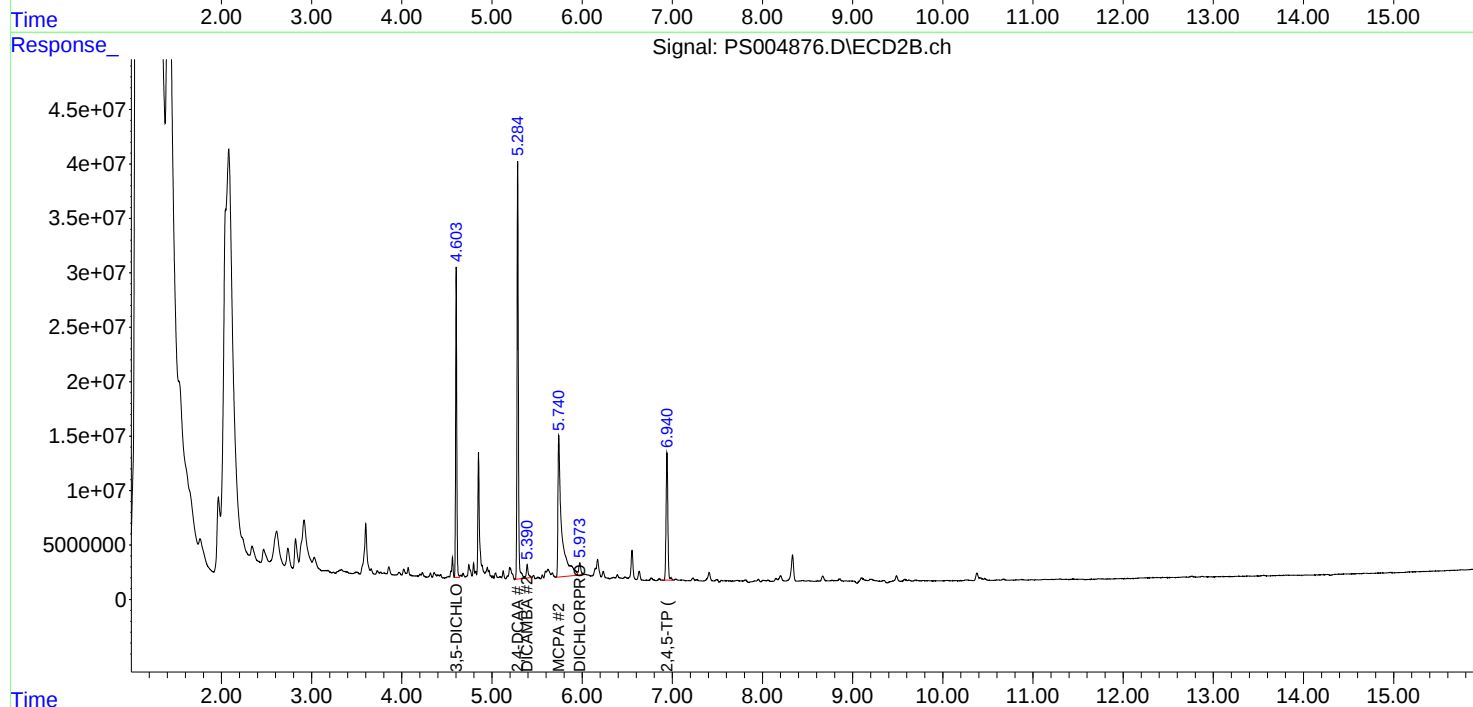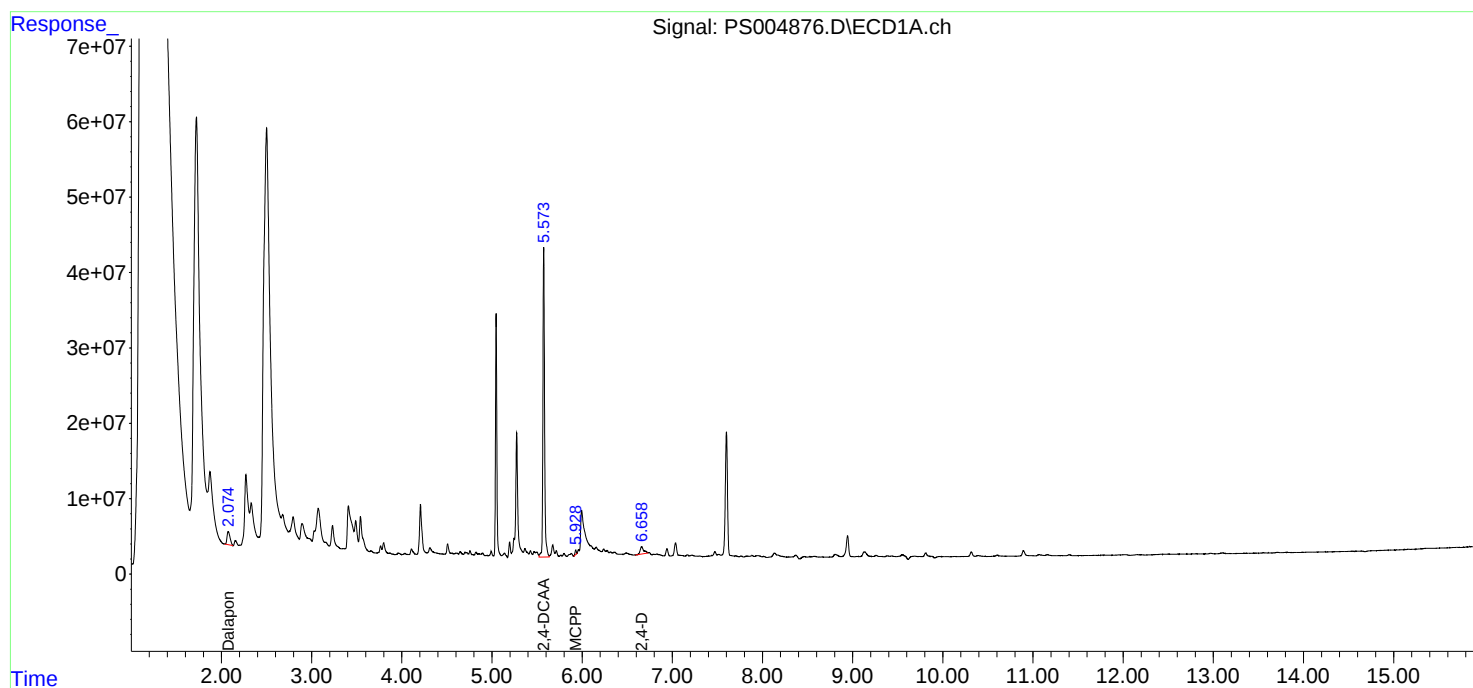


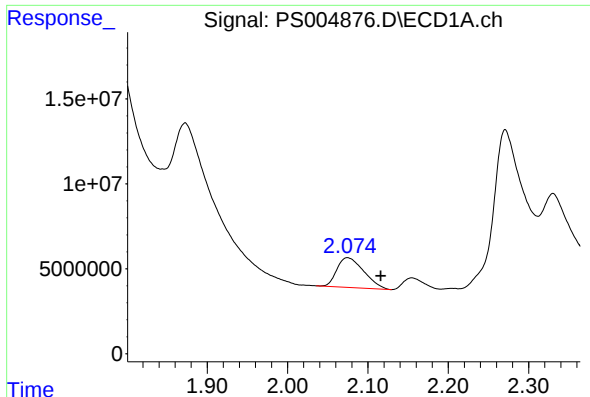

#1 Dalapon


R.T.: 2.075 min
Delta R.T.: -0.041 min
Response: 40680267
Conc: 24.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

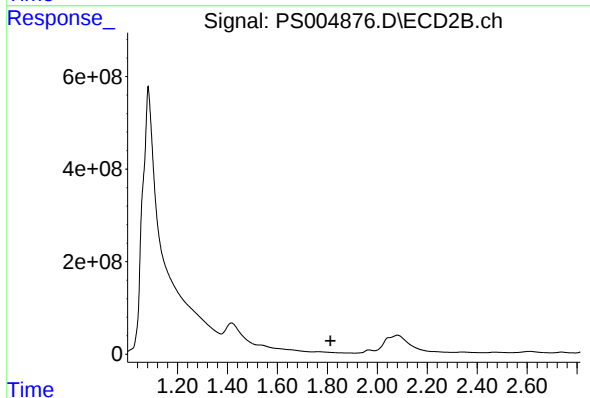


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

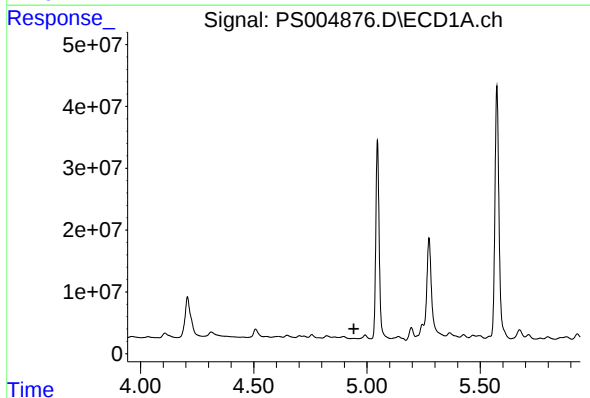


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

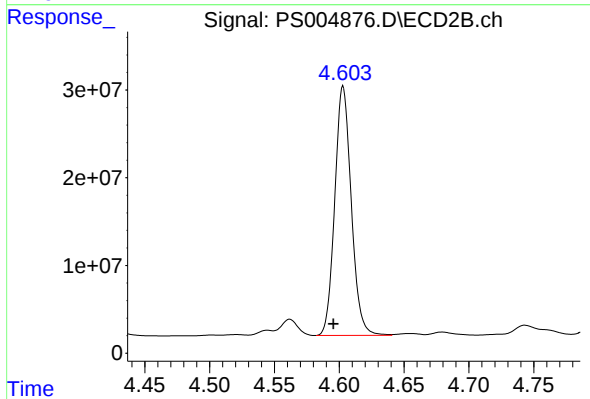

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.603 min
Delta R.T.: 0.008 min
Response: 252040801
Conc: 204.56 ng/ml

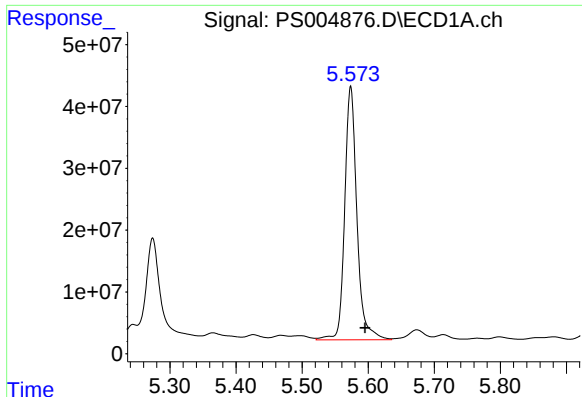

#4 2,4-DCAA


R.T.: 5.574 min
Delta R.T.: -0.022 min
Response: 526175996
Conc: 375.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

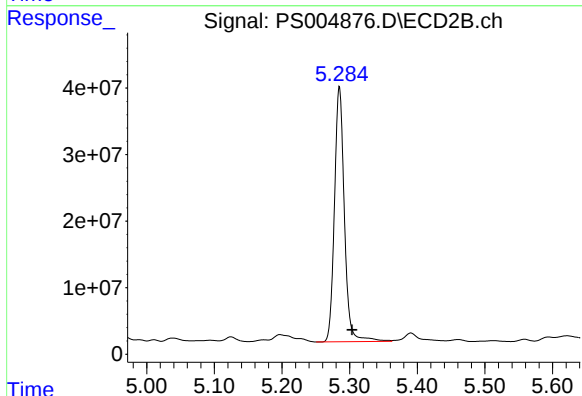


#4 2,4-DCAA

R.T.: 5.285 min
Delta R.T.: -0.019 min
Response: 392008718
Conc: 406.30 ng/ml

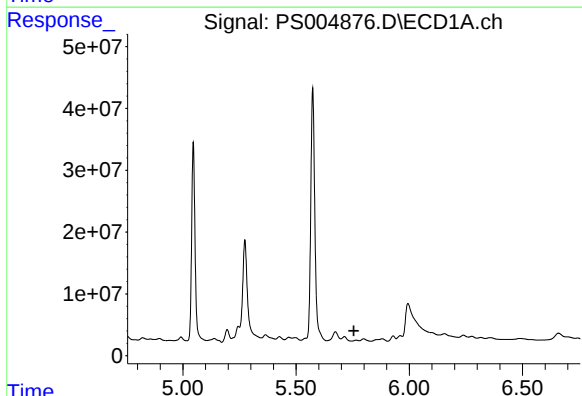


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.755 min
Response: 0
Conc: N.D.

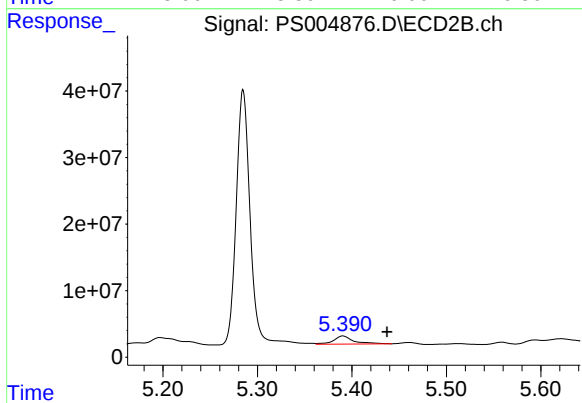

#5 DICAMBA


R.T.: 5.390 min
Delta R.T.: -0.047 min
Response: 17692488
Conc: 4.79 ng/ml

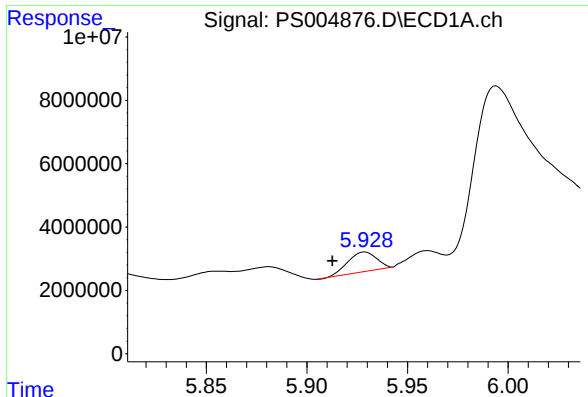

#6 MCPP


R.T.: 5.929 min
Delta R.T.: 0.016 min
Response: 6105561
Conc: 1.47 ug/ml

Instrument :
ECD_S
ClientSampleId :

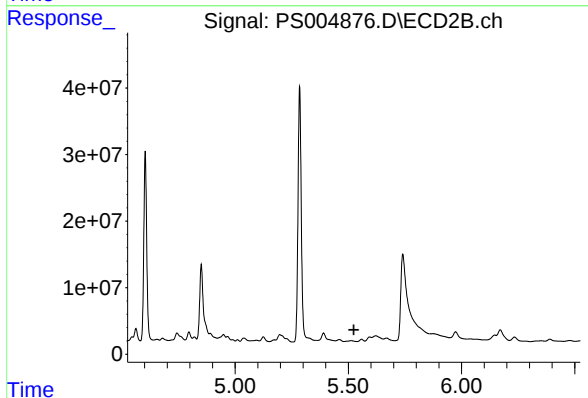


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

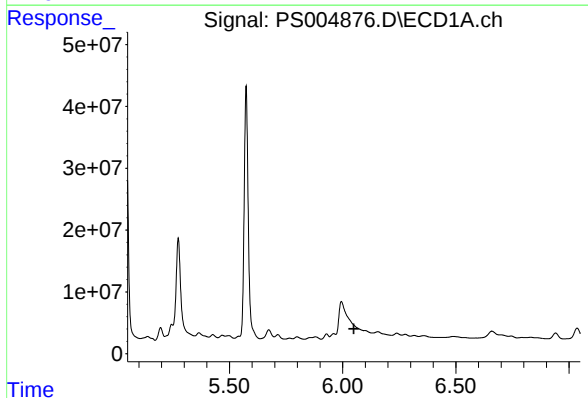


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

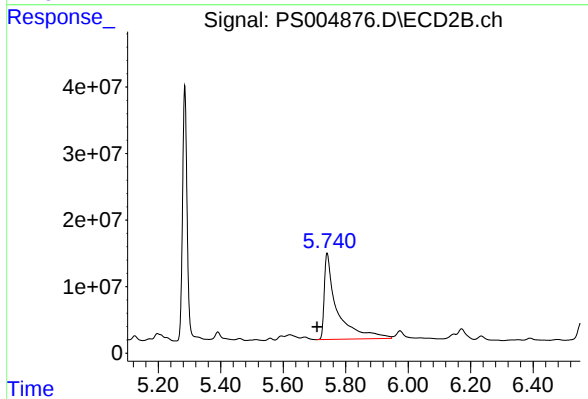

#7 MCPA


R.T.: 5.741 min
Delta R.T.: 0.032 min
Response: 370854588
Conc: 90.64 ug/ml

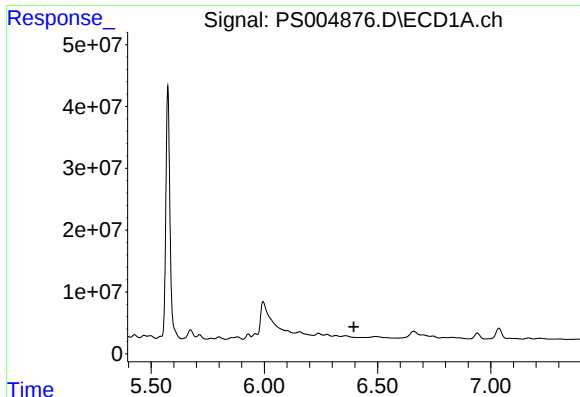

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

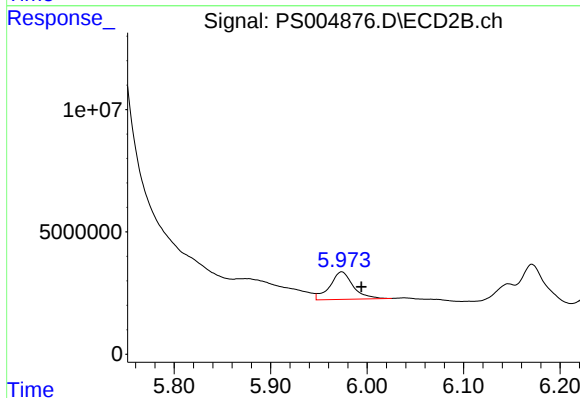


#8 DICHLORPROP

R.T.: 5.974 min
Delta R.T.: -0.021 min
Response: 18863772
Conc: 20.01 ng/ml

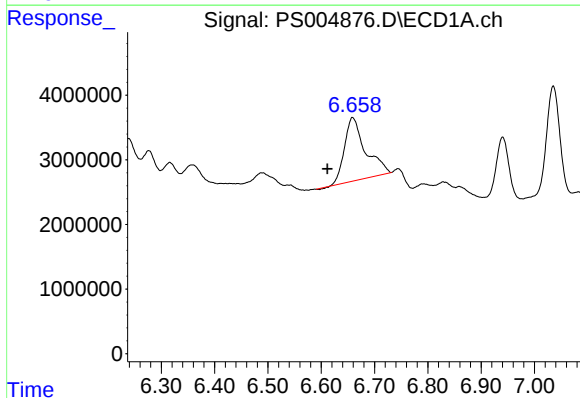


#9 2,4-D

R.T.: 6.659 min
Delta R.T.: 0.047 min
Response: 26746456
Conc: 19.55 ng/ml

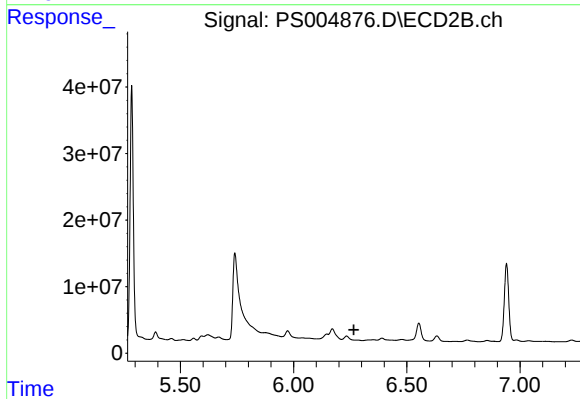

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

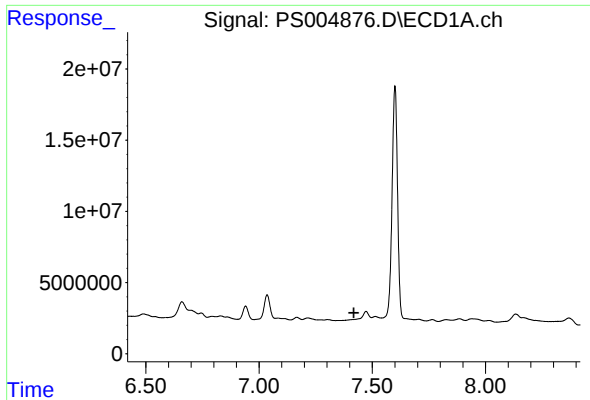

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

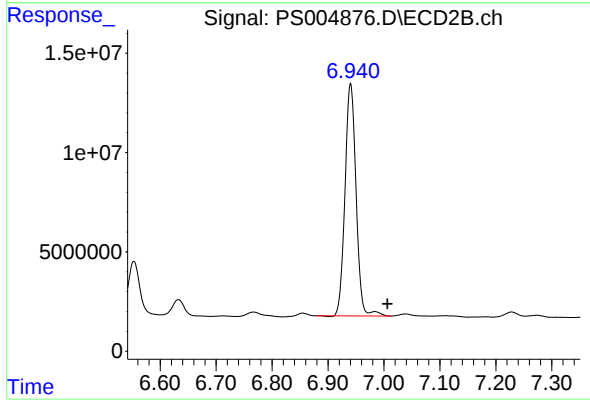

#11 2,4,5-TP (SILVEX)

R.T.: 6.940 min
Delta R.T.: -0.066 min
Response: 160638389
Conc: 31.22 ng/ml