

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
 Data File : PS004879.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2019 11:50
 Operator : SM\AJ
 Sample : K2639-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 05:27:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.574	5.285	545.6E6	378.0E6	389.260	391.744
Target Compounds							
1) T	Dalapon	2.075	0.000	44598753	0	26.904	N.D. #
2) T	3,5-DICHL...	0.000	4.604	0	241.2E6	N.D.	195.770
5) T	DICAMBA	0.000	5.392	0	12240767	N.D.	3.313
6) T	MCP	5.929	0.000	7681855	0	1.845	N.D. #
7) T	MCPA	5.993	5.741	-8177093	437.3E6	N.D.	106.888
8) T	DICHLORPROP	0.000	5.974	0	17240260	N.D.	18.286
9) T	2,4-D	6.679	6.274	67590523	19797355	49.412	18.316 #
10) T	Pentachlo...	6.941	0.000	14415209	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	6.942	0	242.8E6	N.D.	47.186



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
Data File : PS004879.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2019 11:50
Operator : SM\AJ
Sample : K2639-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 05:27:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

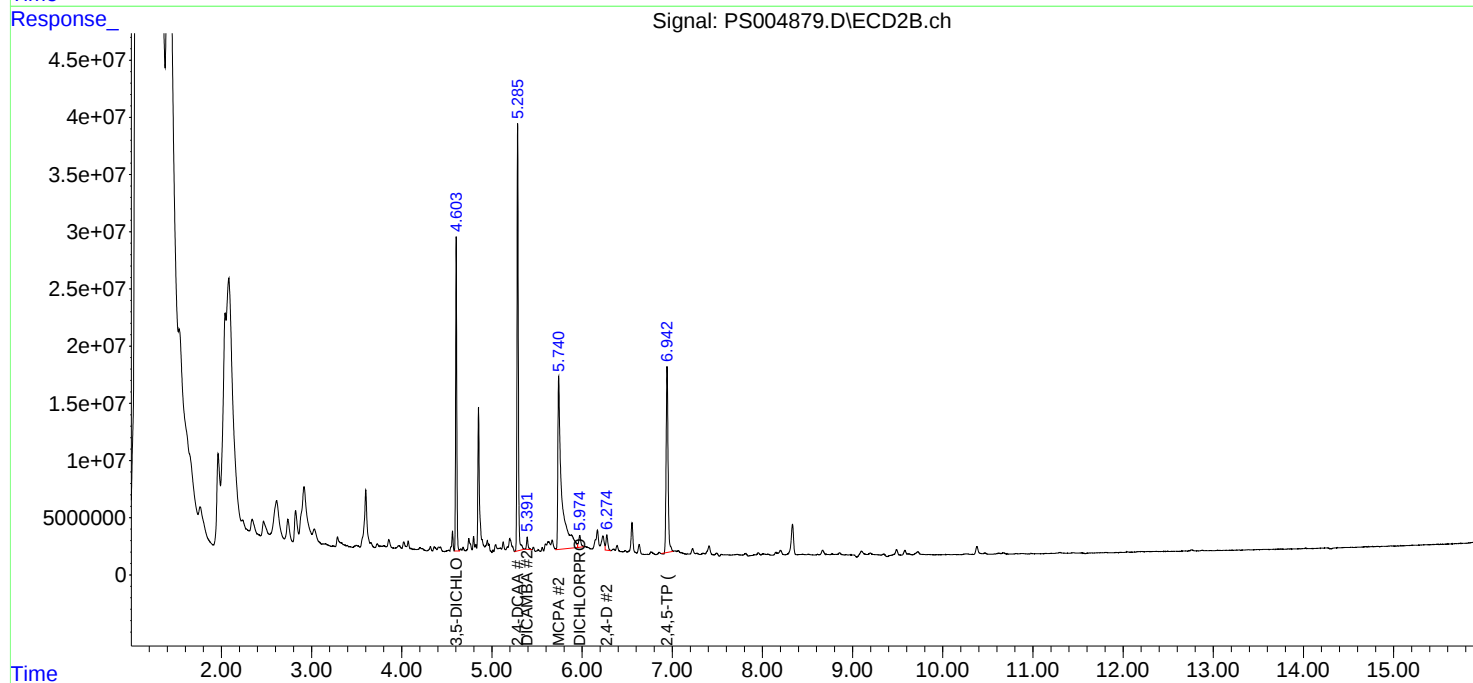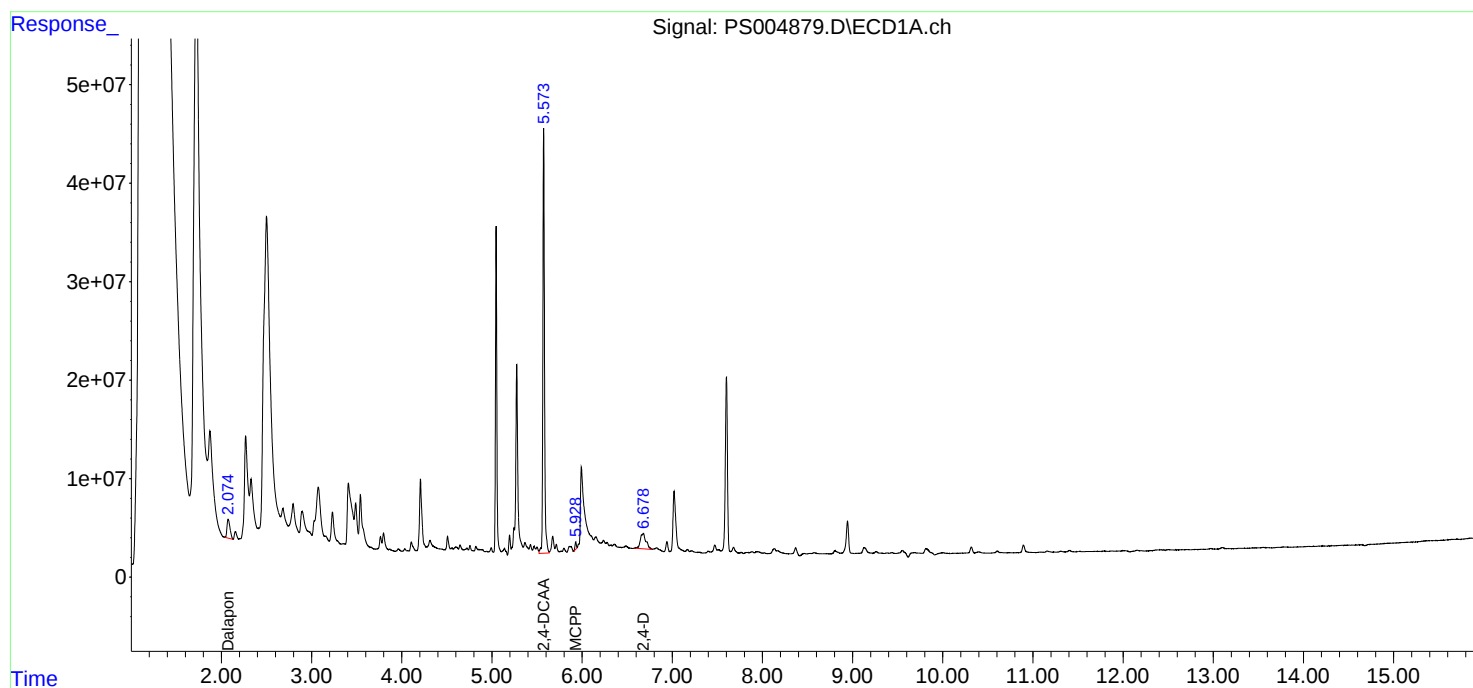


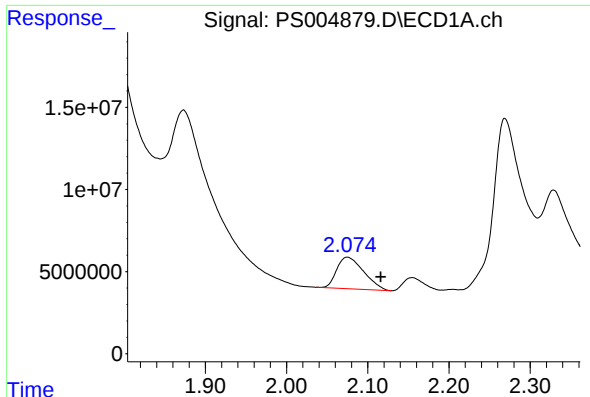

#1 Dalapon


R.T.: 2.075 min
Delta R.T.: -0.041 min
Response: 44598753
Conc: 26.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

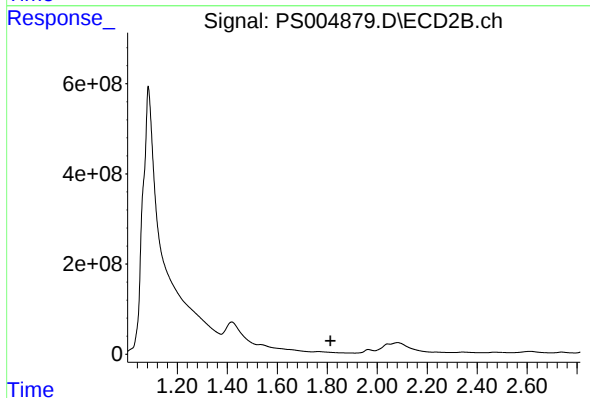


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

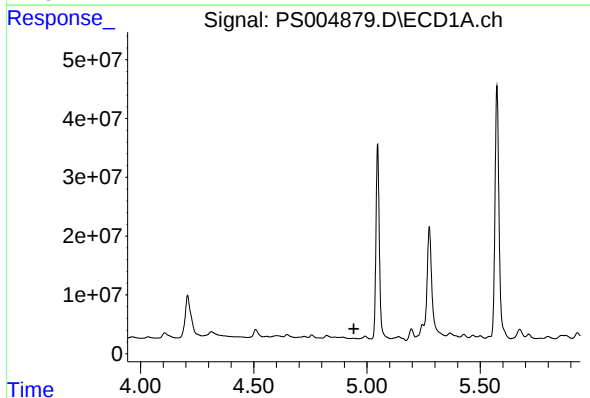


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

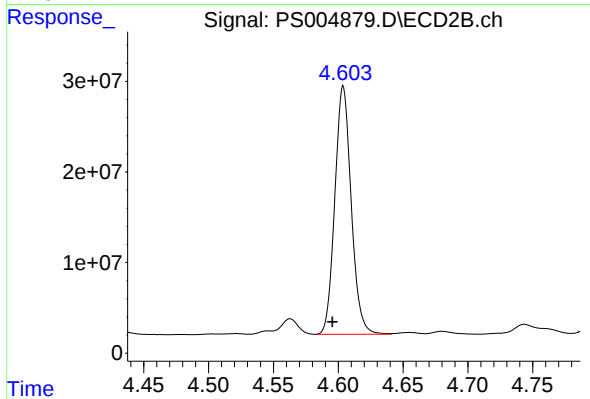

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.604 min
Delta R.T.: 0.008 min
Response: 241213939
Conc: 195.77 ng/ml

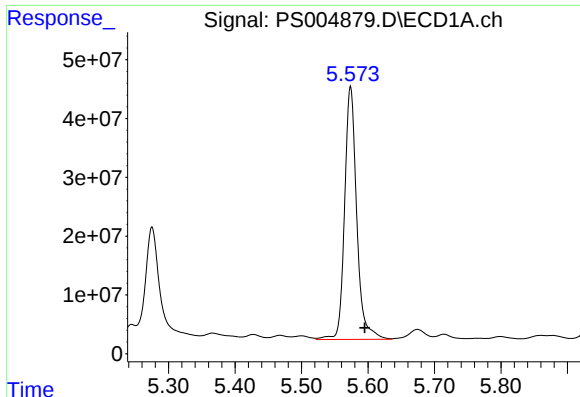

#4 2,4-DCAA


R.T.: 5.574 min
Delta R.T.: -0.021 min
Response: 545647532
Conc: 389.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

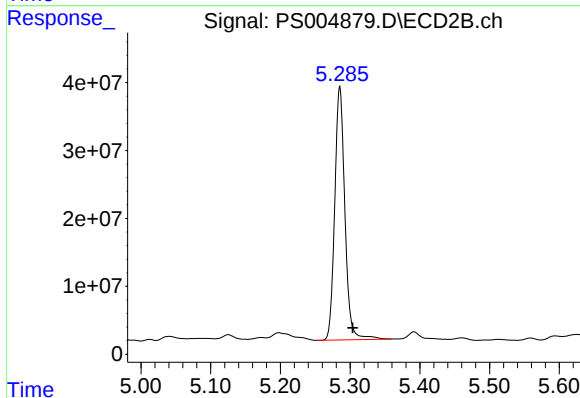


#4 2,4-DCAA

R.T.: 5.285 min
Delta R.T.: -0.018 min
Response: 377968505
Conc: 391.74 ng/ml

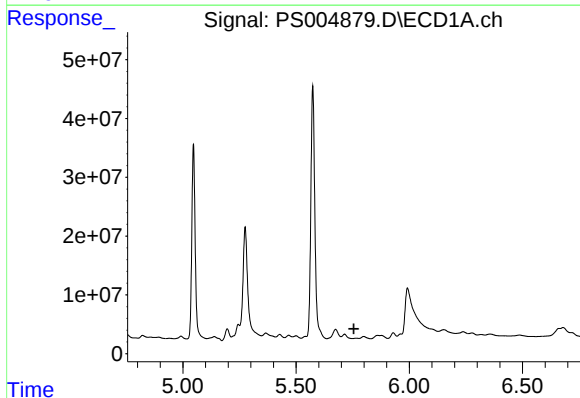


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.755 min
Response: 0
Conc: N.D.

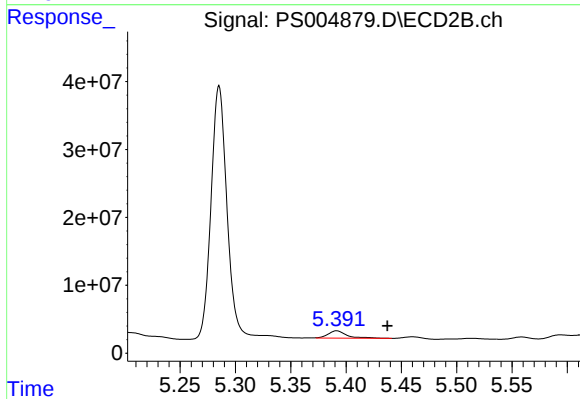

#5 DICAMBA


R.T.: 5.392 min
Delta R.T.: -0.046 min
Response: 12240767
Conc: 3.31 ng/ml

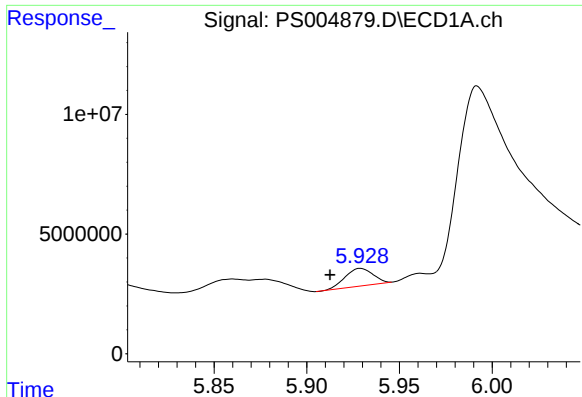

#6 MCPP


R.T.: 5.929 min
Delta R.T.: 0.017 min
Response: 7681855
Conc: 1.85 ug/ml

Instrument :
ECD_S
ClientSampleId :

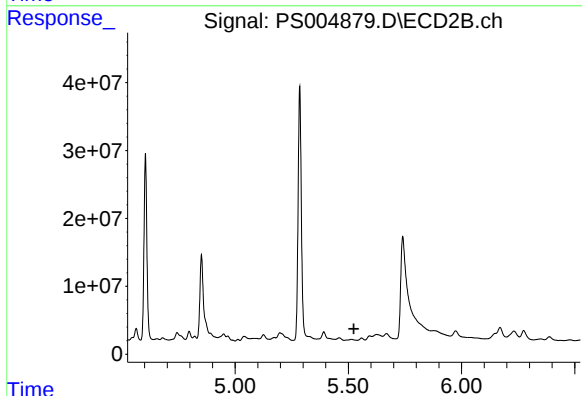


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

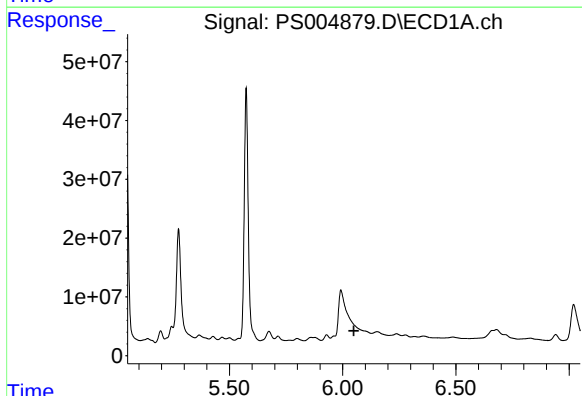


#7 MCPA

R.T.: 5.993 min
Delta R.T.: -0.057 min
Response: -8177093
Conc: N.D.

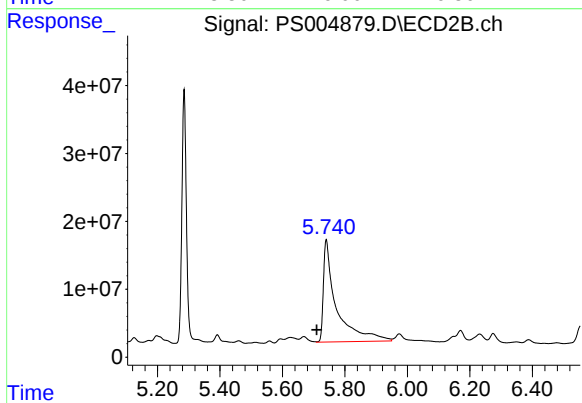

#7 MCPA


R.T.: 5.741 min
Delta R.T.: 0.031 min
Response: 437348183
Conc: 106.89 ug/ml

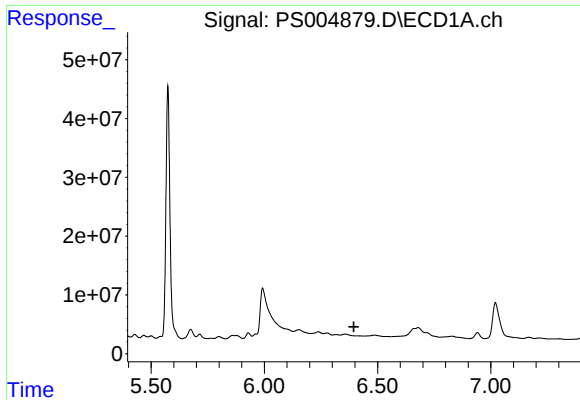

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

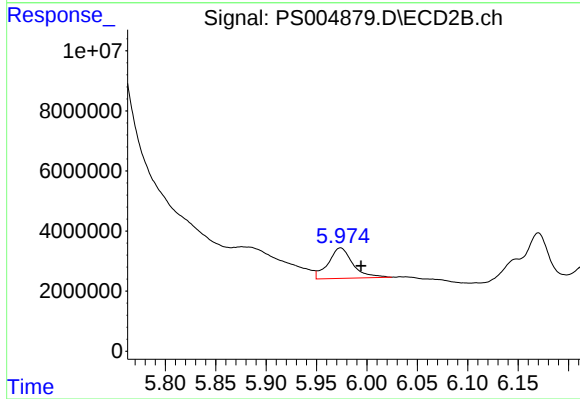


#8 DICHLORPROP

R.T.: 5.974 min
Delta R.T.: -0.020 min
Response: 17240260
Conc: 18.29 ng/ml

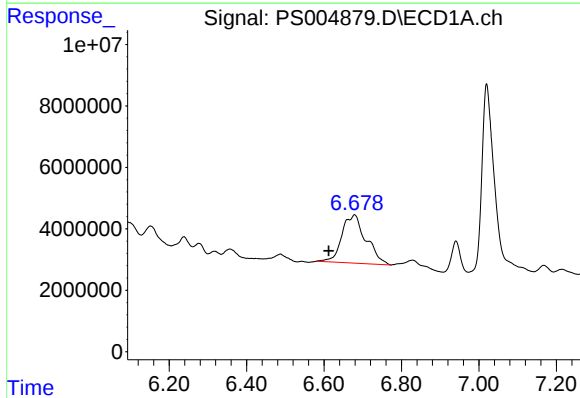


#9 2,4-D

R.T.: 6.679 min
Delta R.T.: 0.067 min
Response: 67590523
Conc: 49.41 ng/ml

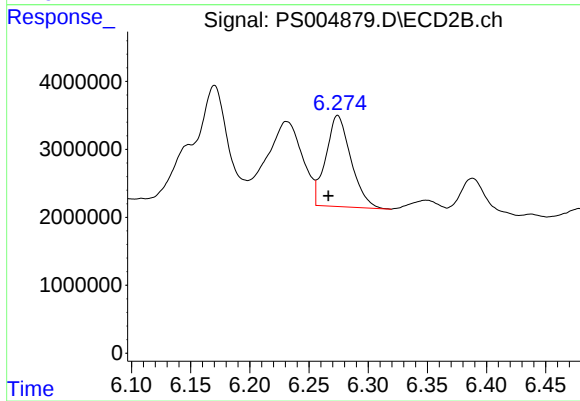

#9 2,4-D


R.T.: 6.274 min
Delta R.T.: 0.008 min
Response: 19797355
Conc: 18.32 ng/ml

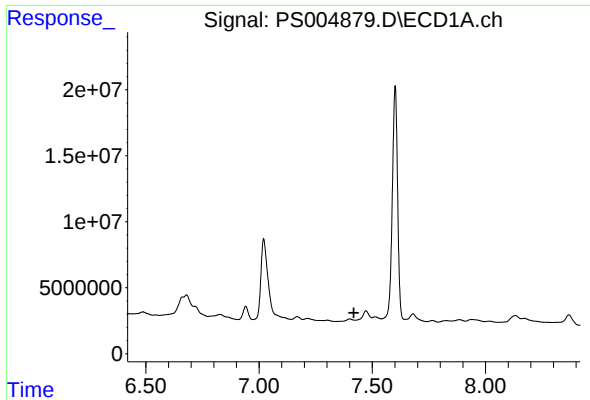

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

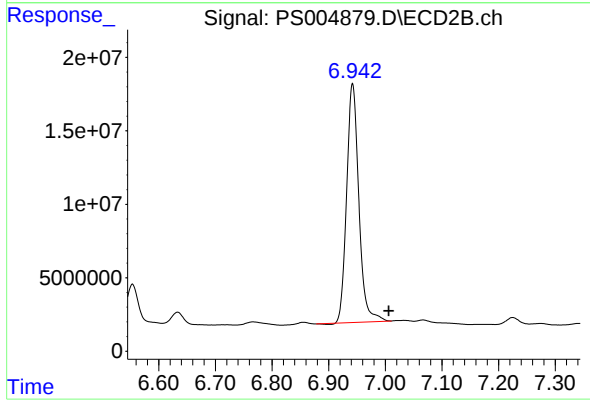

#11 2,4,5-TP (SILVEX)

R.T.: 6.942 min
Delta R.T.: -0.064 min
Response: 242789579
Conc: 47.19 ng/ml