

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
 Data File : PS004883.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2019 13:18
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 05:28:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.592	5.286	646.7E6	476.9E6	461.333	494.323
Target Compounds							
2) T	3,5-DICHL...	4.958	0.000	28303257	0	16.412	N.D. #
5) T	DICAMBA	0.000	5.442	0	32699787	N.D.	8.852
7) T	MCPA	5.985	0.000	1242554	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	5.979	0	20960078	N.D.	22.231
9) T	2,4-D	6.633	0.000	75674119	0	55.321	N.D. #
15) T	Picloram	9.129	0.000	657.6E6	0	63.106	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
Data File : PS004883.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2019 13:18
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 05:28:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

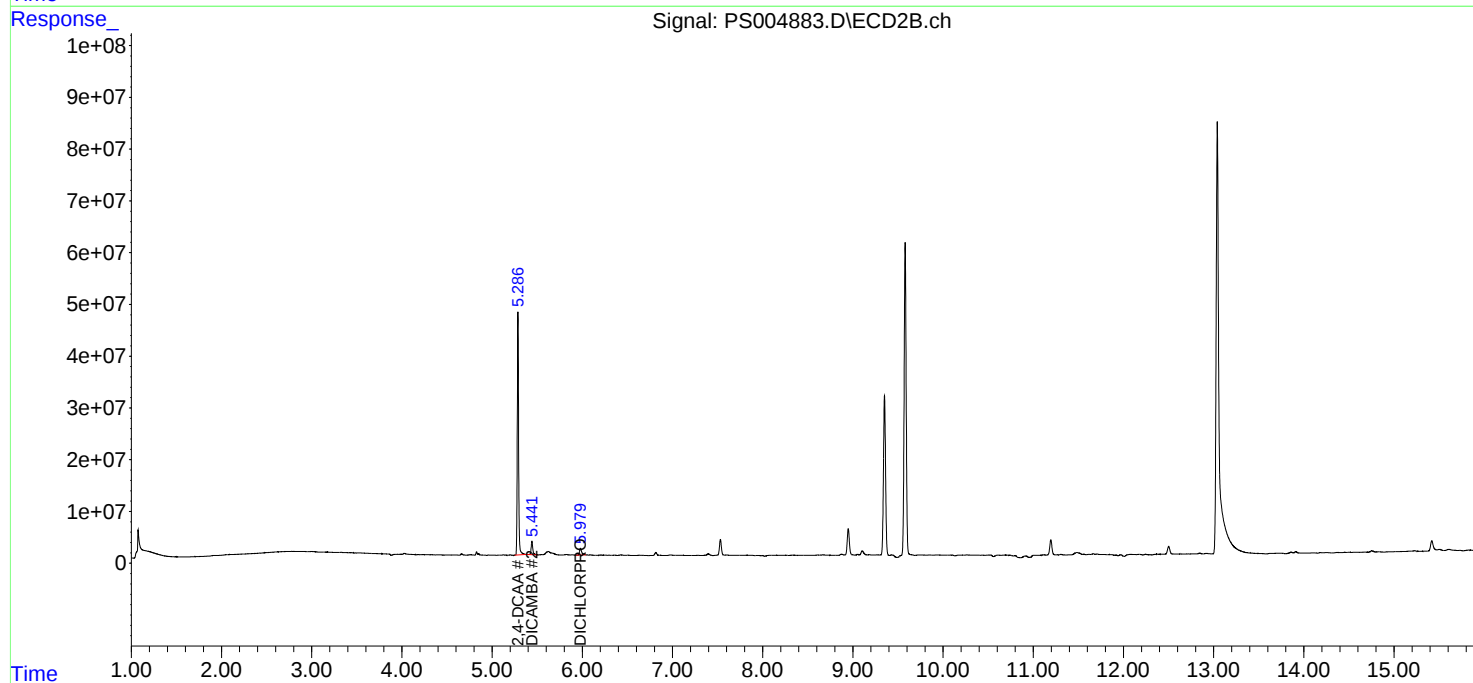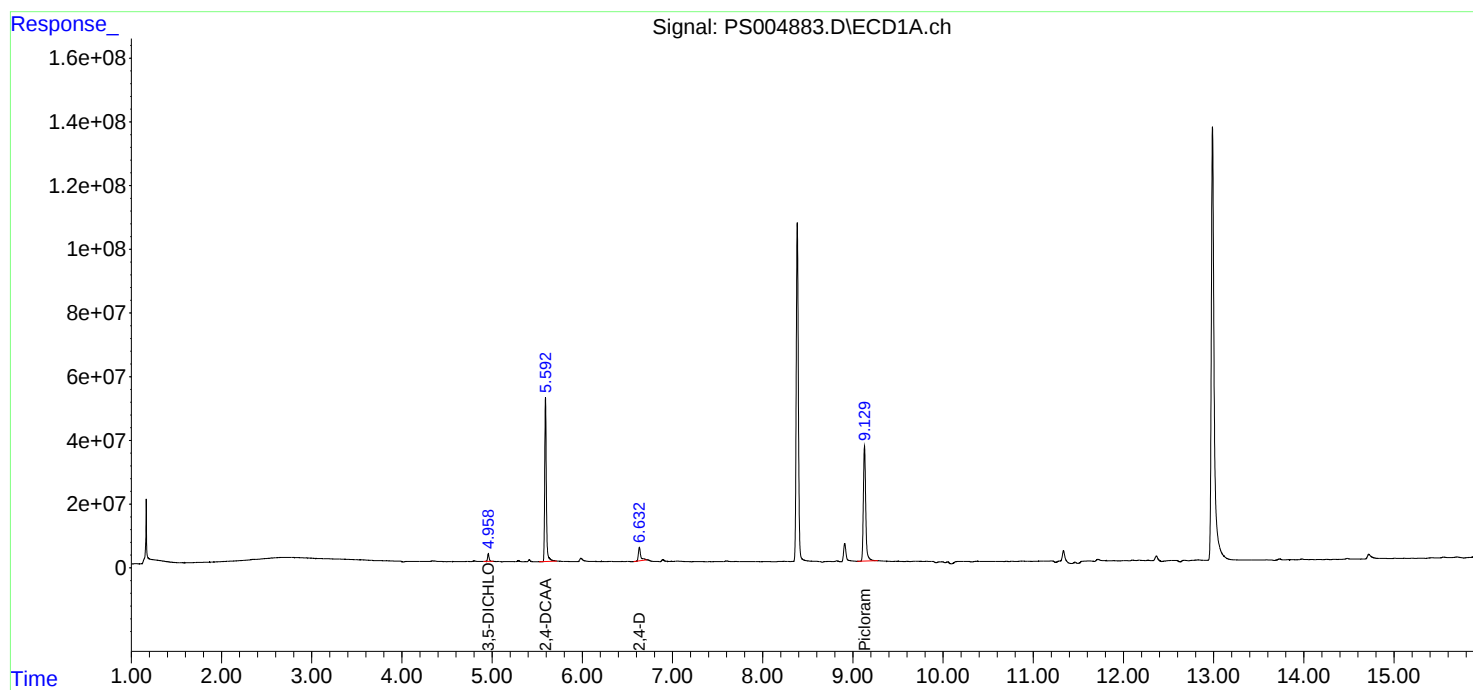


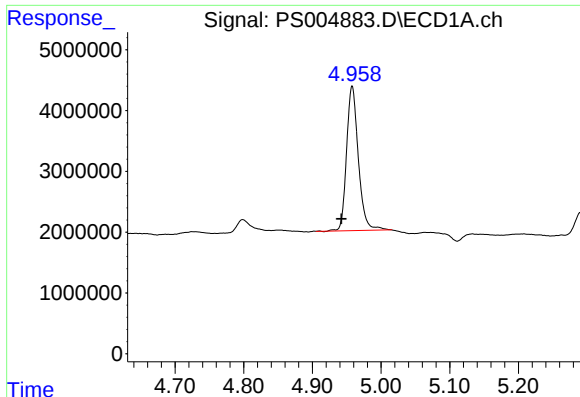

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.958 min
Delta R.T.: 0.016 min
Response: 28303257
Conc: 16.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

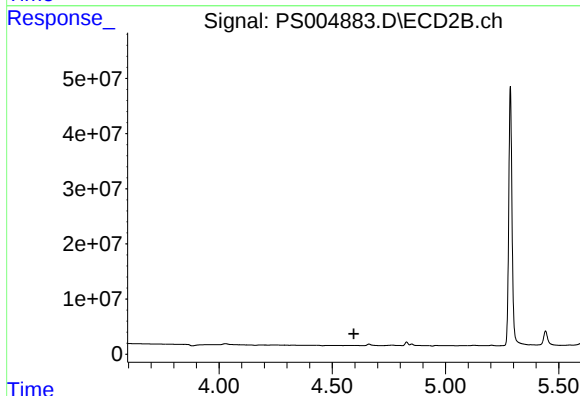


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

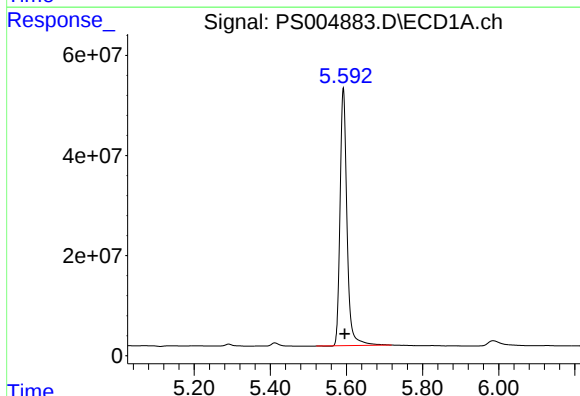


#4 2,4-DCAA

R.T.: 5.592 min
Delta R.T.: -0.003 min
Response: 646676695
Conc: 461.33 ng/ml

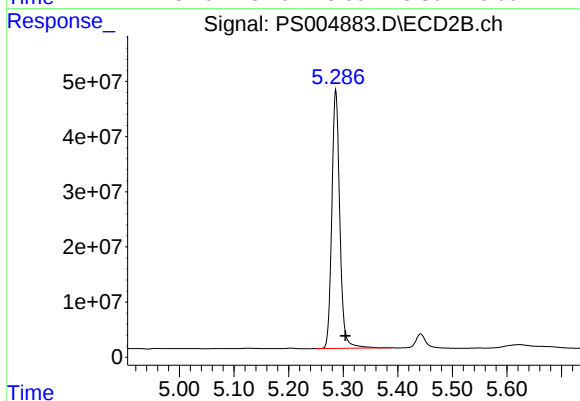

#4 2,4-DCAA


R.T.: 5.286 min
Delta R.T.: -0.017 min
Response: 476940144
Conc: 494.32 ng/ml

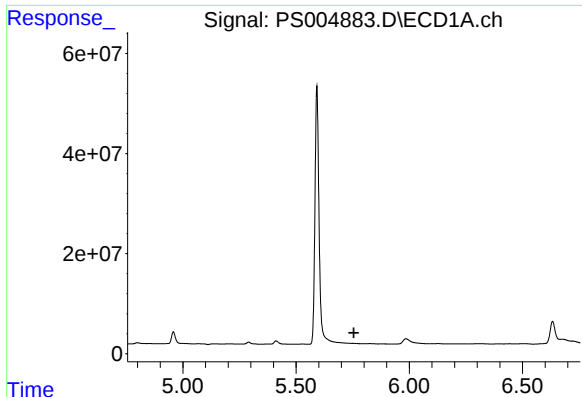

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

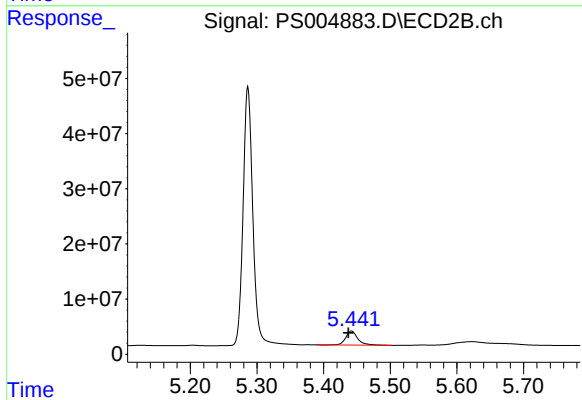


#5 DICAMBA

R.T.: 5.442 min
Delta R.T.: 0.005 min
Response: 32699787
Conc: 8.85 ng/ml

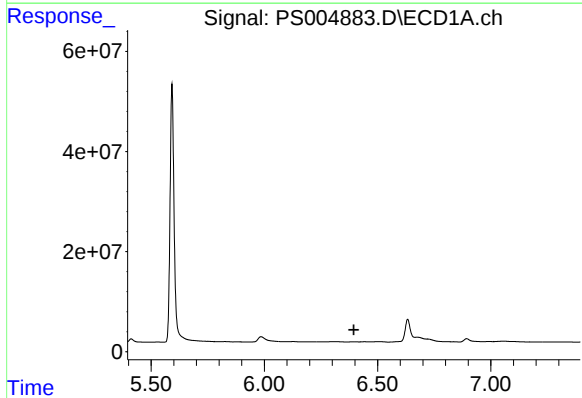


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

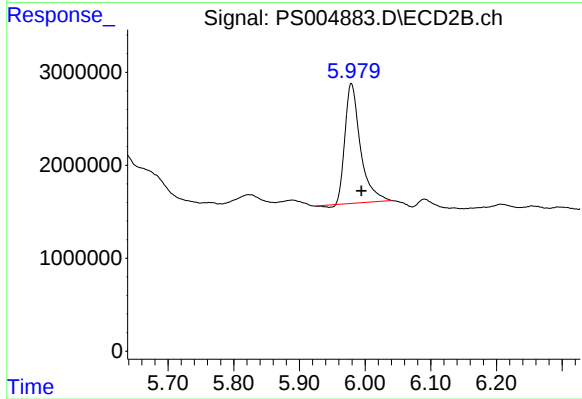

#8 DICHLORPROP


R.T.: 5.979 min
Delta R.T.: -0.015 min
Response: 20960078
Conc: 22.23 ng/ml

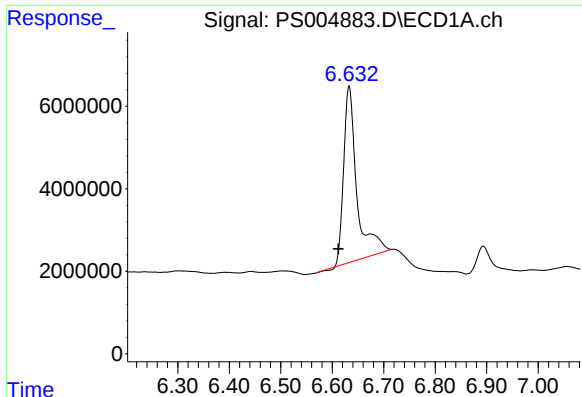

#9 2,4-D


R.T.: 6.633 min
Delta R.T.: 0.021 min
Response: 75674119
Conc: 55.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

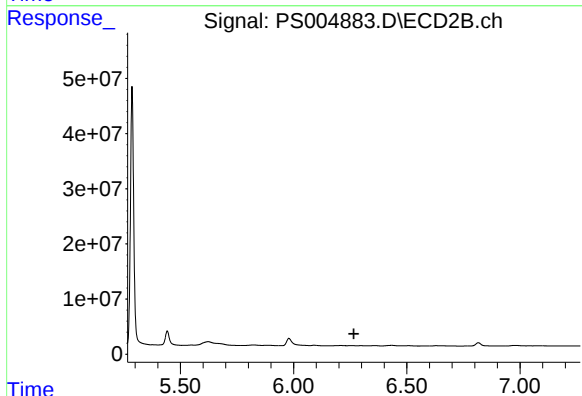


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

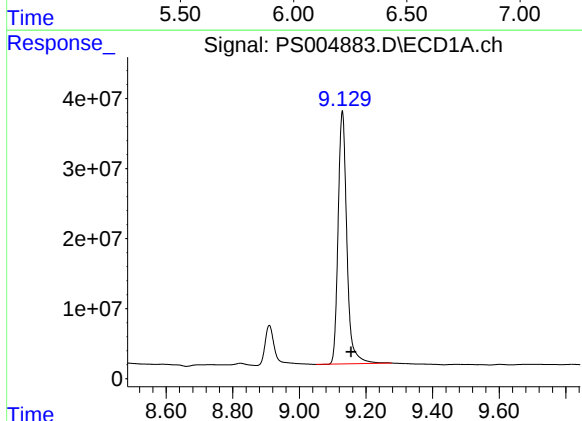

#15 Picloram

R.T.: 9.129 min
Delta R.T.: -0.026 min
Response: 657564889
Conc: 63.11 ng/ml

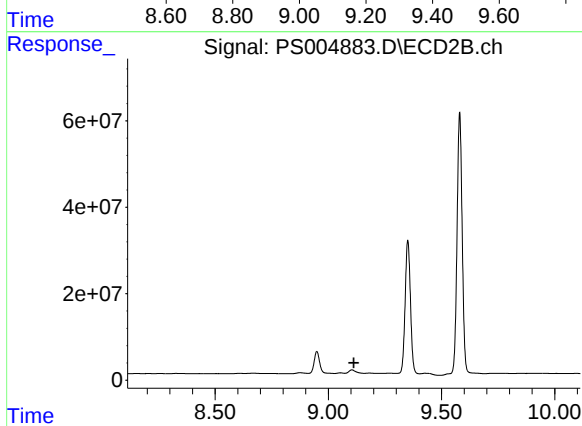

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.113 min
Response: 0
Conc: N.D.