

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
 Data File : PS004885.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2019 14:04
 Operator : SM\AJ
 Sample : K3105-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 05:39:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.577	5.287	528.5E6	376.5E6	377.045	390.208
Target Compounds							
1) T	Dalapon	2.078	0.000	45309592	0	27.333	N.D. #
2) T	3,5-DICHL...	0.000	4.605	0	203.3E6	N.D.	165.022
5) T	DICAMBA	0.000	5.392	0	18786226	N.D.	5.085
6) T	MCP	5.933	5.593	5659878	17258487	1.360	6.299 #
7) T	MCPA	0.000	5.743	0	337.9E6	N.D.	82.584
8) T	DICHLORPROP	0.000	5.975	0	24434806	N.D.	25.917
9) T	2,4-D	6.661	0.000	55146064	0	40.314	N.D. #
11) T	2,4,5-TP ...	0.000	6.942	0	126.5E6	N.D.	24.579
15) T	Picloram	9.146	9.101	58033440	42694657	5.569	5.723
16) T	DCPA	0.000	9.101	0	42694657	N.D.	6.591



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
Data File : PS004885.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2019 14:04
Operator : SM\AJ
Sample : K3105-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 05:39:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

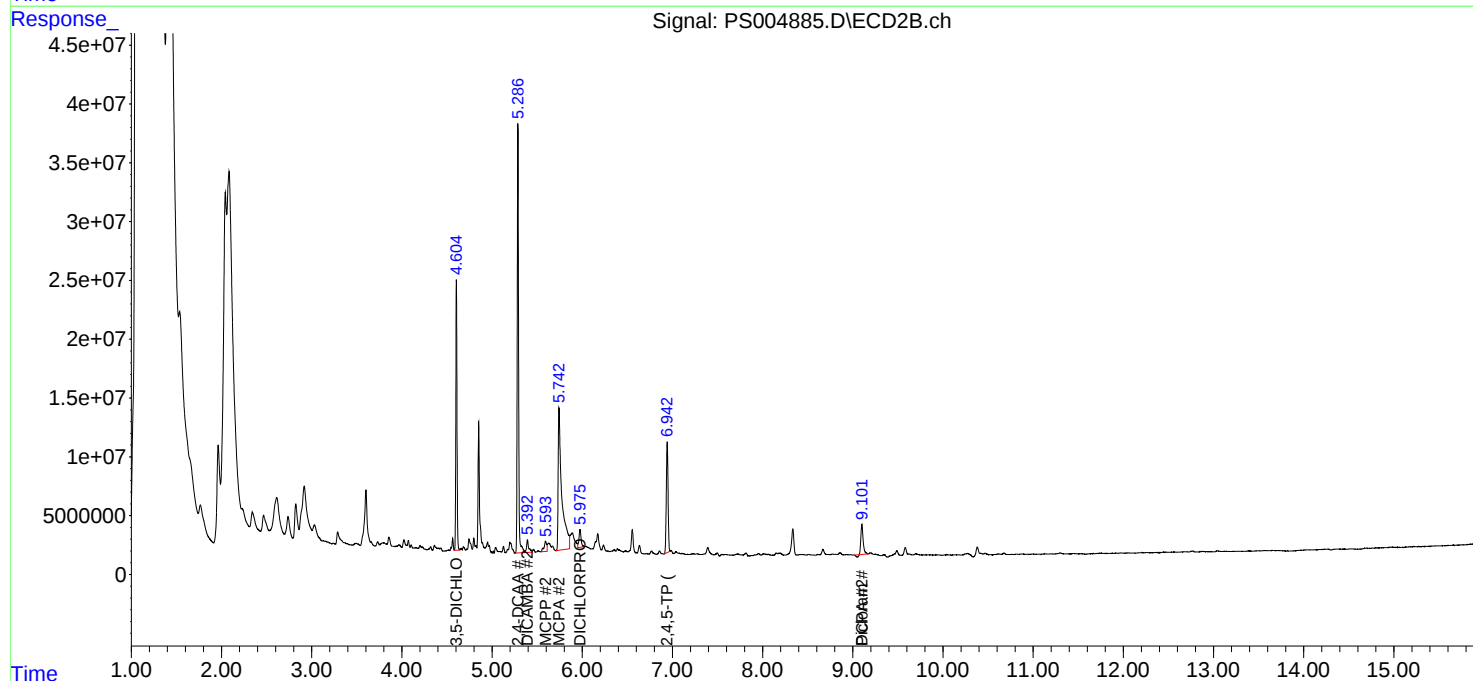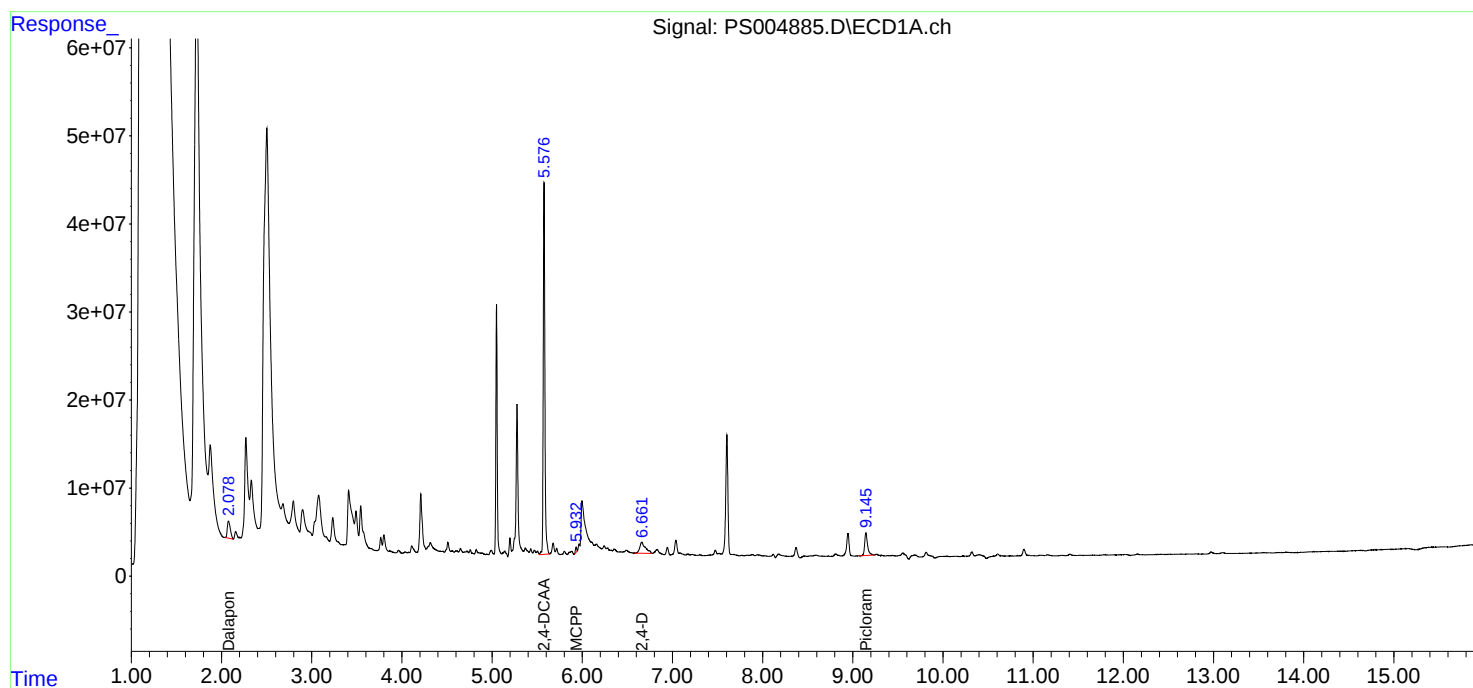


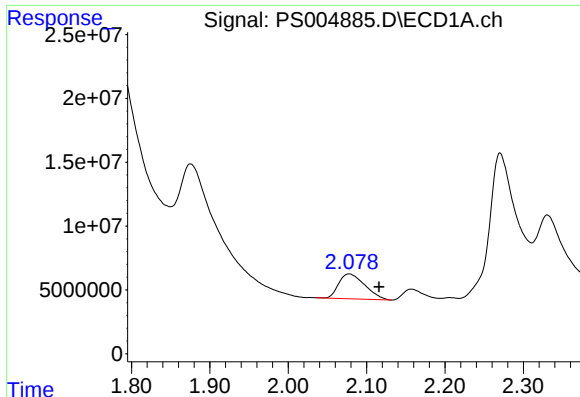

#1 Dalapon


R.T.: 2.078 min
Delta R.T.: -0.038 min
Response: 45309592
Conc: 27.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

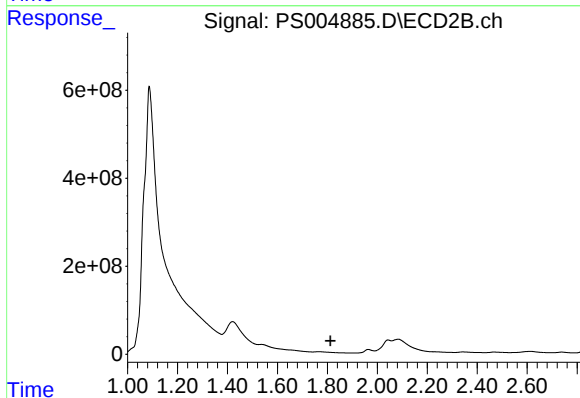


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

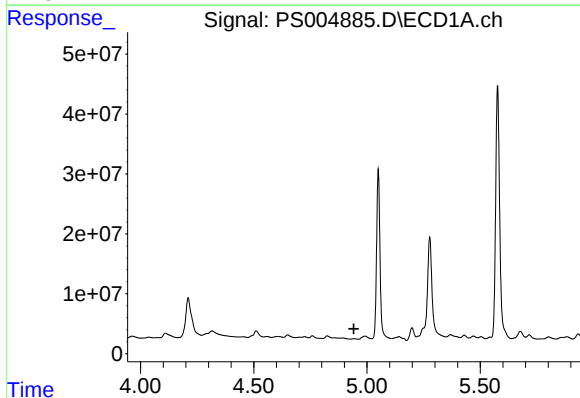


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

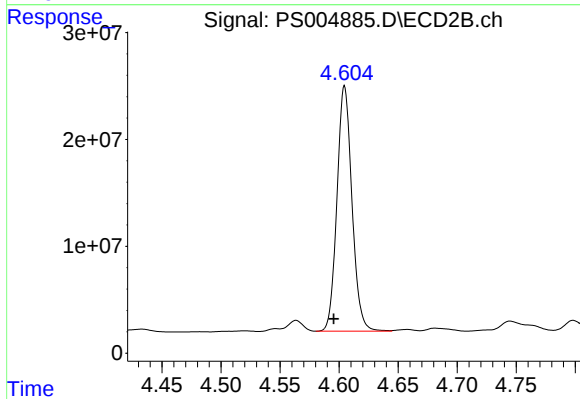

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.605 min
Delta R.T.: 0.009 min
Response: 203328083
Conc: 165.02 ng/ml

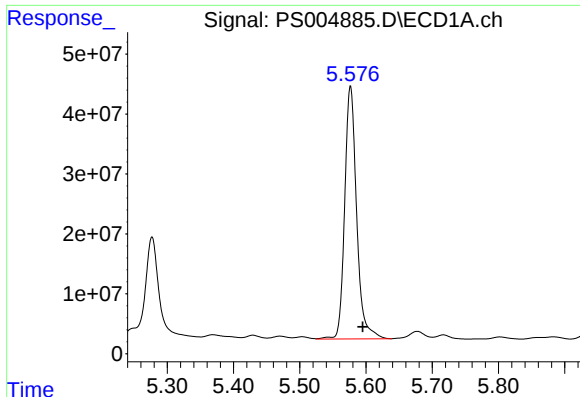

#4 2,4-DCAA


R.T.: 5.577 min
Delta R.T.: -0.019 min
Response: 528524863
Conc: 377.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

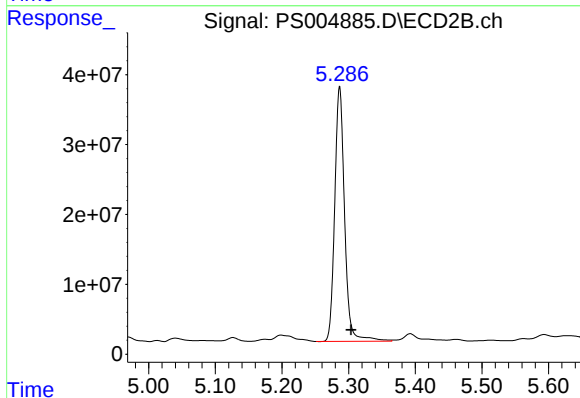


#4 2,4-DCAA

R.T.: 5.287 min
Delta R.T.: -0.017 min
Response: 376486850
Conc: 390.21 ng/ml

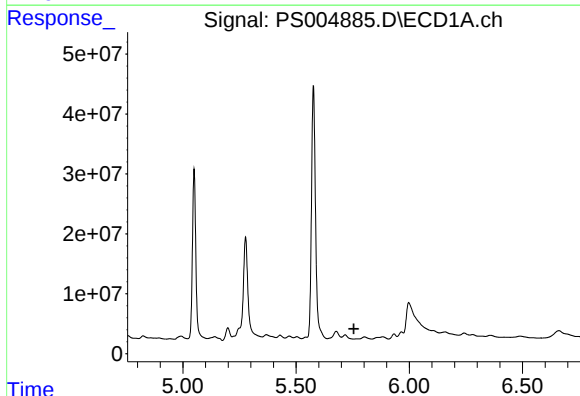


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.755 min
Response: 0
Conc: N.D.

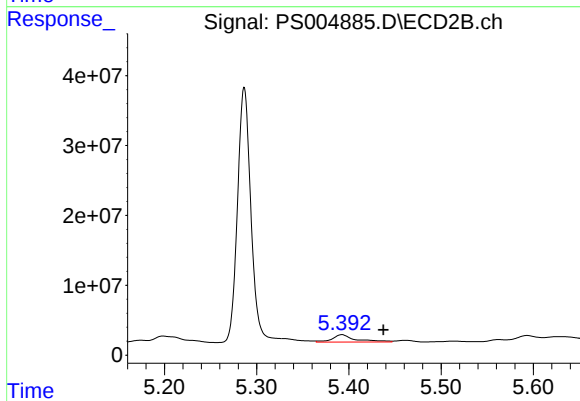

#5 DICAMBA


R.T.: 5.392 min
Delta R.T.: -0.045 min
Response: 18786226
Conc: 5.09 ng/ml

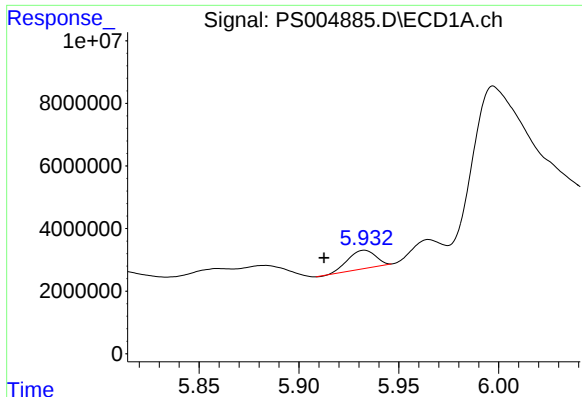

#6 MCPP


R.T.: 5.933 min
Delta R.T.: 0.020 min
Response: 5659878
Conc: 1.36 ug/ml

Instrument :
ECD_S
ClientSampleId :

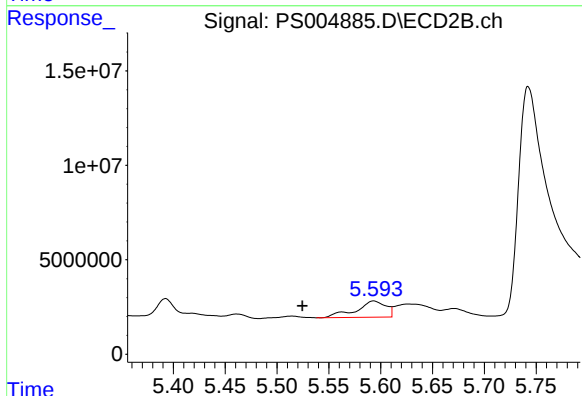


#6 MCPP

R.T.: 5.593 min
Delta R.T.: 0.069 min
Response: 17258487
Conc: 6.30 ug/ml

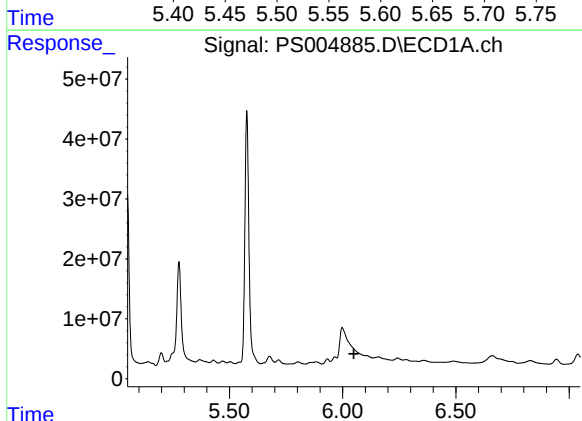


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

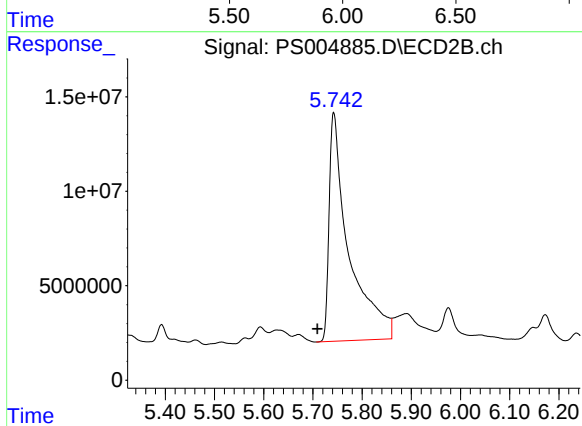

#7 MCPA


R.T.: 5.743 min
Delta R.T.: 0.034 min
Response: 337903498
Conc: 82.58 ug/ml

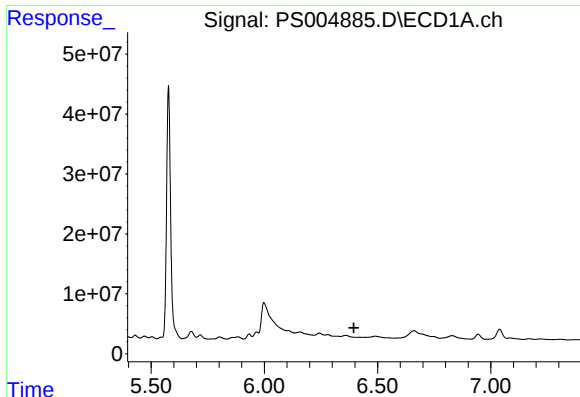

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

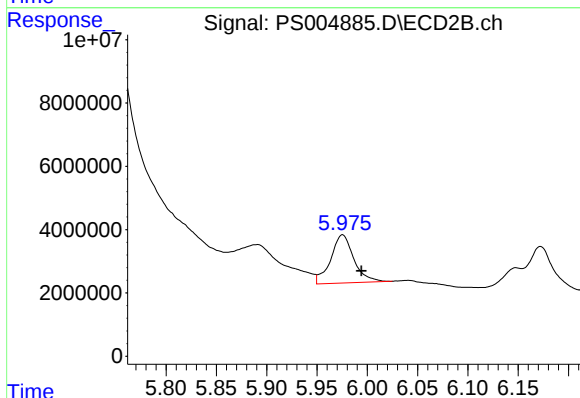


#8 DICHLORPROP

R.T.: 5.975 min
Delta R.T.: -0.019 min
Response: 24434806
Conc: 25.92 ng/ml

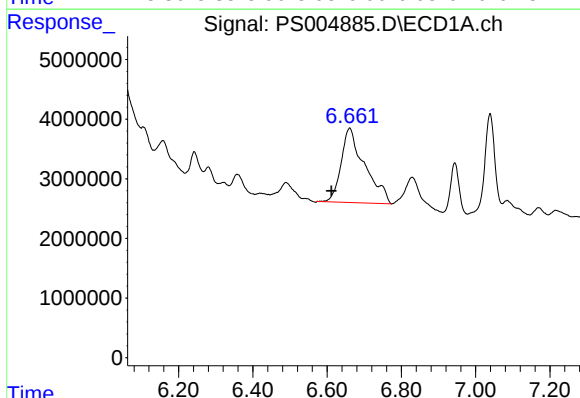


#9 2,4-D

R.T.: 6.661 min
Delta R.T.: 0.049 min
Response: 55146064
Conc: 40.31 ng/ml

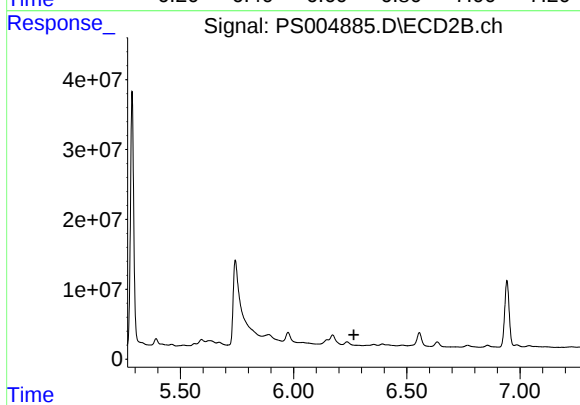

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

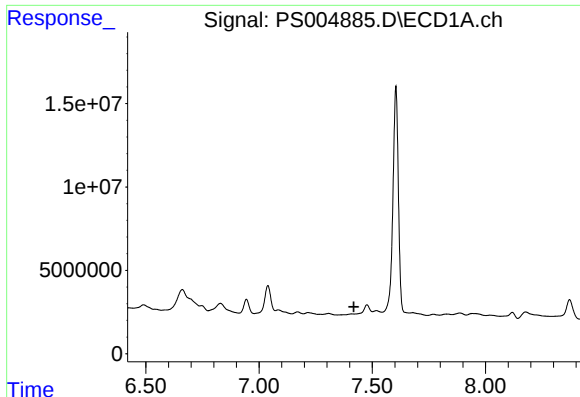

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

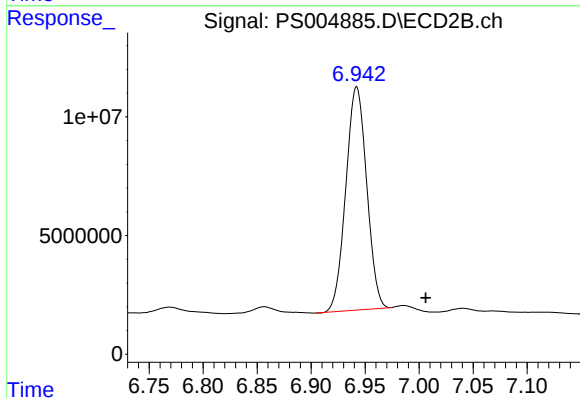


#11 2,4,5-TP (SILVEX)

R.T.: 6.942 min
Delta R.T.: -0.064 min
Response: 126468513
Conc: 24.58 ng/ml

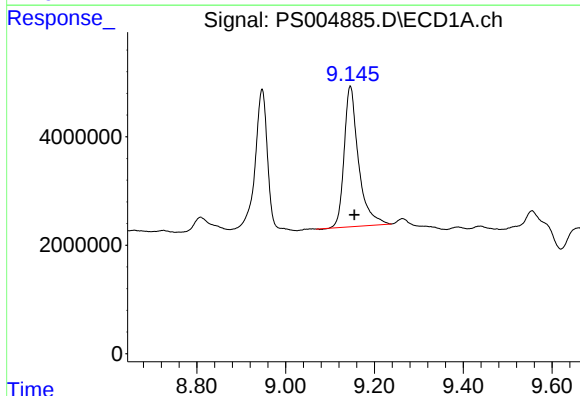


#15 Picloram

R.T.: 9.146 min
Delta R.T.: -0.010 min
Response: 58033440
Conc: 5.57 ng/ml

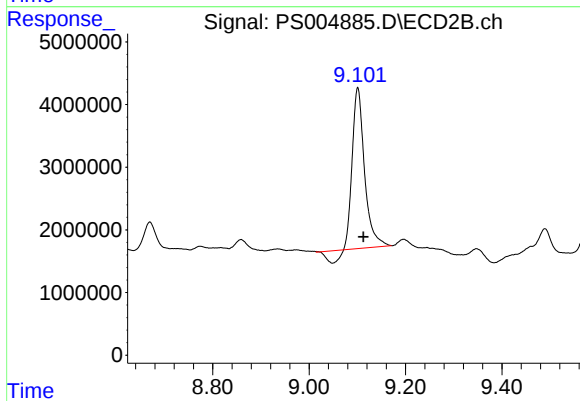

#15 Picloram


R.T.: 9.101 min
Delta R.T.: -0.012 min
Response: 42694657
Conc: 5.72 ng/ml

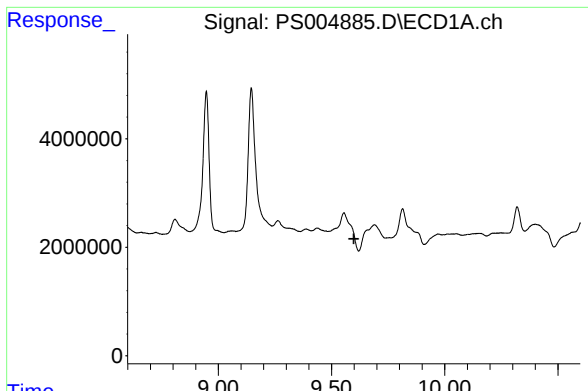

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

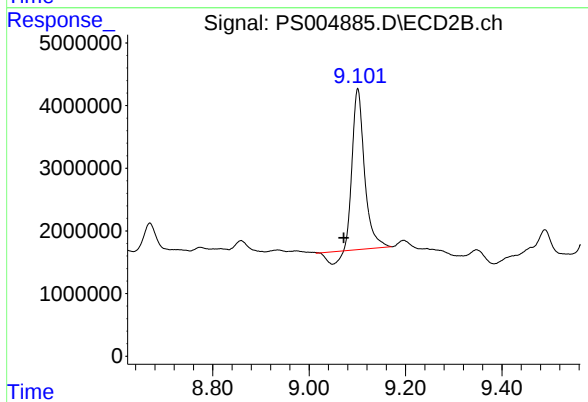

#16 DCPA

R.T.: 9.101 min
Delta R.T.: 0.029 min
Response: 42694657
Conc: 6.59 ng/ml