

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
 Data File : PS004888.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2019 15:10
 Operator : SM\AJ
 Sample : K3124-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 05:40:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.611	5.323	417.4E6	309.7E6	297.803	320.963
Target Compounds							
1) T	Dalapon	2.113	0.000	40557631	0	24.466	N.D. #
2) T	3,5-DICHL...	0.000	4.600	0	9953700	N.D.	8.078
5) T	DICAMBA	5.711	0.000	14132980	0	2.662	N.D. #
7) T	MCPA	6.031	5.779	222.2E6	481.6E6	38.354	117.709 #
8) T	DICHLORPROP	0.000	6.012	0	16105575	N.D.	17.082
9) T	2,4-D	0.000	6.208	0	29745275	N.D.	27.520
10) T	Pentachlo...	0.000	6.591	0	27992699	N.D.	2.279
11) T	2,4,5-TP ...	0.000	6.978	0	84482693	N.D.	16.419
12) T	2,4,5-T	7.636	0.000	135.2E6	0	18.159	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
Data File : PS004888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2019 15:10
Operator : SM\AJ
Sample : K3124-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 05:40:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

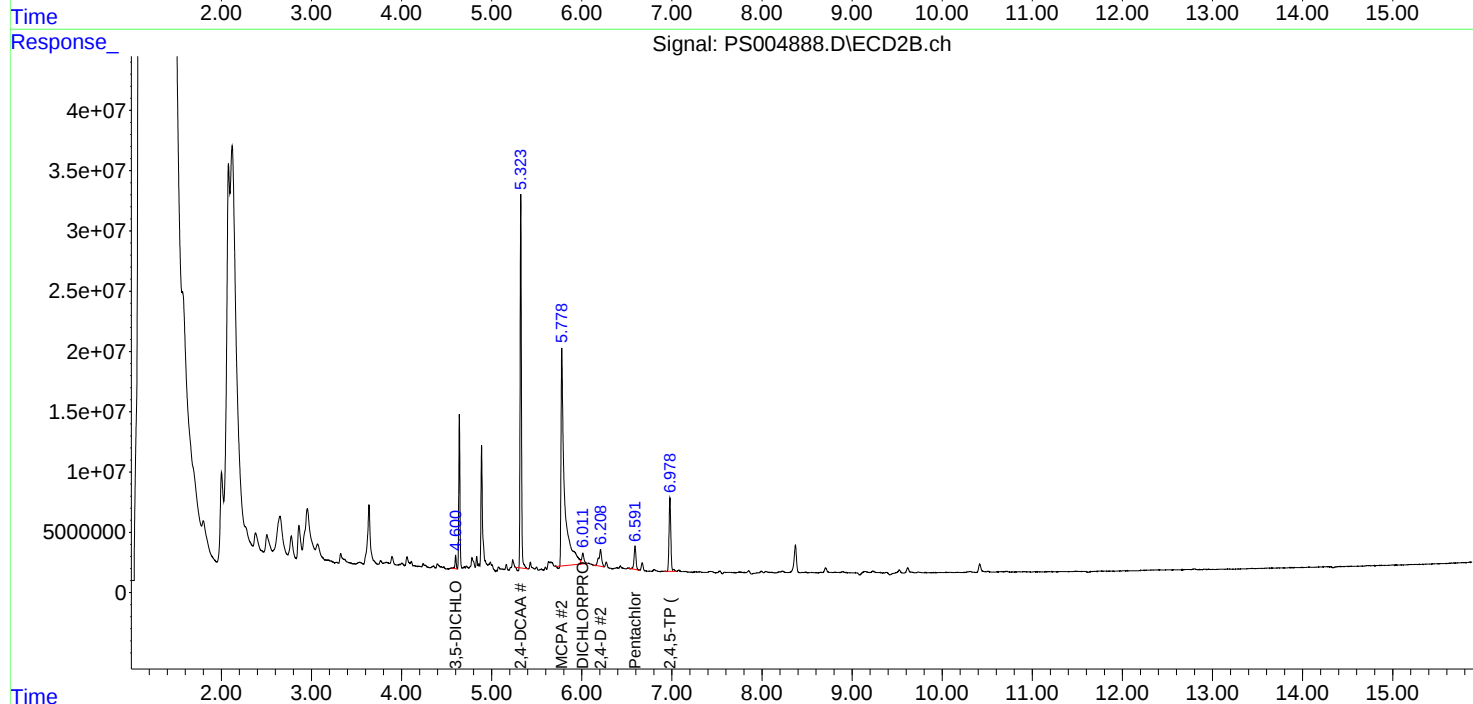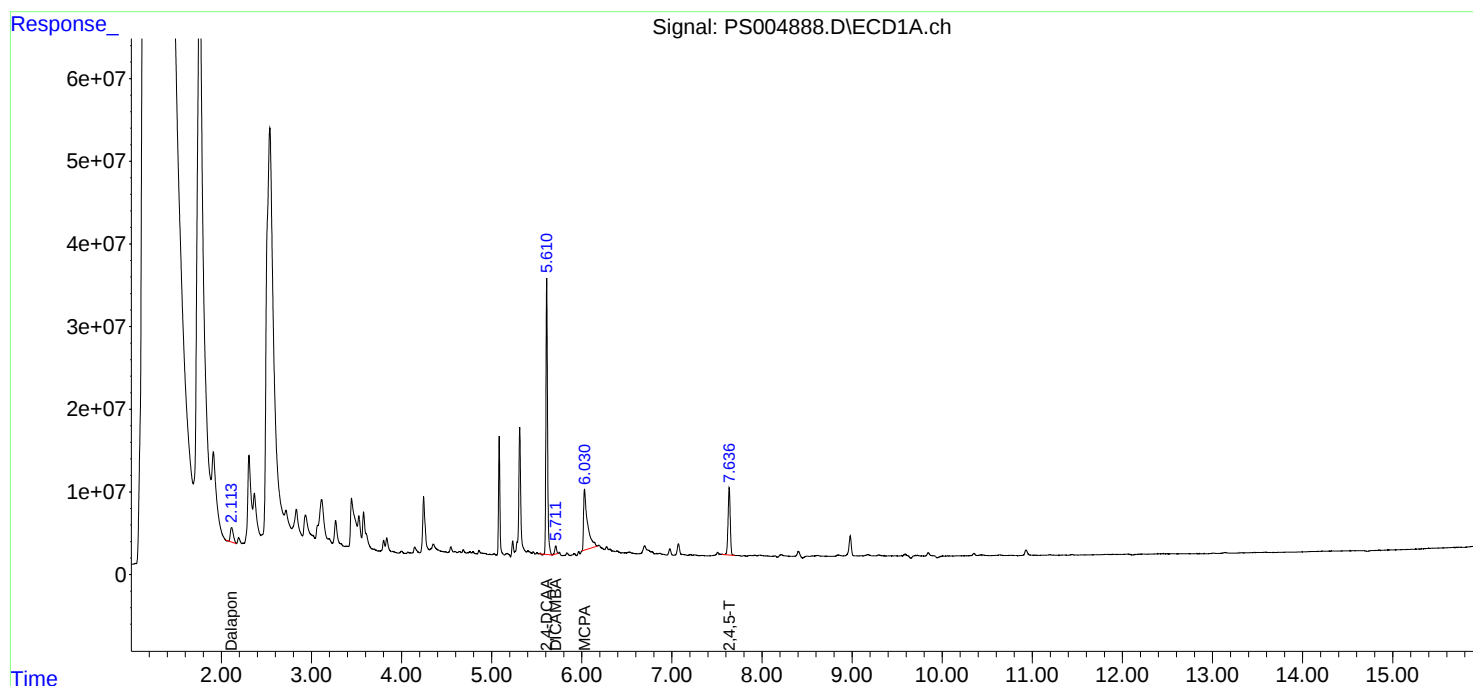


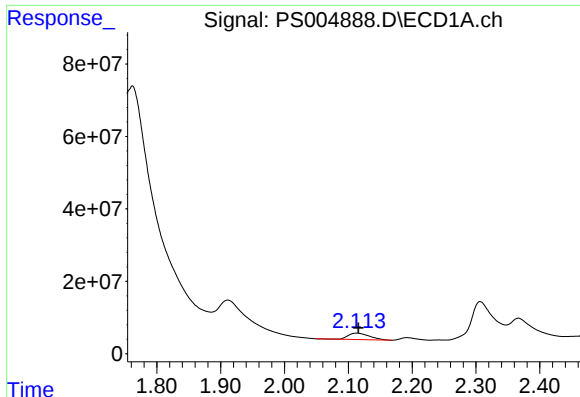

#1 Dalapon


R.T.: 2.113 min
Delta R.T.: -0.003 min
Response: 40557631
Conc: 24.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

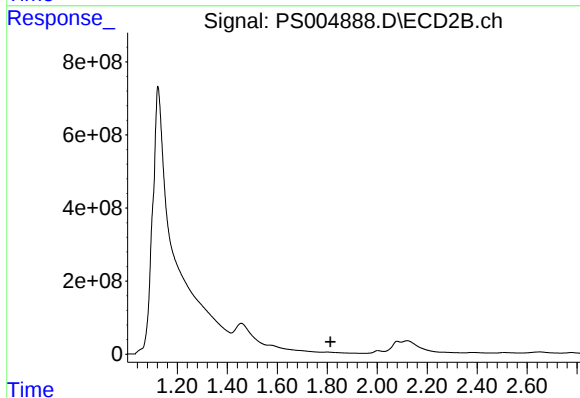


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

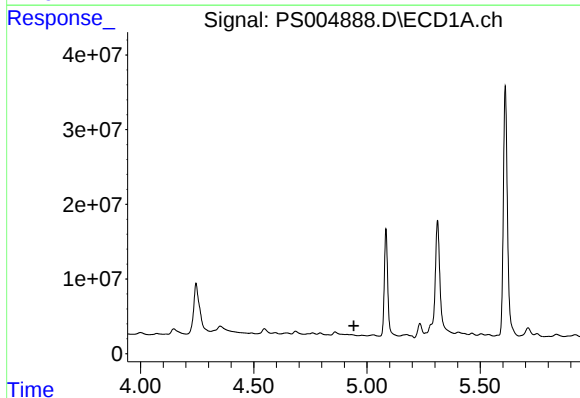


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

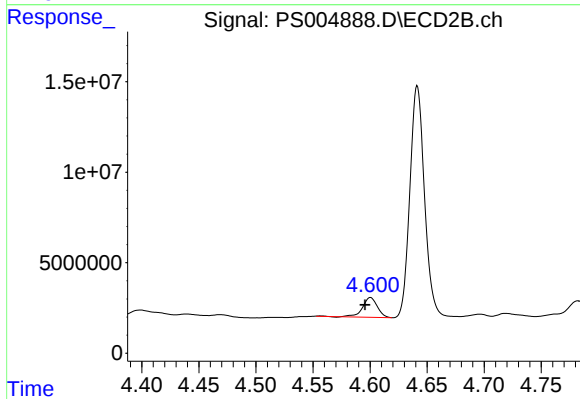

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.600 min
Delta R.T.: 0.005 min
Response: 9953700
Conc: 8.08 ng/ml

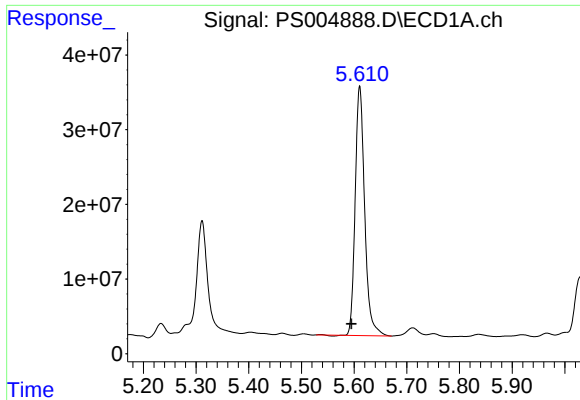

#4 2,4-DCAA


R.T.: 5.611 min
Delta R.T.: 0.016 min
Response: 417447363
Conc: 297.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

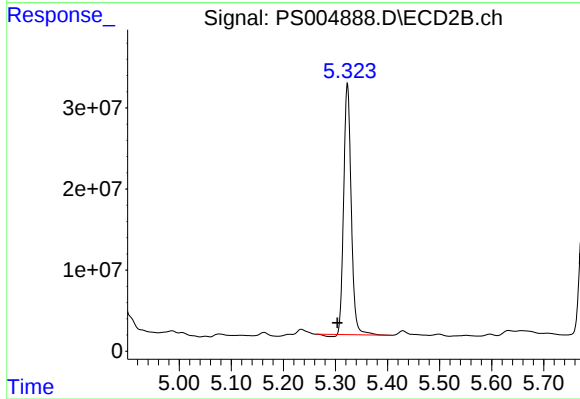


#4 2,4-DCAA

R.T.: 5.323 min
Delta R.T.: 0.019 min
Response: 309676334
Conc: 320.96 ng/ml

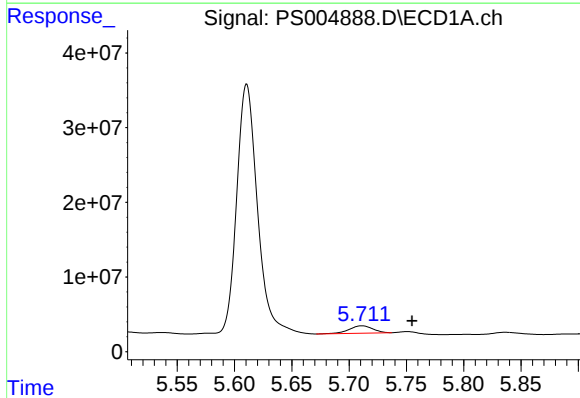


#5 DICAMBA

R.T.: 5.711 min
Delta R.T.: -0.044 min
Response: 14132980
Conc: 2.66 ng/ml

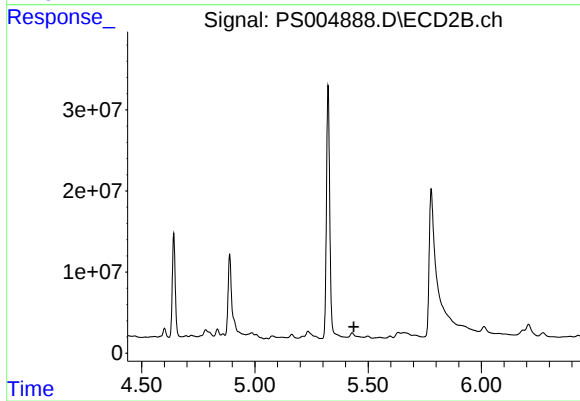

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.437 min
Response: 0
Conc: N.D.

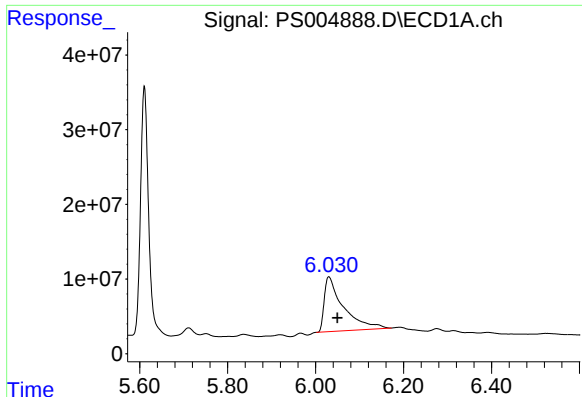

#7 MCPA


R.T.: 6.031 min
Delta R.T.: -0.019 min
Response: 222152903
Conc: 38.35 ug/ml

Instrument :
ECD_S
ClientSampleId :

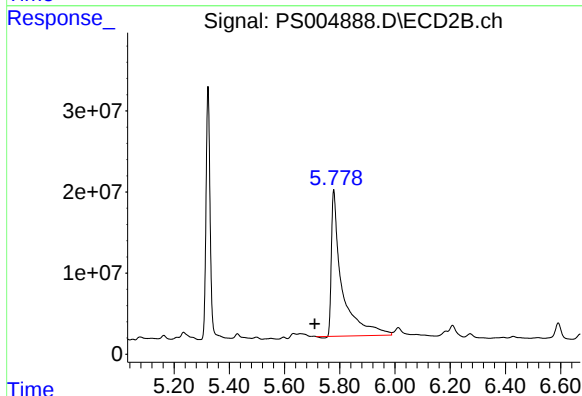


#7 MCPA

R.T.: 5.779 min
Delta R.T.: 0.070 min
Response: 481622795
Conc: 117.71 ug/ml

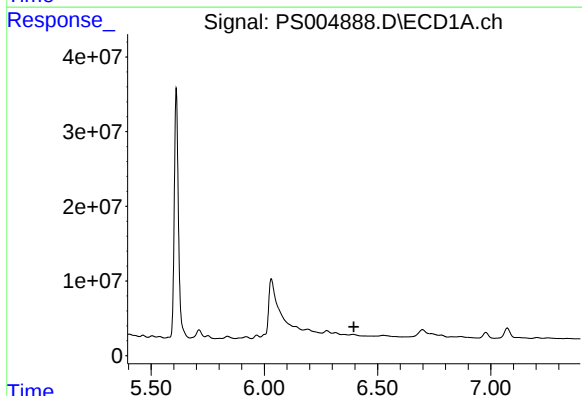


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

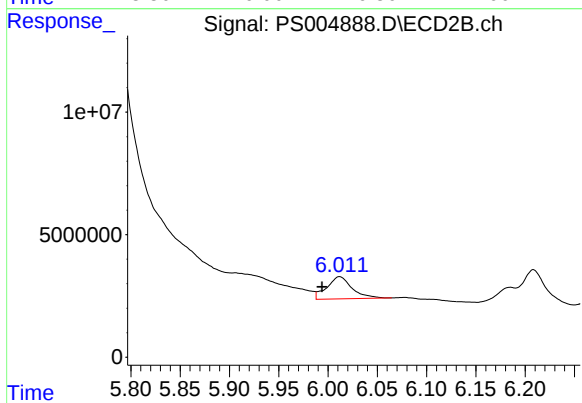

#8 DICHLORPROP


R.T.: 6.012 min
Delta R.T.: 0.018 min
Response: 16105575
Conc: 17.08 ng/ml

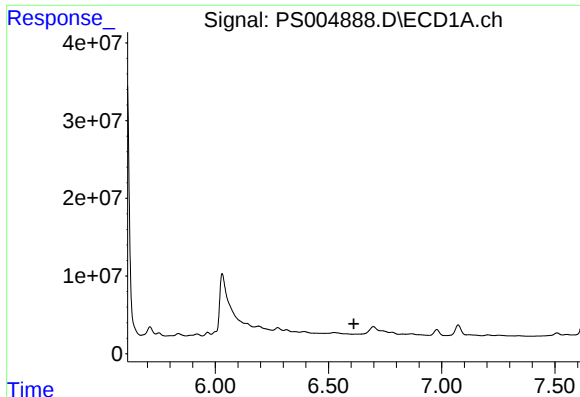

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

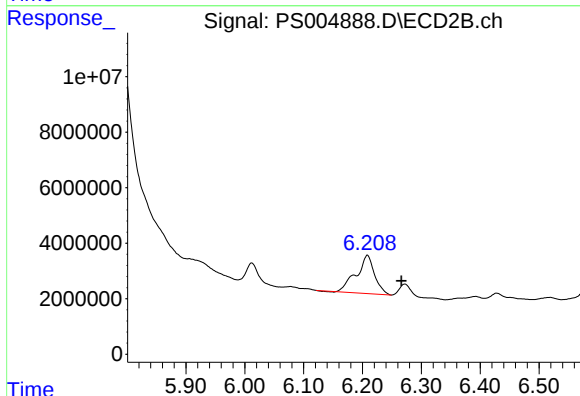


#9 2,4-D

R.T.: 6.208 min
Delta R.T.: -0.058 min
Response: 29745275
Conc: 27.52 ng/ml

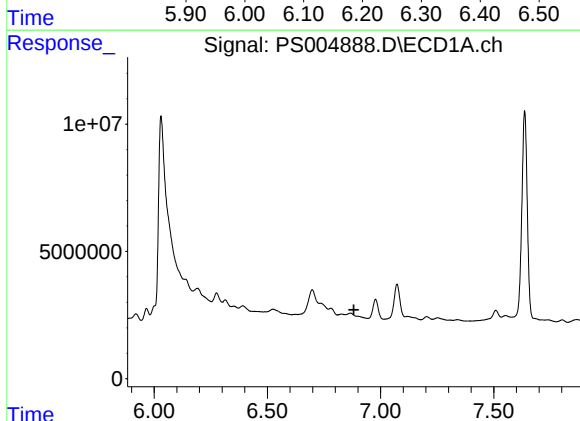


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

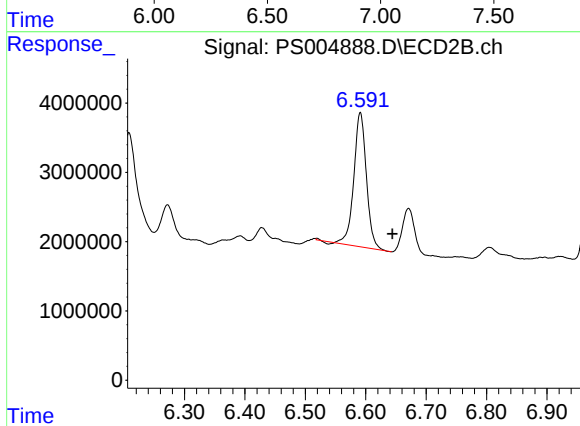

#10 Pentachlorophenol


R.T.: 6.591 min
Delta R.T.: -0.053 min
Response: 27992699
Conc: 2.28 ng/ml

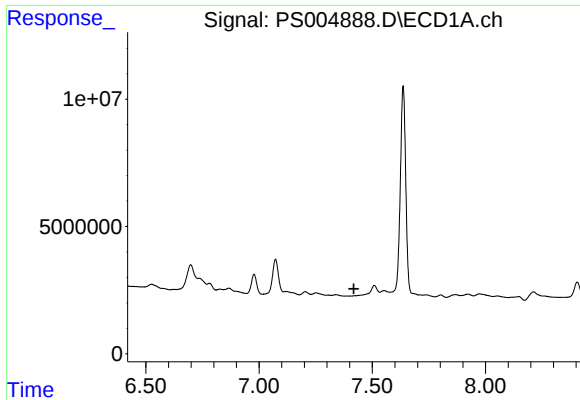

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

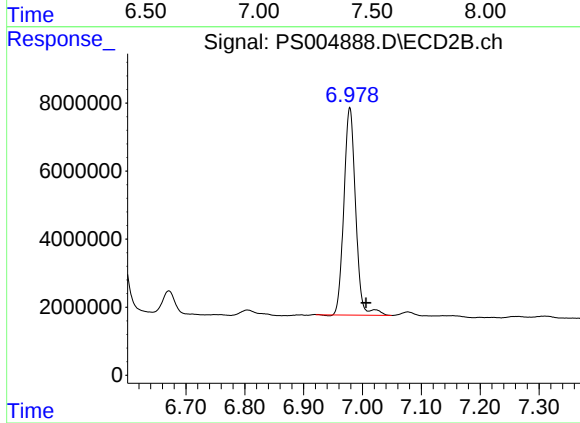


#11 2,4,5-TP (SILVEX)

R.T.: 6.978 min
Delta R.T.: -0.028 min
Response: 84482693
Conc: 16.42 ng/ml

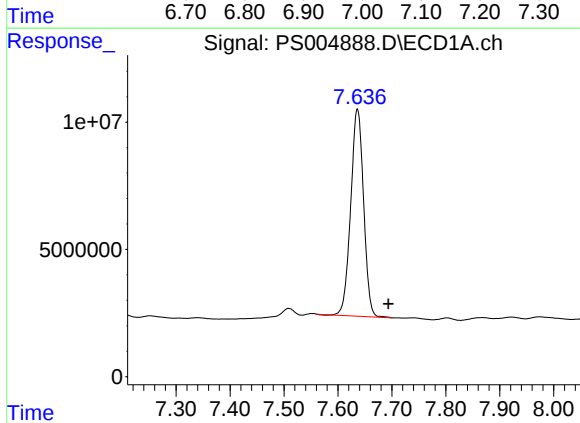

#12 2,4,5-T

R.T.: 7.636 min
Delta R.T.: -0.057 min
Response: 135240989
Conc: 18.16 ng/ml

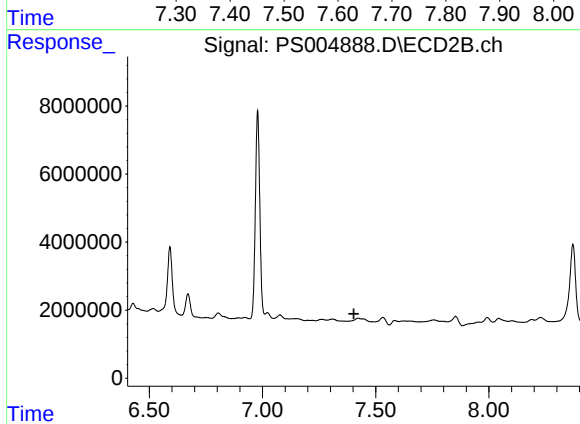

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.404 min
Response: 0
Conc: N.D.