

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
 Data File : PS004890.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2019 16:28
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 05:41:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.578	5.286	665.9E6	490.8E6	475.020	508.712
Target Compounds							
2) T	3,5-DICHL...	4.943	0.000	26435304	0	15.329	N.D. #
5) T	DICAMBA	0.000	5.441	0	56617344	N.D.	15.326
6) T	MCP	5.971	0.000	11534140	0	2.771	N.D. #
8) T	DICHLORPROP	0.000	5.979	0	22135276	N.D.	23.478
9) T	2,4-D	6.620	0.000	255.1E6	0	186.517	N.D. #
15) T	Picloram	9.116	0.000	667.0E6	0	64.011	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060319\
Data File : PS004890.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2019 16:28
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 05:41:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

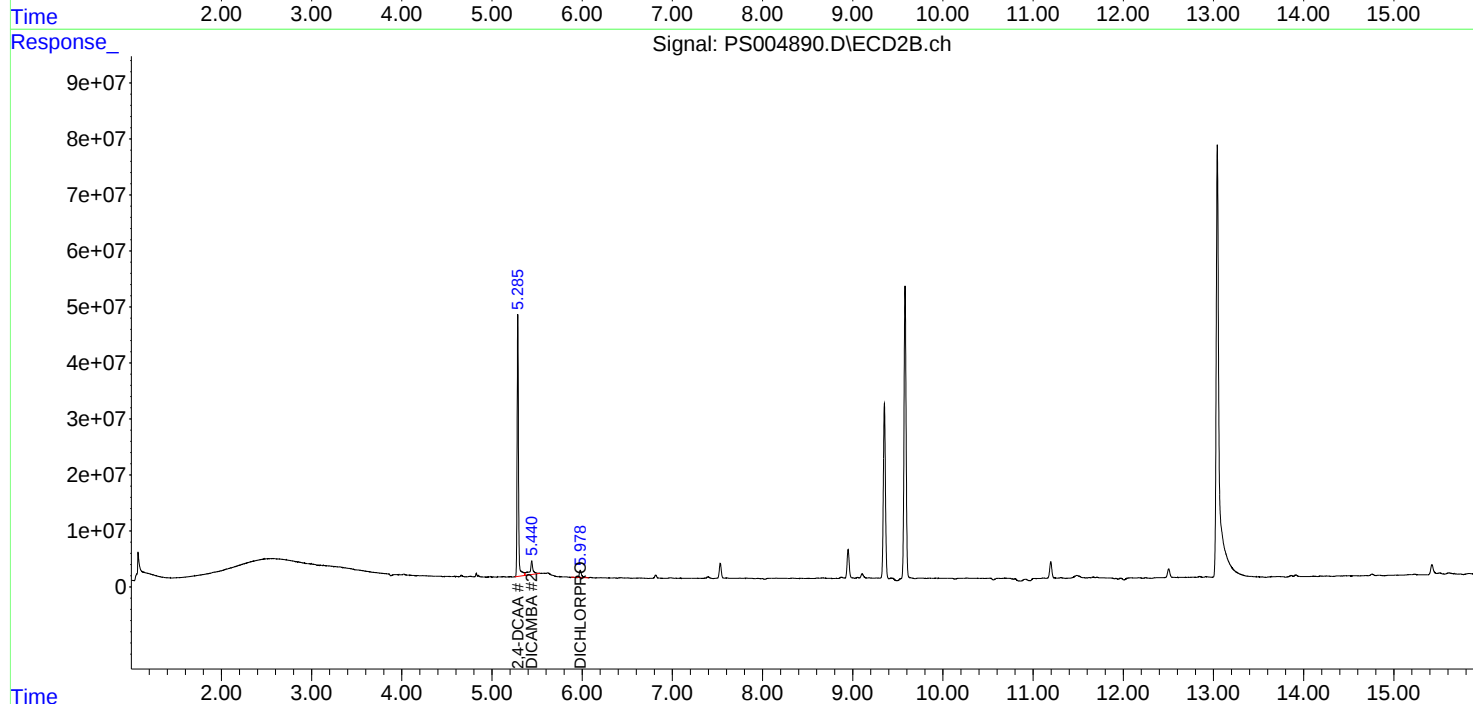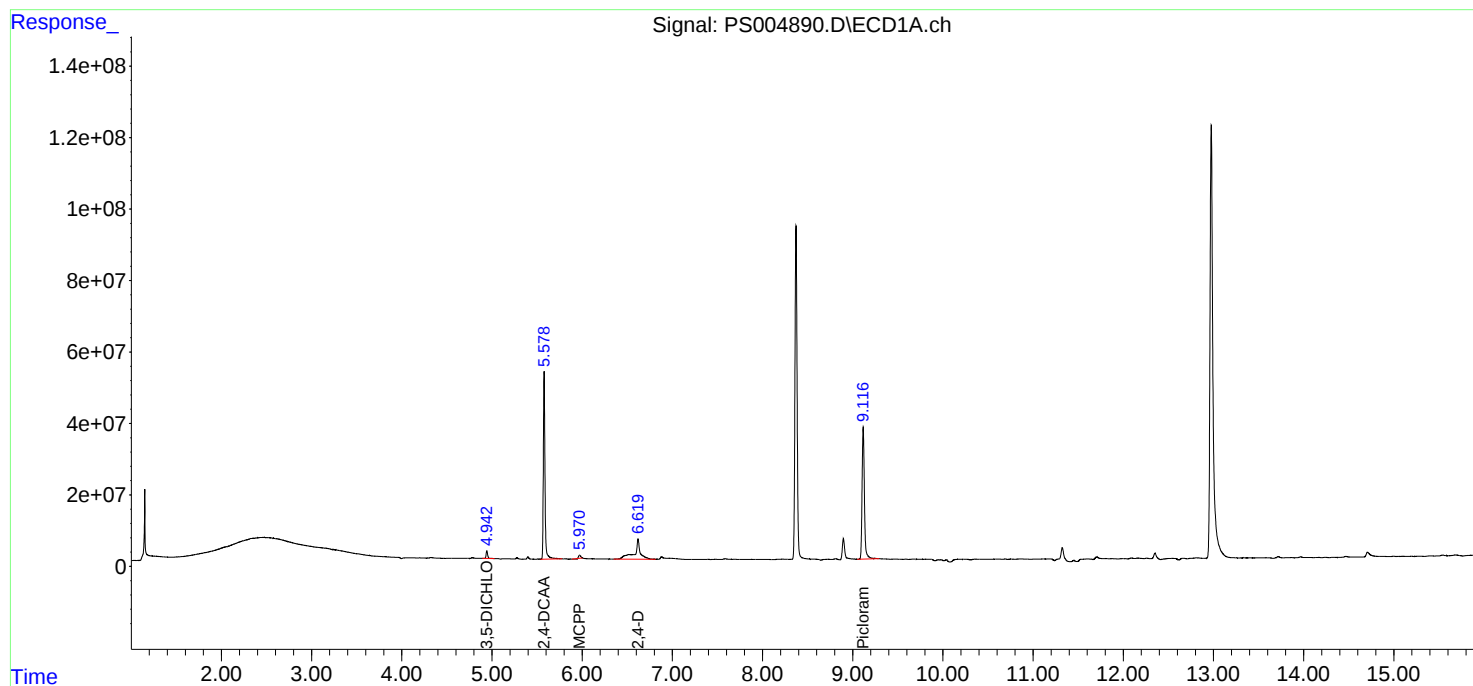


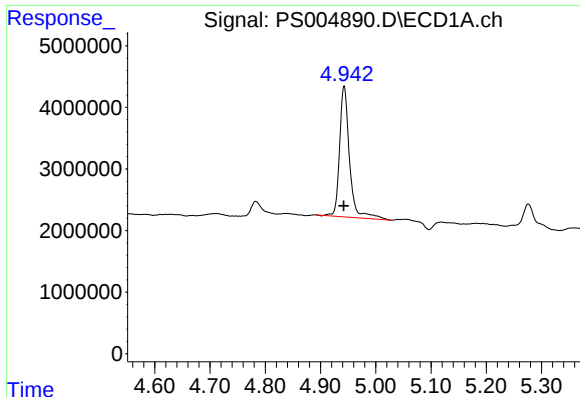

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 26435304
Conc: 15.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

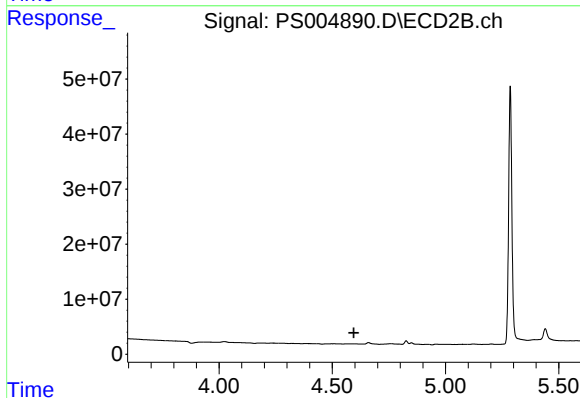


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

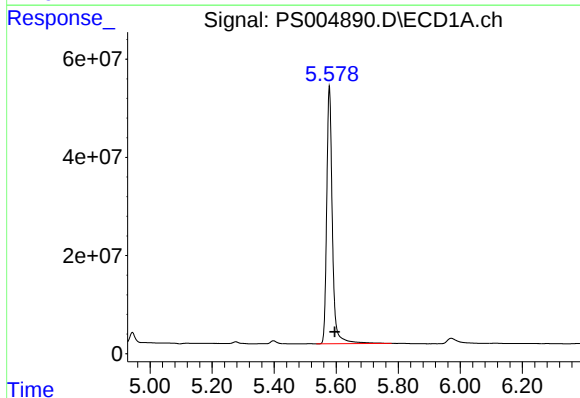


#4 2,4-DCAA

R.T.: 5.578 min
Delta R.T.: -0.017 min
Response: 665861685
Conc: 475.02 ng/ml

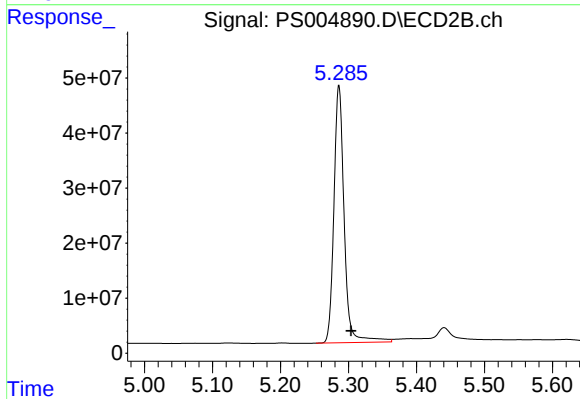

#4 2,4-DCAA


R.T.: 5.286 min
Delta R.T.: -0.018 min
Response: 490823736
Conc: 508.71 ng/ml

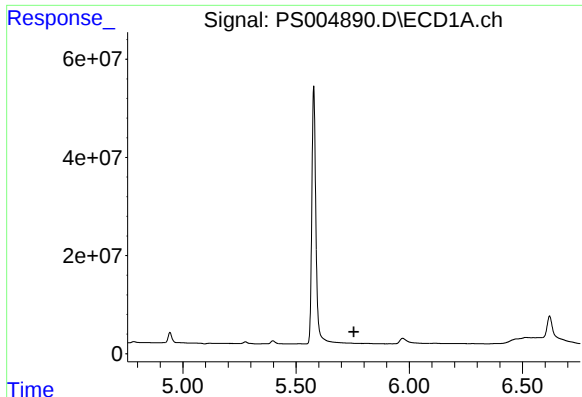

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

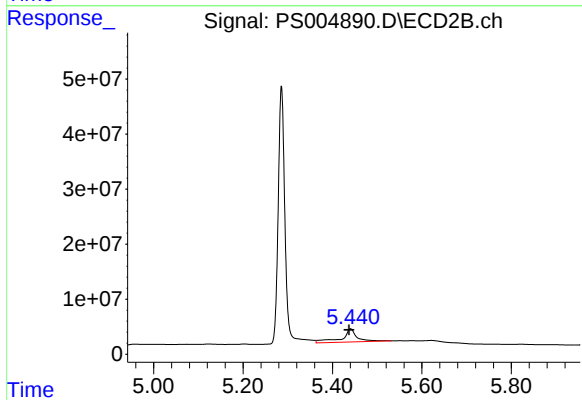


#5 DICAMBA

R.T.: 5.441 min
Delta R.T.: 0.004 min
Response: 56617344
Conc: 15.33 ng/ml

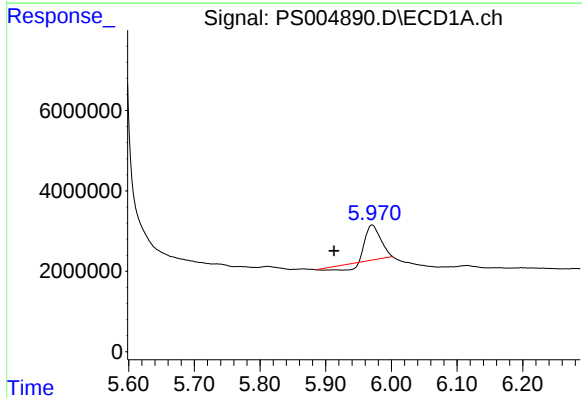


#6 MCP

R.T.: 5.971 min
Delta R.T.: 0.059 min
Response: 11534140
Conc: 2.77 ug/ml

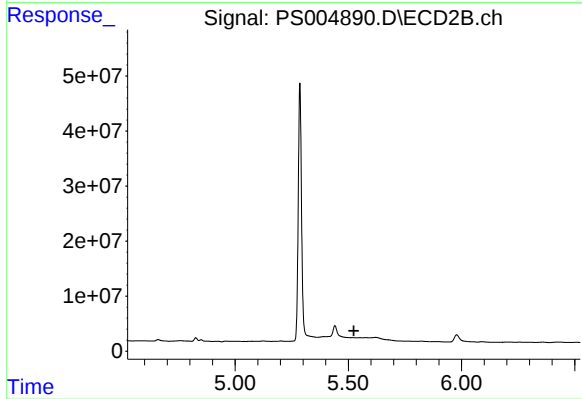

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

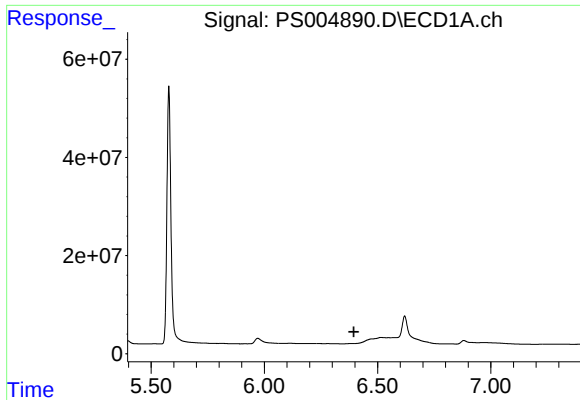

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

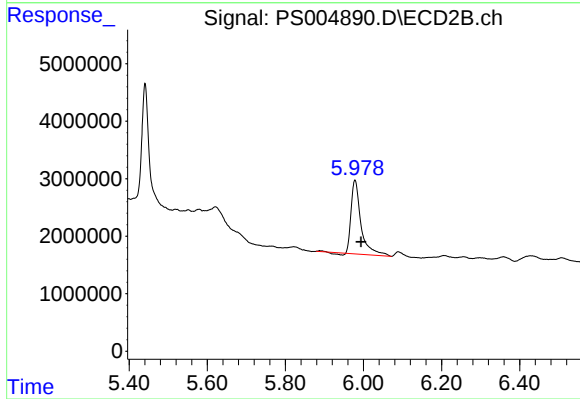


#8 DICHLORPROP

R.T.: 5.979 min
Delta R.T.: -0.015 min
Response: 22135276
Conc: 23.48 ng/ml

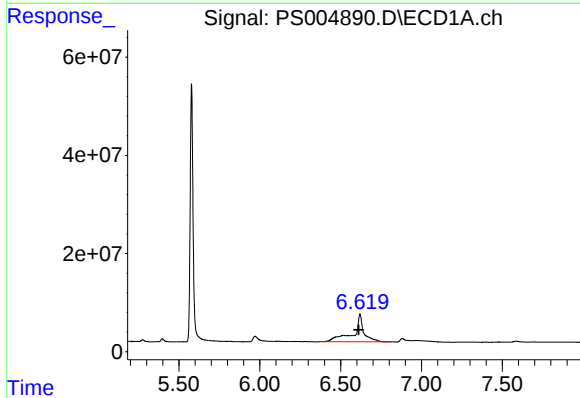


#9 2,4-D

R.T.: 6.620 min
Delta R.T.: 0.008 min
Response: 255138893
Conc: 186.52 ng/ml

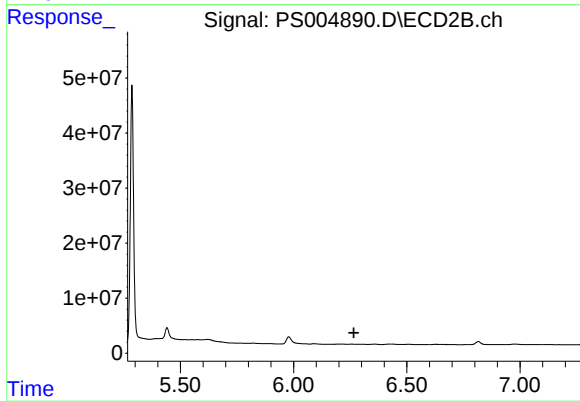

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

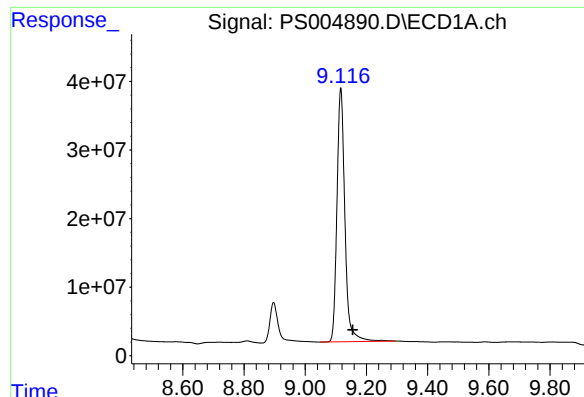

#15 Picloram

R.T.: 9.116 min
Delta R.T.: -0.039 min
Response: 666999472
Conc: 64.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

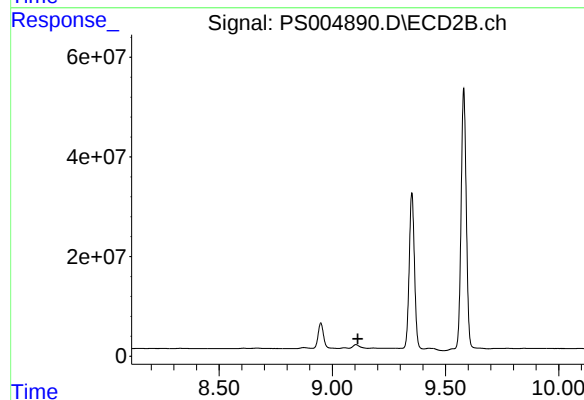

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.113 min
Response: 0
Conc: N.D.