

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060422\
 Data File : PS019603.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 08:41
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 15:37:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.209	6.783	-331602	1099652	N.D.	1.419
Target Compounds							
1) T	Dalapon	2.998	0.000	680248	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.445	5.992	961906	229325	<MDL	<MDL #
3) T	4-Nitroph...	7.051	6.416	-349256	1635891	N.D.	3.822
5) T	DICAMBA	7.419	6.947	425144	455542	<MDL	<MDL #
6) T	MCPD	7.578	7.005	-267413	455857	N.D.	<MDL
7) T	MCPA	7.664	0.000	3268645	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.601	0	634861	N.D.	<MDL
9) T	2,4-D	8.367f	7.814f	3515450	338720	1.229	<MDL #
10) T	Pentachlo...	8.623	8.284	689092	316967	<MDL	<MDL #
11) T	2,4,5-TP ...	9.101f	8.650	138265	301961	<MDL	<MDL #
12) T	2,4,5-T	9.469	9.035	4916908	568262	<MDL	<MDL #
13) T	2,4-DB	9.997	9.548	627572	309292	<MDL	<MDL #
15) T	Picloram	10.970	10.858	20350631	10769517	<MDL	1.674 #
16) T	DCPA	11.433	10.783	2526614	4171146	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060422\
Data File : PS019603.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 08:41
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 15:37:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

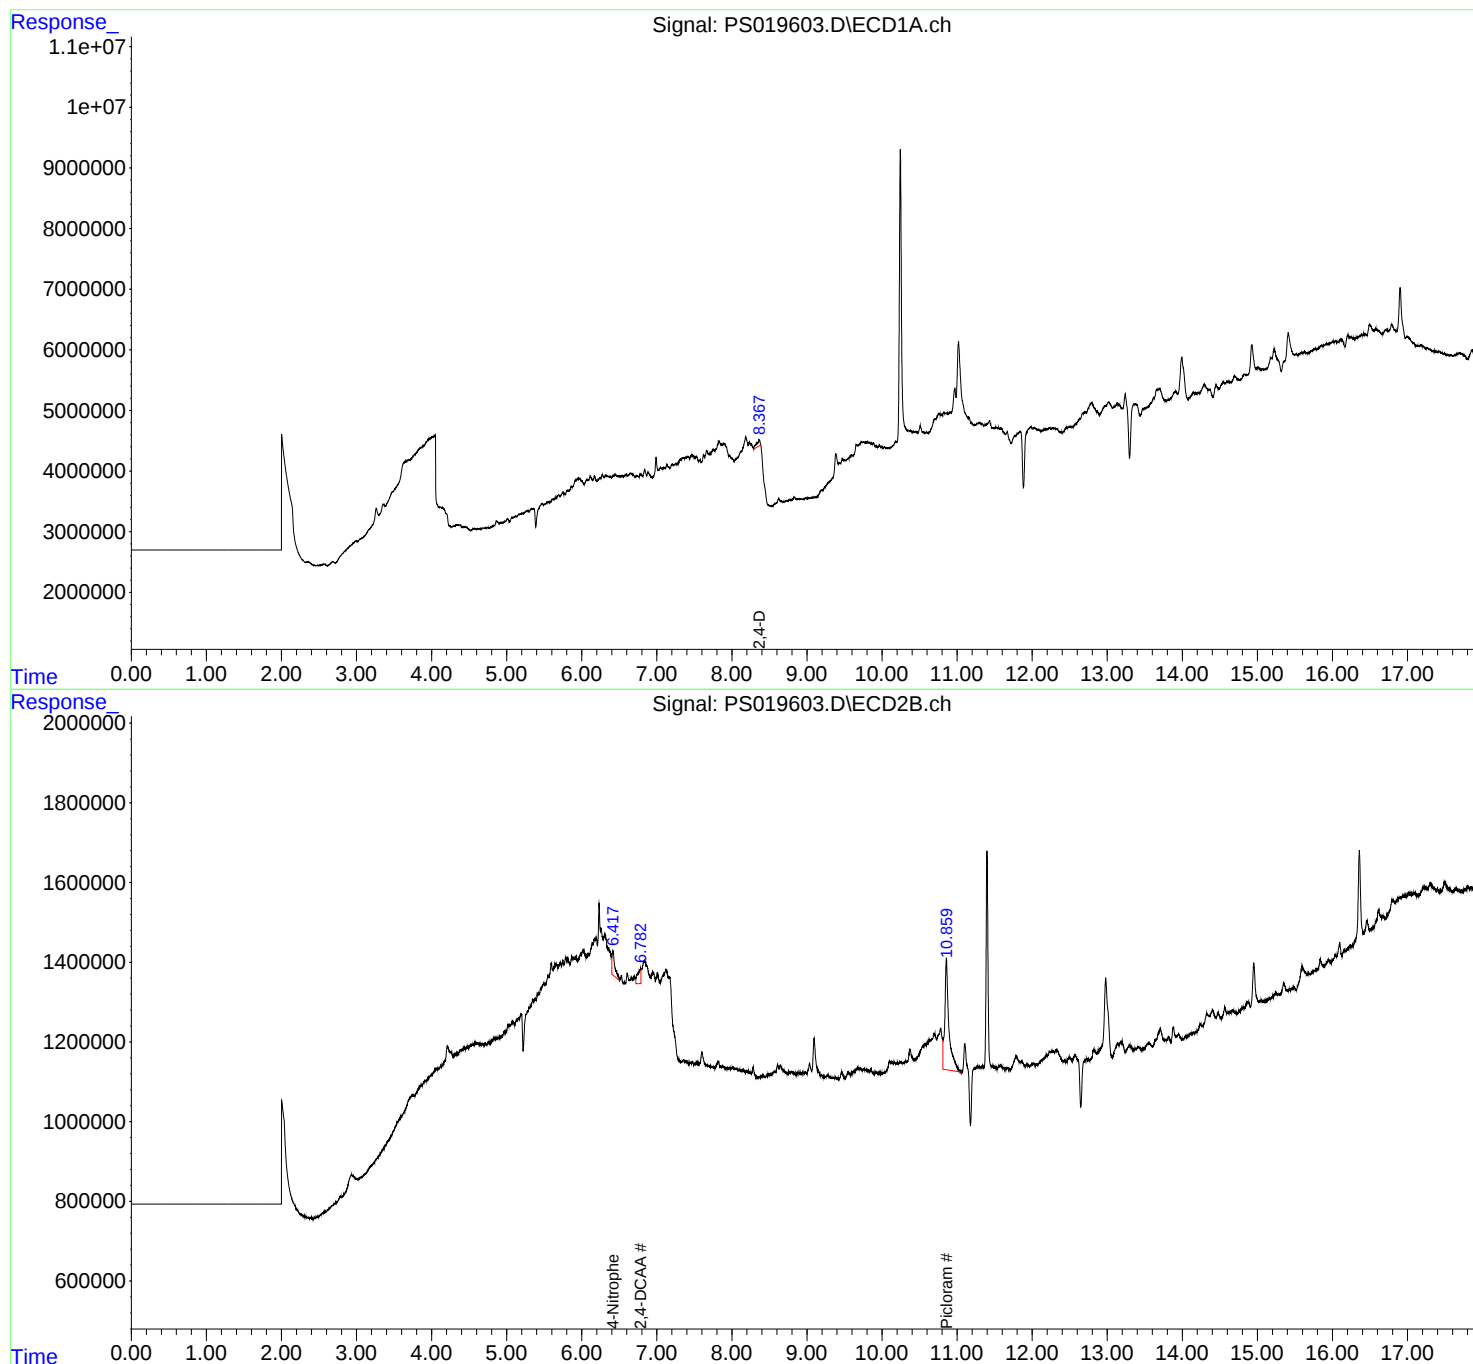


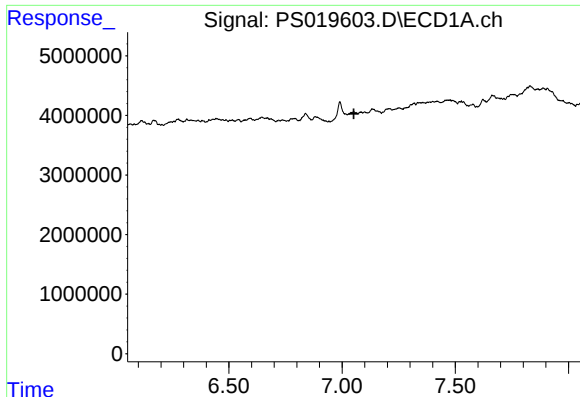

#3 4-Nitrophenol


R.T.: 7.051 min
Delta R.T.: 0.000 min
Response: -349256
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

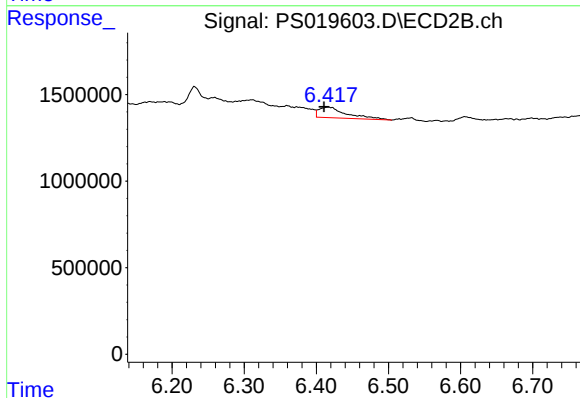


#3 4-Nitrophenol

R.T.: 6.416 min
Delta R.T.: 0.006 min
Response: 1635891
Conc: 3.82 ng/ml

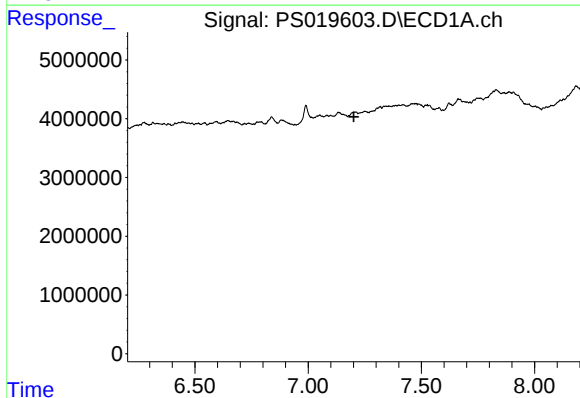


#4 2,4-DCAA

R.T.: 7.209 min
Delta R.T.: 0.007 min
Response: -331602
Conc: N.D.

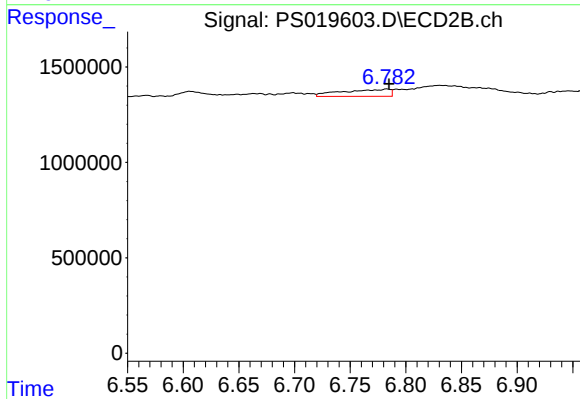

#4 2,4-DCAA


R.T.: 6.783 min
Delta R.T.: -0.002 min
Response: 1099652
Conc: 1.42 ng/ml

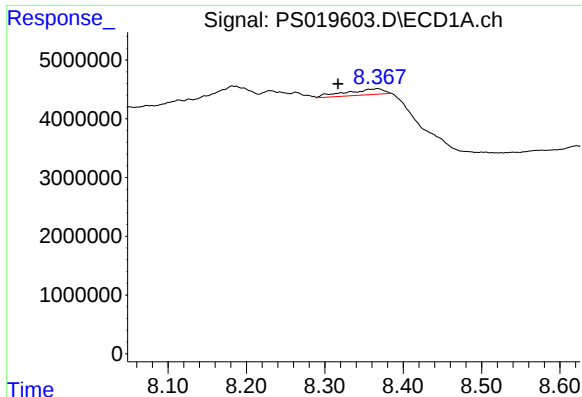

#9 2,4-D


R.T.: 8.367 min
Delta R.T.: 0.050 min
Response: 3515450
Conc: 1.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

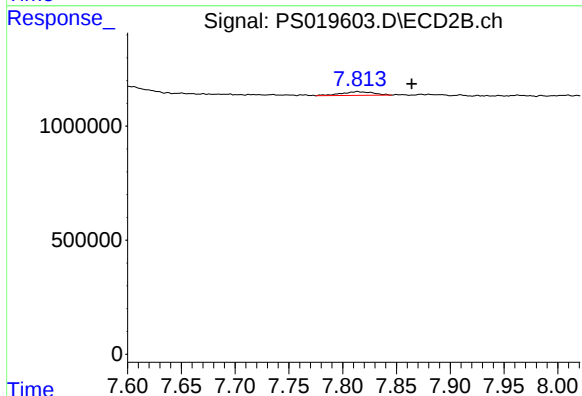


#9 2,4-D

R.T.: 7.814 min
Delta R.T.: -0.050 min
Response: 338720
Conc: N.D.

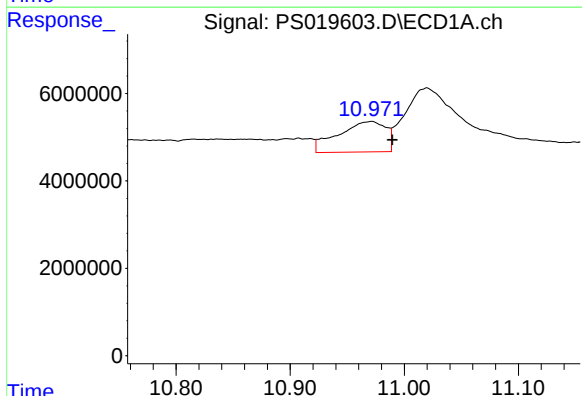

#15 Picloram

R.T.: 10.970 min
Delta R.T.: -0.019 min
Response: 20350631
Conc: N.D.

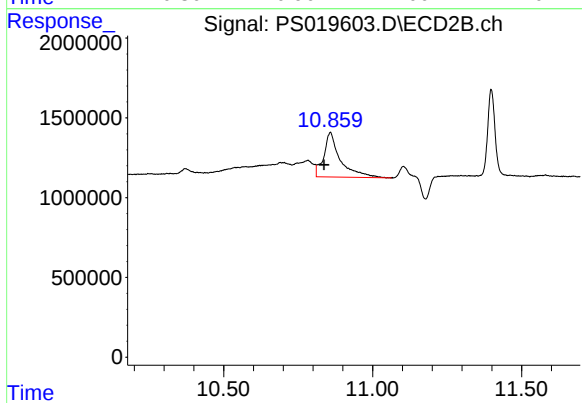

#15 Picloram

R.T.: 10.858 min
Delta R.T.: 0.021 min
Response: 10769517
Conc: 1.67 ng/ml