

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060422\
 Data File : PS019615.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 20:01
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 22:51:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.200	6.784	1158.8E6	466.0E6	483.014	601.333
Target Compounds							
1) T	Dalapon	2.988	0.000	964099	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.461f	5.919f	4354374	434387	1.378	<MDL #
3) T	4-Nitroph...	6.989f	6.389	1998877	603366	2.037	1.410 #
5) T	DICAMBA	0.000	7.003f	0	1244810	N.D.	<MDL
6) T	MCPD	0.000	7.003	0	1244810	N.D.	<MDL
7) T	MCPA	7.704	7.182f	4245765	5821246	<MDL	1.515 #
8) T	DICHLORPROP	0.000	7.634f	0	3156897	N.D.	3.574
9) T	2,4-D	0.000	7.854	0	423191	N.D.	<MDL
10) T	Pentachlo...	8.618	8.286	1078208	1014117	<MDL	<MDL #
11) T	2,4,5-TP ...	9.184	8.655	1819851	394844	<MDL	<MDL #
12) T	2,4,5-T	9.438	9.059	6036011	766866	<MDL	<MDL #
13) T	2,4-DB	10.003	9.568	2599331	454255	<MDL	<MDL #
14) T	DINOSEB	11.152	9.857	9598827	457524	<MDL	<MDL #
15) T	Picloram	10.959	10.889f	363.6E6	4354834	12.251	<MDL #
16) T	DCPA	11.427	10.778	4561480	1778254	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060422\
Data File : PS019615.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 20:01
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 22:51:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

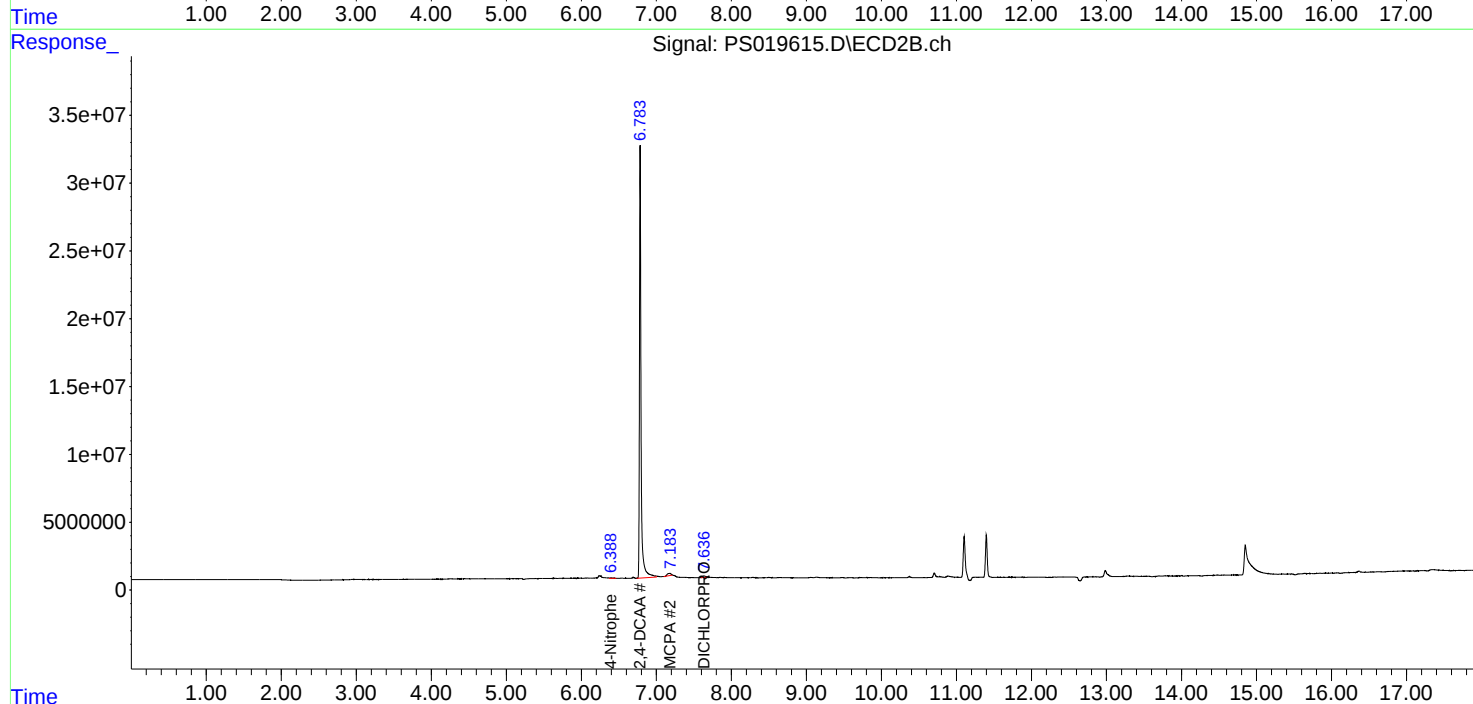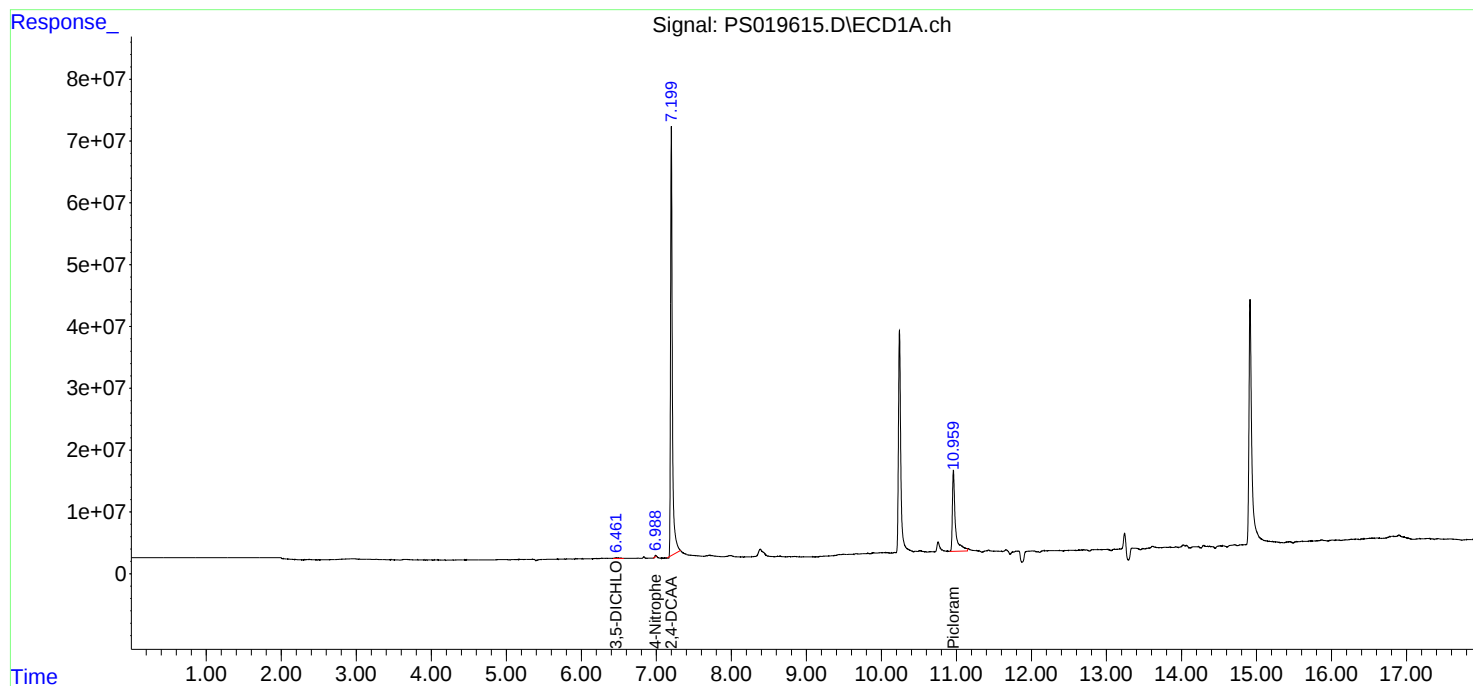


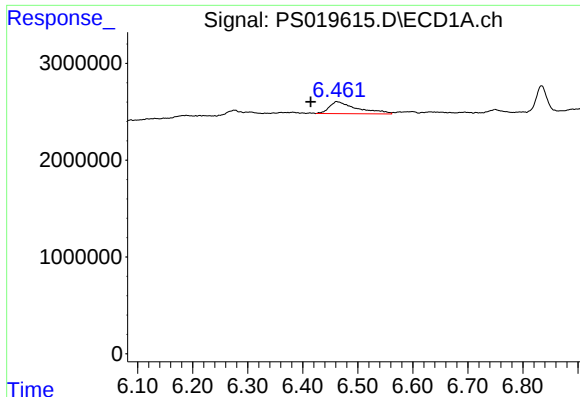

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.461 min
Delta R.T.: 0.047 min
Response: 4354374
Conc: 1.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

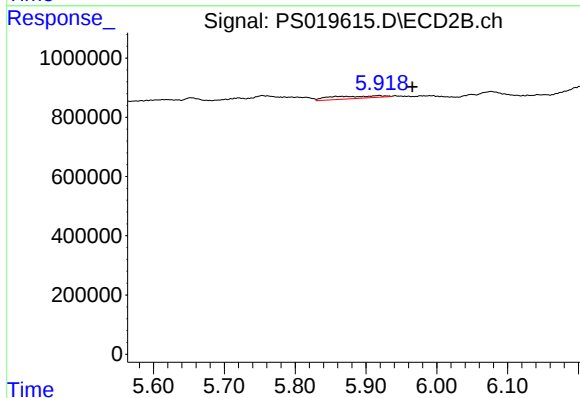


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.919 min
Delta R.T.: -0.047 min
Response: 434387
Conc: N.D.

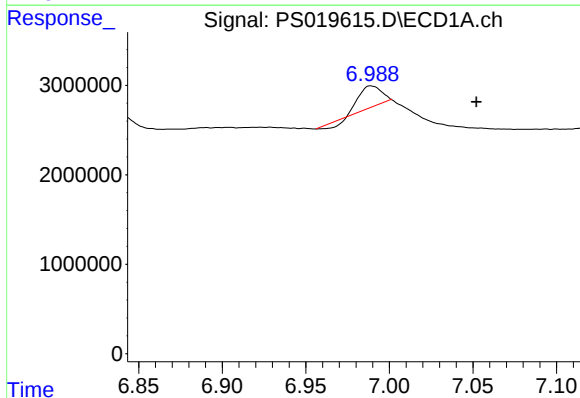


#3 4-Nitrophenol

R.T.: 6.989 min
Delta R.T.: -0.063 min
Response: 1998877
Conc: 2.04 ng/ml

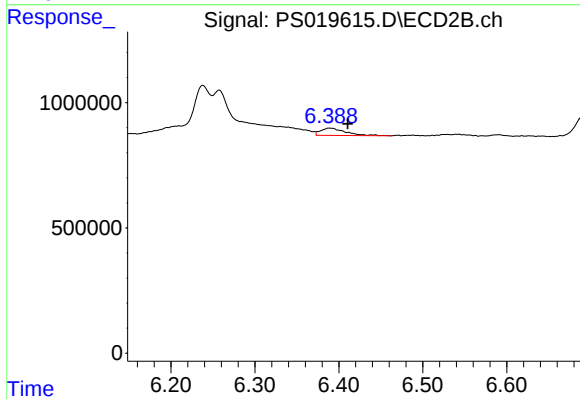

#3 4-Nitrophenol


R.T.: 6.389 min
Delta R.T.: -0.022 min
Response: 603366
Conc: 1.41 ng/ml

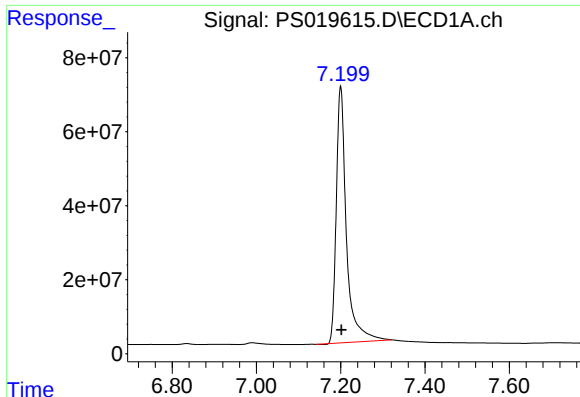

#4 2,4-DCAA


R.T.: 7.200 min
Delta R.T.: -0.002 min
Response: 1158830378
Conc: 483.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

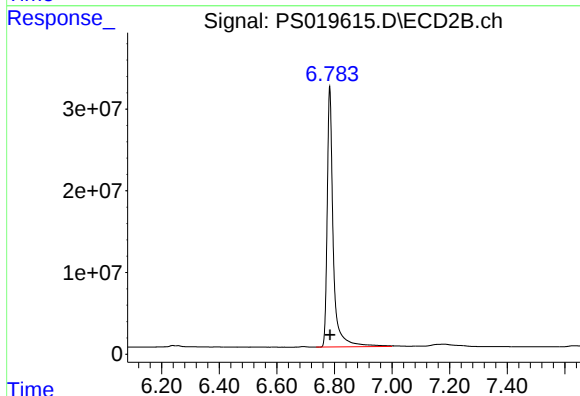


#4 2,4-DCAA

R.T.: 6.784 min
Delta R.T.: -0.001 min
Response: 465954974
Conc: 601.33 ng/ml

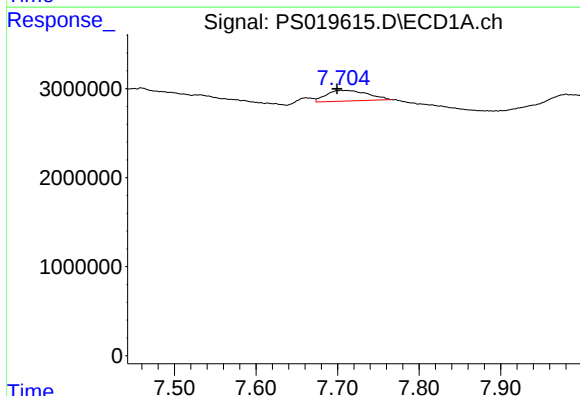


#7 MCPA

R.T.: 7.704 min
Delta R.T.: 0.005 min
Response: 4245765
Conc: N.D.

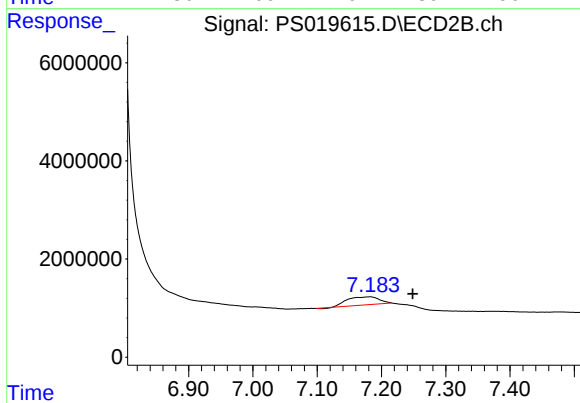

#7 MCPA


R.T.: 7.182 min
Delta R.T.: -0.066 min
Response: 5821246
Conc: 1.51 ug/ml

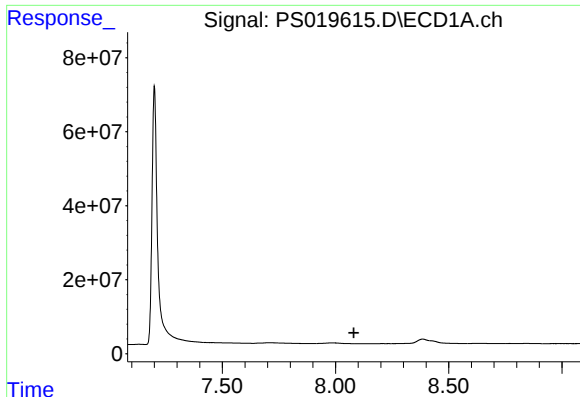

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.081 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

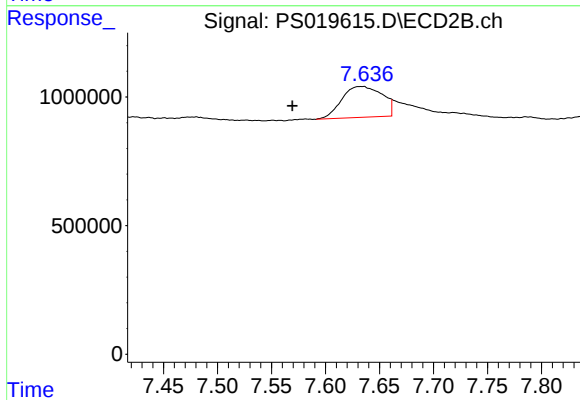


#8 DICHLORPROP

R.T.: 7.634 min
Delta R.T.: 0.065 min
Response: 3156897
Conc: 3.57 ng/ml

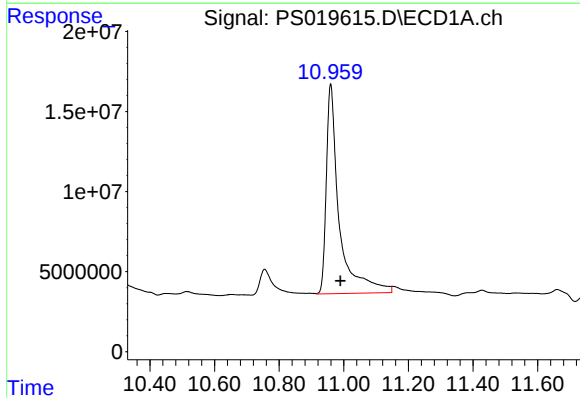

#15 Picloram

R.T.: 10.959 min
Delta R.T.: -0.030 min
Response: 363584957
Conc: 12.25 ng/ml

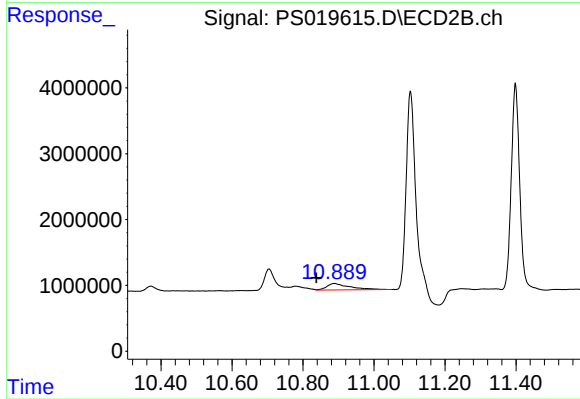

#15 Picloram

R.T.: 10.889 min
Delta R.T.: 0.051 min
Response: 4354834
Conc: N.D.