

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS060422\  
 Data File : PS019609.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 03 Jun 2022 17:38  
 Operator : AJ\MA  
 Sample : N3143-06  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 20220427-SPLP-AMENDED-SB-8-(DISCRETE-COMP-G)

Manual Integrations  
 APPROVED

Reviewed By :Abdul Mirza 06/04/2022  
 Supervised By :Ankita Jodhani 06/06/2022

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 03 19:21:54 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS052422.M  
 Quant Title : 8080.M  
 QLast Update : Wed May 25 02:05:34 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1   | Resp#2  | ng/ml   | ng/ml    |
|-----------------------------|-------|-------|----------|---------|---------|----------|
| -----                       |       |       |          |         |         |          |
| System Monitoring Compounds |       |       |          |         |         |          |
| 4) S 2,4-DCAA               | 7.202 | 6.780 | 1154.0E6 | 440.4E6 | 481.008 | 568.354m |

Target Compounds

-----

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS060422\  
Data File : PS019609.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 03 Jun 2022 17:38  
Operator : AJ\MA  
Sample : N3143-06  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

## Instrument :

ECD\_S

## ClientSampleId :

20220427-SPLP-AMENDED-SB-8-(DISCRETE-COMP-G)

## Manual Integrations



## APPROVED


Reviewed By :Abdul Mirza 06/04/2022

Supervised By :Ankita Jodhani 06/06/2022

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 03 19:21:54 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS052422.M  
Quant Title : 8080.M  
QLast Update : Wed May 25 02:05:34 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

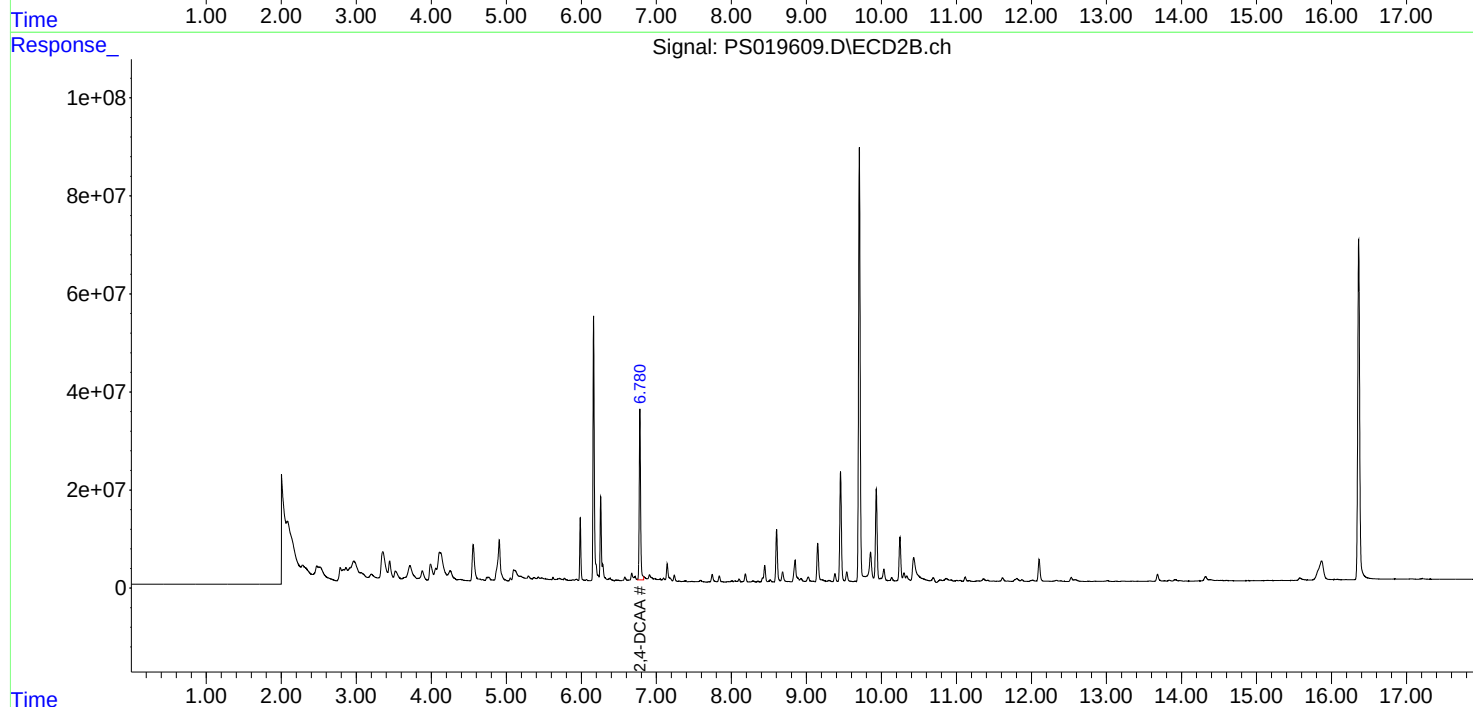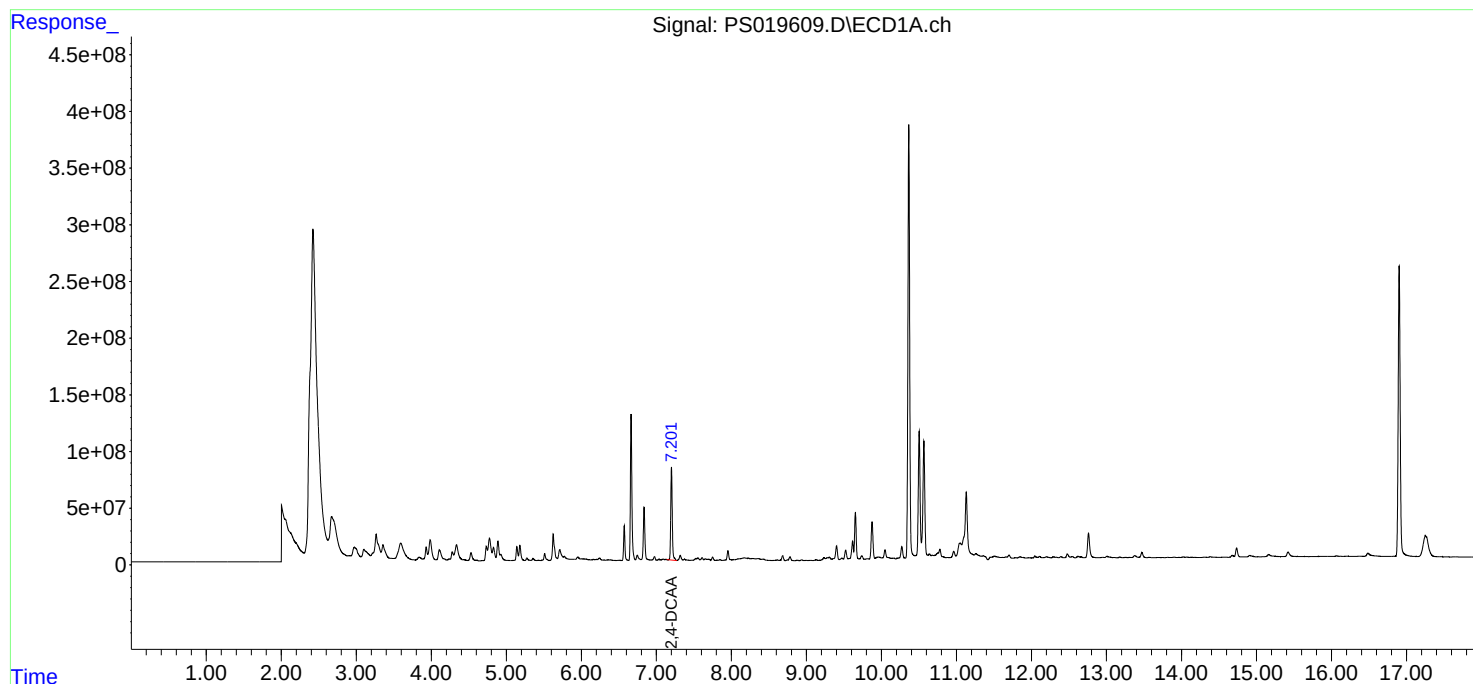

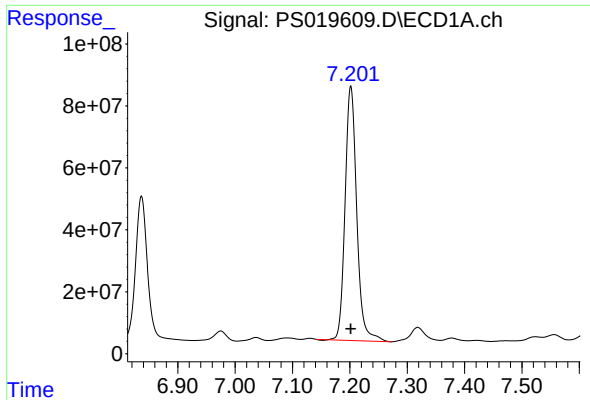


#4 2,4-DCAA

R.T.: 7.202 min  
Delta R.T.: 0.000 min  
Response: 1154017763  
Conc: 481.01 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
20220427-SPLP-AMENDED-SB-8-(DISCRETE-COMP-G)

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 06/04/2022  
Supervised By :Ankita Jodhani 06/06/2022

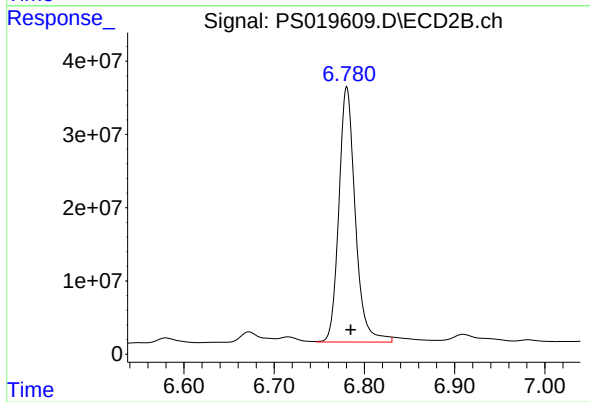

#4 2,4-DCAA

R.T.: 6.780 min  
Delta R.T.: -0.005 min  
Response: 440400726  
Conc: 568.35 ng/ml m