

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060519\
 Data File : PS004929.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2019 08:21
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 01:00:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	4.938	0.000	270.9E6	0	157.101	N.D. #
5) T	DICAMBA	0.000	5.437	0	188.4E6	N.D.	51.007
9) T	2,4-D	6.615	0.000	219.9E6	0	160.789	N.D. #
12) T	2,4,5-T	7.679	7.387	18260969	67218204	2.452	15.082 #
15) T	Picloram	9.137	9.096	296.1E6	152.4E6	28.414	20.425 #
16) T	DCPA	0.000	9.096	0	152.4E6	N.D.	23.523



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060519\
Data File : PS004929.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2019 08:21
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 01:00:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

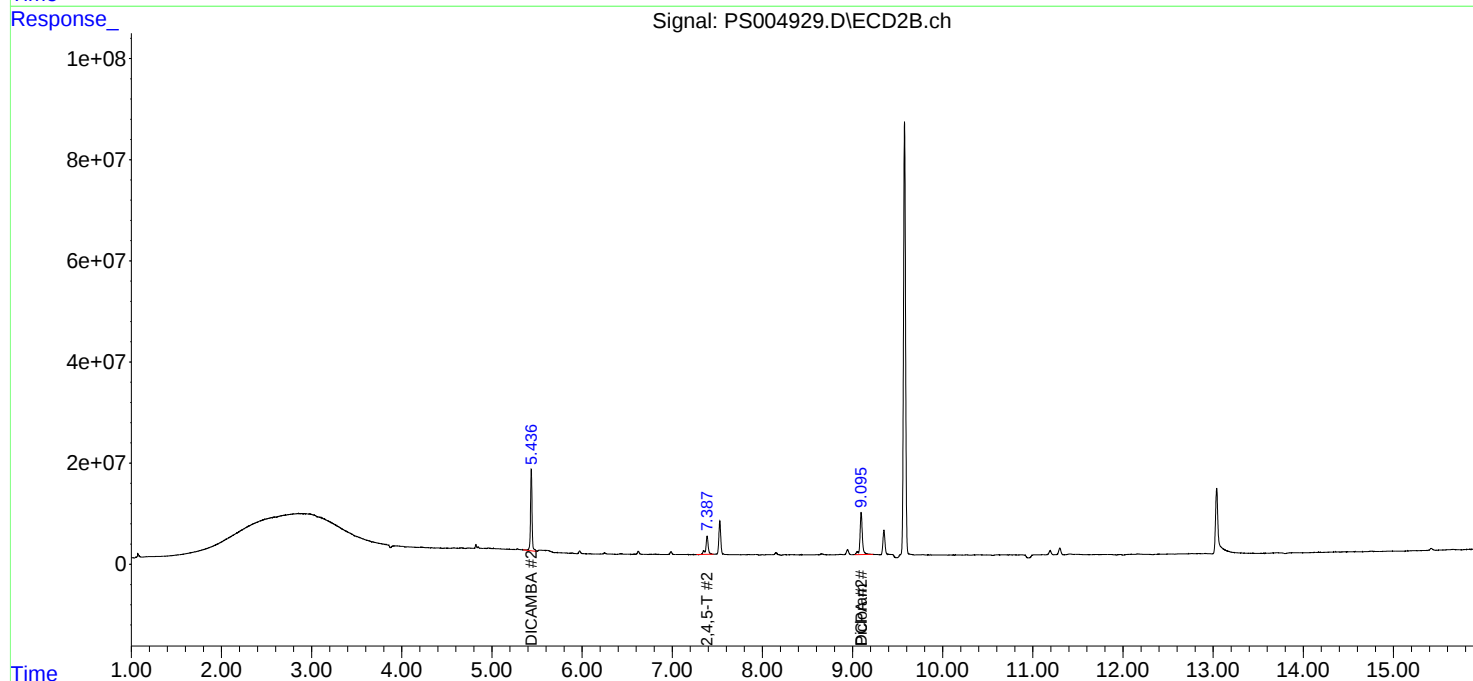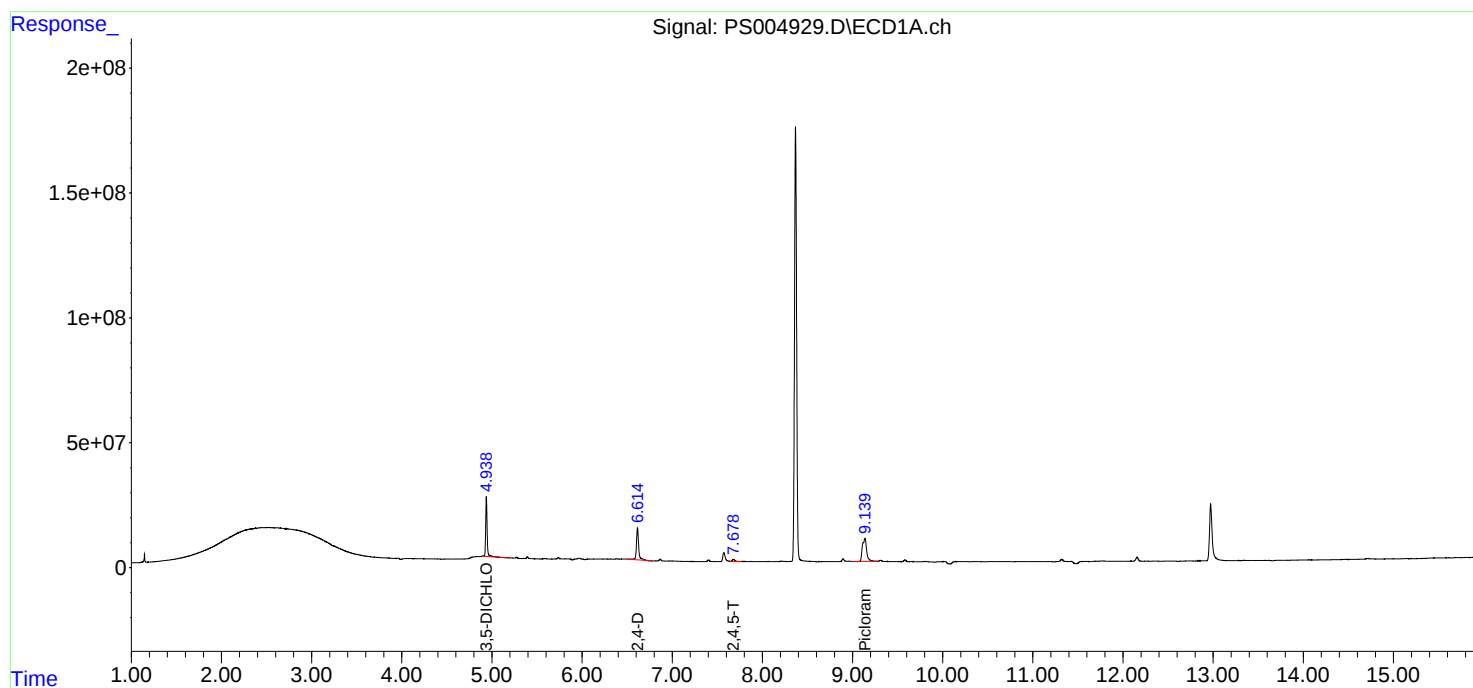


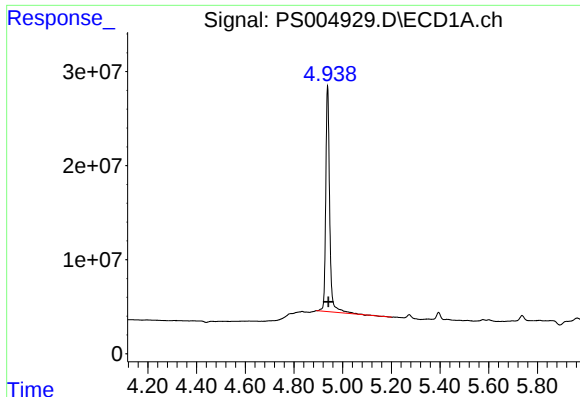

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.938 min
Delta R.T.: -0.004 min
Response: 270931586
Conc: 157.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

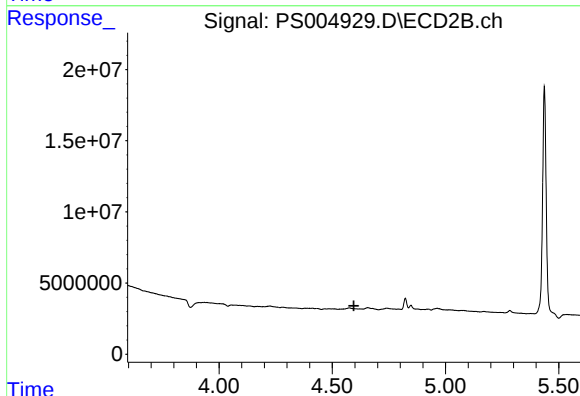


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

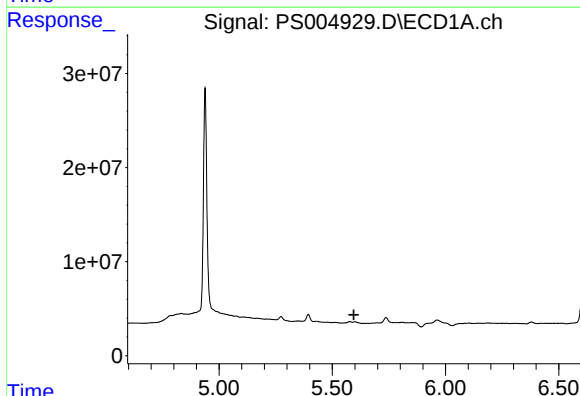


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.595 min
Response: 0
Conc: N.D.

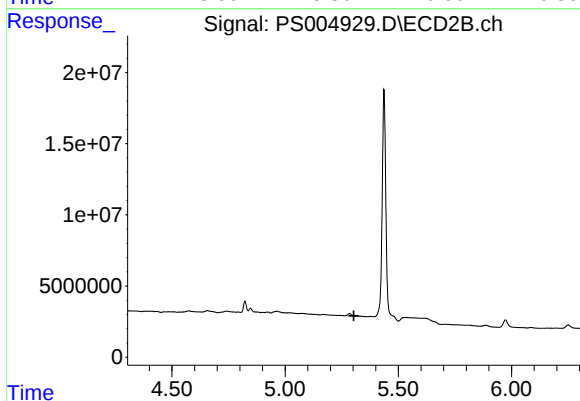

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.304 min
Response: 0
Conc: N.D.

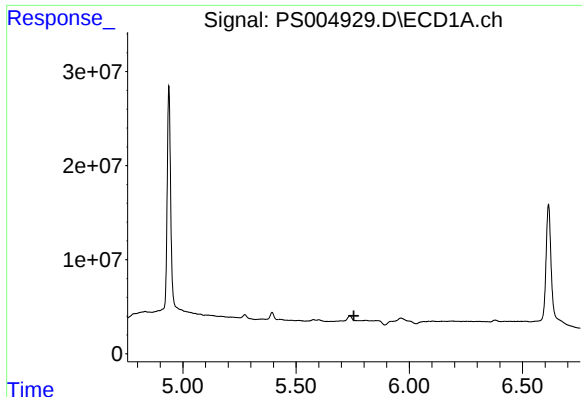

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

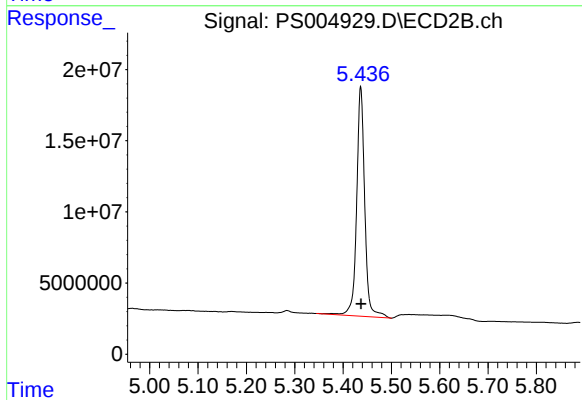


#5 DICAMBA

R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 188430990
Conc: 51.01 ng/ml

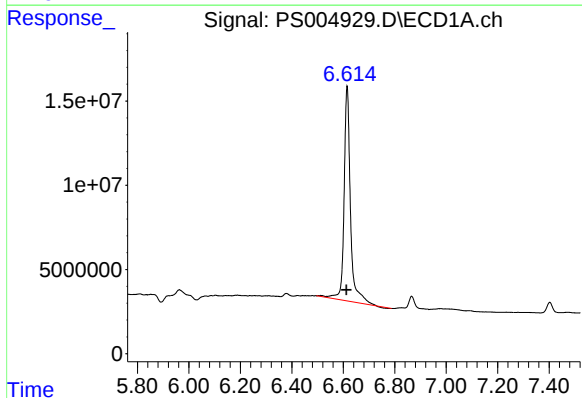


#9 2,4-D

R.T.: 6.615 min
Delta R.T.: 0.003 min
Response: 219945145
Conc: 160.79 ng/ml

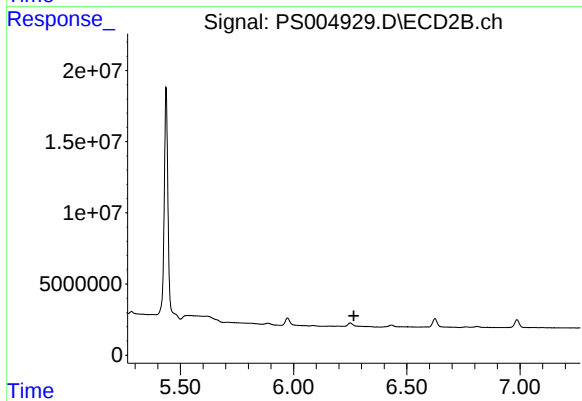

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

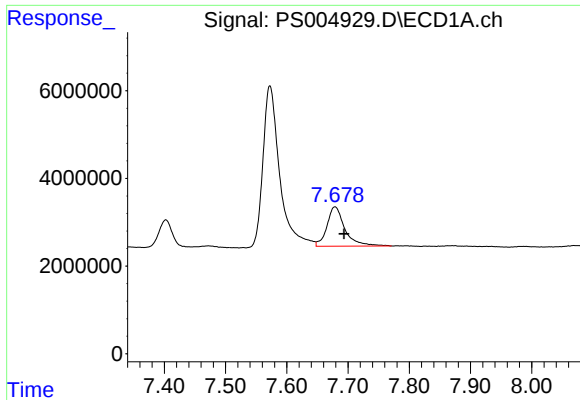

#12 2,4,5-T


R.T.: 7.679 min
Delta R.T.: -0.014 min
Response: 18260969
Conc: 2.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

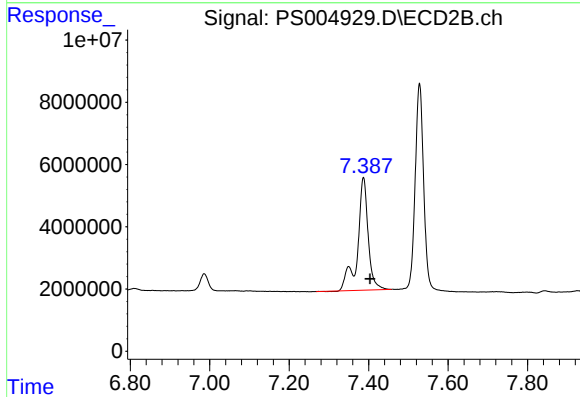


#12 2,4,5-T

R.T.: 7.387 min
Delta R.T.: -0.017 min
Response: 67218204
Conc: 15.08 ng/ml

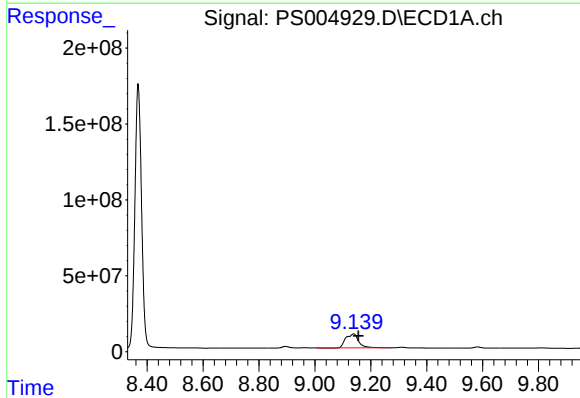


#15 Picloram

R.T.: 9.137 min
Delta R.T.: -0.018 min
Response: 296074383
Conc: 28.41 ng/ml

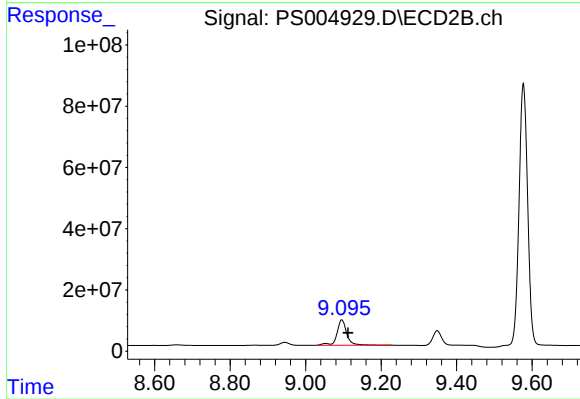

#15 Picloram


R.T.: 9.096 min
Delta R.T.: -0.017 min
Response: 152381553
Conc: 20.43 ng/ml

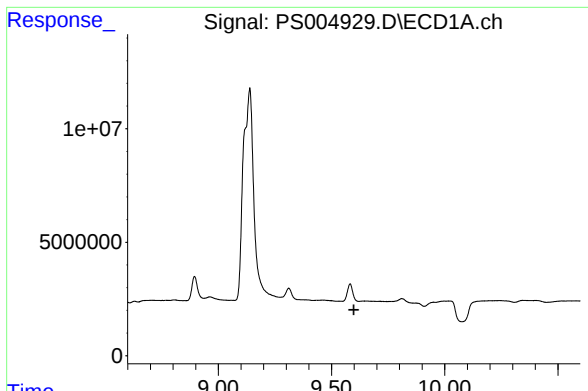

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

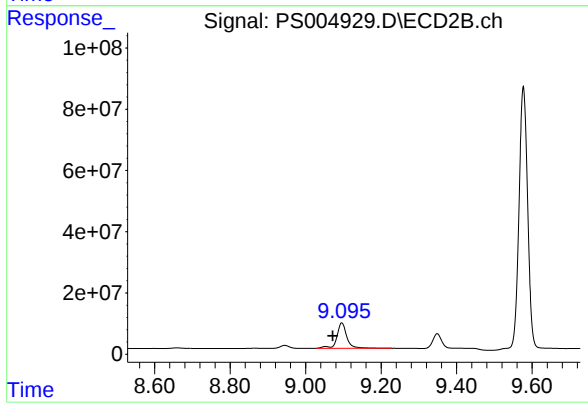

#16 DCPA

R.T.: 9.096 min
Delta R.T.: 0.024 min
Response: 152381553
Conc: 23.52 ng/ml