

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060519\
 Data File : PS004930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2019 12:34
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 01:00:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.593	5.284	800.1E6	567.0E6	570.811	587.647
Target Compounds							
2) T	3,5-DICHL...	4.957	0.000	57236103	0	33.189	N.D. #
3) T	4-Nitroph...	5.412	0.000	14268653	0	22.885	N.D. #
5) T	DICAMBA	5.754	5.438	12279940	54170093	2.313	14.663 #
8) T	DICHLORPROP	0.000	5.974	0	32846004	N.D.	34.838
9) T	2,4-D	6.634	0.000	135.0E6	0	98.667	N.D. #
10) T	Pentachlo...	6.892	0.000	28406751	0	1.618	N.D. #
12) T	2,4,5-T	7.698	7.388	20151922	66914172	2.706	15.014 #
15) T	Picloram	9.132	9.097	1156.3E6	178.3E6	110.968	23.899 #
16) T	DCPA	0.000	9.097	0	178.3E6	N.D.	27.523



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060519\
Data File : PS004930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2019 12:34
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 01:00:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

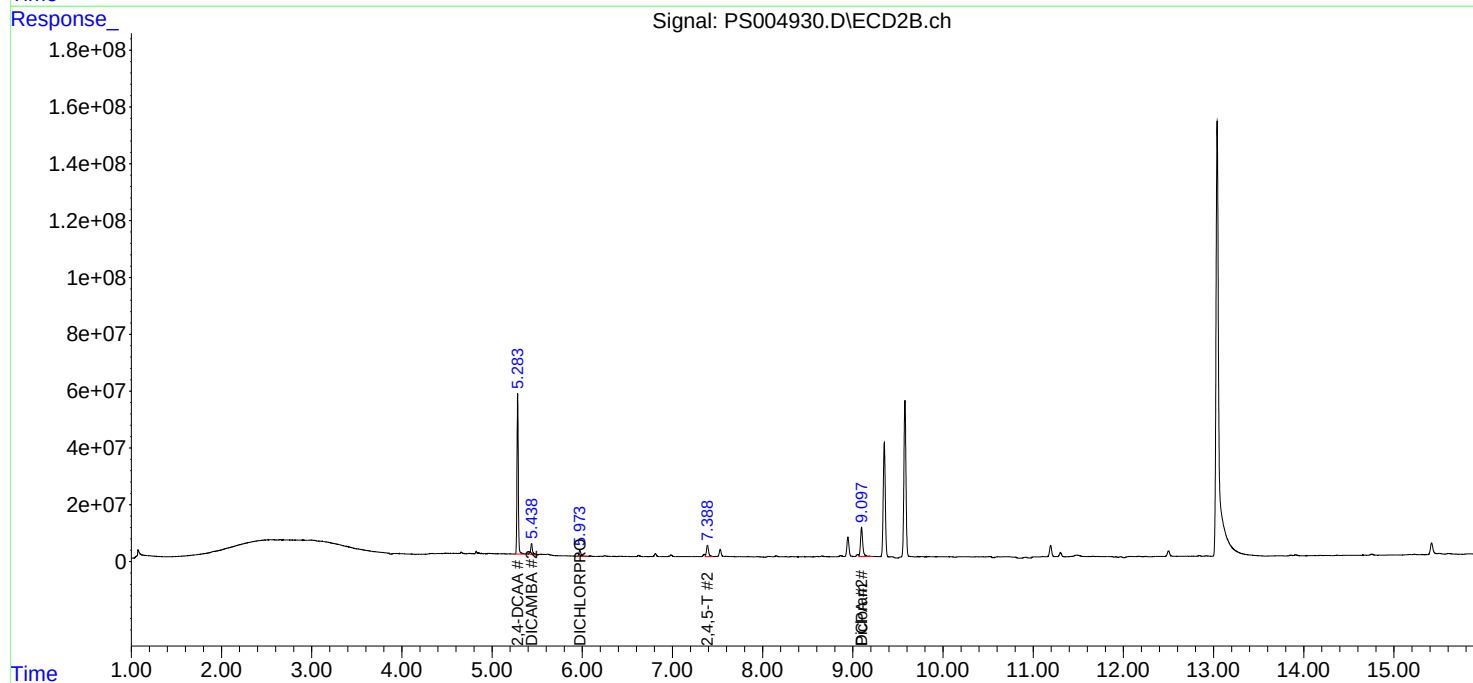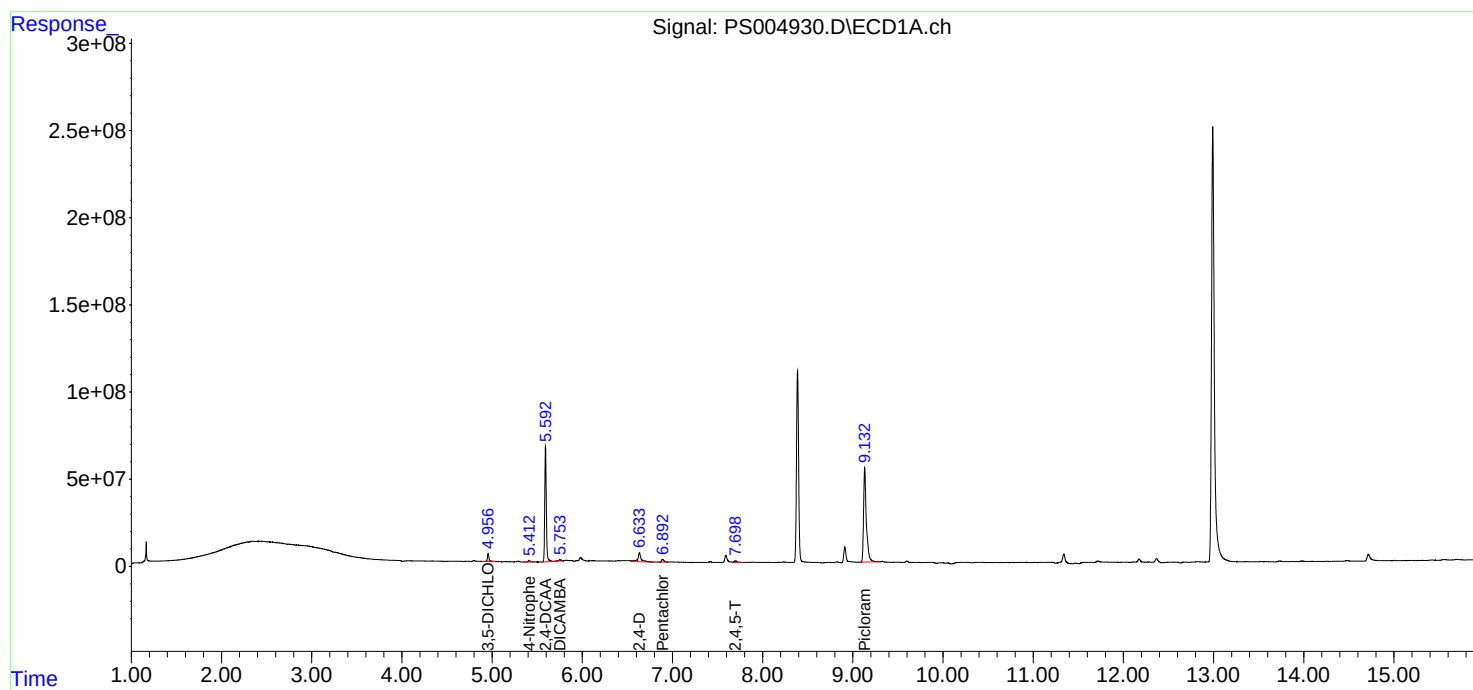


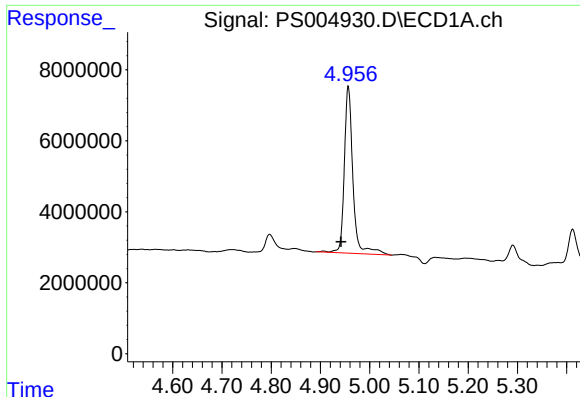

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.957 min
Delta R.T.: 0.015 min
Response: 57236103
Conc: 33.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

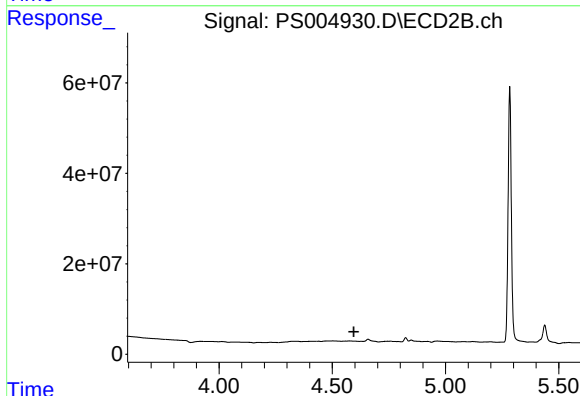


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

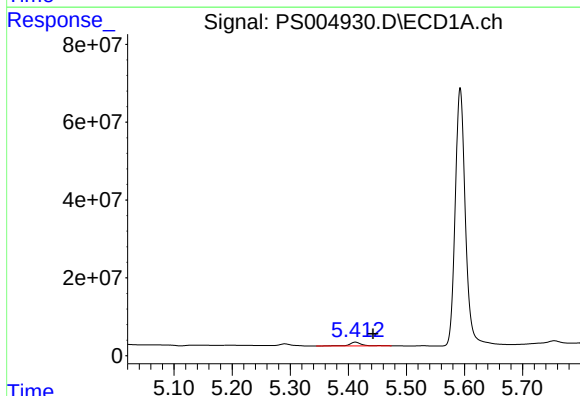


#3 4-Nitrophenol

R.T.: 5.412 min
Delta R.T.: -0.031 min
Response: 14268653
Conc: 22.88 ng/ml

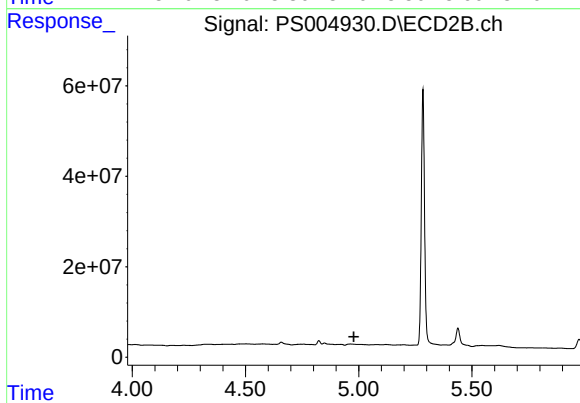

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

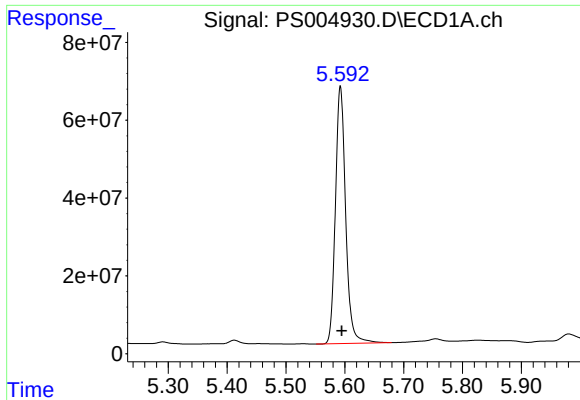

#4 2,4-DCAA


R.T.: 5.593 min
Delta R.T.: -0.003 min
Response: 800137255
Conc: 570.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

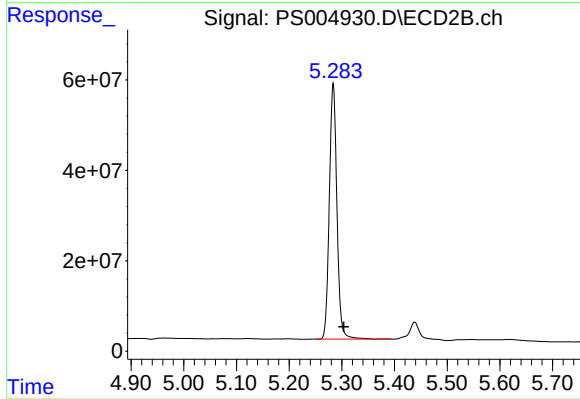


#4 2,4-DCAA

R.T.: 5.284 min
Delta R.T.: -0.020 min
Response: 566983136
Conc: 587.65 ng/ml

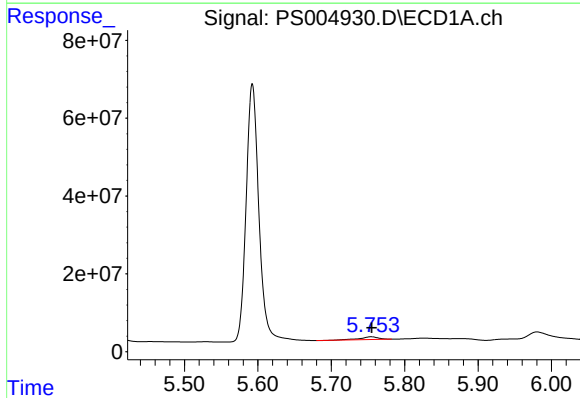


#5 DICAMBA

R.T.: 5.754 min
Delta R.T.: 0.000 min
Response: 12279940
Conc: 2.31 ng/ml

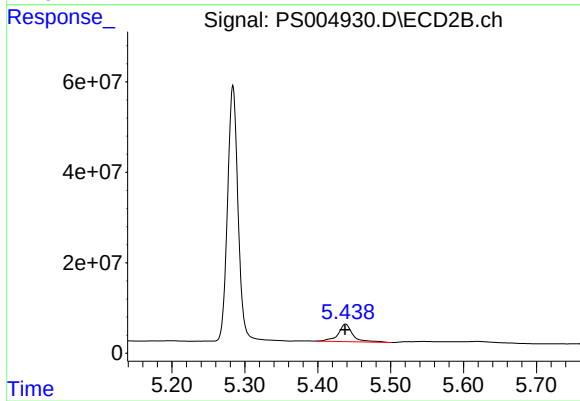

#5 DICAMBA


R.T.: 5.438 min
Delta R.T.: 0.000 min
Response: 54170093
Conc: 14.66 ng/ml

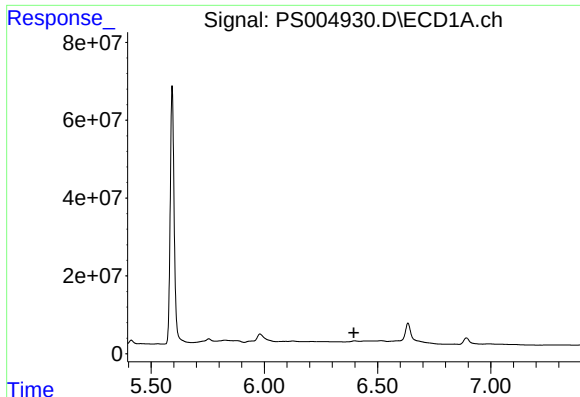

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

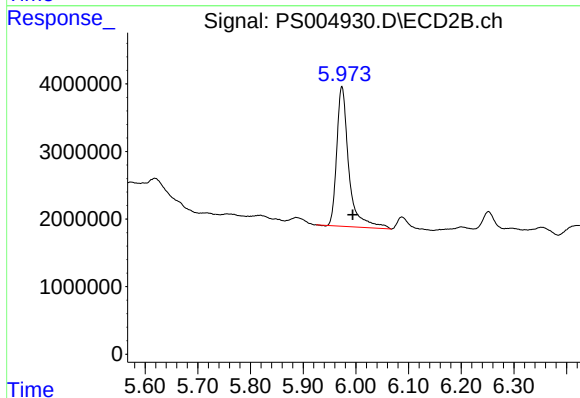


#8 DICHLORPROP

R.T.: 5.974 min
Delta R.T.: -0.021 min
Response: 32846004
Conc: 34.84 ng/ml

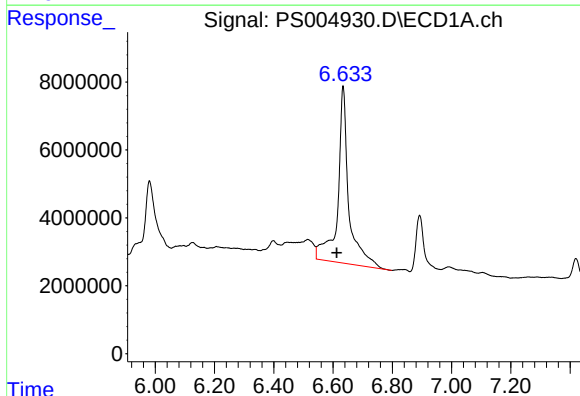


#9 2,4-D

R.T.: 6.634 min
Delta R.T.: 0.022 min
Response: 134967304
Conc: 98.67 ng/ml

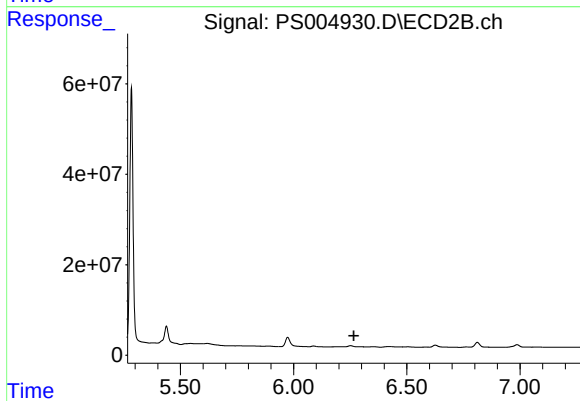

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

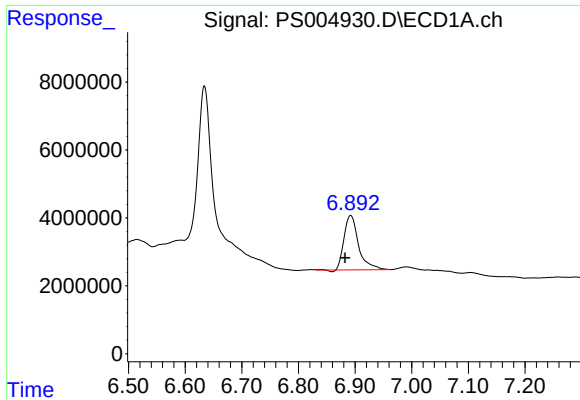

#10 Pentachlorophenol


R.T.: 6.892 min
Delta R.T.: 0.010 min
Response: 28406751
Conc: 1.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

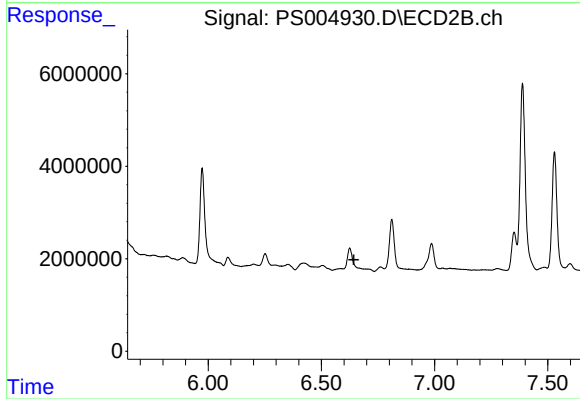


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.644 min
Response: 0
Conc: N.D.

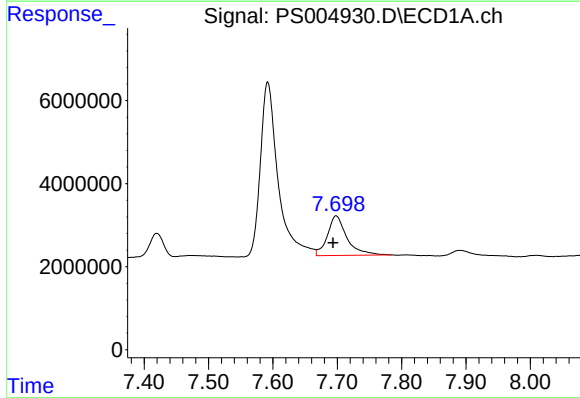


#12 2,4,5-T

R.T.: 7.698 min
Delta R.T.: 0.005 min
Response: 20151922
Conc: 2.71 ng/ml

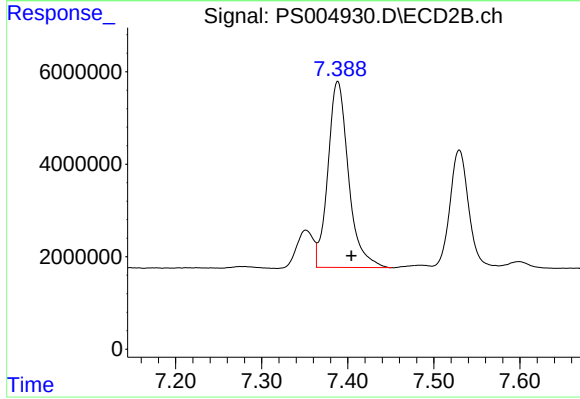

#12 2,4,5-T


R.T.: 7.388 min
Delta R.T.: -0.016 min
Response: 66914172
Conc: 15.01 ng/ml

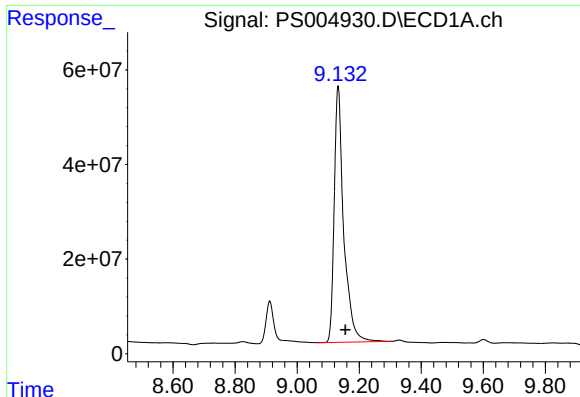

#15 Picloram


R.T.: 9.132 min
Delta R.T.: -0.023 min
Response: 1156290313
Conc: 110.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

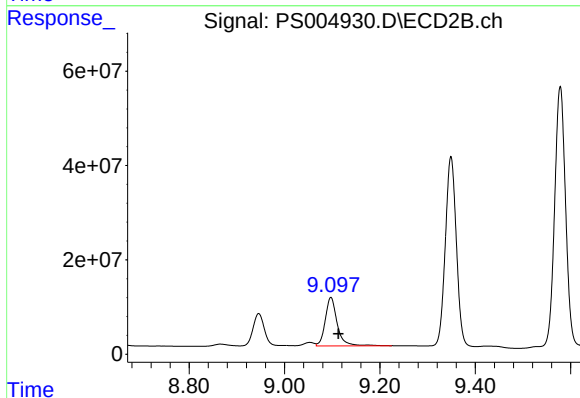


#15 Picloram

R.T.: 9.097 min
Delta R.T.: -0.016 min
Response: 178297167
Conc: 23.90 ng/ml

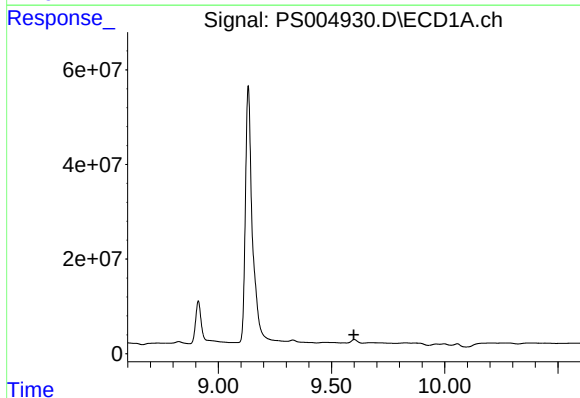

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.599 min
Response: 0
Conc: N.D.

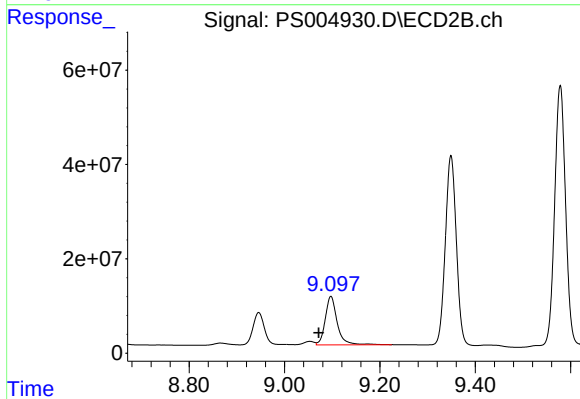

#16 DCPA

R.T.: 9.097 min
Delta R.T.: 0.025 min
Response: 178297167
Conc: 27.52 ng/ml