

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060619\
 Data File : PS004942.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2019 11:35
 Operator : SM\AJ
 Sample : K2638-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 03:37:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.578	5.290	476.6E6	333.7E6	339.995	345.912
Target Compounds							
2) T	3,5-DICHL...	0.000	4.608	0	239.8E6	N.D.	194.602
5) T	DICAMBA	0.000	5.396	0	17412768	N.D.	4.714
6) T	MCP	5.933	0.000	5255540	0	1.262	N.D. #
7) T	MCPA	0.000	5.751	0	192.3E6	N.D.	46.989
8) T	DICHLORPROP	0.000	5.979	0	29614218	N.D.	31.410
9) T	2,4-D	6.665	0.000	25614681	0	18.725	N.D. #
11) T	2,4,5-TP ...	0.000	6.946	0	150.9E6	N.D.	29.328



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060619\
Data File : PS004942.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2019 11:35
Operator : SM\AJ
Sample : K2638-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 03:37:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

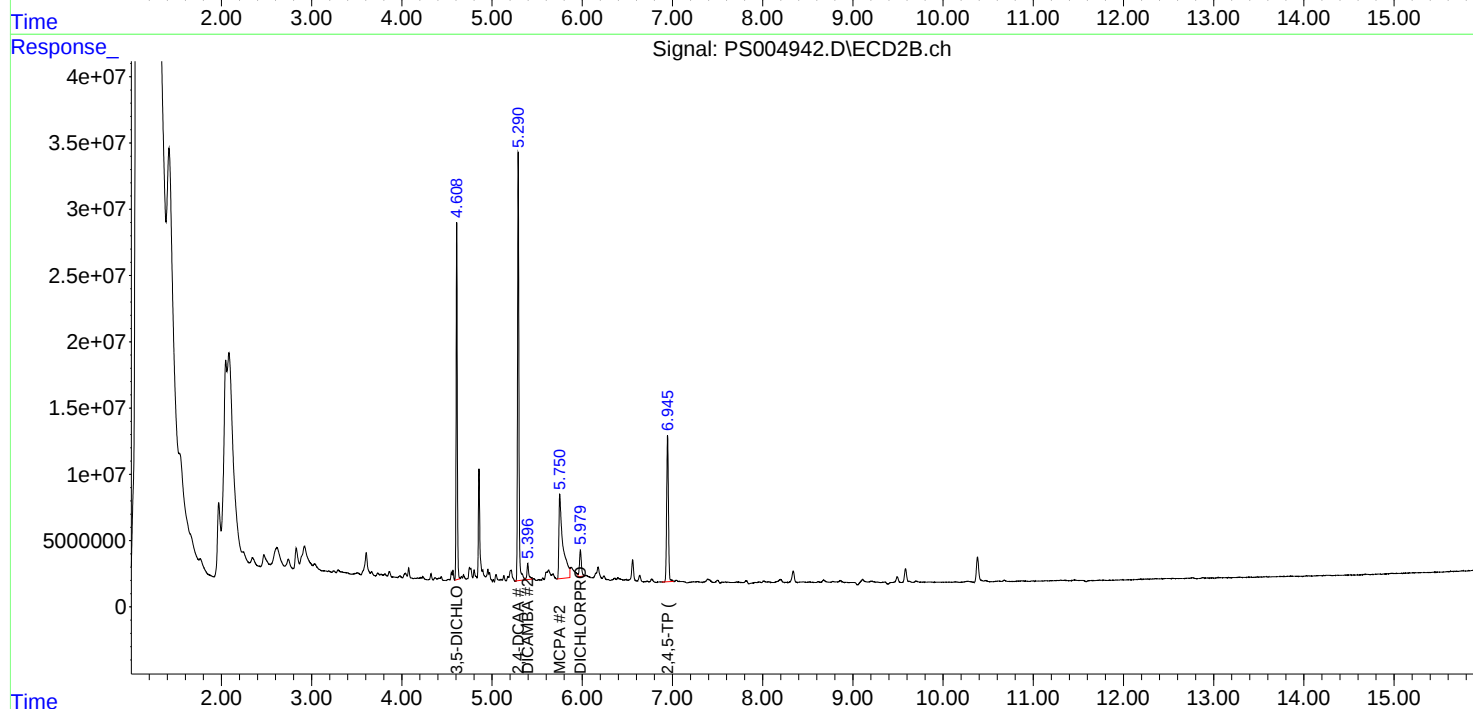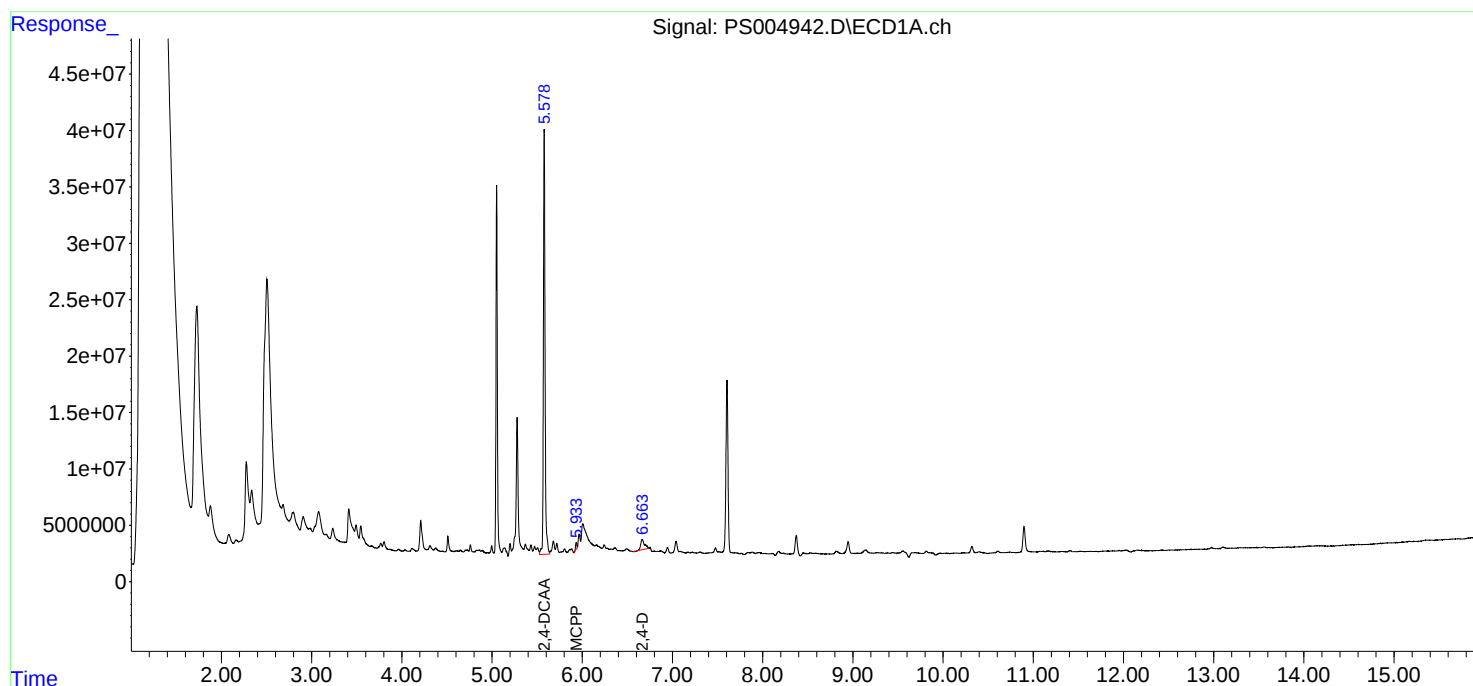


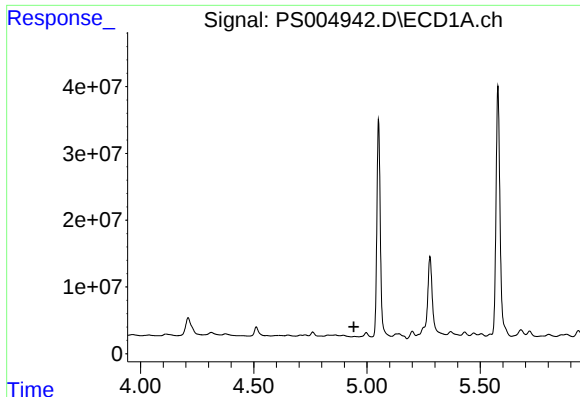

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

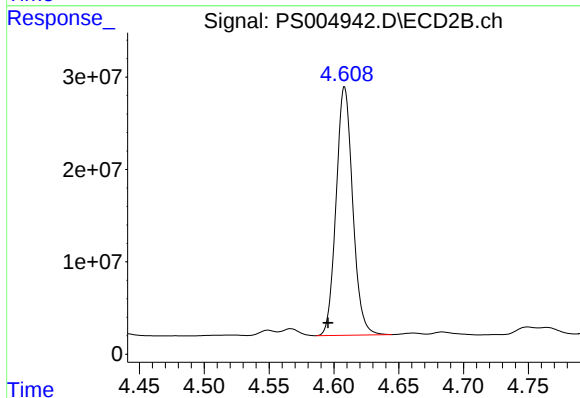


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.608 min
Delta R.T.: 0.013 min
Response: 239774901
Conc: 194.60 ng/ml

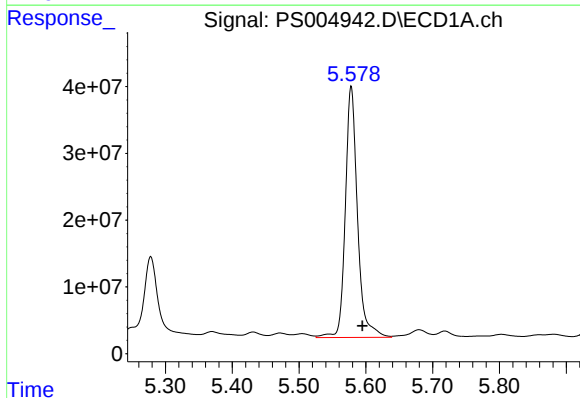


#4 2,4-DCAA

R.T.: 5.578 min
Delta R.T.: -0.017 min
Response: 476590552
Conc: 340.00 ng/ml

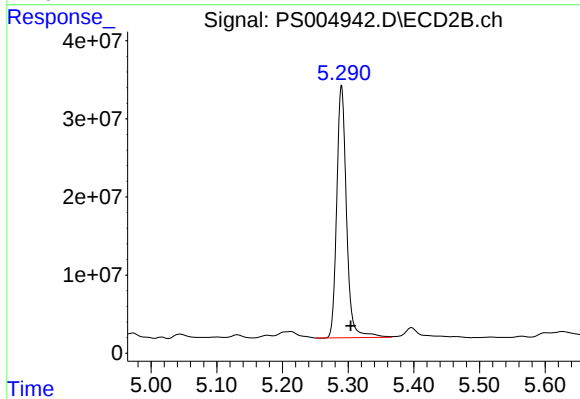

#4 2,4-DCAA


R.T.: 5.290 min
Delta R.T.: -0.014 min
Response: 333748166
Conc: 345.91 ng/ml

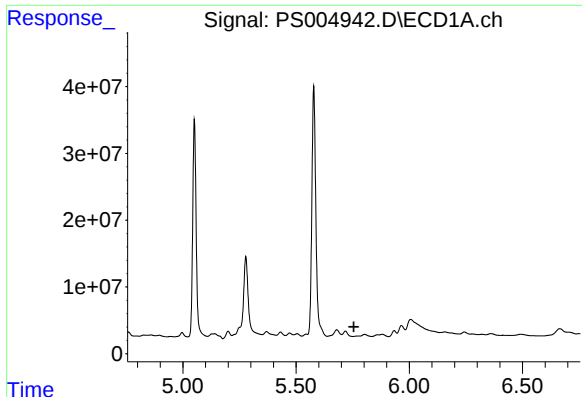

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

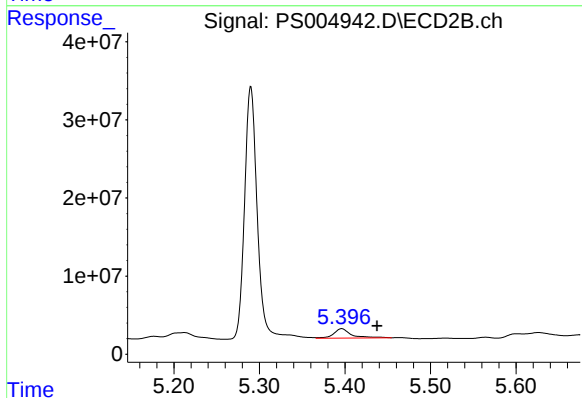


#5 DICAMBA

R.T.: 5.396 min
Delta R.T.: -0.041 min
Response: 17412768
Conc: 4.71 ng/ml

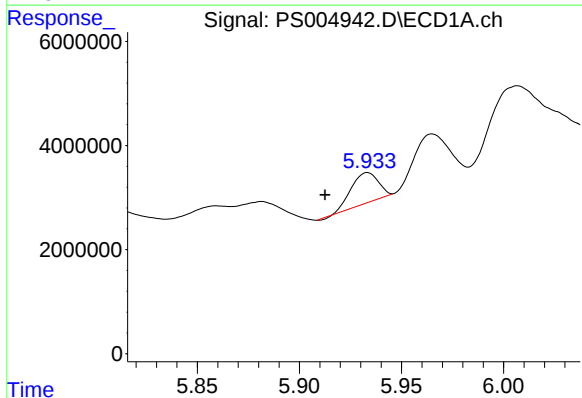


#6 MCP

R.T.: 5.933 min
Delta R.T.: 0.021 min
Response: 5255540
Conc: 1.26 ug/ml

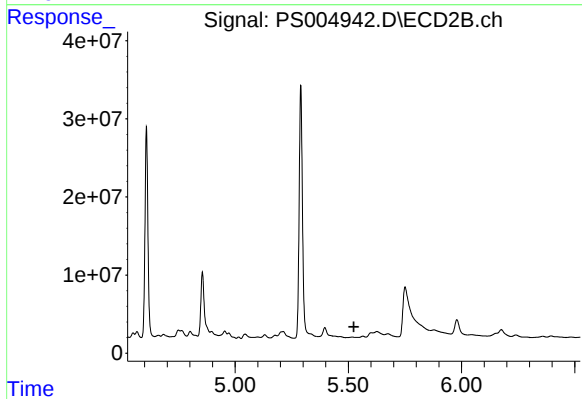

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

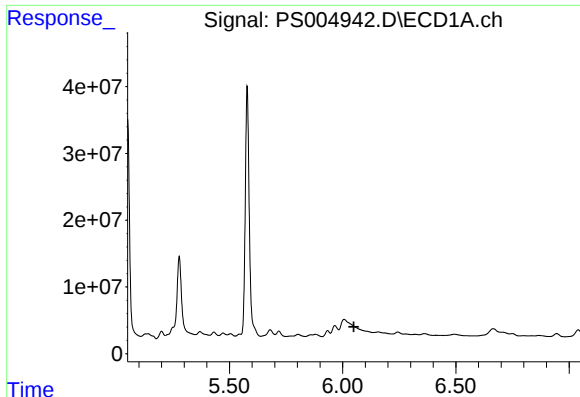

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

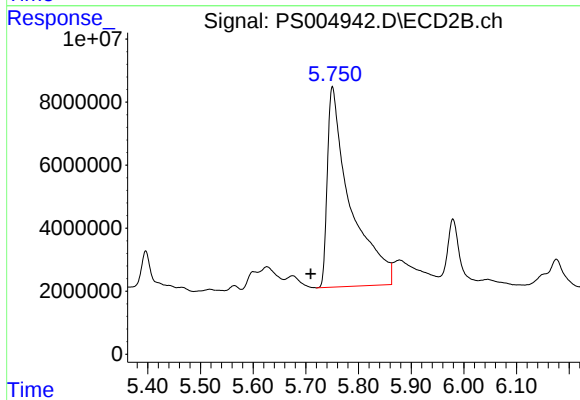


#7 MCPA

R.T.: 5.751 min
Delta R.T.: 0.042 min
Response: 192260666
Conc: 46.99 ug/ml

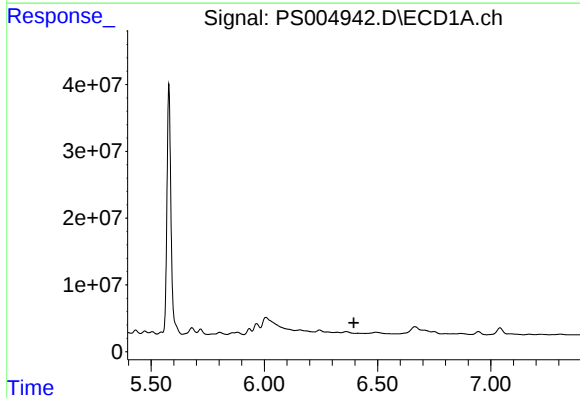


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

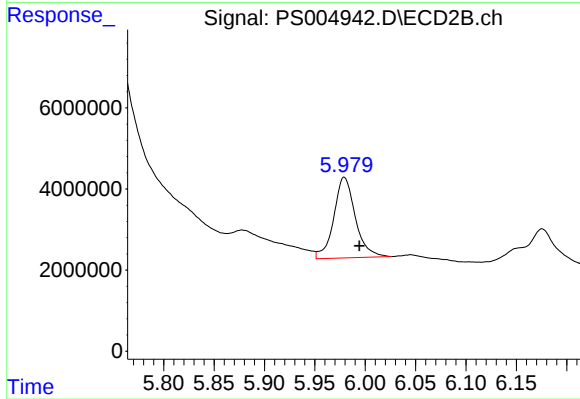

#8 DICHLORPROP


R.T.: 5.979 min
Delta R.T.: -0.015 min
Response: 29614218
Conc: 31.41 ng/ml

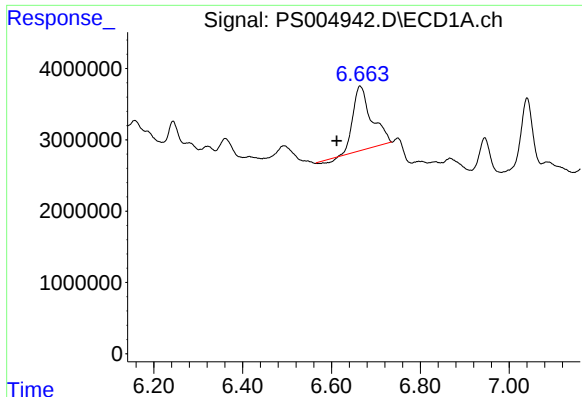

#9 2,4-D


R.T.: 6.665 min
Delta R.T.: 0.053 min
Response: 25614681
Conc: 18.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

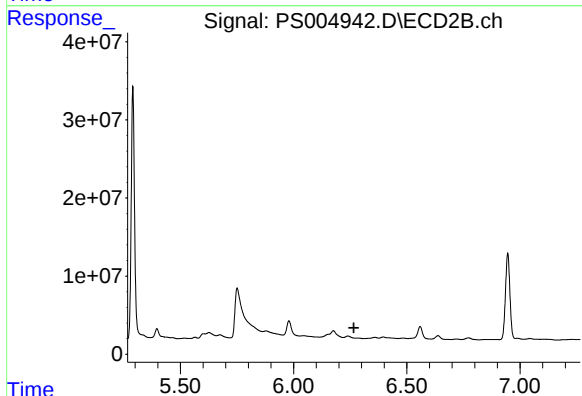


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

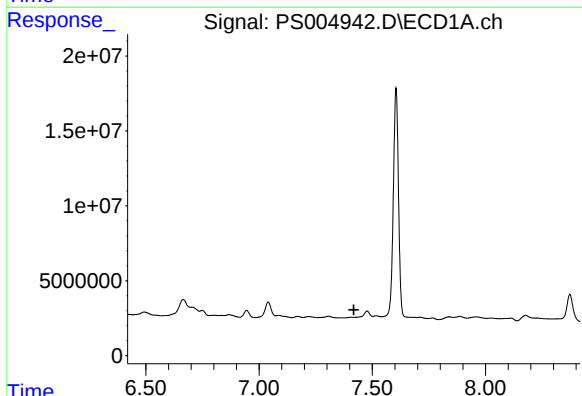

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

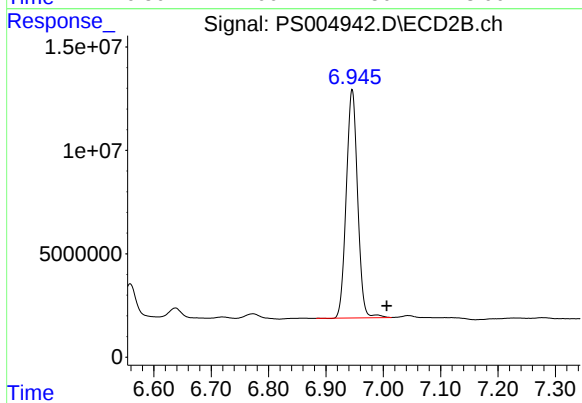

#11 2,4,5-TP (SILVEX)

R.T.: 6.946 min
Delta R.T.: -0.061 min
Response: 150903161
Conc: 29.33 ng/ml