

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060619\
 Data File : PS004948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2019 13:47
 Operator : SM\AJ
 Sample : K3151-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 03:39:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.572	5.285	422.0E6	292.8E6	301.022	303.490
Target Compounds							
2) T	3,5-DICHL...	0.000	4.603	0	218.8E6	N.D.	177.575
5) T	DICAMBA	0.000	5.391	0	12313903	N.D.	3.333
7) T	MCPA	5.990	5.738	11614432	432.7E6	2.005	105.760 #
8) T	DICHLORPROP	0.000	5.974	0	21572704	N.D.	22.881
9) T	2,4-D	6.659	0.000	27769978	0	20.301	N.D. #
11) T	2,4,5-TP ...	0.000	6.940	0	125.6E6	N.D.	24.415



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060619\
Data File : PS004948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2019 13:47
Operator : SM\AJ
Sample : K3151-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 03:39:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

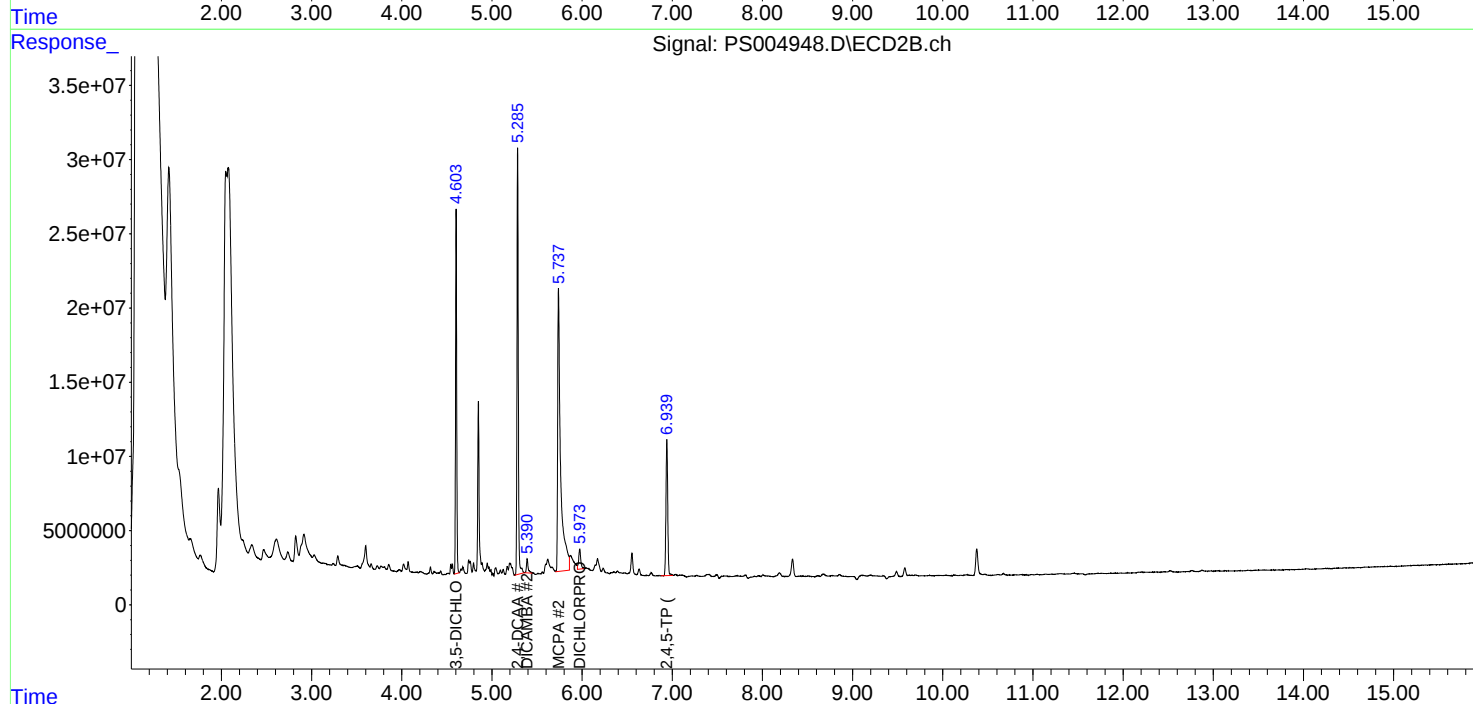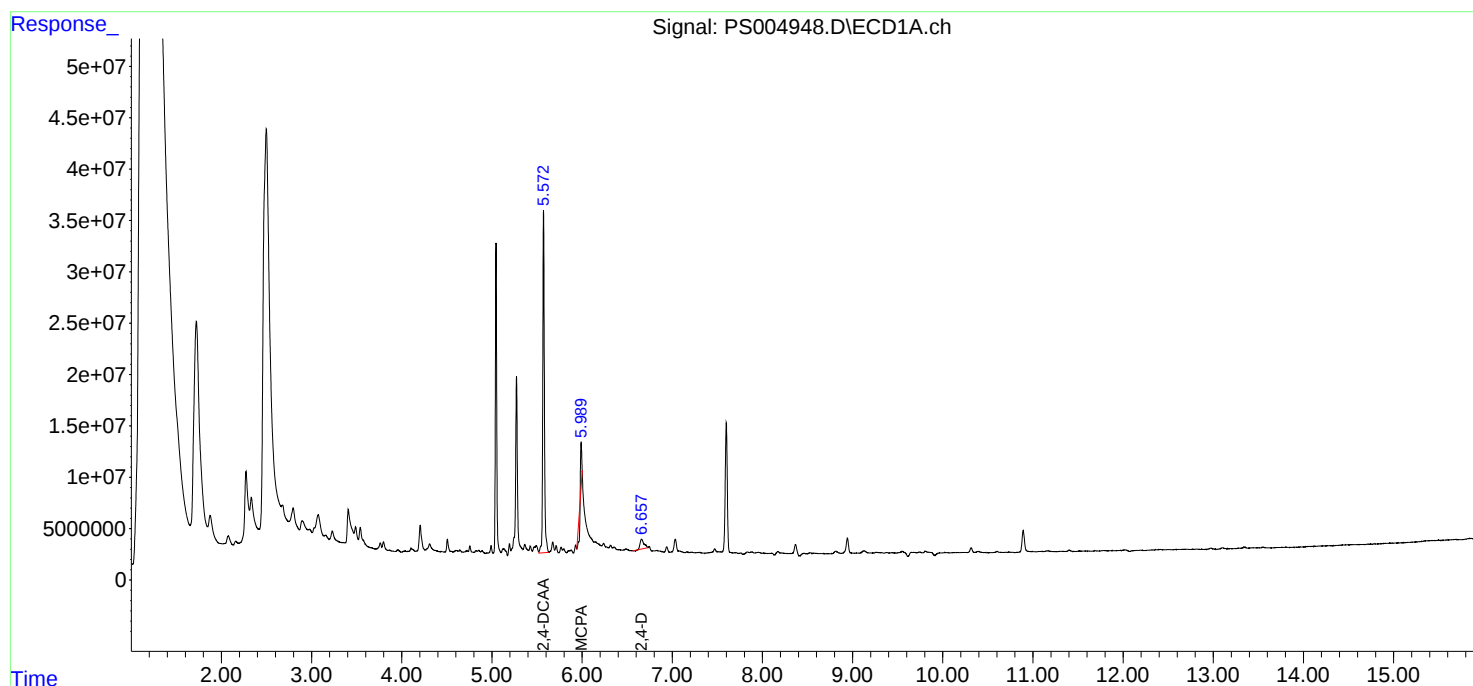


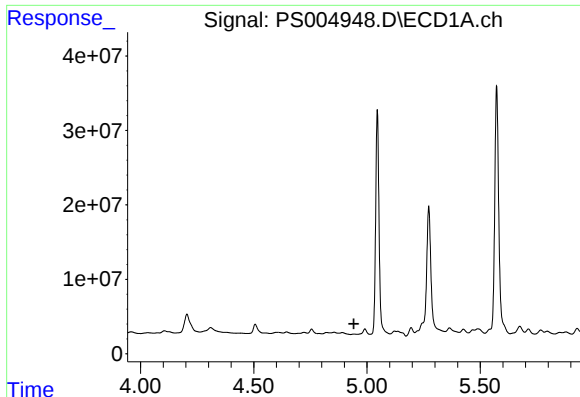

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

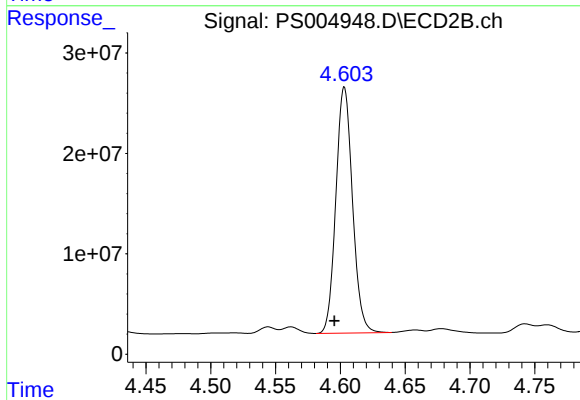


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.603 min
Delta R.T.: 0.008 min
Response: 218794655
Conc: 177.57 ng/ml

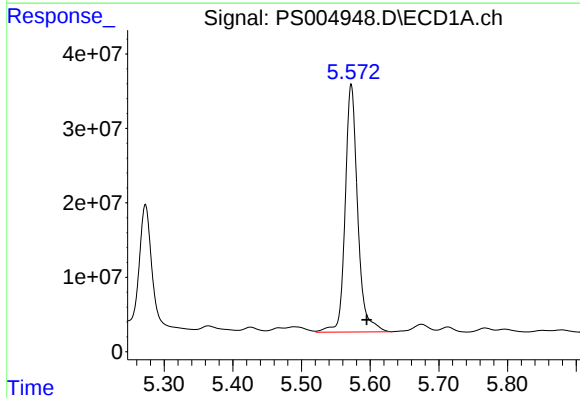


#4 2,4-DCAA

R.T.: 5.572 min
Delta R.T.: -0.023 min
Response: 421959915
Conc: 301.02 ng/ml

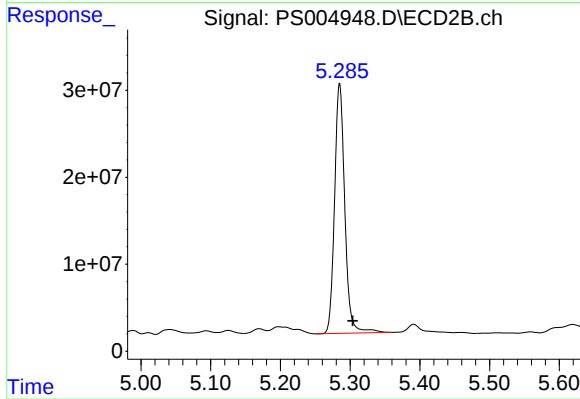

#4 2,4-DCAA


R.T.: 5.285 min
Delta R.T.: -0.019 min
Response: 292818529
Conc: 303.49 ng/ml

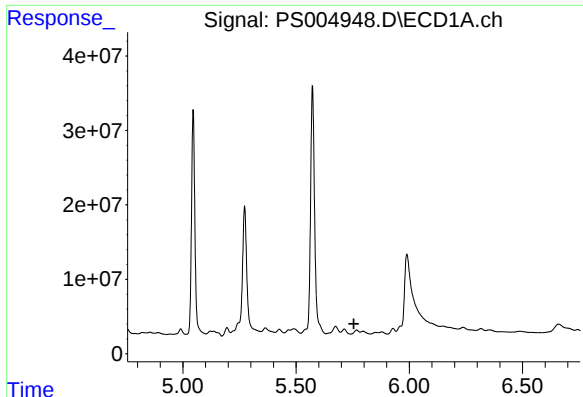

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

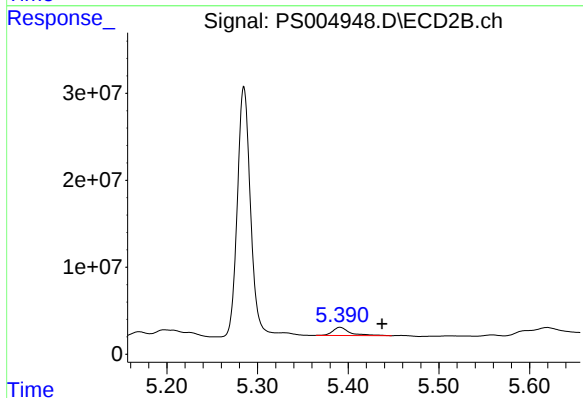


#5 DICAMBA

R.T.: 5.391 min
Delta R.T.: -0.046 min
Response: 12313903
Conc: 3.33 ng/ml

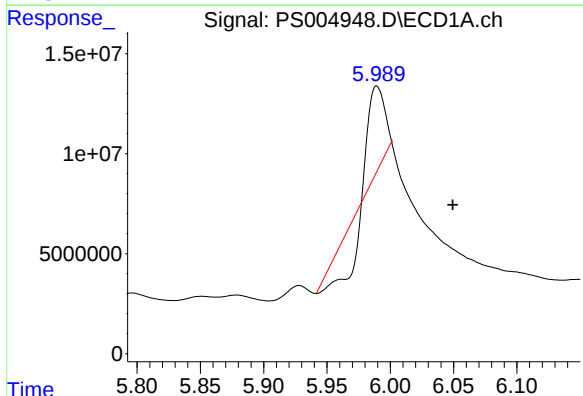


#7 MCPA

R.T.: 5.990 min
Delta R.T.: -0.059 min
Response: 11614432
Conc: 2.01 ug/ml

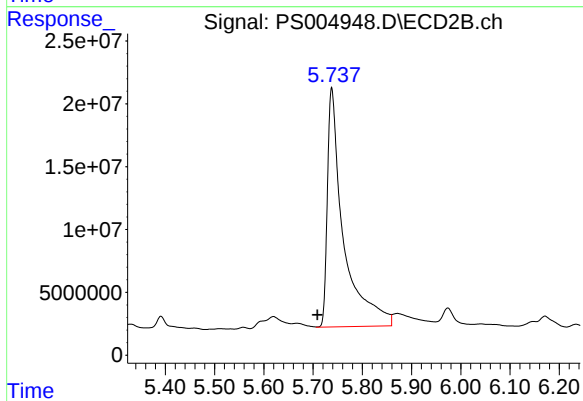

#7 MCPA


R.T.: 5.738 min
Delta R.T.: 0.029 min
Response: 432733318
Conc: 105.76 ug/ml

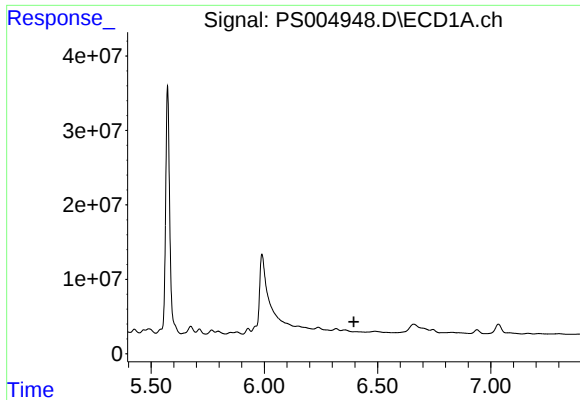

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

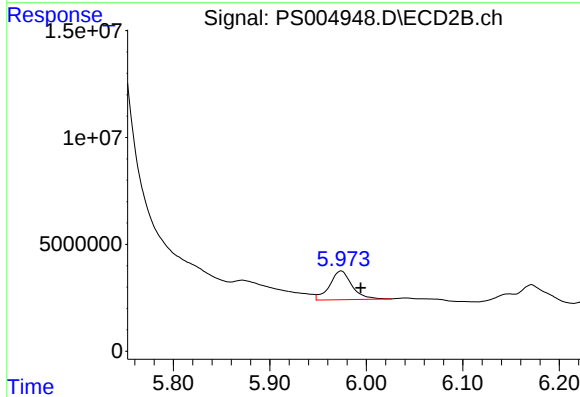


#8 DICHLORPROP

R.T.: 5.974 min
Delta R.T.: -0.021 min
Response: 21572704
Conc: 22.88 ng/ml

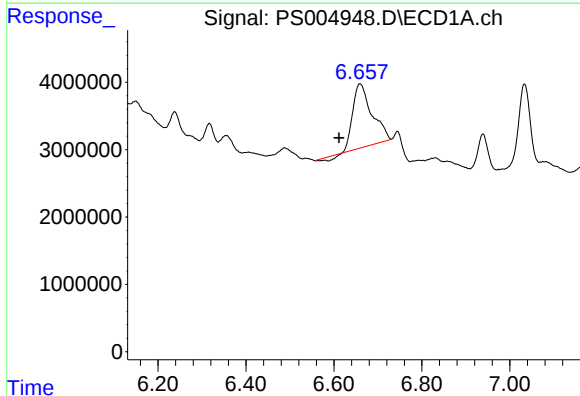


#9 2,4-D

R.T.: 6.659 min
Delta R.T.: 0.047 min
Response: 27769978
Conc: 20.30 ng/ml

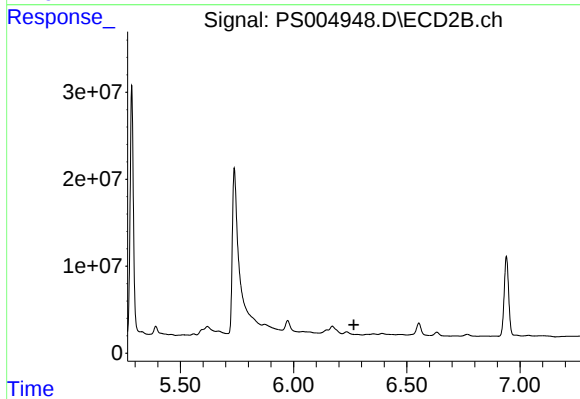

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

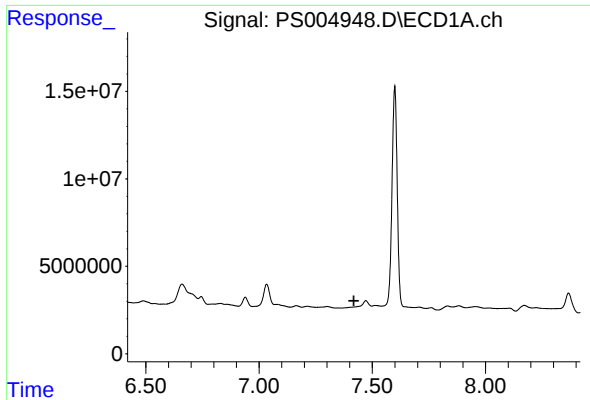

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min

Exp R.T.: 7.419 min

Response: 0

Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

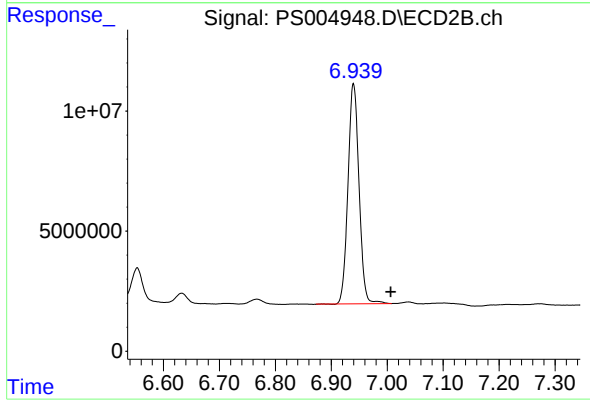

#11 2,4,5-TP (SILVEX)

R.T.: 6.940 min

Delta R.T.: -0.066 min

Response: 125623400

Conc: 24.42 ng/ml