

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060619\
 Data File : PS004960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2019 18:15
 Operator : SM\AJ
 Sample : K3183-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 03:45:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.572	5.284	422.9E6	269.8E6	301.678	279.594
Target Compounds							
2) T	3,5-DICHL...	0.000	4.602	0	290.9E6	N.D.	236.114
3) T	4-Nitroph...	5.373	0.000	47836667	0	76.722	N.D. #
5) T	DICAMBA	5.710	5.390	15224563	19360730	2.867	5.241 #
6) T	MCP	5.926	0.000	11867981	0	2.851	N.D. #
7) T	MCPA	6.066	5.676	26162644	26841592	4.517	6.560 #
8) T	DICHLORPROP	0.000	5.974	0	16284956	N.D.	17.272
9) T	2,4-D	6.659	0.000	9713383	0	7.101	N.D. #
11) T	2,4,5-TP ...	0.000	6.940	0	168.1E6	N.D.	32.669
13) T	2,4-DB	8.223	0.000	130.9E6	0	135.526	N.D. #
14) T	DINOSEB	0.000	8.149	0	61176376	N.D.	15.914



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060619\
Data File : PS004960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2019 18:15
Operator : SM\AJ
Sample : K3183-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 03:45:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

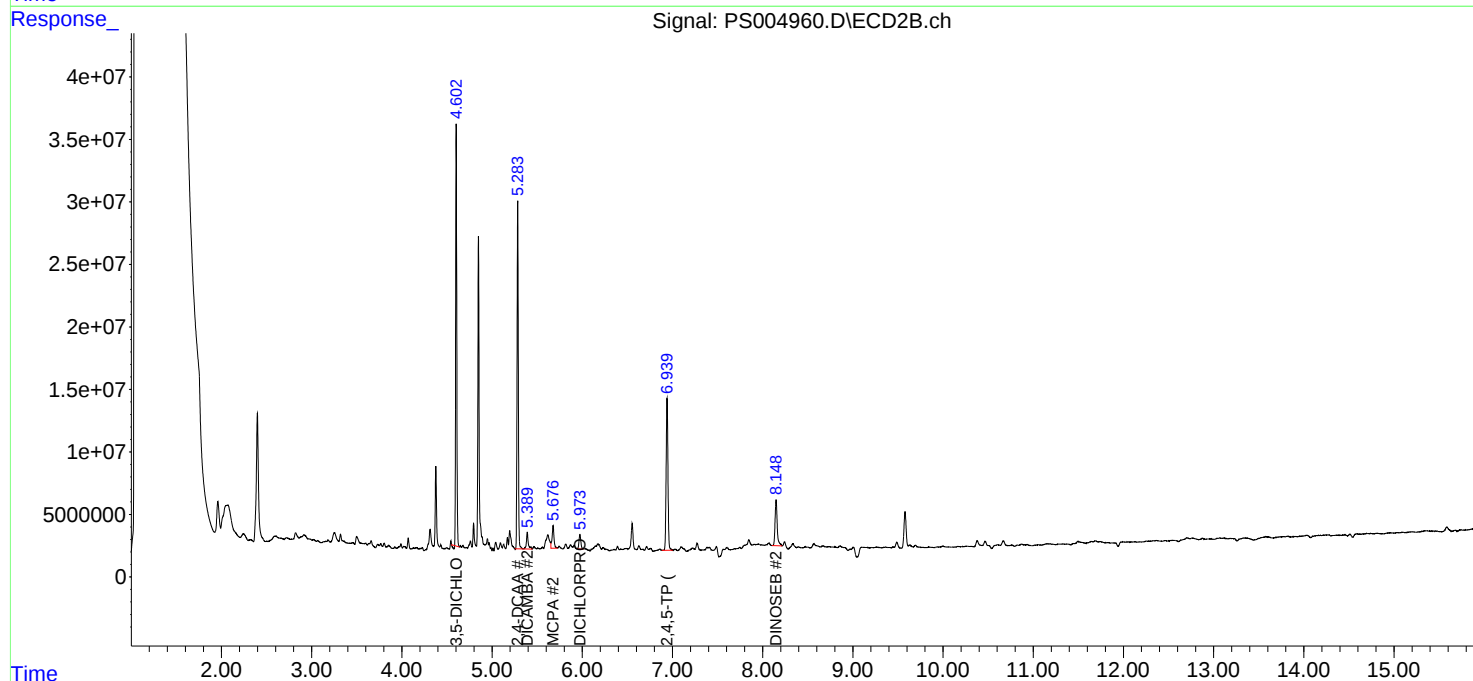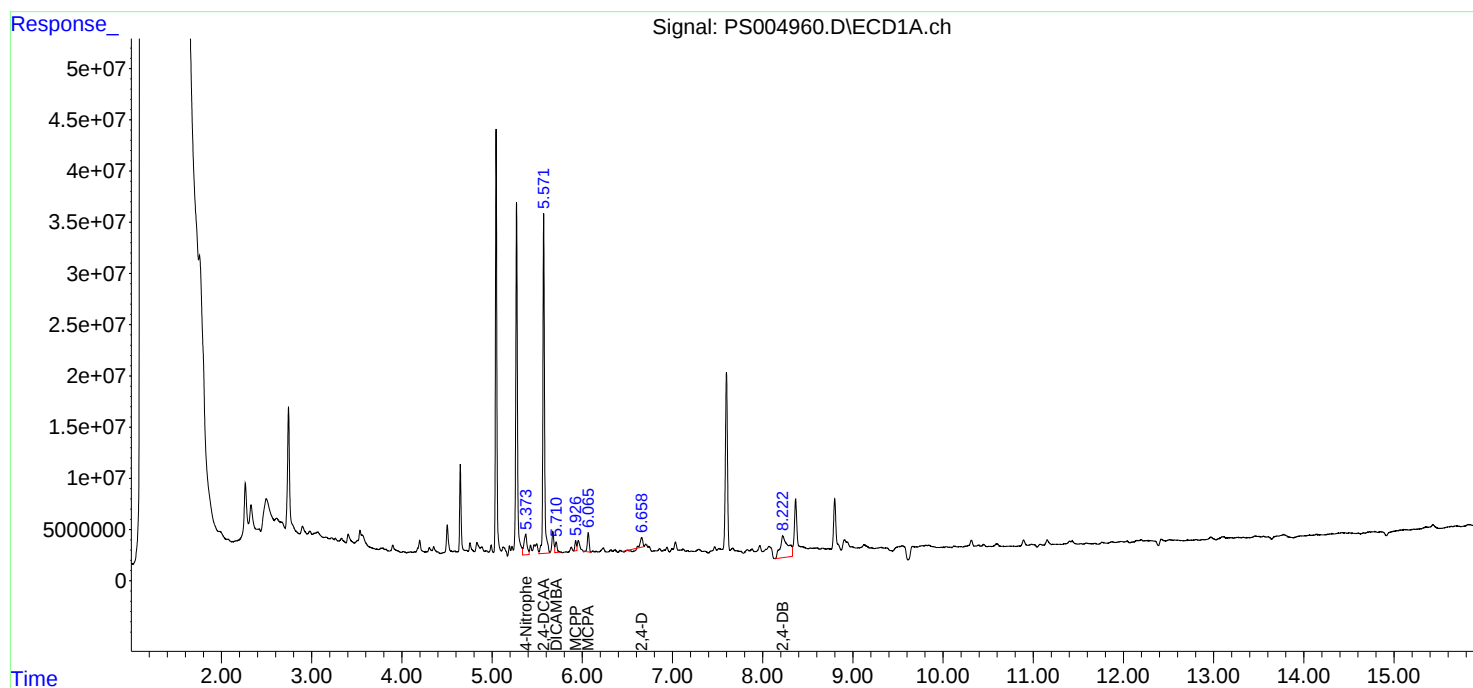


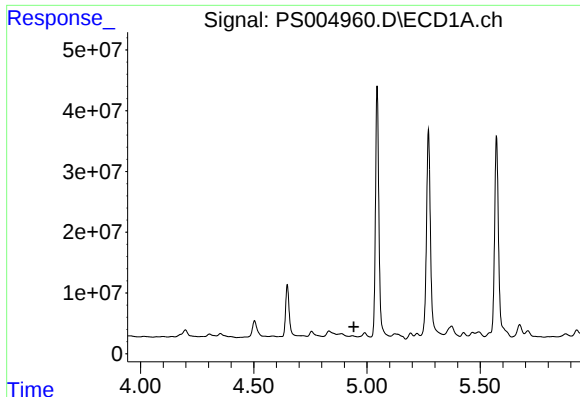

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

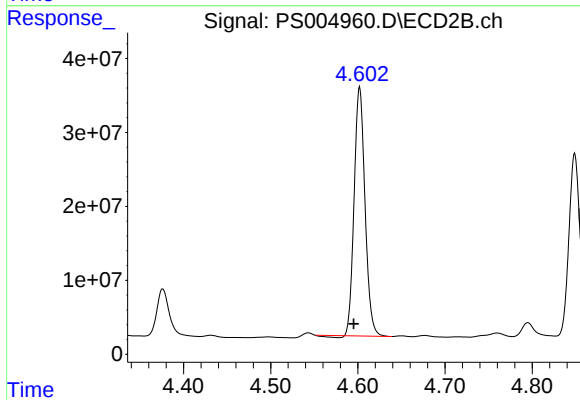


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.602 min
Delta R.T.: 0.007 min
Response: 290922918
Conc: 236.11 ng/ml

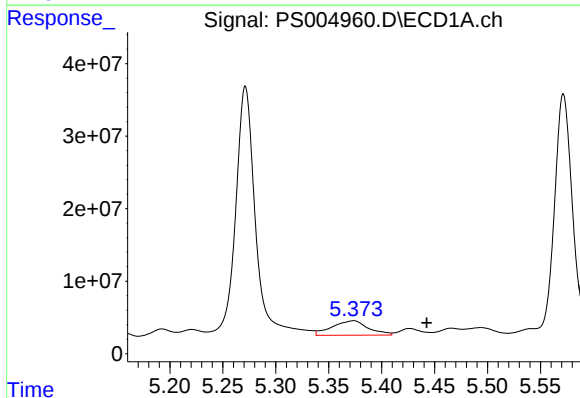


#3 4-Nitrophenol

R.T.: 5.373 min
Delta R.T.: -0.070 min
Response: 47836667
Conc: 76.72 ng/ml

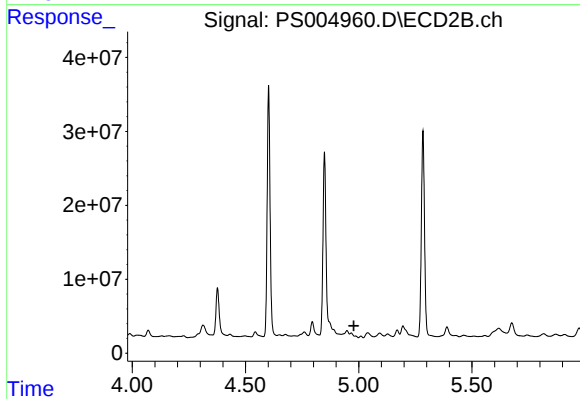

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

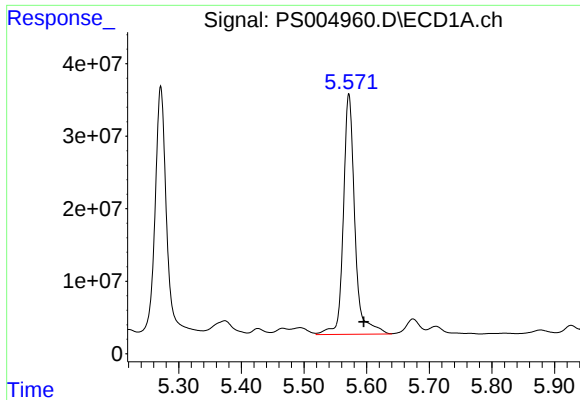

#4 2,4-DCAA


R.T.: 5.572 min
Delta R.T.: -0.023 min
Response: 422878603
Conc: 301.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

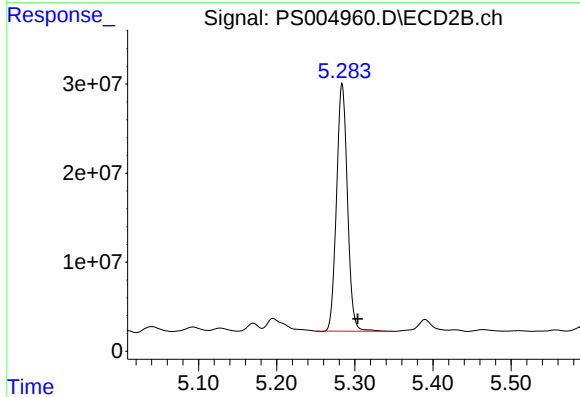


#4 2,4-DCAA

R.T.: 5.284 min
Delta R.T.: -0.020 min
Response: 269762695
Conc: 279.59 ng/ml

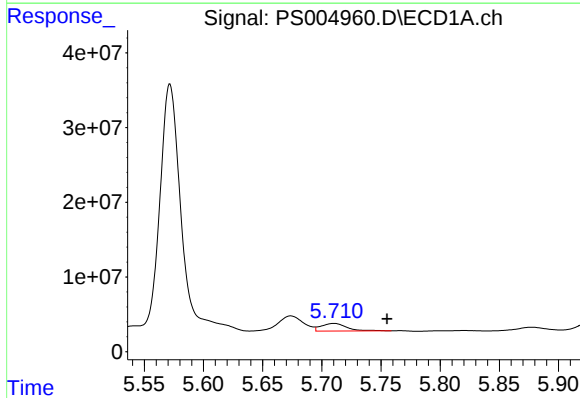


#5 DICAMBA

R.T.: 5.710 min
Delta R.T.: -0.045 min
Response: 15224563
Conc: 2.87 ng/ml

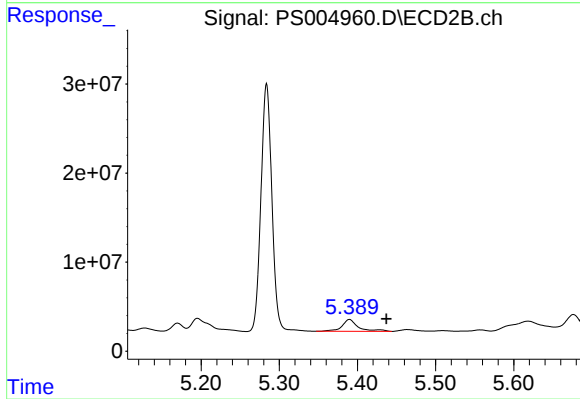

#5 DICAMBA


R.T.: 5.390 min
Delta R.T.: -0.047 min
Response: 19360730
Conc: 5.24 ng/ml

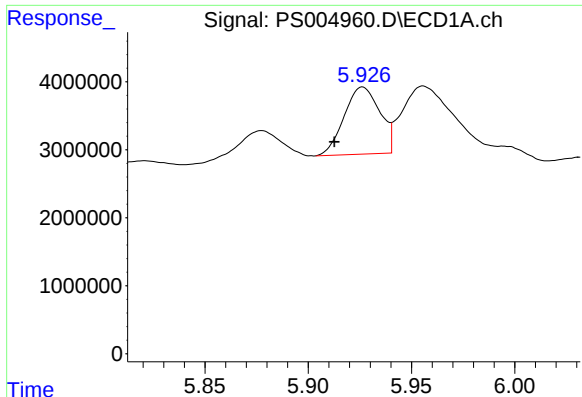

#6 MCPP


R.T.: 5.926 min
Delta R.T.: 0.014 min
Response: 11867981
Conc: 2.85 ug/ml

Instrument :
ECD_S
ClientSampleId :

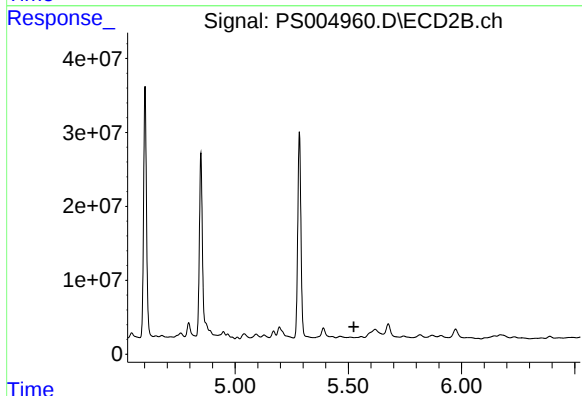


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

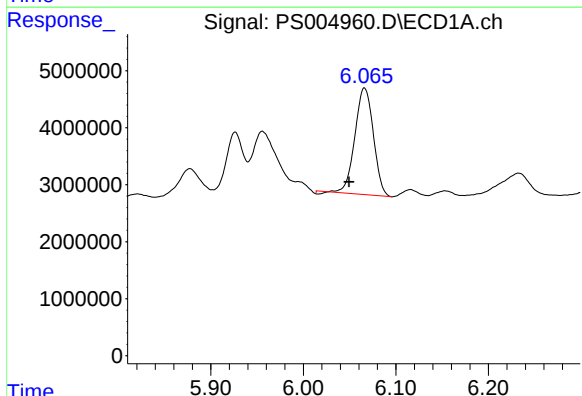


#7 MCPA

R.T.: 6.066 min
Delta R.T.: 0.017 min
Response: 26162644
Conc: 4.52 ug/ml

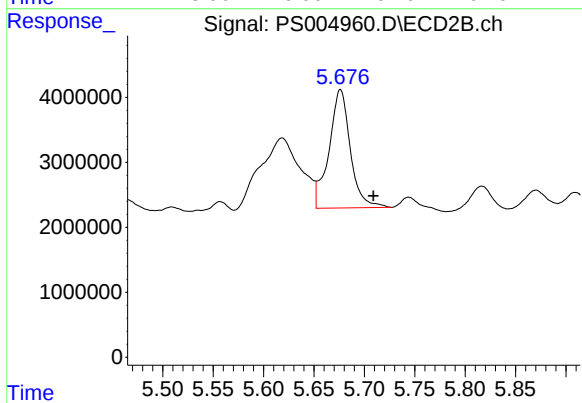

#7 MCPA


R.T.: 5.676 min
Delta R.T.: -0.033 min
Response: 26841592
Conc: 6.56 ug/ml

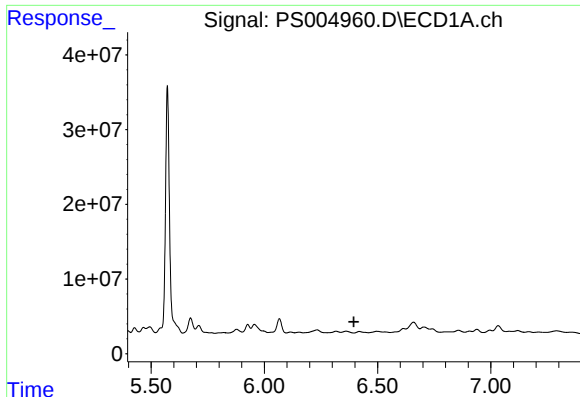

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

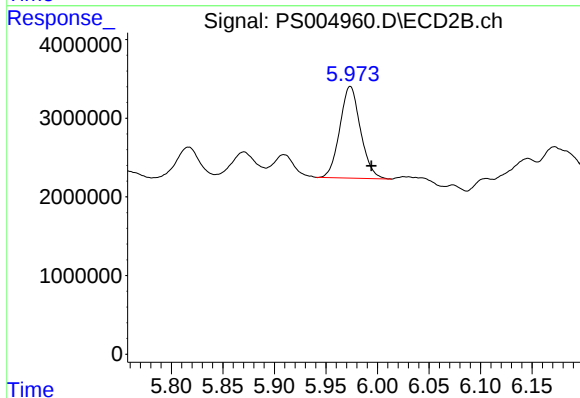


#8 DICHLORPROP

R.T.: 5.974 min
Delta R.T.: -0.021 min
Response: 16284956
Conc: 17.27 ng/ml

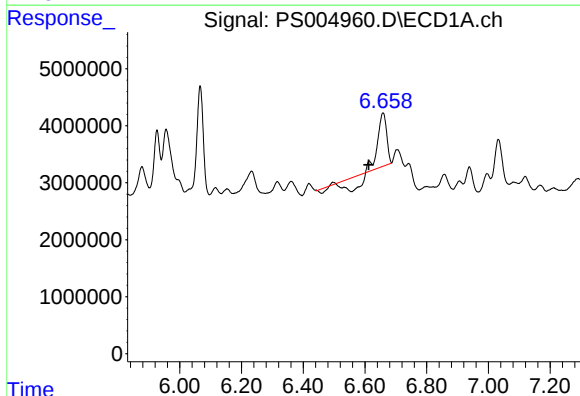


#9 2,4-D

R.T.: 6.659 min
Delta R.T.: 0.047 min
Response: 9713383
Conc: 7.10 ng/ml

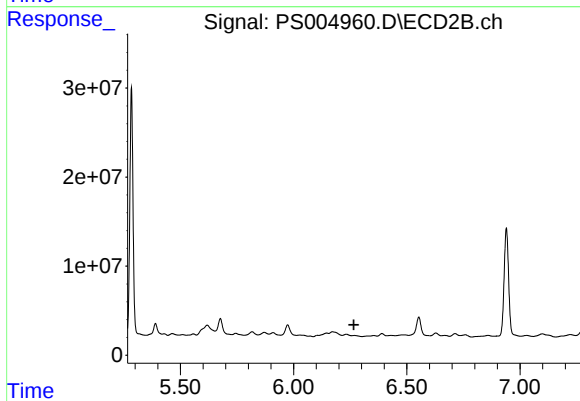

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

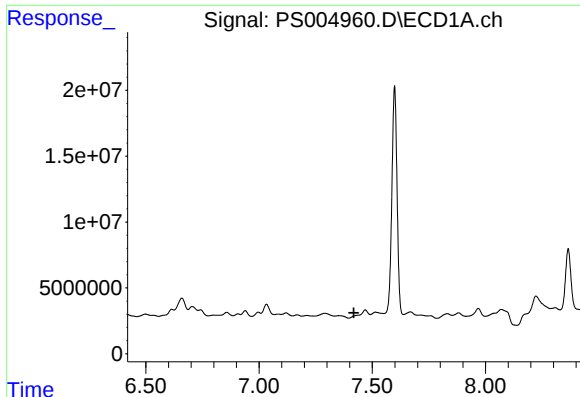

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

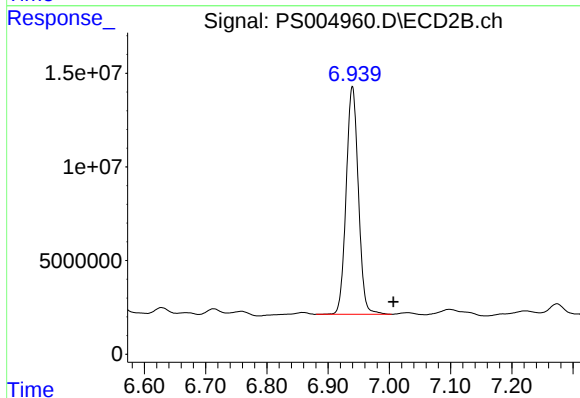


#11 2,4,5-TP (SILVEX)

R.T.: 6.940 min
Delta R.T.: -0.067 min
Response: 168092714
Conc: 32.67 ng/ml

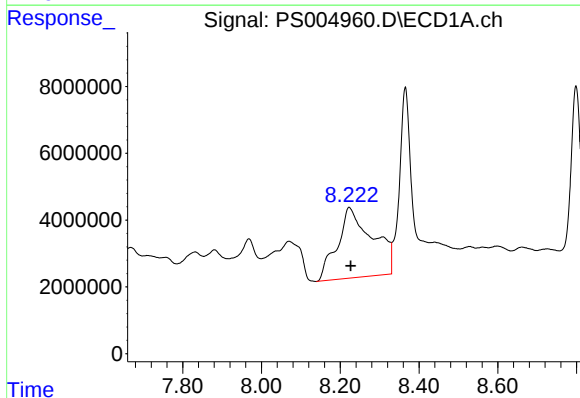


#13 2,4-DB

R.T.: 8.223 min
Delta R.T.: -0.004 min
Response: 130913221
Conc: 135.53 ng/ml

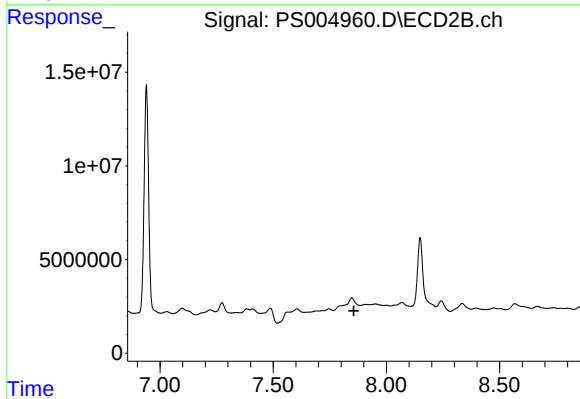

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 7.856 min
Response: 0
Conc: N.D.

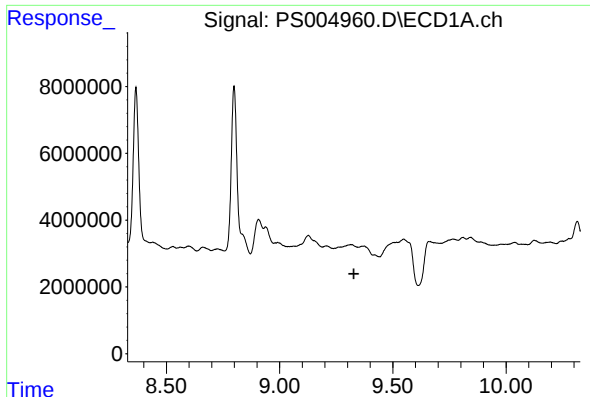

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

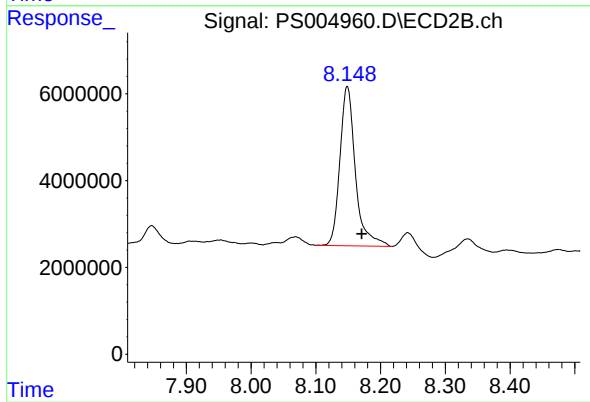

#14 DINOSEB

R.T.: 8.149 min
Delta R.T.: -0.022 min
Response: 61176376
Conc: 15.91 ng/ml