

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060619\
 Data File : PS004965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2019 20:06
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 03:47:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.576	5.289	982.9E6	683.8E6	701.161	708.753
Target Compounds							
2) T	3,5-DICHL...	4.941	0.000	115.7E6	0	67.061	N.D. #
3) T	4-Nitroph...	5.395	0.000	19346338	0	31.028	N.D. #
5) T	DICAMBA	0.000	5.443	0	83514785	N.D.	22.607
6) T	MCP	5.962	0.000	54565528	0	13.107	N.D. #
8) T	DICHLORPROP	0.000	5.979	0	70046229	N.D.	74.294
9) T	2,4-D	6.615	0.000	268.6E6	0	196.382	N.D. #
10) T	Pentachlo...	6.875	0.000	41172596	0	2.345	N.D. #
15) T	Picloram	9.112	9.104	1588.5E6	22427340	152.446	3.006 #
16) T	DCPA	0.000	9.104	0	22427340	N.D.	3.462



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060619\
Data File : PS004965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2019 20:06
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 03:47:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

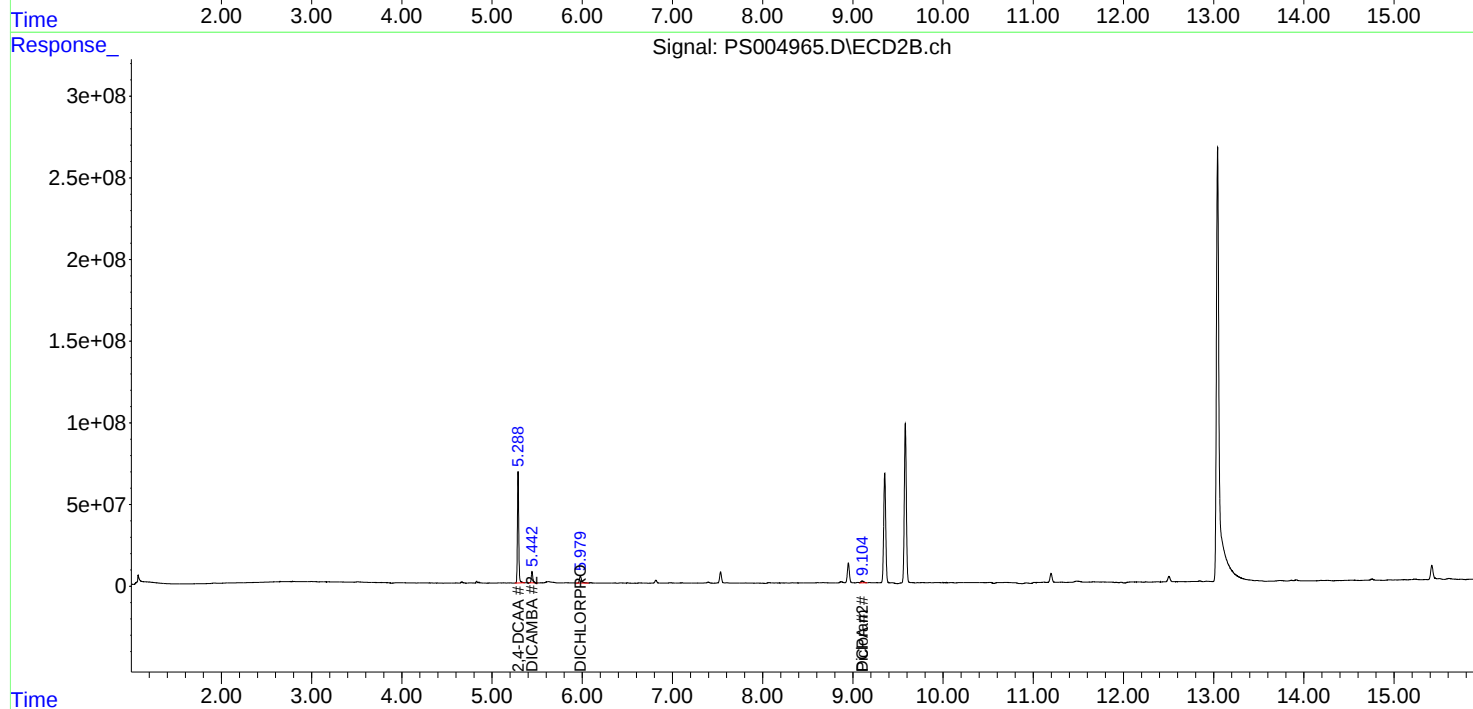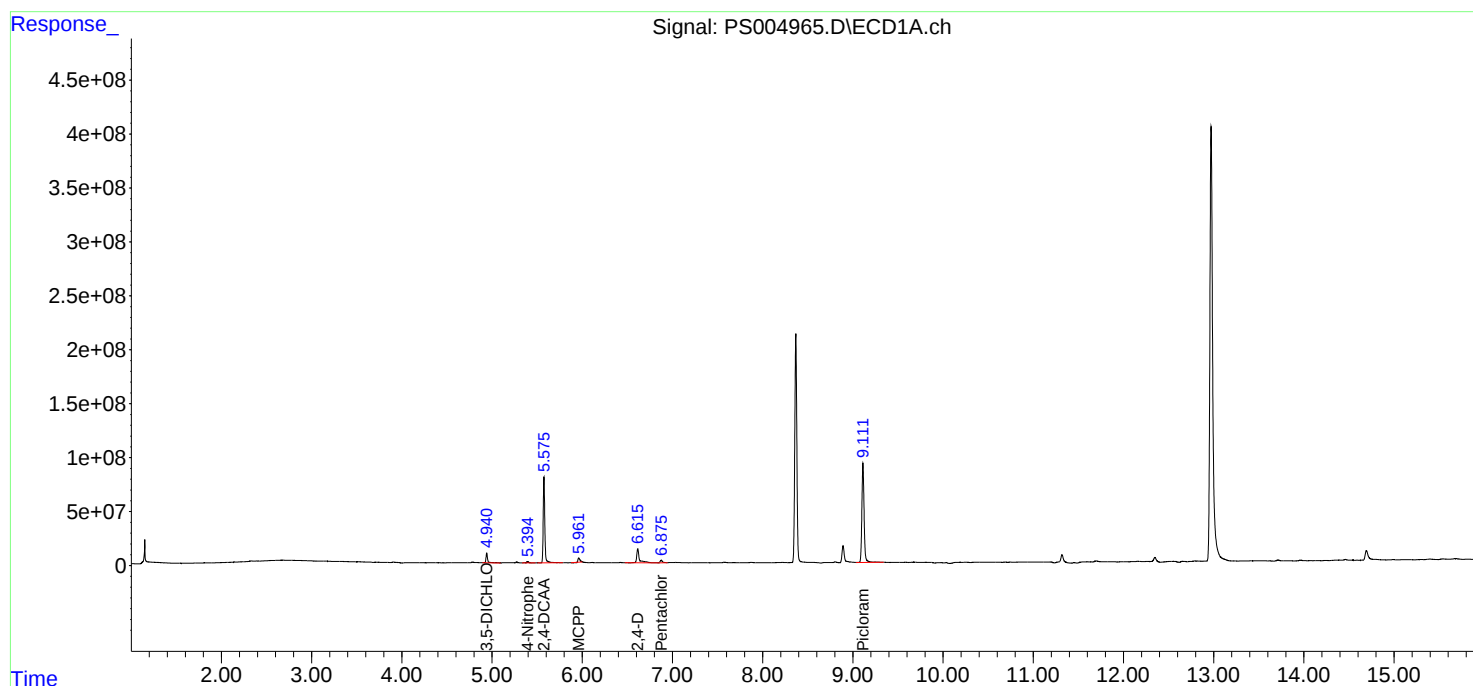


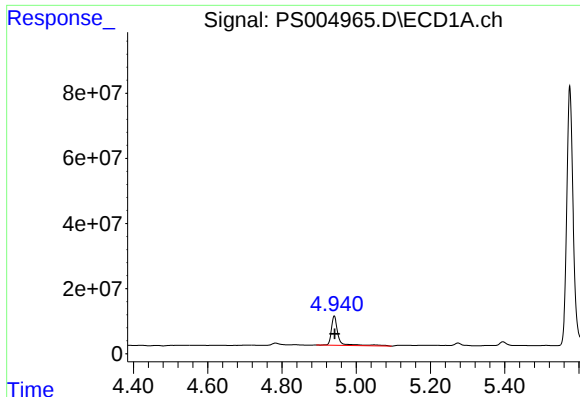

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.941 min
Delta R.T.: 0.000 min
Response: 115652269
Conc: 67.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

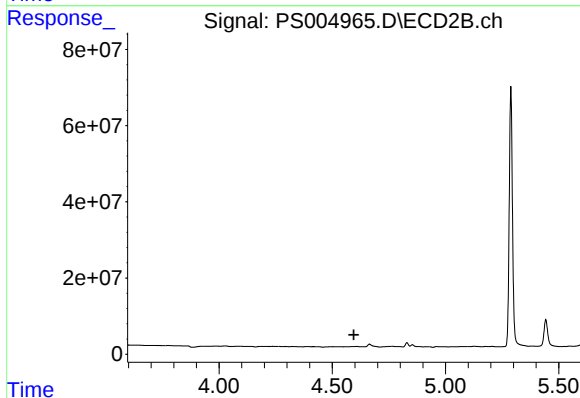


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

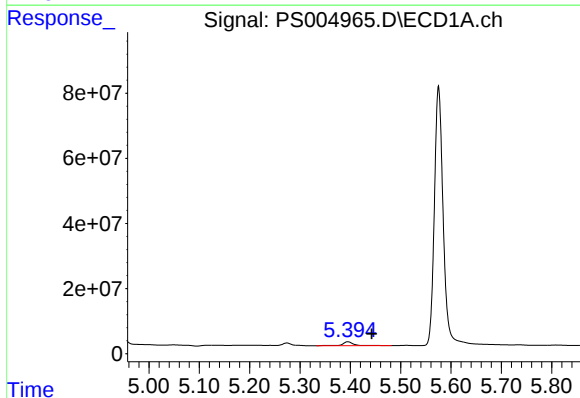


#3 4-Nitrophenol

R.T.: 5.395 min
Delta R.T.: -0.047 min
Response: 19346338
Conc: 31.03 ng/ml

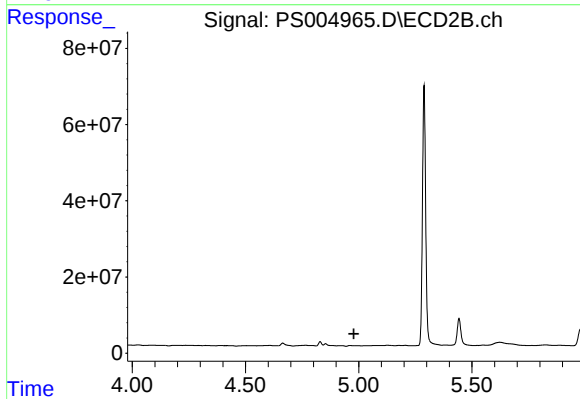

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

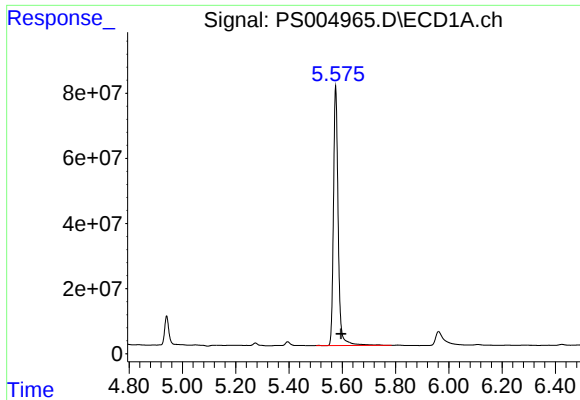

#4 2,4-DCAA


R.T.: 5.576 min
Delta R.T.: -0.019 min
Response: 982857232
Conc: 701.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

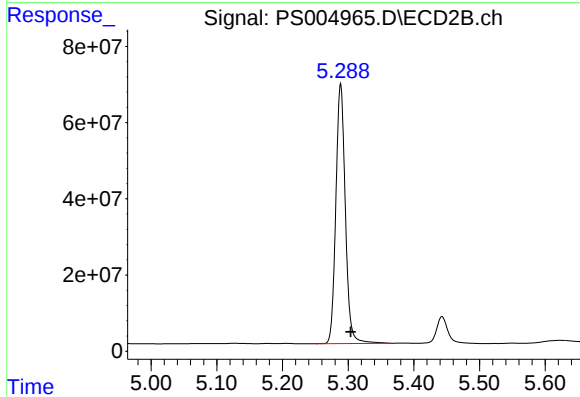


#4 2,4-DCAA

R.T.: 5.289 min
Delta R.T.: -0.015 min
Response: 683830730
Conc: 708.75 ng/ml

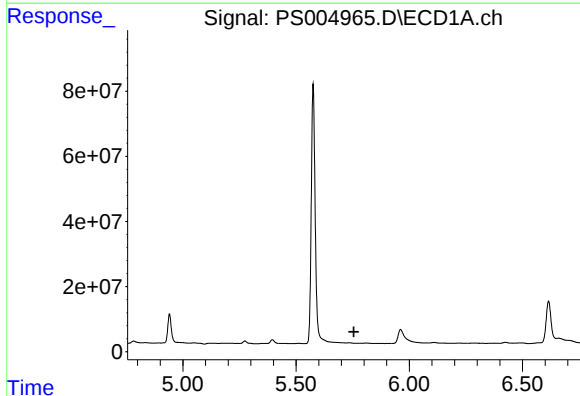


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.755 min
Response: 0
Conc: N.D.

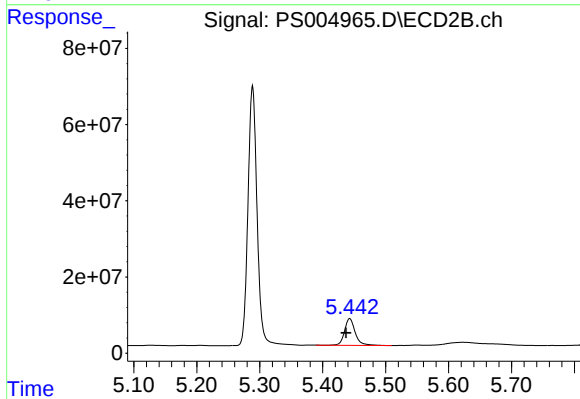

#5 DICAMBA


R.T.: 5.443 min
Delta R.T.: 0.006 min
Response: 83514785
Conc: 22.61 ng/ml

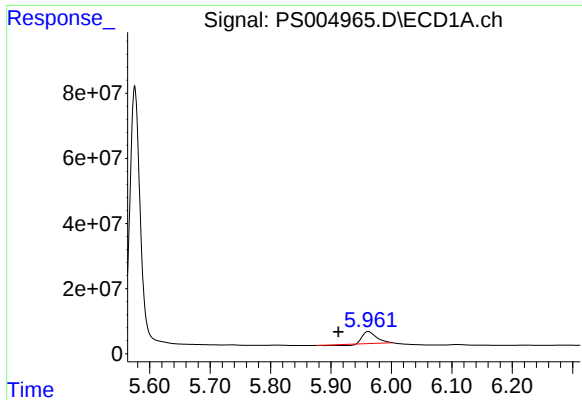

#6 MCP


R.T.: 5.962 min
Delta R.T.: 0.050 min
Response: 54565528
Conc: 13.11 ug/ml

Instrument :
ECD_S
ClientSampleId :

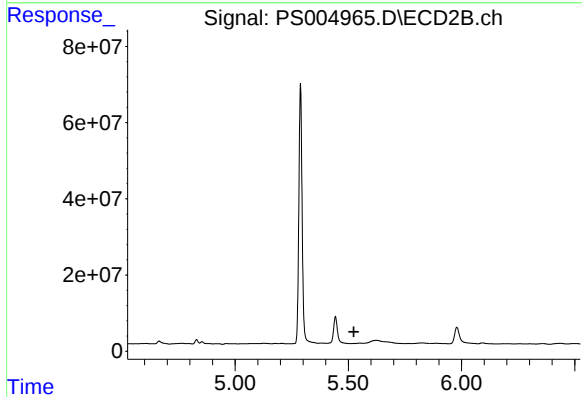


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

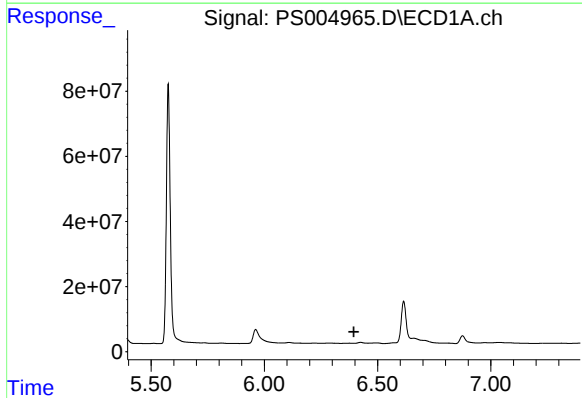


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

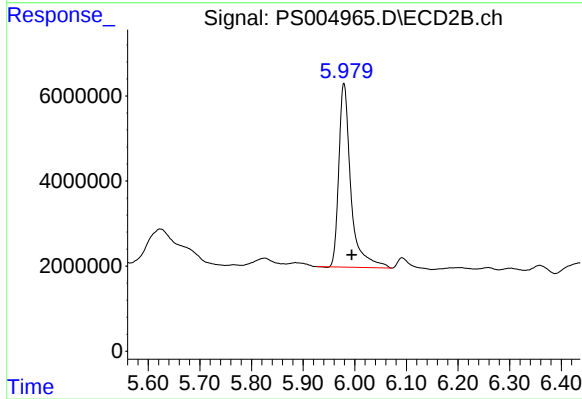

#8 DICHLORPROP


R.T.: 5.979 min
Delta R.T.: -0.015 min
Response: 70046229
Conc: 74.29 ng/ml

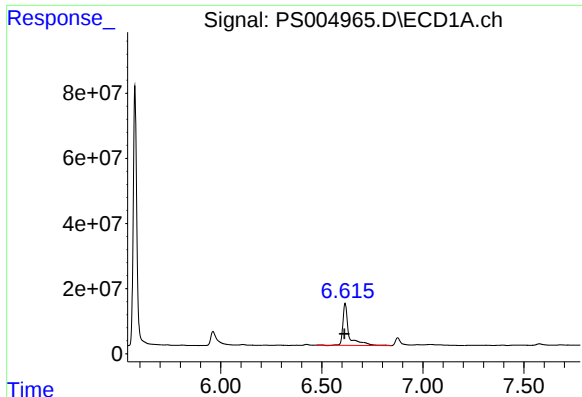

#9 2,4-D


R.T.: 6.615 min
Delta R.T.: 0.003 min
Response: 268632052
Conc: 196.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

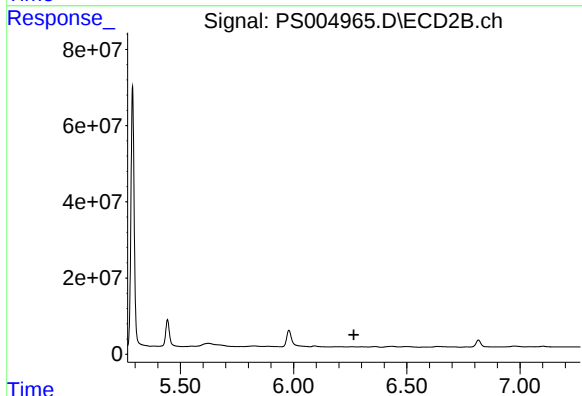


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

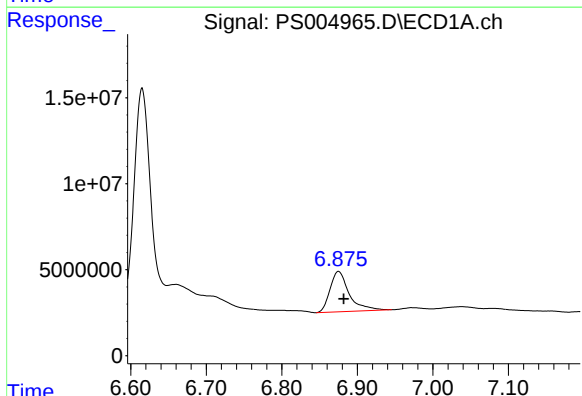


#10 Pentachlorophenol

R.T.: 6.875 min
Delta R.T.: -0.007 min
Response: 41172596
Conc: 2.34 ng/ml

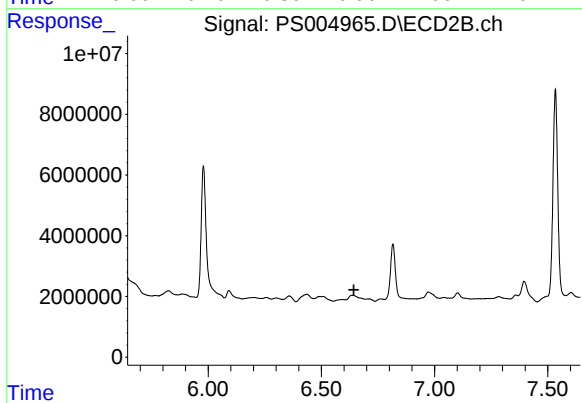

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.644 min
Response: 0
Conc: N.D.

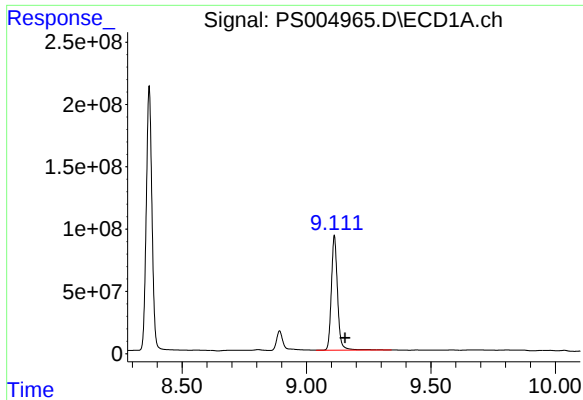

#15 Picloram


R.T.: 9.112 min
Delta R.T.: -0.043 min
Response: 1588487089
Conc: 152.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

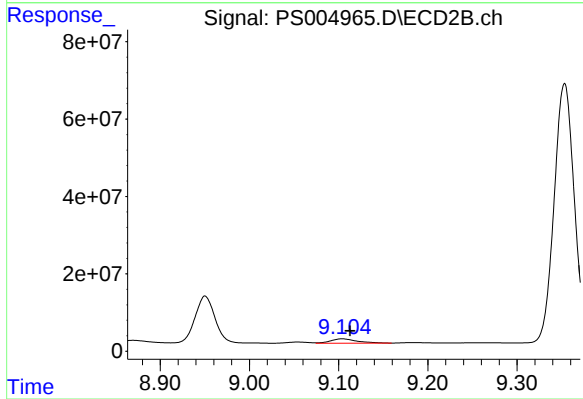


#15 Picloram

R.T.: 9.104 min
Delta R.T.: -0.009 min
Response: 22427340
Conc: 3.01 ng/ml

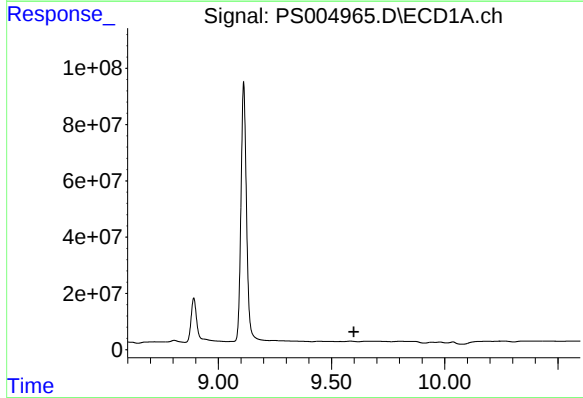

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.599 min
Response: 0
Conc: N.D.

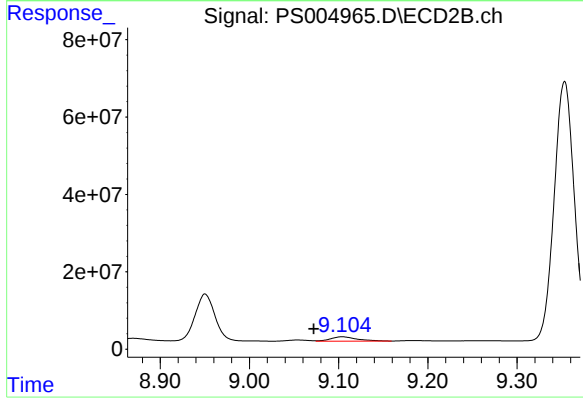

#16 DCPA

R.T.: 9.104 min
Delta R.T.: 0.032 min
Response: 22427340
Conc: 3.46 ng/ml