

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060622\
 Data File : PS019622.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2022 16:11
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 01:15:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.201	6.784	965.7E6	394.7E6	402.527	509.331 #
Target Compounds							
1) T	Dalapon	3.015	0.000	1654201	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.353f	0.000	323037	0	<MDL	N.D. #
6) T	MCP	0.000	7.085f	0	201614	N.D.	<MDL
7) T	MCPA	7.663	0.000	1116341	0	<MDL	N.D. #
10) T	Pentachlo...	8.621	8.287	1995215	1701735	<MDL	<MDL #
11) T	2,4,5-TP ...	9.190	8.656	757479	700792	<MDL	<MDL #
12) T	2,4,5-T	0.000	9.061	0	331108	N.D.	<MDL
13) T	2,4-DB	0.000	9.480f	0	374142	N.D.	<MDL
14) T	DINOSEB	11.211f	9.855	320258	194614	<MDL	<MDL #
15) T	Picloram	10.998	10.894f	435140	7650098	<MDL	1.189 #
16) T	DCPA	11.426	10.781	5159166	2193344	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060622\
Data File : PS019622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2022 16:11
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 01:15:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

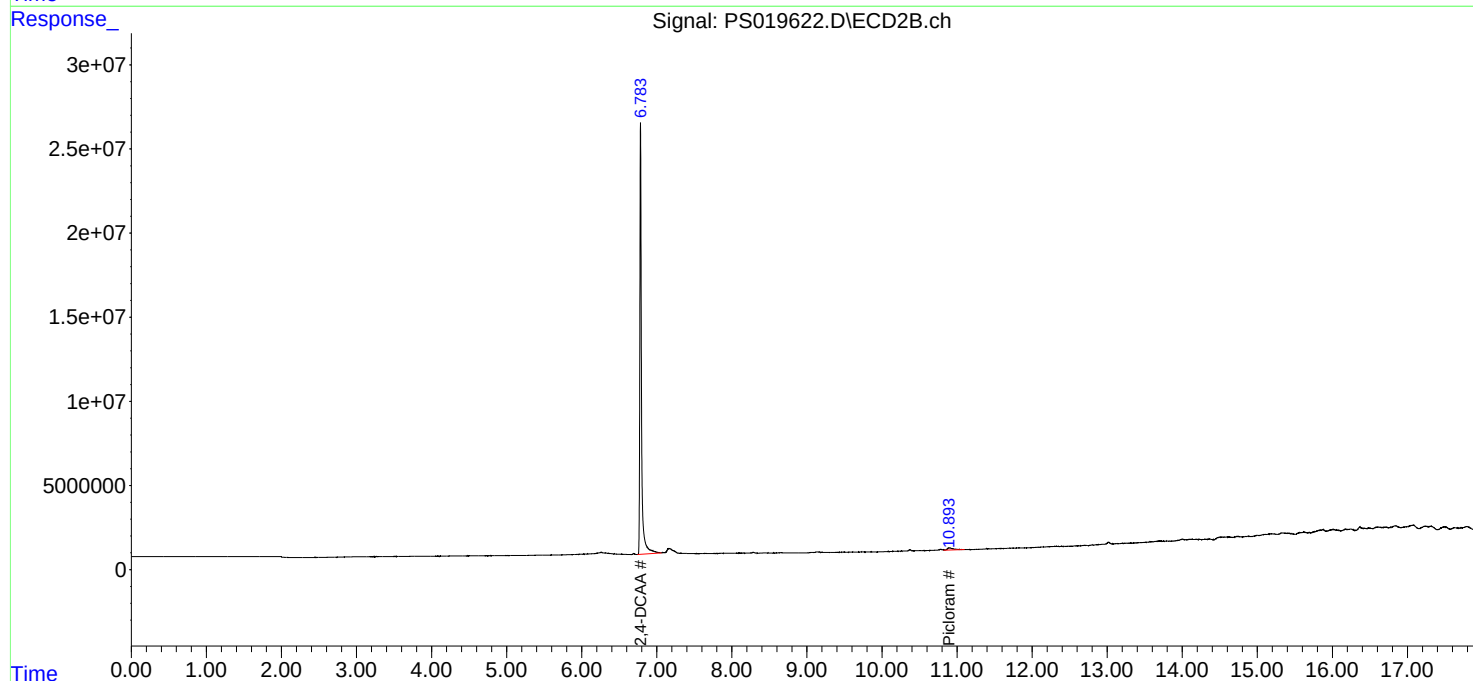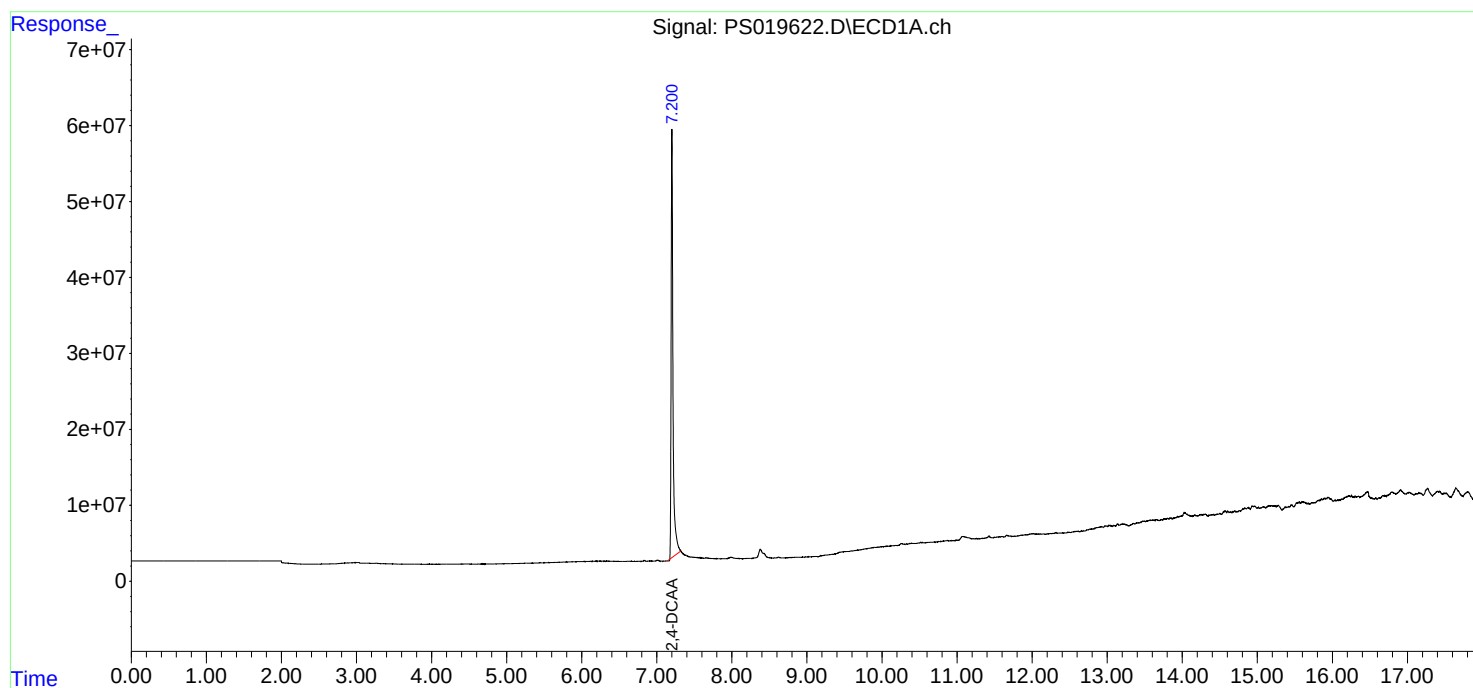


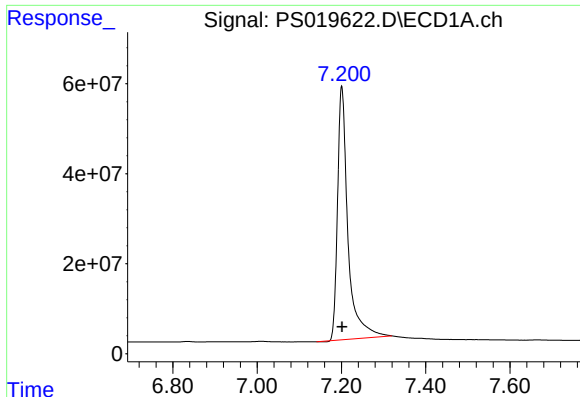

#4 2,4-DCAA


R.T.: 7.201 min
Delta R.T.: 0.000 min
Response: 965728455
Conc: 402.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

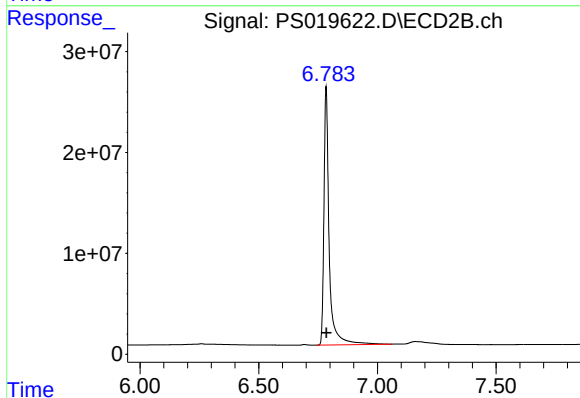


#4 2,4-DCAA

R.T.: 6.784 min
Delta R.T.: -0.001 min
Response: 394665311
Conc: 509.33 ng/ml

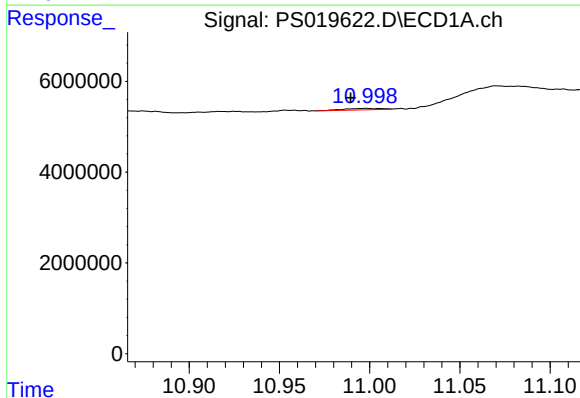

#15 Picloram

R.T.: 10.998 min
Delta R.T.: 0.009 min
Response: 435140
Conc: N.D.

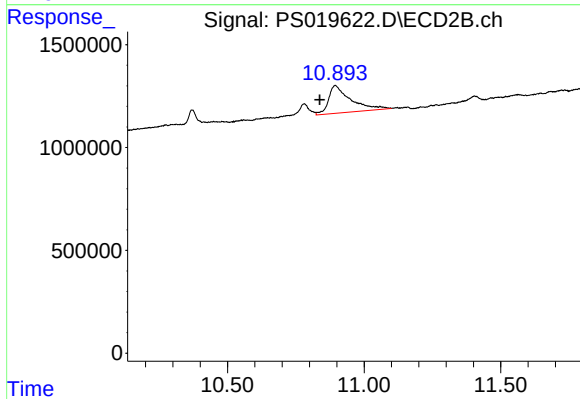

#15 Picloram

R.T.: 10.894 min
Delta R.T.: 0.057 min
Response: 7650098
Conc: 1.19 ng/ml