

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
 Data File : PS004968.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2019 15:09
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:57:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.598	5.306	498.7E6	356.5E6	355.743	369.544
Target Compounds							
12) T	2,4,5-T	7.704	7.411	20213061	69534984	2.714	15.602 #
15) T	Picloram	9.166	9.119	189.4E6	166.7E6	18.178	22.341
16) T	DCPA	9.603	9.119	14547820	166.7E6	1.633	25.729 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
Data File : PS004968.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2019 15:09
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:57:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

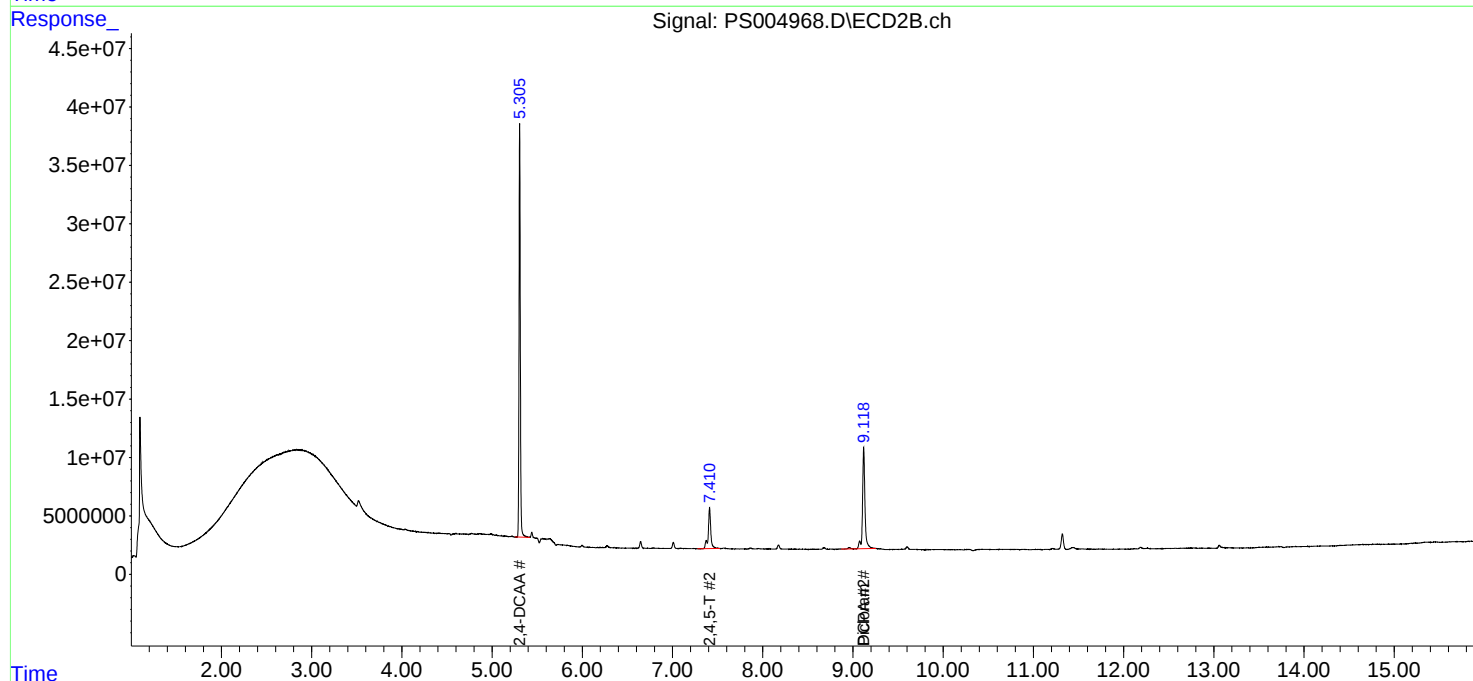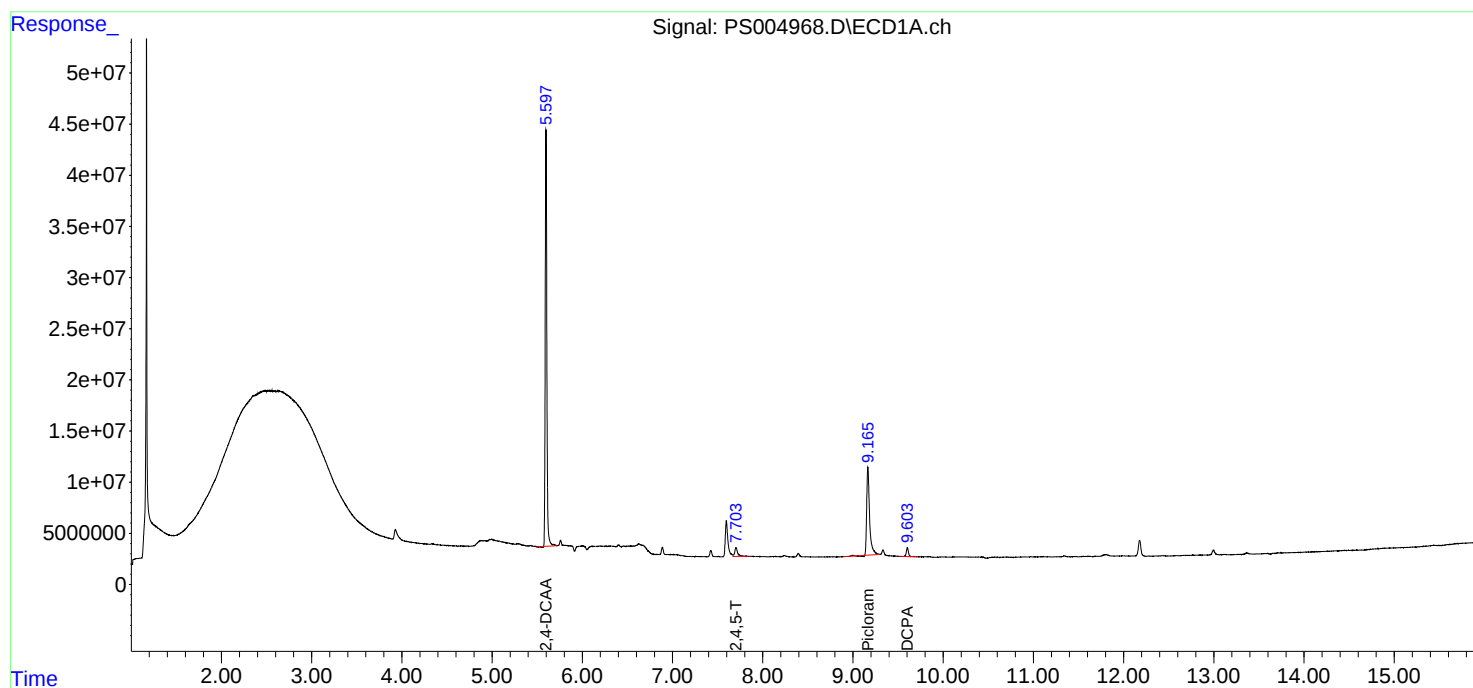


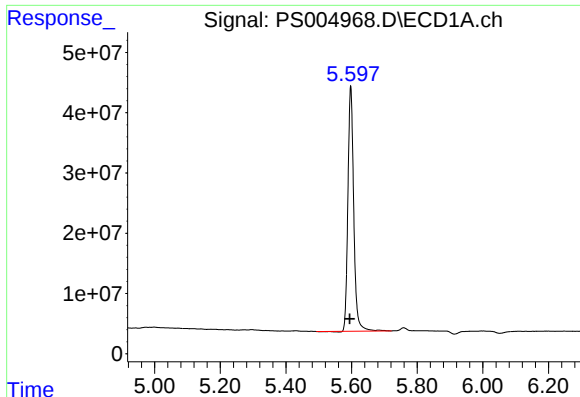

#4 2,4-DCAA


R.T.: 5.598 min
Delta R.T.: 0.003 min
Response: 498664935
Conc: 355.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

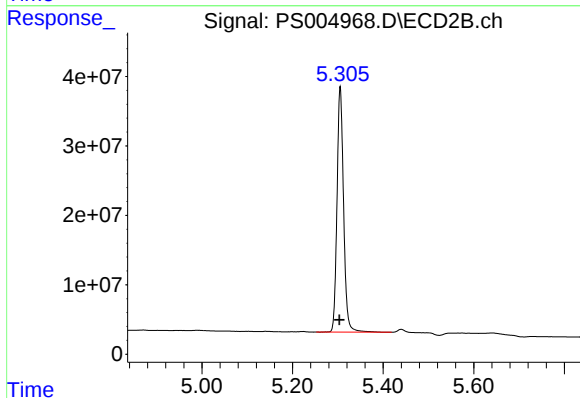


#4 2,4-DCAA

R.T.: 5.306 min
Delta R.T.: 0.002 min
Response: 356549735
Conc: 369.54 ng/ml

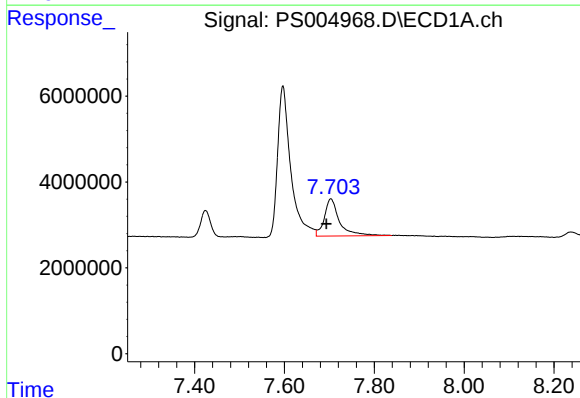


#12 2,4,5-T

R.T.: 7.704 min
Delta R.T.: 0.010 min
Response: 20213061
Conc: 2.71 ng/ml

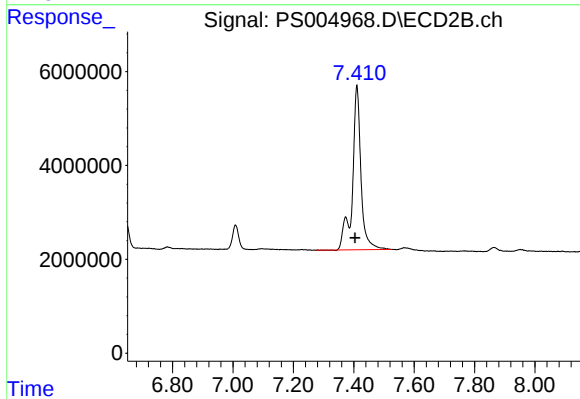

#12 2,4,5-T


R.T.: 7.411 min
Delta R.T.: 0.007 min
Response: 69534984
Conc: 15.60 ng/ml

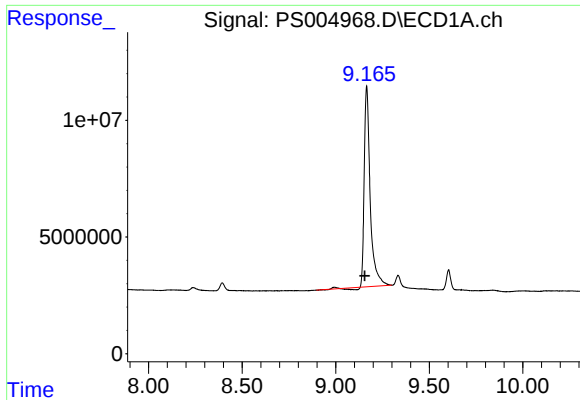

#15 Picloram


R.T.: 9.166 min
Delta R.T.: 0.010 min
Response: 189410015
Conc: 18.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

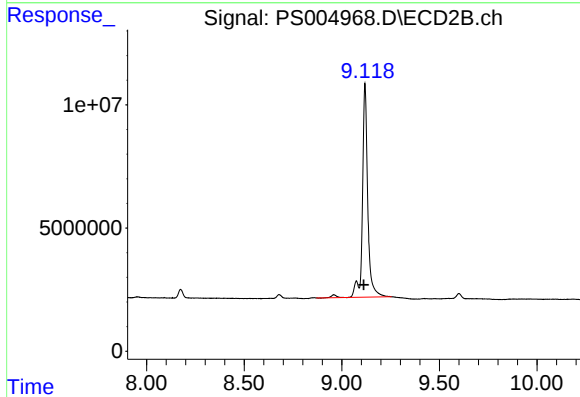


#15 Picloram

R.T.: 9.119 min
Delta R.T.: 0.006 min
Response: 166677208
Conc: 22.34 ng/ml

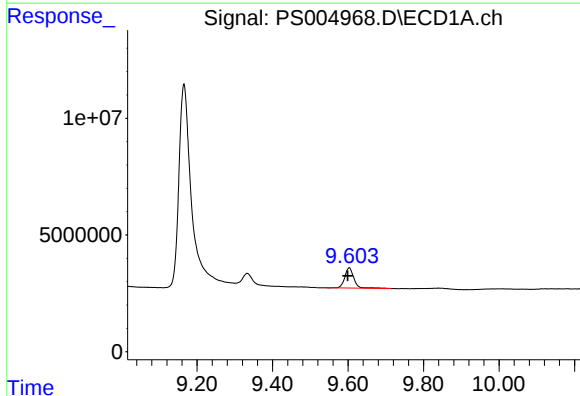

#16 DCPA

R.T.: 9.603 min
Delta R.T.: 0.004 min
Response: 14547820
Conc: 1.63 ng/ml

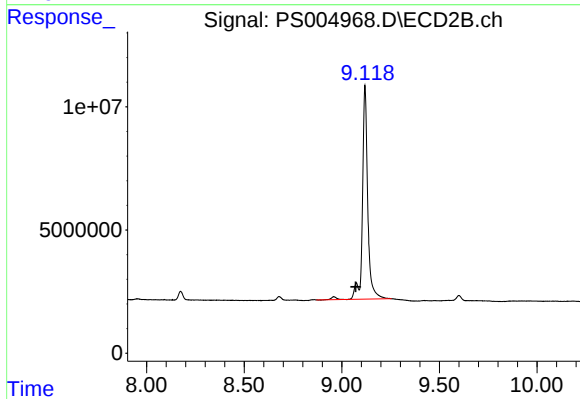

#16 DCPA

R.T.: 9.119 min
Delta R.T.: 0.047 min
Response: 166677208
Conc: 25.73 ng/ml