

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
 Data File : PS004972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2019 17:23
 Operator : SM\AJ
 Sample : PB120425TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:59:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.575	5.287	737.2E6	501.6E6	525.884	519.892
Target Compounds							
2) T	3,5-DICHL...	0.000	4.606	0	275.8E6	N.D.	223.813
3) T	4-Nitroph...	5.378	0.000	35121106	0	56.328	N.D. #
5) T	DICAMBA	0.000	5.394	0	10026590	N.D.	2.714
6) T	MCP	5.930	0.000	9864466	0	2.370	N.D. #
7) T	MCPA	6.069	5.680	25545275	28688496	4.410	7.011 #
9) T	2,4-D	6.662	0.000	18420827	0	13.466	N.D. #
11) T	2,4,5-TP ...	0.000	6.943	0	83838509	N.D.	16.294
13) T	2,4-DB	8.230	0.000	27374206	0	28.339	N.D. #
14) T	DINOSEB	0.000	8.152	0	60216558	N.D.	15.665
15) T	Picloram	0.000	9.107	0	1600506	N.D.	<MDL
16) T	DCPA	0.000	9.107	0	1600506	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
Data File : PS004972.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2019 17:23
Operator : SM\AJ
Sample : PB120425TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:59:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

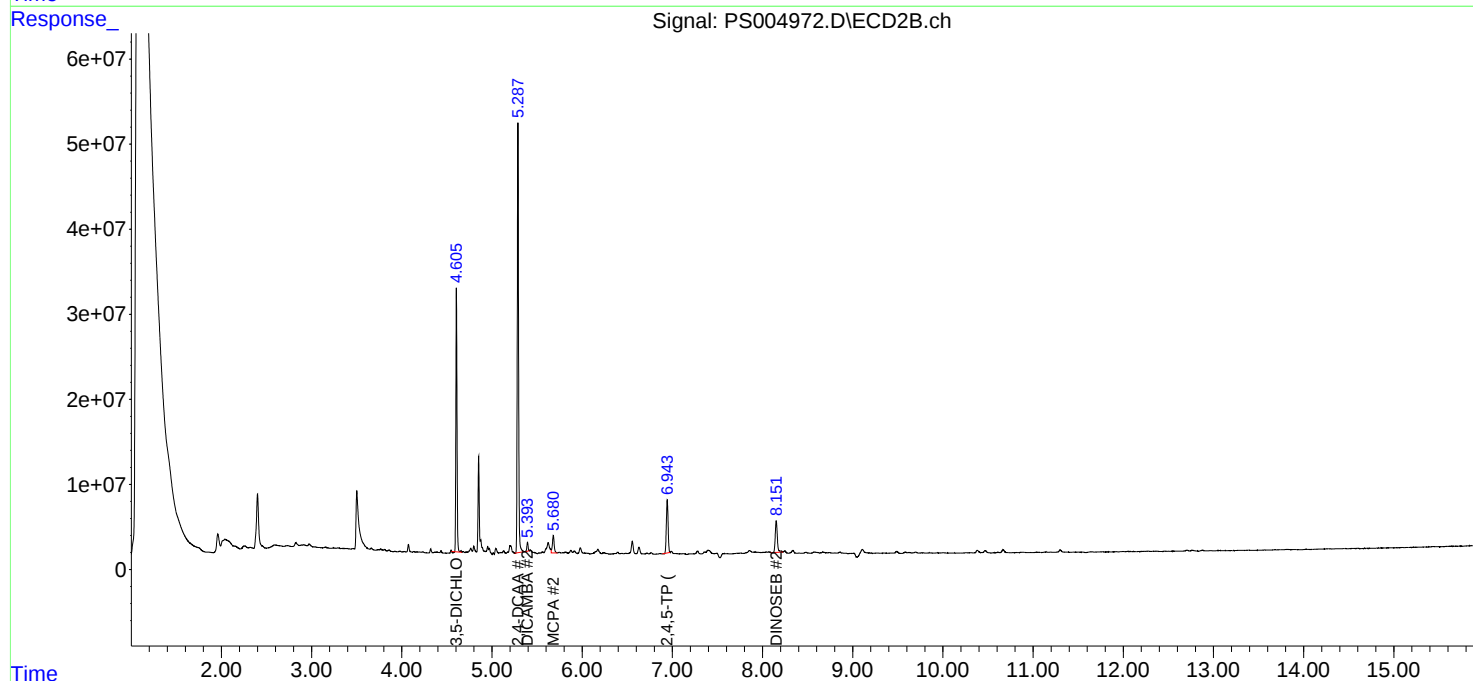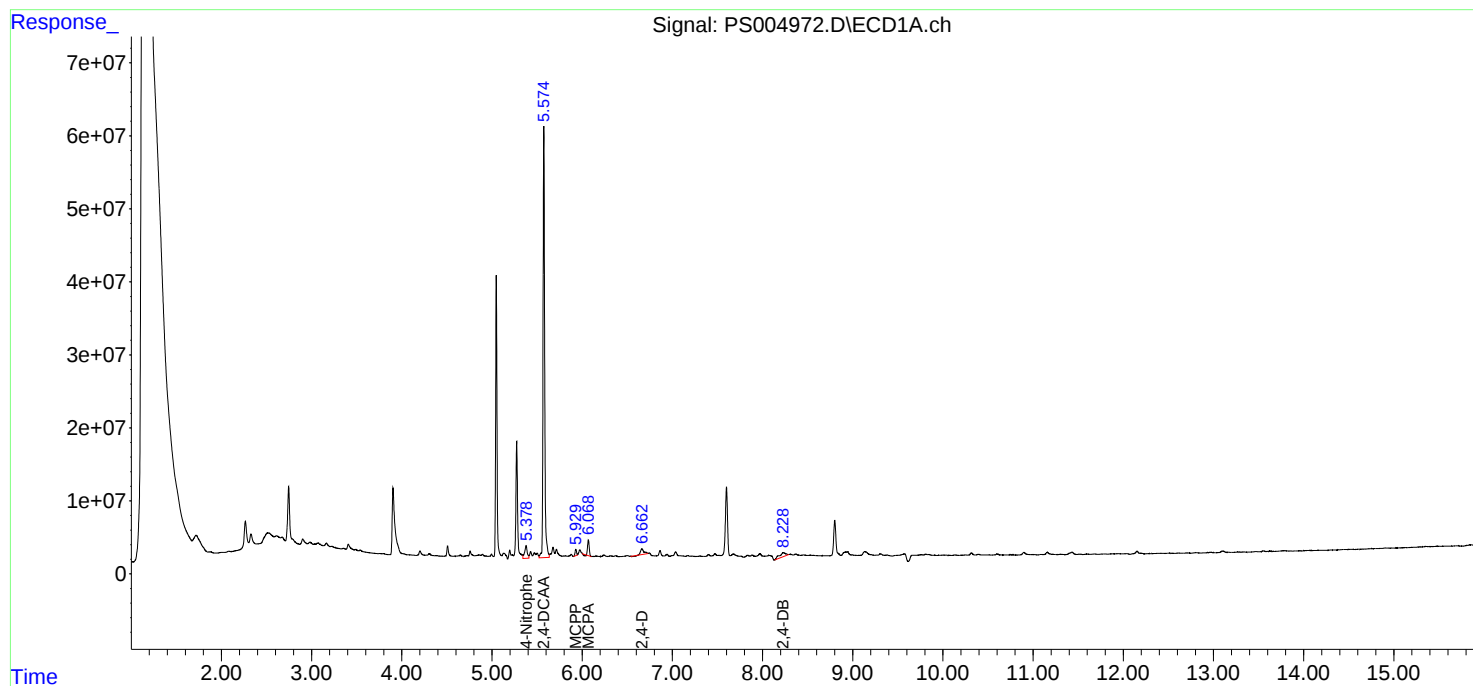


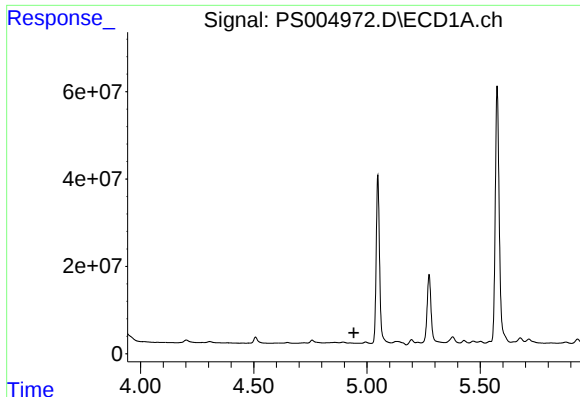

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

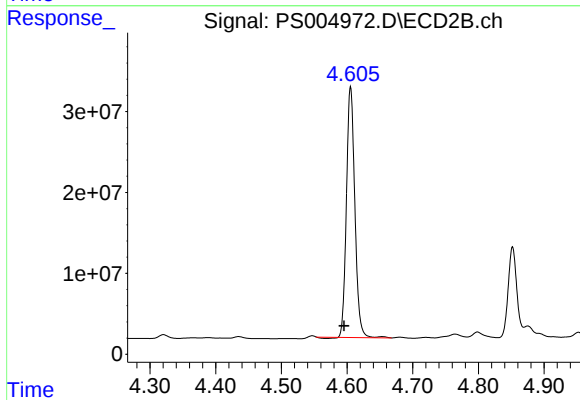


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.606 min
Delta R.T.: 0.010 min
Response: 275765898
Conc: 223.81 ng/ml

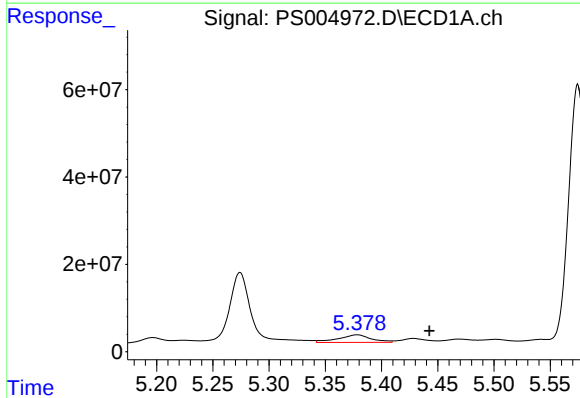


#3 4-Nitrophenol

R.T.: 5.378 min
Delta R.T.: -0.064 min
Response: 35121106
Conc: 56.33 ng/ml

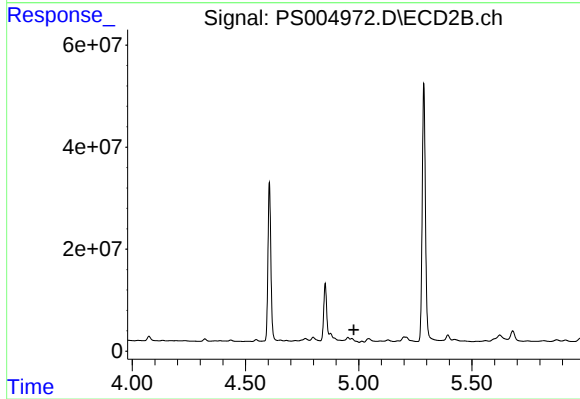

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

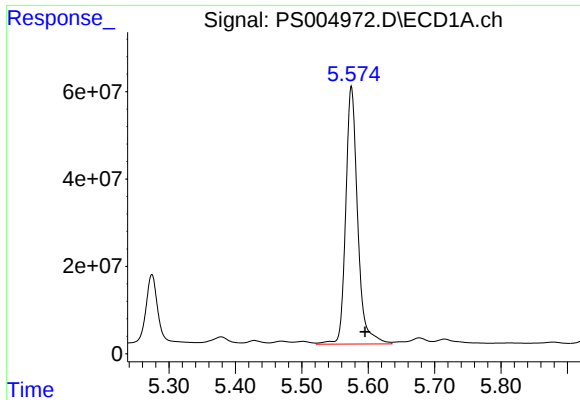

#4 2,4-DCAA


R.T.: 5.575 min
Delta R.T.: -0.020 min
Response: 737161312
Conc: 525.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

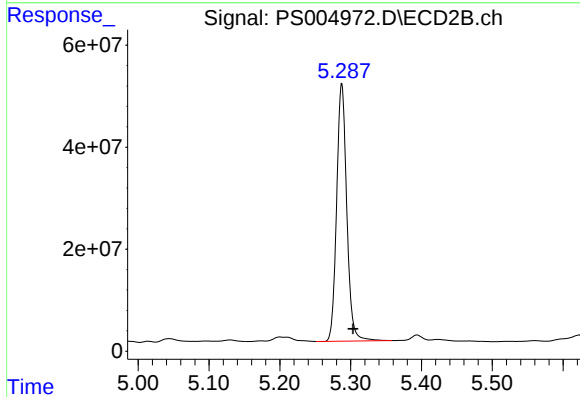


#4 2,4-DCAA

R.T.: 5.287 min
Delta R.T.: -0.016 min
Response: 501610415
Conc: 519.89 ng/ml

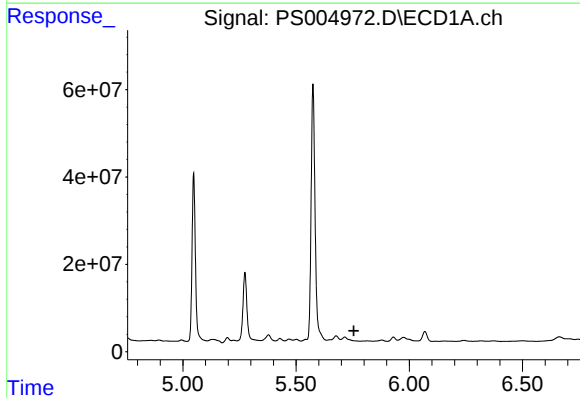


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.755 min
Response: 0
Conc: N.D.

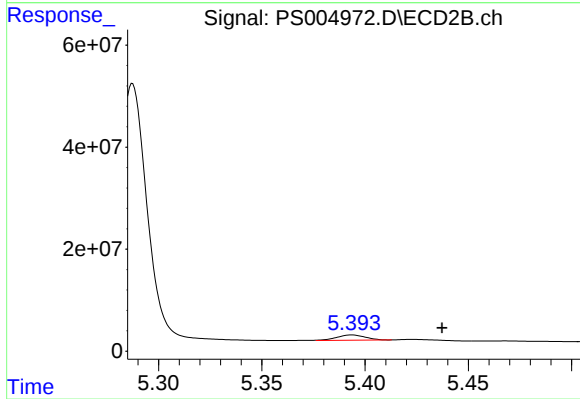

#5 DICAMBA


R.T.: 5.394 min
Delta R.T.: -0.044 min
Response: 10026590
Conc: 2.71 ng/ml

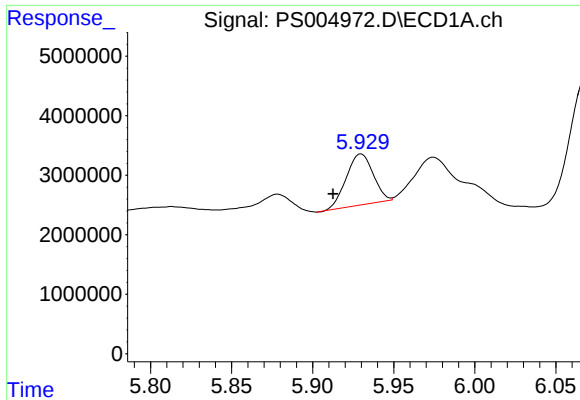

#6 MCPP


R.T.: 5.930 min
Delta R.T.: 0.017 min
Response: 9864466
Conc: 2.37 ug/ml

Instrument :
ECD_S
ClientSampleId :

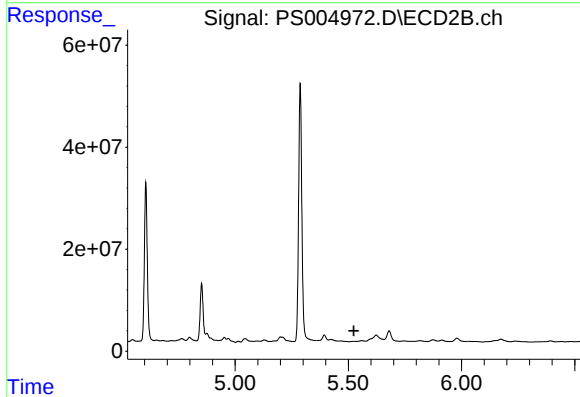


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

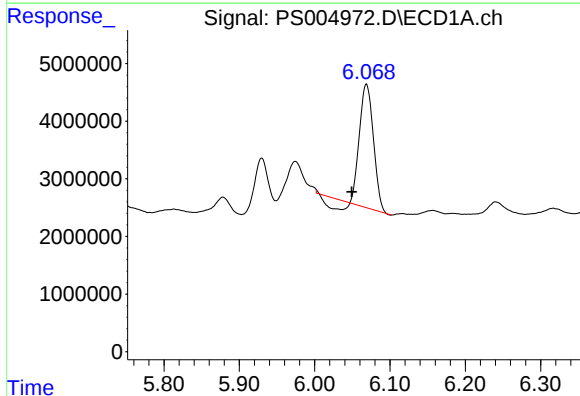


#7 MCPA

R.T.: 6.069 min
Delta R.T.: 0.020 min
Response: 25545275
Conc: 4.41 ug/ml

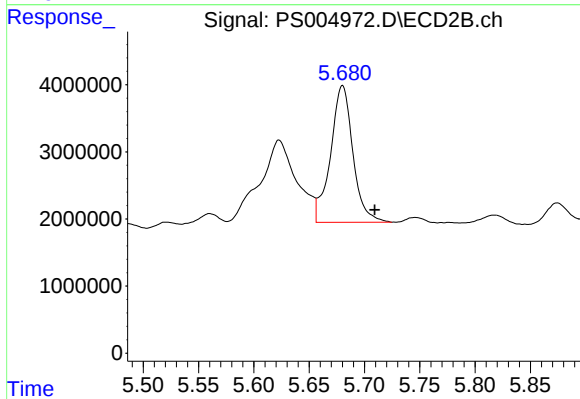

#7 MCPA


R.T.: 5.680 min
Delta R.T.: -0.029 min
Response: 28688496
Conc: 7.01 ug/ml

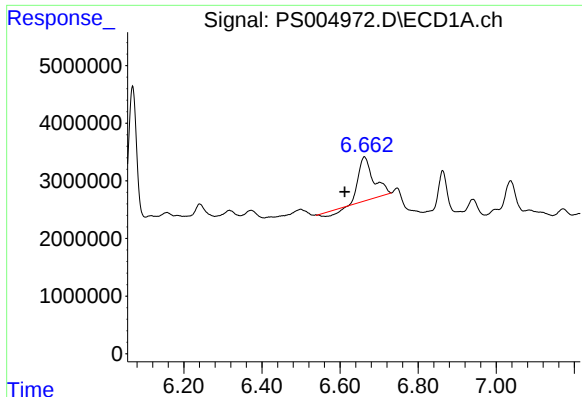

#9 2,4-D


R.T.: 6.662 min
Delta R.T.: 0.051 min
Response: 18420827
Conc: 13.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

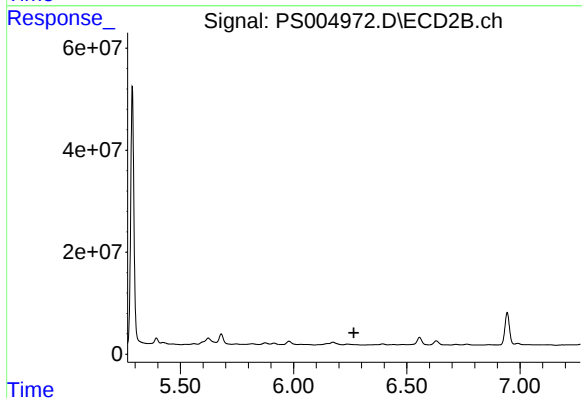


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

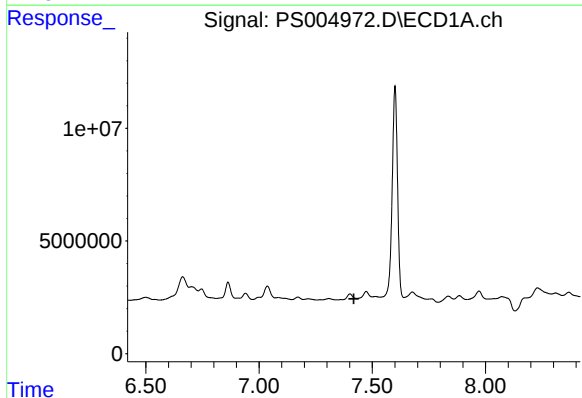


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

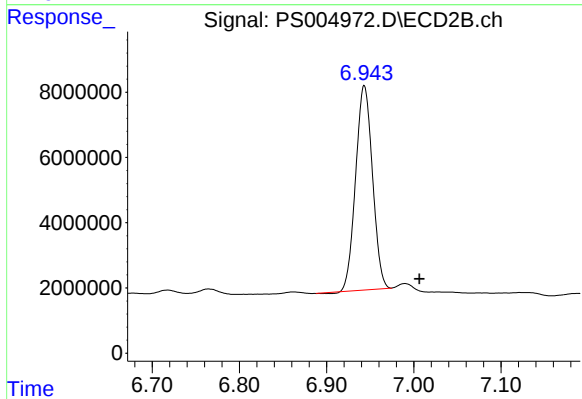

#11 2,4,5-TP (SILVEX)


R.T.: 6.943 min
Delta R.T.: -0.063 min
Response: 83838509
Conc: 16.29 ng/ml

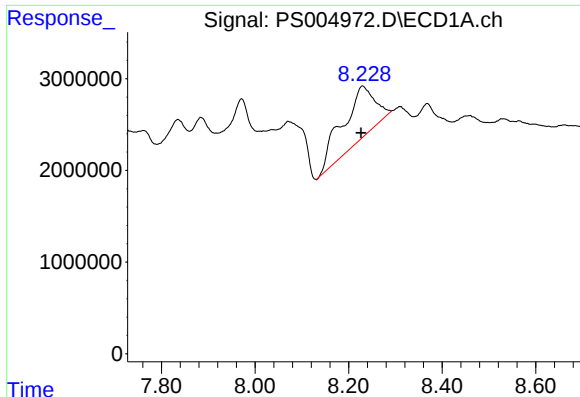

#13 2,4-DB


R.T.: 8.230 min
Delta R.T.: 0.003 min
Response: 27374206
Conc: 28.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

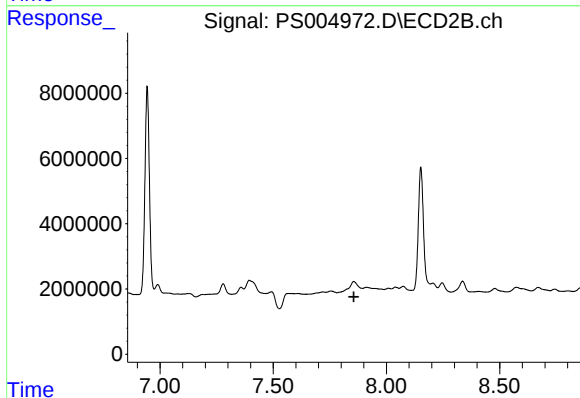


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.856 min
Response: 0
Conc: N.D.

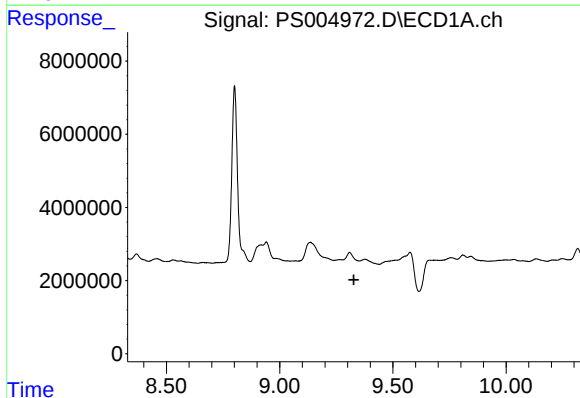

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.328 min
Response: 0
Conc: N.D.

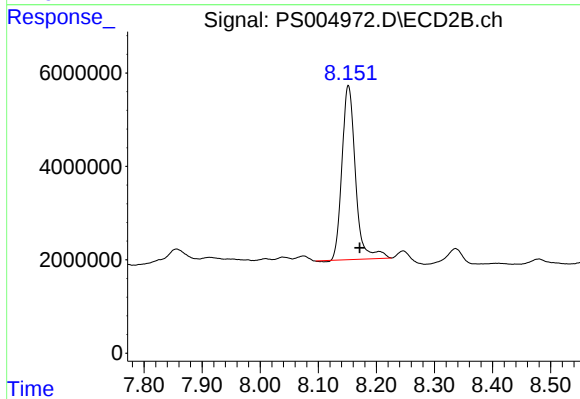

#14 DINOSEB

R.T.: 8.152 min
Delta R.T.: -0.019 min
Response: 60216558
Conc: 15.66 ng/ml