

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
 Data File : PS004973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2019 17:45
 Operator : SM\AJ
 Sample : K3153-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:59:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.573	5.285	382.5E6	245.8E6	272.837	254.744
Target Compounds							
2) T	3,5-DICHL...	0.000	4.603	0	210.2E6	N.D.	170.561
3) T	4-Nitroph...	5.488	4.990	61487476	20504776	98.616	43.266 #
5) T	DICAMBA	5.766	5.391	27082993	17375279	5.101	4.703
6) T	MCP	5.962	0.000	8261101	0	1.984	N.D. #
7) T	MCPA	0.000	5.746	0	151.3E6	N.D.	36.987
8) T	DICHLORPROP	0.000	5.975	0	19916163	N.D.	21.124
9) T	2,4-D	6.663	0.000	24791530	0	18.124	N.D. #
11) T	2,4,5-TP ...	0.000	6.941	0	150.7E6	N.D.	29.287



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
Data File : PS004973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2019 17:45
Operator : SM\AJ
Sample : K3153-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:59:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

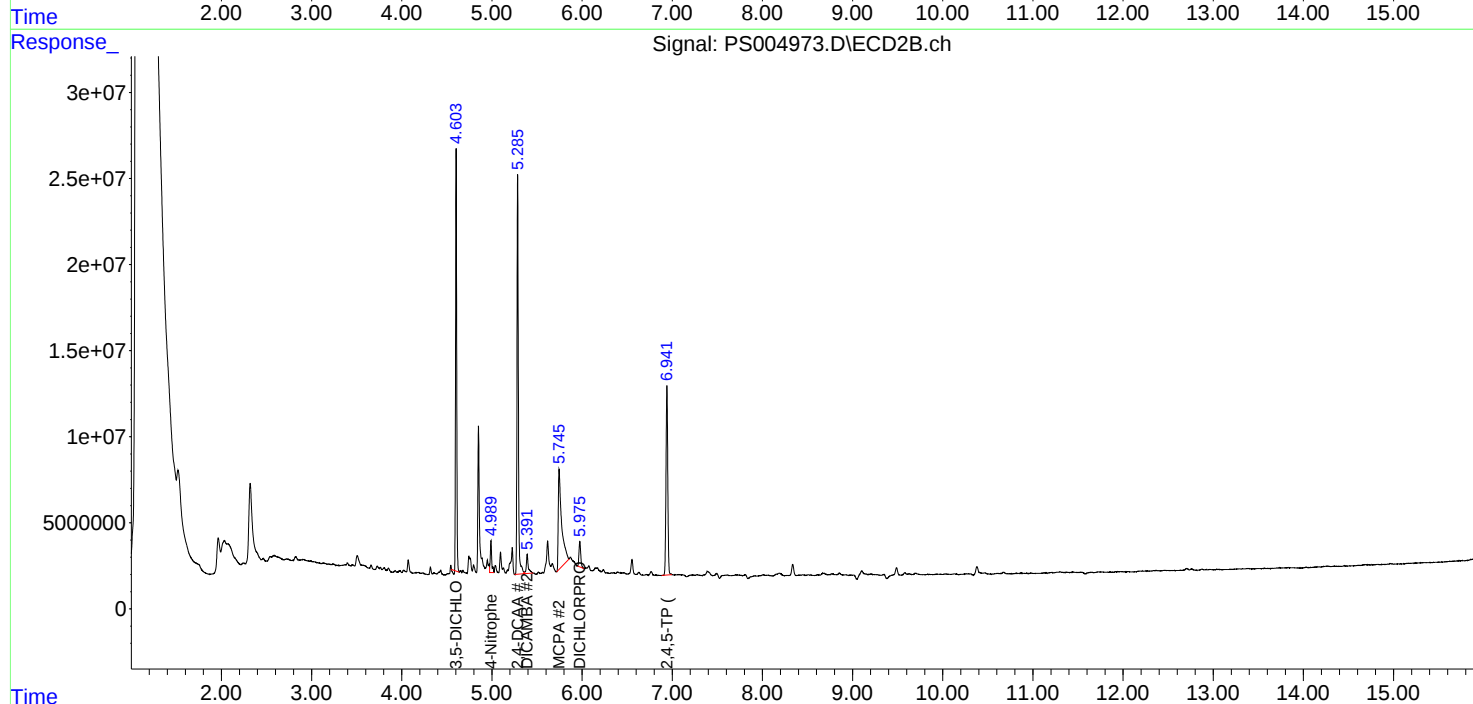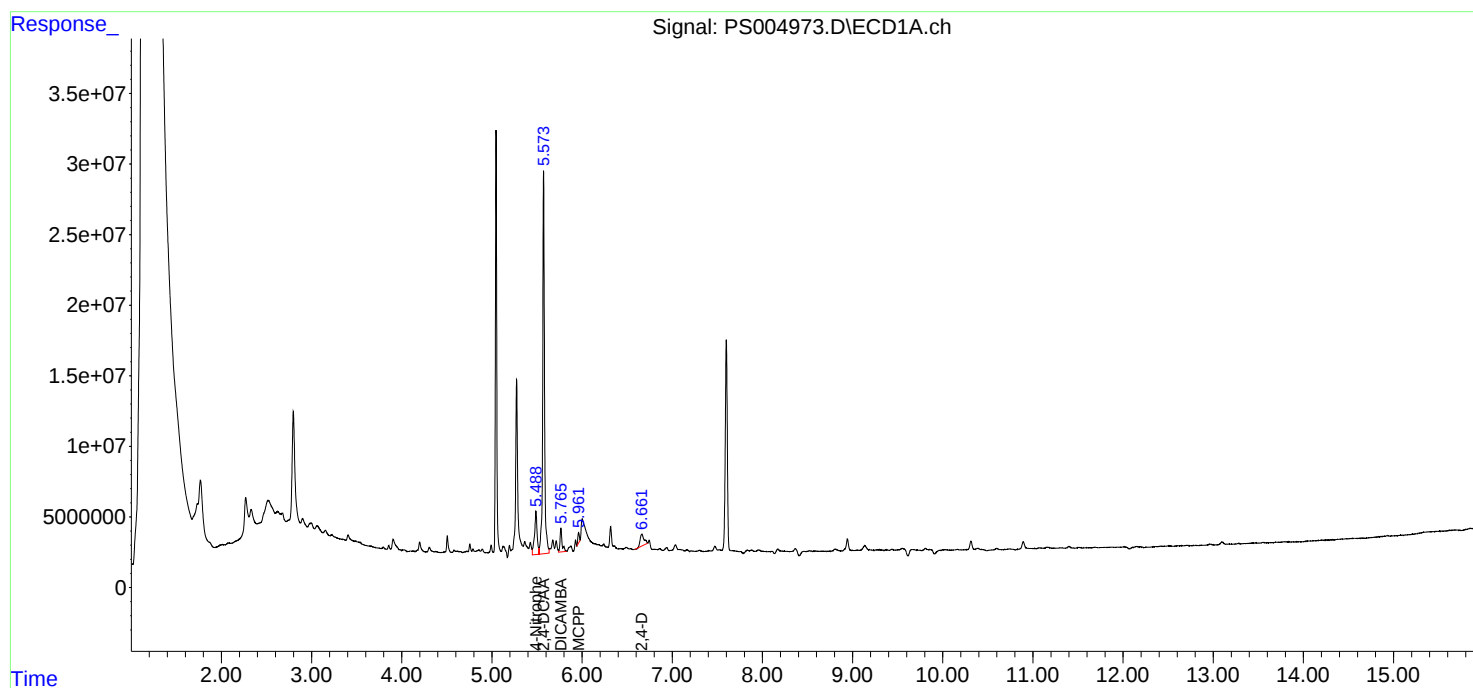


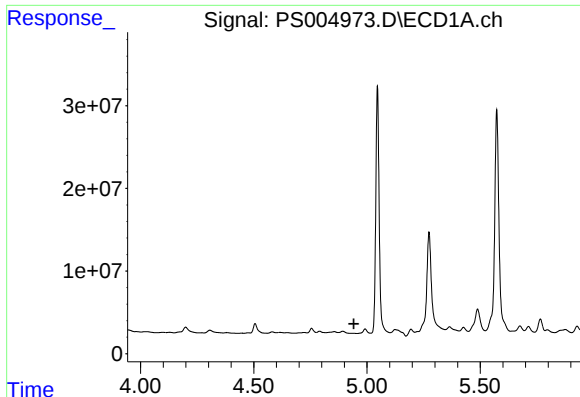

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

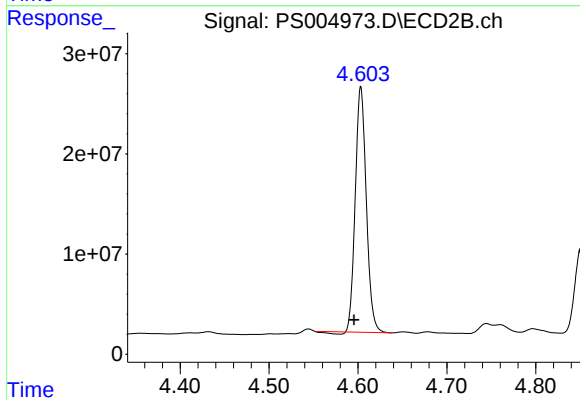


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.603 min
Delta R.T.: 0.008 min
Response: 210153145
Conc: 170.56 ng/ml

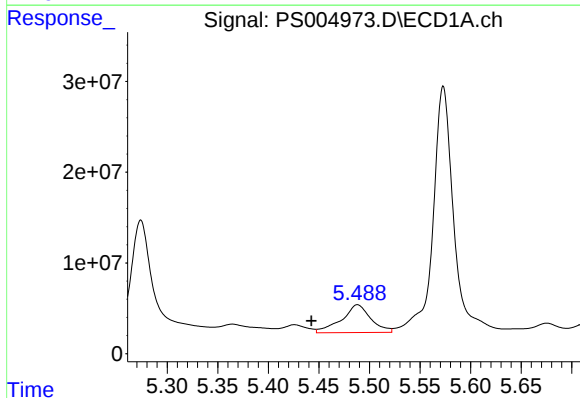


#3 4-Nitrophenol

R.T.: 5.488 min
Delta R.T.: 0.046 min
Response: 61487476
Conc: 98.62 ng/ml

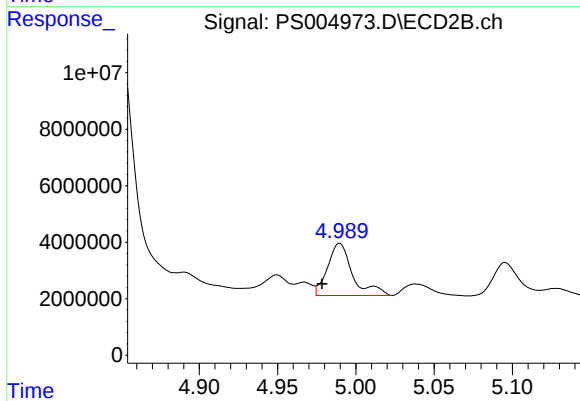

#3 4-Nitrophenol


R.T.: 4.990 min
Delta R.T.: 0.011 min
Response: 20504776
Conc: 43.27 ng/ml

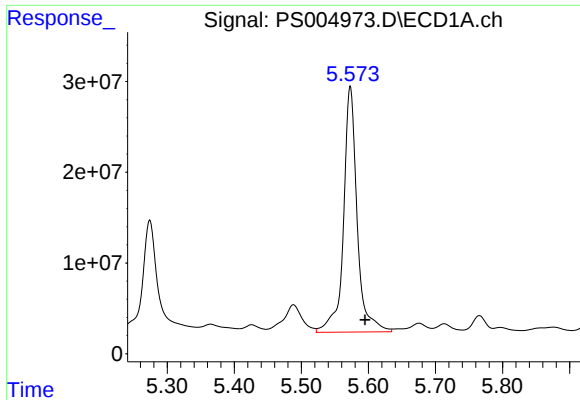

#4 2,4-DCAA


R.T.: 5.573 min
Delta R.T.: -0.022 min
Response: 382450798
Conc: 272.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

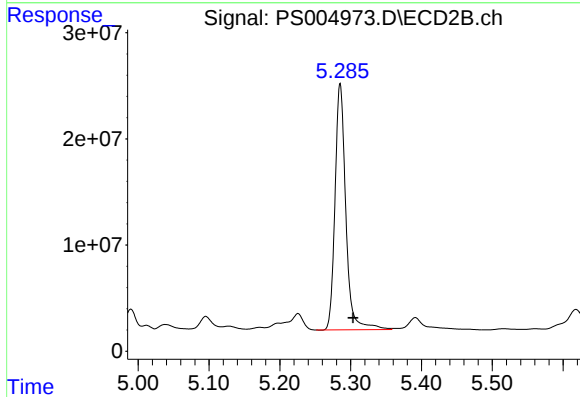


#4 2,4-DCAA

R.T.: 5.285 min
Delta R.T.: -0.018 min
Response: 245785842
Conc: 254.74 ng/ml

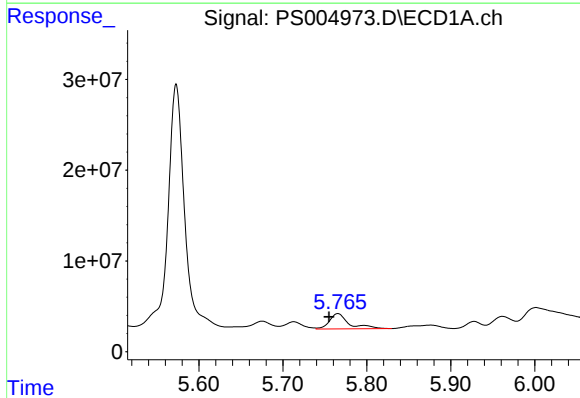


#5 DICAMBA

R.T.: 5.766 min
Delta R.T.: 0.010 min
Response: 27082993
Conc: 5.10 ng/ml

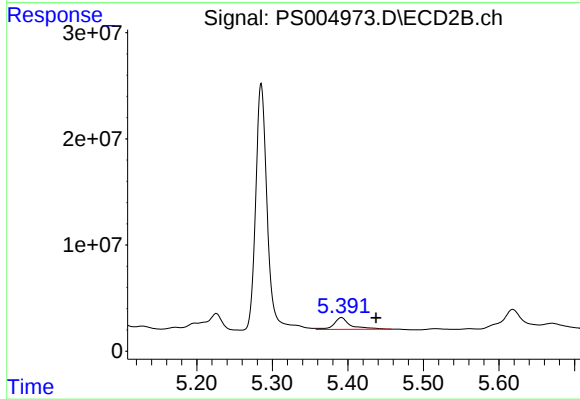

#5 DICAMBA


R.T.: 5.391 min
Delta R.T.: -0.046 min
Response: 17375279
Conc: 4.70 ng/ml

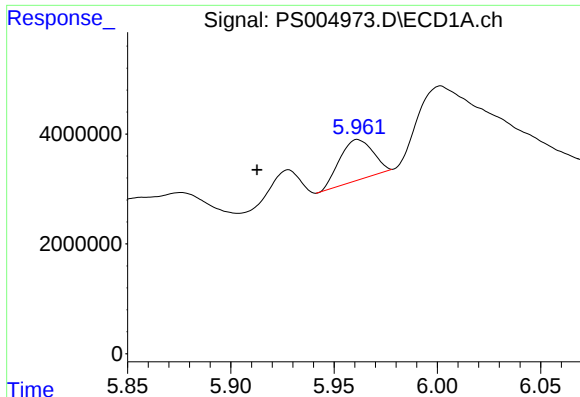

#6 MCPP


R.T.: 5.962 min
Delta R.T.: 0.049 min
Response: 8261101
Conc: 1.98 ug/ml

Instrument :
ECD_S
ClientSampleId :

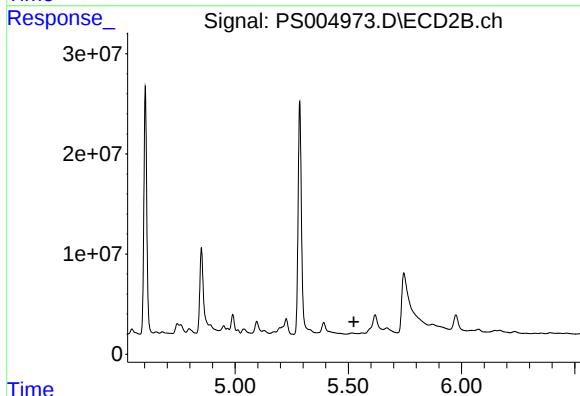


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

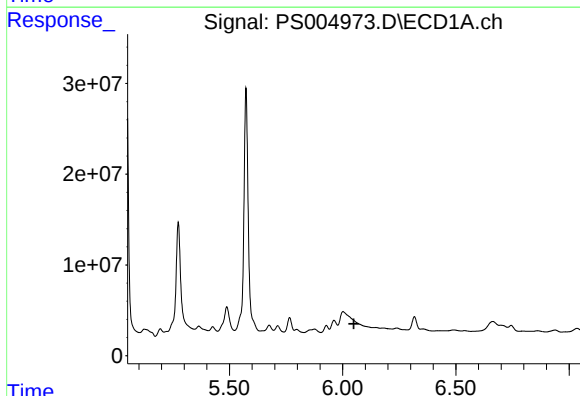


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

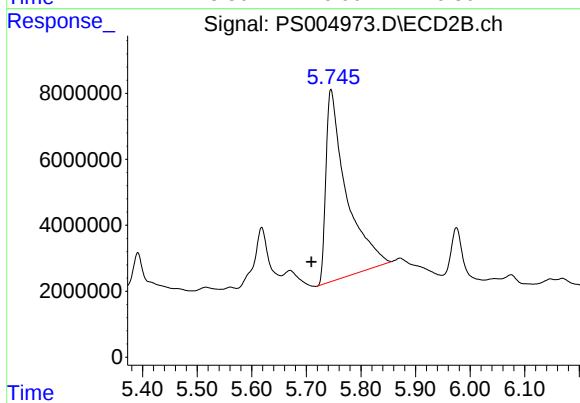

#7 MCPA


R.T.: 5.746 min
Delta R.T.: 0.037 min
Response: 151339508
Conc: 36.99 ug/ml

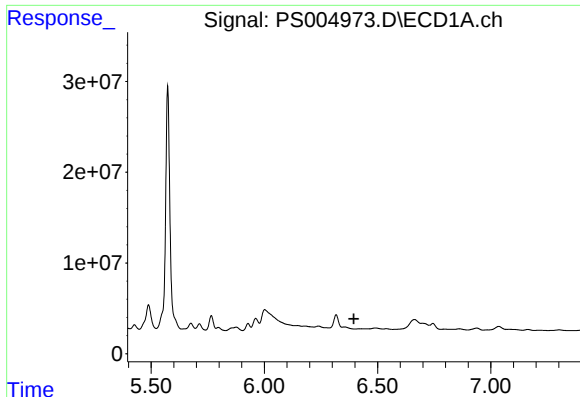

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

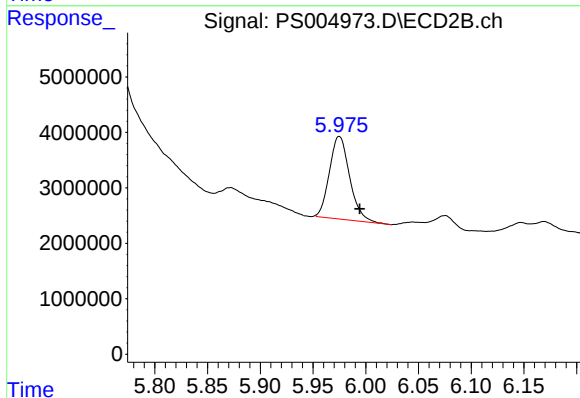


#8 DICHLORPROP

R.T.: 5.975 min
Delta R.T.: -0.019 min
Response: 19916163
Conc: 21.12 ng/ml

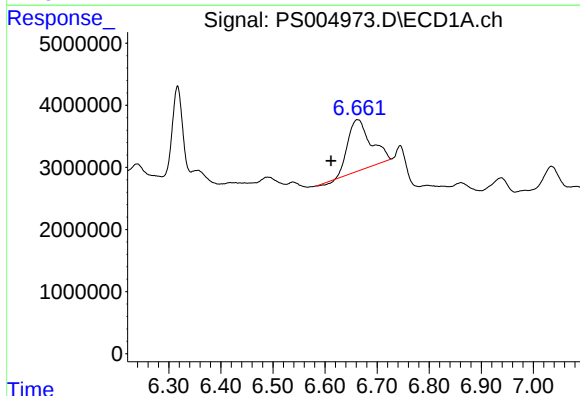


#9 2,4-D

R.T.: 6.663 min
Delta R.T.: 0.051 min
Response: 24791530
Conc: 18.12 ng/ml

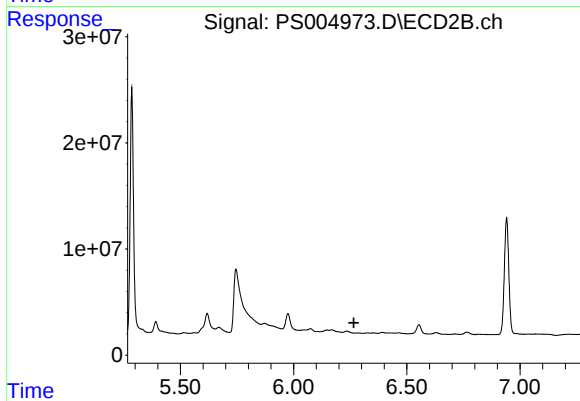

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

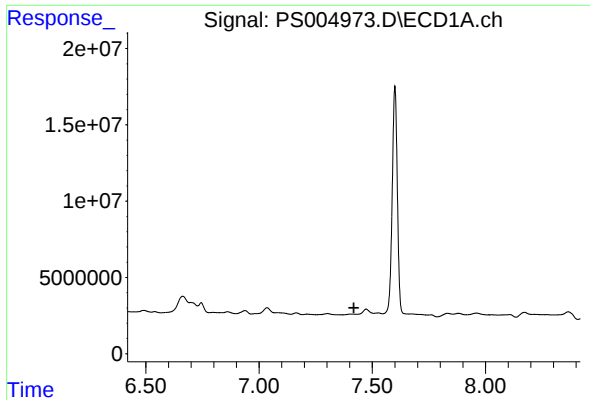

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

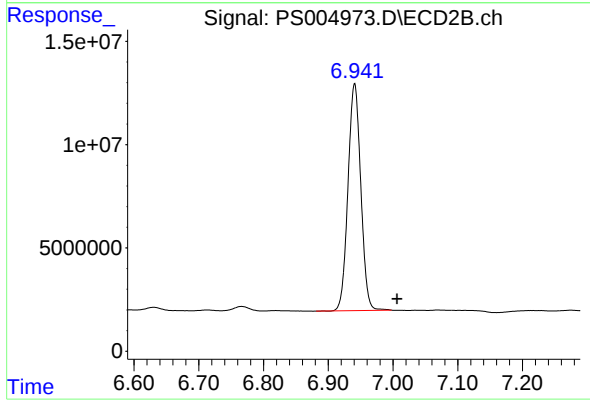

#11 2,4,5-TP (SILVEX)

R.T.: 6.941 min
Delta R.T.: -0.066 min
Response: 150690838
Conc: 29.29 ng/ml