

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
 Data File : PS004976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2019 18:51
 Operator : SM\AJ
 Sample : K3153-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 23:00:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.572	5.284	464.4E6	314.8E6	331.275	326.282
Target Compounds							
2) T	3,5-DICHL...	0.000	4.603	0	250.1E6	N.D.	202.969
5) T	DICAMBA	0.000	5.391	0	16432048	N.D.	4.448
6) T	MCP	5.927	0.000	6560159	0	1.576	N.D. #
7) T	MCPA	0.000	5.742	0	302.2E6	N.D.	73.858
8) T	DICHLORPROP	0.000	5.973	0	22346300	N.D.	23.701
9) T	2,4-D	6.677	0.000	80087718	0	58.548	N.D. #
11) T	2,4,5-TP ...	0.000	6.942	0	308.1E6	N.D.	59.888



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
Data File : PS004976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2019 18:51
Operator : SM\AJ
Sample : K3153-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 23:00:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

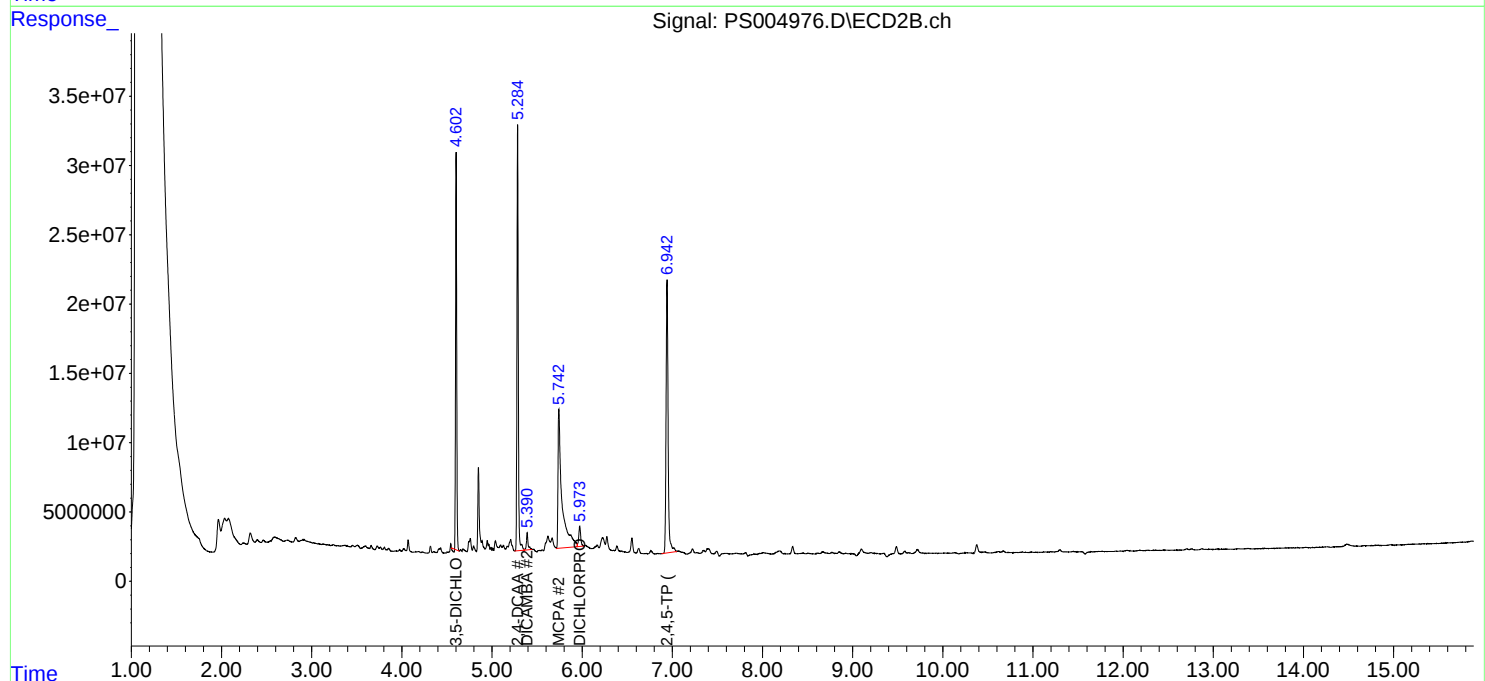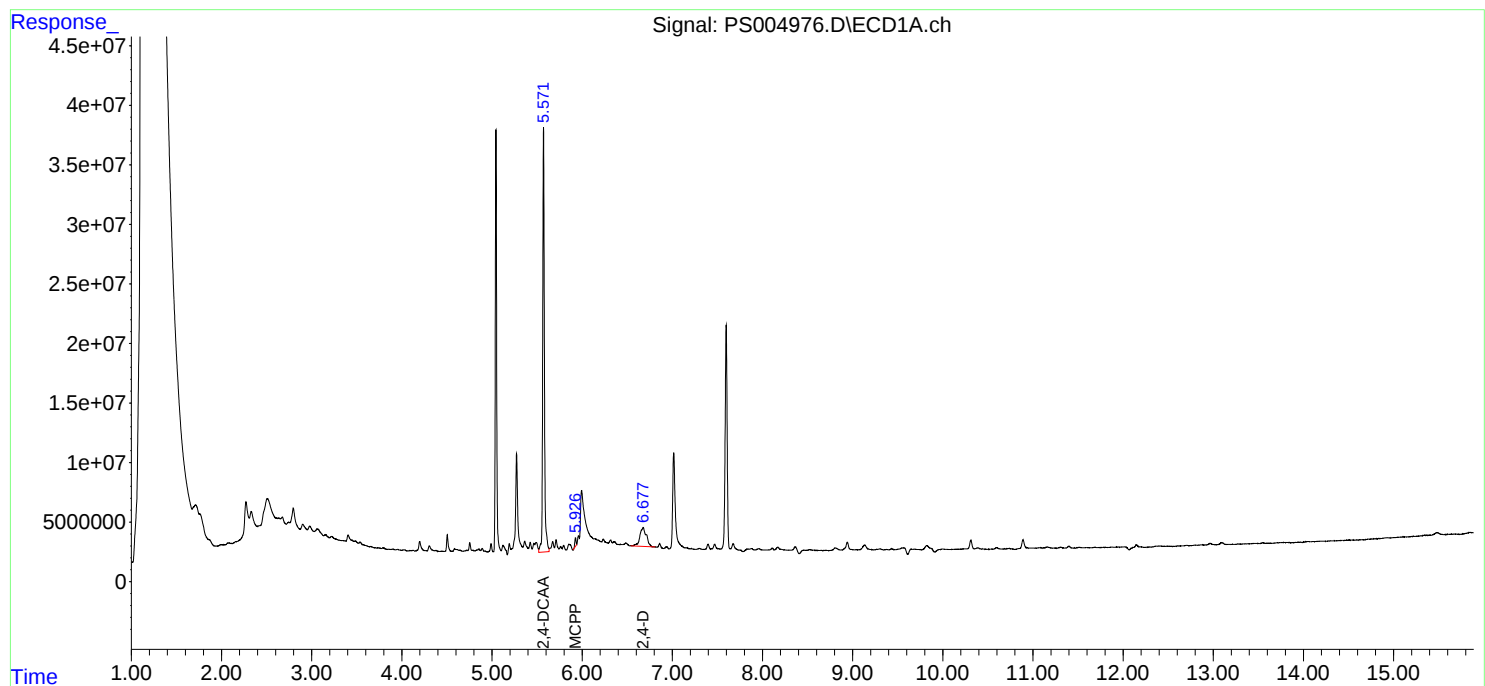


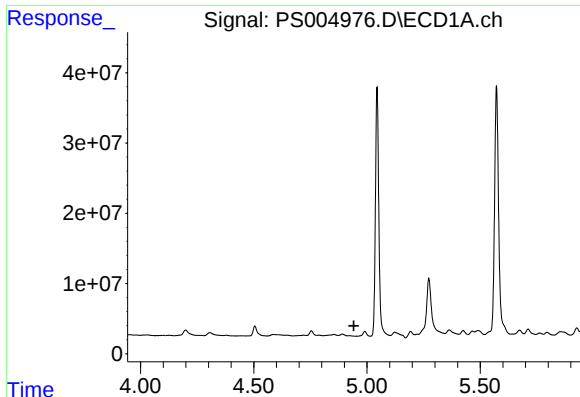

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

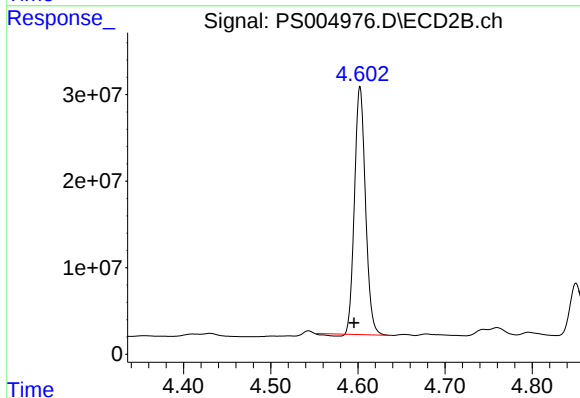


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.603 min
Delta R.T.: 0.007 min
Response: 250083384
Conc: 202.97 ng/ml

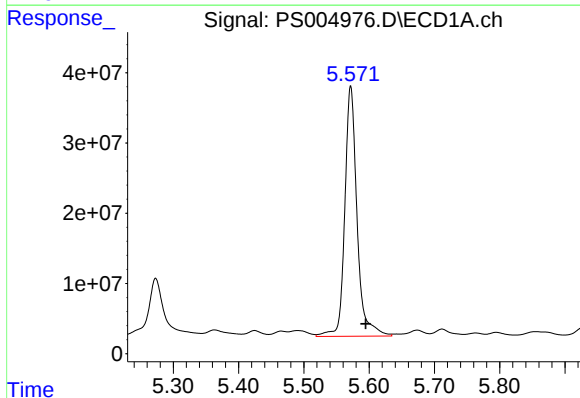


#4 2,4-DCAA

R.T.: 5.572 min
Delta R.T.: -0.023 min
Response: 464367288
Conc: 331.28 ng/ml

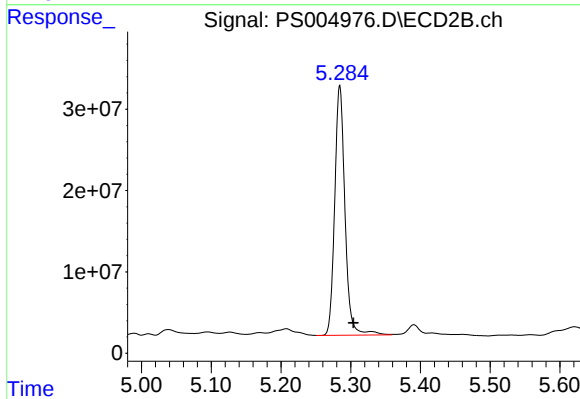

#4 2,4-DCAA


R.T.: 5.284 min
Delta R.T.: -0.019 min
Response: 314808370
Conc: 326.28 ng/ml

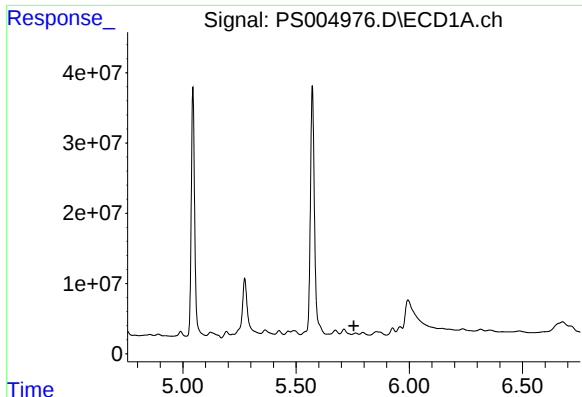

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

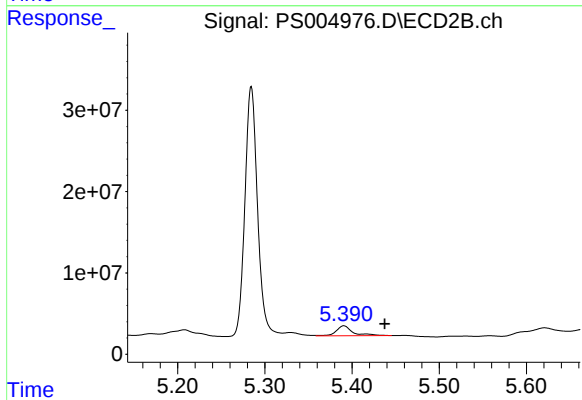


#5 DICAMBA

R.T.: 5.391 min
Delta R.T.: -0.047 min
Response: 16432048
Conc: 4.45 ng/ml

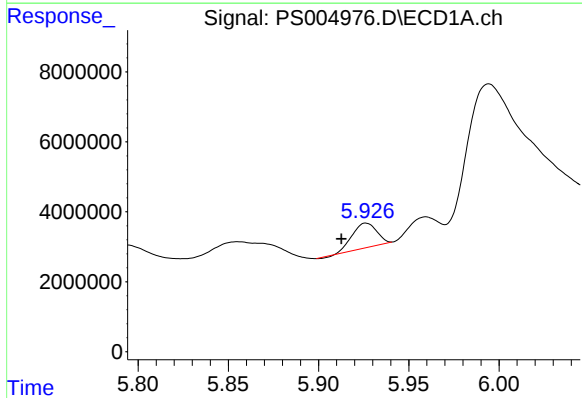


#6 MCPP

R.T.: 5.927 min
Delta R.T.: 0.014 min
Response: 6560159
Conc: 1.58 ug/ml

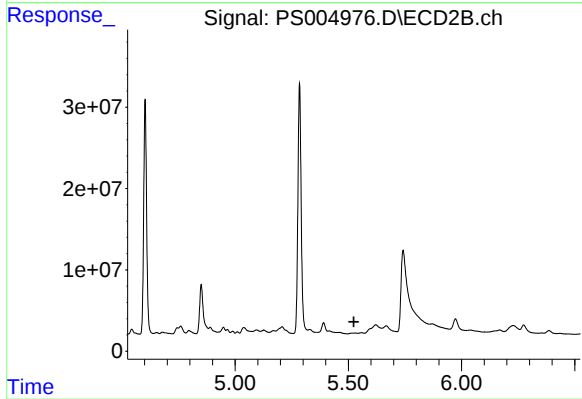

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

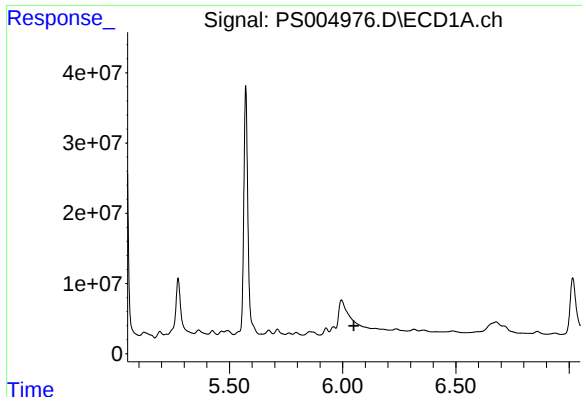

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

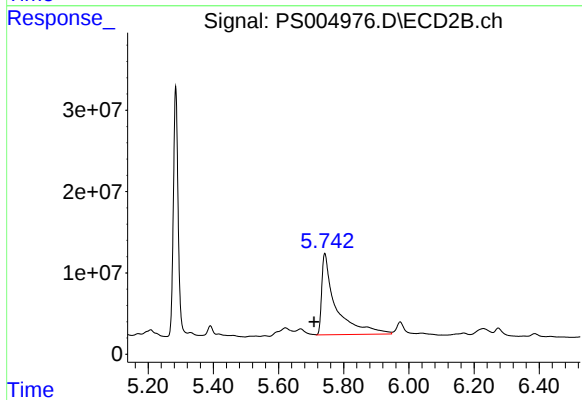


#7 MCPA

R.T.: 5.742 min
Delta R.T.: 0.033 min
Response: 302201088
Conc: 73.86 ug/ml

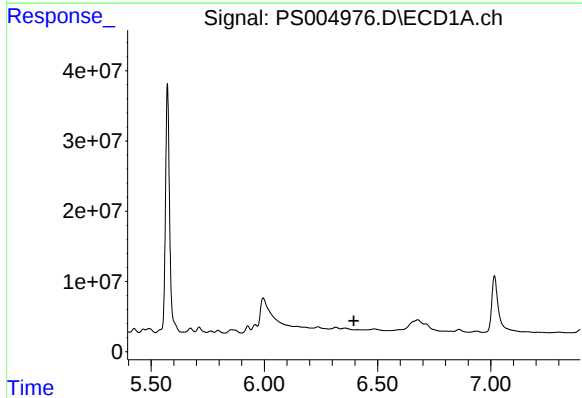


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

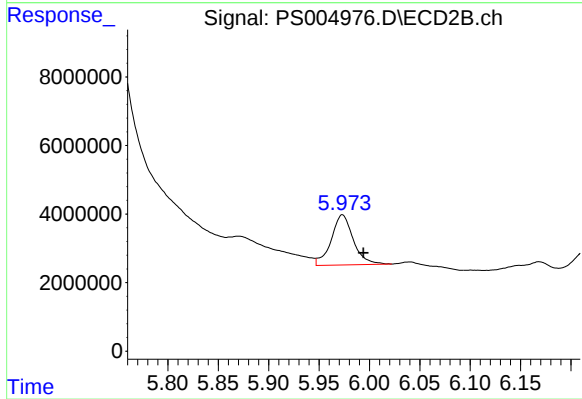

#8 DICHLORPROP


R.T.: 5.973 min
Delta R.T.: -0.021 min
Response: 22346300
Conc: 23.70 ng/ml

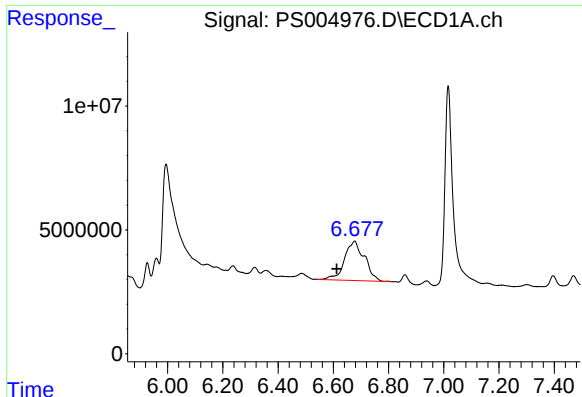

#9 2,4-D


R.T.: 6.677 min
Delta R.T.: 0.065 min
Response: 80087718
Conc: 58.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

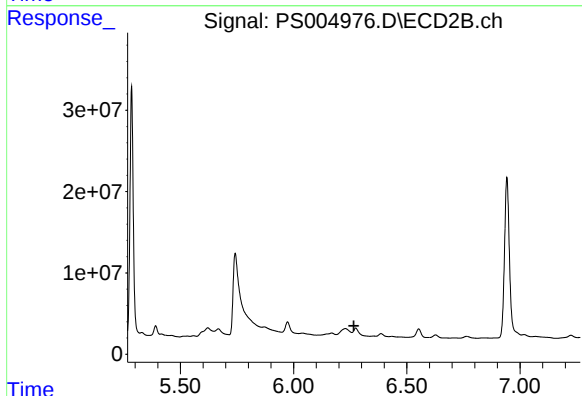


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

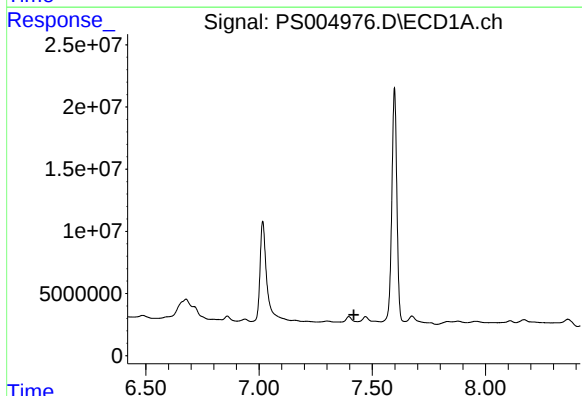

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

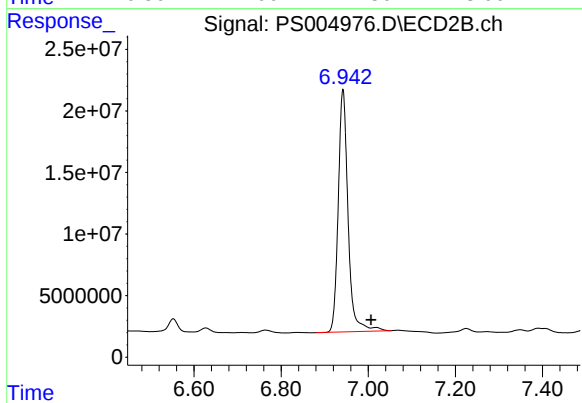

#11 2,4,5-TP (SILVEX)

R.T.: 6.942 min
Delta R.T.: -0.064 min
Response: 308144680
Conc: 59.89 ng/ml