

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
 Data File : PS004977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2019 19:13
 Operator : SM\AJ
 Sample : K3153-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 23:00:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.578	5.291	333.0E6	233.8E6	237.579	242.326
Target Compounds							
2) T	3,5-DICHL...	0.000	4.609	0	194.0E6	N.D.	157.445
5) T	DICAMBA	0.000	5.397	0	10362875	N.D.	2.805
7) T	MCPA	0.000	5.748	0	336.8E6	N.D.	82.322
8) T	DICHLORPROP	0.000	5.980	0	19425099	N.D.	20.603
9) T	2,4-D	6.666	0.000	63011375	0	46.064	N.D. #
11) T	2,4,5-TP ...	0.000	6.947	0	170.3E6	N.D.	33.095



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
Data File : PS004977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2019 19:13
Operator : SM\AJ
Sample : K3153-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 23:00:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

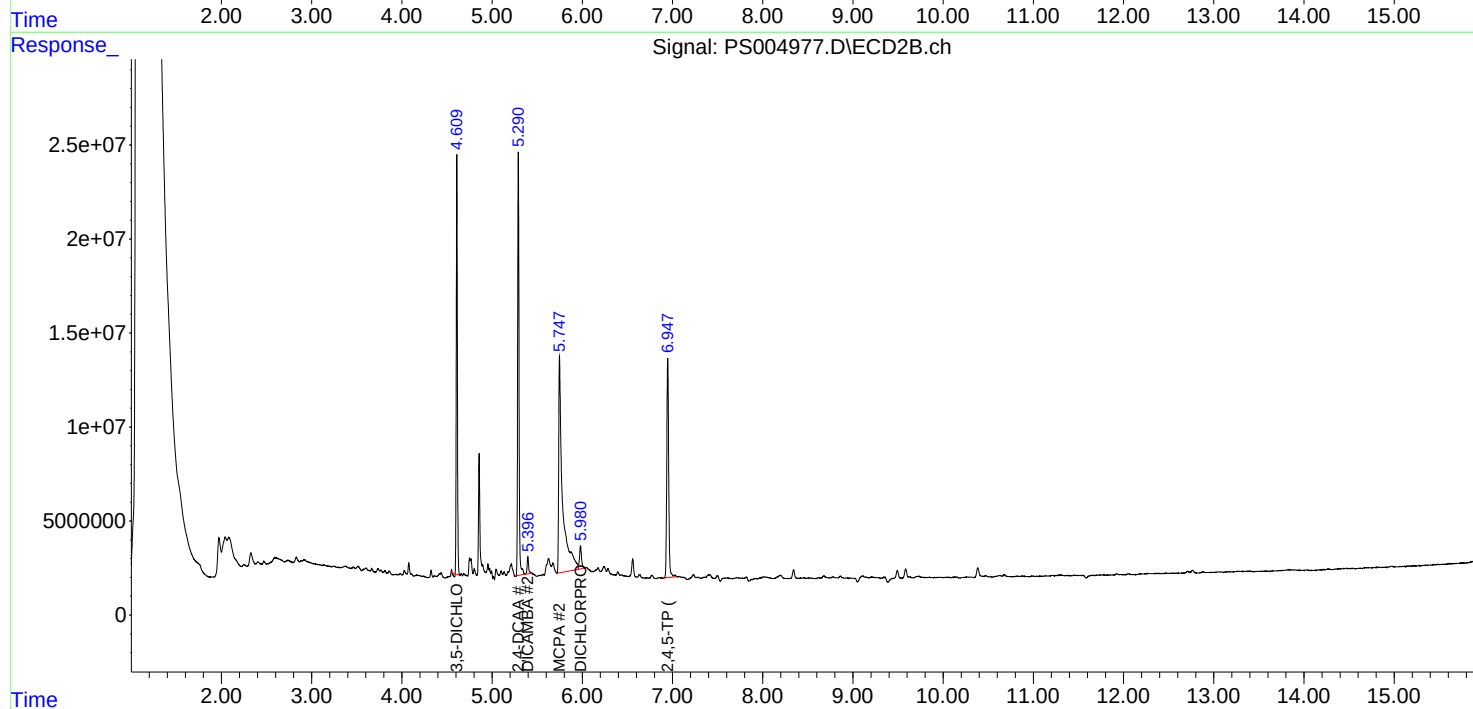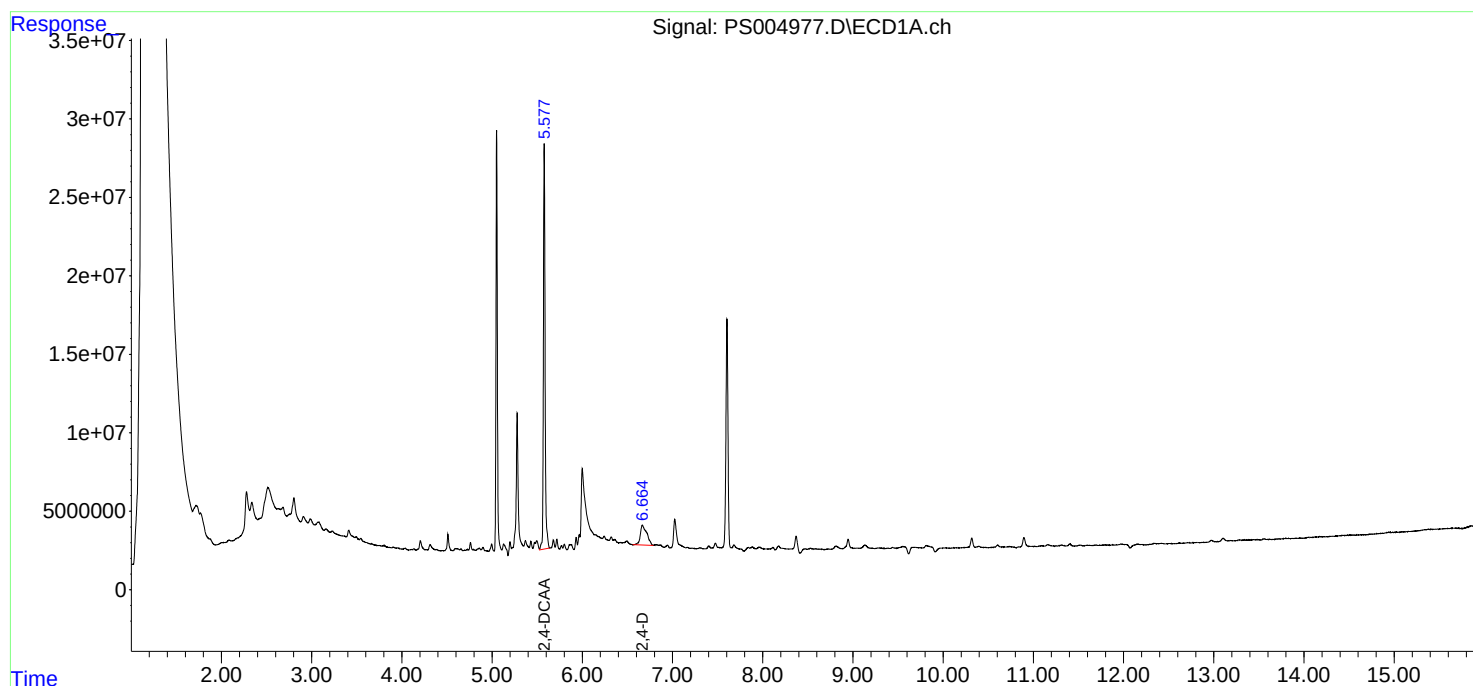


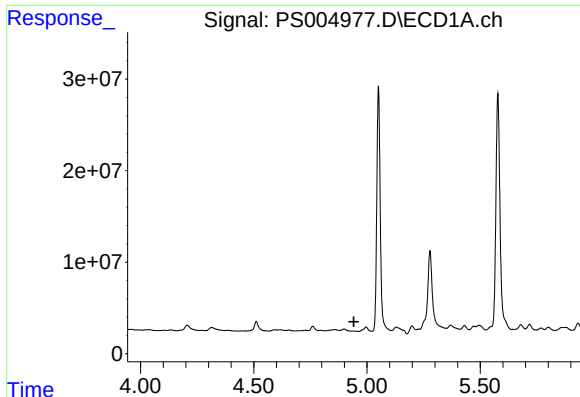

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

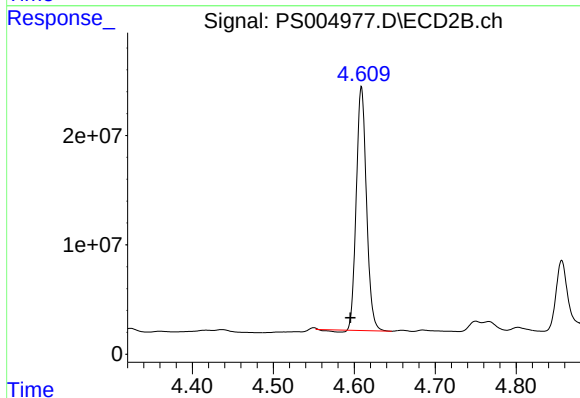


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.609 min
Delta R.T.: 0.013 min
Response: 193992470
Conc: 157.45 ng/ml

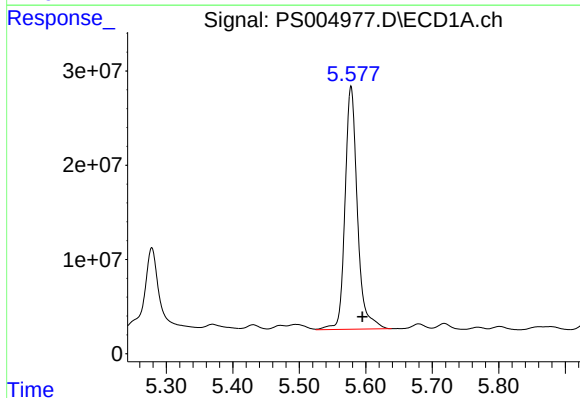


#4 2,4-DCAA

R.T.: 5.578 min
Delta R.T.: -0.017 min
Response: 333028001
Conc: 237.58 ng/ml

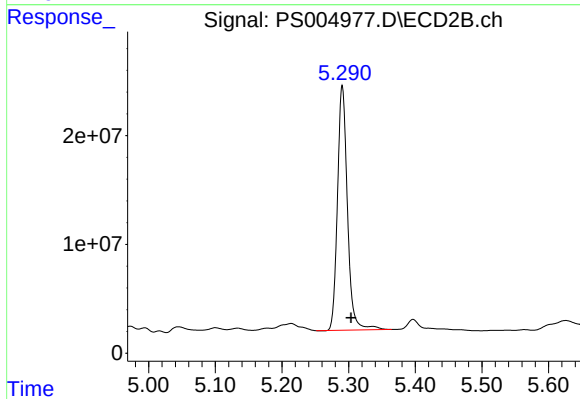

#4 2,4-DCAA


R.T.: 5.291 min
Delta R.T.: -0.013 min
Response: 233804523
Conc: 242.33 ng/ml

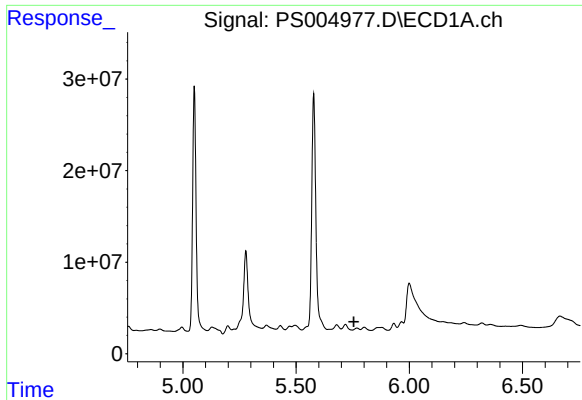

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

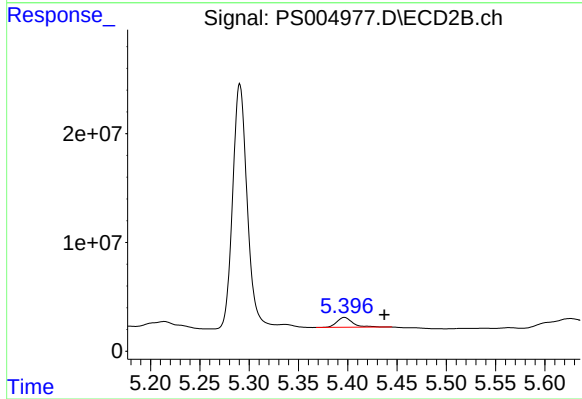


#5 DICAMBA

R.T.: 5.397 min
Delta R.T.: -0.041 min
Response: 10362875
Conc: 2.81 ng/ml

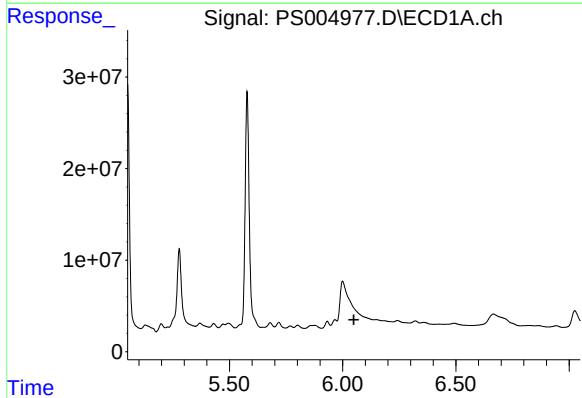


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

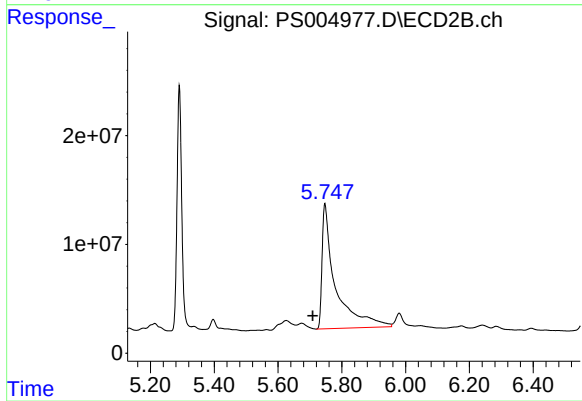

#7 MCPA


R.T.: 5.748 min
Delta R.T.: 0.038 min
Response: 336833137
Conc: 82.32 ug/ml

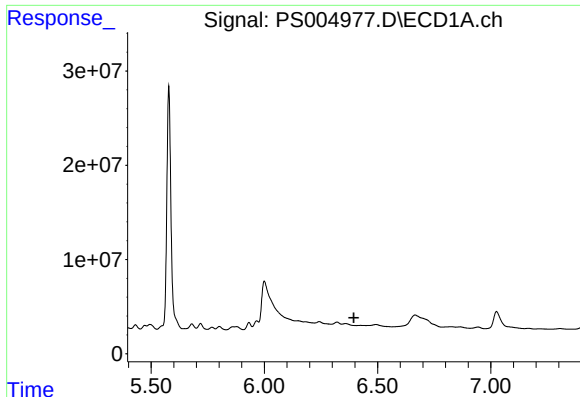

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

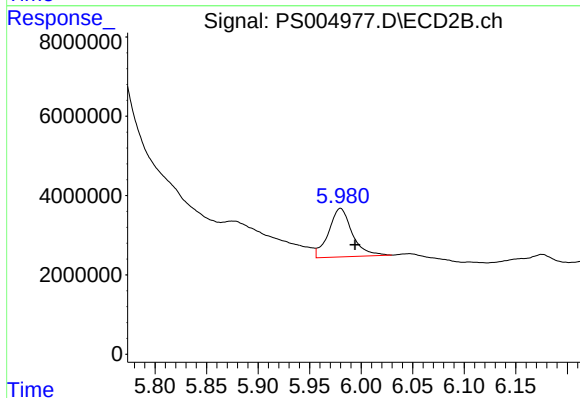


#8 DICHLORPROP

R.T.: 5.980 min
Delta R.T.: -0.014 min
Response: 19425099
Conc: 20.60 ng/ml

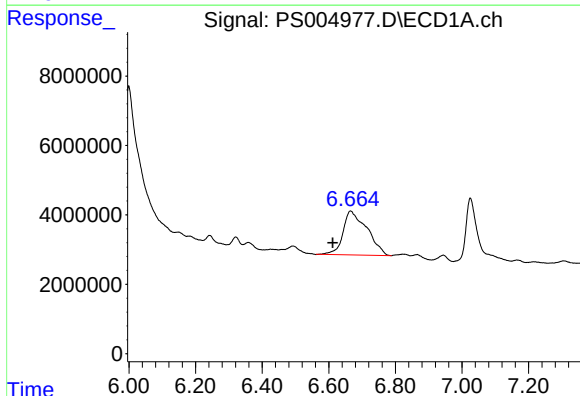


#9 2,4-D

R.T.: 6.666 min
Delta R.T.: 0.054 min
Response: 63011375
Conc: 46.06 ng/ml

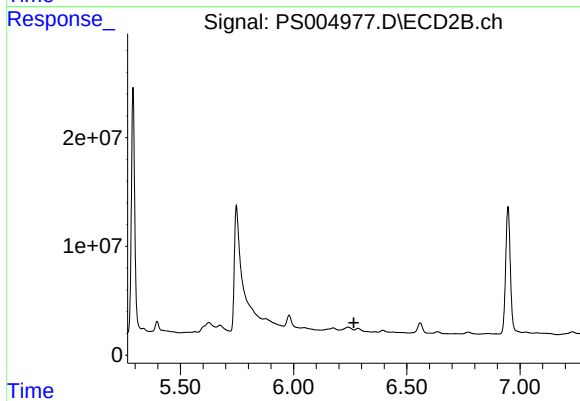

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

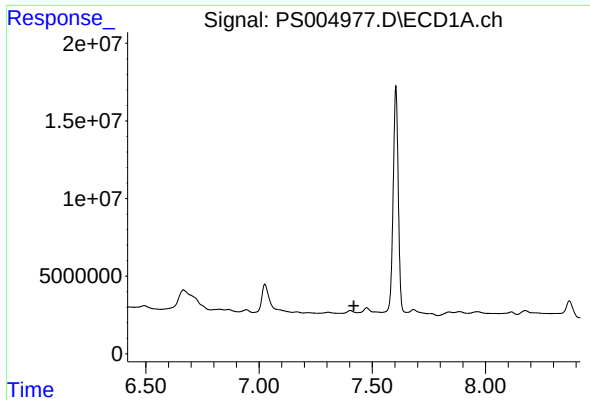

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

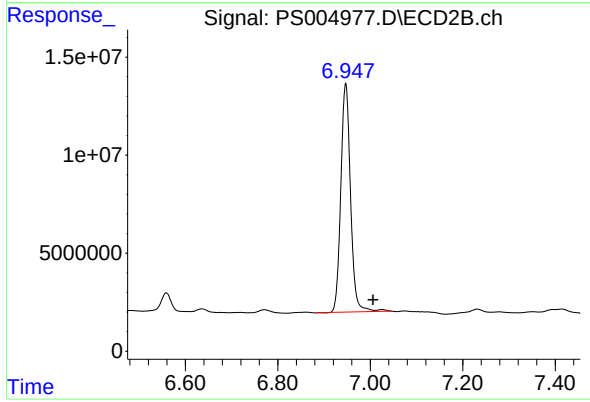

#11 2,4,5-TP (SILVEX)

R.T.: 6.947 min
Delta R.T.: -0.059 min
Response: 170282505
Conc: 33.09 ng/ml