

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
 Data File : PS004978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2019 19:36
 Operator : SM\AJ
 Sample : K3156-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 23:00:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.594	5.307	372.3E6	264.9E6	265.623	274.593
Target Compounds							
2) T	3,5-DICHL...	0.000	4.625	0	179.1E6	N.D.	145.330
7) T	MCPA	6.018	5.764	74574700	322.5E6	12.875	78.815 #
8) T	DICHLORPROP	0.000	5.996	0	18433154	N.D.	19.551
9) T	2,4-D	6.681	0.000	54486968	0	39.832	N.D. #
10) T	Pentachlo...	0.000	6.575	0	14497218	N.D.	1.180
11) T	2,4,5-TP ...	0.000	6.963	0	129.2E6	N.D.	25.110



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
Data File : PS004978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2019 19:36
Operator : SM\AJ
Sample : K3156-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 23:00:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

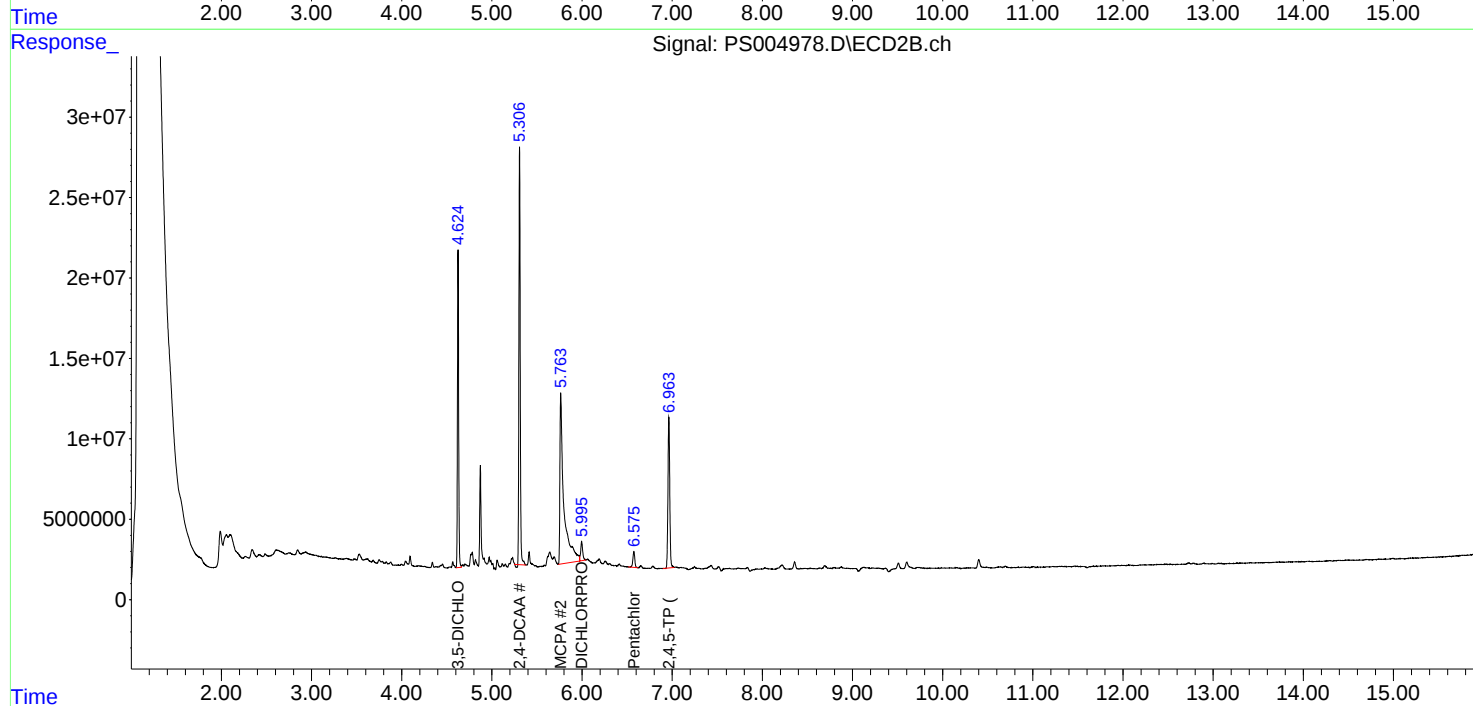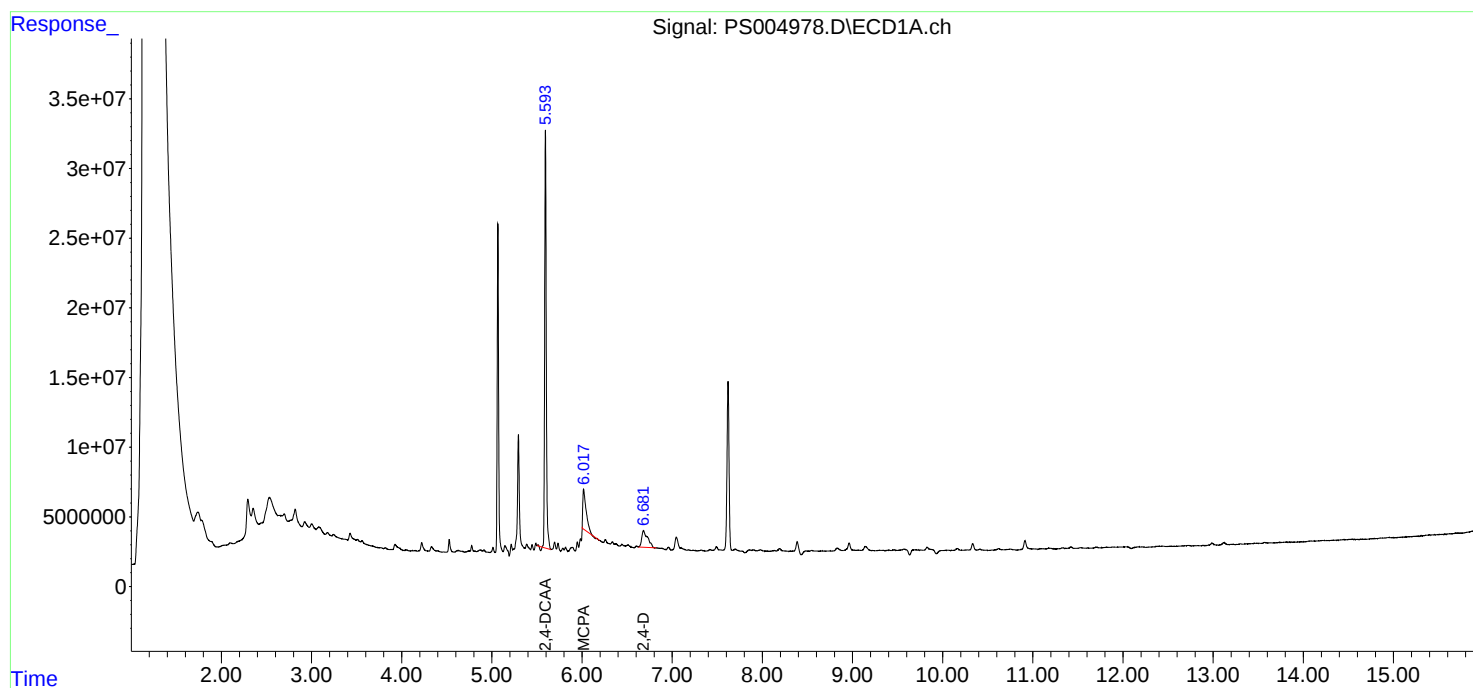


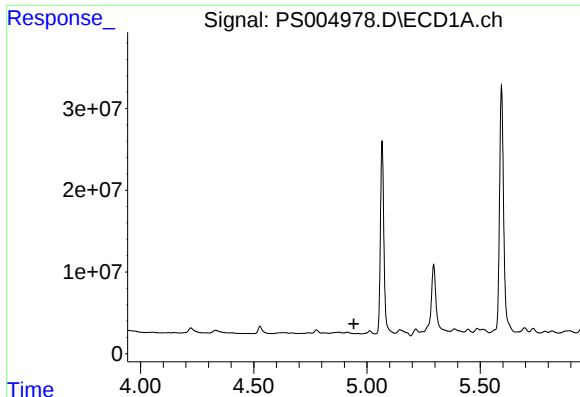

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

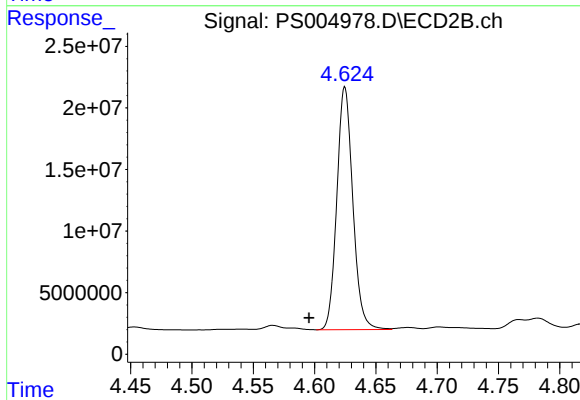


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.625 min
Delta R.T.: 0.029 min
Response: 179064624
Conc: 145.33 ng/ml

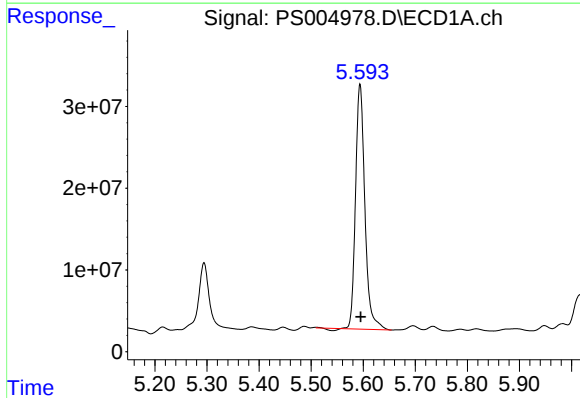


#4 2,4-DCAA

R.T.: 5.594 min
Delta R.T.: -0.001 min
Response: 372338994
Conc: 265.62 ng/ml

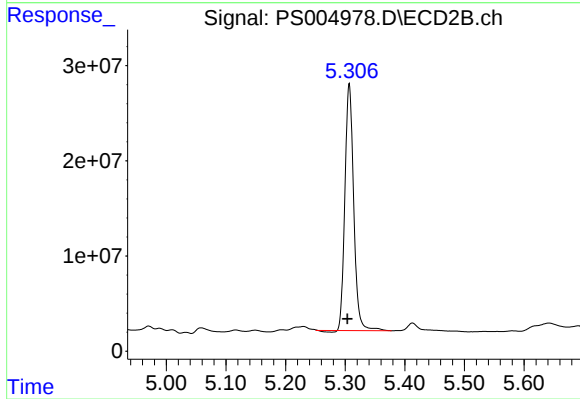

#4 2,4-DCAA


R.T.: 5.307 min
Delta R.T.: 0.003 min
Response: 264937352
Conc: 274.59 ng/ml

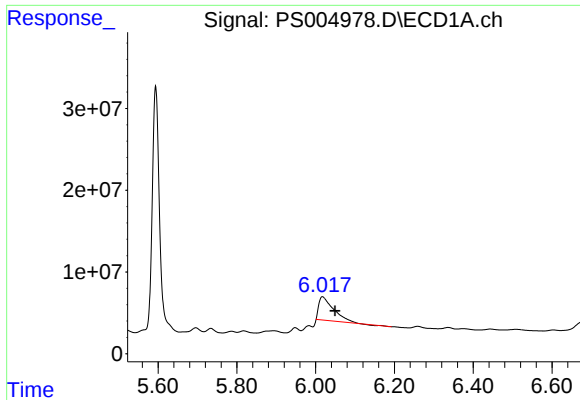

#7 MCPA


R.T.: 6.018 min
Delta R.T.: -0.031 min
Response: 74574700
Conc: 12.88 ug/ml

Instrument :
ECD_S
ClientSampleId :

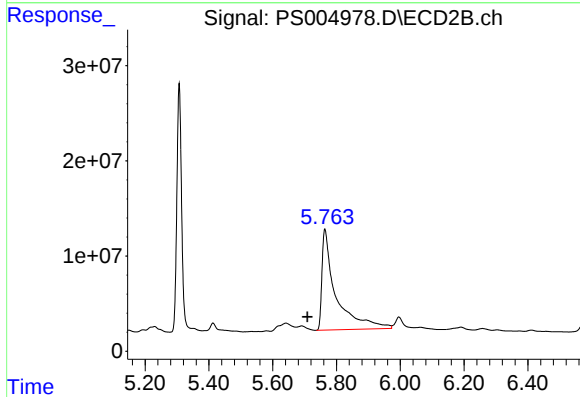


#7 MCPA

R.T.: 5.764 min
Delta R.T.: 0.055 min
Response: 322485279
Conc: 78.82 ug/ml

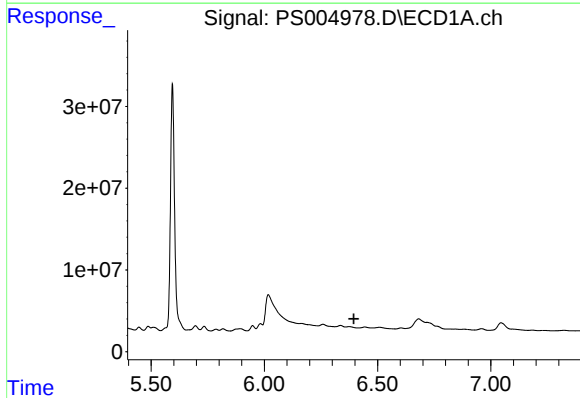


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

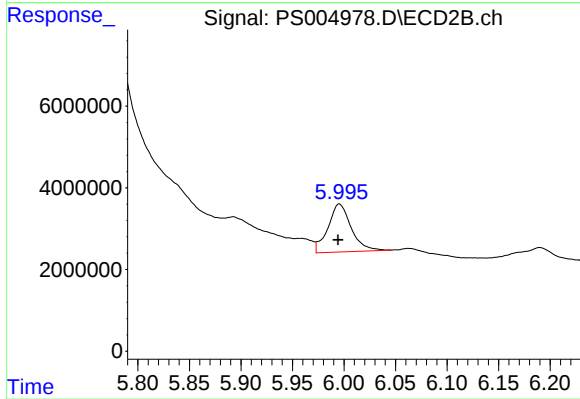

#8 DICHLORPROP


R.T.: 5.996 min
Delta R.T.: 0.002 min
Response: 18433154
Conc: 19.55 ng/ml

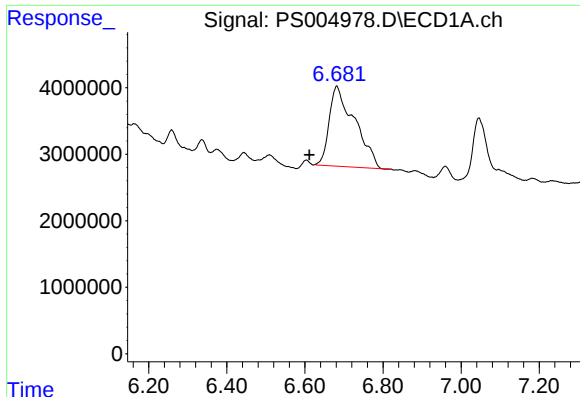

#9 2,4-D


R.T.: 6.681 min
Delta R.T.: 0.070 min
Response: 54486968
Conc: 39.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

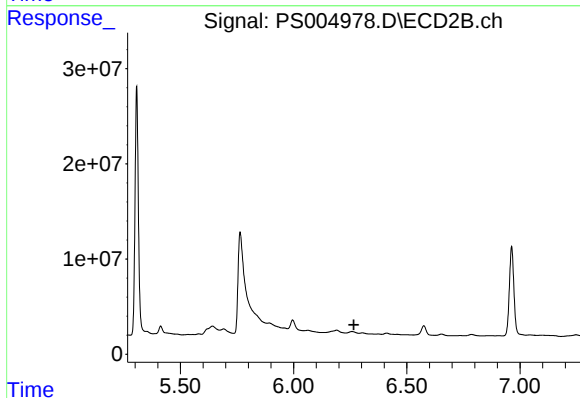


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

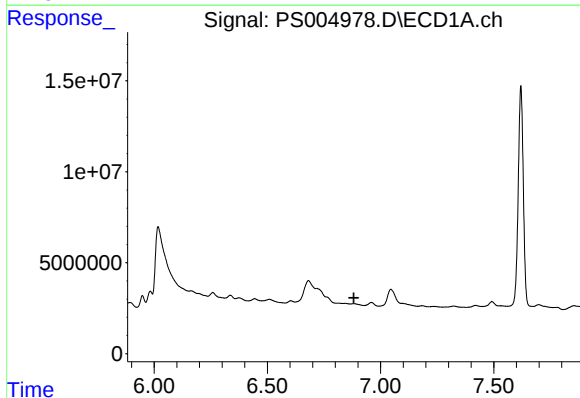


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.882 min
Response: 0
Conc: N.D.

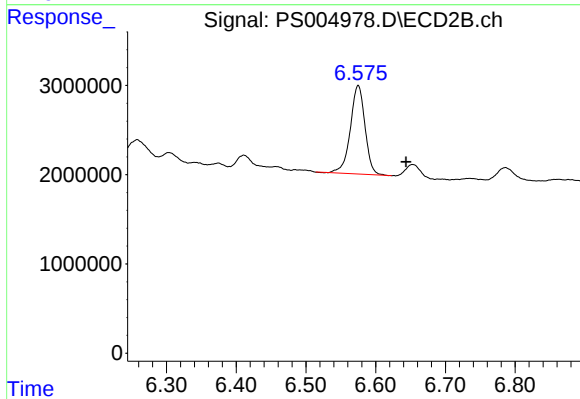

#10 Pentachlorophenol


R.T.: 6.575 min
Delta R.T.: -0.069 min
Response: 14497218
Conc: 1.18 ng/ml

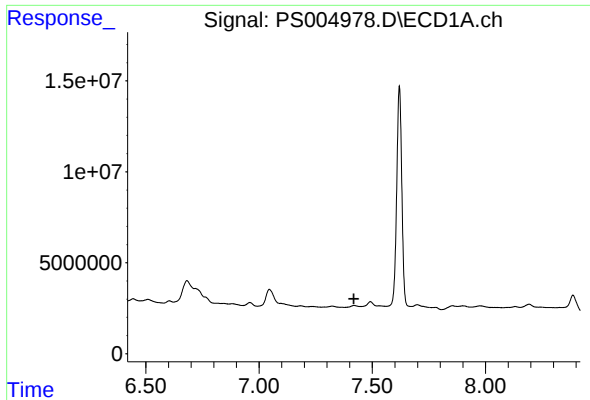

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

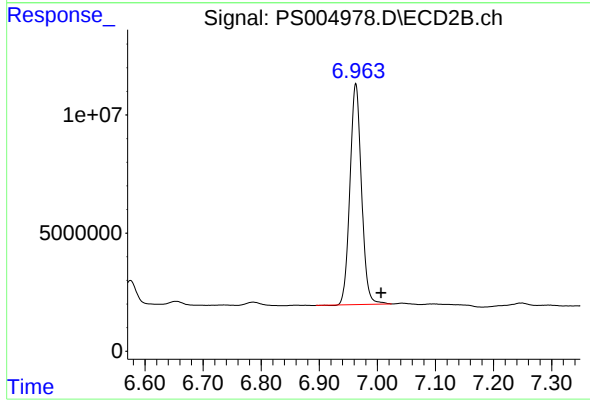

#11 2,4,5-TP (SILVEX)

R.T.: 6.963 min
Delta R.T.: -0.043 min
Response: 129200754
Conc: 25.11 ng/ml