

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
 Data File : PS004979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2019 19:58
 Operator : SM\AJ
 Sample : K3158-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 23:01:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.591	5.288	417.0E6	290.2E6	297.509	300.828
Target Compounds							
2) T	3,5-DICHL...	0.000	4.606	0	275.8E6	N.D.	223.802
5) T	DICAMBA	0.000	5.394	0	14410536	N.D.	3.901
6) T	MCP	5.945	0.000	7598402	0	1.825	N.D. #
7) T	MCPA	0.000	5.744	0	315.4E6	N.D.	77.087
8) T	DICHLORPROP	0.000	5.977	0	20570259	N.D.	21.818
9) T	2,4-D	6.680	0.000	31915024	0	23.331	N.D. #
11) T	2,4,5-TP ...	0.000	6.943	0	186.7E6	N.D.	36.281



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
Data File : PS004979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2019 19:58
Operator : SM\AJ
Sample : K3158-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 23:01:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

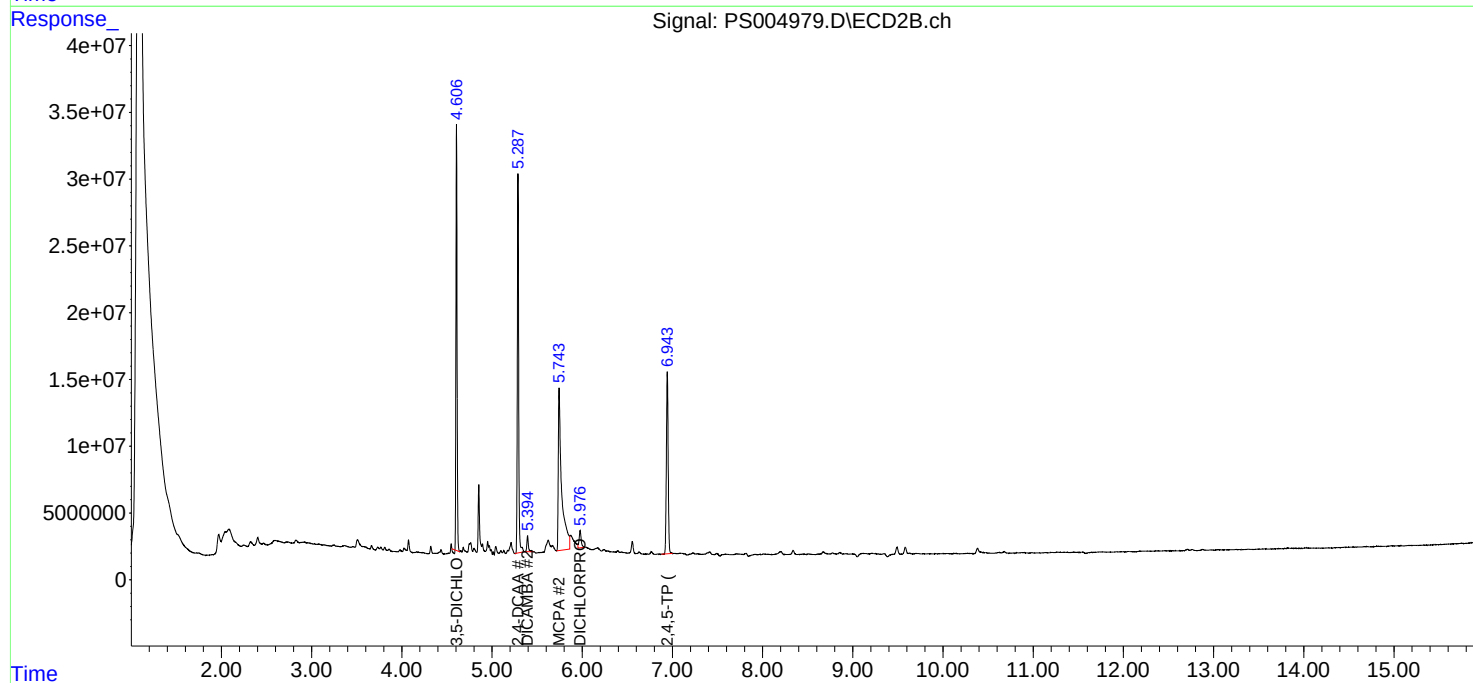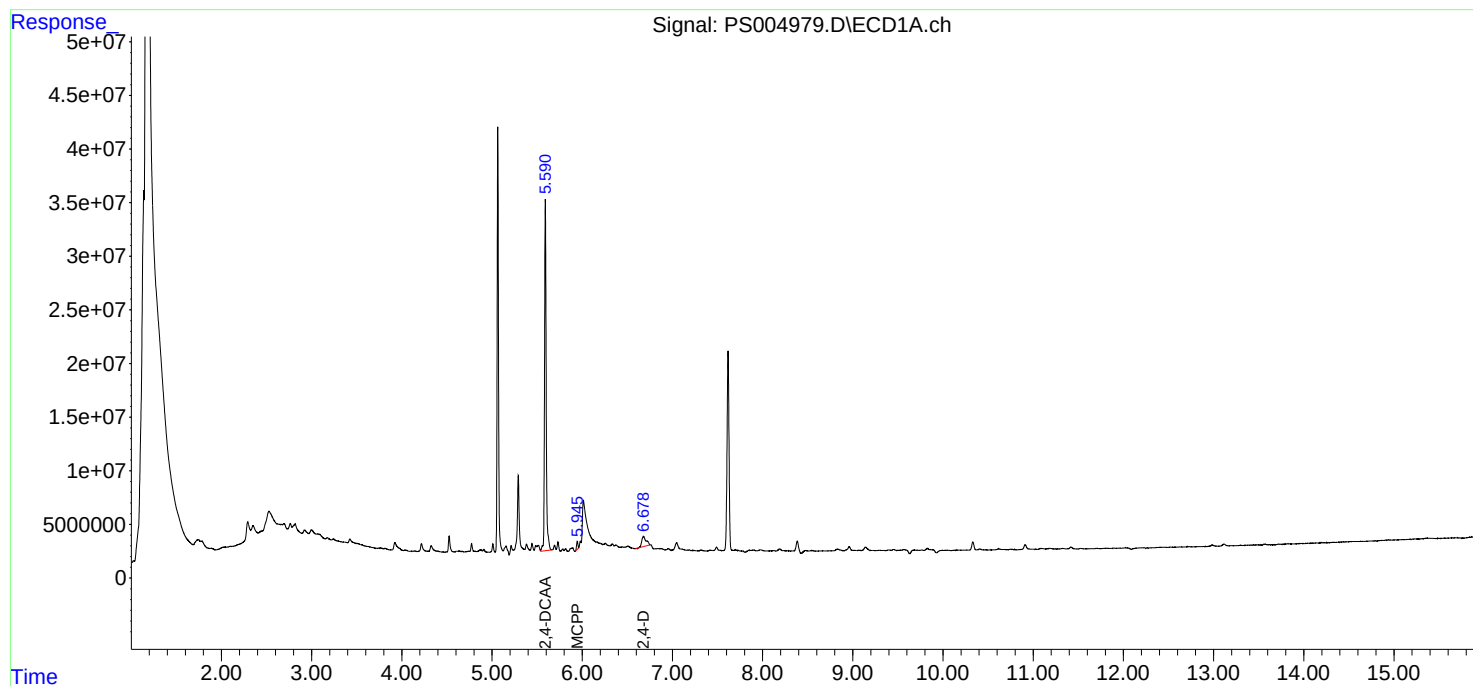


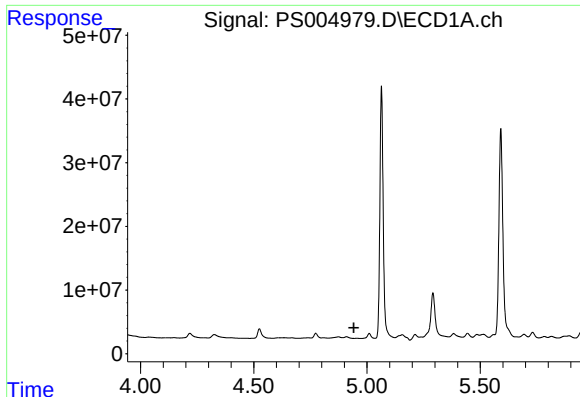

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

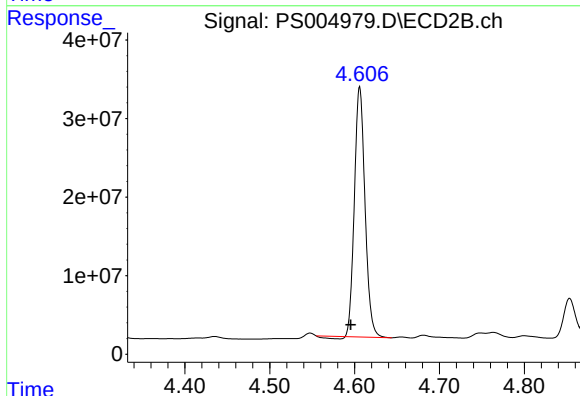


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.606 min
Delta R.T.: 0.011 min
Response: 275753149
Conc: 223.80 ng/ml

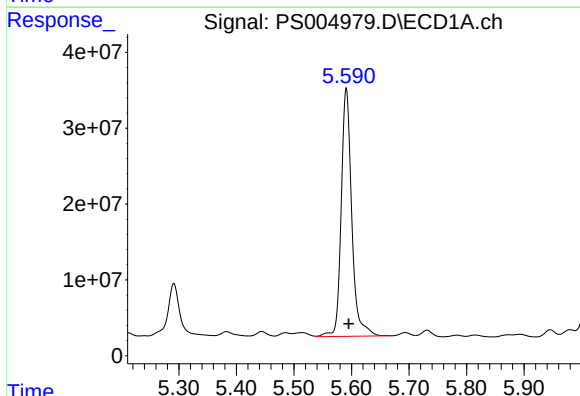


#4 2,4-DCAA

R.T.: 5.591 min
Delta R.T.: -0.004 min
Response: 417034423
Conc: 297.51 ng/ml

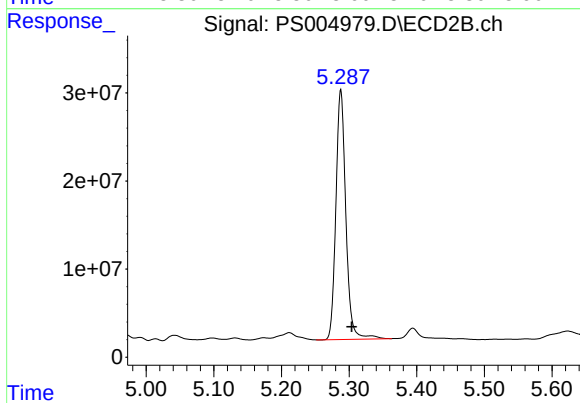

#4 2,4-DCAA


R.T.: 5.288 min
Delta R.T.: -0.016 min
Response: 290249309
Conc: 300.83 ng/ml

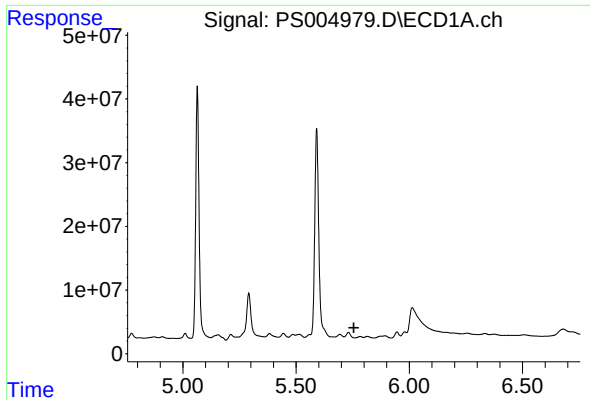

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

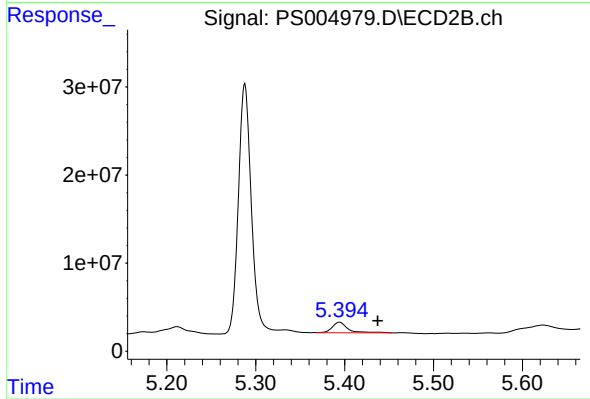


#5 DICAMBA

R.T.: 5.394 min
Delta R.T.: -0.043 min
Response: 14410536
Conc: 3.90 ng/ml

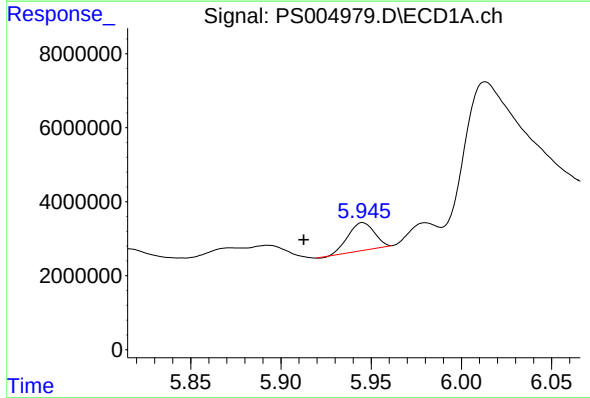


#6 MCP

R.T.: 5.945 min
Delta R.T.: 0.033 min
Response: 7598402
Conc: 1.83 ug/ml

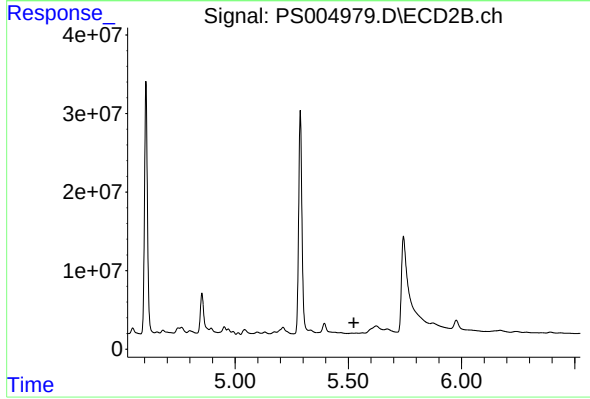

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

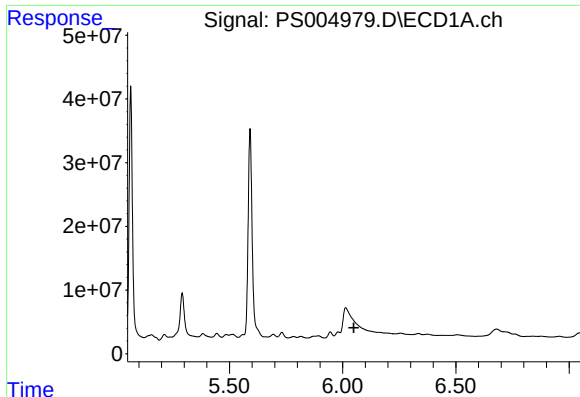

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

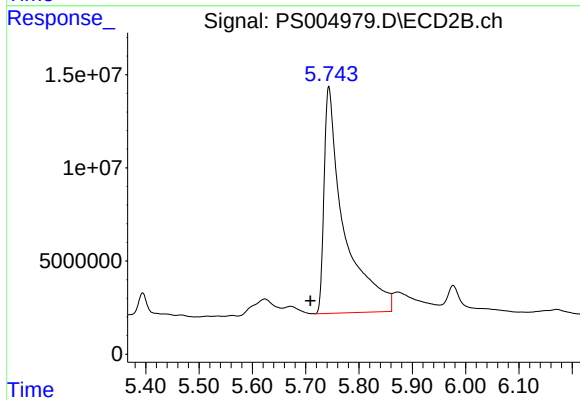


#7 MCPA

R.T.: 5.744 min
Delta R.T.: 0.035 min
Response: 315411872
Conc: 77.09 ug/ml

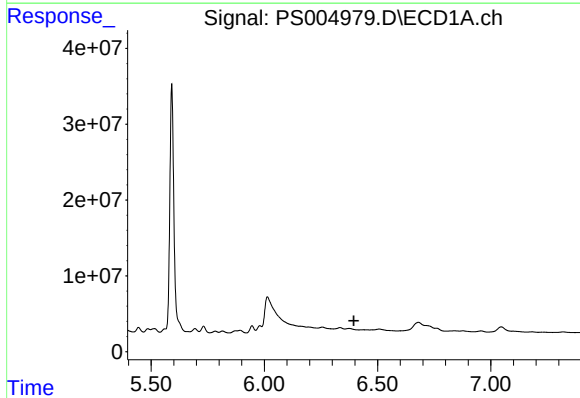


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

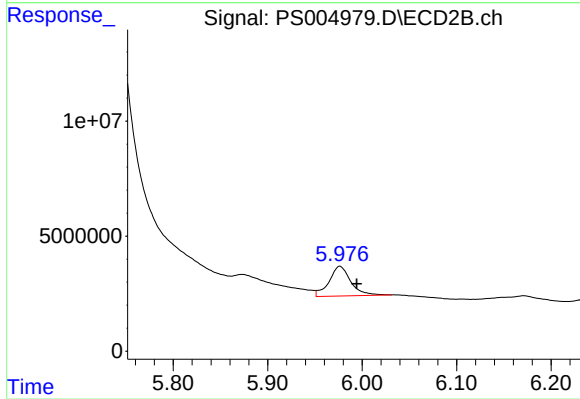

#8 DICHLORPROP


R.T.: 5.977 min
Delta R.T.: -0.018 min
Response: 20570259
Conc: 21.82 ng/ml

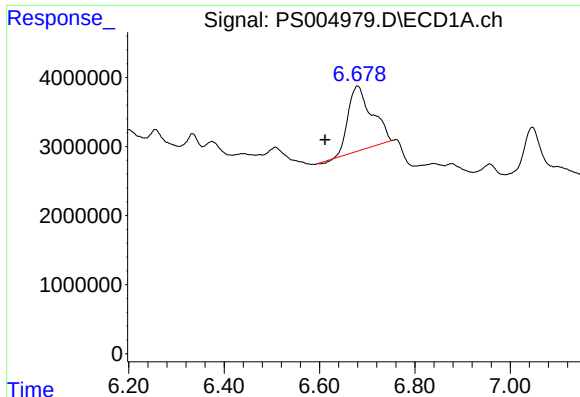

#9 2,4-D


R.T.: 6.680 min
Delta R.T.: 0.068 min
Response: 31915024
Conc: 23.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

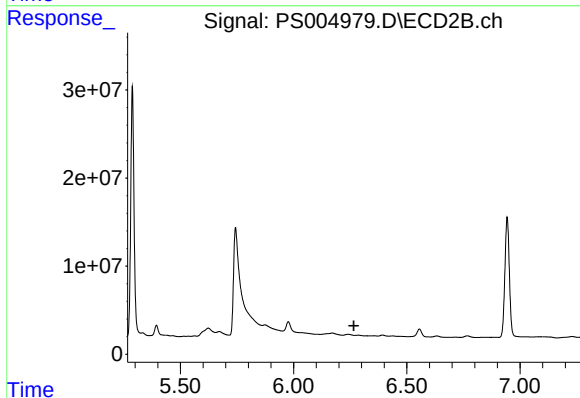


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

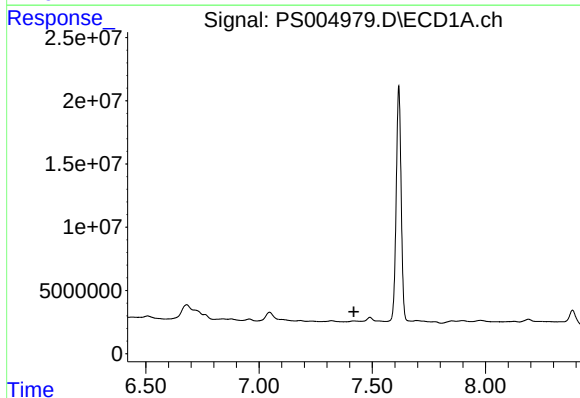

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

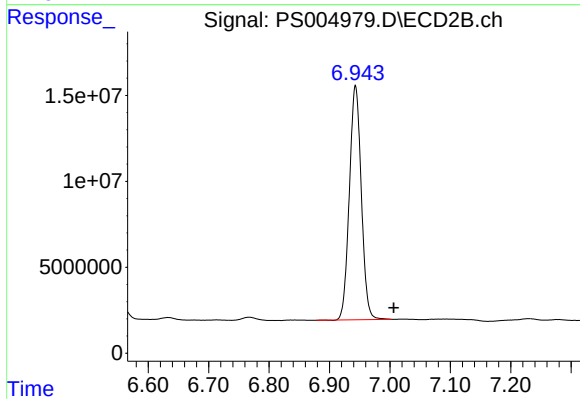

#11 2,4,5-TP (SILVEX)

R.T.: 6.943 min
Delta R.T.: -0.063 min
Response: 186678069
Conc: 36.28 ng/ml