

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
 Data File : PS004980.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2019 20:20
 Operator : SM\AJ
 Sample : K3160-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 23:01:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.587	5.300	456.4E6	296.9E6	325.606	307.673
Target Compounds							
2) T	3,5-DICHL...	5.006	4.618	14887768	287.3E6	8.633	233.142 #
3) T	4-Nitroph...	5.502	5.003	39905627	12656153	64.002	26.705 #
5) T	DICAMBA	5.780	5.406	9555087	14852615	1.800	4.020 #
6) T	MCP	5.941	0.000	8104500	0	1.947	N.D. #
7) T	MCPA	0.000	5.756	0	274.4E6	N.D.	67.052
8) T	DICHLORPROP	0.000	5.988	0	19555053	N.D.	20.741
9) T	2,4-D	6.676	0.000	27507741	0	20.109	N.D. #
11) T	2,4,5-TP ...	0.000	6.955	0	193.1E6	N.D.	37.536



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
Data File : PS004980.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2019 20:20
Operator : SM\AJ
Sample : K3160-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 23:01:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

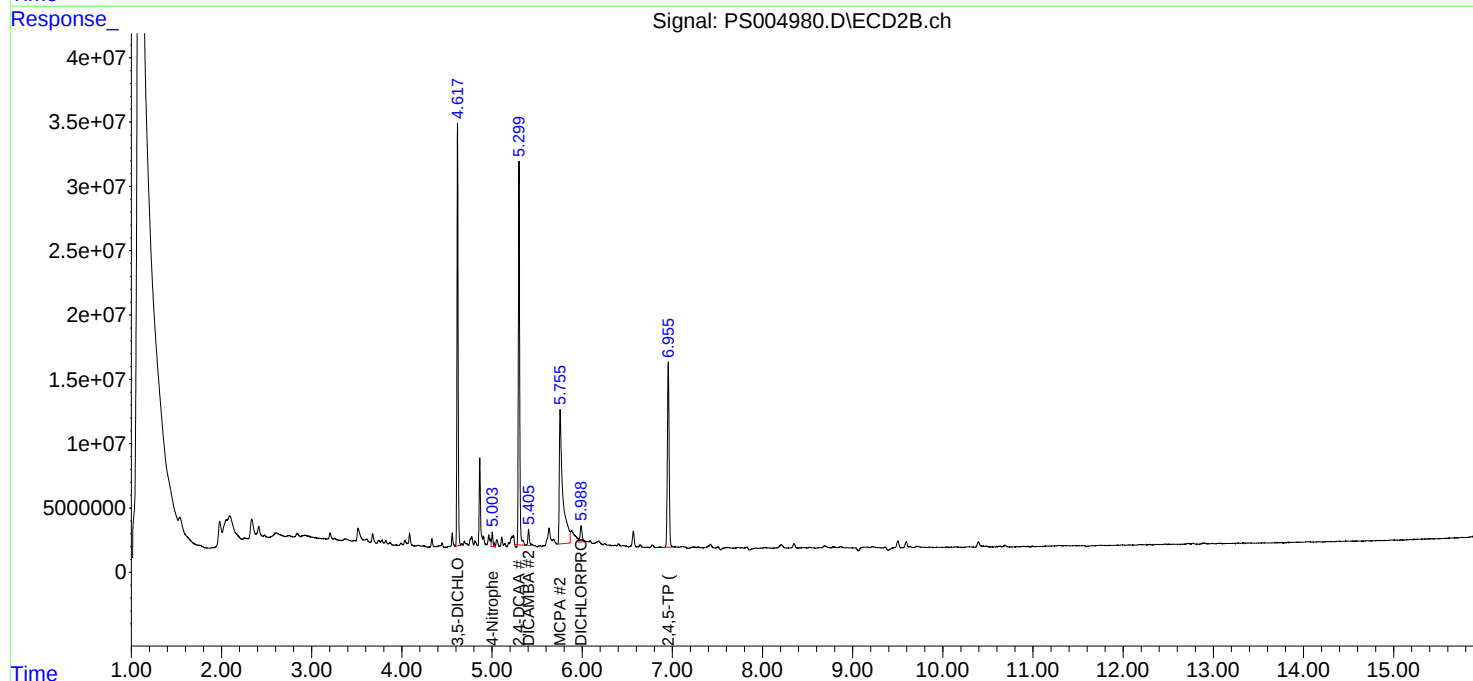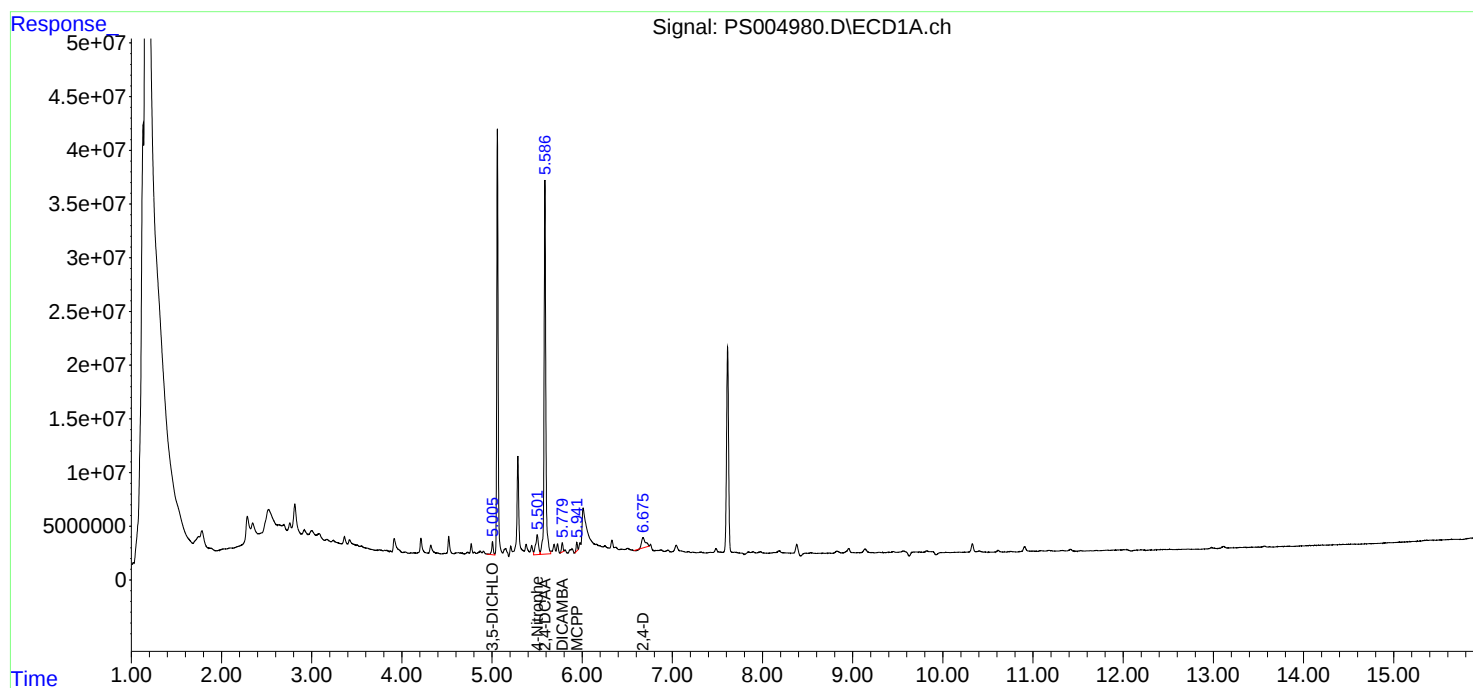


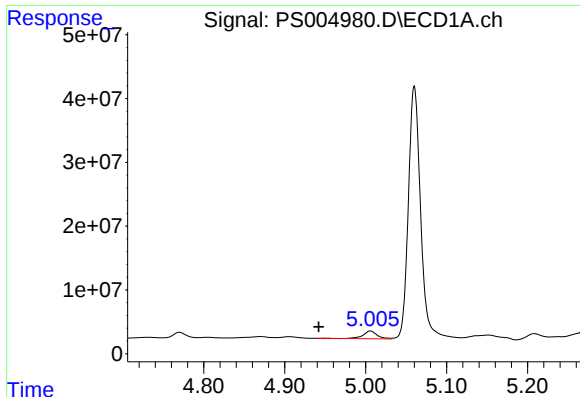

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.006 min
Delta R.T.: 0.064 min
Response: 14887768
Conc: 8.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

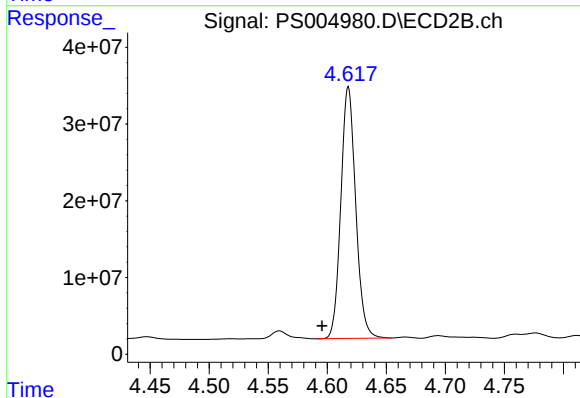


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.618 min
Delta R.T.: 0.022 min
Response: 287260840
Conc: 233.14 ng/ml

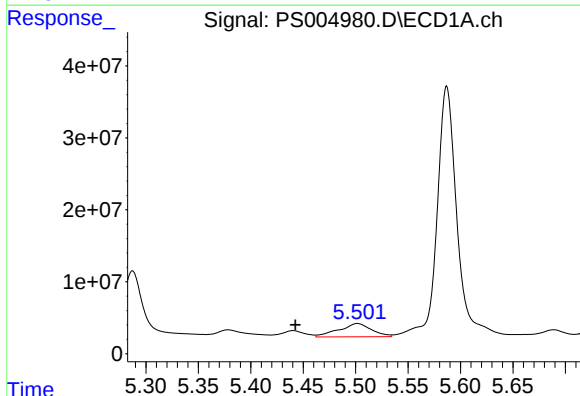


#3 4-Nitrophenol

R.T.: 5.502 min
Delta R.T.: 0.059 min
Response: 39905627
Conc: 64.00 ng/ml

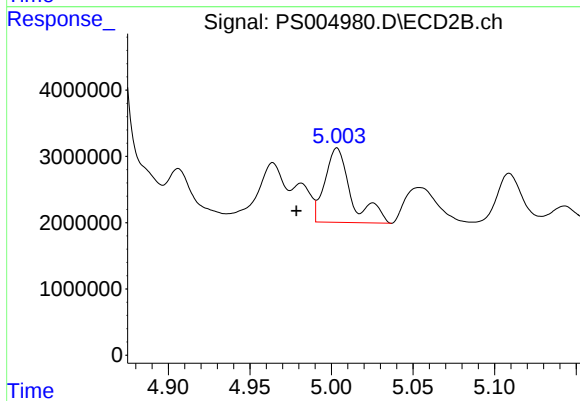

#3 4-Nitrophenol


R.T.: 5.003 min
Delta R.T.: 0.025 min
Response: 12656153
Conc: 26.71 ng/ml

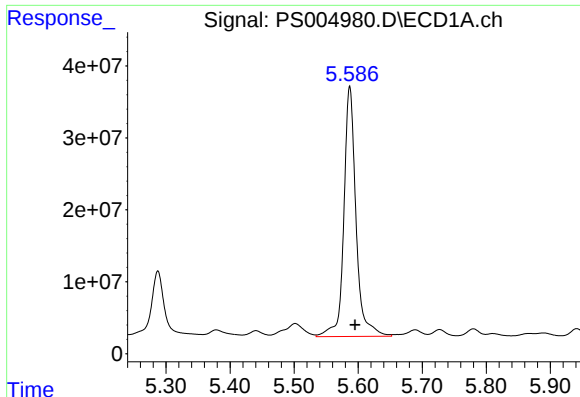

#4 2,4-DCAA


R.T.: 5.587 min
Delta R.T.: -0.008 min
Response: 456420244
Conc: 325.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

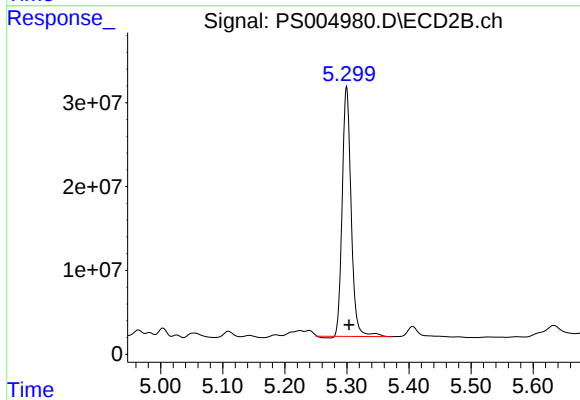


#4 2,4-DCAA

R.T.: 5.300 min
Delta R.T.: -0.004 min
Response: 296853942
Conc: 307.67 ng/ml

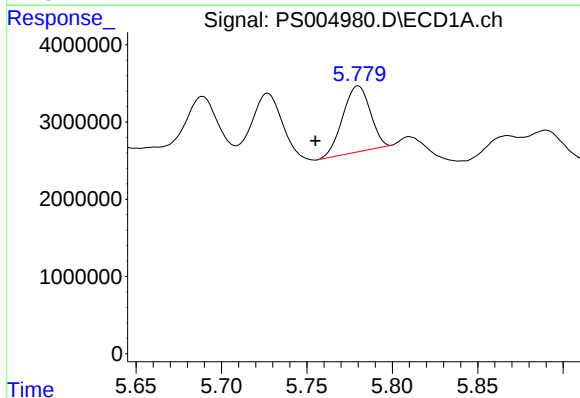


#5 DICAMBA

R.T.: 5.780 min
Delta R.T.: 0.025 min
Response: 9555087
Conc: 1.80 ng/ml

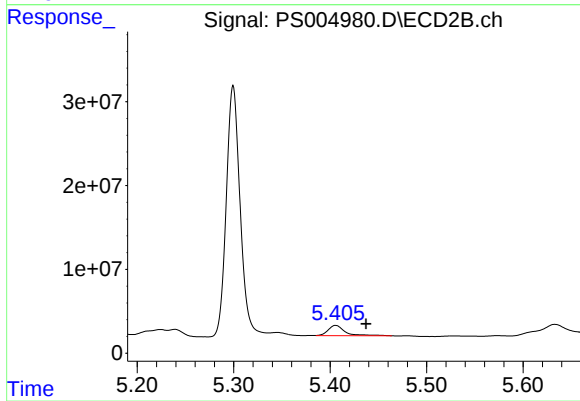

#5 DICAMBA


R.T.: 5.406 min
Delta R.T.: -0.031 min
Response: 14852615
Conc: 4.02 ng/ml

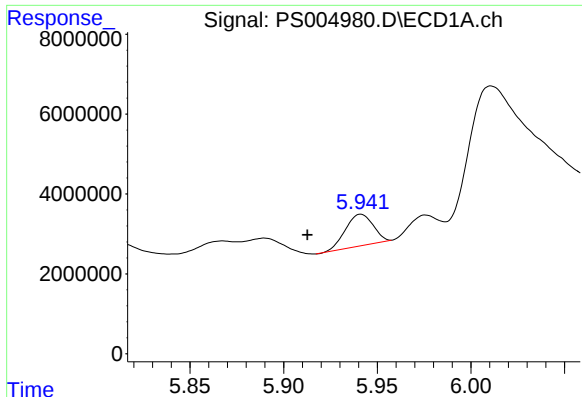

#6 MCPP


R.T.: 5.941 min
Delta R.T.: 0.029 min
Response: 8104500
Conc: 1.95 ug/ml

Instrument :
ECD_S
ClientSampleId :

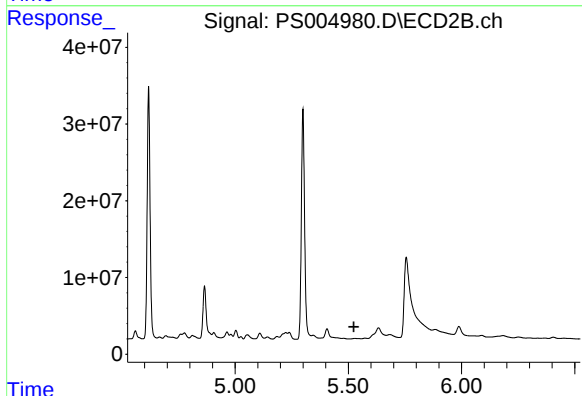


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

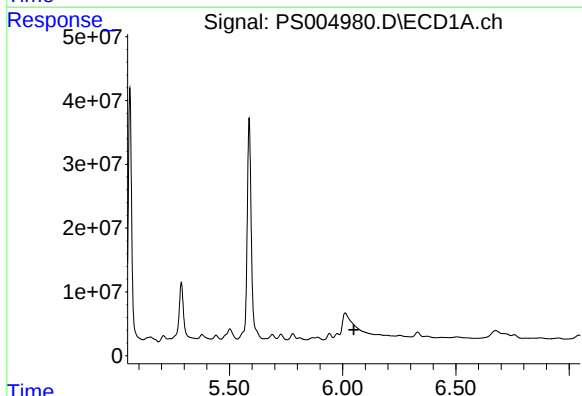


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

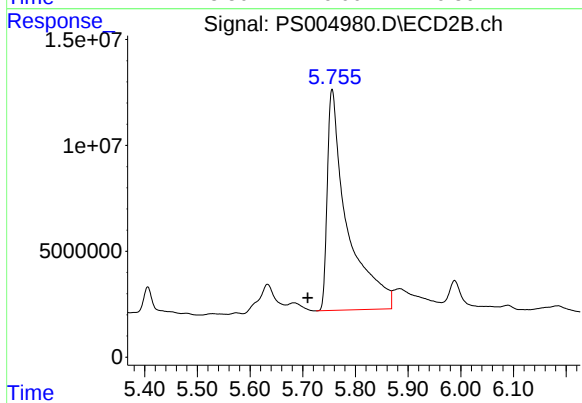

#7 MCPA


R.T.: 5.756 min
Delta R.T.: 0.047 min
Response: 274353613
Conc: 67.05 ug/ml

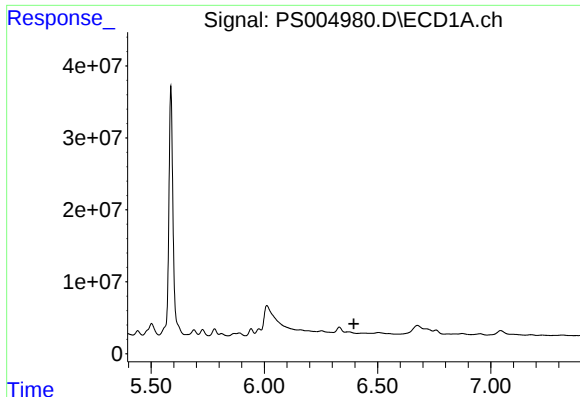

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

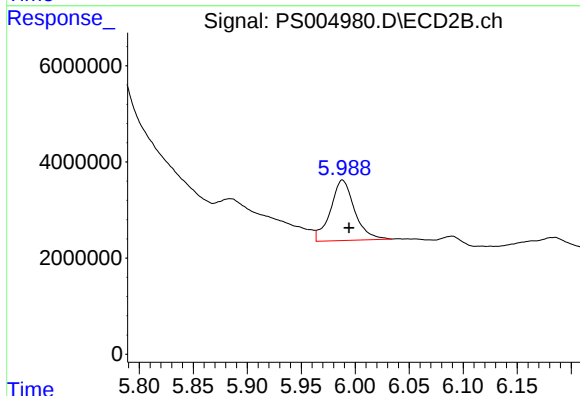


#8 DICHLORPROP

R.T.: 5.988 min
Delta R.T.: -0.006 min
Response: 19555053
Conc: 20.74 ng/ml

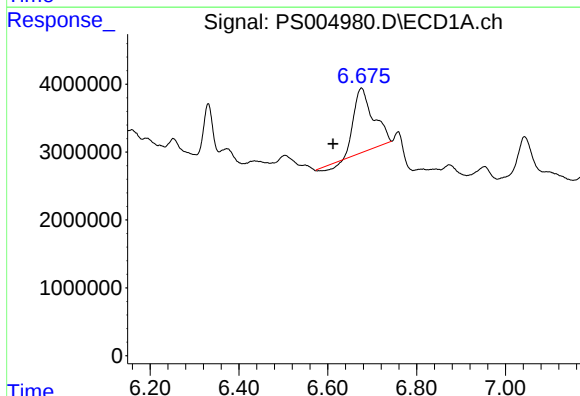


#9 2,4-D

R.T.: 6.676 min
Delta R.T.: 0.064 min
Response: 27507741
Conc: 20.11 ng/ml

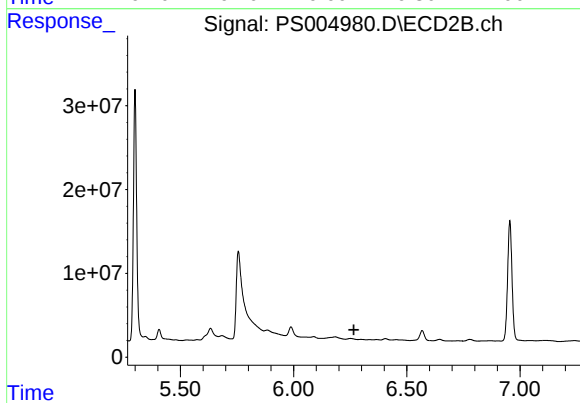

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

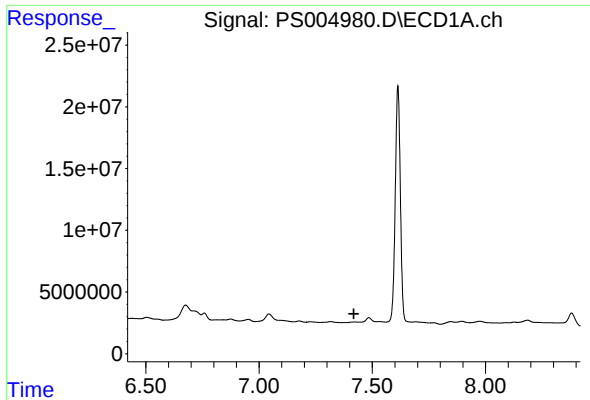

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

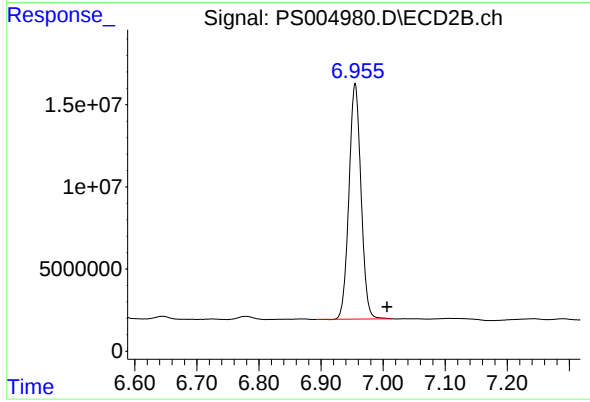

#11 2,4,5-TP (SILVEX)

R.T.: 6.955 min
Delta R.T.: -0.051 min
Response: 193137146
Conc: 37.54 ng/ml