

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
 Data File : PS004981.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2019 20:42
 Operator : SM\AJ
 Sample : K3160-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 23:01:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.590	5.303	411.6E6	282.4E6	293.643	292.744
Target Compounds							
2) T	3,5-DICHL...	5.010	4.621	12482983	295.5E6	7.238	239.842 #
5) T	DICAMBA	0.000	5.409	0	15452090	N.D.	4.183
6) T	MCP	5.945	0.000	7607239	0	1.827	N.D. #
7) T	MCPA	0.000	5.759	0	306.6E6	N.D.	74.943
8) T	DICHLORPROP	0.000	5.992	0	20501523	N.D.	21.745
9) T	2,4-D	6.680	0.000	51903016	0	37.943	N.D. #
11) T	2,4,5-TP ...	0.000	6.958	0	196.2E6	N.D.	38.138



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
Data File : PS004981.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2019 20:42
Operator : SM\AJ
Sample : K3160-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 23:01:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

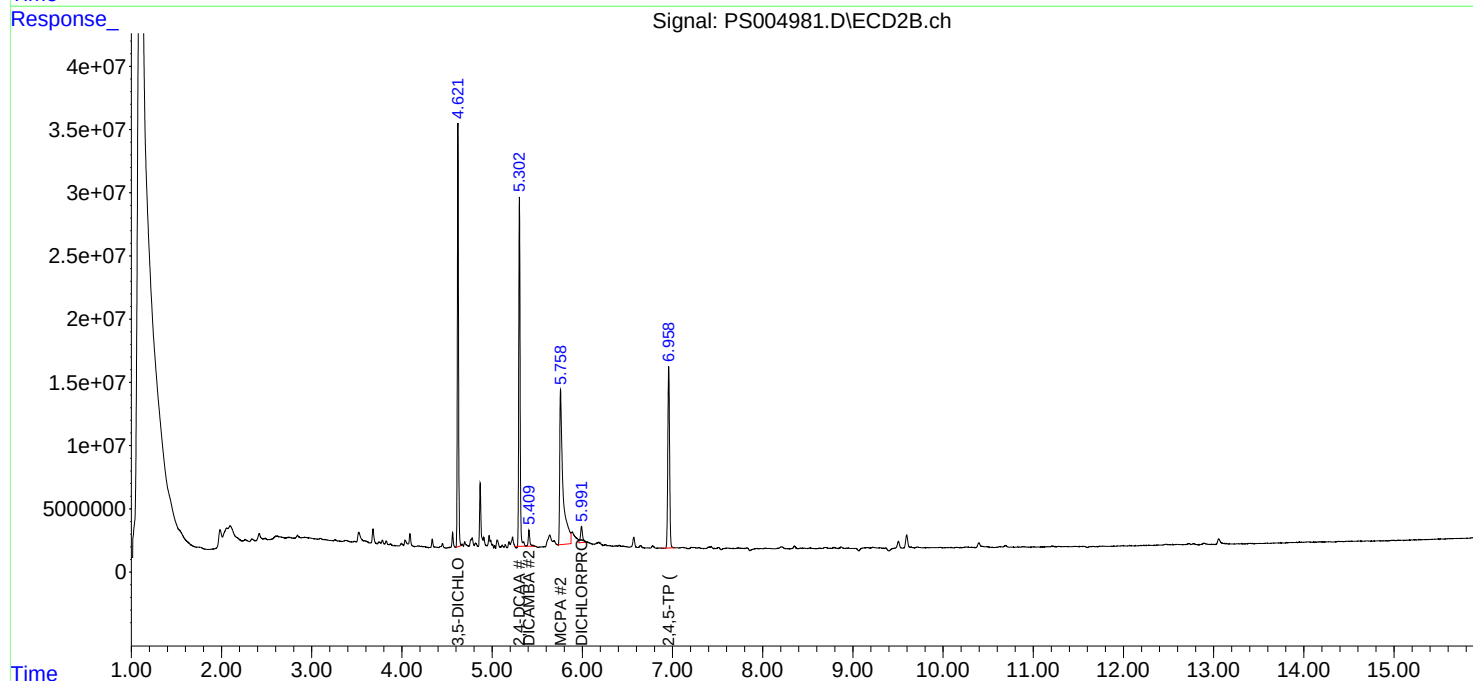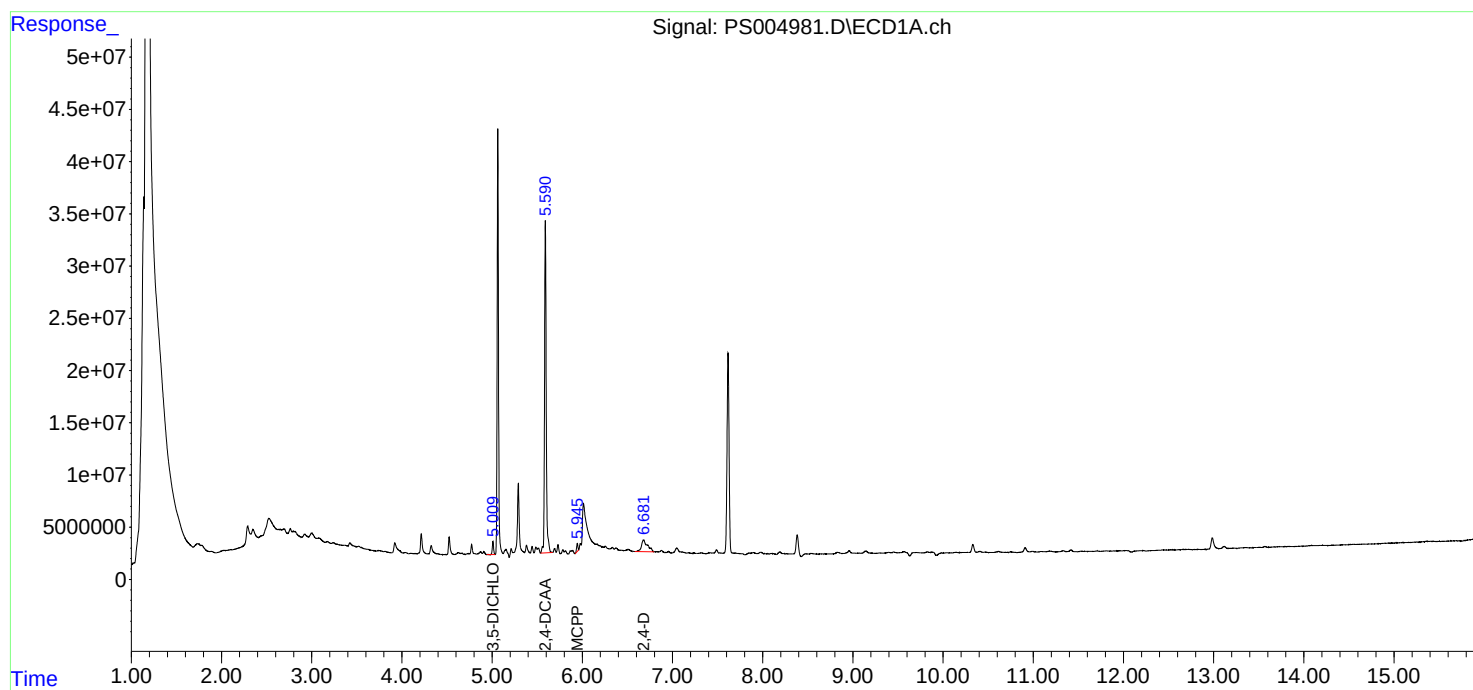


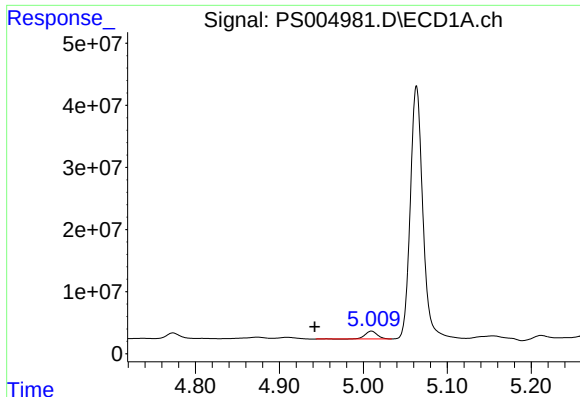

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.010 min
Delta R.T.: 0.068 min
Response: 12482983
Conc: 7.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

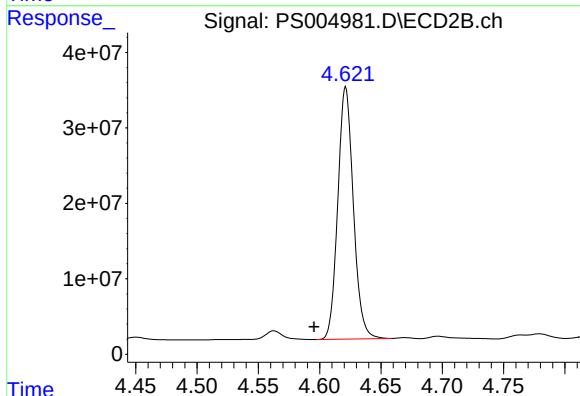


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.621 min
Delta R.T.: 0.026 min
Response: 295515578
Conc: 239.84 ng/ml

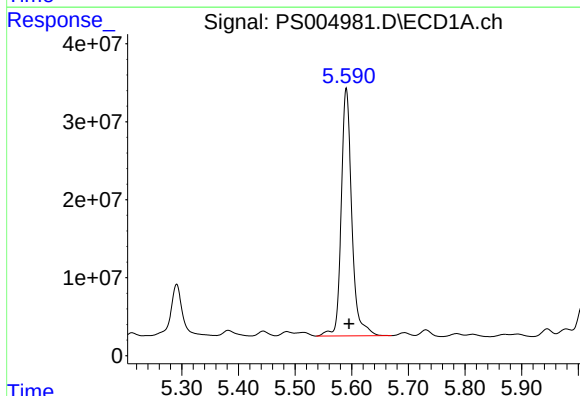


#4 2,4-DCAA

R.T.: 5.590 min
Delta R.T.: -0.005 min
Response: 411615722
Conc: 293.64 ng/ml

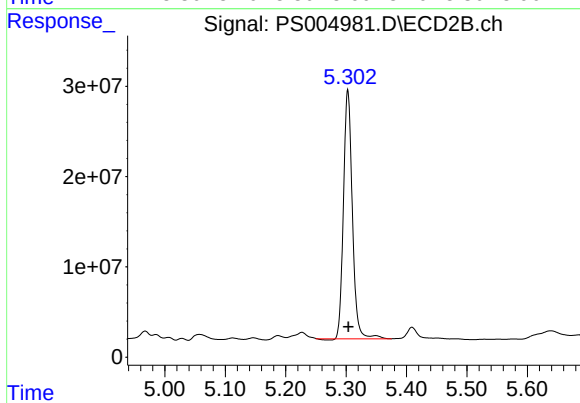

#4 2,4-DCAA


R.T.: 5.303 min
Delta R.T.: 0.000 min
Response: 282449758
Conc: 292.74 ng/ml

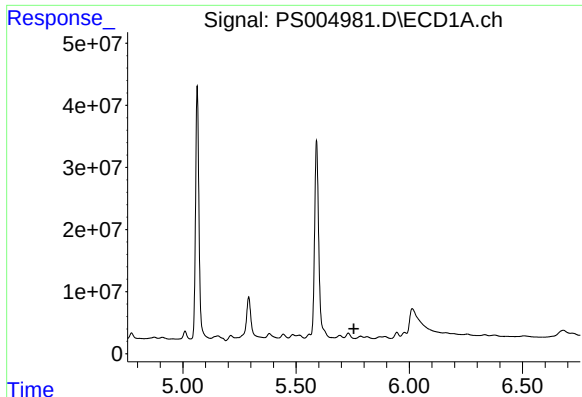

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

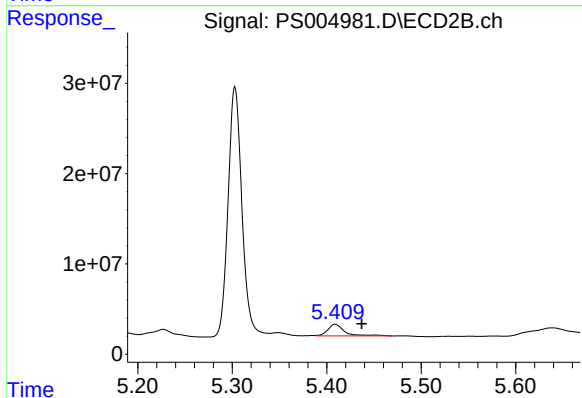


#5 DICAMBA

R.T.: 5.409 min
Delta R.T.: -0.028 min
Response: 15452090
Conc: 4.18 ng/ml

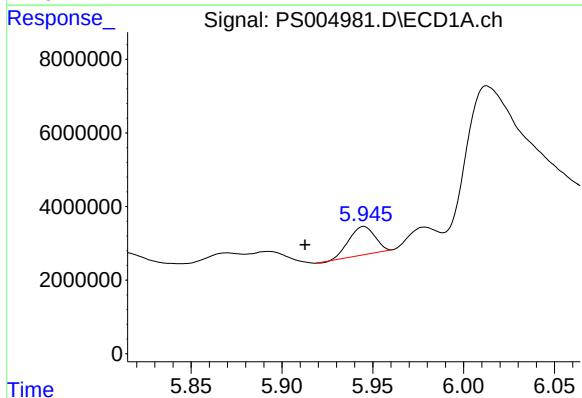


#6 MCP

R.T.: 5.945 min
Delta R.T.: 0.032 min
Response: 7607239
Conc: 1.83 ug/ml

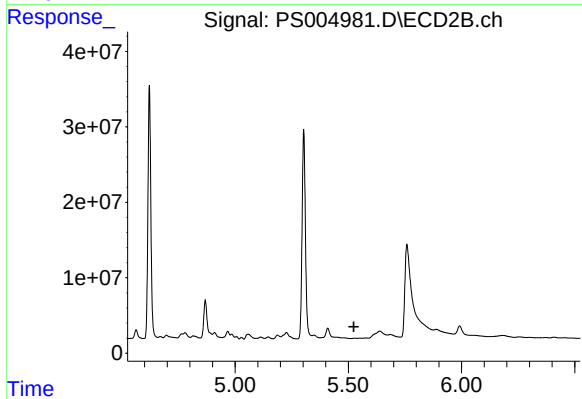

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

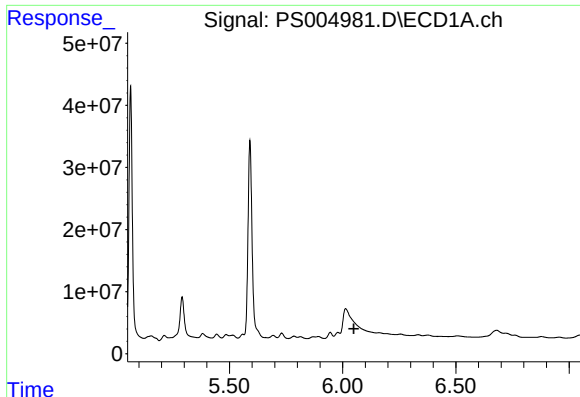

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

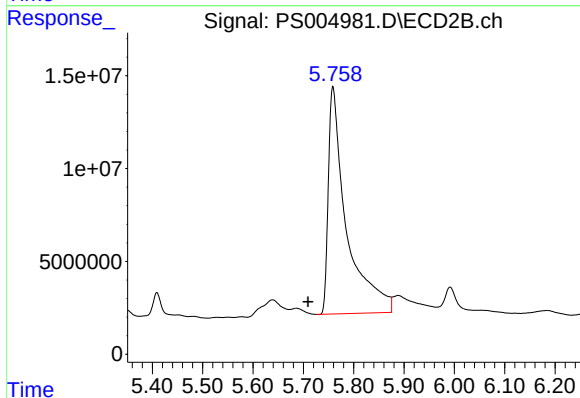


#7 MCPA

R.T.: 5.759 min
Delta R.T.: 0.050 min
Response: 306642200
Conc: 74.94 ug/ml

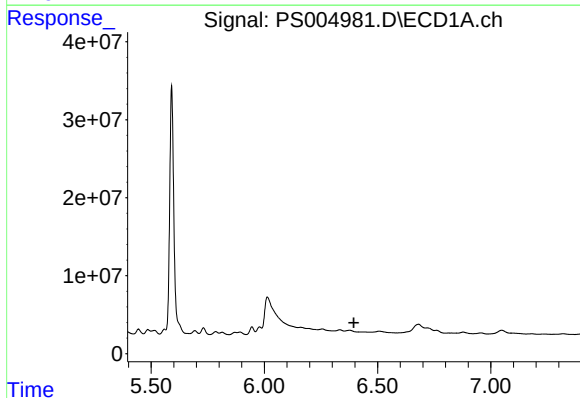


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

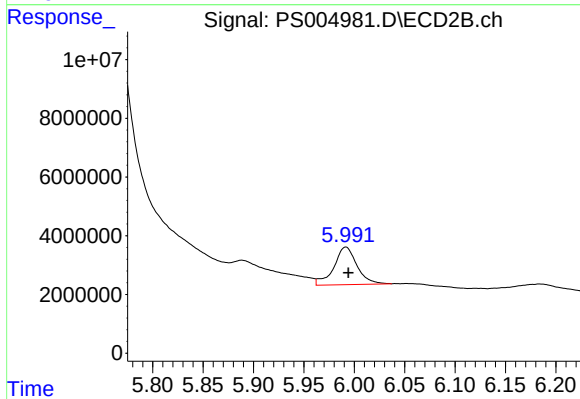

#8 DICHLORPROP


R.T.: 5.992 min
Delta R.T.: -0.003 min
Response: 20501523
Conc: 21.74 ng/ml

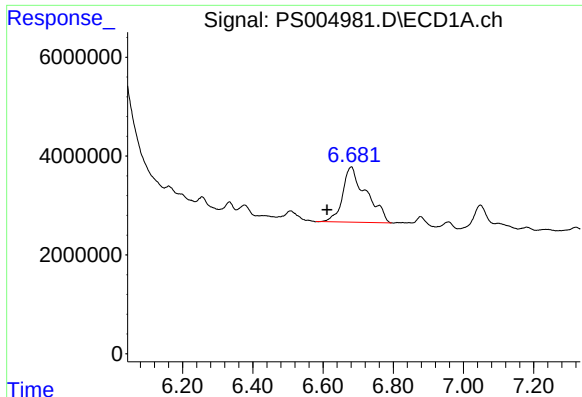

#9 2,4-D


R.T.: 6.680 min
Delta R.T.: 0.068 min
Response: 51903016
Conc: 37.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

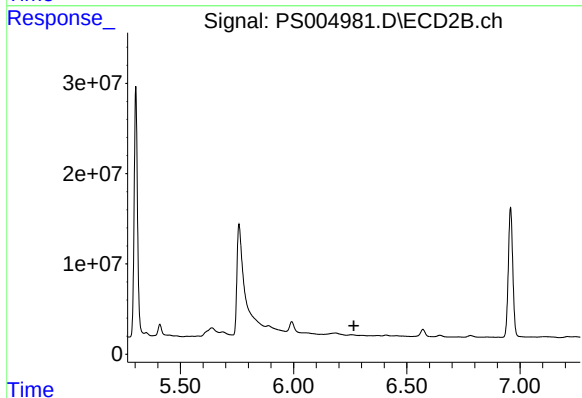


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

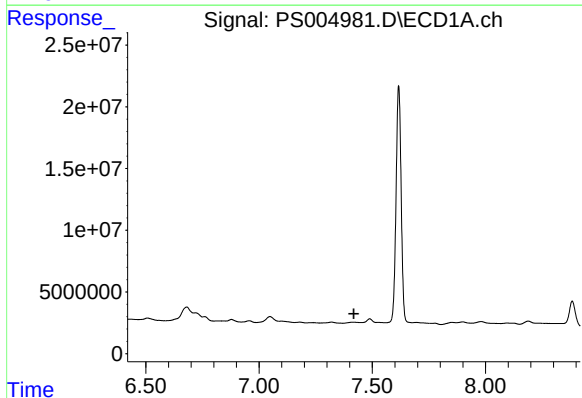

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

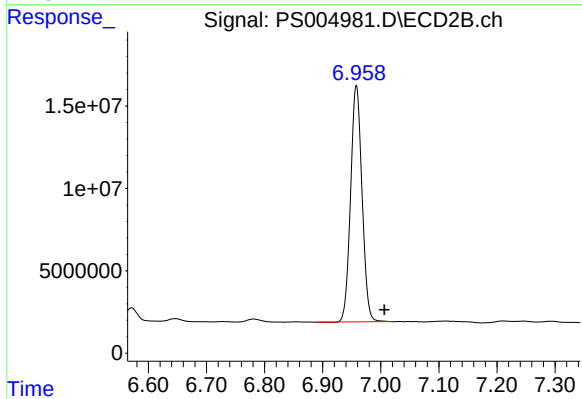

#11 2,4,5-TP (SILVEX)

R.T.: 6.958 min
Delta R.T.: -0.048 min
Response: 196233761
Conc: 38.14 ng/ml