

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
 Data File : PS004982.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2019 21:04
 Operator : SM\AJ
 Sample : K3160-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 23:01:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.592	5.305	428.7E6	291.6E6	305.850	302.191
Target Compounds							
2) T	3,5-DICHL...	5.011	4.623	14066087	297.1E6	8.156	241.122 #
3) T	4-Nitroph...	5.383	0.000	17775186	0	28.508	N.D. #
5) T	DICAMBA	0.000	5.411	0	14963765	N.D.	4.051
6) T	MCP	5.946	0.000	8196944	0	1.969	N.D. #
7) T	MCPA	6.017	5.762	61018471	260.2E6	10.535	63.582 #
8) T	DICHLORPROP	0.000	5.994	0	21025558	N.D.	22.301
9) T	2,4-D	6.679	0.000	51663015	0	37.768	N.D. #
11) T	2,4,5-TP ...	0.000	6.960	0	198.8E6	N.D.	38.643



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060719\
Data File : PS004982.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2019 21:04
Operator : SM\AJ
Sample : K3160-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 23:01:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

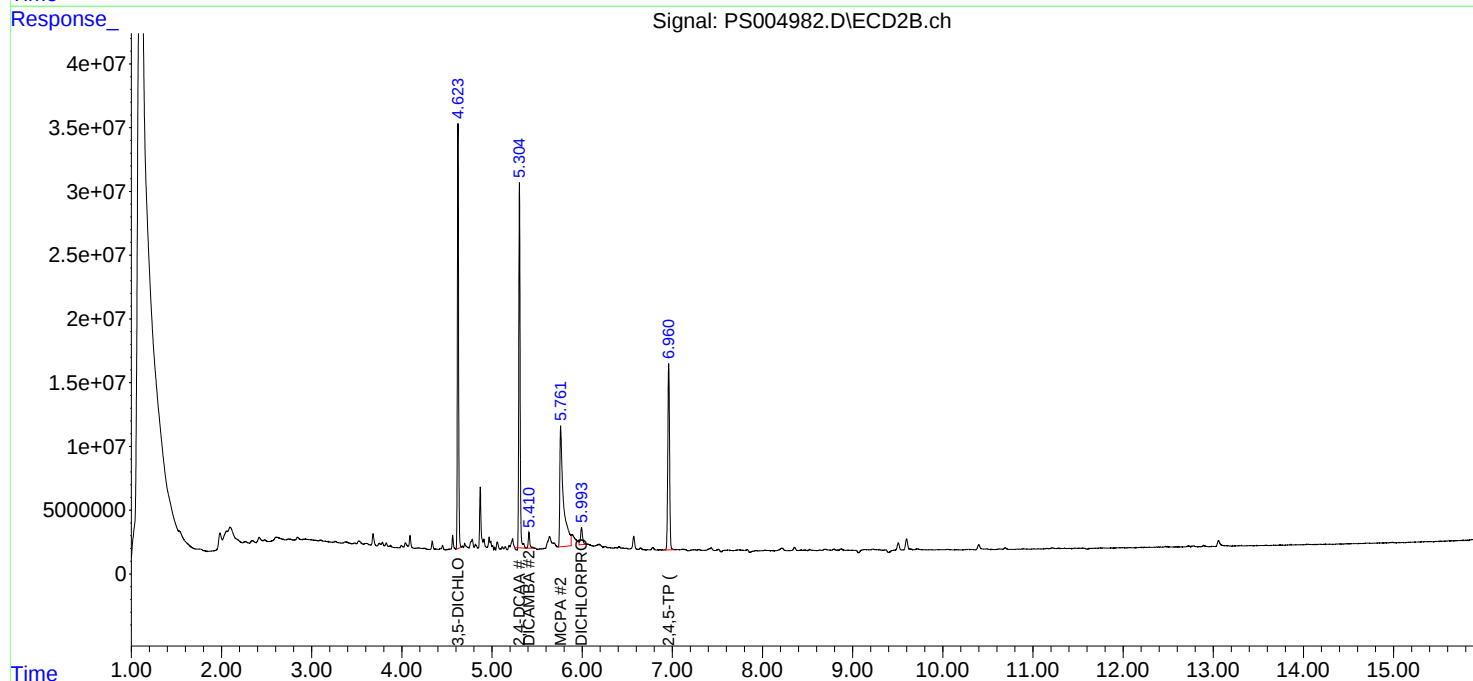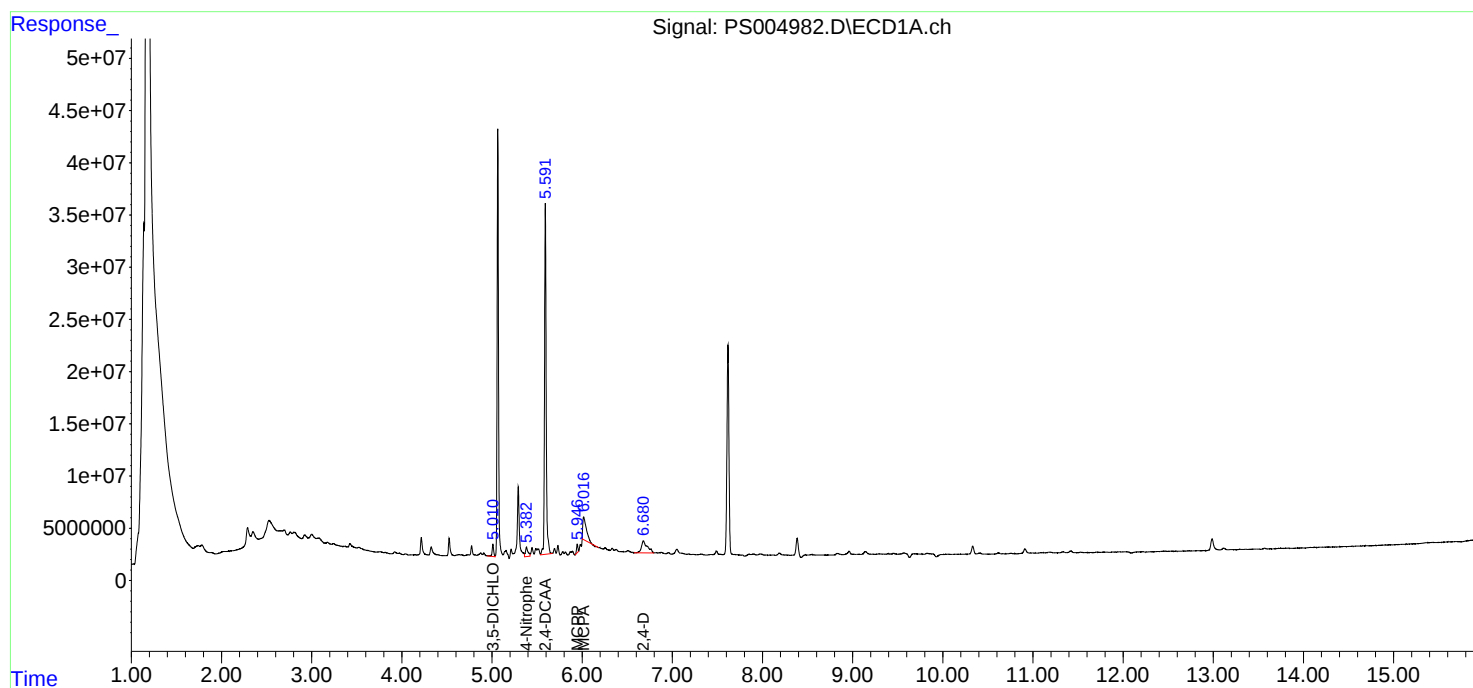


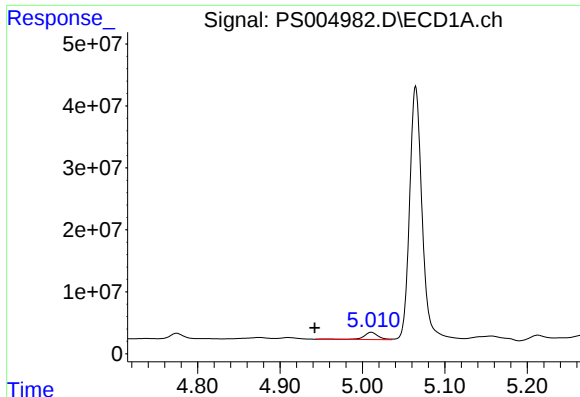

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.011 min
Delta R.T.: 0.069 min
Response: 14066087
Conc: 8.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

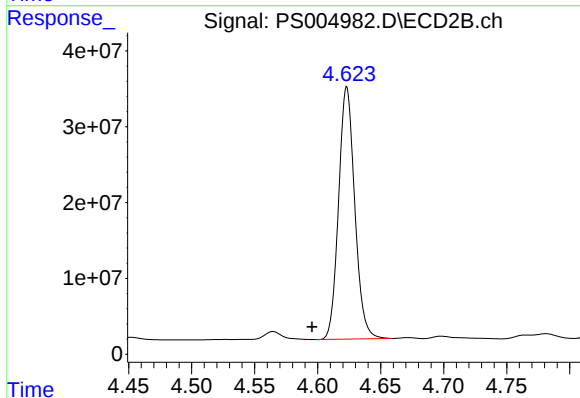


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.623 min
Delta R.T.: 0.028 min
Response: 297093231
Conc: 241.12 ng/ml

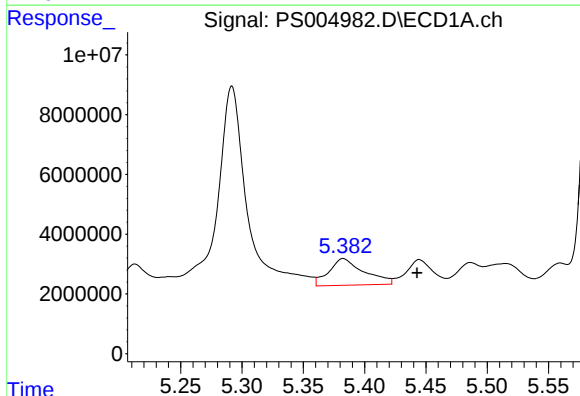


#3 4-Nitrophenol

R.T.: 5.383 min
Delta R.T.: -0.060 min
Response: 17775186
Conc: 28.51 ng/ml

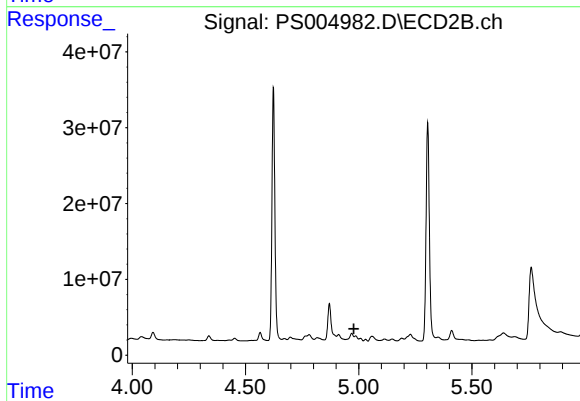

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

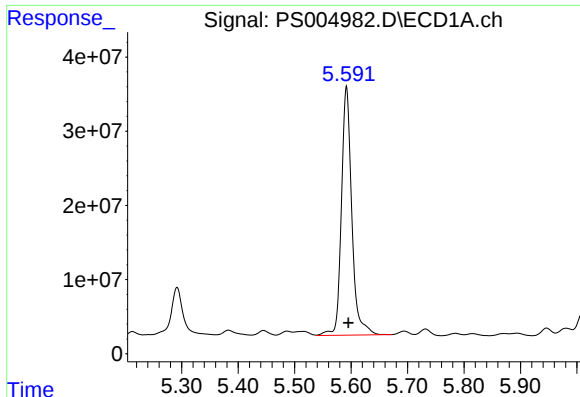

#4 2,4-DCAA


R.T.: 5.592 min
Delta R.T.: -0.003 min
Response: 428726527
Conc: 305.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

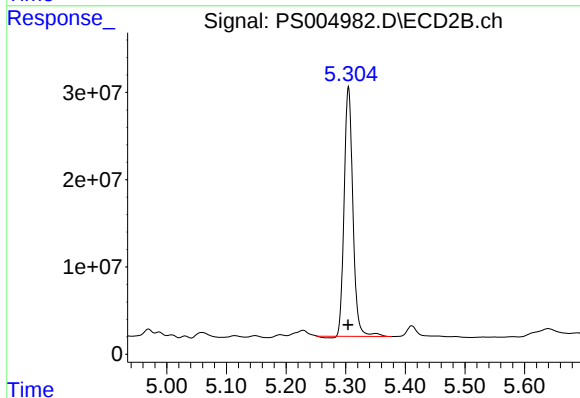


#4 2,4-DCAA

R.T.: 5.305 min
Delta R.T.: 0.000 min
Response: 291565127
Conc: 302.19 ng/ml

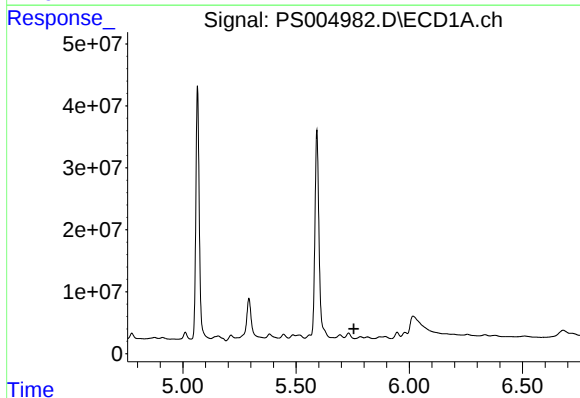


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.755 min
Response: 0
Conc: N.D.

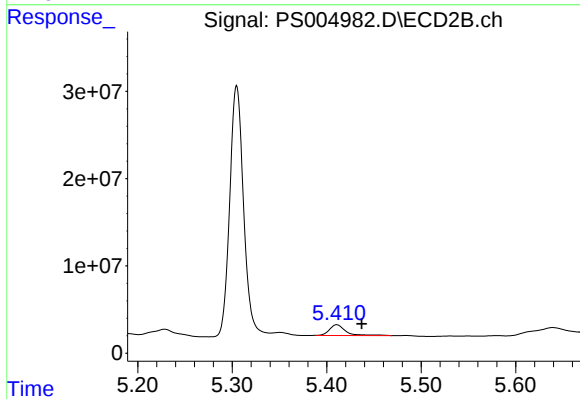

#5 DICAMBA


R.T.: 5.411 min
Delta R.T.: -0.027 min
Response: 14963765
Conc: 4.05 ng/ml

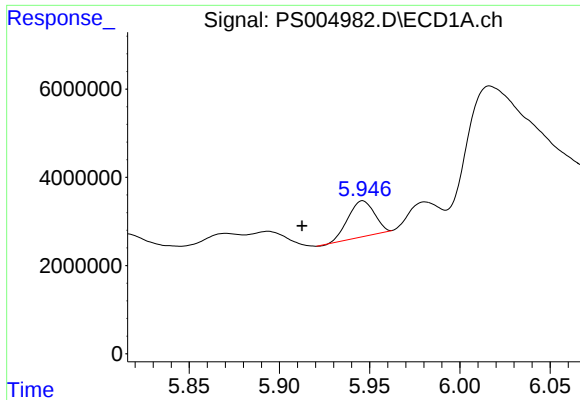

#6 MCPP


R.T.: 5.946 min
Delta R.T.: 0.034 min
Response: 8196944
Conc: 1.97 ug/ml

Instrument :
ECD_S
ClientSampleId :

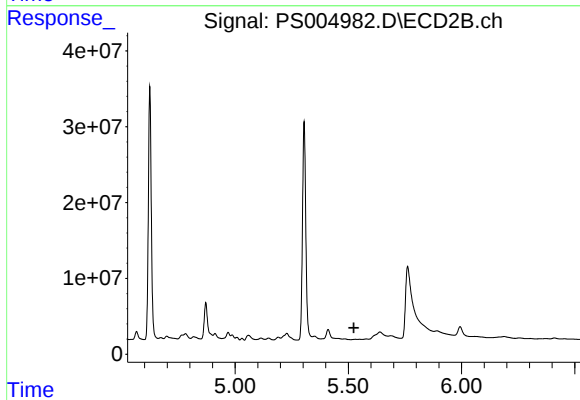


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

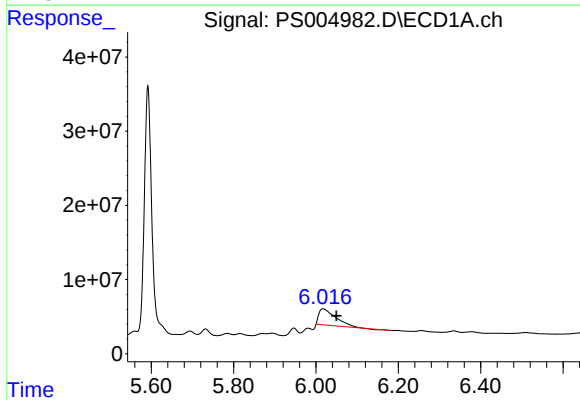


#7 MCPA

R.T.: 6.017 min
Delta R.T.: -0.032 min
Response: 61018471
Conc: 10.53 ug/ml

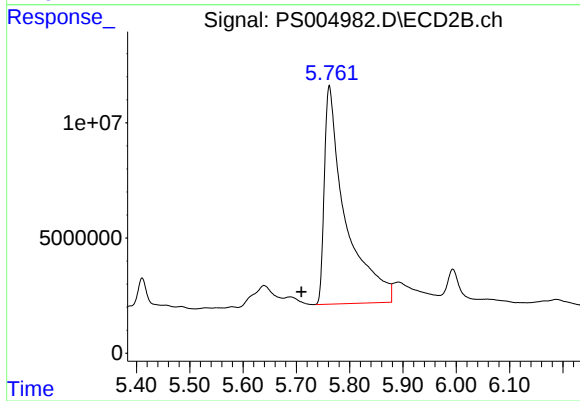

#7 MCPA


R.T.: 5.762 min
Delta R.T.: 0.053 min
Response: 260156059
Conc: 63.58 ug/ml

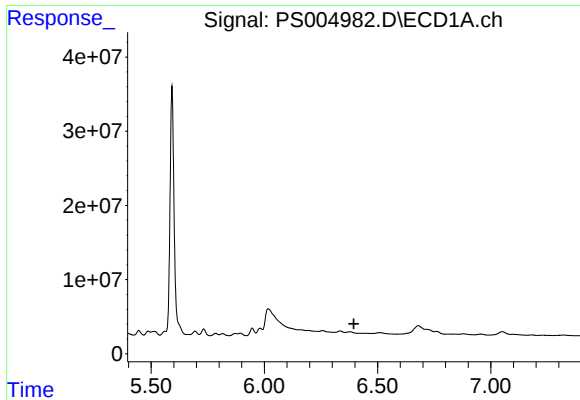

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

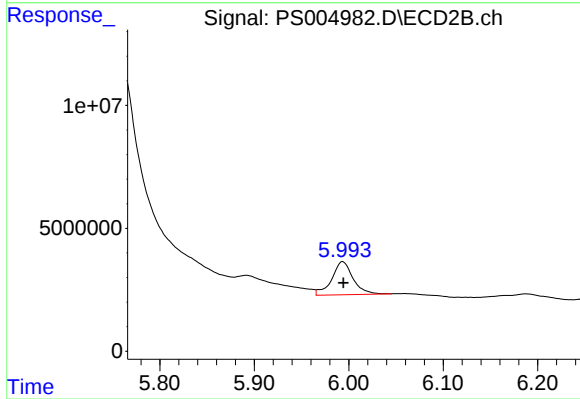


#8 DICHLORPROP

R.T.: 5.994 min
Delta R.T.: 0.000 min
Response: 21025558
Conc: 22.30 ng/ml

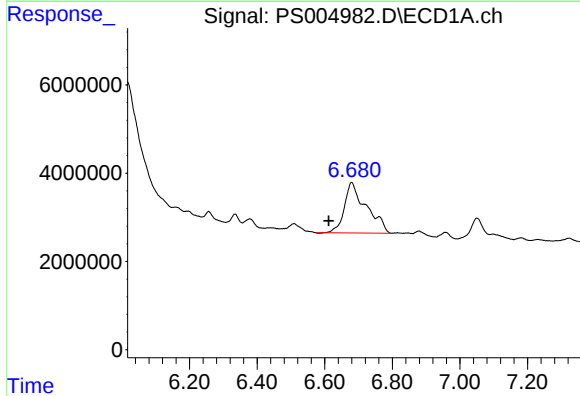


#9 2,4-D

R.T.: 6.679 min
Delta R.T.: 0.068 min
Response: 51663015
Conc: 37.77 ng/ml

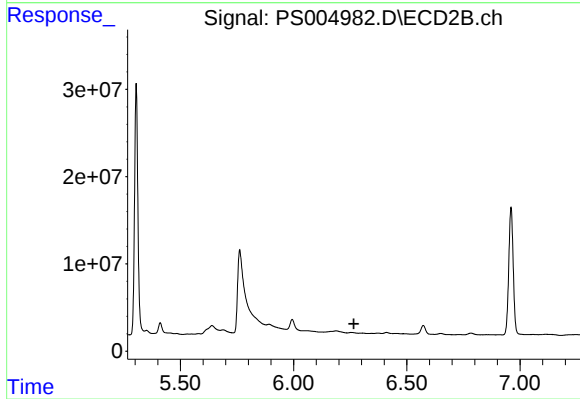

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

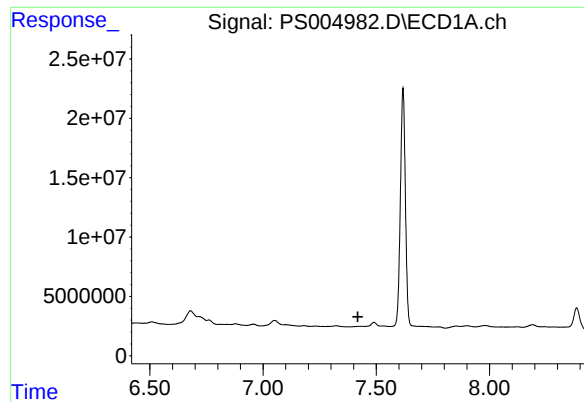

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

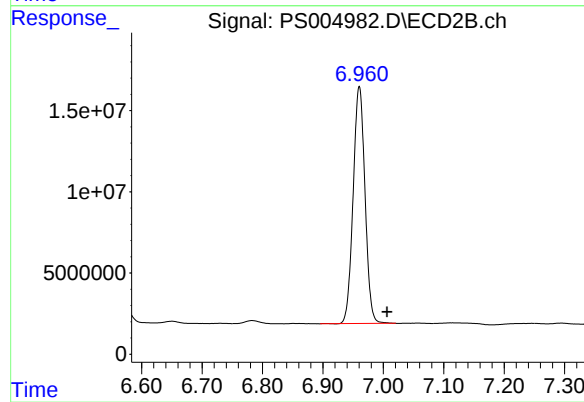

#11 2,4,5-TP (SILVEX)

R.T.: 6.960 min
Delta R.T.: -0.046 min
Response: 198831872
Conc: 38.64 ng/ml