

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061219\
 Data File : PS005012.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2019 02:29
 Operator : SM\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 07:56:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 13 07:54:47 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.587	5.300	978.8E6	728.4E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.113	1.809	1183.7E6	910.0E6	682.500	682.500
2) T	3,5-DICHL...	4.936	4.593	1296.4E6	873.7E6	697.500	697.500
3) T	4-Nitroph...	5.437	4.976	312.6E6	305.7E6	682.500	682.500
5) T	DICAMBA	5.747	5.434	3927.3E6	2663.4E6	705.000	705.000
6) T	MCPD	5.906	5.523	311.7E6	200.8E6	70.500	70.500
7) T	MCPA	6.044	5.709	434.6E6	285.6E6	69.750	69.750
8) T	DICHLORPROP	6.386	5.990	966.9E6	669.8E6	705.000	705.000
9) T	2,4-D	6.603	6.262	950.3E6	739.5E6	705.000	705.000
10) T	Pentachlo...	6.872	6.639	13380.6E6	8935.7E6	712.500	712.500
11) T	2,4,5-TP ...	7.409	7.001	5497.3E6	3734.5E6	712.500	712.500
12) T	2,4,5-T	7.684	7.400	5559.3E6	3248.9E6	712.500	712.500
13) T	2,4-DB	8.217	7.852	665.5E6	445.4E6	712.500	712.500
14) T	DINOSEB	9.316	8.166	4487.3E6	2699.1E6	705.000	705.000
15) T	Picloram	9.144	9.108	7169.2E6	4866.8E6	712.500	712.500
16) T	DCPA	9.588	9.067	6816.6E6	4647.4E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061219\
Data File : PS005012.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2019 02:29
Operator : SM\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 07:56:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Thu Jun 13 07:54:47 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

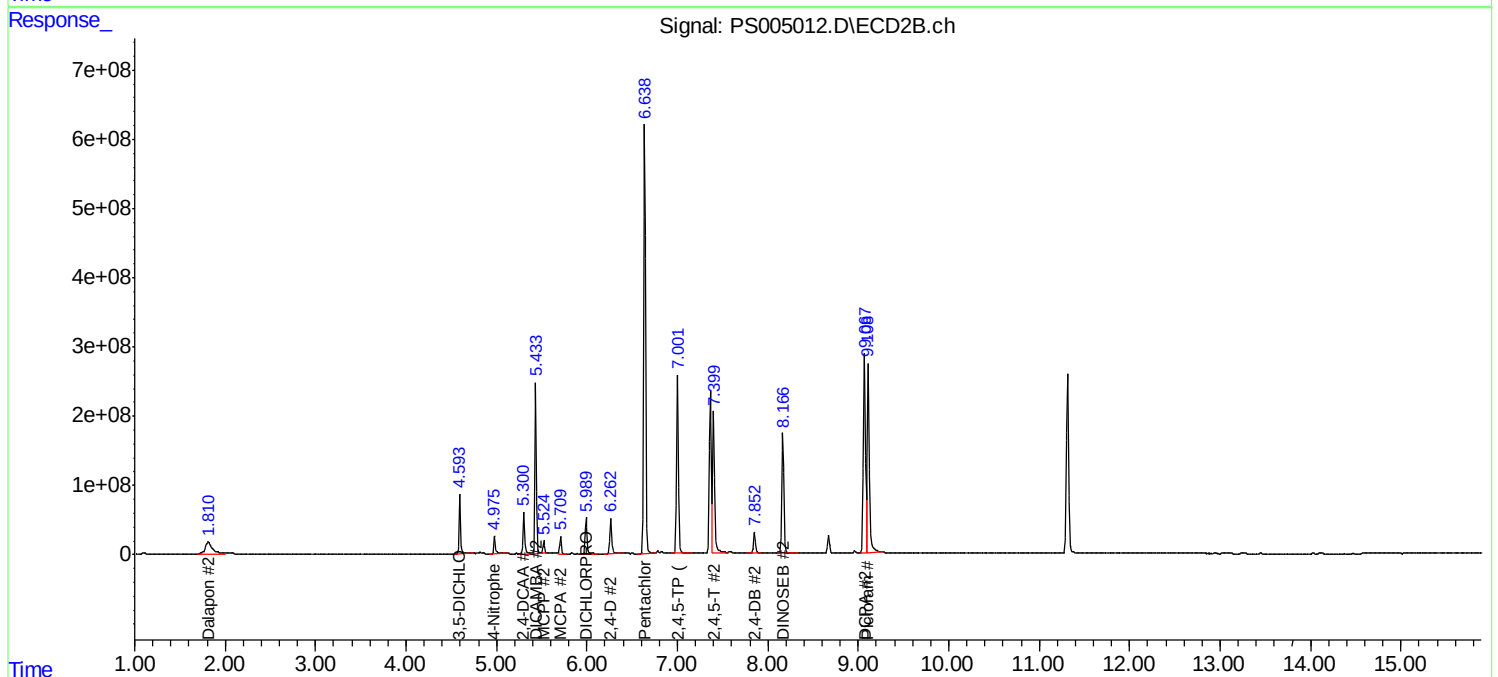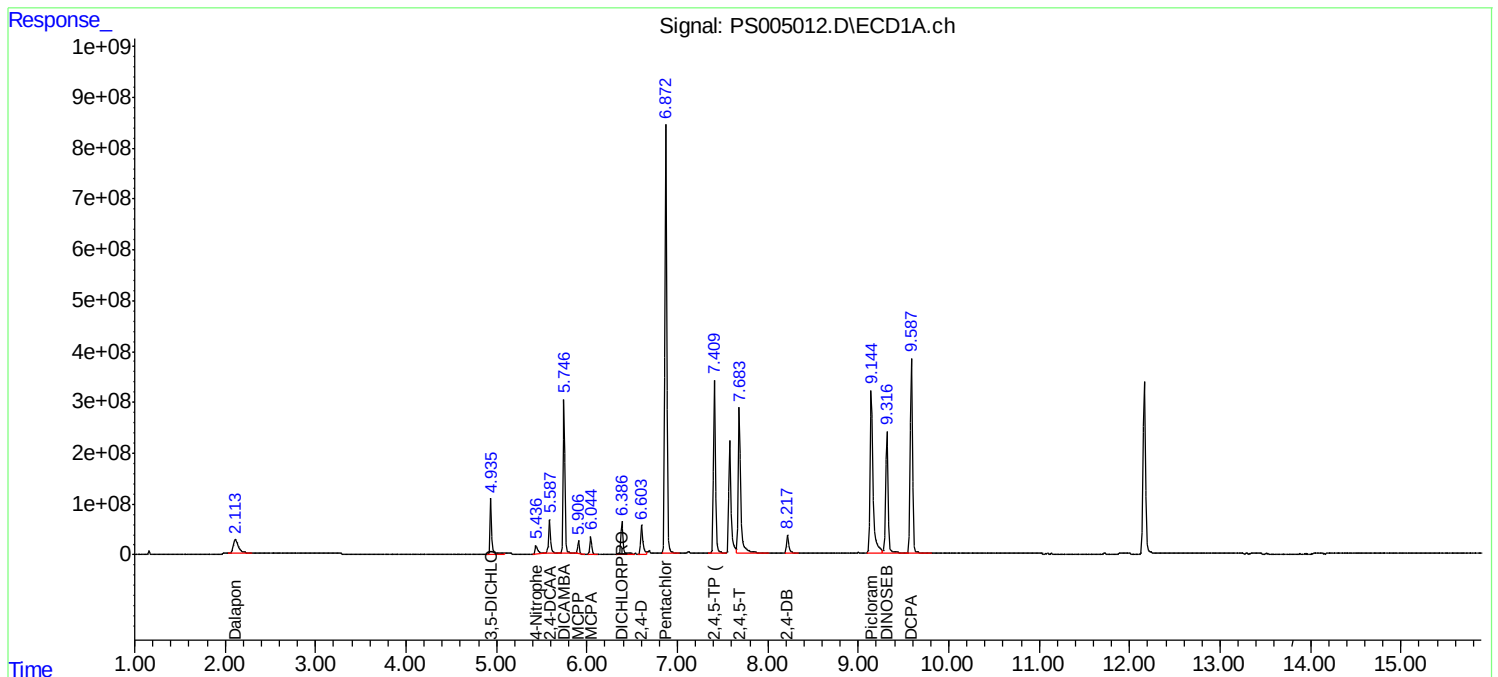


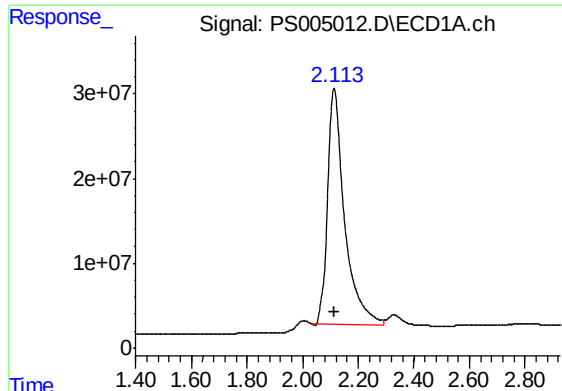

#1 Dalapon


R.T.: 2.113 min
Delta R.T.: 0.000 min
Response: 1183745560
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

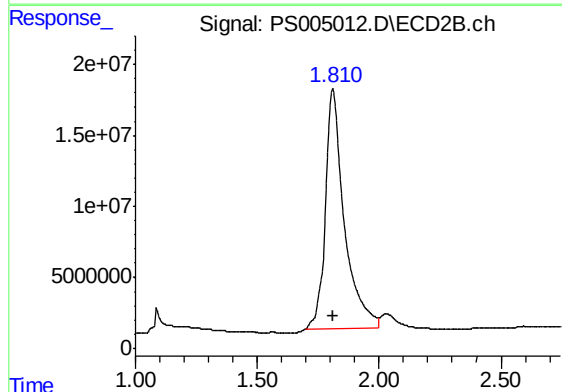


#1 Dalapon

R.T.: 1.809 min
Delta R.T.: 0.000 min
Response: 909951996
Conc: 682.50 ng/ml

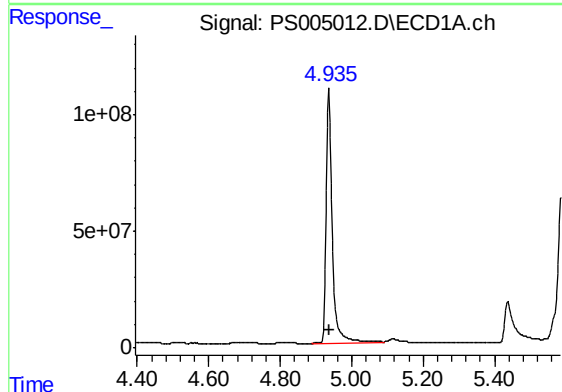


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 1296353469
Conc: 697.50 ng/ml

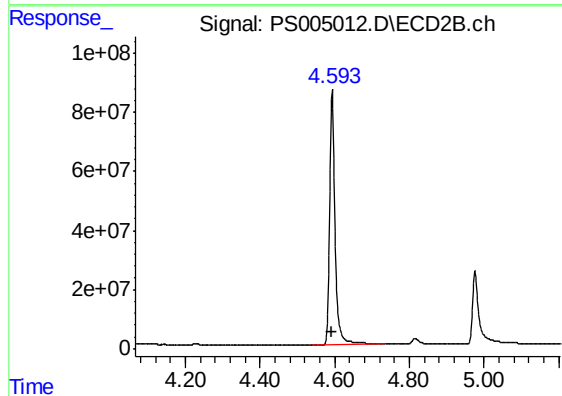

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.593 min
Delta R.T.: 0.000 min
Response: 873671627
Conc: 697.50 ng/ml

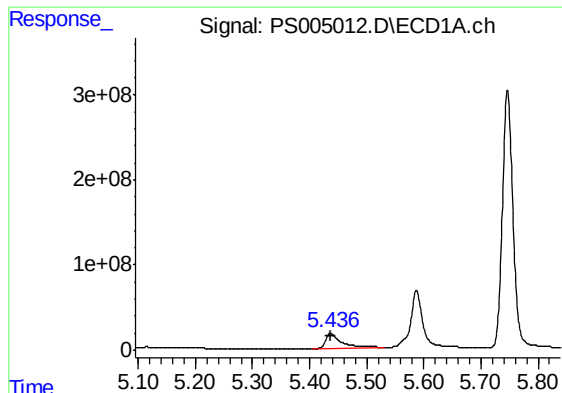

#3 4-Nitrophenol


R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 312641049
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

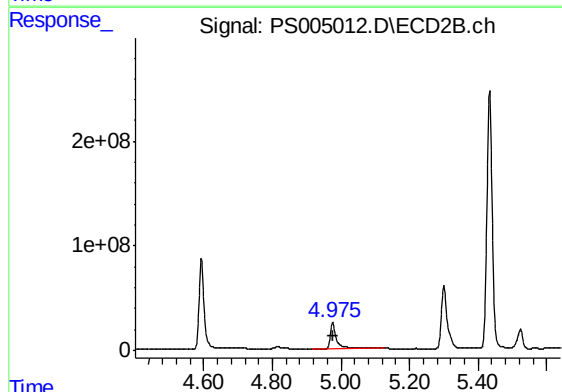


#3 4-Nitrophenol

R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 305719268
Conc: 682.50 ng/ml

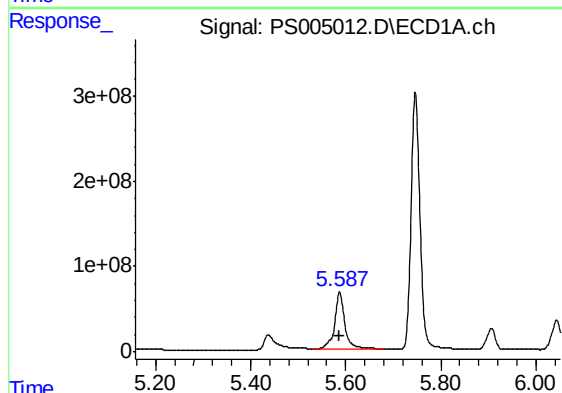


#4 2,4-DCAA

R.T.: 5.587 min
Delta R.T.: 0.000 min
Response: 978769159
Conc: 750.00 ng/ml

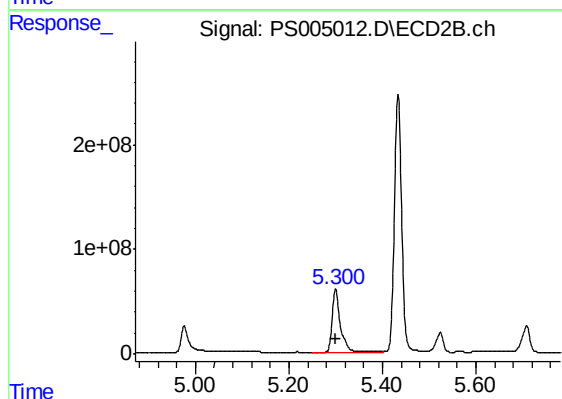

#4 2,4-DCAA


R.T.: 5.300 min
Delta R.T.: 0.000 min
Response: 728352049
Conc: 750.00 ng/ml

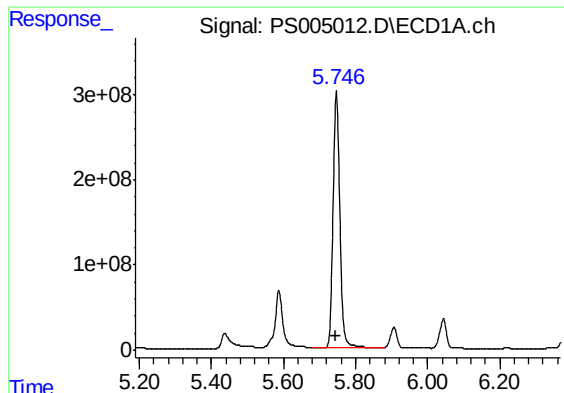

#5 DICAMBA


R.T.: 5.747 min
Delta R.T.: 0.000 min
Response: 3927312447
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

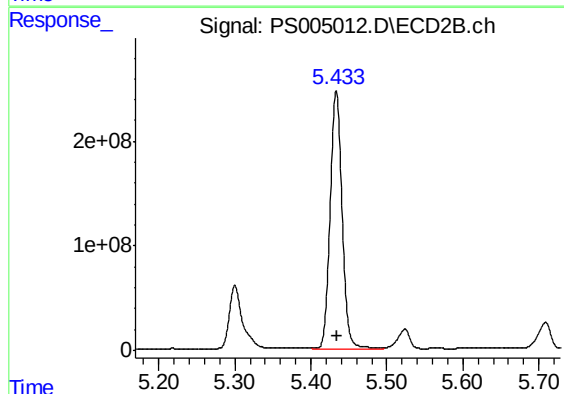


#5 DICAMBA

R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 2663383176
Conc: 705.00 ng/ml

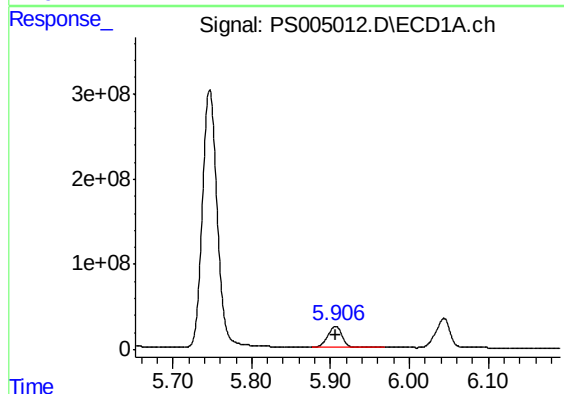


#6 MCPP

R.T.: 5.906 min
Delta R.T.: 0.000 min
Response: 311734007
Conc: 70.50 ug/ml

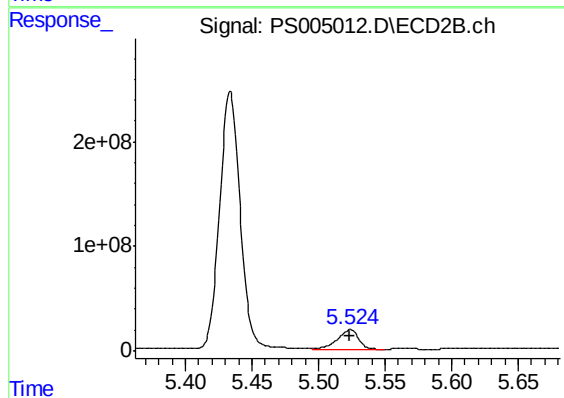

#6 MCPP


R.T.: 5.523 min
Delta R.T.: 0.000 min
Response: 200809121
Conc: 70.50 ug/ml

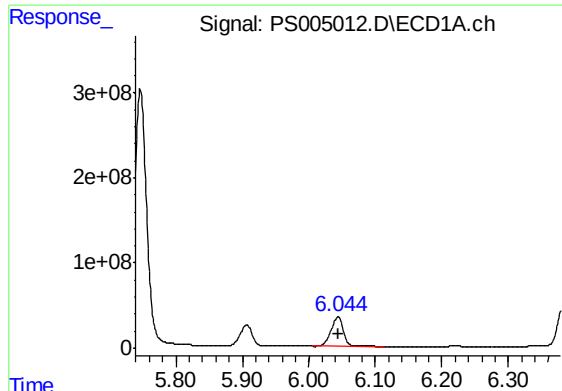

#7 MCPA


R.T.: 6.044 min
Delta R.T.: 0.000 min
Response: 434584786
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

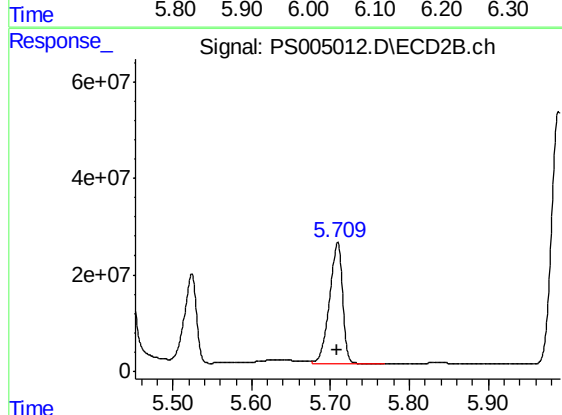


#7 MCPA

R.T.: 5.709 min
Delta R.T.: 0.000 min
Response: 285595375
Conc: 69.75 ug/ml

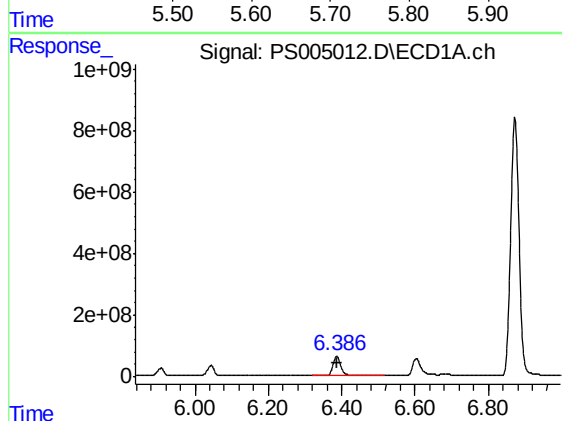


#8 DICHLORPROP

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 966919915
Conc: 705.00 ng/ml

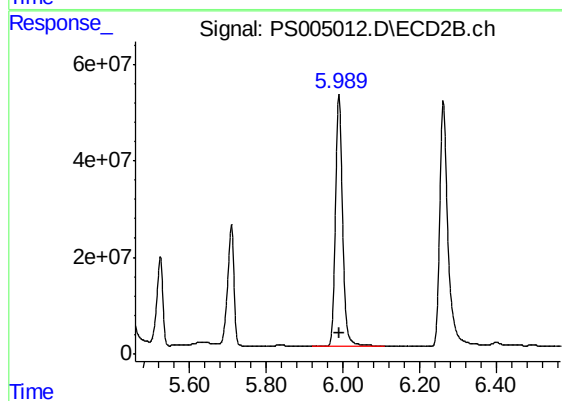

#8 DICHLORPROP


R.T.: 5.990 min
Delta R.T.: 0.000 min
Response: 669750450
Conc: 705.00 ng/ml

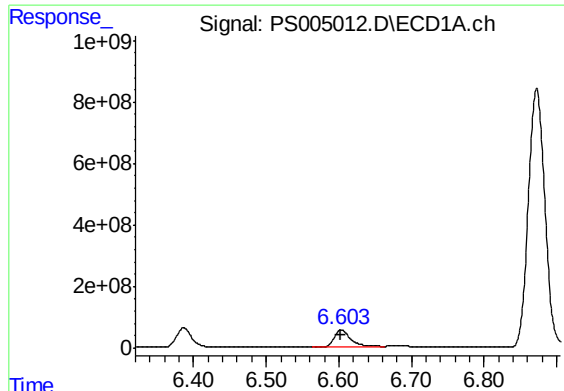

#9 2,4-D


R.T.: 6.603 min
Delta R.T.: 0.000 min
Response: 950321616
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

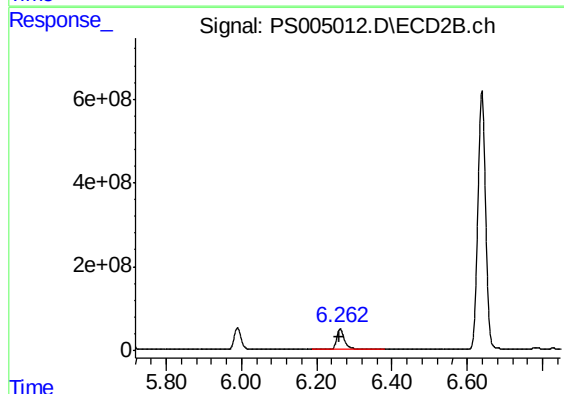


#9 2,4-D

R.T.: 6.262 min
Delta R.T.: 0.000 min
Response: 739518286
Conc: 705.00 ng/ml

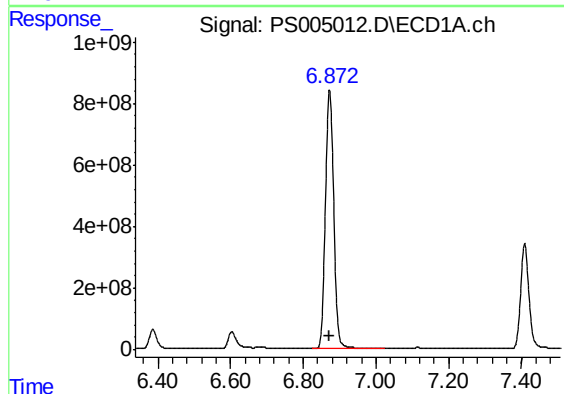


#10 Pentachlorophenol

R.T.: 6.872 min
Delta R.T.: 0.000 min
Response: 13380617488
Conc: 712.50 ng/ml

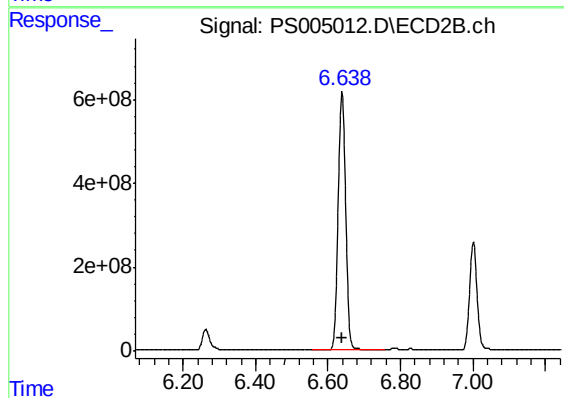

#10 Pentachlorophenol


R.T.: 6.639 min
Delta R.T.: 0.000 min
Response: 8935741379
Conc: 712.50 ng/ml

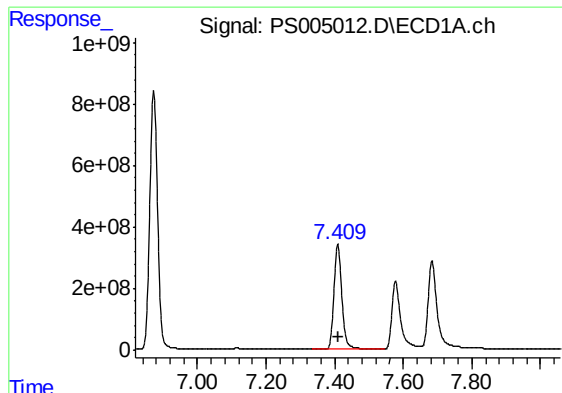

#11 2,4,5-TP (SILVEX)


R.T.: 7.409 min
Delta R.T.: 0.000 min
Response: 5497329729
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

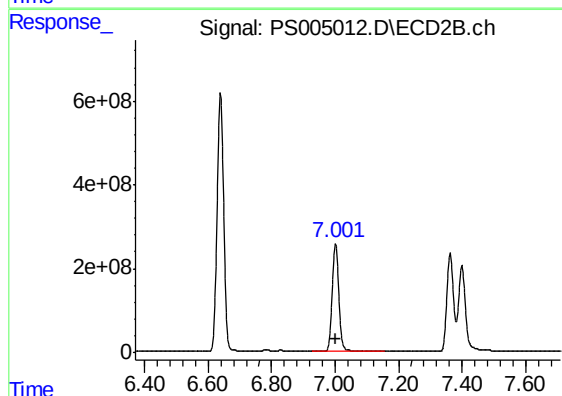


#11 2,4,5-TP (SILVEX)

R.T.: 7.001 min
Delta R.T.: 0.000 min
Response: 3734480454
Conc: 712.50 ng/ml

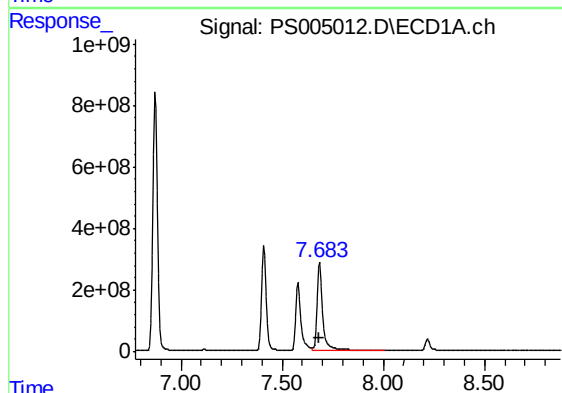


#12 2,4,5-T

R.T.: 7.684 min
Delta R.T.: 0.000 min
Response: 5559323549
Conc: 712.50 ng/ml

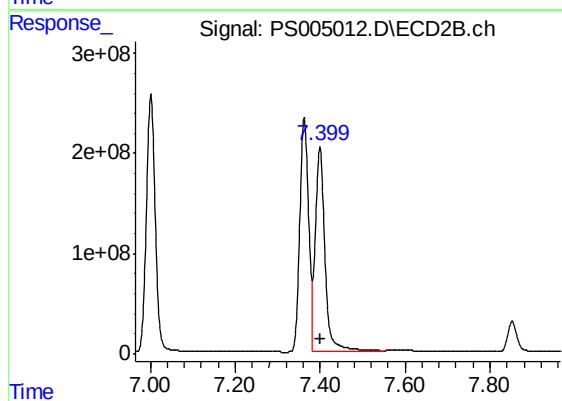

#12 2,4,5-T


R.T.: 7.400 min
Delta R.T.: 0.000 min
Response: 3248910383
Conc: 712.50 ng/ml

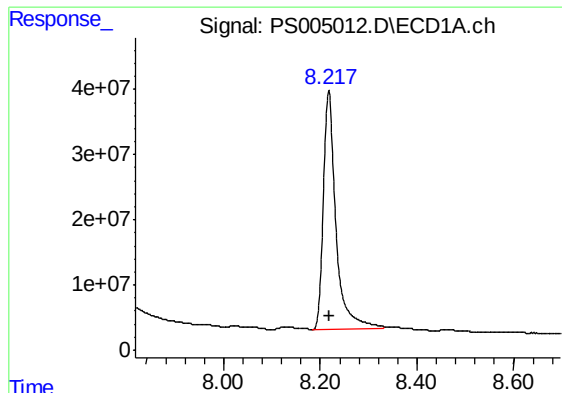

#13 2,4-DB


R.T.: 8.217 min
Delta R.T.: 0.000 min
Response: 665498116
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

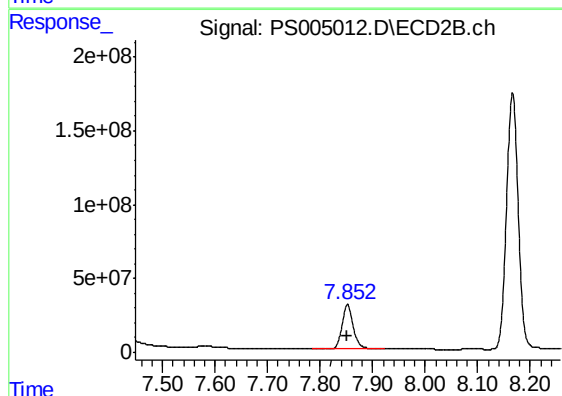


#13 2,4-DB

R.T.: 7.852 min
Delta R.T.: 0.000 min
Response: 445388413
Conc: 712.50 ng/ml

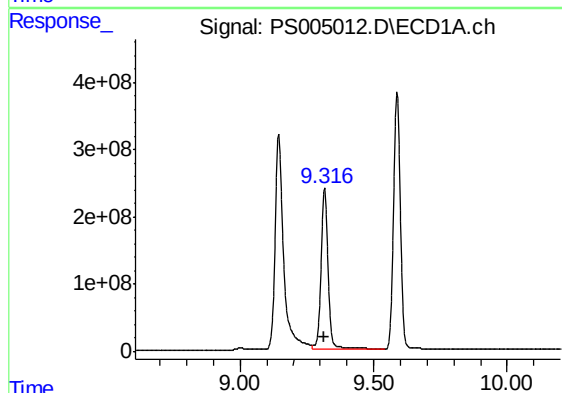


#14 DINOSEB

R.T.: 9.316 min
Delta R.T.: 0.000 min
Response: 4487284919
Conc: 705.00 ng/ml

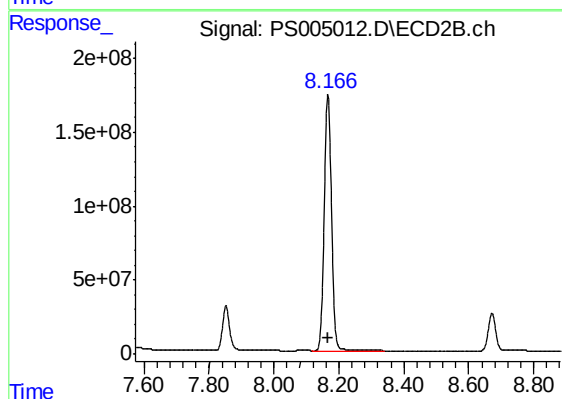

#14 DINOSEB


R.T.: 8.166 min
Delta R.T.: 0.000 min
Response: 2699139953
Conc: 705.00 ng/ml

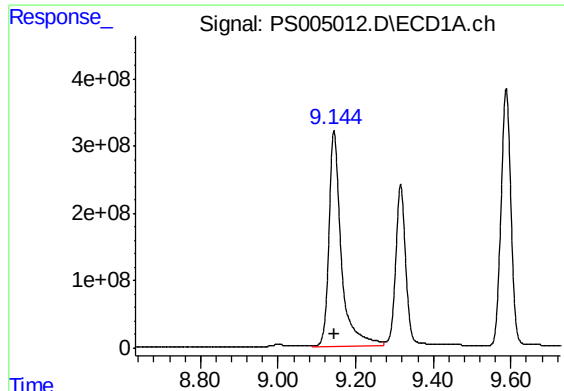

#15 Picloram


R.T.: 9.144 min
Delta R.T.: 0.000 min
Response: 7169237350
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

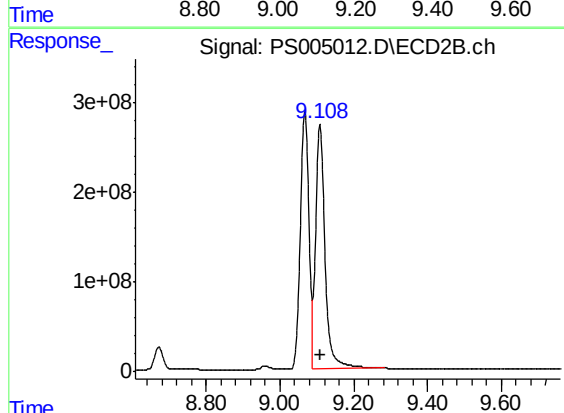


#15 Picloram

R.T.: 9.108 min
Delta R.T.: 0.000 min
Response: 4866830648
Conc: 712.50 ng/ml

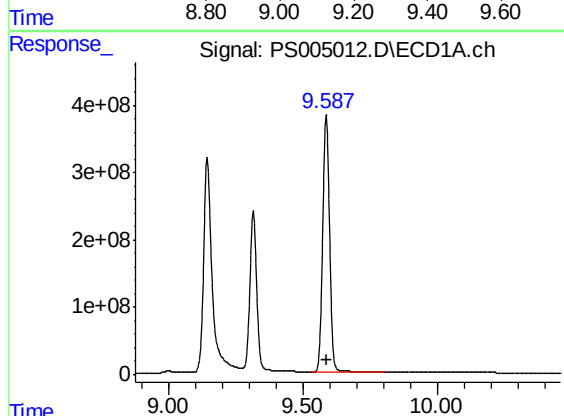

#16 DCPA

R.T.: 9.588 min
Delta R.T.: 0.000 min
Response: 6816616838
Conc: 720.00 ng/ml

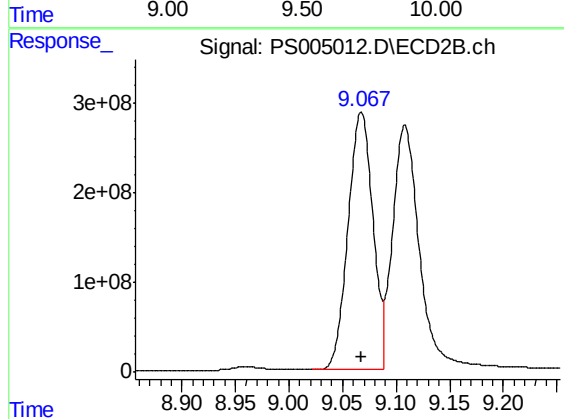

#16 DCPA

R.T.: 9.067 min
Delta R.T.: 0.000 min
Response: 4647384900
Conc: 720.00 ng/ml