

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061418\
 Data File : PS000350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2018 15:54
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 00:57:12 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
 Quant Title : 8080.M
 QLast Update : Thu May 31 04:46:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.815	11.188	175.8E6	150.9E6	497.877	480.574
Target Compounds							
10) T	Pentachlo...	14.083	13.635	3317990	2640980	0.664	0.599
15) T	Picloram	17.370	17.142	6773859	4870629	2.590	2.286
16) T	DCPA	0.000	17.142	0	4870629	N.D.	2.357 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061418\
Data File : PS000350.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2018 15:54
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 00:57:12 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
Quant Title : 8080.M
QLast Update : Thu May 31 04:46:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

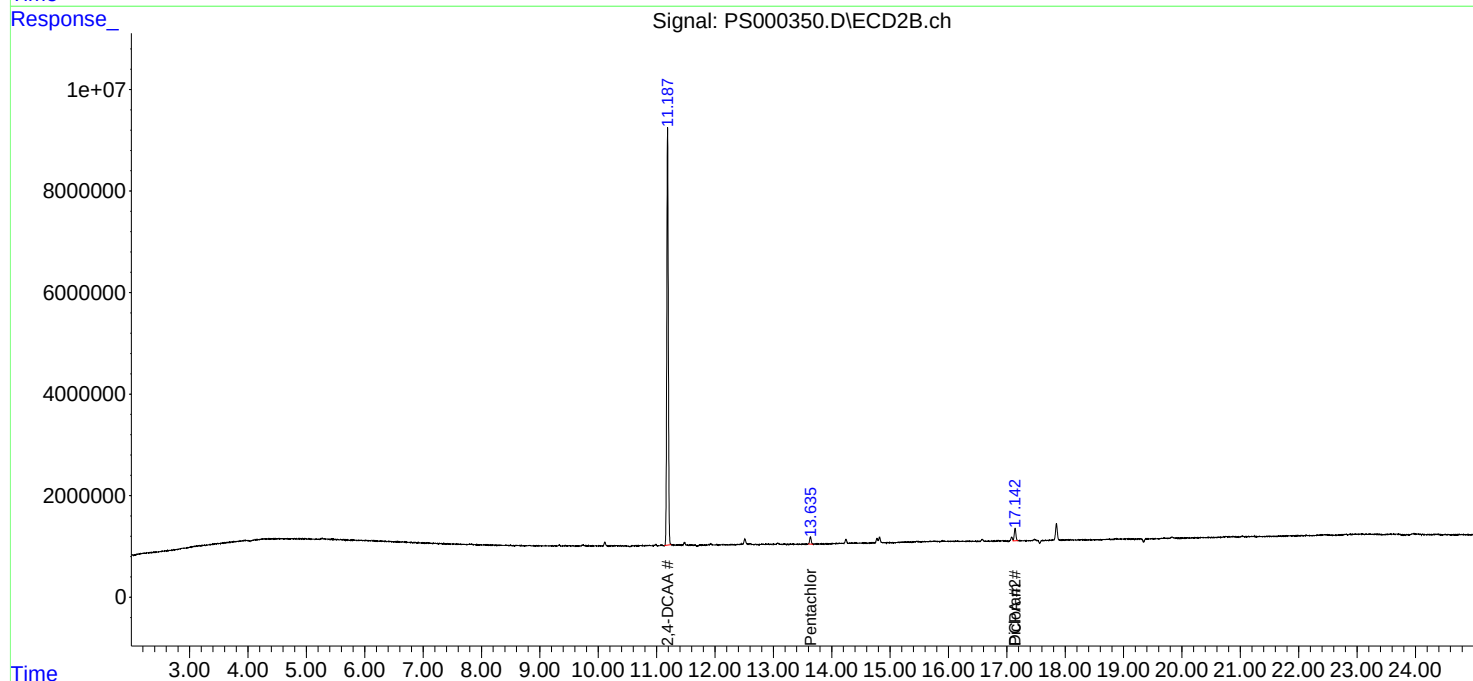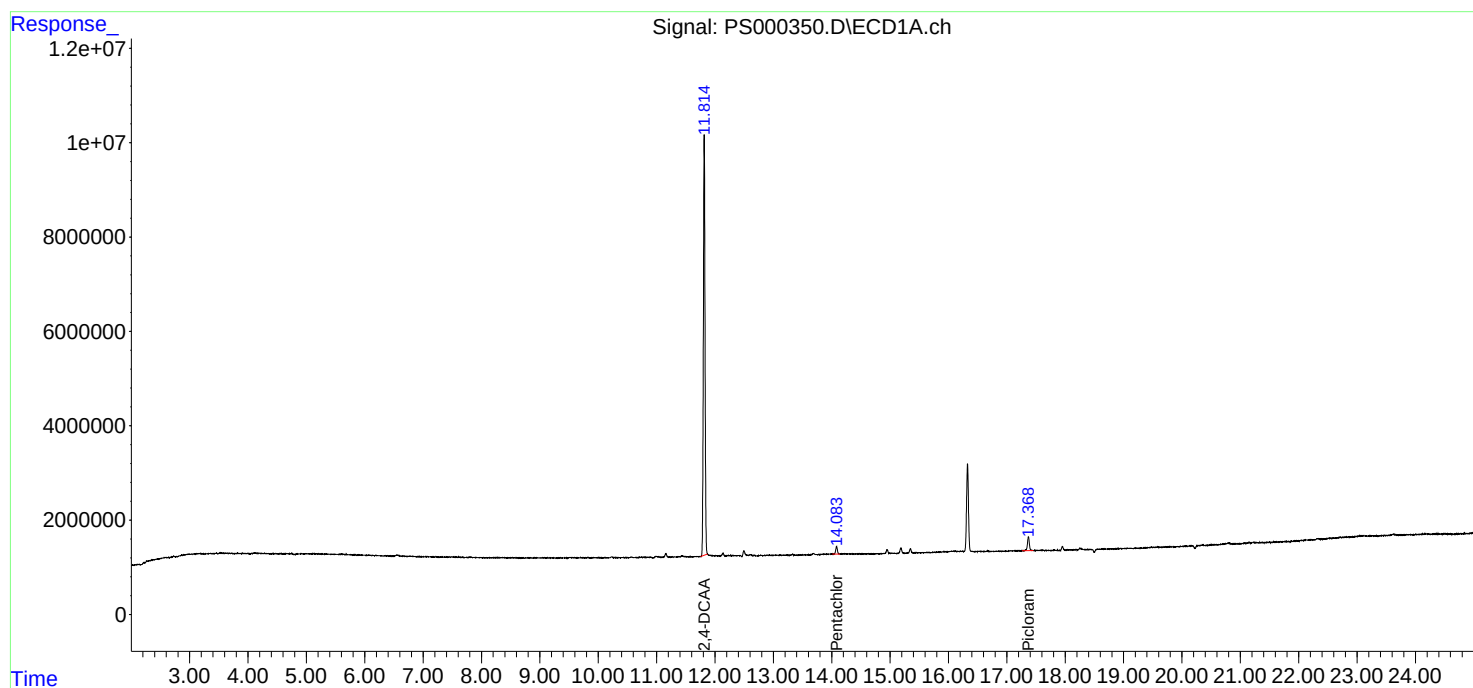


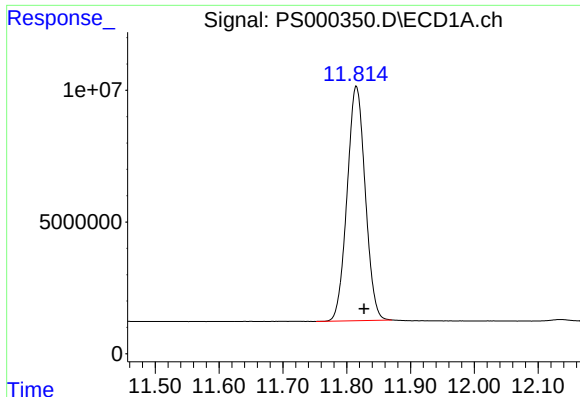

#4 2,4-DCAA


R.T.: 11.815 min
Delta R.T.: -0.012 min
Response: 175788480
Conc: 497.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

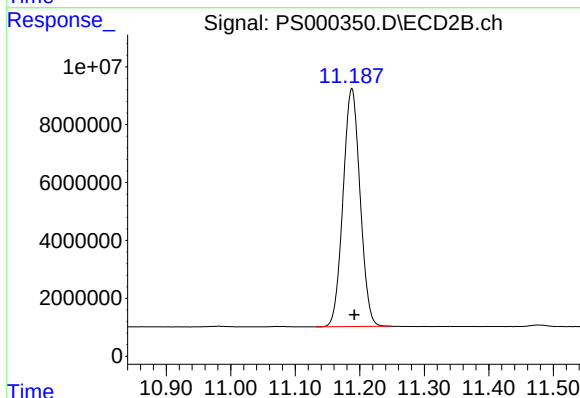


#4 2,4-DCAA

R.T.: 11.188 min
Delta R.T.: -0.004 min
Response: 150949308
Conc: 480.57 ng/ml

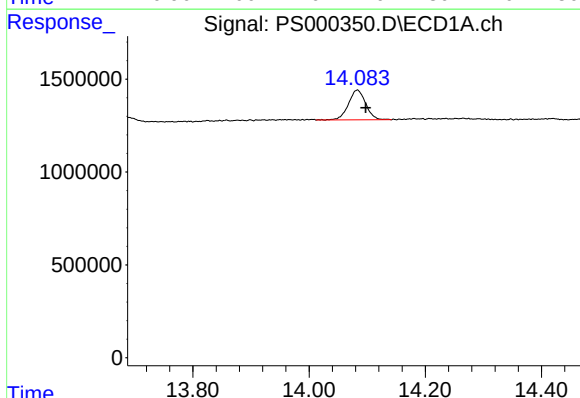


#10 Pentachlorophenol

R.T.: 14.083 min
Delta R.T.: -0.015 min
Response: 3317990
Conc: 0.66 ng/ml

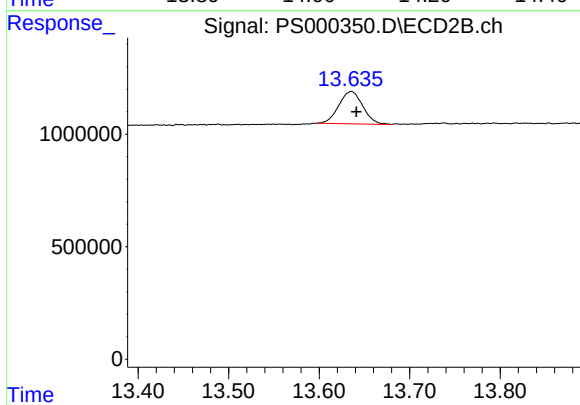

#10 Pentachlorophenol


R.T.: 13.635 min
Delta R.T.: -0.006 min
Response: 2640980
Conc: 0.60 ng/ml

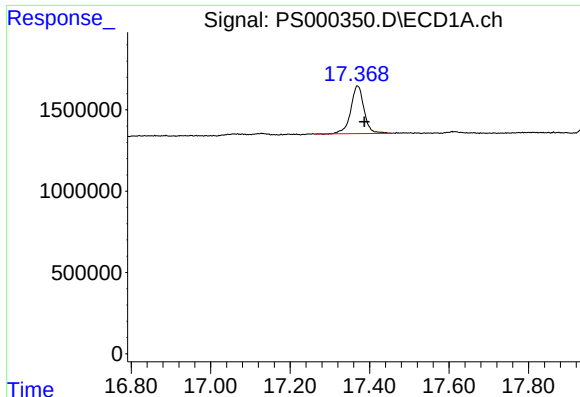

#15 Picloram


R.T.: 17.370 min
Delta R.T.: -0.017 min
Response: 6773859
Conc: 2.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

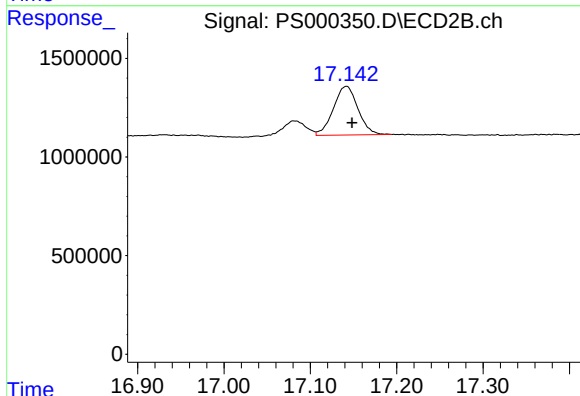


#15 Picloram

R.T.: 17.142 min
Delta R.T.: -0.006 min
Response: 4870629
Conc: 2.29 ng/ml

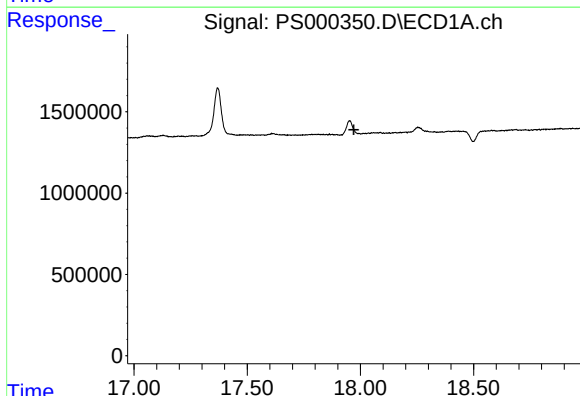

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.971 min
Response: 0
Conc: N.D.

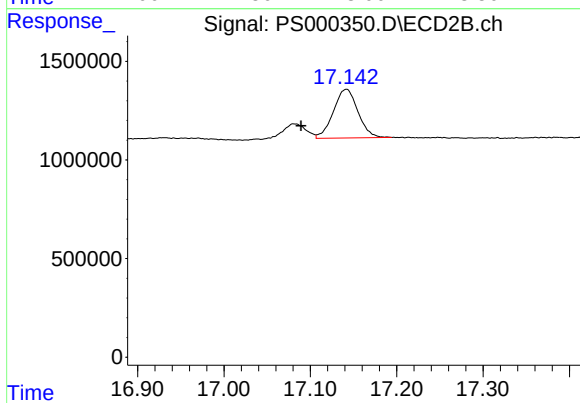

#16 DCPA

R.T.: 17.142 min
Delta R.T.: 0.053 min
Response: 4870629
Conc: 2.36 ng/ml