

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061418\
 Data File : PS000354.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2018 18:59
 Operator : UA
 Sample : PB110193TB
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 00:58:49 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
 Quant Title : 8080.M
 QLast Update : Thu May 31 04:46:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.826	11.199	110.7E6	100.9E6	313.451	321.169
Target Compounds							
1) T	Dalapon	3.122	0.000	7437473	0	15.559	N.D. #
2) T	3,5-DICHL...	0.000	9.346	0	1756996	N.D.	3.979 #
3) T	4-Nitroph...	11.485	10.356	5672370	6186310	24.352	33.218 #
5) T	DICAMBA	0.000	11.443	0	3928869	N.D.	3.551 #
10) T	Pentachlo...	14.094	13.646	3677383	-979746	0.736	N.D. #
11) T	2,4,5-TP ...	0.000	14.182	0	23211145	N.D.	13.494 #
15) T	Picloram	17.380	17.152	4397412	3748502	1.681	1.759
16) T	DCPA	17.966	17.096	2794025	63776	1.154	0.031 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061418\
Data File : PS000354.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2018 18:59
Operator : UA
Sample : PB110193TB
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 00:58:49 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
Quant Title : 8080.M
QLast Update : Thu May 31 04:46:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

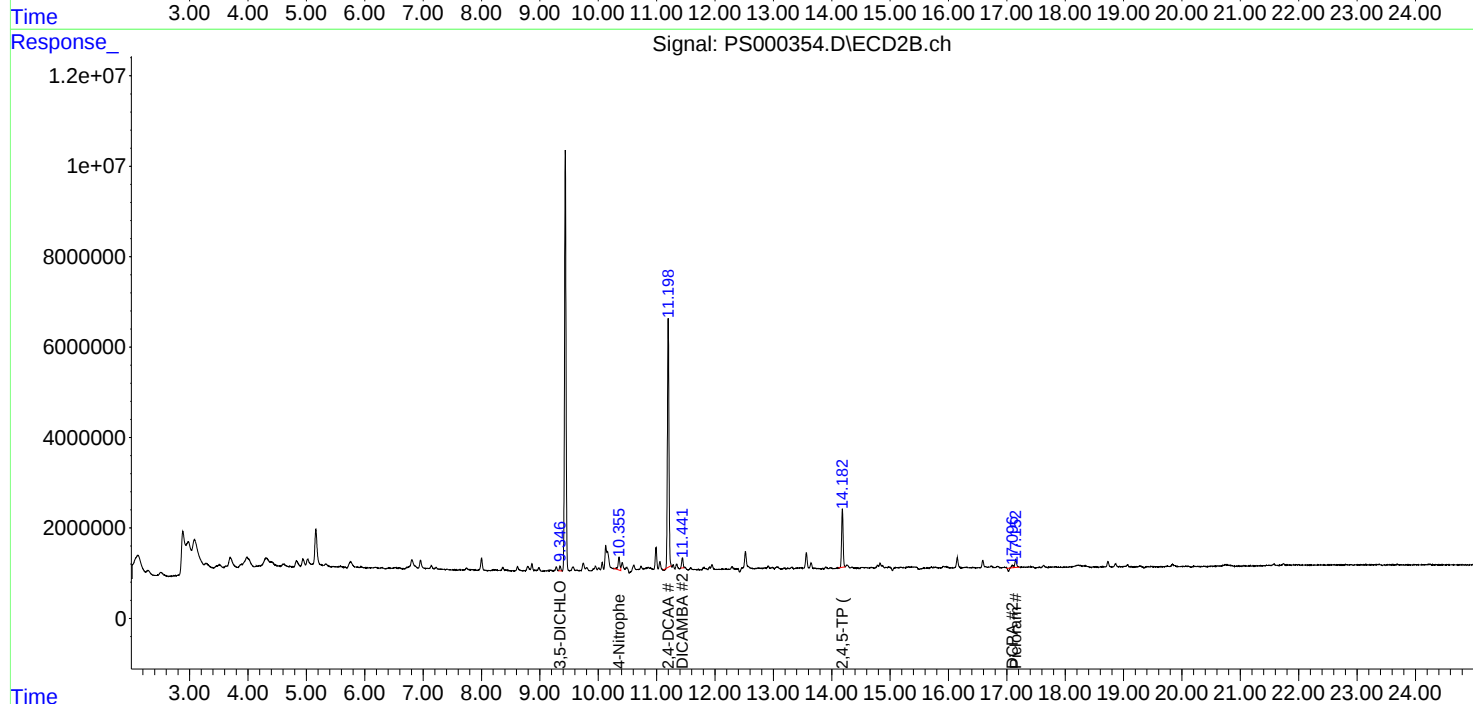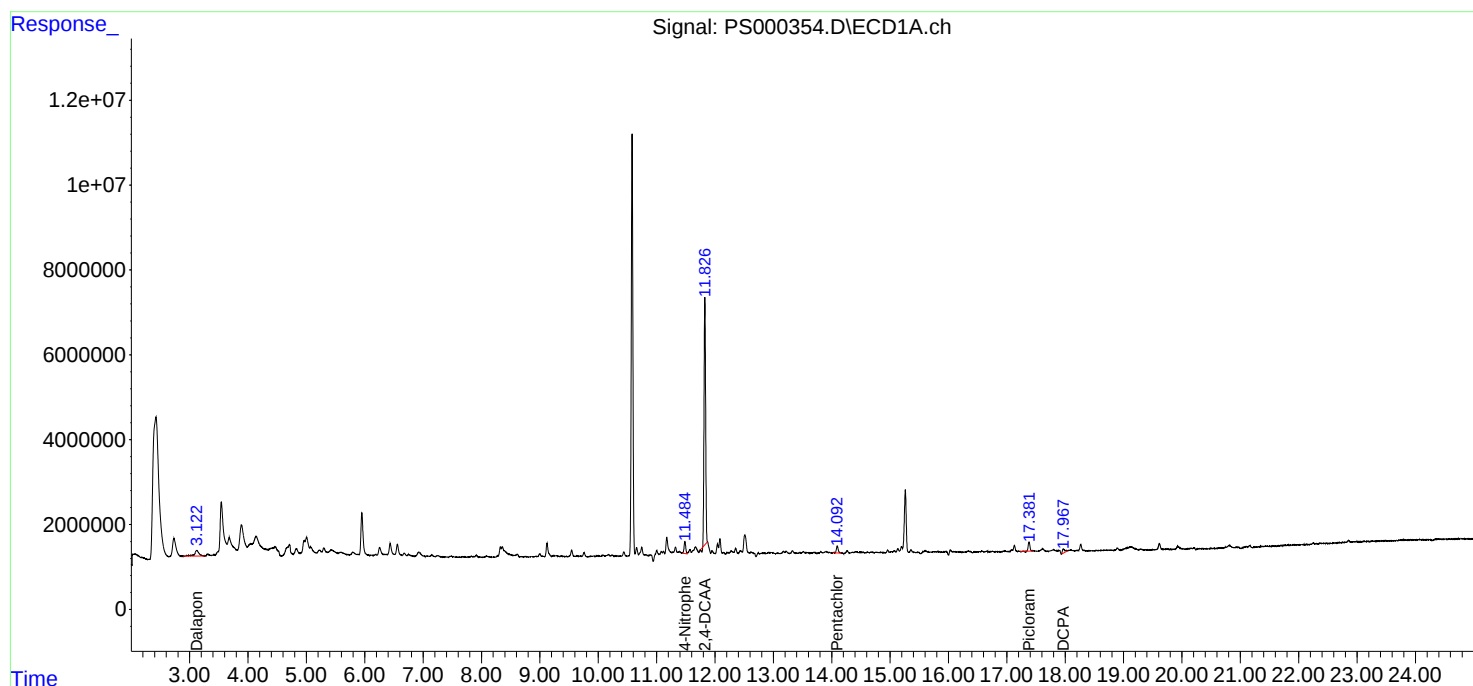


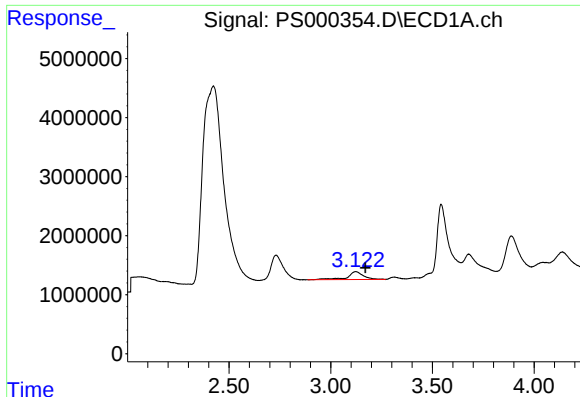

#1 Dalapon


R.T.: 3.122 min
Delta R.T.: -0.048 min
Response: 7437473
Conc: 15.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

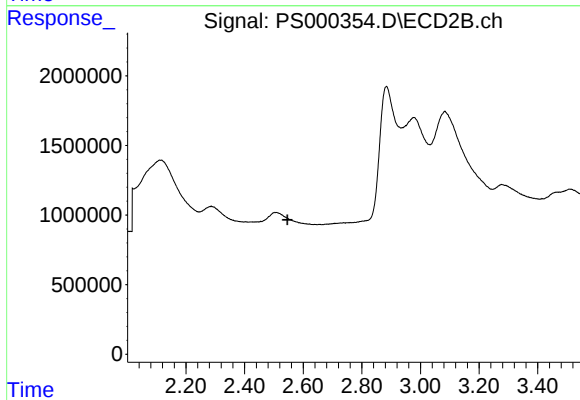


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.546 min
Response: 0
Conc: N.D.

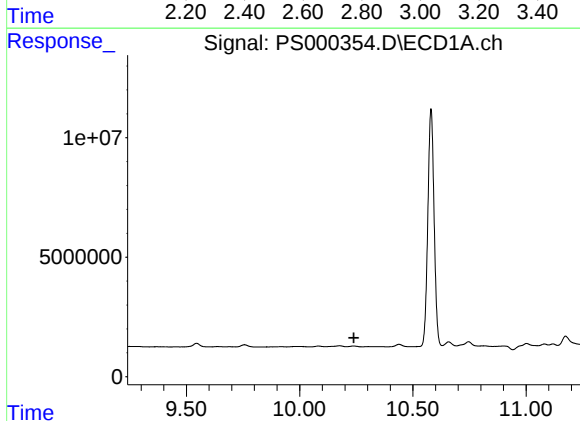


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.239 min
Response: 0
Conc: N.D.

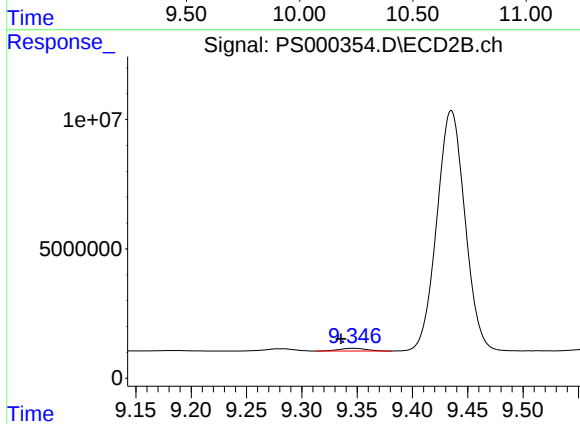

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.346 min
Delta R.T.: 0.011 min
Response: 1756996
Conc: 3.98 ng/ml

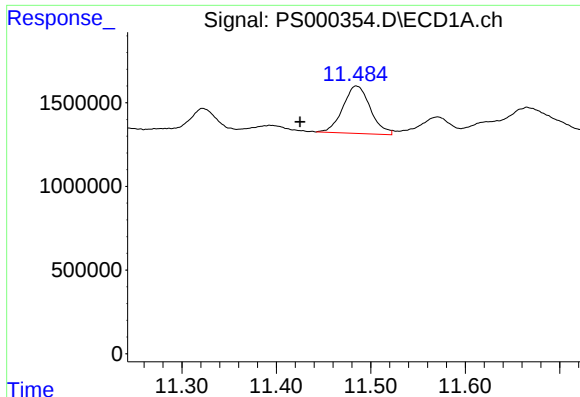

#3 4-Nitrophenol


R.T.: 11.485 min
Delta R.T.: 0.060 min
Response: 5672370
Conc: 24.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

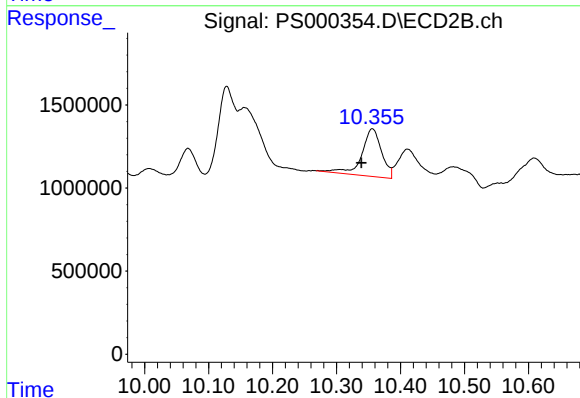


#3 4-Nitrophenol

R.T.: 10.356 min
Delta R.T.: 0.017 min
Response: 6186310
Conc: 33.22 ng/ml

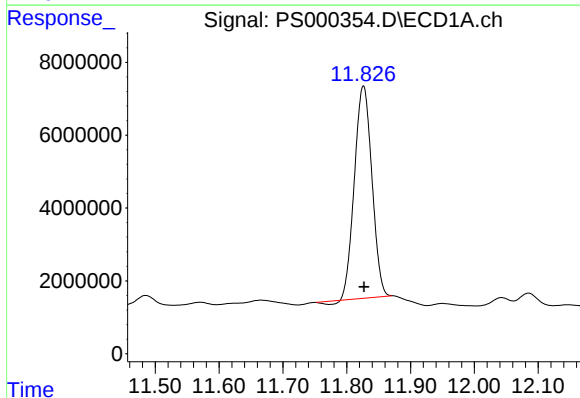


#4 2,4-DCAA

R.T.: 11.826 min
Delta R.T.: -0.001 min
Response: 110672117
Conc: 313.45 ng/ml

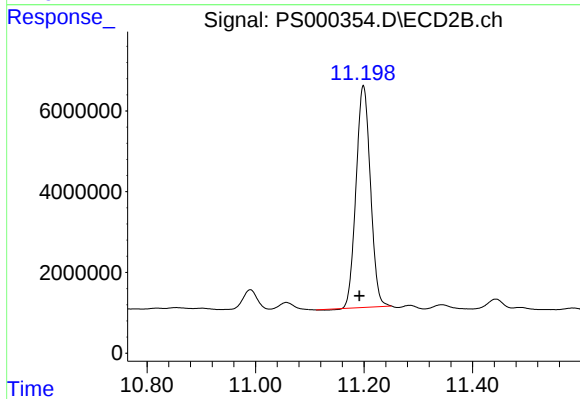

#4 2,4-DCAA


R.T.: 11.199 min
Delta R.T.: 0.007 min
Response: 100879756
Conc: 321.17 ng/ml

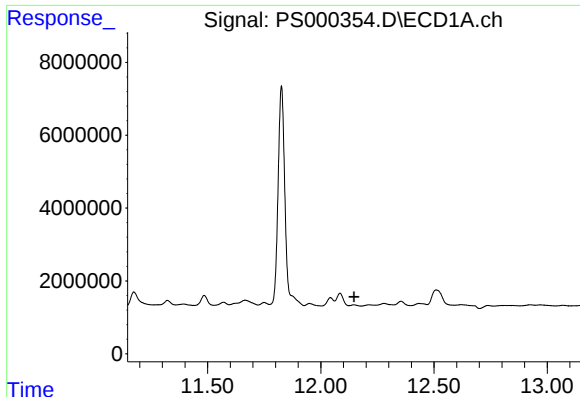

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 12.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

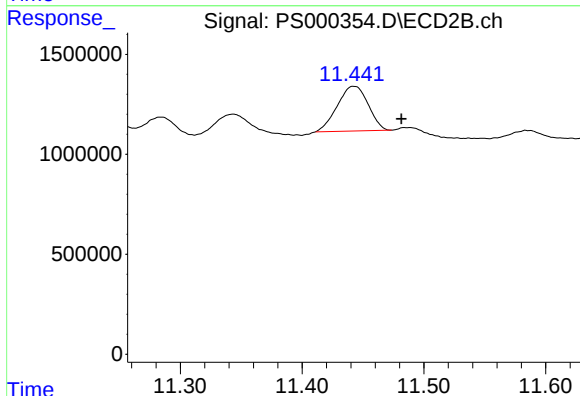


#5 DICAMBA

R.T.: 11.443 min
Delta R.T.: -0.039 min
Response: 3928869
Conc: 3.55 ng/ml

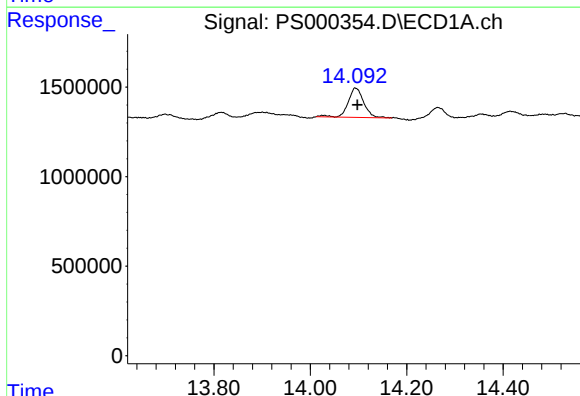


#10 Pentachlorophenol

R.T.: 14.094 min
Delta R.T.: -0.004 min
Response: 3677383
Conc: 0.74 ng/ml

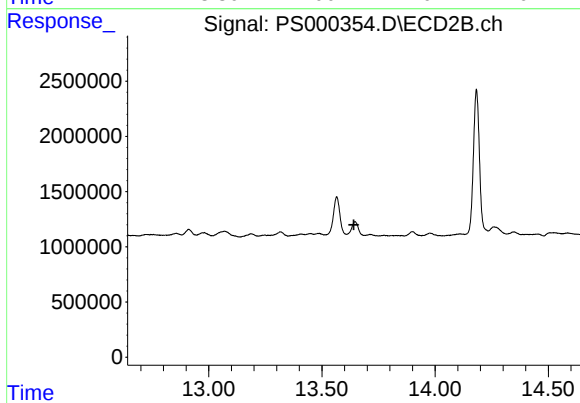

#10 Pentachlorophenol


R.T.: 13.646 min
Delta R.T.: 0.005 min
Response: -979746
Conc: N.D.

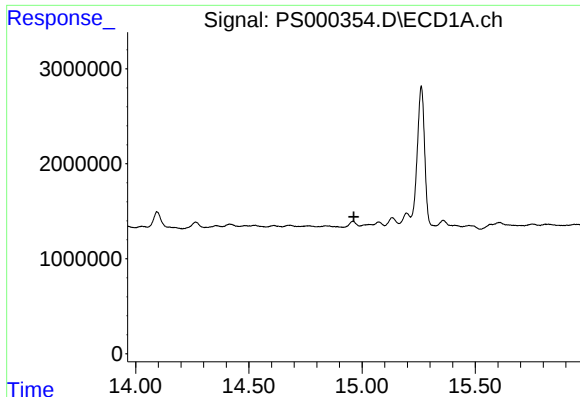

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.964 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

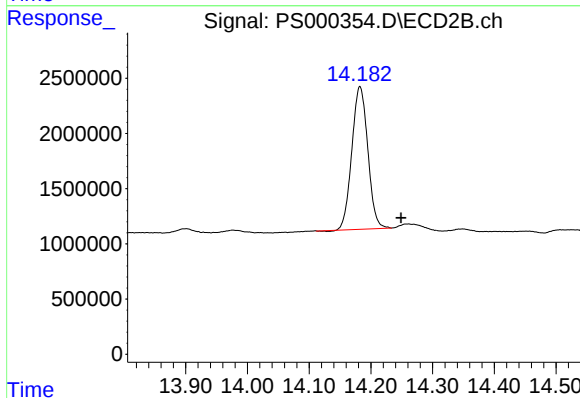


#11 2,4,5-TP (SILVEX)

R.T.: 14.182 min
Delta R.T.: -0.067 min
Response: 23211145
Conc: 13.49 ng/ml

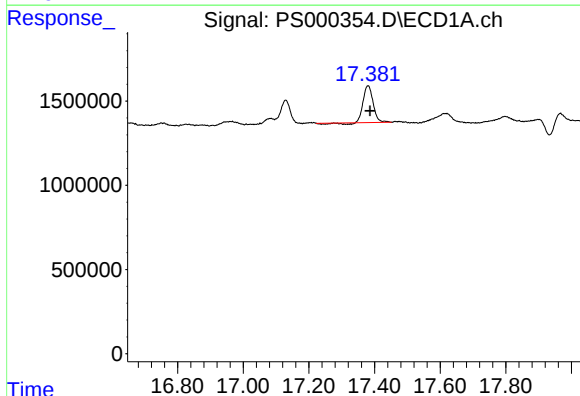


#15 Picloram

R.T.: 17.380 min
Delta R.T.: -0.007 min
Response: 4397412
Conc: 1.68 ng/ml

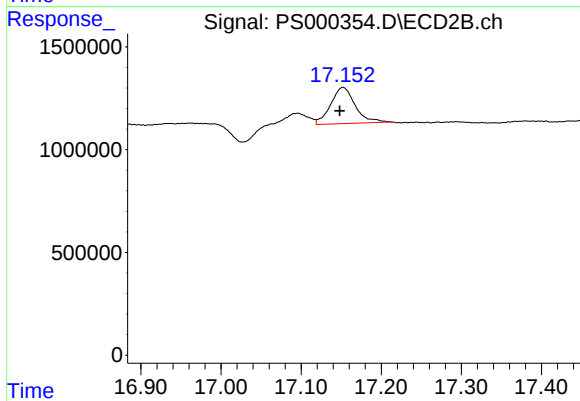

#15 Picloram


R.T.: 17.152 min
Delta R.T.: 0.004 min
Response: 3748502
Conc: 1.76 ng/ml

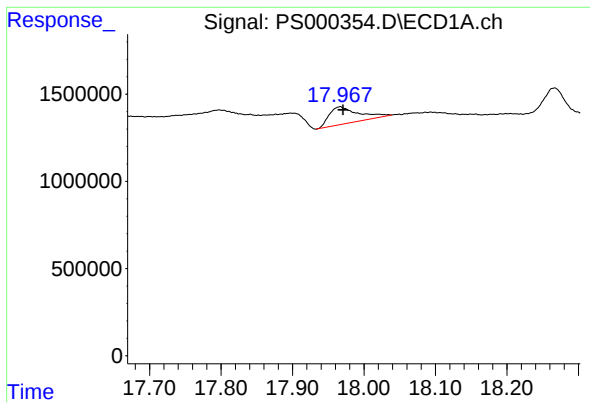

#16 DCPA

R.T.: 17.966 min
Delta R.T.: -0.005 min
Response: 2794025
Conc: 1.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

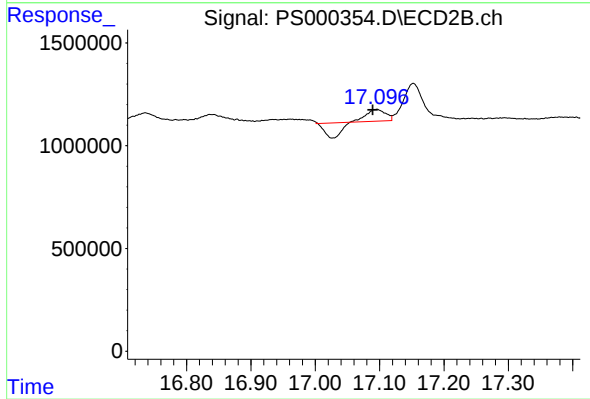

#16 DCPA

R.T.: 17.096 min
Delta R.T.: 0.007 min
Response: 63776
Conc: 0.03 ng/ml