

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS061418\  
 Data File : PS000363.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 14 Jun 2018 23:37  
 Operator : UA  
 Sample : J3372-05  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 15 01:02:13 2018  
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS052118.M  
 Quant Title : 8080.M  
 QLast Update : Thu May 31 04:46:50 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1  | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|--------------|--------|--------|---------|---------|---------|---------|
| -----                       |              |        |        |         |         |         |         |
| System Monitoring Compounds |              |        |        |         |         |         |         |
| 4) S                        | 2,4-DCAA     | 11.816 | 11.190 | 121.3E6 | 106.4E6 | 343.620 | 338.890 |
| Target Compounds            |              |        |        |         |         |         |         |
| 3) T                        | 4-Nitroph... | 11.475 | 10.348 | 4937299 | 4220253 | 21.197  | 22.661  |
| 5) T                        | DICAMBA      | 0.000  | 11.434 | 0       | 3058722 | N.D.    | 2.765 # |
| 7) T                        | MCPA         | 12.728 | 0.000  | 1278985 | 0       | 0.683   | N.D. #  |
| 15) T                       | Picloram     | 0.000  | 17.143 | 0       | 4932138 | N.D.    | 2.315 # |
| 16) T                       | DCPA         | 0.000  | 17.143 | 0       | 4932138 | N.D.    | 2.387 # |
| -----                       |              |        |        |         |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS061418\  
Data File : PS000363.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 14 Jun 2018 23:37  
Operator : UA  
Sample : J3372-05  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 15 01:02:13 2018  
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS052118.M  
Quant Title : 8080.M  
QLast Update : Thu May 31 04:46:50 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

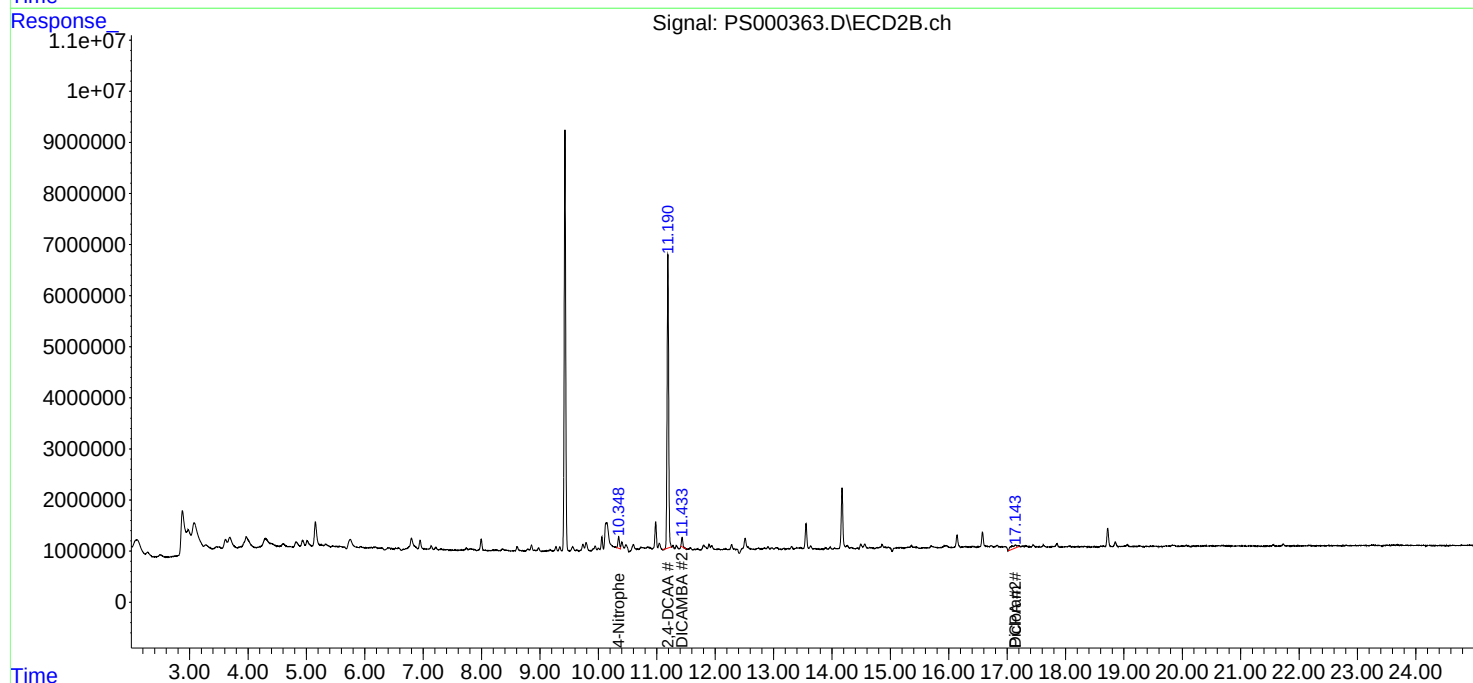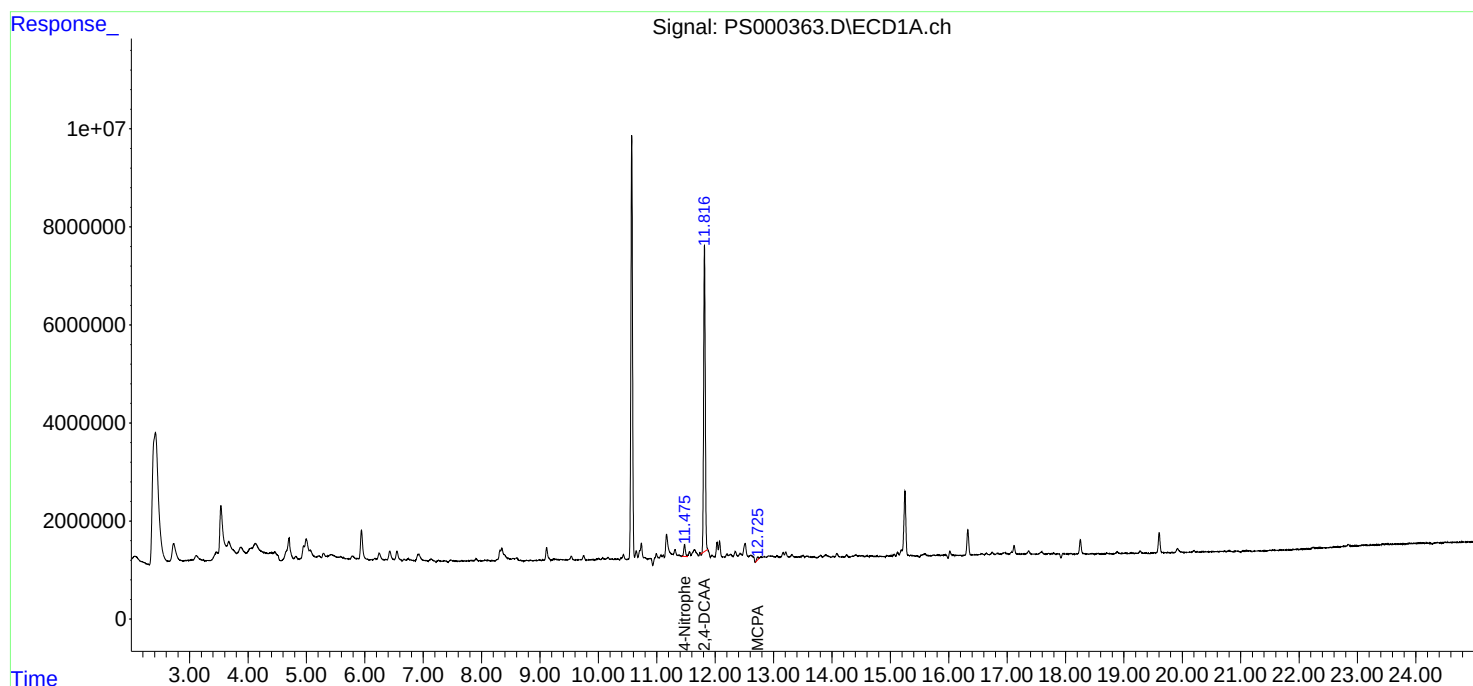


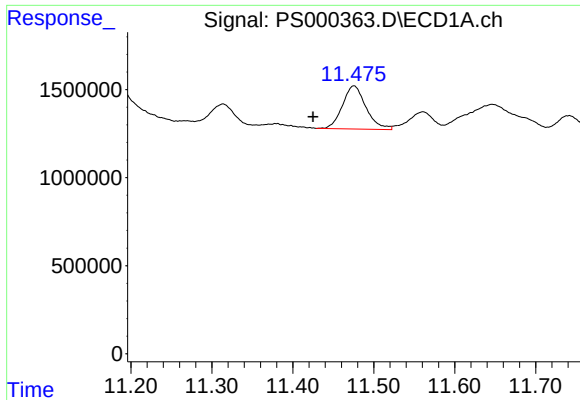

#3 4-Nitrophenol


R.T.: 11.475 min  
Delta R.T.: 0.050 min  
Response: 4937299  
Conc: 21.20 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

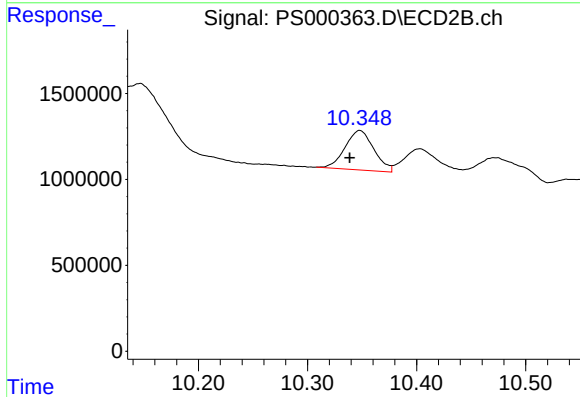


#3 4-Nitrophenol

R.T.: 10.348 min  
Delta R.T.: 0.009 min  
Response: 4220253  
Conc: 22.66 ng/ml

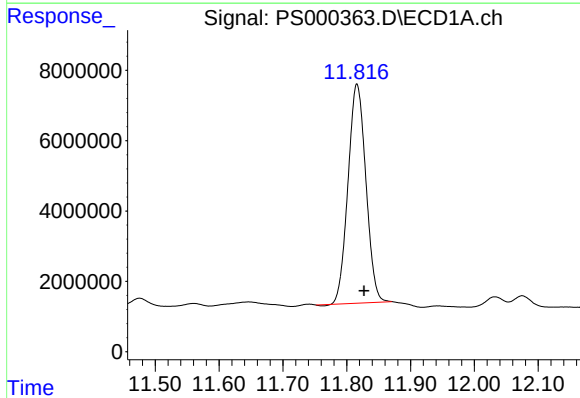


#4 2,4-DCAA

R.T.: 11.816 min  
Delta R.T.: -0.011 min  
Response: 121324212  
Conc: 343.62 ng/ml

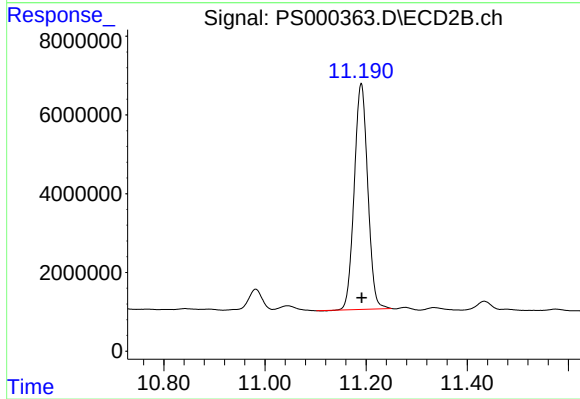

#4 2,4-DCAA


R.T.: 11.190 min  
Delta R.T.: -0.001 min  
Response: 106445882  
Conc: 338.89 ng/ml

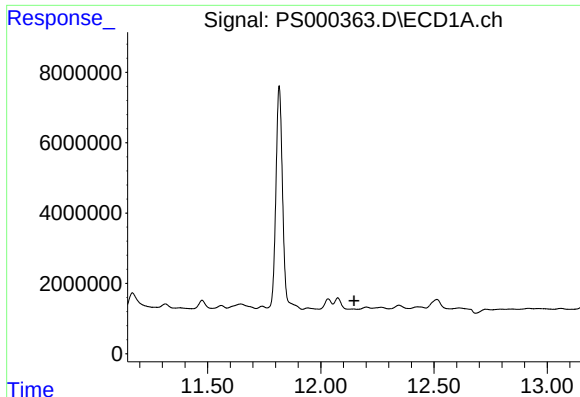

#5 DICAMBA


R.T.: 0.000 min  
Exp R.T.: 12.147 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

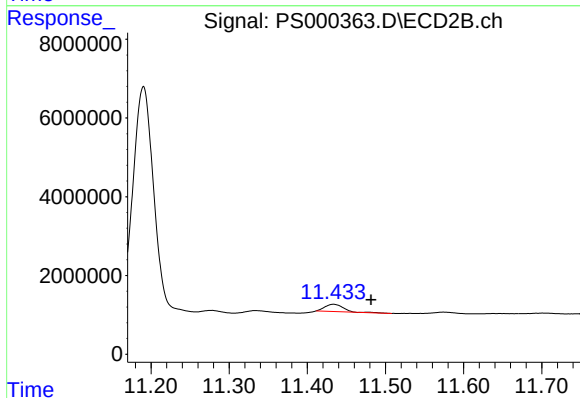


#5 DICAMBA

R.T.: 11.434 min  
Delta R.T.: -0.048 min  
Response: 3058722  
Conc: 2.76 ng/ml

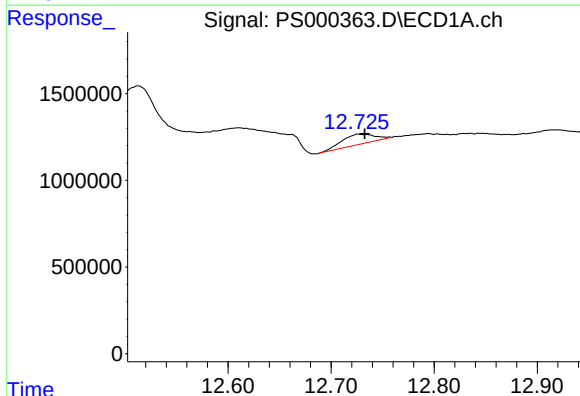


#7 MCPA

R.T.: 12.728 min  
Delta R.T.: -0.004 min  
Response: 1278985  
Conc: 0.68 ug/ml

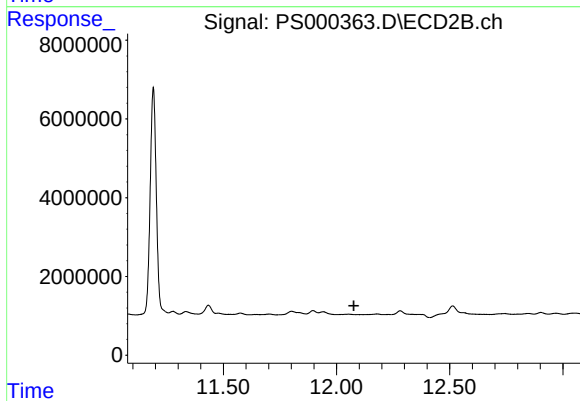

#7 MCPA


R.T.: 0.000 min  
Exp R.T.: 12.077 min  
Response: 0  
Conc: N.D.

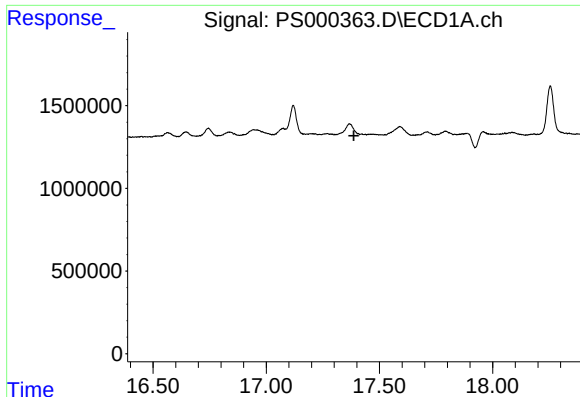

#15 Picloram


R.T.: 0.000 min  
Exp R.T. : 17.387 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

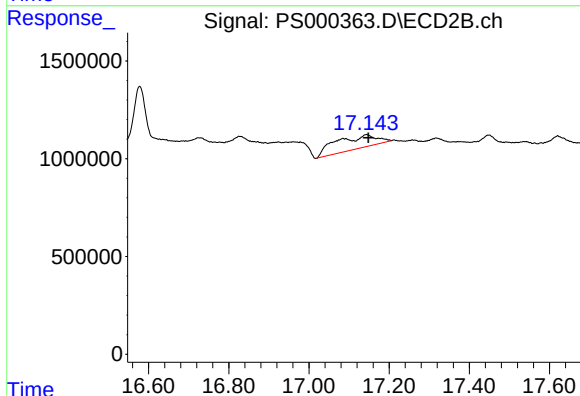


#15 Picloram

R.T.: 17.143 min  
Delta R.T.: -0.005 min  
Response: 4932138  
Conc: 2.31 ng/ml

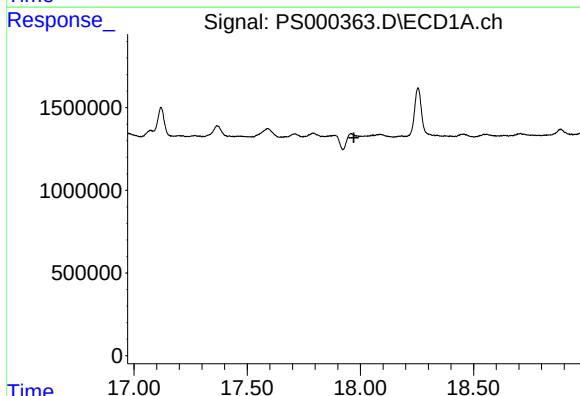

#16 DCPA

R.T.: 0.000 min  
Exp R.T. : 17.971 min  
Response: 0  
Conc: N.D.

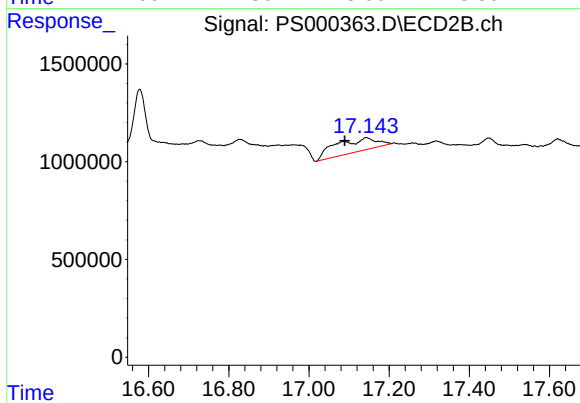

#16 DCPA

R.T.: 17.143 min  
Delta R.T.: 0.054 min  
Response: 4932138  
Conc: 2.39 ng/ml