

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061418\
 Data File : PS000363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2018 23:37
 Operator : UA
 Sample : J3372-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SB-30COMP

Manual Integrations
 APPROVED

UGO
 6/15/2018 12:09:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 01:02:13 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
 Quant Title : 8080.M
 QLast Update : Thu May 31 04:46:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	11.816	11.190	125.6E6	107.4E6	355.718m	341.839m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061418\
Data File : PS000363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2018 23:37
Operator : UA
Sample : J3372-05
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SB-30COMP


Manual Integrations
APPROVED

UGO
6/15/2018 12:09:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 01:02:13 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
Quant Title : 8080.M
QLast Update : Thu May 31 04:46:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

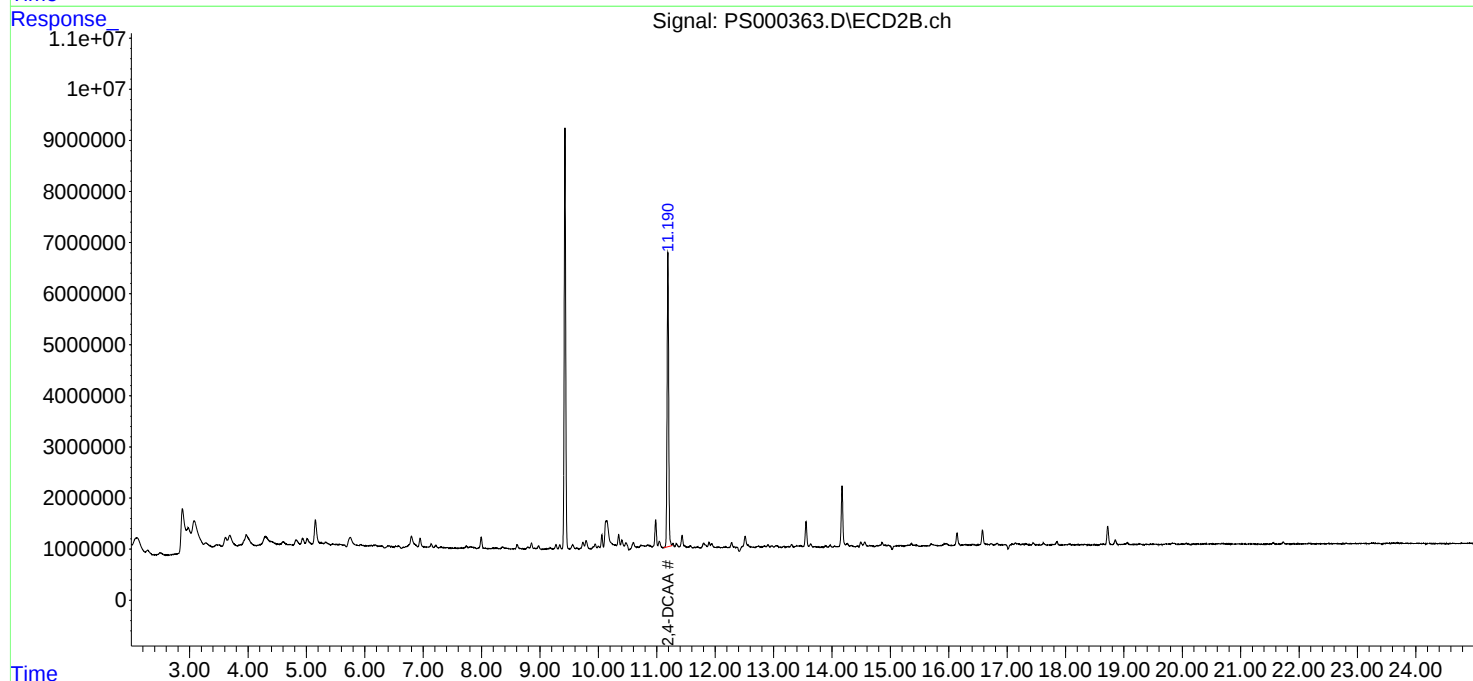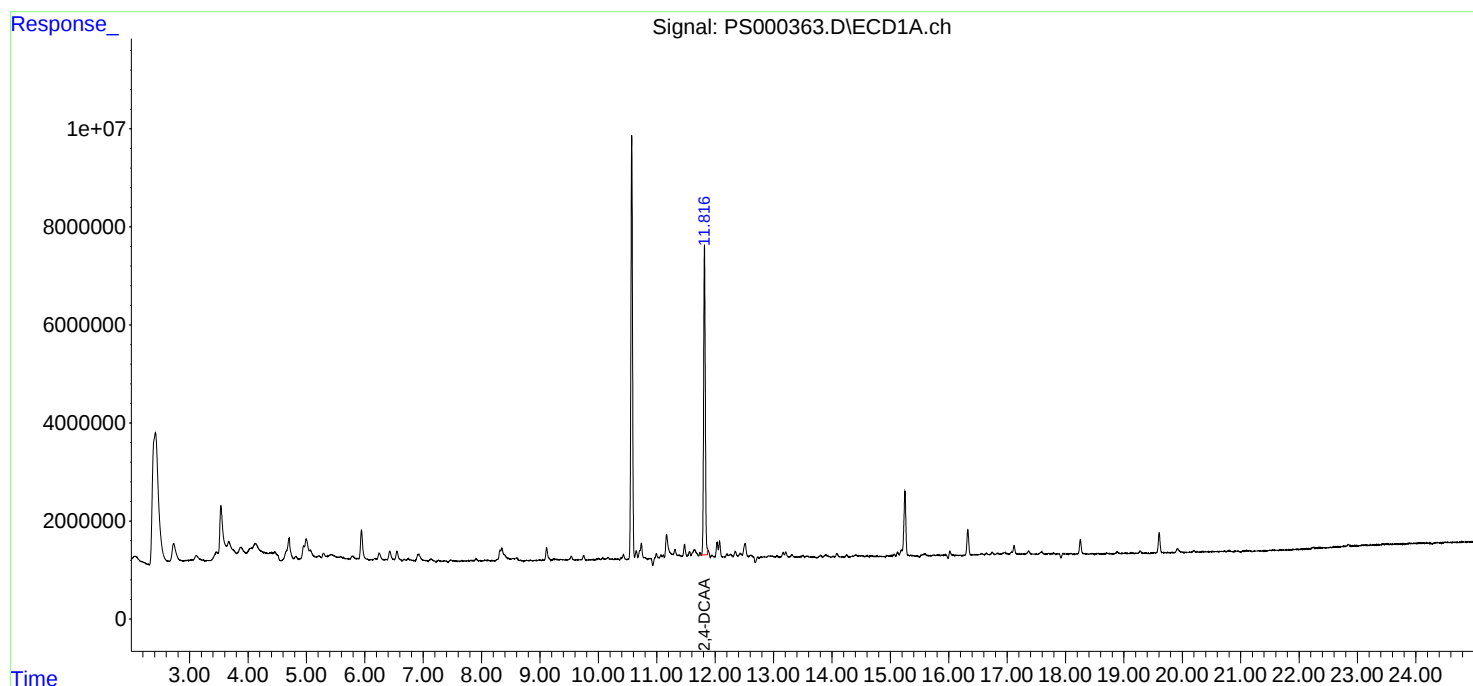

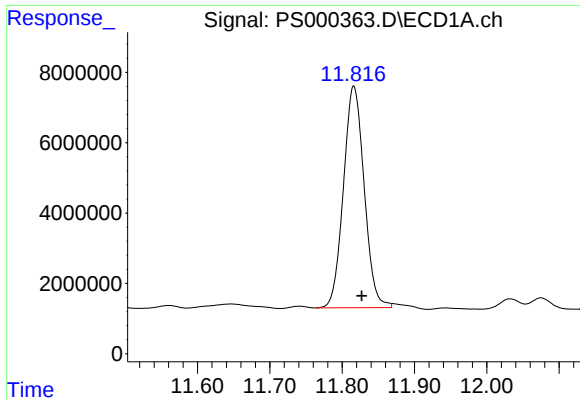


#4 2,4-DCAA

R.T.: 11.816 min
Delta R.T.: -0.012 min
Response: 125595711
Conc: 355.72 ng/ml m

Instrument :
ECD_S
ClientSampleId :
SB-30COMP

Manual Integrations
APPROVED

UGO
6/15/2018 12:09:38 PM

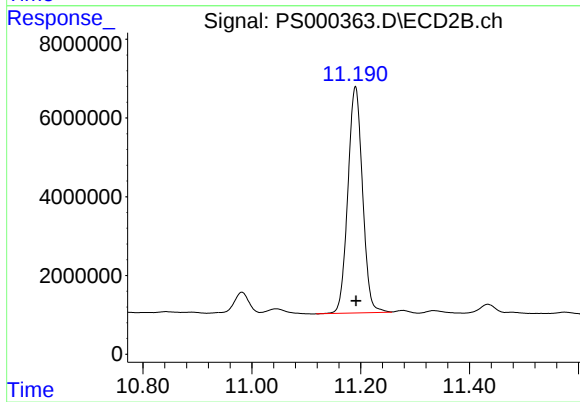

#4 2,4-DCAA

R.T.: 11.190 min
Delta R.T.: -0.002 min
Response: 107372303
Conc: 341.84 ng/ml m