

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061419\
 Data File : PS005023.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2019 16:08
 Operator : SM\AJ
 Sample : PB120603BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB120603BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 22:54:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.590	5.303	669.3E6	482.4E6	507.893	483.639
Target Compounds							
2) T	3,5-DICHL...	0.000	4.621	0	50189802	N.D.	39.217
5) T	DICAMBA	0.000	5.420	0	16525818	N.D.	4.303
7) T	MCPA	5.994	5.694	19466328	33502288	3.106	7.948 #
9) T	2,4-D	0.000	6.201	0	21181277	N.D.	19.792
10) T	Pentachlo...	0.000	6.570	0	29905067	N.D.	2.321
12) T	2,4,5-T	7.604	0.000	37681181	0	4.716	N.D. #
15) T	Picloram	0.000	9.131	0	34340999	N.D.	5.034



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061419\
Data File : PS005023.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2019 16:08
Operator : SM\AJ
Sample : PB120603BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB120603BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 22:54:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

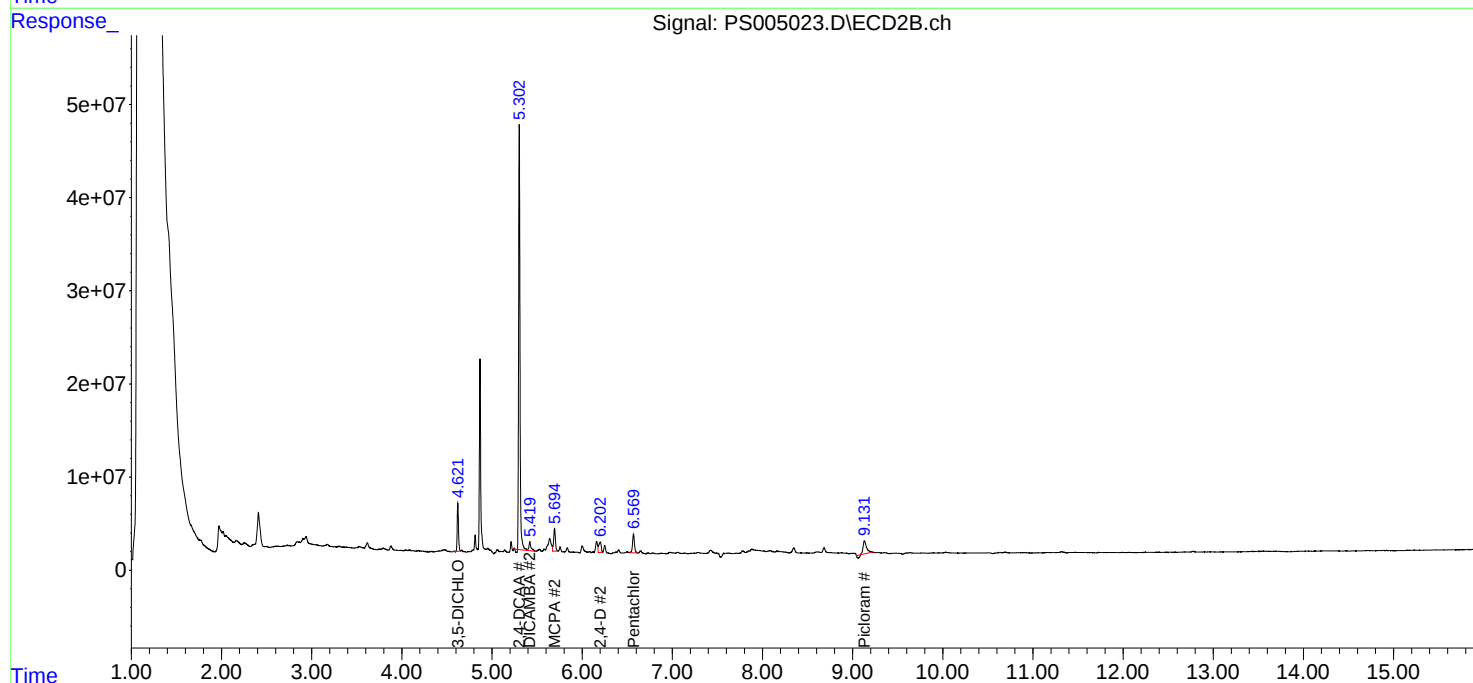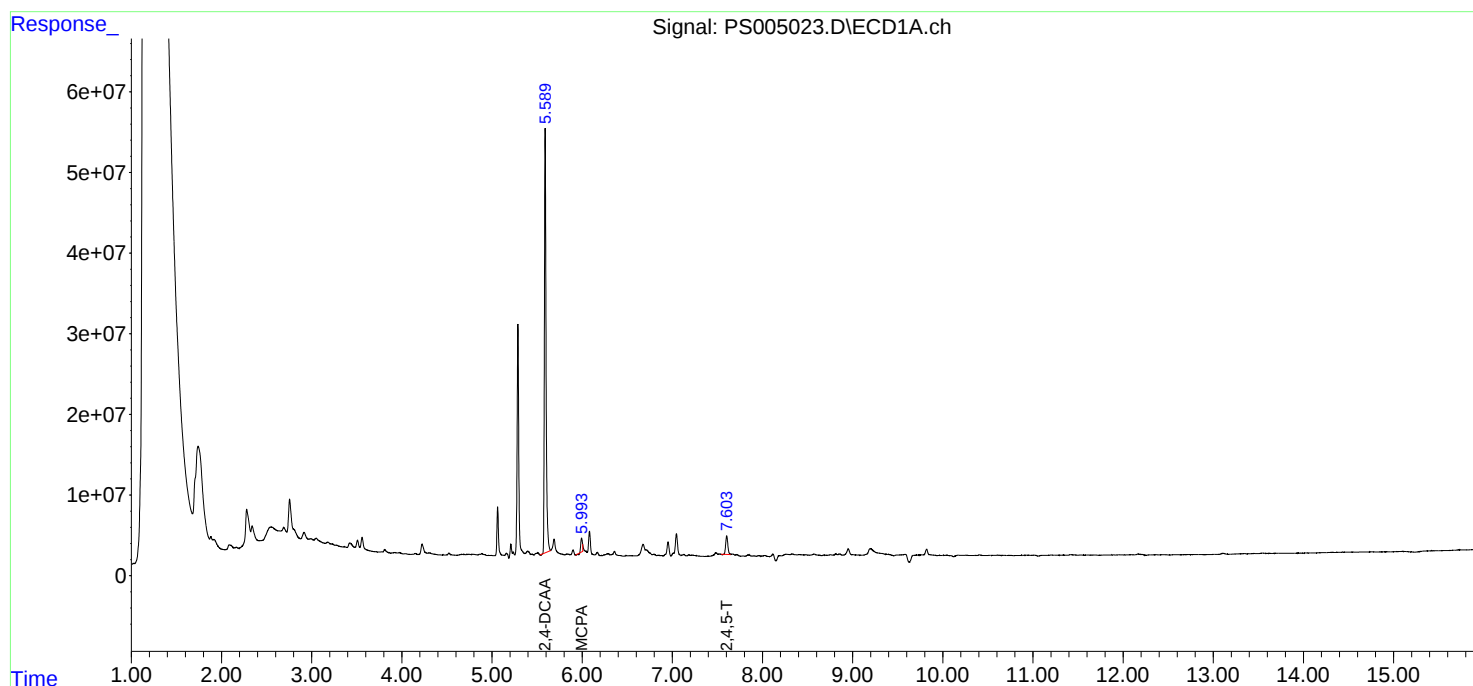


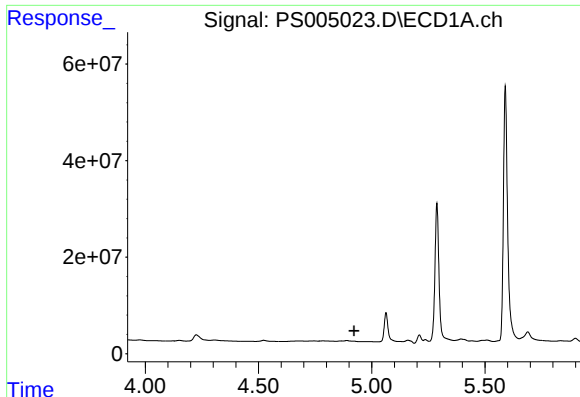

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.922 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB120603BL

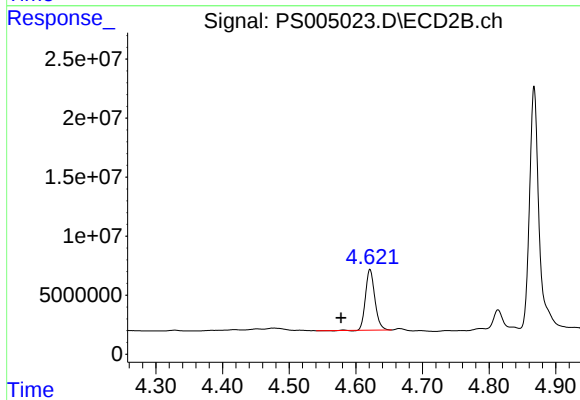


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.621 min
Delta R.T.: 0.044 min
Response: 50189802
Conc: 39.22 ng/ml

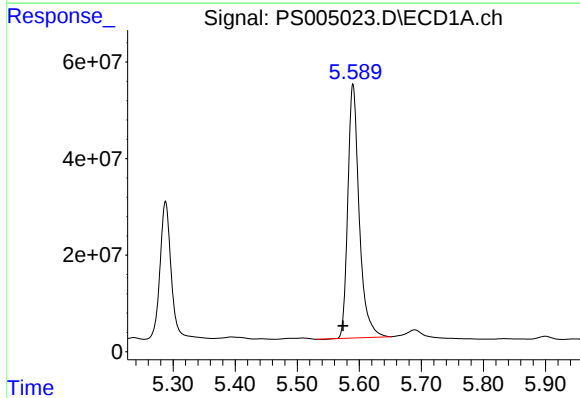


#4 2,4-DCAA

R.T.: 5.590 min
Delta R.T.: 0.016 min
Response: 669299635
Conc: 507.89 ng/ml

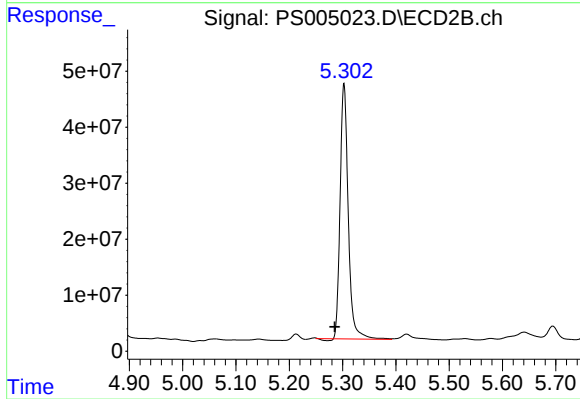

#4 2,4-DCAA


R.T.: 5.303 min
Delta R.T.: 0.018 min
Response: 482447568
Conc: 483.64 ng/ml

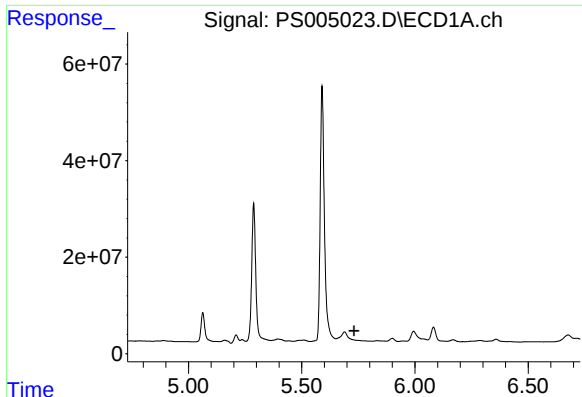

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.731 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB120603BL

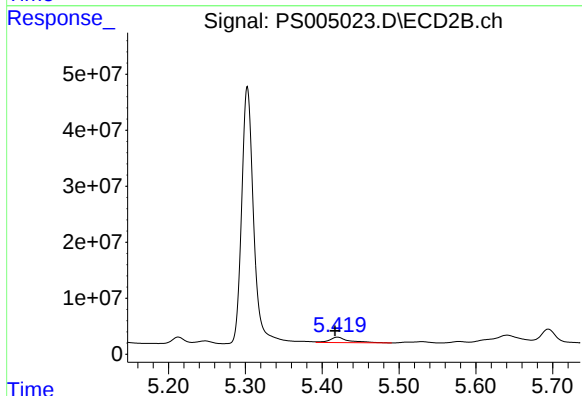


#5 DICAMBA

R.T.: 5.420 min
Delta R.T.: 0.003 min
Response: 16525818
Conc: 4.30 ng/ml

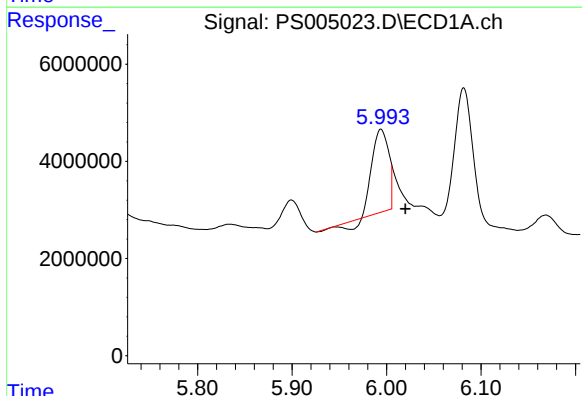


#7 MCPA

R.T.: 5.994 min
Delta R.T.: -0.026 min
Response: 19466328
Conc: 3.11 ug/ml

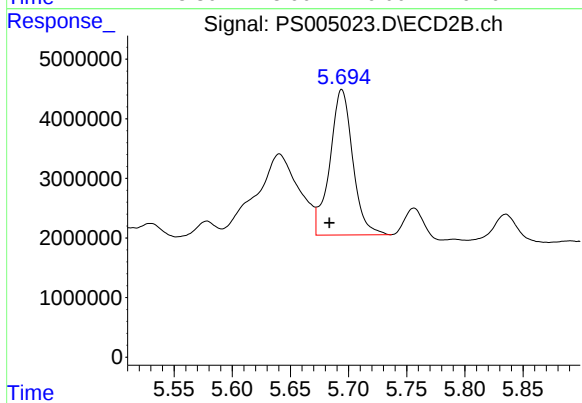

#7 MCPA


R.T.: 5.694 min
Delta R.T.: 0.011 min
Response: 33502288
Conc: 7.95 ug/ml

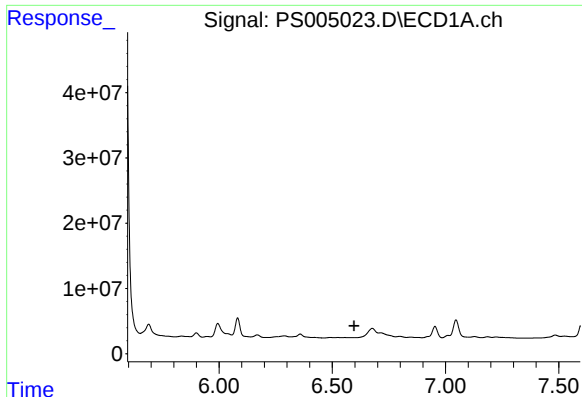

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.596 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB120603BL

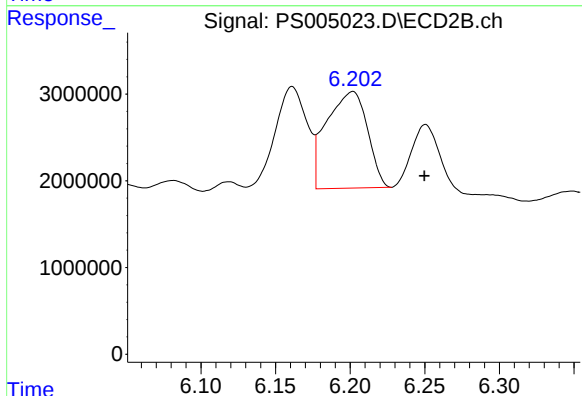


#9 2,4-D

R.T.: 6.201 min
Delta R.T.: -0.048 min
Response: 21181277
Conc: 19.79 ng/ml

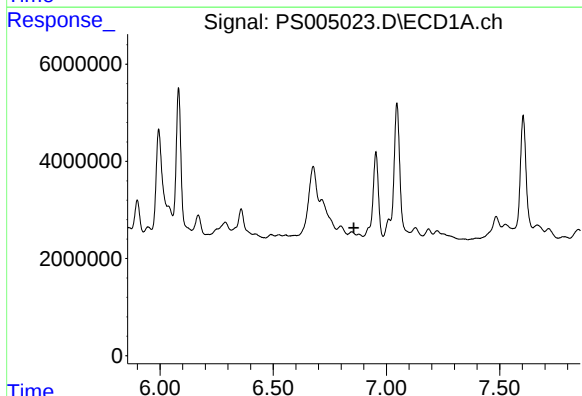


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.856 min
Response: 0
Conc: N.D.

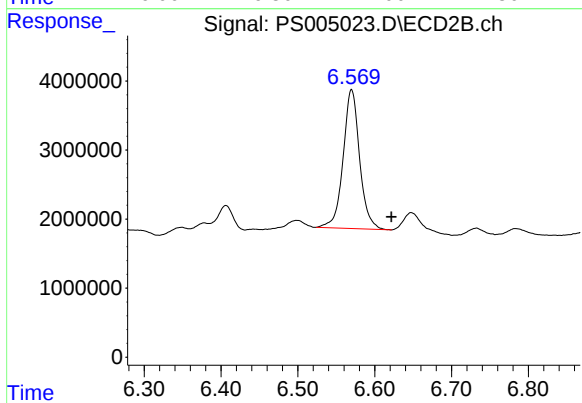

#10 Pentachlorophenol


R.T.: 6.570 min
Delta R.T.: -0.052 min
Response: 29905067
Conc: 2.32 ng/ml

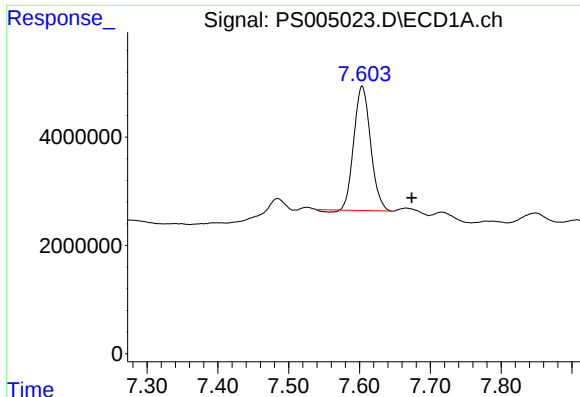

#12 2,4,5-T


R.T.: 7.604 min
Delta R.T.: -0.070 min
Response: 37681181
Conc: 4.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB120603BL

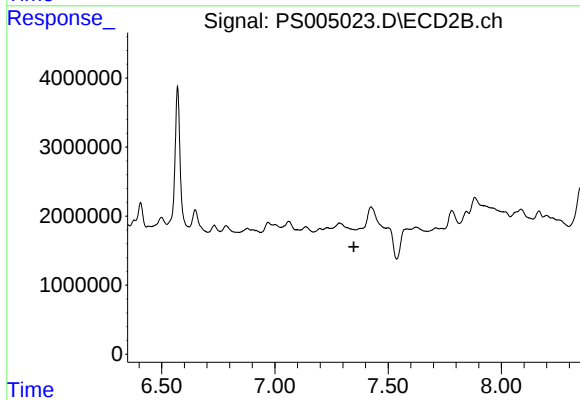


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.349 min
Response: 0
Conc: N.D.

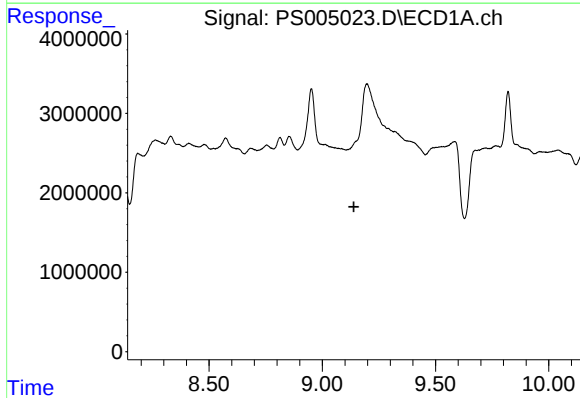

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.139 min
Response: 0
Conc: N.D.

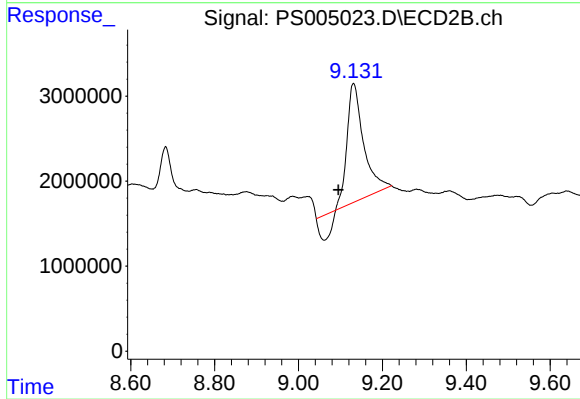

#15 Picloram

R.T.: 9.131 min
Delta R.T.: 0.036 min
Response: 34340999
Conc: 5.03 ng/ml