

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061419\
 Data File : PS005031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2019 19:04
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 22:57:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.605	5.317	525.3E6	383.6E6	398.643	384.498
Target Compounds							
2) T	3,5-DICHL...	4.968	0.000	1399.4E6	0	742.475	N.D. #
5) T	DICAMBA	0.000	5.470	0	1074.9E6	N.D.	279.882
6) T	MCP	0.000	5.470	0	1074.9E6	N.D.	372.003
9) T	2,4-D	6.642	0.000	964.1E6	0	714.480	N.D. #
15) T	Picloram	9.142	0.000	308.5E6	0	31.078	N.D. #
16) T	DCPA	0.000	8.981	0	41328745	N.D.	6.267



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061419\
Data File : PS005031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2019 19:04
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 22:57:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

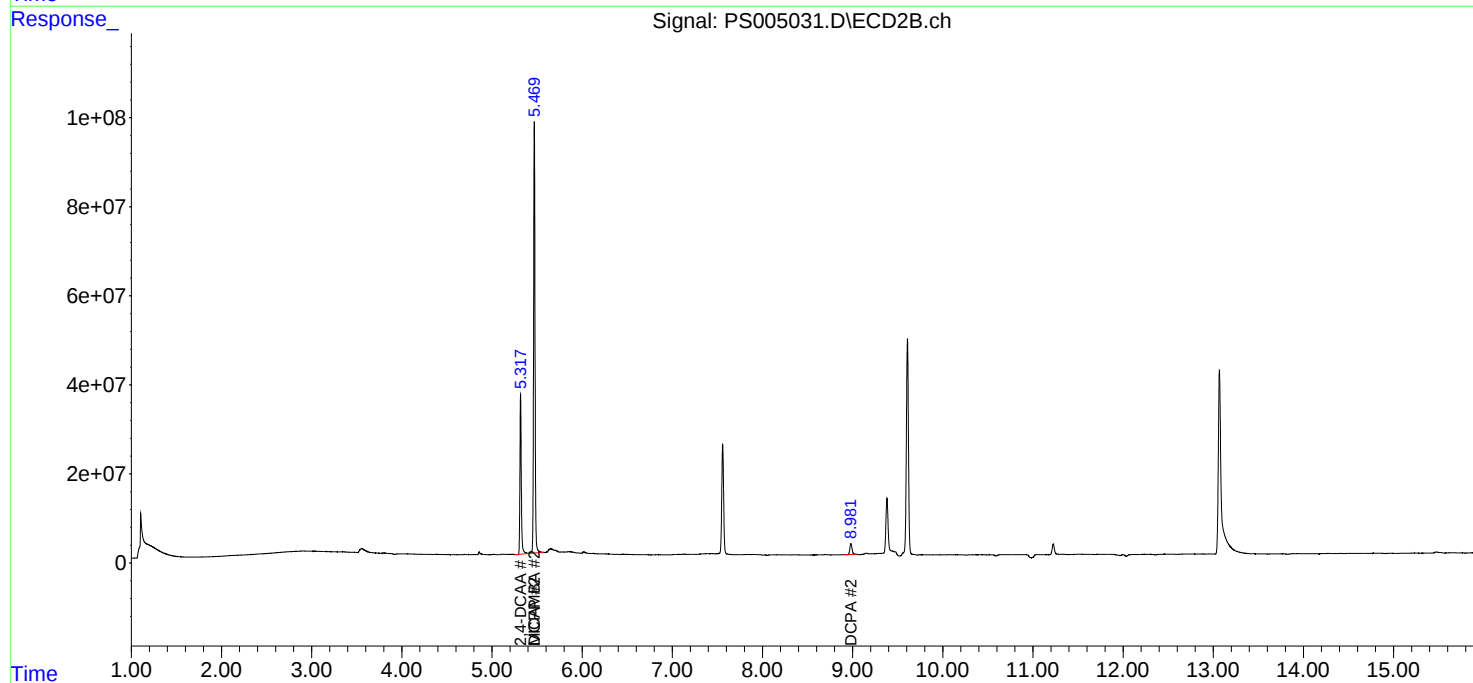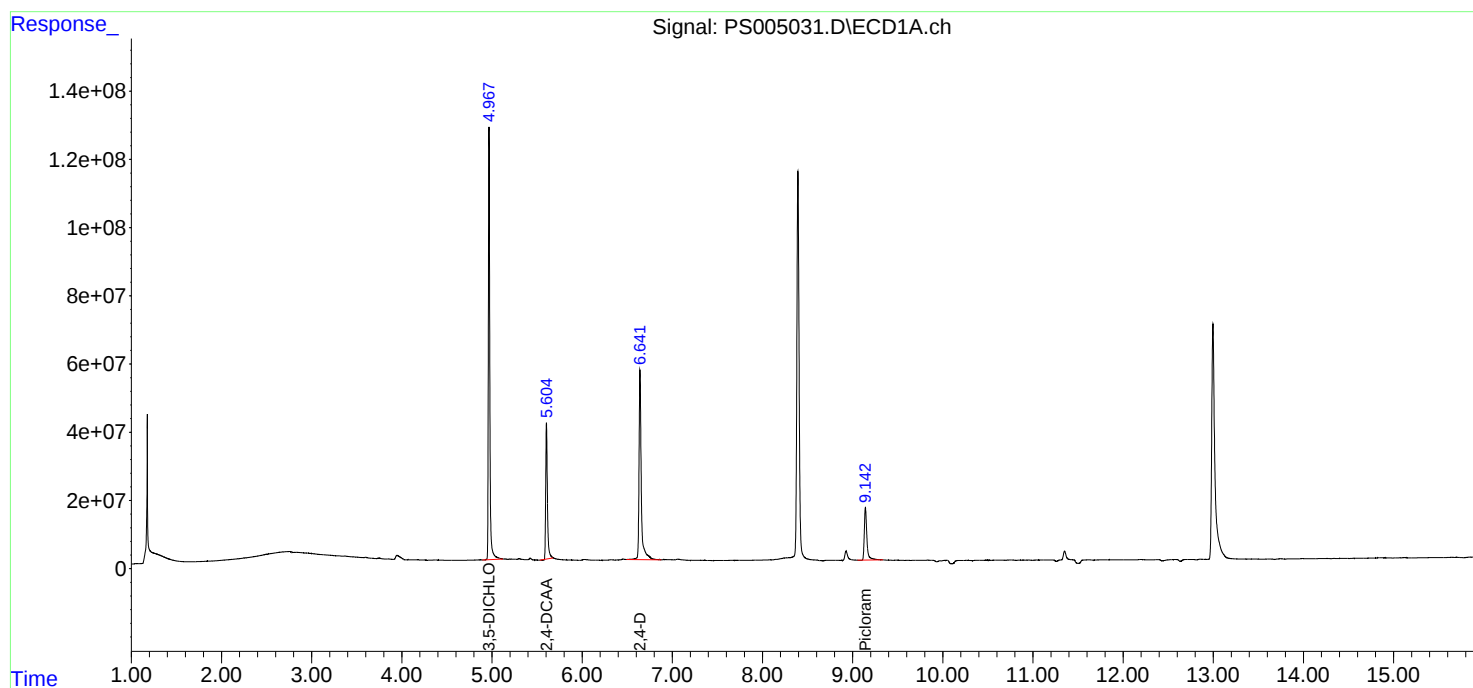


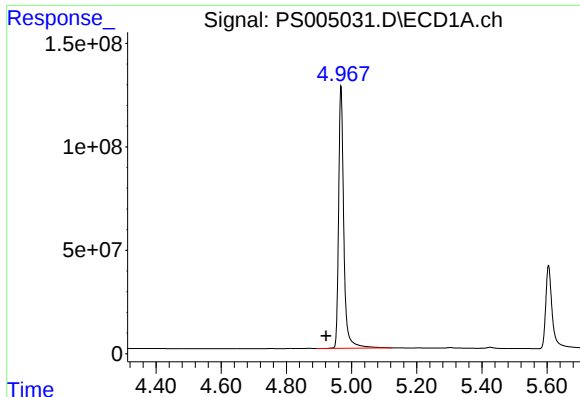

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.968 min
Delta R.T.: 0.046 min
Response: 1399447020
Conc: 742.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

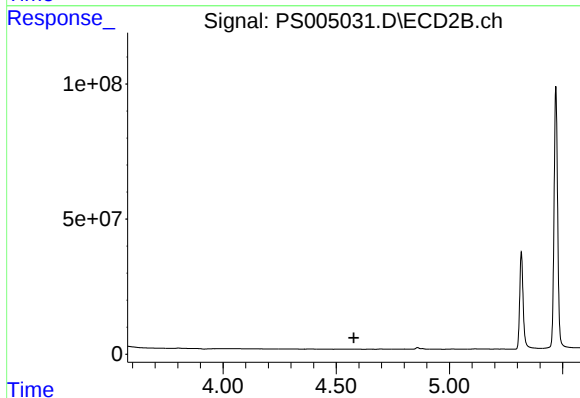


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.578 min
Response: 0
Conc: N.D.

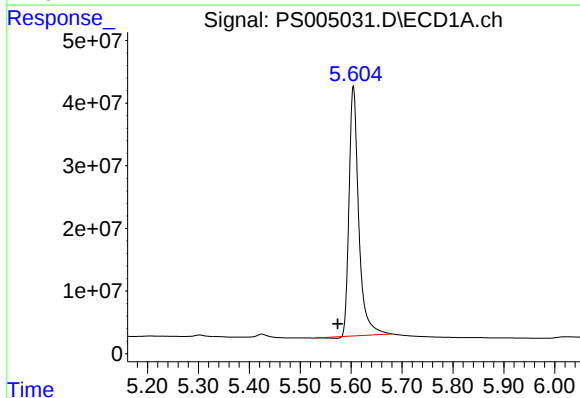


#4 2,4-DCAA

R.T.: 5.605 min
Delta R.T.: 0.031 min
Response: 525329310
Conc: 398.64 ng/ml

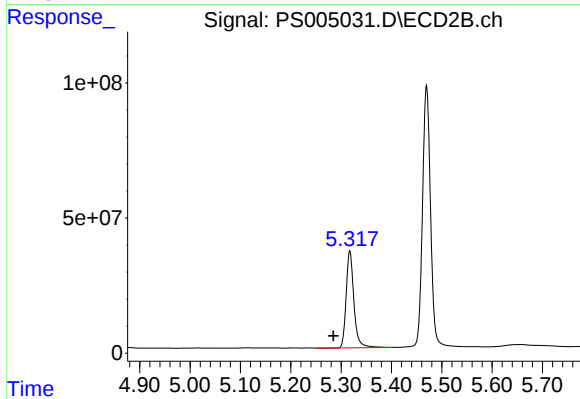

#4 2,4-DCAA


R.T.: 5.317 min
Delta R.T.: 0.032 min
Response: 383550471
Conc: 384.50 ng/ml

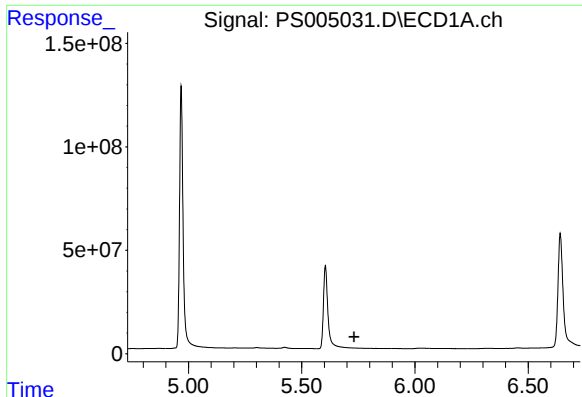

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.731 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

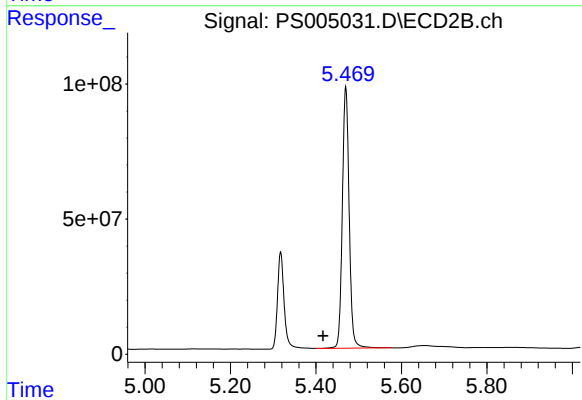


#5 DICAMBA

R.T.: 5.470 min
Delta R.T.: 0.053 min
Response: 1074887303
Conc: 279.88 ng/ml

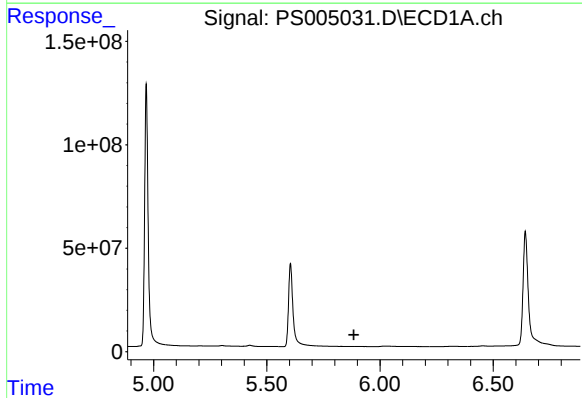


#6 MCP

R.T.: 0.000 min
Exp R.T.: 5.885 min
Response: 0
Conc: N.D.

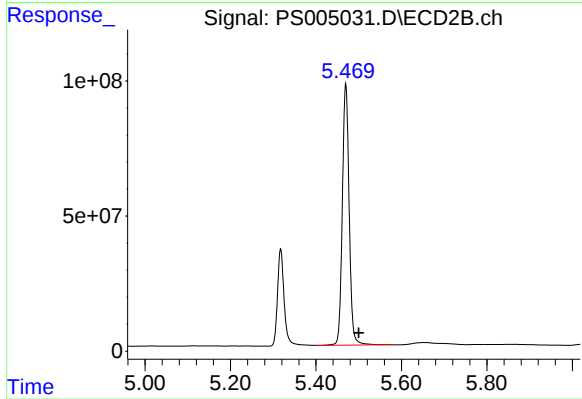

#6 MCP


R.T.: 5.470 min
Delta R.T.: -0.030 min
Response: 1074887303
Conc: 372.00 ug/ml

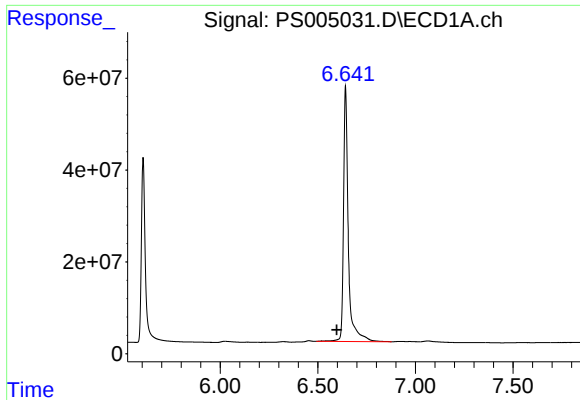

#9 2,4-D


R.T.: 6.642 min
Delta R.T.: 0.046 min
Response: 964081484
Conc: 714.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

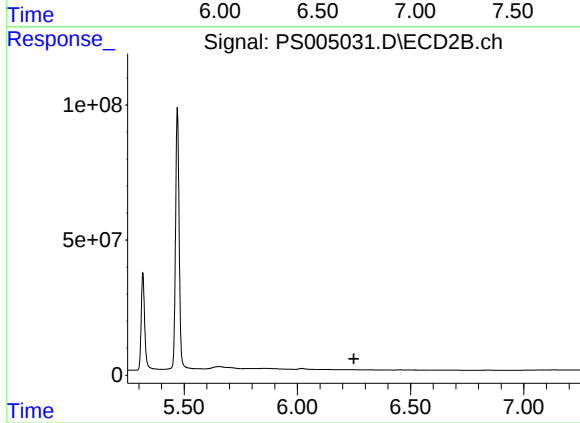


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.250 min
Response: 0
Conc: N.D.

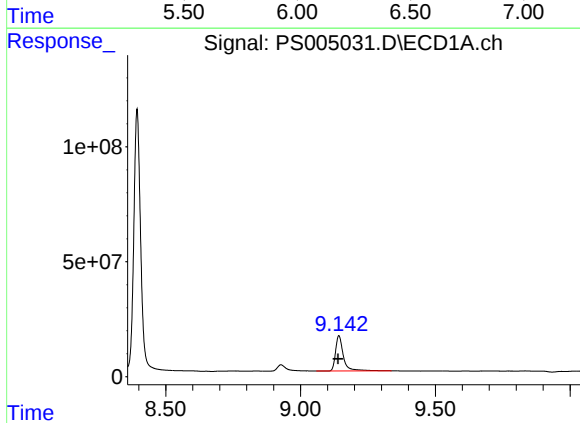


#15 Picloram

R.T.: 9.142 min
Delta R.T.: 0.003 min
Response: 308545383
Conc: 31.08 ng/ml

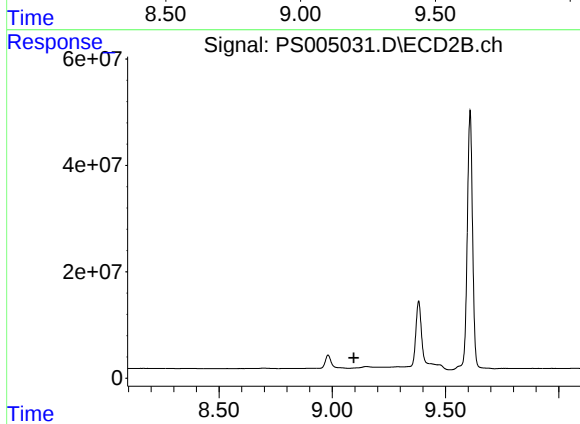

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

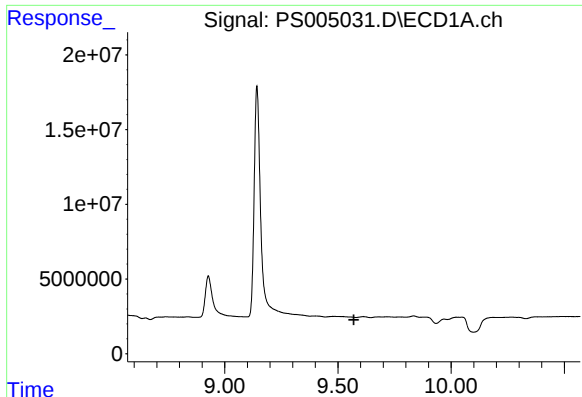

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.571 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

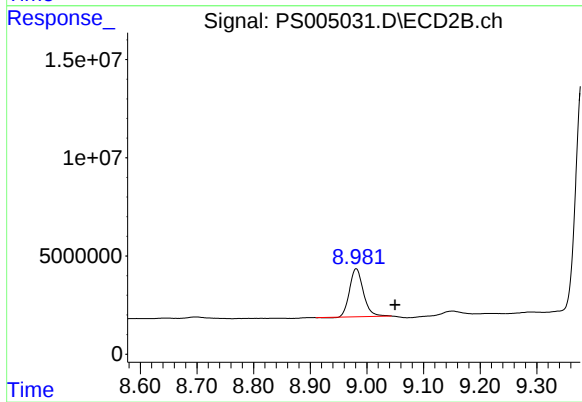

#16 DCPA

R.T.: 8.981 min
Delta R.T.: -0.069 min
Response: 41328745
Conc: 6.27 ng/ml