

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061518\
 Data File : PS000367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 09:29
 Operator : UA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 13:18:33 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
 Quant Title : 8080.M
 QLast Update : Thu May 31 04:46:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) T	DICAMBA	12.140	11.470	4291374	3216891	3.281	2.908
9) T	2,4-D	13.691	13.067	2580171	2063623	5.721	5.368
10) T	Pentachlo...	14.088	13.631	16158582	13200799	3.233	2.997
11) T	2,4,5-TP ...	14.955	14.239	10383160	8490761	5.238	4.936
12) T	2,4,5-T	15.353	14.772	12420344	9836914	6.334	5.968
14) T	DINOSEB	17.617	15.893	9137973	7519089	6.244	6.079
15) T	Picloram	17.375	17.139	20254733	14236071	7.743	6.682
16) T	DCPA	17.957	17.081	15849619	13164046	6.546	6.370


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061518\
Data File : PS000367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 09:29
Operator : UA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 13:18:33 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
Quant Title : 8080.M
QLast Update : Thu May 31 04:46:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

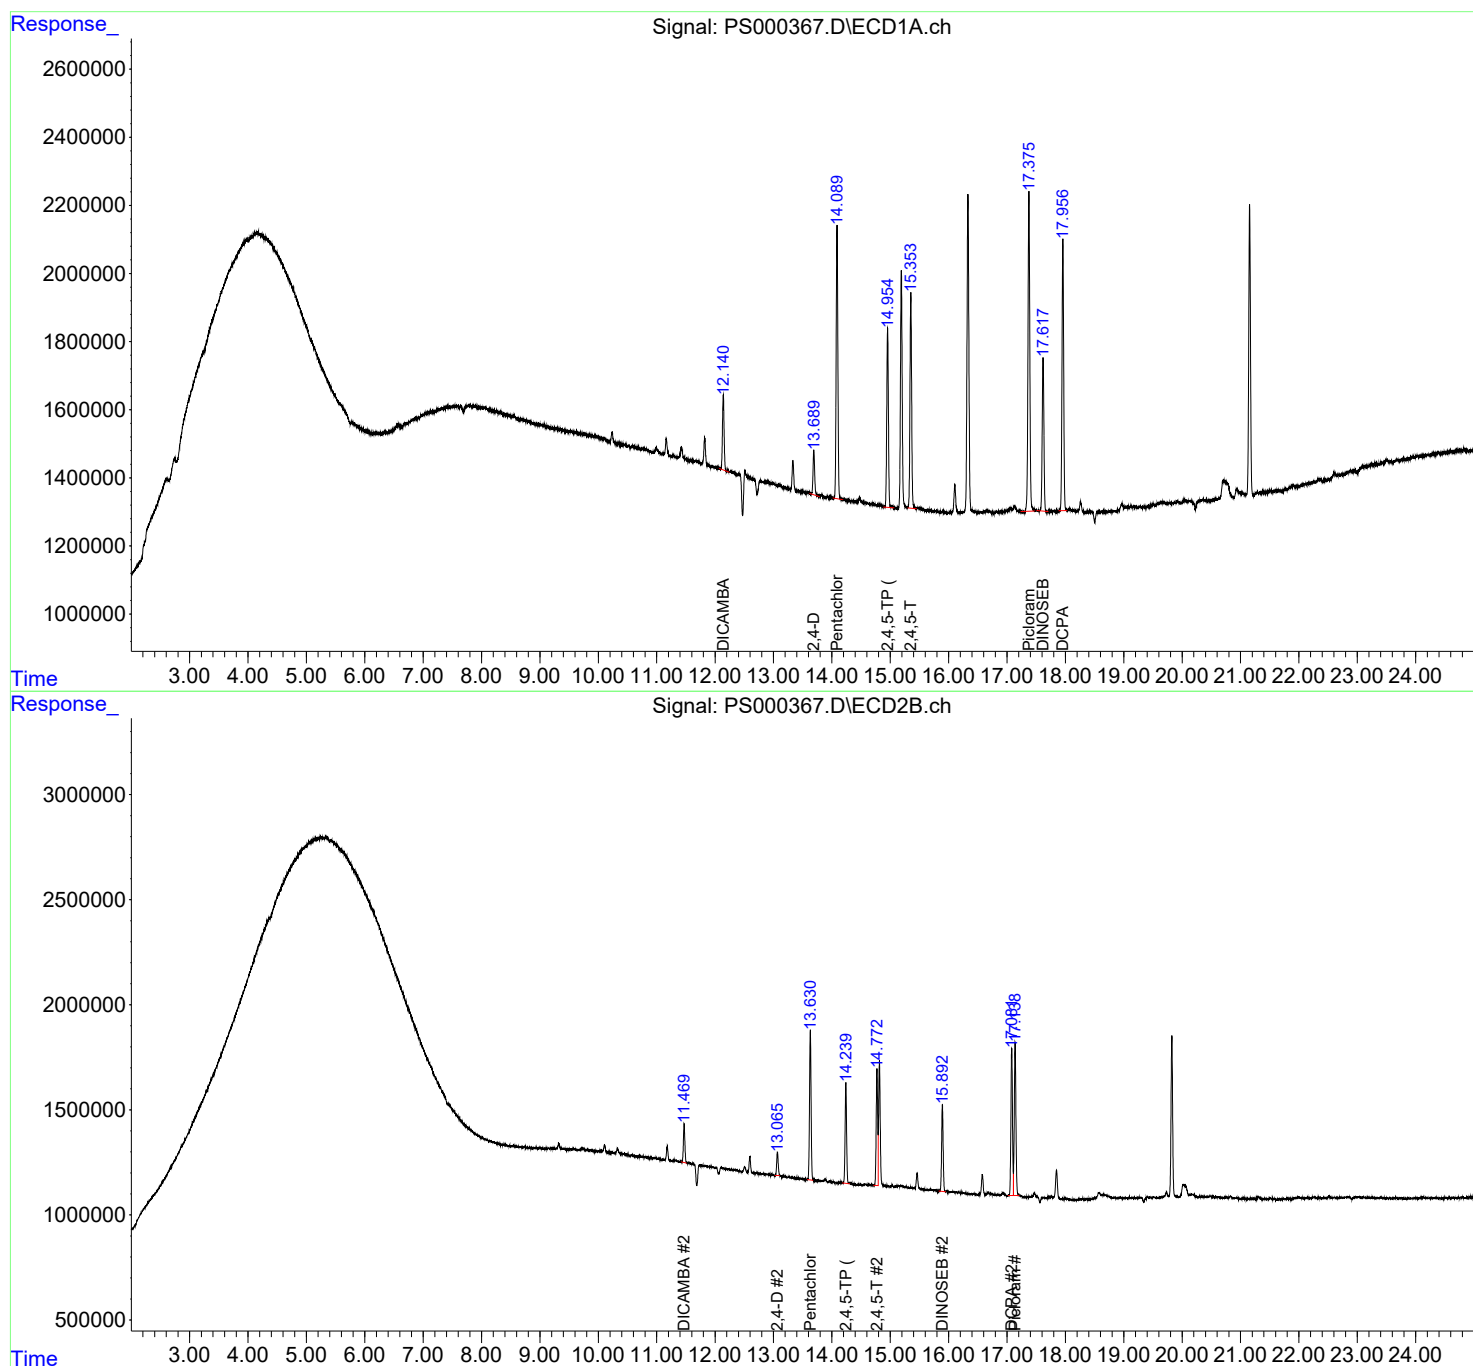


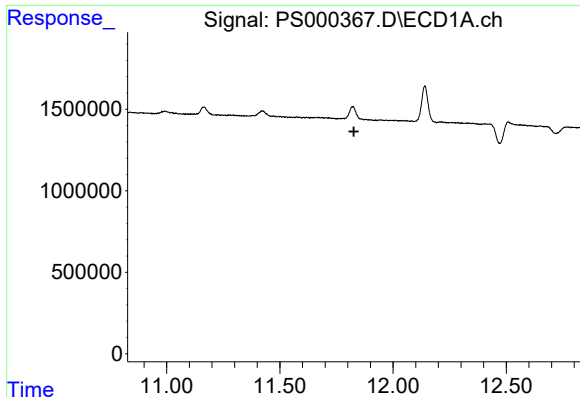

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 11.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

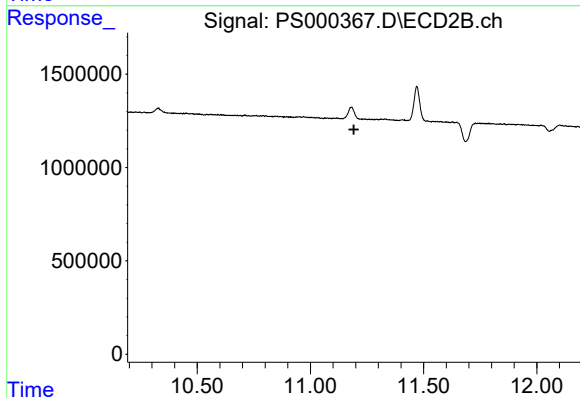


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 11.192 min
Response: 0
Conc: N.D.

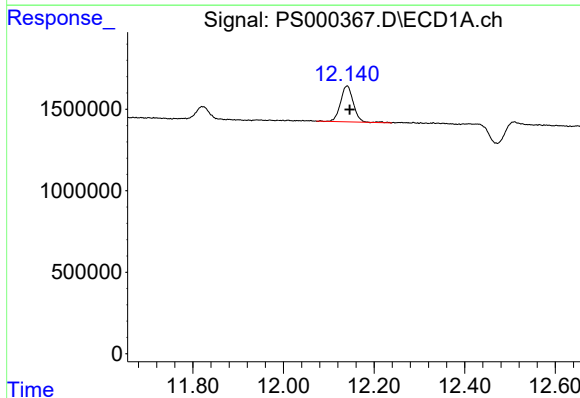


#5 DICAMBA

R.T.: 12.140 min
Delta R.T.: -0.007 min
Response: 4291374
Conc: 3.28 ng/ml

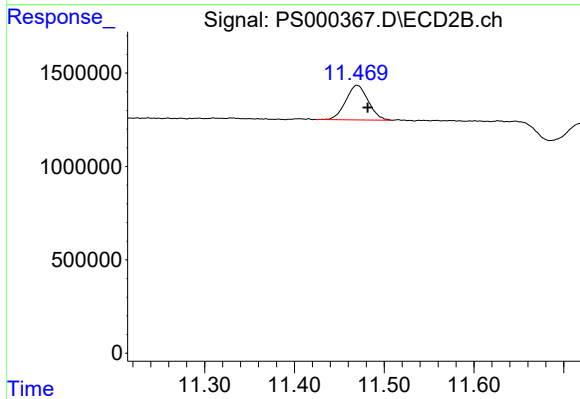

#5 DICAMBA


R.T.: 11.470 min
Delta R.T.: -0.012 min
Response: 3216891
Conc: 2.91 ng/ml

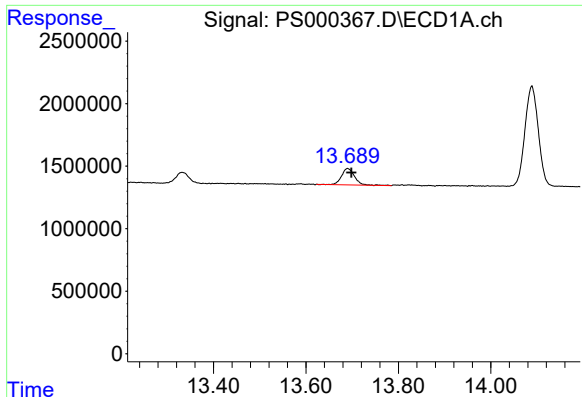

#9 2,4-D


R.T.: 13.691 min
Delta R.T.: -0.007 min
Response: 2580171
Conc: 5.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

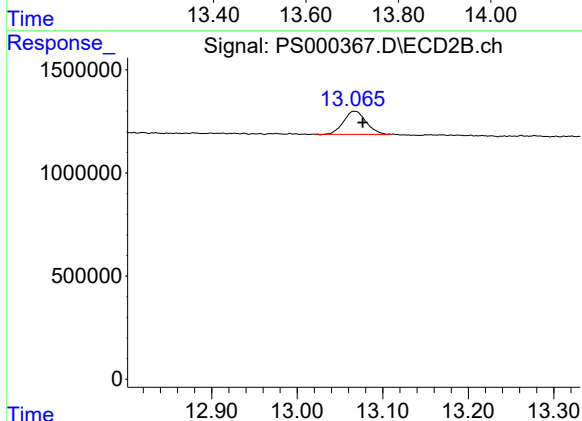


#9 2,4-D

R.T.: 13.067 min
Delta R.T.: -0.010 min
Response: 2063623
Conc: 5.37 ng/ml

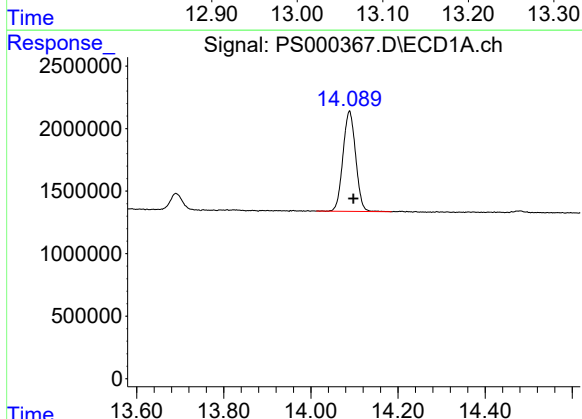


#10 Pentachlorophenol

R.T.: 14.088 min
Delta R.T.: -0.009 min
Response: 16158582
Conc: 3.23 ng/ml

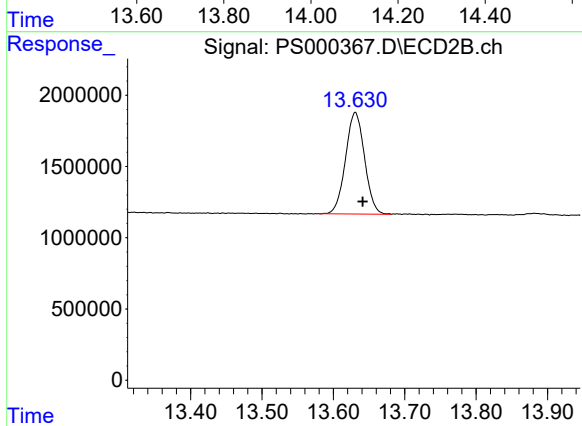

#10 Pentachlorophenol


R.T.: 13.631 min
Delta R.T.: -0.010 min
Response: 13200799
Conc: 3.00 ng/ml

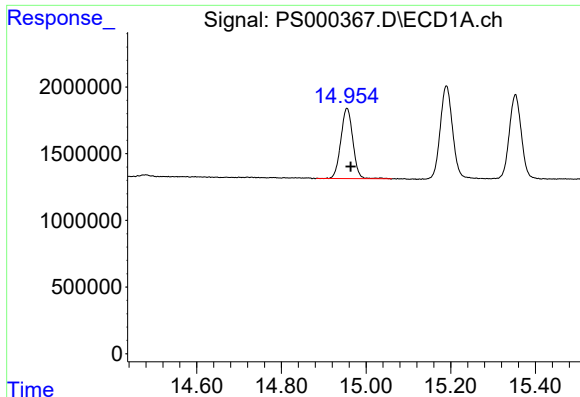

#11 2,4,5-TP (SILVEX)


R.T.: 14.955 min
Delta R.T.: -0.009 min
Response: 10383160
Conc: 5.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

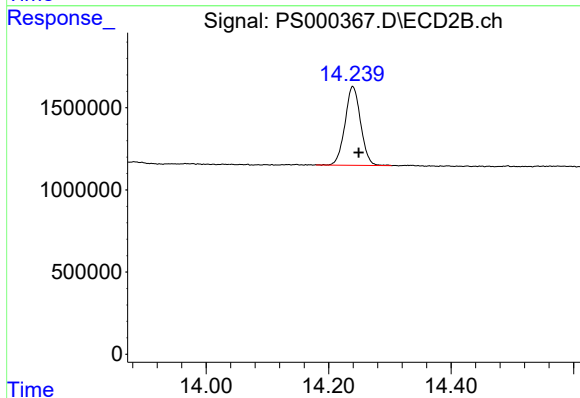


#11 2,4,5-TP (SILVEX)

R.T.: 14.239 min
Delta R.T.: -0.010 min
Response: 8490761
Conc: 4.94 ng/ml

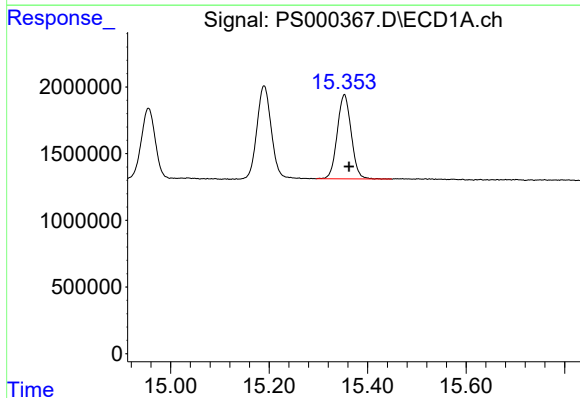


#12 2,4,5-T

R.T.: 15.353 min
Delta R.T.: -0.010 min
Response: 12420344
Conc: 6.33 ng/ml

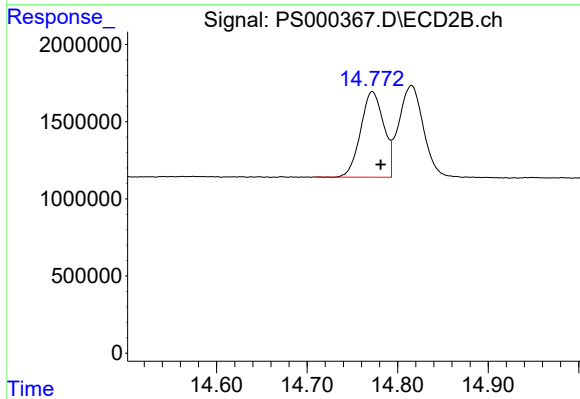

#12 2,4,5-T


R.T.: 14.772 min
Delta R.T.: -0.009 min
Response: 9836914
Conc: 5.97 ng/ml

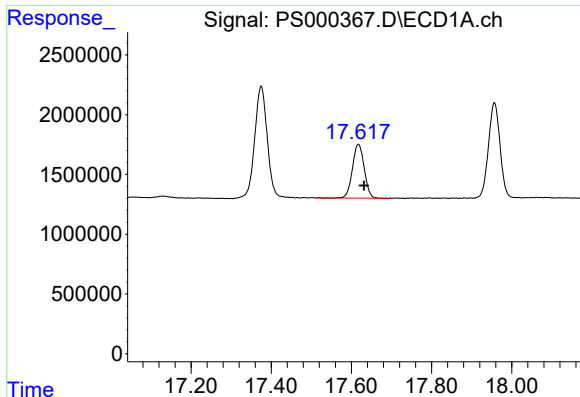

#14 DINOSEB


R.T.: 17.617 min
Delta R.T.: -0.014 min
Response: 9137973
Conc: 6.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

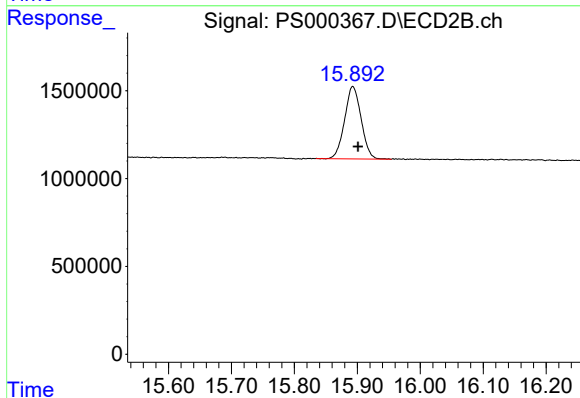


#14 DINOSEB

R.T.: 15.893 min
Delta R.T.: -0.009 min
Response: 7519089
Conc: 6.08 ng/ml

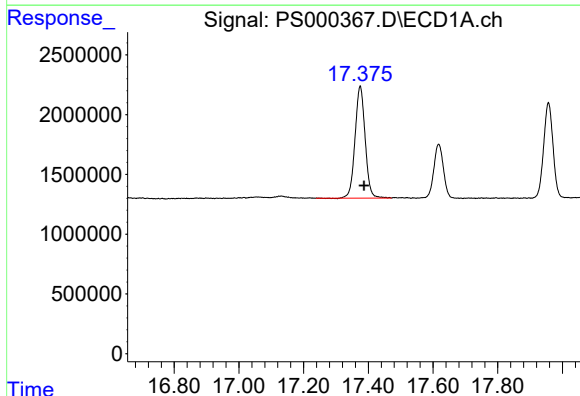


#15 Picloram

R.T.: 17.375 min
Delta R.T.: -0.012 min
Response: 20254733
Conc: 7.74 ng/ml

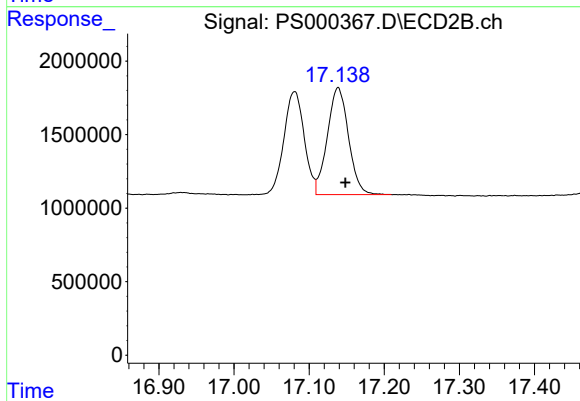

#15 Picloram


R.T.: 17.139 min
Delta R.T.: -0.010 min
Response: 14236071
Conc: 6.68 ng/ml

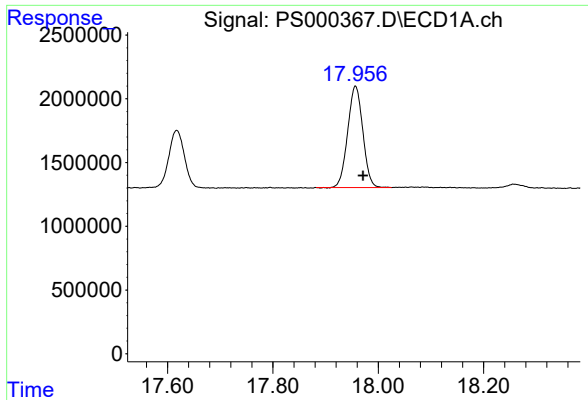

#16 DCPA

R.T.: 17.957 min
Delta R.T.: -0.014 min
Response: 15849619
Conc: 6.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

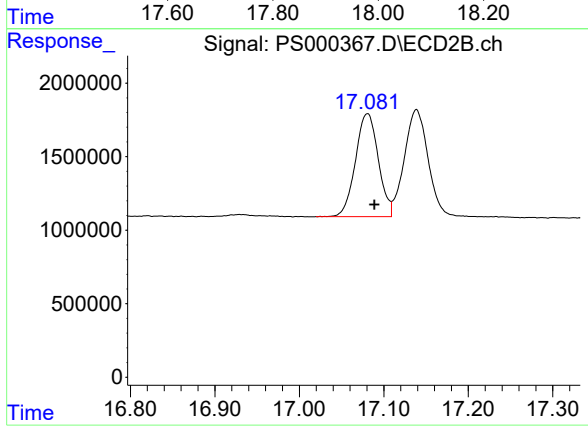

#16 DCPA

R.T.: 17.081 min
Delta R.T.: -0.008 min
Response: 13164046
Conc: 6.37 ng/ml