

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061518\
 Data File : PS000368.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 10:00
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 13:19:01 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
 Quant Title : 8080.M
 QLast Update : Thu May 31 04:46:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.813	11.185	178.8E6	152.8E6	506.294	486.433
Target Compounds							
15) T	Picloram	17.368	17.139	4561166	3058582	1.744	1.436
16) T	DCPA	0.000	17.139	0	3058582	N.D.	1.480 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061518\
Data File : PS000368.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 10:00
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 13:19:01 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
Quant Title : 8080.M
QLast Update : Thu May 31 04:46:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

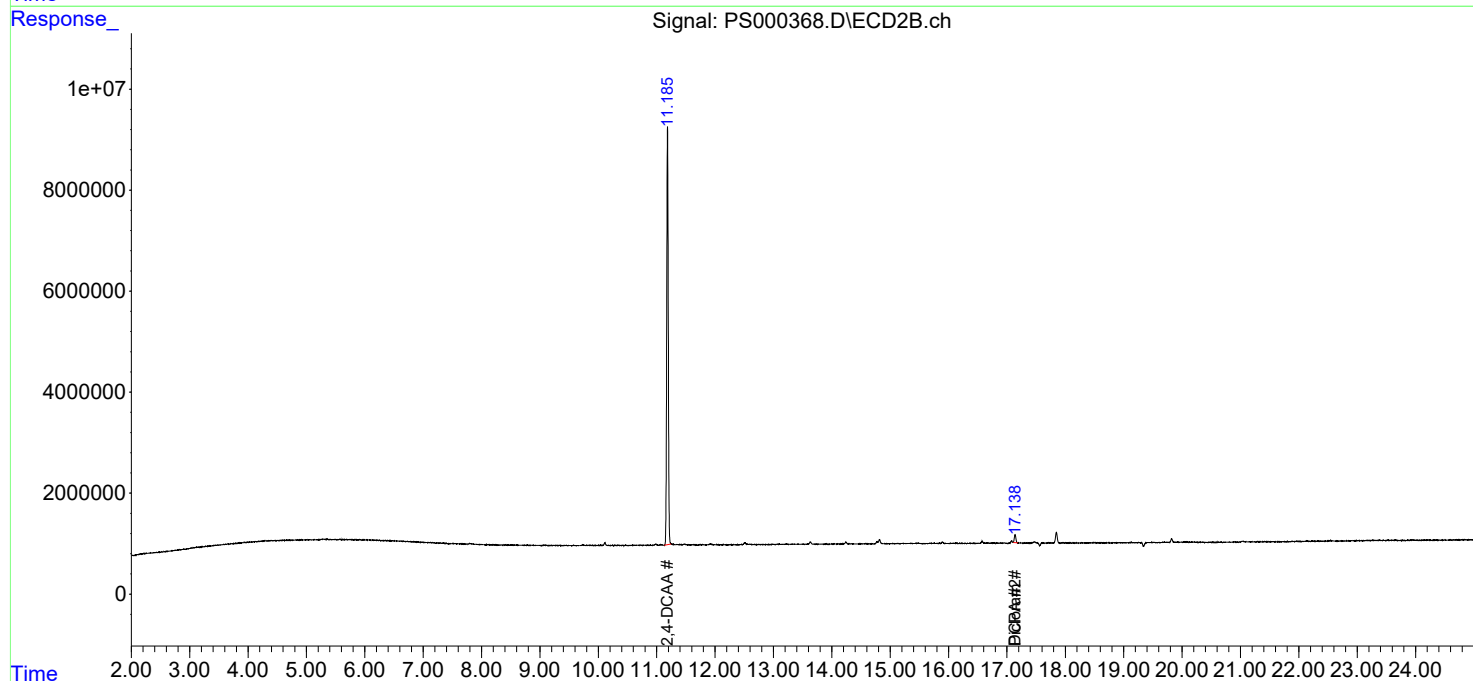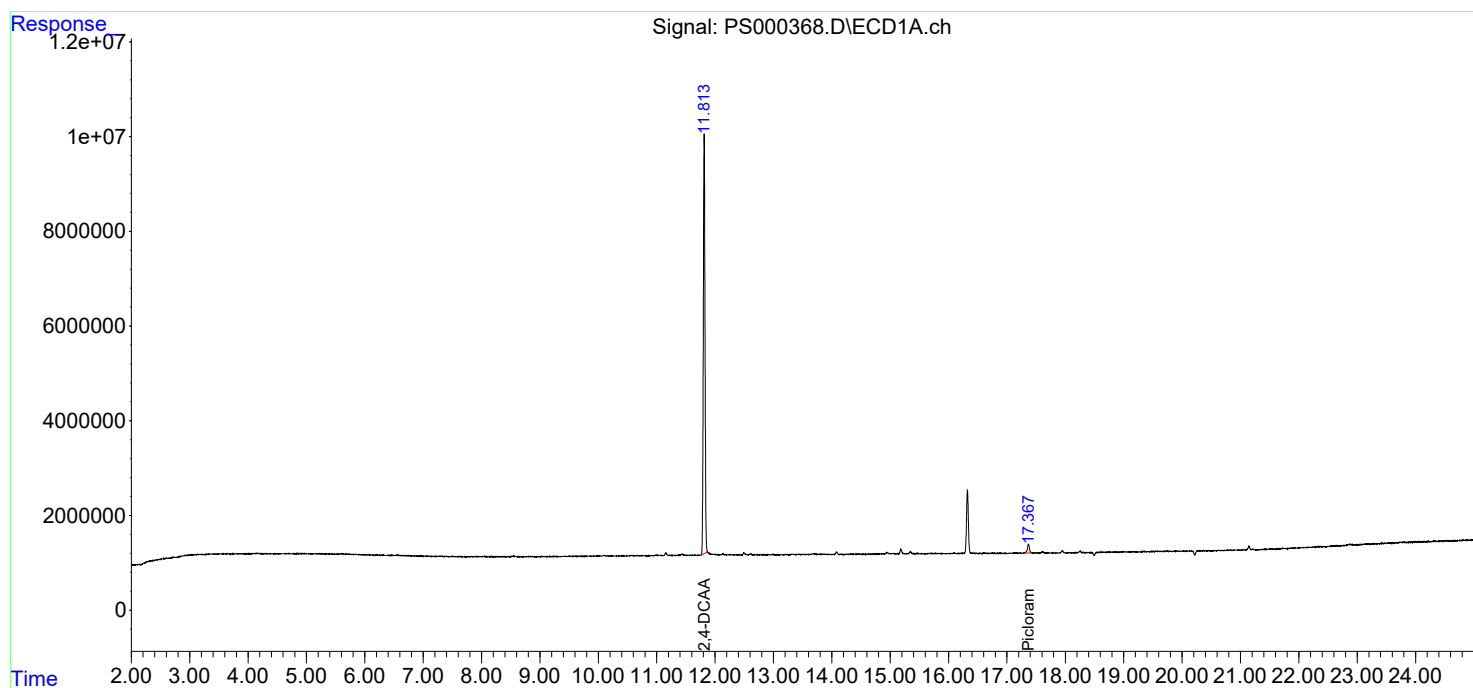


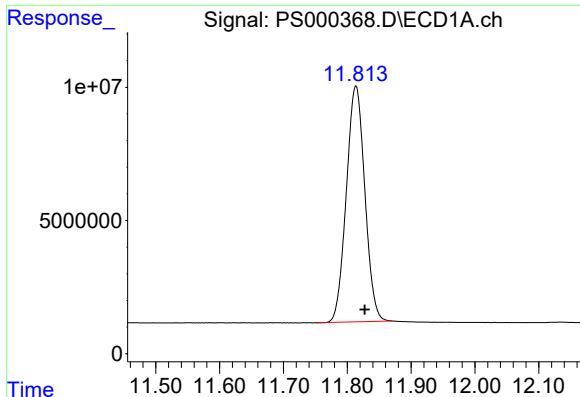

#4 2,4-DCAA


R.T.: 11.813 min
Delta R.T.: -0.014 min
Response: 178760442
Conc: 506.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

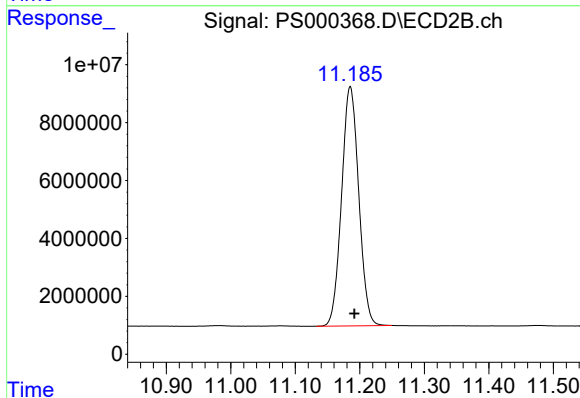


#4 2,4-DCAA

R.T.: 11.185 min
Delta R.T.: -0.006 min
Response: 152789602
Conc: 486.43 ng/ml

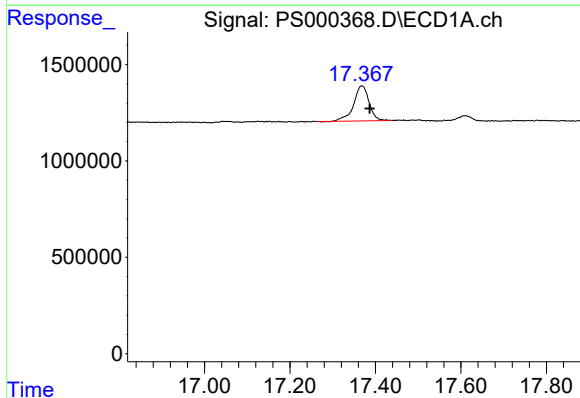


#15 Picloram

R.T.: 17.368 min
Delta R.T.: -0.019 min
Response: 4561166
Conc: 1.74 ng/ml

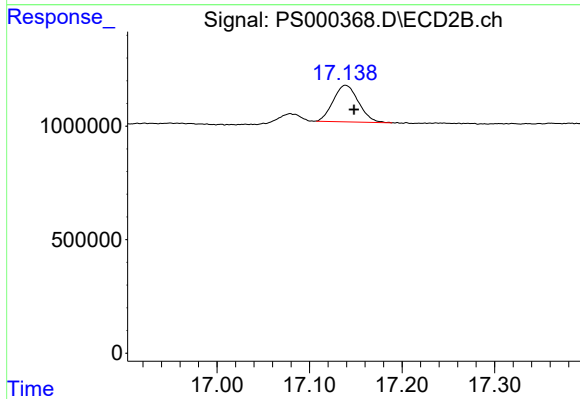

#15 Picloram


R.T.: 17.139 min
Delta R.T.: -0.009 min
Response: 3058582
Conc: 1.44 ng/ml

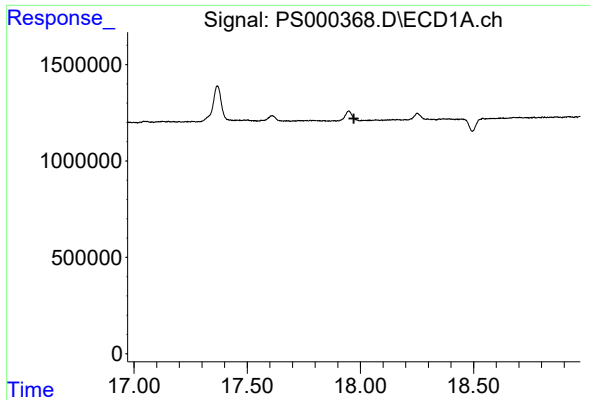

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

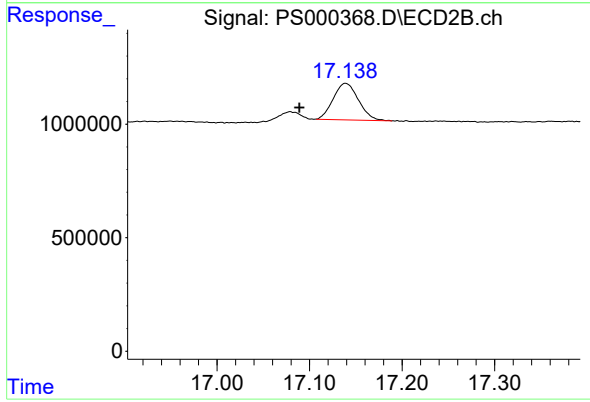

#16 DCPA

R.T.: 17.139 min
Delta R.T.: 0.050 min
Response: 3058582
Conc: 1.48 ng/ml